# **Managements**

## MestReNova Manual

© 2017 MESTRELAB RESEARCH

# **MestreNova 11**

by MESTRELAB RESEARCH

This is the manual of MestreNova 11

### MestreNova Manual

### © 2017 MESTRELAB RESEARCH

All rights reserved. No parts of this work may be reproduced in any form or by any means - graphic, electronic, or mechanical, including photocopying, recording, taping, or information storage and retrieval systems - without the written permission of the publisher.

Products that are referred to in this document may be either trademarks and/or registered trademarks of the respective owners. The publisher and the author make no claim to these trademarks.

While every precaution has been taken in the preparation of this document, the publisher and the author assume no responsibility for errors or omissions, or for damages resulting from the use of information contained in this document or from the use of programs and source code that may accompany it. In no event shall the publisher and the author be liable for any loss of profit or any other commercial damage caused or alleged to have been caused directly or indirectly by this document.

# **Table of Contents**

Part I	Introduction	11
1	Formats supported	11
2	System Requirements	12
	Windows System Requirements Mac OS X System Requirements Linux System Requirements	12
Part II	Installation Guide	14
Part III	Mnova 11	20
Part IV	Shortcuts	25
Part V	Fast Visual Guide to process routine 1D-NMR	
	datasets	29
Part VI	Fast Visual Guide to process routine 2D-NMR datasets	35
Part VII	The Mnova interface	41
1	Multipage Software	
	Multipage Software Working on a Single Page	
		45
2 3	Working on a Single Page	45 47
2 3	Working on a Single Page Data Browser	45 47 49
2 3 4	Working on a Single Page Data Browser Mnova Menus & Toolbars	45 47 49 66
2 3 4 5	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard	45 47 49 66 70
2 3 4 5 6	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties	45 47 49 66 70 83
2 3 4 5 6 7	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus	45 47 49 66 70 83 92 96
2 3 4 5 6 7 8	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization	45 47 49 66 70 83 92 96
2 3 4 5 6 7 8 9	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus	45 47 49 66 70 83 92 96 99
2 3 4 5 6 7 8 9	Working on a Single Page         Data Browser         Mnova Menus & Toolbars         Intelligent NMR Clipboard         Properties         Preferences         Menus and Toolbars Customization         Context Menus	45 47 49 66 70 83 92 96 99 100
2 3 4 5 6 7 8 9 10 11 12	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus Localization Layout Templates How to measure coupling constants? The Crosshair Tool Multiple Crosshair for 2D analysis	45 47 49 66 70 83 92 96 99 100 106 107
2 3 4 5 6 7 8 9 10 11	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus Localization Layout Templates How to measure coupling constants? The Crosshair Tool Multiple Crosshair for 2D analysis Zooming	45 47 49 66 70 83 92 96 99 100 106 107 111
2 3 4 5 6 7 8 9 10 11 12	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus Localization Layout Templates How to measure coupling constants? The Crosshair Tool Multiple Crosshair for 2D analysis	45 47 49 66 70 83 92 96 99 
2 3 4 5 6 7 8 9 10 11 12	Working on a Single Page Data Browser Mnova Menus & Toolbars Intelligent NMR Clipboard Properties Preferences Menus and Toolbars Customization Context Menus Localization Layout Templates How to measure coupling constants? The Crosshair Tool Multiple Crosshair for 2D analysis Zooming Full View	45 47 49 66 70 83 92 96 99 100 100 106 107 111 117 118

5

		100
16	Increasing and Decreasing Intensity	
17	Undo & Redo	
18	Graphics and Annotations	
Part VIII	Processing Basics	127
1	1D NMR Processing Tour	
2	2D NMR Processing Tour	
3	Stacked NMR Processing	
	How to apply a peak picking or an integration analysis in stacked mode?	
	Setup Arrayed Spectra	
	Table of stacked items	
4	Stacked Options and Properties	
4		
	Group Delay FID Shift	
	Diagonal Suppresion	-
	Signal Suppresion	
	Apodization	171
	Truncation	
	Frequency Shift	
	Zero Filling and Linear Prediction Drift Correction	
	The FT Command	
	NUS Processing	
5	Phase Correction with Mnova	
6	Baseline Correction with Mnova	
7	Symmetrization	
8	Tilt 45	
9	Reducing t1 Noise	
10	Covariance NMR	
11	Normalization	
12	Binning	
13	Compression	
14	Smoothing	
15	Denoise	
16	Resolution Booster	
17	Reference Deconvolution	
18	Inverting, Transposing and Reversing Spectra	
19	Processing Templates	232
Part IX	Analysis Tools	236
1	Chemical Shift Referencing	
	Absolute Reference of x-Nuclei experiments	
	Reference of 2D-NMR spectra with the 1D external trace	

### MestreNova Manual

2	Peak Picking	
	Peak Picking Options	
	Impurities Auto detection	
	GSD (Global Spectral Deconvolution)	
	What else can I do with GSD?	
	Peaks Table and Reports	
	Peak Picking Properties	
3	Integration	
•	-	
	Integrals Table	
	Integral Properties	
4	Multiplets analysis	
	Multiplet Manager	
	Using GSD for multiplets analysis	
	Setting multiplets	
	How to resolve overlapped multiplets?	310
	Multiplets Table and Reports	
	Multiplet Analysis options	
	Multiplets Properties	
	Importing spectral data from literature to synthesize a spectrum	
5	Automatic Analysis	
6	How to carry out assignments?	
-	Assignments Table	
	Transfering assignments through datasets	
	Assisted assignment by using the predictions	
	Copy assignments from one molecule to another	
	Assignments Properties	
7	Assignments roperties	
'	-	
	Single Mode	
	Verification Results panel	
	Options	
	Troubleshooting a negative result	
	Rank potential molecular candidates	
	Verification in batch mode	
	Verify Viewer	
-		
8	Molecules Editor	398
	Molecular Structure	
	Compounds Table	412
9	NMR Prediction	415
	Random Forest prediction	
	Modgraph NMR Predict Desktop	
	Running predictions	
	Automatic Assignments	
	Predict & Highlight	
	Predict & Compare	
	Predict & Verify	
	Prediction Database	
	3D Molecule Viewer	
	Prediction Options and Properties	-
	NMRPredict Server-Based	
10	Tables	

© 2017 MESTRELAB RESEARCH

7

468


1	Line Fitting (Deconvolution)	468
	Line Fitting Properties	
2	TD Quantitation	
	TD Quantitation panel	
3	DOSY Transform	
4	Data Analysis Quick Start Guide	
	Data Analysis	491
	Data Analysis panel	
	Data Analysis Properties	
	T1 Analysis	
	Reaction Monitoring (R-M)	
	Importing Datasets Selecting Regions	
	Practical Example	
5	Reference Alignment.	
6	Align Spectra	
7	PCA	539
8	J-Correlator	
9	Arithmetic	547
10	Spin Simulation	
	Spin Simulation panel	559
Part XI	qNMR	563
Part XI	qNMR Concentration Workflow	563
	Concentration Workflow	<b>563</b>
	-	<b>563</b> 
	Concentration Workflow	<b>563</b> 
1	Concentration Workflow qNMR Settings Purity qNMR	563 
1 2 3	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR	563 
1 2 3	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script	563 564 567 573 580 585 591
1 2 3 <b>Part XII</b> 1	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script Scripting with Mnova	563 564 567 573 580 585 591 597
1 2 3 <b>Part XII</b> 1	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script Scripting with Mnova Connecting scripts with Mnova objects	563 
1 2 3 <b>Part XII</b> 1 2	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script Scripting with Mnova Connecting scripts with Mnova objects Connecting scripts with Mnova GUI	563 564 567 573 580 585 591 597 604 605
1 2 3 Part XII 1 2 3	Concentration Workflow	563 564 567 580 585 591 597 604 605 609
1 2 3 Part XII 1 2 3 4	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script Scripting with Mnova Connecting scripts with Mnova objects Connecting scripts with Mnova GUI Mnova processing scripts Mnova properties scripts	563 564 567 573 580 585 591 604 605 609 610
1 2 3 Part XII 1 2 3 4 5	Concentration Workflow	563 564 567 .573 .580 .585 591 597 604 605 609 611
1 2 3 Part XII 1 2 3 4 5 6	Concentration Workflow qNMR Settings Purity qNMR Batch qNMR Purity Calculator script Scripting with Mnova Connecting scripts with Mnova objects Connecting scripts with Mnova GUI Mnova processing scripts Mnova properties scripts GUI Actions Running Scripts from the command line	563 
1 2 3 Part XII 1 2 3 4 5 6 7	Concentration Workflow	563 564 567 573 580 585 591 585 591 604 605 609 610 611 612 615
1 2 3 <b>Part XII</b> 1 2 3 4 5 6 7 8	Concentration Workflow	563 564 567 .573 .580 .585 .585 .591 597 604 605 609 610 611 612 615 620

Part X Advanced Menu

Part XIII	Tutorials	640
1	Importing Spectrum Parameters	
2	Basics on Arrayed-NMR Data Analysis	
3	Superimposed Spectra	
4	How to process Varian DEPT spectra?	
5	Mnova for metabonomics	
-	Show Traces in 2D-NMR	
6		
7	Manual Phase Correction in 2D-NMR	
8	Pasting Spectra into Reports	
9	How to predict a spectrum with NMRPredict Desktop?	704
Part XIV	Mass Plugin	711
1	First Steps with the Mass Plugin	
2	Working with the MS plugin	
-	MS Browser	
	Mass Analysis	
	Peak Detection (Integration)	
	Spectrum Selection Mode	
	Elemental Composition	
	Molecular Match	
	New Mass chromatogram	
	MS Spectrum Prediction	
	Trace Baseline Correction	
	Align traces retention times	
	Traces autoalignment Peak Purity	
	Chromatography	
	Background and UV subtraction	
	MS Tables	
	Context menu	
	Properties and layouts	
	Preferences	
Part XV	Mnova Database	788
1	Create a Database	
2	Connecting to the Server	
3	Saving items to Database	
4	Displaying database contents	792
	Operations	
_	Searching in the Database	
5	View Results	
6	Deleting items/Records	
7	User Preferences	
8	Managing Databases	
	Create custom fields	

© 2017 MESTRELAB RESEARCH

Cont	tents	9
	l	
9 Mnova DB scripts		

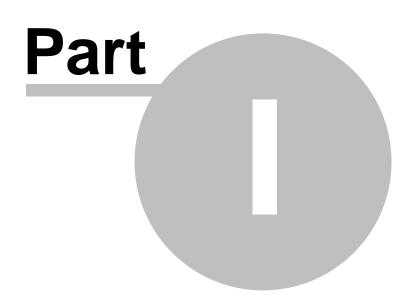

### 1 Introduction

Welcome to **MestReNova (Mnova)**. **Mnova** is the latest Nuclear Magnetic Resonance and LC/GC/MS data processing, visualization, simulation, prediction, presentation and analysis software package available on the market. This **Help Manual** introduces you to this new software, ensuring that you can use it successfully and achieve good results right from the start. We strongly suggest that you print this manual and follow it when first using **Mnova**, as this will make your introduction to the software very simple and painless, and will make sure that you quickly identify all the main functionality in the software.

**Mnova** is the natural evolution of our very popular application **MestReC**. However, it is more than a new version of **MestReC**. Whilst including all the NMR processing and analysis functionality present in MestReC, it is a completely new development and a completely new concept which will open up a whole new range of possibilities when storing and sharing data within organizations, changing the way in which scientists process and report NMR and LC/GC/MS data. **Mnova** has been designed to make NMR and LC/GC/MS both more convenient and more powerful, and to give the user improved results with minimum effort.

The program provides a variety of **conversion facilities** for most NMR and LC/GC/MS spectrometer and chromatogram formats and includes all the conventional processing, displaying, and plotting capabilities of an NMR program, as well as more advanced processing techniques with a very user friendly graphical interface. To read a little bit more on the main features, and familiarize yourself with the principles behind the program, follow this guide.

### **1.1** Formats supported

Here you can see a list of some of the main formats supported by Mnova:

**NMR:** Bruker Aspect 2000/3000, Bruker UXNMR/XWIN-NMR, Bruker WinNMR, GE/Nicolet, Galactic (\*.spc), JEOL Alice (.als), JEOL Delta, JEOL EX/GX, JEOL Fastflight (.fft), JEOL Lambda (.nmfid, .nmdata, .nmf, .nmd), Magritek Prospa (\*1D, \*2D), Old Gemini, SIMPSON, Siemens Magneton Vision, Tecmag (.tnt), Varian Gemini/VXR from VHelper, Varian VNMR, VARIAN/Chemagnetic Spinsight (data), Philips Achieva, Siemens Syngo.

Other NMR formats: ASCII (.txt), Mnova (.mnova), ZIP (.zip), MestReC (.mrc), NUTS Type 1-3, SwaN-MR, JCAMP-DX (.jcamp, .dx, .jdx, .jcm), ACD-Labs (1D), Int 32 WinNMR, LCModel ASCII, Sparky 2D

MS: Currently supported formats on Windows Agilent – ChemStation, MassHunter, Ion Trap Bruker – Xmass, Compass[1] and Daltonics[1] Waters – MassLynx Thermo Scientific – Xcalibur mzData and mzXML JEOL – MSQ 1000, FastFlight AB SCIEX – Analyst[1] AB SCIEX Data Explorer Shimadzu NetCDF ANDI-MS

Currently supported formats on Mac / Linux Agilent – ChemStation Bruker – XMass FSU – Midas mzData and mzXML Waters - MassLynx (Mac only)

[1] At present, Mnova MS supports Bruker Compass, Daltonics and Analyst files but it is necessary to have the vendor software installed on the same computer for this to work. We recommend to have installed Mnova on the spectrometer computer and export your MS datasets as .mnova format to use them in any other computer without the vendor software. For further information please email us to support@mestrelab.com

### **1.2** System Requirements

Before installation, please read this chapter. In this section you will find information on which hardware and software requirements must be met before you can install Mnova. In any case, it is worth noting that Mnova is a **multiplatform** software which will run alternatively on Windows, Mac OS X, Linux and Unix-like systems. From now on, multiplatform laboratories will be able to allow each researcher to work on their Operating System of choice, and to seamlessly share data and processing capabilities with other researchers working on different platforms. There is no longer a need to have three different software packages, and three different file formats, for different Operating Systems.

The minimum and recommended system requirements for the software are:

Windows
Mac OS X
Linux

### **1.2.1 Windows System Requirements**

The *minimum* recommended configuration for Mnova installation is at least Pentium 300 MHz, 128MB RAM, a VGA color monitor with 800 x 600 pixels resolution, a compatible mouse and Windows Vista as operating system. However, ideal system requirements for optimum operation of the software are Pentium 1,6 GHz or higher CPU with 512 Mb or more of RAM memory and Windows 7, W8 or W10.

Mnova will not install under Windows XP or lower. The default installation requires about 200 Mb of disk space.

If you are going to install (or uninstall) the program on a Windows system, be sure you have administrator privileges, because the installation procedure is going to install several files in your system folders. If you don't have such privileges, you won't be able to install or uninstall the program correctly.

### 1.2.2 Mac OS X System Requirements

Mnova requires at least Mac OS X 10.7 (Lion), with Intel architecture. The current version of Mnova is also compatible with 10.8 (Mountain Lion) and 10.9 (Mavericks).

### 1.2.3 Linux System Requirements

Mnova requires at least Pentium 300 MHz, 128MB RAM, Video Adapter Super VGA (800 x 600) with X Library (Xlib). Please, make sure to choose the correct setup file for your Operating System (Debian Wheezy, OpenSUSE 12.3 and 13.1, Fedora 20, Ubuntu 12.04 and 13.10, Red Hat Enterprise 5 or 6 and Mageia 3.0)



### 2 Installation Guide

### Instructions to Install and Activate an Individual Copy of Mnova:

1. If you are going to install the program on a Windows XP system, be sure you have administrator privileges, because the installation procedure is going to install several files in your system folders. If you don't have such privileges, you won't be able to install or uninstall the program correctly.

2. On each host, download the Mnova SETUP file from our website at <u>http://mestrelab.com/software/mnova-suite/download/</u>. Then, double click on the Mnova SETUP file and follow the instructions as they appear on screen.

If you have had a version of Mnova installed previously, the installer will inform you that it is necessary to uninstall the previous version of Mnova. Make sure that this version is closed and click OK and then OK again to confirm. This will uninstall Mnova from your computer. You will get a message to inform you that uninstall was successful: click 'Continue'.

Once you have read and accepted the terms of the License Agreement, click on "**Next**" and select the destination folder where the program files will be placed in your computer. We suggest that you accept all the installation defaults. Once you have chosen the Start Menu Folder as prompted by the installer, click on "**Install**". This will install the application on your computer. On completing the installation, it will prompt you to select "**Finish**" to run the application.

3. Run the application on each host. The following dialog, notifying you that some licenses (for some plugins) were not found, will appear:

Registration Wizard	? ×
You will need on	e or several license files to use MestReNova
If you have already saved your license file(s) to your computer press the <i>Install</i> button to install it(them)	If you still need to get a license file, please select one of the following options:
Install	Eval Buy
Host ID: JBE32-3PX8B05L	F4W]]-XF7VC8A2

4a. If you want to make a trial, click on the 'Eval' button to be redirected to a website. Once there select if you want to do a 'Single Trial' or a Campus Trial':

Home // Free and fully-featured Mnova trial

# Free and fully-featured Mnova trial Ayone can try Mnova for free during 45 days by completing a very simple registration process. To start it just select the type of test you want to run. Image: select the type of test you wa

You will be redirected to a web page where you will be asked for a few registration details. An illustrative example appears below.

Products	
Mnova Suite	
Mnova NMR Mnova	NMRPredict Desktop 🗹 Mnova MS 🖉 Mnova Verify 🗹 Mnova DB
Others	
Mnova NMR Lite M	spin
Host ID	
Host ID •	How to get your Host ID (this field will normally be prefilled)
- Contact Details	
Salutation Nam	e · Surname ·
Please select	
Email •	Organization •
Country +	Market · Role ·
Please select	▼ Please select ▼ Please select ▼
ou will receive Mestrelab	newsletters, updates and promos
Tick this box if you do n	ot want to be informed of interesting features and new Mnova versions and plugins
GET A FREE EVALUATION LIC	ENSE

Your evaluation license will be generated after having clicked on 'Get a free evaluation license'.

4b. Alternately if you press the 'Buy' button you are again redirected to a web-page where a similar procedure occurs. However, instead of receiving a license right away your registration information and your Host ID number are automatically sent to our Sales Department by e-mail. They will handle your purchase request and, once the financial formalities are complete, you will receive your licence file with installation and activation instructions by e-mail.

4c. If you have already a license file, click on the 'Install' button and go to the step 8.

5. It will display a window (Step 2/4) to inform you that you will receive an email to confirm your details

Home // evaluate // single // Single trial - Form received

### Single trial – Form received

Thank you, we have properly received your form and sent you an auto-email so that you confirm your email address and details.

So please open the email we have sent to pablo@mestrec.com, click on the link included on the email and just confirm your data to download your license file.

Add us to your email address book

Make sure our emails end up in your inbox by adding the domains @mestrelab.com and @mestrec.com to your email address book or trusted-sender list

6. Once you have received the email, please click on the link to confirm that you are a human and **your email address and details are valid**. This will display a new window (Step 3/4) which will allow you to obtain your license file just by clicking on the 'Confirm email and download license files' button.

### Single Trial – Download your license and get started

You are now at the step 2. You just need to confirm your email address and you will get your license(s) file(s)

1. Fill in the form with your trial details

- 2. Confirm your email and details
- 3. Start your individual trial



2- Confirm your email and details

Click on the button below to confirm your email (pablo@mestrec.com) and download your license file for the Host ID: JBE32-3PX8B05L-F4WJJ-XF7VC8A2

Confirm email and download license files

7. Save the 'Evaluation License' file on your disc.

Trial Resources	1- Trial licenses and	l details.	
	Click here to download a requested.	I the license files	you have
1- Trial licenses details	The activation is really simp tip in case you need help.	e but you can cheo	ck this training
2- Learning to use the software			
3- Support	Trial licenses details for JBE32-3PX8B05L-F4W		
4- Purchase Mnova	Name	Tested	Expiry date
5- Email and newsletter management	Mnova NM	R Yes	2012-10-11
	Mnova		

### Single Trial – Download your license and get started

8. Drag&drop the license files to Mnova in order to activate it. You can also follow the menu ' Help/Get-Install Licenses' and click on 'Install' button.



9. This will open the 'Select License File' dialog (see the picture below). Navigate on your Windows browser until you find the license file (or a .zip file containing several licenses), and double click on it and select it. Now you should be able to run the application without receiving an error message dialog.

elect a Licens	e File			2
Buscar en:	C Lic	<u>-</u>	] 🗢 🖻 🗗 🗐	0
Documentos recientes Escritorio Vis documentos	MS.lic MS.lic MNR.lic NPL.lic	zip		
Mi PC	Nombre:	I	•	Abrir
	Tipo:	All Files (*.*)	-	Cancelar
		License Files (*.lic) License zipped Files (*.zip) All Files (*.*)		-

To install Mnova on Linux: download the Mnova SETUP file from a web address provided by us, and:

Debian, Ubuntu (\*.deb): type from the command line interface: dpkg -i namefile.deb Other (\*.rpm): type from the command line interface: rpm -i namefile.rpm

To update Mnova:

Debian, Ubuntu (\*.deb): type from the command line interface: dpkg -i namefile.deb Other (\*.rpm): type from the command line interface: rpm -U namefile.rpm


### How to uninstall Mnova?

To **uninstall Mnova** on Windows; navigate to the Mestrelab Research S.L\MestReNova folder and double-click on **'Uninst' \***. Finally confirm by clicking 'Yes'.

To uninstall Mnova on Mac, just move the application to the bin.

To uninstall Mnova in Linux:

Debian, Ubuntu (\*.deb): type from the command line interface: dpkg -r mestrenova Other (\*.rpm): type from the command line interface: rpm -e MestReNova

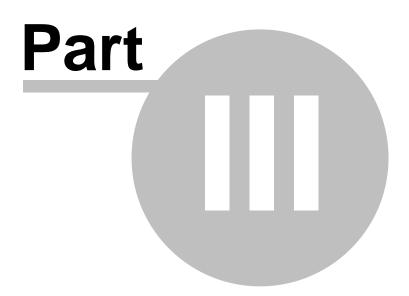

### 3 Mnova 11

### Welcome to Mnova 11

In our case, the fact that this is a *commercial release* means the following:

- 1.We have tested **Mnova** in-house as far as possible to make sure that we deliver to you a version which is robust, already of high quality, and which does not present any apparent bugs. However, you may find a small number of bugs which we have not yet identified. Please tell us about any you discover by e-mailing us at <a href="mailto:support@mestrelab.com">support@mestrelab.com</a>
- 2. There are some advanced functionalities which will be included in the forthcoming commercial releases, but which are not yet in this version. The reason for this is that, in order to bring you the advantages of Mnova as soon as possible, we are bringing you the core functionality and more, while we complete some advanced and important but less-used functions. As a valued user of Mnova you will be notified the moment these additional functions become available as upgrades. As a result of this you may find some features which were present in the final release of MestReC, our current application, are not yet implemented into this commercial version of Mnova. A list of such features, together with their planned time of inclusion in the software, can be found below.
- 3. Although we have now released the product commercially, we are, as ever, very interested in your feedback, bug reports and implementation suggestions. Please keep this coming, as we plan for continuous and rapid improvement of the application, to make forthcoming releases even more in tune with our customer needs.

### What's New? (click here to read the changelog)

### <u>Mnova NMR</u>

**Automatic Analysis** Denoising Use GSD knowledge in multipoint baseline correction Improved Reference Deconvolution Improved Group Delay Correction New preference to pop-up the table of when opening a new molecule Ability to apply layout templates to specific pages of a document **GSD** Parallelization Capability to report the 'Processing Template' Zero Filling and LP dialog has been improved Improvements in PCA to load/save 'preparation files' and integral regions Data Browser display experiment types Capability to open CNMR JCAMP-DX from Wiley Ability to setup 1D spectra as a trace in superimposed 2D spectra via drag&drop Import more parameters from Bruker TopSpin JCAMP files Special processing for the NUTS Type 1 files produced with Oxford Instruments software NUS processing has been improved so that 2D FID's can now (optionally) be reconstructed during importing. Support NUS spectra in JEOL format Drag and drop compatibility with new data storage format from VNMRJ3.2 FID reconstruction for Pure Shift experiments 1D traces in 2D spectra are updated automatically after applying Absolute Reference Script Import Directory Stack has been redesigned

Capability to select color of integral regions in Data Analysis

Auto track moving peaks (in Data Analysis) Correction for gradient nonlinearity in DOSY processing Ability to deactivate automatic DEPT processing (from Varian) New Preference for automatic PureShift reconstruction Improve "regions" autophasing for spectra with "hidden" regions New Shortcuts to delete integrals and peaks manually

### Improvements in the assignment tool

**Assisted Assignments** Capability to show 1H and 13C assignments in atom labels Report 13C peaks with multiplicity New icon to Delete Correlation option Assign multiplets when copying assign molecule to a new dataset Do not remove all correlations involved when deleting one of the shifts in case of ambiguous assignments Remove all correlations involved when deleting an assigned multiplet, peak or integral. H-H correlations between diastereotopic protons are deduced Remove all correlations involved when deleting the shift value of an assignment When assigning symmetric Hs only one of the Cs get assigned from the HSQC correlation Second H of a diastereotopic CH2 are deduced form the HSQC Ability to add overlapping multiplets by assigning to a 2D range Ability to turn off help pop-ups when using Assignment tool Improvements in the report assignments script Avoid message for transfer of 2D assignments to 1H multiplets when only a C is assigned Ability to recalculate the 2D deductions after making changes in the 2D spectra Multiplicity in 13C Peaks table is automatically filled according to the assignments In CH2 assignment if Ha is assigned show Hb label by default when assigning the second H Ability to delete assignments graphically from the spectrum

### Mnova MS

### Peak purity calculation

Capability to load/save the Peak Detection options Capability to specify the desired resolution to build the centroid spectrum Capability to load/save the Elemental Composition and Molecular Match settings Align traces automatically depending on the LCMS machine Improved vertical axis label for chromatograms New converter Advion MS data

### Mnova NMRPredict Desktop

Capability to select the default solvent reference in 19F and 15N NMR predictions Capability to update predicted spectra in stacked plots Ability to get highlighting like in Predict &Highlight using predictions read from a file via script Capability to calculate <sup>3</sup>J HNCH couplings New Random Forest Prediction

### Mnova Verify

Modify the name of the option to run Verification in single mode 2D peak picking independent of the visual threshold

### **Mnova Database**

Capability to add flags to database field definitions Set field 'Preview' instead of 'Chemical Structure' from Molecule item to be shown in DB Browser Port property in the DBClient

Need to wrap texts when displaying fields with long text string Auto-scale of row height to the content of the field Sample scripts for peak search and multiplet search in db Ability to store UV/DAD and ELSD chromatograms in a DB Capability to manage users from Active Directory Hide password when adding it to the DB connection dialog

### **Scripting Engine**

Add the function Dir.searchPaths Link annotations to spectral coordinates Ability to set several Pageltem properties Ability to set Pageltem's fill style Capability to get events from all engines Implement the function Pageltem.setLinkedItems Using Multiopen with Mnova files behaviour should be different Implement ability to modify the sampling scheme via scripting

### Molecular drawing

Show arrows for HMBC correlations with heteronuclei (15N, 29Si...) Chemical structure in a pop-up window Show PhysChem properties in columns Ability to rotate fragments of a molecule Prediction Data should be kept after editing the molecule with the Normalize Explicit Hydrogens Numbering command. Prediction Data should be kept after editing the molecule with the Normalize Numbering, Concatenate Numbering, Add/Remove/Normalize Explicit Hydrogens commands. Prediction Data should be kept after editing the molecule with the command. Ability to show correlation arrows by hovering the mouse over each atom Assignments data should be kept after editing the molecule with some of the commands Change the background color when selecting a cell in Compounds table Ability to change the font size of atom numbers from the molecule in Compounds table Rotating function Mirror function (top-down, left-right) Split a molecule and work with the parts individually Ability to edit a molecule from the Compounds table Capability to draw unknown stereobonds Table of Compounds opens automatically when importing a molecule Read molecule parameters from JCAMP

• ... and more minor bugs fixed.

Our plan is to distribute a new release approximately every four months. The functionalities you can expect to see added to the software during the intervening period are:

- Derivative Processing of Spectra
- GEN-2D NMR, Processing to Improve Resolution in the Indirect Dimension.
- Spectral Editing

- Graphical User Interface Enhancements
- New Analysis tools

We hope that you will find this version of Mnova to be one of the most complete NMR processing and analysis tools available in the market, combined with a revolutionary interface and many new, original and innovative features.

During the commercial release periods, we will welcome your **feedback**, both in the form of bug reports and also of implementation suggestions and feedback on current development. Please write with any of these to <u>support@mestrelab.com</u>

Thank you once again for your support of our development effort!




### 4 Shortcuts

Mnova provides shortcuts for finding commonly sought tools. You can see a list of these commands by following the menu 'Help/Shortcuts':

	Command	Shortcut	*
1	🧸 Analysis > Assignments > Manual Assignment	A	
2	Analysis > Assignments > Swap Assignments	S	
3	∬ Analysis > Integration > Manual	I	
4	🍌 Analysis > Multiplets Analysis > Manual	J	
5	🗶 Analysis > Peak Picking > Manual Threshold	к	
6	📌 Analysis > Peak Picking > Peak by Peak	Ctrl+K	
7		R	
8	X Analysis > Reference > Reference	L	
9	Close	Ctrl+F4	
10	${f T}$ Edit > Annotate > Text	т	1
11	Edit > Copy	Ctrl+C	
12	Sedit > Create New Page	Ctrl+M	
13	℅ Edit > Cut	Ctrl+X	
14	🗱 Edit > Delete	Del	
15	👔 Edit > Paste	Ctrl+V	
16	🥐 Edit > Redo	Ctrl+Y	
17	🔄 Edit > Select All	Ctrl+A	
18	🕈 Edit > Undo	Ctrl+Z	
19	🔀 File > Export to PDF	Ctrl+D	
20	File > New Document	Ctrl+N	
21	🔛 File > Open Directory	Ctrl+I	
22	🦰 File > Open	Ctrl+0	
23	🖶 File > Print	Ctrl+P	
24	拱 File > Save	Ctrl+S	
25	Help > Contents	Ctrl+F1	
26	Integral Manager	Shift+I	
27	Multiplet Manager	Shift+J	
28	Frocessing > Apodization	w	
29	A Processing > Baseline > Baseline Correction	В	
30	Processing > Fourier Transform	Shift+F	
31	✤ Processing > Phase Correction > Manual Correction	Shift+P	
32	+ View > Crosshair	c	
33	SA View > Cuts > Cut	x	
34	Niew > Cuts > Restore	v	E
35	Lev View > Expansion	E	
36	. ✓ View > Intensity > Decrease	-	
37	₩ View > Intensity > Fit to Highest Intensity	н	

2017 MESTRELAB RESEARCH

26

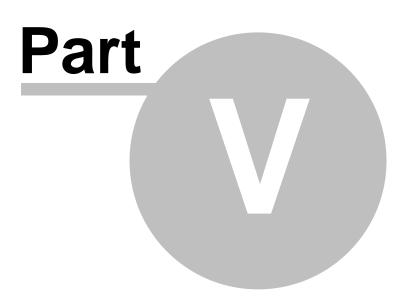


### 5 Fast Visual Guide to process routine 1D-NMR datasets

You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder)

Go through the following procedure to process a routine 1D-NMR spectrum:

1. Drag and drop the folder containing the FID file into Mnova to get your spectrum fully processed. If the folder contains a .mol file, the molecular structure will be also displayed. (You can also follow the menu 'File/Open')

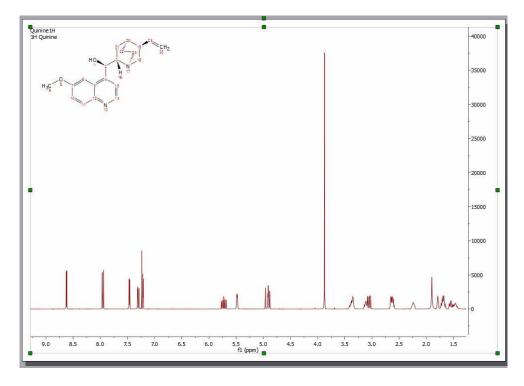


2. If your spectrum is not referenced, you can calibrate it by clicking on the 'Reference' button and then selecting the peak you want to be a reference point.


Old Shift:	7.25	2 ppm	1	Auto Tuning
New Shift:	7.26	0 ppm	\$	+/-: 0.100 ppm 🙄
🗹 Annotal	ion.	CDCI3		

3. Click on the 'Baseline Correction' icon Ker to correct the Baseline of your spectrum.

4. To paste the Parameters Table on the spectral window, just follow the menu: 'View/Table/ Parameters' and click on the **'Report'** icon. Please bear in mind that you can resize any object by just clicking and dragging on any border. In this case the spectrum has been resized in order to put the table at the right side of the page.

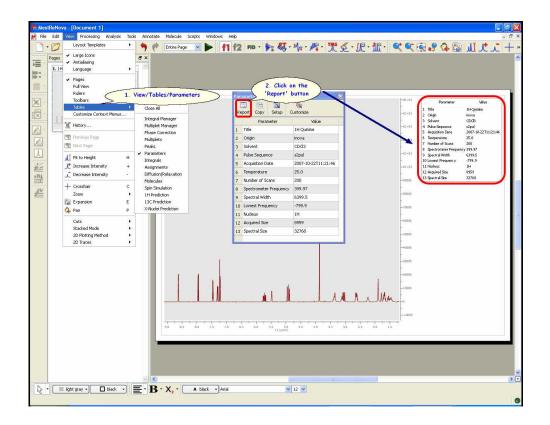


5. Apply an automatic multiplet analysis by clicking on the **'Multiplet Analysis'** icon **the 'Multiplet Analysis'**. It will apply an automatic Peak Picking analysis with solvent and impurities recognition. As you can see in the example below the CDCI3 signal has been detected and its peak label appears in red.

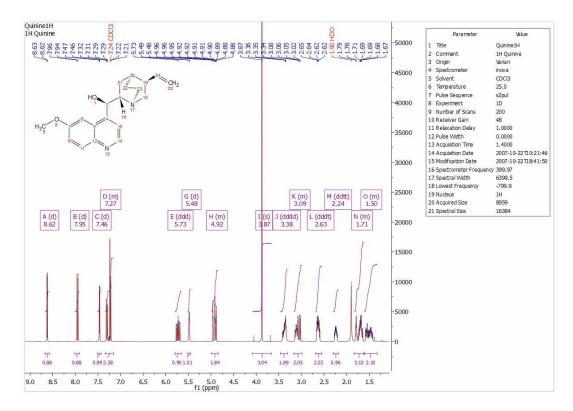

6. Double click on the multiplet box to normalize the 'multiplet integral' values:


Name:	J= 4.4 Hz,	IH) Class:	a	
9209406 j	3.623 ppm [		u	
J-List:				۵ 🗼
6	Purple	4 in molecul	•	Discard Peal
Nuclides:	-	. Thir moleces	Auto	)
	Integral: 1	.00		

7. To obtain the multiplet report list just right click on the multiplet box and select 'Report Multiplets':

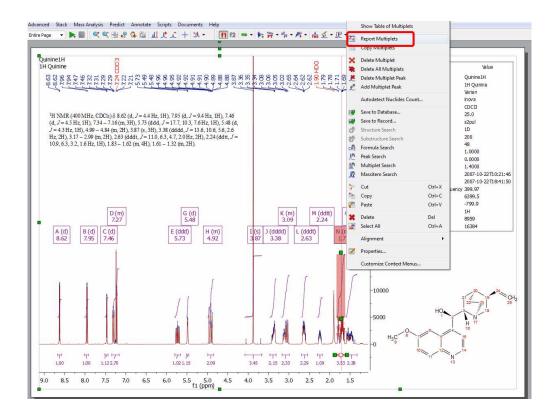

Please bear in mind that you can freely move any Mnova object just by clicking&dragging. In the example above we have moved the molecular structure and the multiplet report

8. You can copy the multiplet report to the clipboard by right clicking on the multiplet box and selecting 'Copy Multiplets' (or by selecting 'Copy Text' on the Multiplet Table) and then paste the report in another document just by using Ctrl+V (or Cmd+V in Mac).

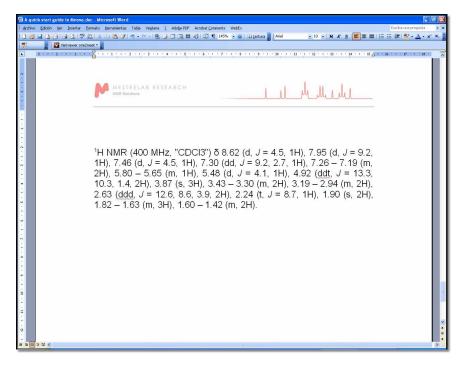

9. Finally, you will be able to save  $\blacksquare$ , print  $\boxdot$  or export to PDF  $\blacksquare$ , the document by clicking on the applicable icon in the toolbar.

### See also:

1D Processing Tour Fast Visual Guide to process routine 2D-NMR experimental data

Watch a miniclip on this functionality at this link




### 6 Fast Visual Guide to process routine 2D-NMR datasets

(Not available in Mnova Lite)

You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder)

The procedure to process a 2D-NMR spectrum is very similar with the monodimensional one:

1. Drag&drop the folder containing the spectral files or click on the **'Open File'** icon **'** and select the FID file (or SER file in Bruker) to obtain the processed 2D-NMR spectrum. **Mnova** will select the processing functions for you (FT, Phase Correction, etc) but, of course, you may change and optimize any of them and then re-process the data if you wish.

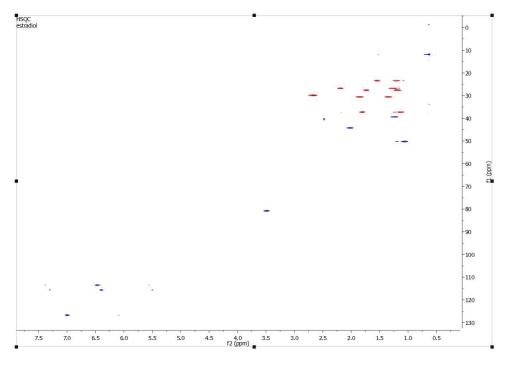

2. Mnova automatically detects the 1D spectra and use them as external traces of a 2D plot if the applicable option is checked under the 'Edit/Preferences/NMR/Import' menu.

If the 'Auto Attach Traces' option is not checked, you can drag and drop any currently opened 1D-NMR spectrum to a 2D NMR dataset in order to get them as traces. Here you can see how the page number 1, containing a 1H dataset is dropped to the HSQC to get the horizontal trace:



× -▲四日 豊米 · ● ● \* 送号 田舎 留放外 部九 小 い ● ● ----2.0 in. Drag&Drop the page 2 for the vertical trace (mdd) 70

> 5.0 4.5

The same can be done with the page 2 (containing a 13C spectrum) to get the vertical trace:

Here you can see the result:

7.0

6.5

6.0 5.5


15

0.5

2.5 2.0 1.5 1.0

3.0


4.0 f2 (ppm) 3.5

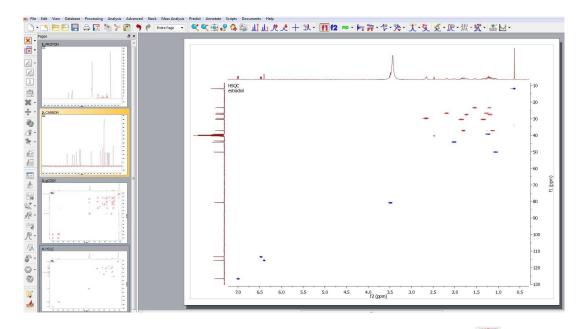


3. To calibrate your spectrum, just click on the '**Reference**' toolbar button  $\mathcal{I}$  and then select the peak you want to be a reference point. Finally, select the desired reference along f2 and then along f1:

Reference along f2	Reference along f1
f1         Old Shift:         7.215 ppm         2           New Shift:         7.215 ppm         \$	101.038 ppm           New Shift:           101.14 ppm
OK Cancel Solvents >>	OK Cancel Solvents >>


If you have your 1H and 13C NMR spectrum loaded, you can use the 'Absolute Reference' feature to reference 2D & C-13, by clicking on the 'Absolute Reference' button of the toolbar (or by following the menu 'Analysis/Absolute Reference'):

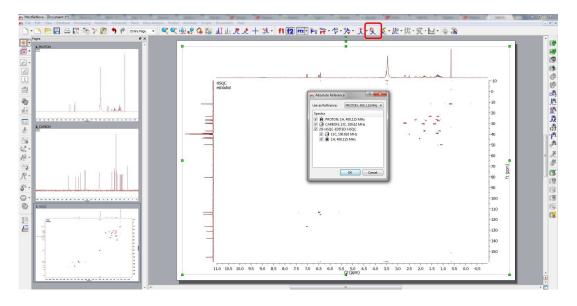

4. Click on the **'Peak Picking'** icon store to run a Peak Picking analysis and follow the menu 'View/ Tables/Parameters' to display the 'Parameters' Table'.

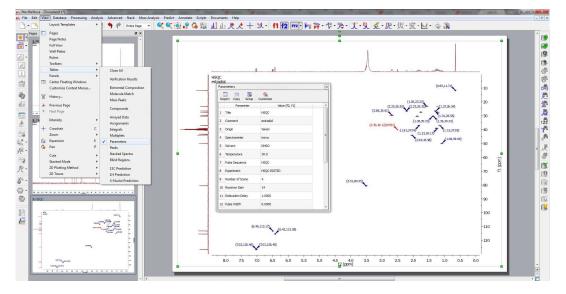

5. Then, click on the 'Report' button to paste the table on your page and move it to the right (by clicking&dragging). Finally resize the 2D spectrum to get the report below:

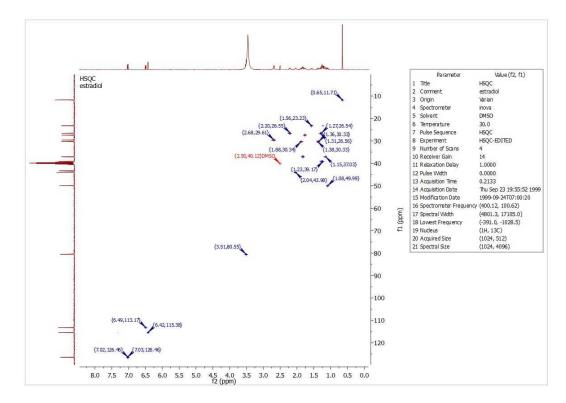

#### See also: <u>Fast Visual Guide to process routine 1D-NMR experimental data</u> <u>1D Processing Tour</u> <u>2D Processing Tour</u>

Manual Phase Correction in 2D-NMR


Watch a miniclip on this functionality at this link



# 7 The Mnova interface

The **Mnova** interface has been designed to minimize the learning curve for the new user, by capitalizing on familiarity and commonality with some of the most commonly used general software packages on the market. The interface consists of a main page window with a menu bar, toolbars, dialog boxes, rulers, active window tabs, etc. giving users total flexibility in the organization of their data. With **Mnova** you will only need a couple of mouse clicks to open and process your NMR data automatically. When you first open **Mnova**, you will immediately notice a few things which represent the fundamental graphical principles of the program:

- First of all, the software is multipage, à la Powerpoint.
- The **Mnova** Graphical User Interface is based on the 'What You See Is What You Get' principle ( **WYSIWYG**).
- The **Mnova** graphical engine makes extensive use of the anti-aliasing technique to produce very high quality spectral plotting.

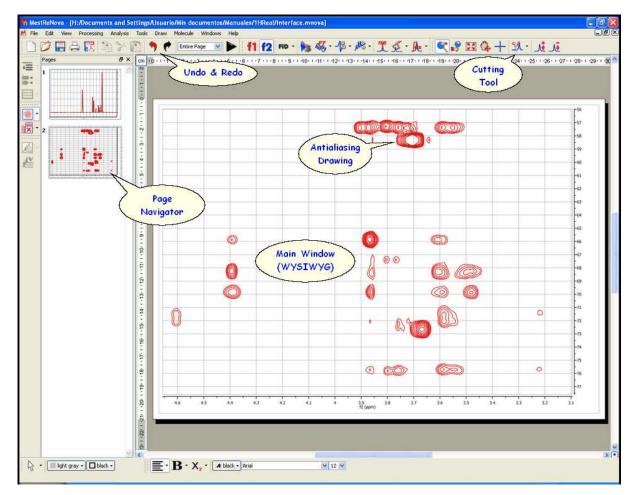

• The program includes a powerful Undo/Redo mechanism within a standard toolbar.

In a few minutes you will gain a good command of the most powerful and modern tools provided by Mnova, such as:

- One single command to open and process FIDs in any file format
- Powerful drawing tools with advanced text editing capabilities.
- Cutting tool to exclude uninteresting regions from the spectrum.
- Powerful scripting engine.
- Molecular viewer with assignment capabilities.
- Prediction of 1H and 13C NMR from chemical structures.
- And much more...


#### See also:

Multipage Software Working on a single page Zooming Cutting Undo & Redo Graphics & Annotations

### 7.1 Multipage Software

The **Mnova interface** is designed to look and feel like **MS PowerPoint**. We think that the great majority of people in science are familiar with this presentation and reporting software, and that making our program behave in a very similar way to Powerpoint will ensure that even new users find it very easy to work with from the very start.

The first thing you will notice is that the software is **Multipage**, and incorporates a **page navigator**, which is placed, by default, as a column on the left hand side of the screen.

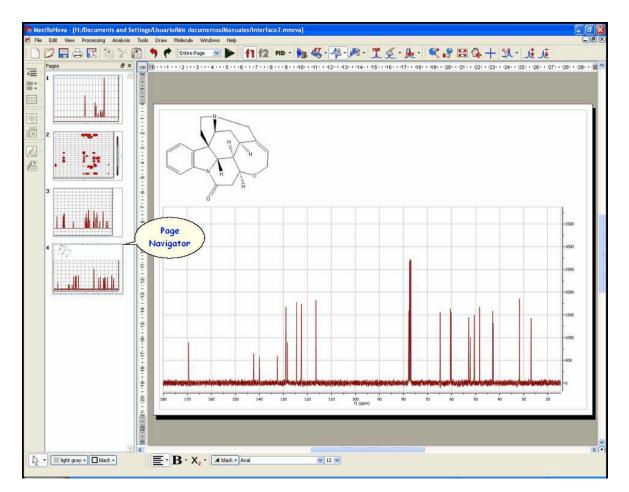

The **Mnova document** is a **Multipage Document**. This means that *all pages within a single document will be saved as a single document*. This will allow you to keep, for example, different experiments for a certain sample (<sup>1</sup>H, <sup>13</sup>C, homonuclear and heteronuclear 2D correlations) as a single, unified document.


The active slide is highlighted in blue, and will appear in the main paper area of the document. This is the page to which all selected operations will be applied. You can choose the desired spectrum just by clicking on it on the page navigator or by following the menu 'View/Previous or Next Page'. In the same way, if you have highlighted any spectrum in the page navigator, you can move to the previous or the next spectrum by using the up or down arrow keys.

There are a number of things you can achieve by working on the page navigator:

- ✓ You can alter the order of the pages by left clicking on a page, dragging it and releasing the mouse to drop it at the desired position.
- ✓ You can Create a New Page by selecting 'Edit/Create New Page', by right clicking on the page navigator window and selecting 'Create New Page' or by holding <Ctrl>+M (or Cmd + M in Mac).
- ✓ You can Delete an undesired spectrum by 'Edit/Delete" or by right clicking on the spectrum or on the page navigator and selecting 'Delete'. A selected spectrum can also be deleted using the 'Del' key.
- ✓ You can select more than one page by holding the <Ctrl> key (or Cmd in Mac) whilst clicking on the desired pages. When more than one page is selected, all operations (zooming, cutting, processing, etc.) will be applied to all selected pages.
- ✓ You can copy a page to the clipboard by pressing the <Ctrl> key (or Cmd in Mac) and then left clicking on the desired page, then dragging and releasing it whilst still holding <Ctrl> (or Cmd in Mac). Of course, a page can also be copied by selecting it and then choosing 'Edit/Copy', or <Right</p>

Click> and then Copy or by using the keyboard shortcut <Ctrl+C> (or Cmd+C for Mac). Any of these methods can be followed to copy one or several pages at a time, depending on what is selected when applying these operations.

- ✓ Conversely, a page or several pages can be pasted by using 'Edit/Paste', or <Right Click> and then Paste or by using the keyboard shortcut <Ctrl+V> (or Cmd+V for Mac).
- ✓ Finally, you can hide or move the page navigator, by clicking on the boxes highlighted on the picture below (or by following the menu 'View/Pages').

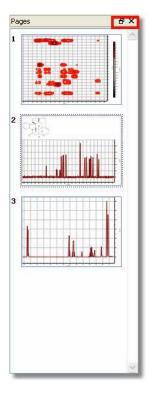

In order to navigate from one page to the other, you can use the page navigator or the arrows controls shown in the picture below (at the right down corner of the spectral window). You will be able to show the page navigator by clicking on the last button of the picture below:




You can edit the title of the spectrum shown in the page navigator by right clicking on it and selecting ' Edit Page Title' or by following the 'Edit menu':

		👫 Edit Page Title 🛛 🛜 🔀
°r Cut	Ctrl+X	Title
🏠 Сору	Ctrl+C	Quinine HSQC NMR
🗶 Delete	Del	
Select All	Ctrl+A	
📑 Create New Page	Ctrl+M	OK Cancel
Edit Page Title		

# 7.2 Working on a Single Page

Whilst **Mnova** is a multipage document, it also allows you to have several objects (e.g. spectra) within a single page. The easiest way of placing two spectra on the same page is to simply select one of them, copy it (**'Edit/Copy'**, <Right Click> and **Copy** or <Ctrl+C> (or Cmd+C for Mac)) and then paste it directly on the desired page (Select the desired page and press 'Edit/Paste', <Right Click> and **Paste** or <Ctrl+V> (or Cmd+V in Mac)).

Note that the **active object** is highlighted with **green squares** (in the green circle in the figure below). Any **Mnova** object can be **resized** and **moved** by just clicking and dragging on the corner boxes or on the object respectively. Note also that any other objects selected but not active will be highlighted with white squares (in a blue circle in the figure below) (To select more than one object, hold the <Ctrl> (or Cmd in Mac) key while clicking on the desired objects. To select all objects on a page, just choose 'Edit/Select All' or the keyboard shortcut <Ctrl+A> (or Cmd+A in Mac).

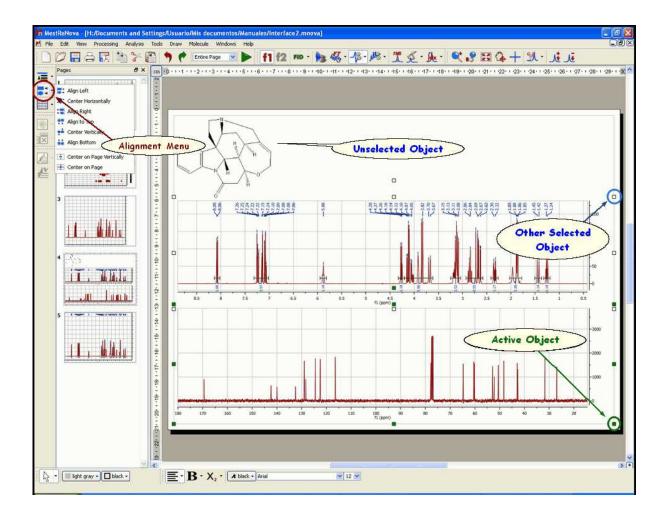

Once more than one object (spectrum or otherwise) has been placed on the same page, it can be manipulated and placed on the page by using the scroll menu shown in the figure below, accessible via the **'Alignment'** icon



This scroll menu will allow you to Align Left, Right, Top and Bottom, to Center Horizontally or Vertically (applying this last operation with multiple objects selected will Superimpose them). Of course, you can move the spectrum selected in a given direction using the arrow keys of your keyboard. Remember that multiple objects must have been selected for these commands to work effectively. You can also superimpose several spectra by using the 'Superimpose' feature.


Utilities The superimpose option is very useful when attempting to identify a known compound present in a complex mixture or when comparing similar compounds.

Any operations applied to the active object will also be applied to the other selected objects (zooming, panning, cutting, processing operations, etc) as was the case with multiple pages selected.

If the Mnova document is huge and contains several pages, you can save only some of the pages, by selecting them in the page navigator and following the menu 'File/Saves as/MestReNova Pages (\*.mnpag)'

### 7.3 Data Browser

As you know, you can load datasets into Mnova just by dragging&dropping the folder(s) containing the raw data. Alternatively, you can just load the FID by following the 'File/Open' (Ctrl/Cmd +O as a shortcut) and since Mnova 9.1.0, you could also use the Data Browser to load your datasets, just by double clicking on the applicable folder (or by dragging&dropping):

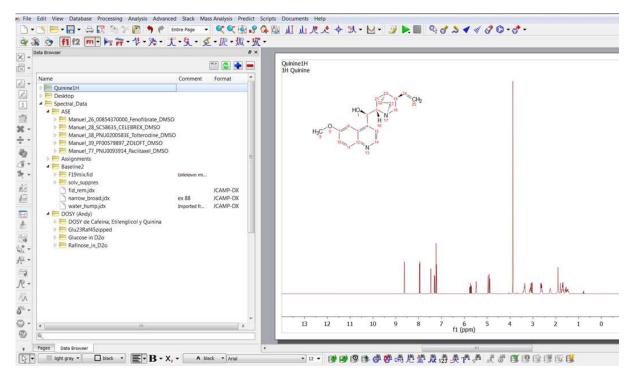

If the Data Browser is not displayed on your screen, just follow the menu 'View/Panel/Data Browser'.

You can register several data locations just by clicking on the applicable button or by dragging and dropping (into the browser) the folder containing the datasets:



These data locations are the same as in "Edit/Preferences/General/Open&Save/Open Locations".

The data browser will handle all spectral and molecule formats from all vendors, but the user will be entitled to filter some of the formats:

and and	ile Format Filt				3 <u></u>	
	File Formats					
				Format		•
	AB SCIEX	(Analyst (*.wiff	.)			=
	AB SCIEX	Data Explorer	(*.dat *.t2d)			
	🔽 Agilent C	hemStation (*.	ms *.ch)			
	🔽 Agilent Io	on Trap (*.yep)				
	🔽 Agilent N	/lassHunter (*.b	oin)			
	Bruker As	spect 2000/300	0 (*.*)			
	Bruker Co	ompass (analys	is.baf fid <mark>s</mark> er	)		
	Bruker UX	XNMR/XWIN-N	IM <mark>R (fid 1r s</mark>	er 2rr)		
	🔽 Bruker W	IN-NMR (*.fid	*.ser *.1r *.r <mark>r</mark> )			
	CS Chem	Draw (*.cdx)				
	GE/Nicol	et (*.*)				
	Galactic ( Check All	(*.spc) Uncheck All	]			*
	Wildcards					
	Whitelist:					
	Blacklist: *.tx	t *.csv *.xml *.*	• *			

In case of Bruker datasets all openable data will be listed in the tree view: fid and all 1r's or ser and all 2rr's. The spectral titles will be shown directly in the panel and also be available as tool-tips. Hovering the cursor over the spectra folder or fid/ser file related will display some information. In case of Bruker files, the parm.txt file is shown as tooltip. In case of Varian files, the content of Comment field will be displayed.


			<b>**</b>
Name	NAME Manuel_77_PNU0093914_DMSO	mment	Format
	EXPNO 24 PROCNO 1 Date_ 20110410 Time 9.27 INSTRUM av600 PROBHD 5 mm CPTCI 1H- PULPROG hmbcetgpl2nd TD 2048 SOLVENT DMSO NS 4 DS 16 SWH 9615.385 Hz FIDRES 4.695012 Hz AQ 0.1065980 sec RG 1024 DW 52.000 usec DE 6.00 usec	Quinine tled 2co ak_HSQC ROTON ak_COSY ak TOCS	Zip Files Varian VNMR Molfile
<ul> <li>▲ ➡ pd</li> <li>▲ ➡</li> <li>▲ ➡<td>TE 300.0 K CNST6 120.0000000 CNST7 165.0000000 CNST38 8.0000000 CNST30 0.5981128 D0 0.00000300 sec D1 1.5000000 sec D6 0.06250000 sec D16 0.00020000 sec IN0 0.00001380 sec</td><td>ak_TOCS</td><td>Bruker UXNMR/XWIN-NMR Bruker UXNMR/XWIN-NMR Bruker UXNMR/XWIN-NMR</td></li></ul>	TE 300.0 K CNST6 120.0000000 CNST7 165.0000000 CNST38 8.0000000 CNST30 0.5981128 D0 0.00000300 sec D1 1.5000000 sec D6 0.06250000 sec D16 0.00020000 sec IN0 0.00001380 sec	ak_TOCS	Bruker UXNMR/XWIN-NMR Bruker UXNMR/XWIN-NMR Bruker UXNMR/XWIN-NMR

At the bottom of the Data Browser you will find a 'search feature' that will work with wildcards and strings in the same way. For example, you will get the same result by typing ".mol" or "\*.mol" in the search cell, and both searches take equal time:

III		•				
bl		*				
Data Bro Search by wildcard						

## 7.4 Mnova Menus & Toolbars


The graphical user interface is the part of Mnova that you interact with to perform tasks; it consists of a main page window, page navigator, menus, toolbars, dialog boxes... giving users total flexibility in the organization of their data.

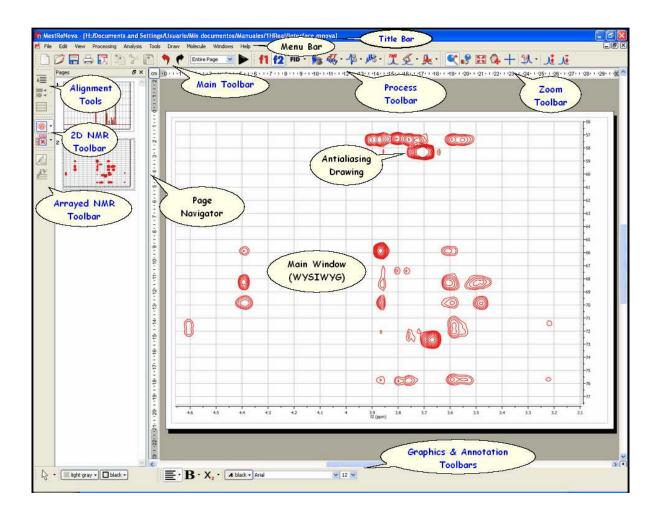

Title Bar: This blue bar shows the name of the active document

**Menu and Toolbars:** All Mnova commands and functions can be accessed from the menus and toolbars. The toolbars contain icons which offer shortcuts to many commonly used functions (you can select which ever toolbars you would like to display from the View menu). The user will be able to change the location of the toolbars to anywhere in the screen just by clicking on the border and dragging. Menu and toolbars are <u>fully customizable</u>

**File Menu:** In addition to the usual File commands (such as: 'New', 'Open', 'Open Directory', 'Close', 'Save', 'Save as', 'Page setup', 'Print' or 'Exit') you will find:

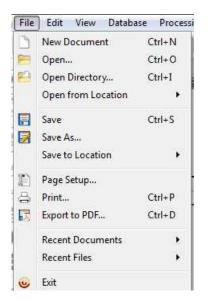

Mnova is able to import several spectral formats, image files and molecular structures (.mol) as you can see in the picture below:

All Files (*.*)	
MestReNova Document (*.mnova)	
MestReNova Layout Template (*.mnlt)	
Bruker Aspect 2000/3000 (*.*)	
Bruker UXNMR/XWIN-NMR (fid 1r ser 2rr)	4
Bruker WIN-NMR (*.fid *.ser *.1r *.rr)	1
GE/Nicolet (*.*)	-I
Image Files (".bmp *.gif *.jpg *.jpeg *.png *.pbm *.pgm *.pp JCAMP-DX (*.jcamp *.dx *.jdx *.jcm)	I
JEOL Alice (*.als)	-I
JEOL Delta (*.*)	-I
JEOL EX/GX (*.gxd)	-I
JEOL Lambda (*.nmfid *.nmdata *.nmf *.nmd)	-I
MestReC (*.mrc)	-I
Molfiles (*.mol)	-I
Nuts (*.*)	-I
Old Gemini (*.*)	-I
Siemens Magnetom Vision (*.raw)	-I
SwaN-MR (*.*)	-I
Tecmag (*.tnt)	1
Varian Gemini/VXR from VHelper (*)	1
Varian VNMR (fid)	
Varian/Chemagnetics Spinsight (data)	

Please bear in mind that the user will also be able to load any spectrum from the command line, just by typing the path where the Mnova exe file is located, followed by the path where the FID (or ser) file is stored. For example:

"C:\Programs Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" "C:\Documents and Settings\User\My documents\1HReal\fid"

The user will be able to save the spectra in different formats by following the menu 'File/Save as', as you can see in the picture below:

MestReNova Document (*.mnova)	~
MestReNova Layout Template (*.mnlt)	
ASCII Text File (*.txt)	
Adobe PDF Files (*.pdf)	
BMP Image Files (*.bmp)	
Encapsulated PostScript (*.eps)	
Enhanced Metafile (*.emf)	
JCAMP-DX (*.jcamp)	
JPEG Image Files (*.jpeg)	
MestReC (*.mrc)	
MestReNova Integral Regions (*.txt)	
MestReNova Integrals (*.txt)	
MestReNova Peaks (*.txt)	
PNG Image Files (*.png)	
PPM Image Files (*.ppm)	1.1
PostScript (*.ps)	
SVG Image Files (*.svg)	
TIFF Image Files (*.tiff)	
XBM Image Files (*.xbm)	1200
XPM Image Files (*.xpm)	~

Please bear in mind that you can also save the integral regions, the peaks and the template used in your document by using this command.


**'Export to PDF'**: This is a useful option to convert your Mnova document to PDF. You will be able to export the 'Current Page', the 'Selected Pages' or the 'Whole Document':

	? 🛛
<ul> <li>O Selected Pages</li> </ul>	Whole Document
	Cancel
	⊙ Selected Pages ○

Follow the 'Edit/Preferences/General/Print&PDF' menu to select the PDF export resolution.

'Recent Documents' & 'Recent Files': Dragging the mouse to these options you will able to select the most recent documents or files.

Edit Menu: In addition to the usual Edit Functions (such as Cut, Copy, Paste, Paste Special, Insert Object,...) you will find:

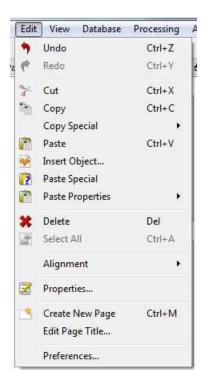


<u>'Undo & Redo'</u>: Mnova implements very powerful Undo and Redo capabilities. If you select 'Undo', Mnova will reverse the last change done to the document, restoring it to its previous state. The Redo command reverses the undo. These tools are incorporated in the Standard Toolbar, so they will be fully described further on.

Copy Special: to copy the dataset just as an image (very useful for large datasets), without OLE properties but reducing the file size of the document.

Insert Object: to insert any other object from a third application.

Paste Special: to paste from the clipboard any object copied in a third application.

You can copy&paste the spectral properties or the regions from one spectrum to another, just by pressing 'Ctrl/Cmd+C' in the original spectrum and then following the menu 'Edit/Paste Properties' in the other spectrum (or spectra, if you have previously selected them in the page navigator):




**'Delete'**: This command is used to delete a spectrum. Alternatively, a spectrum can be deleted by right clicking on it and then selecting **Delete** on the pop-up menu or by using the 'Delete' key while the spectrum is selected.

**'Select All'**: Selects all spectra on the same page. This command is very useful when, for example, the user needs to apply the same processing to all spectra simultaneously.

'Alignment': The Alignment sub-menu is frequently used to neatly align spectra. To use the alignment toolbar, click on the spectra to be aligned and then press the alignment control desired. The alignment command will apply only to the selected spectra.


By clicking on this item, a sub-menu window will open and the user will be able to align (or otherwise manipulate) several selected spectra on the same page.




This menu will allow the user to 'Bring to Front' or 'Send to Back' a selected spectrum (or an object) as well as 'Bring Up' or 'Bring Down' it.


This menu allows the user to determine how items on a page (generally spectra) or items within a spectrum (chemical structures, titles, expansion spectra etc) are positioned with regard to overlapping.

The documents may have multiple layers, hence we have the commands 'Bring to Front', 'Send to Back' as well as 'Bring Up' (a level) or 'Send Down' (a level). The tool 'Send to Back' is also very useful to create 'semi-transparent' shapes, as you can see in the picture below:

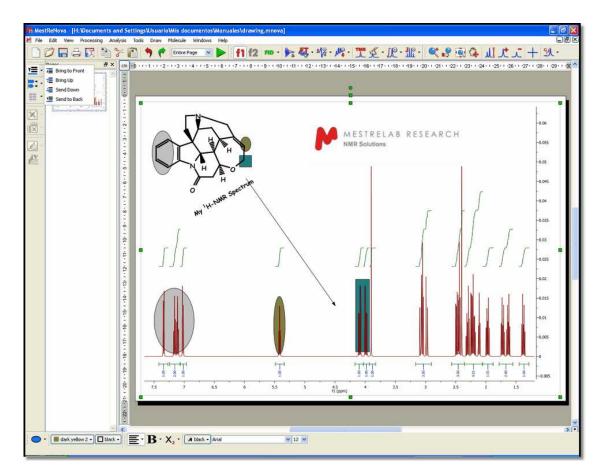

In the same way, the user can 'Align Left', Right, Top and Bottom, and 'Center Horizontally' or Vertically (applying this last operation with multiple objects selected will Superimpose them). The user can also center the selected spectrum (or spectra) on the page (vertically and horizontally). Finally the user can apply the functions 'Tile Vertically' and 'Tile Horizontally' to separate the spectra on the same page (as shown below).

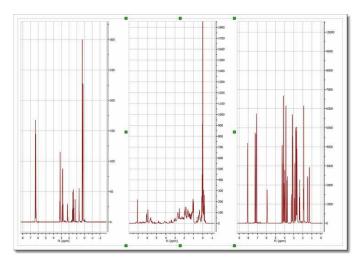

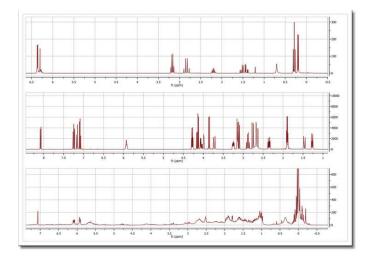


Alignment tools can also be found on the left vertical toolbar area.

<u>Properties</u>: Mnova will allow the user to customize nearly all the attributes of the spectrum. The user can select the properties of the spectrum by following the menu 'Edit/Properties' or by double clicking the left mouse button or pressing the right mouse button on the spectrum display and selecting '*Properties*' from the *pop-up* menu.

The user will be able to save his/her own properties just by clicking on the **Save Properties**' icon . The Saved Properties will be opened by clicking on the '**Load Properties**' icon (red square in the picture above).

We will not go into further detail here since all the property pages should be self-explanatory and a description of each one can be found in its applicable section of this manual and in this <u>chapter</u>

**Edit Page Title:** you can edit the title of the page shown in the page navigator by right clicking on it and selecting 'Edit Page Title' or by following the 'Edit menu' (please bear in mind that the title of the spectrum can not be changed due to integrity reasons):



The 'Edit Page Title' dialog box will be displayed and you will be able to select or type the desired title of the 'Page'

Edit Page Title	?
Title	
H:/Documents and Set Quinine 1H 1H Quinine	tings/Usuario/Escritorio/Quinine 1H/fid
	OK Cancel

This window will contain the 'Data File Name', the 'Title' and the 'Comment' which appears in the Parameters Table:

1.15	port Copy Set				
1	Parameter	Value	1		
	Data File Name	H:/Documents and Settings/Usuario/Escritorio/Quinine 1H/fid	l		
	Title	Quinine 1H	I		
	Comment	1H Quinine			
ł	origin	Variari	1		
5	Spectrometer	inova			
6	Solvent	CDCl3			
7	Temperature	25.0			
8	Pulse Sequence	s2pul			
9	Number of Scans	200			
10	Receiver Gain	48			

Please bear in mind that the comment of the 'Parameters Table' will be updated on the 'Edit Page Title' until you click on the 'OK' button of the 'Edit Page Title' dialog box (at this moment the comment will be fixed and the changes made in the 'Parameters Table' will no longer be updated to the 'Edit Page Title' window).

**Preferences:** From this window, you will be able to change the options of the Mnova Interface, plugins, NMR and drawing tools.



See also: Prefrences.

**View Menu:** The 'View' menu is where the user may select which toolbars, tables, rulers... are visible. In addition, it has other commands, such as:

	Layout Templates	3 <b>)</b>				
-	Large Icons					
	Antialiasing					
_	Language	•				
	Pages					
	Full View					
	Rulers					
	Toolbars					
	Tables	•				
	Panels	()				
	Center Floating Windows					
	Customize Context Menus					
T	History					
2	Previous Page					
W.	Next Page					
IL	Fit to Height	н				
	Increase Intensity					
	Decrease Intensity	373				
+	Crosshair	C				
	Zoom					
	Expansion	E				
0	Pan	P				
	Cuts					
	Stacked Mode					
	2D Plotting Method	•				
	2D Traces					

'Pages': This option allows the user to remove the page navigator (activated by default).

**'Full View'**: (Not to be confused with 'Full Spectrum) will bring up a miniature view of the entire working document with the active area of the spectrum highlighted in blue, as you can see in the picture below:

th Mes	tReNova - [H:/Documents and Setting	s/Usua	ario/Mis documentos/Manuales/Quinine	<b>Visual Verification</b>	.mnova]				
File 🕅	Edit View Processing Analysis Tool	; Drav							_ 8 ×
		9 (	🥐 Entire Page 💌 🕨 🚹 f 2	FID - 涛 👯	· 1/4 · 1/4 · 1 1 2 5 ·	12 · 111 · 11. +	🦿 🗣 😰 🐍	JI.	ti
	Pages & ×	cm I -	1 1 0 1 1 2 1 3 1 4 1 5 1 6 1 7						
<b>⊼</b> ≣ •	1. js1pquin	•	<i>4</i> –						1
5		-	5.8		8388	7	88		
- 33	-292-	- 0	16.8		208 201 201 201 201 201 201 201 201 201 201	ż	128		
	a a a l	-					["		
		-					-+00		
		-	29-23-24				100	8	
	2. js1pmquin	40							
	25 <sup>20</sup> - 1	9	13. 18-15	19			-330	0	
14		2	H	18			Ĩ.		
N	12	-					-300	0	
10 E		-	~						
学が思い		on -					-250	0	
36	3. js1pmquin	9	A (d) 8.71		B (dd) 8.00	)	⊂(d) 7.51	Istoq	
	200-	÷					-200	•	
	The state of the state state of the state state of the st	12							
		1.1					-150	0	
	and the second s	14 1 13			ſ		-		
					J		-100	di C	
	×	- 15			()		-		
	Integrals 8 ×	18							
	Report Copy Delete Setup	- 12			- 11		- M		
	Range Normalized Absolute	- 18	H		H	-			
	1 8.778.65 1.00 23251.18	92 -	9		101		1.03		
	2 8.08 7.95 1.01 23393.62	8	8.8 8.7 8.6 8	5 84 83	8.2 8.1 8.0 F1 (ppm) 8.0	7.9 7.8 7.7 7	6 7.5 7.4		
	3 7.56 7.45 1.09 25266.96	- &			•				
		<							D O
	Full Yew								8×
					Í.			1	
								-	
			I I I I			an a Mar .		-	
	a - a - a - a			a an ataa a	<u> </u>	2	a		
8.	• 🔳 light gra • 🔲 black • 📃 •	В·	X2 - A black - Arial	12 🔽					
									0
_		_							

You will be able to toggle the Full View window by using the F2 key. This will allow you to get a 'Super Fast' panning.

See also: Full View.

'Rulers': Click here to show or hide the rulers.

**'Toolbars'**: This item of the 'View' menu allows the user to select which toolbars are visible on screen. Click the name of a toolbar to select it for display. Click again to deselect. You can attach a toolbar to any side of the graphical interface by dragging it to where you want it attached.

ĝ	NMR Process				
	NMR Zoom				
	2D NMR				
	Arrayed NMR	2			
	Drawing				
	Drawing Text				

**'Main'**: This toolbar contains the standard file operations 'New', 'Open', 'Save', 'Print Tools' and 'Export to PDF', the editing operations 'Copy', 'Cut', 'Paste', 'Undo' and 'Redo', and the 'Page Width' drop-down menu which will be fully described in the zooming chapter.



'NMR Processina':

'Alignment': Contains all the alignment tools. These commands are duplicated on the 'Edit' menu.



This toolbar contains the

most frequently used NMR processing tools..

The 'f1' and 'f2' commands are used to set the processing frequency dimension (f1 or f2).

'FID': to see the **original FID** or the **processed FID** (FID') by clicking on the appropriate sub-menu item on the FID-icon side-bar. There are several further options in the scroll-down menus which will be fully described in the <u>Processing Chapter</u>.

"<u>Apodization</u>" (or *window function processing*): Windowing is a technique for manipulating the FID to either remove the "sinc" wiggles from the peak bases resulting from the truncation of the FID (apodization) or optimize the spectral resolution or remove various other acquisition artifacts or any combination of the above. You can find a full description of this tool further on in the <u>Fourier Transform</u> chapter.

<u>'FT'</u>: This command transforms the time domain FID into the frequency domain spectrum. It will be described in detail in the <u>Fourier Transform</u> chapter.

<u>'Phase Correction'</u>: This process adds constant (`Zero Order') and linear (First Order about the pivot point) phase to the spectrum in order to obtain pure phase line-shapes. If you click on this icon, Mnova will carry out an automatic phase correction. This process will be described further in its applicable chapter ('Phase Correction').

<u>'Baseline Correction'</u>: This is a very important processing step to obtain good quality spectra, with all the signals connected by a flat line. Mnova will apply an automatic baseline correction if the user clicks on this icon. If you are interested in studying <u>'Baseline Correction' in Mnova</u> in depth, please refer to the applicable chapter in this manual.

**'Reference'** : Click on this icon to calibrate your spectrum by assigning the position of an internal standard (such as TMS or a solvent peak). Mnova offers you a list of the most common deuterated solvent chemical shifts to calibrate the spectrum. Again, you can find a full description of this tool further on in the **'Chemical Shift Referencing'** chapter.

<u>'Peak Picking'</u>: Clicking on this tool will select all the peaks in the spectrum using a default threshold, mark them, indicate their chemical shifts and tabulate the shifts. You can find an advanced description of this tool in the <u>applicable chapter</u>.

<u>'Integration'</u>: Integration is used to estimate the number of species (e.g. protons) associated with a peak in the spectrum. Manual and fully automatic routines are available. Please read the '<u>Integration'</u> chapter for more information about this tool.



This toolbar contains the following functions:

'Zooming': This tool is used to expand the spectral regions on screen. Mnova incorporates several

ways of zooming, such as zoom in, manual zoom, full spectrum, and panning.


'Fit to Height' and <u>'Increase and Decrease Intensity'</u>: These tools scale the data of your NMR spectrum

'<u>Crosshair</u>': These two orthogonal lines forming a crosshair are available on the 'View' menu (or by pressing the <c> key) for reporting positional information, and for help in visualizing peak alignments.


'<u>Cutting</u>': Allows the user to hide regions of the spectrum, when they are of no interest. These tools are fully described in later chapters.




**'2D NMR'**: This toolbar contains the plotting methods for 2D NMR display. Mnova incorporates four 2D-NMR spectra representation modes. The most commonly used mode is the 'Contour Plot'. T his representation provides a good global view of the data points and allows a precise location of all signals (except the weakest). Nevertheless, the relative intensities and the multiplet structure of many signals can be difficult to interpret. In the following picture, a section of a spectrum in Contour Plot is shown:




A faster alternative in computational terms is the 'Bitmap Plot'. Mnova uses this representation as a default mode; the intensity of each point is represented by a colored scale, thus making relative intensities easier to interpret. If only positive intensities are plotted, the color scale is from red (high intensity) to blue (low intensity). In the figure below, you can see a spectrum shown in Bitmap Plot:



A '**Stacked Plot'** provides a *pseudo-3D* visualization of the data. This kind of representation is useful for revealing weaker signals and for comparing the intensities of different signals in the spectrum. A stacked plot is shown below:



'Whitewashed Stacked Plot': In the called 'Stacked Plot' mode, all the individual traces that compose a 2D experiment or an arrayed experiment are superimposed on each other, so it can be difficult to obtain a clear view. However, this problem can be avoided using the 'Whitewashed Stacked' mode. In this mode all the individual traces are plotted, but the traces are not "transparent", so that the characteristic 3D look is obtained. The contrast between the 'Stacked Plot' and 'Whitewashed Stacked' modes can be appreciated in the figure below.

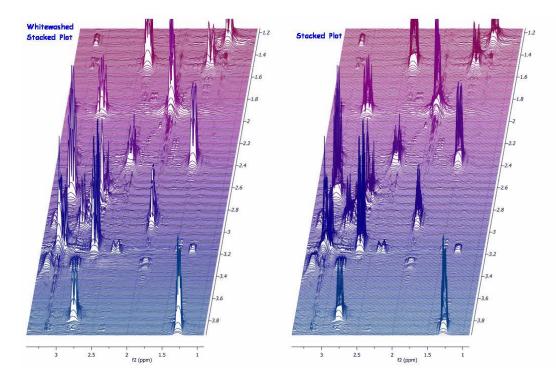

**'Show traces'**: this tool allows the user to show and setup the vertical and horizontal traces of a bidimensional spectrum. The user can increase or decrease the intensity of the traces simply by scrolling the mouse wheel (windows only for the moment) after hovering the cursor over the desired trace. To move the trace hold the Shift key down while scrolling the mouse wheel over the trace.

<u>'Stacked NMR:</u> Mnova includes a general-purpose fitting module designed to analyze stacked experiments such as relaxation, kinetics or DOSY experiments, using a robust working environment. The user can find a full description of this tool further on in the <u>Stacked NMR</u> tutorial.

**'Drawing'**: You can draw an object by using these tools. You can choose the line color (default is black) and the fill color (default is light grey).

**'Drawing Text'**:  $B \cdot X_{2} \cdot A = B \cdot X_{2}$ 

'<u>Tables</u>': **Mnova** groups all spectra-relevant information into the so-called '**Tables Window'**, available from the **View** menu. This option allows the user to see the spectral parameters (Acquisition Parameters are selected in the figure below), or Peaks (shown in the blue square), Integrals (in the red ellipse) or any of the other parameter classes as indicated on the tabs at the lower edge of the window.

	Parameter 🔺	f1	
1	Acquired Size	32768	
2	Lowest Frequency	-1280.631	
3	Origin	UXNMR, Bruker Analytische Messtechnik Gmb	н
4	Owner	rgry	
5	Pulse Sequence	2g30	
6	Solvent	CDCI3	
7	Spectral Size	32768	
8	Spectral Width	6172.839	
9	Spectrometer Frequency	300.135	
10	Temperature	300.00	
11	Title		

#### See also: <u>Tables</u>

'History': This tool opens a list of the previous operations applied to the spectrum. The document history saves a list with all the changes (with date and time) which the user has applied since the file was opened. This command is very useful if you have a saved file but you do not remember the steps you took in processing it.

**'Previous and Next Page'**: These commands are used to scroll trough the page navigator. Of course, the user can use the 'Page Up' or 'Page Down' keys to obtain an identical result.

The user can also select the desired spectrum by simply clicking on it on the page navigator (and then, can navigate to the previous or the next by using the up or down arrow keys). The rest of the 'View' Menu has already been explained above.

**Processing Menu:** The Processing menu allows the user to select which tools should be applied when processing the NMR spectrum. The user can also find the most frequently used tools in the toolbar.



**'Full Processing'**: This tool allows the user to automate the full processing of both 1D & 2D NMR data sets. The user can find a full description of this tool further on in the <u>Automated Processing</u> chapter.

**'Recent Full Processing'**: You can find here the most recent Full Processing archives. **'Set Processing Dimension'**: The user can choose the dimension (f1 or f2) to apply the processing.

f1 f2

This tool is also present in the NMR process toolbar.

**'Break Processing On'**: By default, when a new dataset is opened and time domain data (a 'fid' file for example) are selected, Mnova immediately applies appropriate fid pre-processing (Apodization) followed by Fourier transformation. If you wish to intervene in this process 'Break Processing On' allows you to halt the processing when, for example, the raw data are loaded, so that you can adjust apodization, zero filling, linear prediction or the Fourier transform parameters before continuing processing. (This is fully described further on in the <u>1D NMR Processing</u> chapter)

The following commands are described in more detail in the <u>Processing Basics</u> chapter:

<u>'Diagonal Suppression'</u>: This option is used to remove the signal on the diagonal from homonuclear spectra. Mnova applies this tool automatically prior to the FT.

<u>'Signal Suppresion</u>': This tool is used to remove any undesired signal such as a solvent resonance, from the spectrum.

<u>'Drift Correction</u>': This tool is used to remove the spurious peak which may appear at the transmission frequency when the the integral of the FID is non zero. The transmission frequency is known as "o1" on Bruker spectrometers and as "sfrq" on Varian instruments. Some texts refer to this as "Zero Frequency" but quadrature detection ensures that we don't have to deal with negative frequencies.

<u>'Apodization'</u>: This is used to remove the so-called "Sinc Wiggles" which can appear at the base of peaks when the FID has been truncated. Generally a decaying exponential "window function" is applied to the truncated FID to 'force' the FID to zero.

<u>'Truncate'</u>: This technique may be used to shorten the acquisition data time series. If the FID, for example, decays to zero in 0.5 seconds and the acquisition time was 2 seconds, the FID consists of 25% signal and 75% noise. Since both 0 and a 90 degrees phase shifted spectra are collected a time series data length of twice the FID time is required for maximum information content. Truncating the FID at about 1.0 second will reduce the amount of storage required with no data loss. At a later time Zero Filling may be used to cosmetically adjust the spectrum's appearance.

"Zero Filling and LP": Zero Filling allows FID time series data which has just decayed to zero at the end of the acquisition time to be extend by one further "acquisition time" by appending zero data points equal in number to those in the FID. This avoids the data loss which normally would result when half the data points are assigned to the "imaginary" part of the frequency spectrum optimizes frequency resolution of the spectrum. Zero filling beyond this point only improves the digital resolution of the lines which can still be useful although no new data is revealed.

LP (Linear Prediction) can be used to approximate a complete FID when data are missing from the start or the end of the transient. Typically if the FID has been truncated and has not decayed to zero by the end of the acquisition time, LP may be used to predict, based on the existing data, the missing (truncated) data. This is an alternative to applying a severe window function to avoid the peak-base (sinc) oscillations or wiggles caused by a sudden change in the FID. The "synthetic FIDs" obtained along f1 in indirectly observed 2D experiments are almost always truncated and linear prediction can be applied to very good effect.

<u>'Fourier\_Transform'</u>: Transforms the *time-domain signal (*acquisition data) into a frequency-domain representation (spectrum)

<u>'Phase Correction'</u>: Mixes the real and imaginary components of the spectrum in order to obtain pure phase lineshapes. During the detection process the receiver reference signal's phase may differ from that of the magnetization vectors by a fixed amount. This may be corrected by adding or subtracting a constant phase shift to the transformed data (the Zero Order phase correction).

The delay after the last transmitter pulse until the receiver becomes active allows the magnetization vectors to evolve slightly according to their chemical shifts, introducing a frequency dependant phase shift which may be corrected by the First Order phase correction.

**<u>'Baseline'</u>**: This tool attempts to connect all the spectral signals by a horizontal line.

<u>'Symmetrization</u>': This function, used in homonuclear correlation spectroscopy, replaces all signals which are symmetrically positioned about the diagonal by the smaller of the two signals. In this way unsymmetrically positioned noise and artifacts are removed. This technique should be used with caution since any symmetrical noise or artifacts will be preserved and may be mistaken for genuine signals.

<u>'Tilt 45'</u>: This technique is most frequently used with homonuclear J-resolved spectra where the effect of couplings in the f2 dimension is not required.

<u>'Reduce t1 Noise'</u>: This function reduces the streaks of noise parallel to f1 which often accompany strong 2D signals and are due to instrument instabilities.

<u>Normalize</u>: The intensity of 1D NMR spectral signals is generally displayed in intensity units based on the instrument's receiver digitizer's maximum range in bits. Normalization allows the intensity to be displayed in terms of some spectral feature such as the height of the tallest peak or some arbitrary peak or the total spectral area. In most cases post-acquisition signal suppression (Processing/Signal Suppression) is needed to remove solvent signals.

Normalization can be used to investigate the manner in which the intensities of some signals are changing from one sample to another while other signals remain constant. Examples include chemical kinetics and pharmaceutical drug degradation studies.

<u>'Binning'</u>: Chemical processes within cells are often tracked through the study (metabolomics) of the small-molecule metabolites produced. Typically many 1H spectra are taken and studied statistically. To render the many data points in a typical spectrum tractable they are "binned" into around 200 ins (or buckets) and each bin is integrated. Thus from the original spectrum a metabolic "finger print" is extracted for further analysis.

Binning is a technique used in metabolomics to reduce the many data points in a typical 1H spectrum to a small number of representative values.

<u>'Compression'</u>: This tool is used to reduce the size of spectral data with minimal loss of information. This is useful when many spectra must be taken and stored for possible later analysis.

<u>'Smoothing</u>': This technique is used to reduce the effect of noise on a spectrum and possibly reveal signals embedded in, or distorted by, noise. Noise contains rapid fluctuations which are are generally faster than the rates of change of genuine signals. Smoothing applies a low-pass filter to the spectral data to remove these rapid fluctuations while having minimal effect on signals.

<u>Resolution Booster:</u> A new frequency domain post processing method which yields a considerable resolution enhancement.

<u>'Invert, Transpose and Reverse'</u>: Invert effectively adds 180 degrees of constant phase to the entire spectrum.


Transpose switches the axes in a 2D experiment. In a heteronuclear 2D Bruker place f2 horizontally while Varian place it vertically. The user of one vendor looking at the other's data would be more comfortable with the spectrum transposed.

Reverse switches the spectral data around the transmitter (excitation) frequency. This might be required to correct data that had been incorrectly processed. A peak at x ppm below the transmitter frequency will appear at x ppm above the transmitter frequency after applying 'Reverse'.

'Arithmetic': to carry out arithmetic operations with or processed spectra.

### 7.5 Intelligent NMR Clipboard


The clipboard is for sure one of the most useful features in any modern Operating System and it is used for short-term data storage and/or data transfer between documents or applications, via copy and paste operations. Any modern application should support clipboard operations and, of course, <u>Mnova</u> is no exception. However, Mnova goes one step further compared to other applications as I will try to show in this post.



Following the same principles as standard Office applications, with <u>Mnova</u> you can copy any object (e.g. spectra, molecules, etc) into the clipboard and paste it either in Mnova (for example in a different page) or in any other application such as MS Office. The peculiar thing is that once a spectrum has been transferred to the clipboard (via Ctrl/Cmd+C), you can 'paste' it into another spectrum. Three examples will illustrate this new feature.

### Example #1


You have processed a spectrum and integrated carefully in order to quantify some signals of interest. Next you realize that you also want to integrate a different spectrum but using exactly the same integral regions as those in the first spectrum. There are several ways to do that in Mnova, but a very simple one involves copying the first spectrum into the clipboard and then selecting 'Paste Properties/ NMR Integrals' from the Edit menu. You can paste these integrals either to a single spectrum or to a bunch of selected spectra (or pages). The same can be used for the peaks

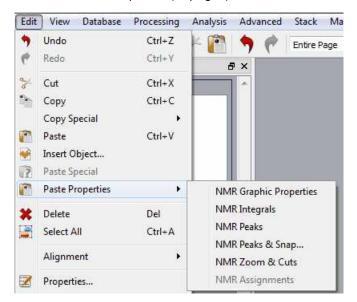

### Example #2

You have customized the graphical properties of a spectrum (e.g. fonts, colors, grid, etc) and you find


that you want to rapidly apply the same graphical settings to another spectrum. Once more, this is very easy with the clipboard: copy the first spectrum (Ctrl/Cmd+C) and then select the target spectrum and issue command 'Paste NMR Graphic Properties'.

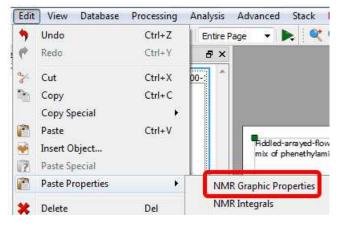


See also this <u>blog post</u>

### Example 3 (NMR Peaks & Snap)

When copying the peaks to a new spectrum, Mnova has an option to automatically snap the peaks to its nearest peak. A peak that would be automatically picked using the current peak picking threshold. For this option, the user is able to define a chemical shift window (the maximum chemical shift changes expected in f1 and f2).

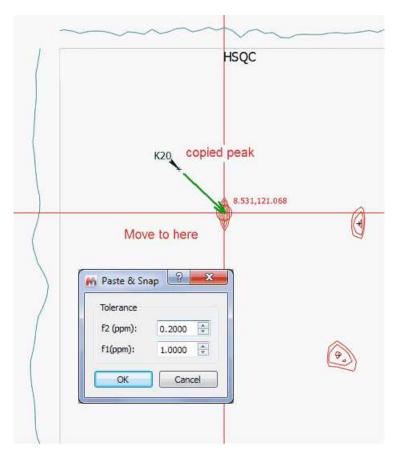

Mnova also allows the user to click-drag and move a peak label to a new location, by using the 'Move Peaks' tool under the Peak Picking scroll down menu.




### Example 4 (Zoom&Cuts)

This option will be used to copy the zoom and cuttings from one spectrum to another (or others).

#### Example 5 (NMR assignments)

This feature will copy the assignments from one molecule to another. The mechanism will be: Ctrl/Cmd+C in the assigned molecule, followed by clicking on the new molecule and applying 'Edit/Paste Properties/NMR Assignments' command. Please bear in mind that the numbering of the common parts of both molecules must be the same.

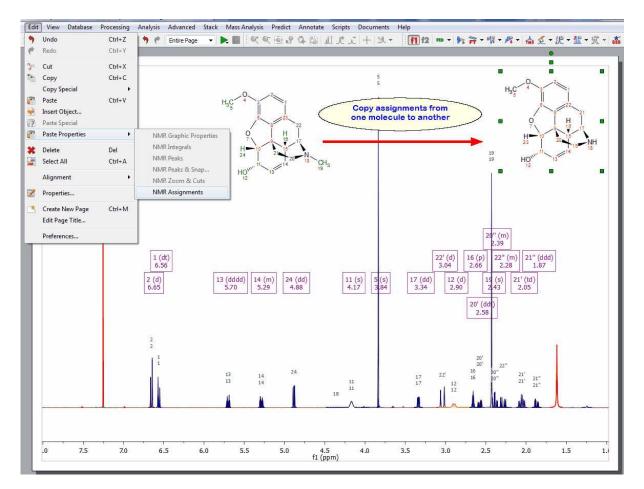

Another way would be to just copy&paste the molecular structure with the assignments and make the structural changes in one of the molecules.


### 7.6 Properties

**Properties:** Mnova will allow the user to customize nearly all the attributes of the spectrum. The user can select the properties of the spectrum by following the menu 'Edit/Properties' or by double clicking the left mouse button or pressing the right mouse button on the spectrum display and selecting '*Properties*' from the *pop-up* menu.

You can see in the pictures below the geometry and the Spectrum properties of a 2D NMR experiment.

Seometry NMR Spectr	uii				
Jnits: cm 💌			Angle		
X:	14.90	4	Angle		
x: Y:	14.90	*	Angle:	0.00	A T
	10.55	(¥)			
Size	122				
Width: 28.80	E Lock				
Height: 20.09					
Properties			0	OK Cance	el Apply
Seometry NMR Spectro	um		gend	OK Cance	2
Seometry NMR Spectro	um	Les Width		OK Cance 4.23 mm	
Seometry NMR Spectro General Grid JD	um		ŧ.		2
Seometry NMR Spectra General Grid JD 2D	um	<u>Wi</u> dth <u>T</u> ext V	: Vidth:	4.23 mm 12.70 mm	
Seconetry NMR Spectry General Grid JD Cond Cond Cond Cond Cond Cond Cond Cond	um	Width Text V Palett	: Vidth:	4.23 mm 12.70 mm Standard	
Seometry NMR Spectra General Grid JD 2D	um	Width Text V Palett Numbe	: Vidth: e:	4.23 mm 12.70 mm Standard 55:	
Secone try NMR Spectro General Grid JD D Traces Stacked		Width <u>T</u> ext V Palett Numbe	: Vidth: e: er of Positive Contou er of Negative Contou	4.23 mm 12.70 mm Standard 55:	() () () () () () () () () () () () () (
Seometry NMR Spectry General Grid JD 2D Stacked Scales		Width Text V Palett Numbe Scaline	: Vidth: e: er of Positive Contou er of Negative Contou	4.23 mm 12.70 mm Standard rs: urs:	Image: Contract of the second secon
Seconetry NMR Spectry General Grid JD D D Traces Stacked A Scales Horizontal		Width Text V Palett Numbe Scaline	: Vidth: e: er of Positive Contou er of Negative Conto g:	4.23 mm 12.70 mm Standard s: urs:	<ul> <li>Image: Constraint of the second second</li></ul>
Geometry NMR Spectry General Grid Grid D Comparison Com		Width Text V Palett Numbe Scaline	: Vidth: e: er of Positive Contou er of Negative Conto g:	4.23 mm 12.70 mm Standard s: urs:	<ul> <li>Image: Constraint of the second second</li></ul>
General Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid JD Comeral Grid Comeral Grid Comeral Grid Comeral Grid Comeral Grid Comeral Grid Comeral		Width Text V Palett Numbe Scaline	: Vidth: e: er of Positive Contou er of Negative Conto g:	4.23 mm 12.70 mm Standard s: urs:	<ul> <li>Image: Constraint of the second second</li></ul>

From this set of tabbed pages you can change, for instance, the spectrum's geometry (position, angle, size), the traces size, the 'Background', the 'Line-Style' (line, crosses or circles), the 'Line Colour' and the 'Line Width'. Bear in mind that a 'Line Width' of zero indicates a *cosmetic pen*. This means that the *pen* width is always drawn one pixel wide, independent of the transformation set on the painter . In 2D NMR spectra, you can set the legend, the number of contours, ploting method, show traces and customize the palette. The user can also set the scales' properties, change the grids, the aspect of the axes and margins or the units (ppm, Hz, points, seconds), for a more convenient representation of the spectrum. You can change the color of the spectrum background to suit your eyesight, your working hours, or your mood. Enjoy complete freedom on how to present your data! Transparency is also supported! Here you can see an example:

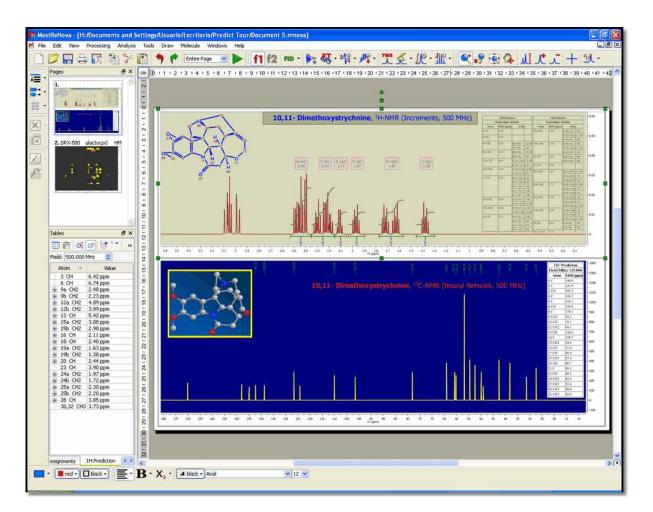

Check the 'Title' box of the 'Spectrum/Common' properties to **show the title on your spectrum**. You can select the position/alignment/offset of the title and also to customize the format by clicking on this icon . This will display a dialog box where you will be able to add 'Line Breaks', desired 'Parameters' of the Parameters Table e.g. (Title, Comment, Solvent, Owner, etc). From here you can also select the Name, Dimension, Max Length or Position. You can also add any 'Path' (with the capability to select the Level, Max Length or Position) or the 'Spectrum Number', just by selecting it on the 'Available Macros' panel and clicking on this icon **Solvent** to the title. Finally click on OK.

tadata Geometry NMR Spectrum				
General	Background			
Grid			_	
1D	Color:			
	Opacity:		0 %	A V
Scales	🔽 Title			
Horizontal	Font:	MS S	hell Dlg 2	*
Vertical	Format: {parm,			
Peaks	Tornadi (pani)	nde j	j.	
Integrals	Position:		Inside	-
Multiplets	Alignment:		Left	•
🝌 Integrals	Offset		/	
Fitting	Horizontal:		0.000	
Assignments	Vertical:	/	0.00%	(A). 97
1 <sup>21</sup>				? <u>x</u> )
Macro Editor		-		
Text			[	ОК
{parm, "Title"}{br}{path, 1, 15, l}{parm, "C	Comment"}			Cancel
Add Macro				
Available Macros:	Parameters:			
Line Break		me Val	ue l	
Parameter	1 Level	1		
Path Spectrum Number	2 Max Len			
- spectrum Number	3 Position	1		

Here you can see an example where we have changed the font of the title and added several parameters (Title, Solvent, Comment, Pulse Sequence and Temperature) to the title of the spectrum:

Text OK Igarm, "Title"; {u; {parm, Solvent} {u; {parm, "Conment"; {parm, "Pulse Sequence"; {br; {parm, "Temperature"; } Cancel	
Add Macro  Add Macros: Parameters:  Line Break Parameter Parameter Path Spectrum Number  Default Restore	Comic Sans MS - nce"}{br}{parm,"Temperature"}

The user will be able to select the desired 2D spectrum palette and also customize his own palette by selecting for example 'Custom 1' in the 'Palette scroll down menu and then clicking on the '**Palette Editor**' button is to display the '**2D-Spectrum Palette**' dialog box, where the user will be able to customize the desired palette (Name, Level Growth, Colors, Number of Levels, etc..). You can select the number of the positive and negative contours and also the scaling (in the 'Properties' dialog box) as you can see in the picture below:


- E							
Seometry NMR Spectrum							
General	E Leg	end					
Grid Grid	Width:			4.23 m	m		
1D 1D	<u>T</u> ext W	idth:		12.70 1	nm	A V	
4 💽 2D							
Traces	Palette		*				
💰 Stacked	Numbe	Number of Positive Contours: Number of Negative Contours:					
Scales	Numbe						
Horizontal	Scaling	Scaling:					
Vertical	Ploting	method:		Bitmap	•		
n 2D Spectrum Palette						2 X	
Name	Palette						
		Min %	Max %	Color	Key	*	
Custom 1	1.4	19.659	100.000	COIOT			
New Palette Generator		24.660	49.659				
Level Growth	-	12.246	24.660		0	=	
Mode: Exponential •	4 6	5.081	12.246			()	
Factor:	5 3	3.020	6.081		V		
Colors	6 1	L.500	3.020		E		
	] 7 (	).745	1.500				
Template: Grayscale 🔻	8 (	0.370	0.745				
Template: Grayscale   Number of Levels: 20							
Construction Construction	1 <u></u>	0.184	0.370				

If you want to obtain monochrome printouts different with the ones that already exist in the Palette scroll down menu, please follow the procedure below to create a palette in pure black with no grayscale:

- 1. Run Mnova and load your 2D-NMR spectrum.
- 2. Double click on the spectral window to open the 'Properties dialog box'
- 3. Select 'Custom 1' on the 'Palette' scroll down menu
- 4. Click on the 'Palette Editor' button (just at the right side of the scroll down menu)
- 5. Select 'Grayscale' on the 'Template' colours scroll down menu
- 6. Click on the 'Generate' button

7a. If you have 10 levels, check the 10th level of the palette and then click on the light-grey rectangle (just at the left side of the check mark) and select the black colour. Finally click on 'OK' buttons.

7b. If you have 20 levels, do the same with the 20th level and so on...

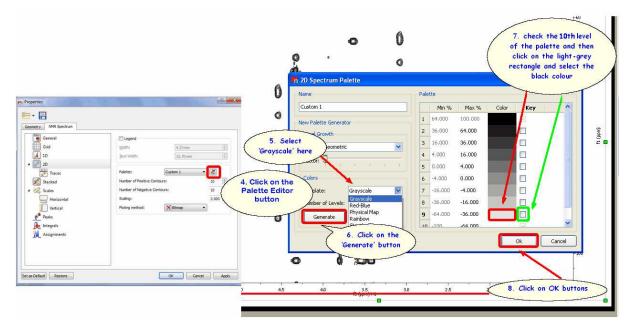


For further information, please take a look a this video

Let's take a look at another situation: how to make all positive contours a scale of greens and all negative contours a scale of blues?

In this case, you will only need to select in the '2D Spectrum Palette' dialog box the first and the last colour of the positive peaks and the same for the negatives. For example, imagine that you have 10 positive contours, then you will need to select the colour of the contour 1 as 'dark green' (for example) and then check the applicable mark at the right side. Finally, select the colour of the contour number 10 as 'light green' and check the mark. Do the same for the negative peaks; in this case the contour number 11 will be 'light blue' and the number 20 will be 'dark blue'. Please take a look at the screenshot below for further information.

ame	Pale	tte		
		Min %	Max %	Color Key
	1	49.659	100.000	
	2	24.660	49.659	
	3	12.246	24.660	
	4	6.081	12.246	
ustom 1	5	3.020	6.081	
	6	1.500	3.020	
	7	0.745	1.500	
	8	0.370	0.745	
	9	0.184	0.370	
ew Palette Generator	10	0.000	0.184	
Level Growth	11	-0.184	0.000	
	12	-0.370	-0.184	
Mode: Exponential	13	-0.745	-0.370	
Factor:	14	-1.500	-0.745	
	15	-3,020	-1.500	
Colors	16	-6.081	-3.020	
	17	-12.246	-6.081	
Template: Grayscale 💌	18	-24,660	-12.246	
Number of Levels: 20	19	-49.659	-24.660	
Generate	20	-100	-49.659	

You can see below an expanded signal after having applied the resulting palette (obtained in the previous step):

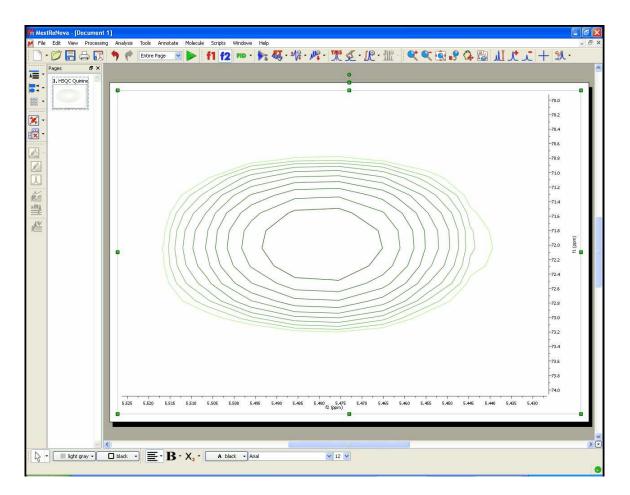

You can change the colours of the 2D overlaid spectra by following the above procedure (but changing the colours). You will find below two overlaid spectra with different colours (one red and the other purple). Please bear in mind that you can move from one spectrum to another (in the overlaid) by holding down the 'Shift' key and using the arrow keys (or the mouse wheel):

Properties		- 7 🛛
		_ @ ×
1	Spectrum	27 1 20 1 23 1 30
the second	Common 1D Spectrum 2D Spectrum	
Spectrum		
Scales	Width: 4.23 mm	•
	Text Width:	-20
Peaks	Palette: Custom 1 💓 🙀	-
	Number of Positive Contours:	-30
	Number of Negative Contours:	-40
1	Scaling: 2.000 🗘	-50
		-60
👫 2D Spectrum	Palette	-
Name	Palette	-70
Custom 1	Min % Max % Color Key	-80 (udd)
- New Palette Gene		-90 2 .
Level Growth	2 12 246 24 560	-100
Mode: Expone	4 6.081 12.246	-110
Factor:	<b>5</b> 3.020 6.081	
Colors	6 1.500 3.020	-120
Template: Number of Leve		-130
Generate	9 0.184 0.370	-140
		-150
	Ok Cancel	por esta
-	8 95 90 85 80 75 70 65 60 55 50 45 4.0 35 3.0 25 2.0 1.5 12(ppm)	
		•
	2	
		100
		×
🔓 📲 light gr	ay v 🔲 black v 📕 🖕 🖪 v X <sub>2</sub> v 🖪 black v Arial 🔤 12 💌	
		0

Of course, you can also make your 2D spectrum with a single color (no ramp). Once you are in the 'Palette Editor' dialog box, double click on the coloured rectangle of the level number 1 and select the desired colour, do the same with the level number 10 (bear in mind that you select the same colour) and uncheck any other key mark that could be in the other levels:

Eustom 1	and the second se		20	Min %	Max %	Color	Key	
Lascon 1			1	64,000	100,000			
			2	36.000	64.000			
ew Palette Generat	or		3	16,000	36.000			
Level Growth			4	4,000	16.000			3. Uncheck
Mode: Geometric	8	~	5	0.000	4.000			the other
Factor: J	2 2 2 2		6	-4.000	0.000			levels
Colors			7	-16.000	-4.000			
			8	-36.000	-16.000			
Template:	Grayscale	~	9	-64.000	-36.000			
Number of Levels:	10		10	-100	-64.000			
Generate	2. Do the same	with				_		

You can change the 'Scale Properties':

General Grid	C <u>o</u> lor:		•
1D	Line Width:	2.5	
2D	MS Shell Dlg 2 <u>M</u> argin:	<u>F</u> ont	
Stacked			
Horizontal Vertical			
Mr. Integrals			

From here the user can change the properties of the horizontal and vertical scales:

eometry NMR Spectrum	V Horizontal	
Grid Grid	V Label:	sds (sus)
🗼 1D	Units:	(ppm 🔹
4 💽 2D	Max. Significant Digits:	6
Traces	Primary Tics:	<u>- 0</u>
🔣 Stacked	Secondary Tics:	1
<ul> <li>Scales</li> </ul>	Position:	Тор 💌
Horizontal		Bottom
Vertical		Top Center
Peaks		
M Integrals		
Assignments		


The user can include the spectrum title (the title set previously on the spectrometer at acquire time) on any axis label by typing '\$t\$' in its applicable edit box. Bear in mind that, Mnova will only show the first line of the original title. This title appears by default on each page of the page navigator.

Hovering the cursor over the label edit box will reveal other commands for including information on the axis label, such as: u = Lowercase Units; U = Uppercase Units; d = Lowercase Dimension;

\$D\$: Uppercase Dimension; or \$1n\$ = Observed Nucleus (e.g. 1H, 13C...).

You can select the Maximum significant digits and the number of Primary and Secondary tics of the scales and to select the position of the scales.

The user will be able to save his/her own properties just by clicking on the **Save Properties**' icon (green square in the picture above). The Saved Properties will be opened by clicking on the '**Load Properties**' icon '(red square in the picture above). You can set the current properties as default by clicking on the 'Set as Default' button. Clicking on the 'Restore' button, will restore the predefined properties.

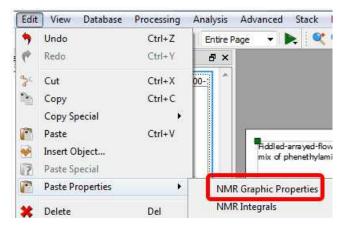

The user can also modify many other features such as the parameters and properties of the peaks or integrals. We will not go into further detail here since all the property pages should be self-explanatory and a description of each one can be found in its applicable section of this manual.

For example: once any table has been reported, you can change its properties (position, size, fill and border) by double clicking on it:


👫 Properties 🛛 🕐	🔀 💏 Properties 🛛 🖓	×
Geometry Shape	Geometry Shape	
Geometry Shape	Geometry Shape	
Position     Angle       X:     3.30        Angle:     0.00	Style: Transparent Color: Opacity: 100 %	
V: 3.41	Line Color: I black v	
Auto     Width: 5.81      Lock     Height: 6.02	Width: 0 V Style: None V	
OK Cancel Apply	OK Cancel Apply	

Or for the molecules:

Atoms Bonds Arrow	ws General		
Rotate with Molecule Symbols Show Carbons: All Show Others: All Font: A	☑ Terminals rial ►	Resize Fonts with     Iabel     Format: {atomNur     Font:     Assignments     Color:     Show Quality	

This box can be accessed by double clicking on the molecule, or by right clicking and then scrolling down to 'Properties'.

The text boxes will also have its own 'Properties', even we can add text properties to the page items and edit them by selecting the 'Metadata' tab:

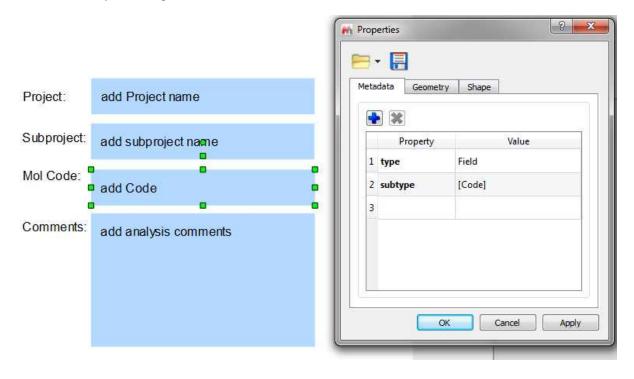

# 7.7 Preferences

Following the menu 'Edit/Preferences' ('MestReNova/Preferences' in Mac), you will be able to change the options of the Mnova interface, plugins, NMR. mass, molecule, scripting and drawing tools.

General	Plug-ins I	Database	NMR I	Mass Mol	lecule Scrij	💋 🎐 oting Drawin	ng Tools
Interface	Print & PDF	Updates	Memory	Open & Sav	ve		
🔽 Vertio	liasing Drawing cal Tabs in Dock e: English						
Mouse So	2000						
Modify in	tensity scale: ( ffer:	Enabled Small	•				
Event But							

You can save/load the preferences by using the applicable buttons.

From the General Preferences, you will be able to choose between large or small toolbar icons.

**'Antialiasing'**: This is the technique used to minimize the distortion artifacts known as *aliasing* when representing a high-resolution signal at a lower resolution.

*Aliasing* is an effect that causes different continuous signals to become indistinguishable when sampled. *Aliasing* also refers to the distortion or artifact that is caused by a signal being sampled at high resolution (on the spectrometer) and then rendered on the PC video-display at lower resolution.

The 'Antialiasing' is checked by default in Mnova.

Vertical Tabs in Dock Areas: it will display the tabs vertically in the dock widgets (useful when having a lot of dock widgets opened in the lateral dock and most of the tabs displayed horizontally are not visible):

Peaks	Mul	plets					8 ×	May
_		eport Mult	iplets 👻	Copy Multiplets	Setup F	Report 👻	XX Delete	NB-
Integrals Assignments	( 6	, J = 8.9 82 (dd, J	Hz, 1H J = 9.0, 2	z, DMSO) δ 12 ), 7.67 – 7.56 († 2.4 Hz, 1H), 6.6 16 (t, J = 7.0 H	m, 2H), 7 56 (d, J =	.22 - 7.13	2 (m, 2H),	
Compounds	Ē	Name	Shift	Range	H's	Integral	Absolute	
Comp	1	I (t)	1.16	1.21 1.12	6	6.07	84747.14	
	2	Н (q)	3.50	3.55 3.44	4	3.99	55775.57	
vultiplets	з	G (d)	6.66	6.69 6.64	1	0.99	13774.08	
Mult	4	F (dd)	6.82	6.86 6.78	1	0.99	13795.59	
hai	5	E (m)	7.17	7.22 7.12	2	1.98	27717.43	
- vo	6	D (m)	7.61	7.67 7.56	2	2.03	28351.48	
meters	7	C (d)	7.71	7.75 7.68	1	0.96	13453.24	
Parameters		B (s)	8.93	8.95 8.90	1	0.95	13202,28	
-	8	A (s)	12.27	12.29 12.24	1	1.04	14490.05	
-	8							
1H Prediction Parameters	8							

Language: Chinese, English, Japanese, Russian and Spanish versions of Mnova are currently available.

**Mouse Scroll**: The 'Modify Intensity Scale' enables/disables changing the spectra intensity/threshold via the mouse wheel. It also allows to enable it but requiring that the Alt key is pressed. The 'Event Buffer' will only affect to high sensitive mouses/trackpads (Like the magic mouse and magic trackpad from Mac) in any other device the change of this setting won't affect. It sets the event buffer size (or even disable it).

**Print&PDF Exporting:** From here you can select the PDF export resolution or the use of polylines when printing.

Interface	Print & PDF	Updates	Memory	Open & Save
🔽 Polylir	es when printing	10		
PDF Expo	rt Resolution: S	creen Resolu	tion 🔻	
PDF Expo	rt Resolution:	Screen Resolu	tion 🔻	
Metafile e	xporting/copying	p:		

Metafile exporting/copying: By default the option is checked and the text will be drawn by the GDI+ engine natively as text. If the option is unchecked then the GDI+ engine will draw the text as paths. The differences between both options are:

With the native text drawing option, the resulting metafile could be slightly different from what you see in Mnova due to differences on how GDI+ renders text.

With the other option, the text should be shown exactly as Mnova shows, but the texts objects in the metafile aren't no more text objects, they are vector graphics objects, so user couldn't edit the text by typing/deleting characters

If you work with huge datasets, in order to avoid **memory** issues, you can uncheck the memory

options to be able to copy your spectra to clipboard or to disable the Undo feature.

**Open&Save**: to set one or more locations as default open/close directories. A document can be saved as pdf in one of these default directories (via 'Save As' and choosing the pdf filter). The default open and save directories can be accessed via File/Open from Location and Save to Location.

	-	- 14		1		(nP	-1-	
			2.5	-	<b>4</b>			
General	Plug-ins	Database	NMR	Mass	Molecule	Scripting	Drawing Tools	
Interface	Print & PDF	Updates	Memory	Open & Save				
Locations								
Open			+					
and the second se					Path			
Open Save			Settings/Usu	ario/Mis docu	mentos/Drop	box/MESTREI	LAB/TESTING/ASVTESTSET/Public	*
	C:/Do	cuments and	1					
Save		uments and Plugins/Test		iles				

From the '**Plugins Preferences'** dialog box, you will be able to ignore any plugin, which will be very useful in the case of concurrent (floating) licenses, in order to 'liberate' the license of those plugins which will not in use.


In any case, please bear in mind that Mnova allow users to only take the plugins they are **using** as opposed to the plugins which are **installed**.

c	General	Plug-ir	s Database NMR M	🧉 🐗 Iass Mole	cule Scripting Drawi	15 ing Tools
		Ignored	Name	Licensed To	Issued By	
1	V		Mnova Verify	Pablo	Mestrelab Research S.L.	
2			🦸 Database	Pablo	Mestrelab Research S.L.	
3			Document     Drawing Tools		Mestrelab Research S.L. Mestrelab Research S.L.	
4 5			M Drawing loois	Pablo	Mestrelab Research S.L.	
5 6	1		Modgraph NMRPredict Server	Papio	Mestrelab Research S.L.	
7	121		Modgraph NMRPredict Deskto	n Pablo	Mestrelab Research S.L.	
, 8			Molecule		Mestrelab Research S.L.	
9			MMR	Pablo	Mestrelab Research S.L.	
10			n NMR Predictor	£893568	Mestrelab Research S.L.	
11	[V]		n Scripting		Mestrelab Research S.L.	
12	$\overline{\vee}$		n OLE Container		Mestrelab Research S.L.	
13			💰 Mnova Batch Verify	Pablo	Mestrelab Research S.L.	
14	1		💣 Mnova Batch qNMR	Pablo	Mestrelab Research S.L.	
15	1		💰 Mnova Screen	Pablo	Mestrelab Research S.L.	
16	$\overline{\mathbb{Z}}$		률 Mnova qNMR	Pablo	Mestrelab Research S.L.	
17	1		💰 Reaction Monitoring	Pablo	Mestrelab Research S.L.	
Ad	Ivanced Pli	ug-ins Dire	tory			
r	:AlsersAls	suario/Apol	ata/Roaming/Mestrelab Research S.L./	MestReNova BE	TA/plugins	

From the '**NMR Preferences**' dialog box, you will be able to select the mode of the '2D palette mapping' (default, absolute and dynamic).

references	8
General Plug-ins Database NN	MR Mass Molecule Scripting Drawing Tools
Drawing Import Processing Save	DataProc
Palette Mapping Mode:	Default 🔻
Contour Drawing Mode:	High Resolution 👻
1D	
Threshold:	256
GSD Peaks Display Resolution Factor	

From this dialog box, you will also be able to select threshold of the limit of the number of points showed in the spectral window. For example if your spectral window has less than 128 points (and you have this option checked), you will see the points (as crosses) drawn on it; as you can see in the picture below. If the spectral window has more than 128 points, you will see the spectrum as usual.

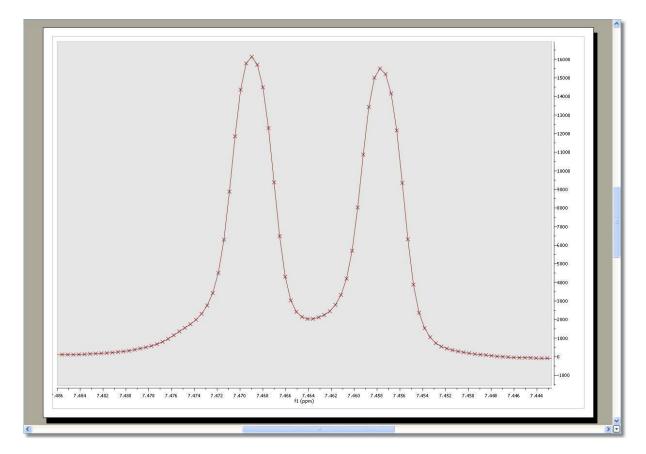

From this Preferences menu you can also select the GSD display resolution factor.

The GSD peaks extend over all the spectra but when drawing we are cutting the display at some point to speed up the drawing. By default Mnova uses the peak width by a factor to "cut" the peak display. This behavior is the default one but is optional. The user will be able to change it in the preferences (NMR tab) just by checking "GSD Peaks Display Resolution Factor". And if it's checked you can adjust the factor (10 by default) to be multiplied by the width.

From this menu, but selecting the Import tab, the user can select the option to import the apodization, zero filling, linear prediction options from the spectrometer and also the default phase correction method (Imported or Automatic). From here you can also select to apply automatic <u>phase</u> and <u>baseline</u> corrections, <u>apodization</u>, <u>absolute reference</u>, <u>fit to highest compound</u>, <u>VnmrJ DEPT processing</u> or pureShift FID reconstruction :

eferences	
General Plug-ins Database NMR Mass	Molecule Scripting Drawing Tools Publications
Drawing Import Processing Save DataProc Parameters	
Apodization	
Zero Filling	
Linear Prediction	
Apply	
Drift Correction	Absolute Reference
Automatic Phase Correction	Automatic Apodization
Baseline Correction	Fit to Highest Compound
VnmrJ DEPT Processing	VureShift FID Reconstruction
CSV	
Step Precision: 0.000100	
Traces	
Auto Attach Traces	
	OK Save Load Cancel

If the the 'Auto Attach Traces' box is checked; the 1D spectra of the document will be used as projections of a 2D.

Under the 'Processing' tab, you will have a preference to use multiple CPU cores to speed up the 'processing&analysis' of stacked spectra:

	100			2	S.	
General	Plug-ii	ns Databas	e N	IMR	Mass	Mo
Drawing	Import	Processing	Save	DataProc	-12	

Selecting the 'Save' tab will allow you to compress the data on storing:

		-				
General	Plug-ins	Database	NMR	Mass	Molecule	Drawing Tool
Drawing	Import Sa	ve DataPro	oc			
1022010220104201042	on ss FID Compres um Compressior			.2 versions of	_	
ri specar	in compression	Lossy (reco		10.00	51) 	

From the '**Mass Preferences'**, the user will be allowed to select the saving options (item only or item +dataset). When the option 'Synchronized chromatogram's Time Scale' is selected, you will be able to zoom, pan and cut to all showing chromatograms. You will find also an option to fit to height after zoom (selected by default). When this option is checked, a fit to height is applied after making a horizontal zoom in a mass spectrum or a chromatogram. In case of the other zoom modes (vertical or in both dimensions), a fit to height is never applied.

General	Verify
<u>Saving</u> C	ptions
Item	Qnly
🔘 Item	& <u>D</u> ataset
Your cho	ice will affect only to newly imported items.
Scales B	ehavior:
🔽 Fit to	Height After Zoom
Sync	hronized Chromatogram's Time Scale

From the **'Molecule Preferences**', you will be able to save the numbering when you export the molecule to a .mol file (via File/Save as'), 'import molecule styles' (when you paste special) and auto-renumbering on importing or joining fragments:

Preferences				?			
General Plug-ins Data	base NMR	Mass	Molecule	Scripting	Drawing Tools	Publications	
✓ Save Numbering to Molfiles			💟 Import Mol	ecule Styles			
Auto-renumbering							
On Importing			On Joining Fragments				
Expand Labels On Importing     Automatically Open Table Of Cor	npounds When Impor	ting A Molecule					
PhysChem Properties							
🔽 Update When Editing							
Open Babel Folder							
Autodetect							
Select						8	
Keyboard Editing Always Availabl	e						

From the **'Scripting Preferences**', you will be able to select the scripting folders and also to create events to run script events by default:

		-			<b>a</b>	{}	1
Gen <mark>e</mark> ral	Plug-ins	Database	NMR	Mass	Molecule	Scripting	Drawing Tools
Directories	Events						
C:\Prog	ramData/Mes	)/Mestrelab Re trelab Research Data\Roaming	n S.L./MestR	eNova BETA/	scripts	BETA/scripts	*
						_	

From the '**Drawing Tools Preferences**', you will be able to select the exporting 'Resolution' and 'Quality' of the graphics and also the resolution of the image copying:

_		EM.	2	-		B
General	Plug-ins	DB	NMR	Mass	Molecule	Drawing Tools
	5 ( <b>5 3</b> (5))	56.50	0.22227624	14500775	1.51624546557	2
Image Expor	tina					
image Expor						
1970 - BA	Display Resolution	on 🌲				

## 7.8 Menus and Toolbars Customization


Mnova allows you to customize the menus and toolbars by following the menu: 'View/Customize User Interface/Customize Toolbars (or 'Menu Bar') or by right clicking on the toolbar and selecting 'Customize Toolbars'.

This will display the 'Customize Toolbars' dialog box (similar dialogs will appear to customize the menu bars or context menus):

Toolbars	Toolbar Commands	All Commands
Image: Second	Plots-> Traces->	<ul> <li>Eind:</li> <li>Advanced</li> <li>Advanced&gt;Data Analysis</li> <li>Advanced&gt;Line Fitting</li> <li>Advanced&gt;Reaction Mo</li> <li>Advanced&gt;Reaction Mo</li> <li>Advanced&gt;qNMR</li> <li>Advanced&gt;qNMR</li> <li>Advanced&gt;qNMR</li> <li>Advanced&gt;qNMR</li> <li>Analysis</li> <li>Analysis&gt;Integration</li> <li>Analysis&gt;Peak Picking</li> <li>Analysis&gt;Predict Highlis</li> </ul>

From here, you will be able to customize the selected 'Toolbar' (highlighted in red in the picture above) by just using the arrow icons to add, remove or sort the desired features. Click on the applicable buttons to add R, remove Rename any created toolbar.

Let's see how to add the 'Report Multiplets' feature to the 'NMR Process' toolbar:

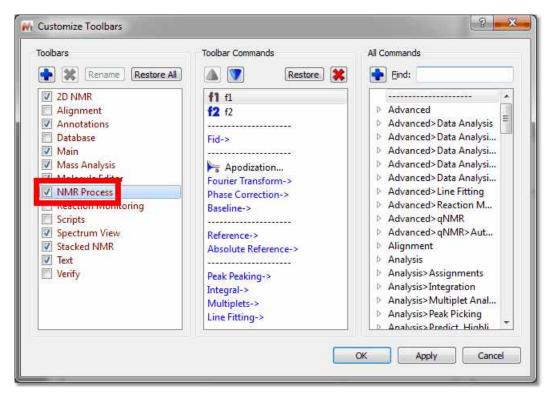


1st: Select the 'NMR Process' toolbar from the 'Toolbars list:

2nd: Navigate to the 'Report Multiplets' feature in the 'All Commands' part of the menu (at the left side of the window), or type the name of the feature in the finder field:

oolbars	Toolbar Commands	All Commands
<ul> <li>Rename Restore All</li> <li>2D NMR</li> <li>Alignment</li> <li>Annotations</li> <li>Database</li> <li>Main</li> <li>Mass Analysis</li> <li>Molecule Editor</li> <li>NMR Process</li> <li>Reaction Monitoring</li> <li>Scripts</li> <li>Spectrum View</li> <li>Stacked NMR</li> <li>Text</li> <li>Verify</li> </ul>	Restore Restore Restore Reference-> Peak Peaking-> Integral-> Line Fitting-> Reference->	<ul> <li>Eind: multiplets</li> <li>Analysis&gt;Multiplet Anal Show Multiplets MS Spec Vertical Axis</li> <li>NMR Multiplets-&gt;</li> <li>NMR Multiplets</li> <li>MR Delete Multiplet P Add Multiplet P Measure J Edit Multiplet</li> <li>Delete All Multiplet</li> <li>Delete All Multi Copy manpress</li> <li>Delete All Multi Edit Peak Type Set Peak Comp</li> </ul>

3rd: Click on the 'Blue plus' button 💽 to add the 'Report Multiplets' feature to the 'Toolbars Command'.

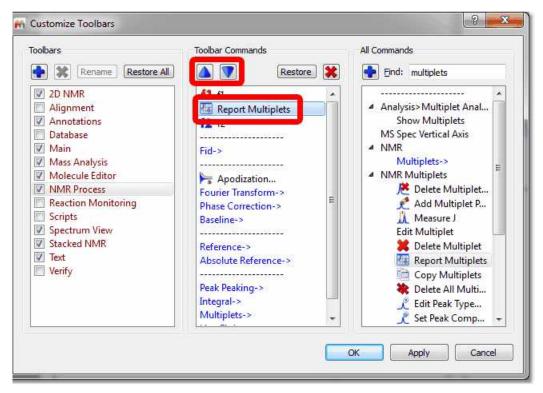

4th: Use the up/down arrow buttons to sort the button inside the toolbar and click on OK. The 'Report Multiplets' button will appear in the 'NMR Process' toolbar:



Please bear in mind that you will be able to remove the undesired features from the toolbar, just by clicking on the 'red cross' button of the 'Customize Toolbars' dialog box.

You can select between three predefined GUI setups (including configuration for the menu bars, toolbars and context menus) by following the menu 'View/**Manage User Interfaces'**.

View	Database Processing Analysis	Predict Mass Analysis Scripts Documents Help
	Layout Templates	Manage Custom Interfaces
	Manage User Interfaces	
	Customize User Interface	
	Pages Page Notes Previous Page Next Page	Basic Intermediate *Expert
	Full View Well Plates Rulers	
	Toolbars	OK Cancel
	Tables	

From here you can select between the 'Basic', 'Intermediate' and 'Expert' (default) just by double clicking on the desired one or by using the 'green check mar' button. Those files can be found in the MestReNova/Data installation folder (with the extension .mncs).


If you want to create any new GUI setup, just customize your toolbars and menus; follow the menu 'View/Manage User Interfaces' and click on the 'blue plus button' to add a new 'Custom Interface':

Manage Custom Interfaces	2 ×
2 🔁 🖊 🕱	
Basic Create new custom user interfa	ce from current
Intermediate	
Expert	
*Custom 1	
OK	Cancel

You can overwrite any existing 'custom GUI' by customizing the toolbars and menus and clicking on the button below:

Basic	rwrite selected use	r interface with curre
Intermediate		
Expert		
Custom 1		

Follow the menu: File/Save as/MestReNova Customization (\*.mncs) to save (or export) the customization of the Toolbars:



Then, you will be able to open any Customization file just by following the menu 'File/Open' or dragging&dropping (exactly in the same way as this would be applied to a spectrum).

You can also add any created script on the toolbar, but please bear in mind that the script file will need to have the same name that the function which you want to call. For example, if the name of the function is 'example', then the name of the script will be 'example.qs'. Then, you will need to add this line with the applicable 'Name in Menu' at the beginning of the script:

//<GUI menuname="Name In Menu" tooltip="My ToolTip" icon="/path/to/icon"/>

Finally, store the script in the Mnova scripts folder and restart Mnova to be able to see the script in the scroll down menu of the 'Run Script' icon and in the list of icons in the customize toolbar dialog box.




#### 7.9 Context Menus

Mnova incorporates very useful context menus to make it easier to perform some common tasks. The contents of the context menu will depend on the window area clicked. For example if you right click (or

Ctrl+Click in Mac) on a 2D spectral window, you will obtain the following contextual menu:

	Show Traces	
	2D Plotting Method	۲
	Phase Correction	×
	Baseline	•
	Peak Picking	•
	Integration	•
TM5	Reference	L
	Save to Database	
	Save to Record	
S	Structure Search	
en la	Substructure Search	
CAS	Formula Search	
甩	Peak Search	
譜	Multiplet Search	
JA.	Massitem Search	
冎	Advanced Search	
3	Cut	Ctrl+X
1	Сору	Ctrl+C
1	Paste	Ctrl+V
×	Delete	Del
	Select All	Ctrl+A
	Alignment	×
Z	Properties	
	Customize Context Menu	IS

If you right click on a multiplet box, you will obtain:

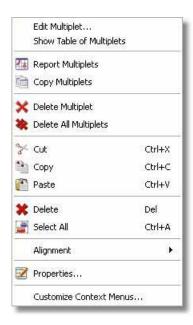


#### On a molecule:

Ĥ	Predict 1H Spectrum	
0	Predict 13C Spectrum	
0	Predict 19F Spectrum	
-	Predict 15N Spectrum	
0	Predict 170 Spectrum	
S	Predict 29Si Spectrum	
	Predict 31P Spectrum	
	Save to Database	
d'	Structure Search	
M	Peak Search	
30	Cut	Ctrl+X
	Сору	Ctrl+C
r	Paste	Ctrl+V
*	Delete	Del
2	Select All	Ctrl+A
	Alignment	\$
2	Properties	
	Customize Context Menu	s

You will also find useful contextual menus on 1D spectral windows, page navigator, integral curves, traces, axis etc.

Follow the menu 'View/Customize/Customize Context Menus' to customize the selected 'Context Menu' as it is explained in this <u>chapter</u> (for toolbars).

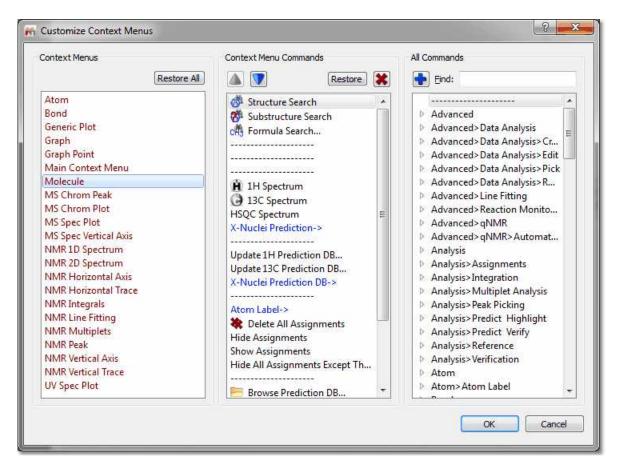

## 7.10 Localization

#### Localization:

English, Japanese, Russian and Spanish versions of Mnova are currently available. The user will be able to select the desired idiom by following the menu 'Edit/Options/Language':


		-
General	Plug-ins	DB
Interface		
	Large Toolba	r Icons
	Large Toolba	
Language:	The sum searce wa	
Language: Updates	Antialiasing [	

Once, the user had selected the desired language, a dialog box will be displayed to inform that it will

be needed to restart Mnova in order to obtain the change of the language .



The Japanese version is shown in the picture below:

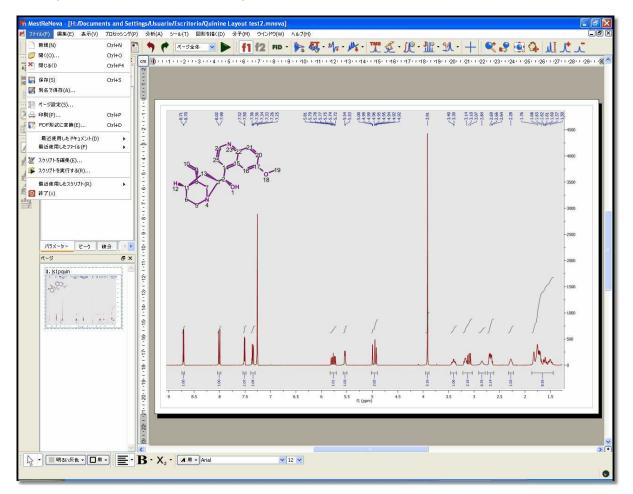


We plan to update once per year the different translations of the software, so you may find the newest feature menus without translating (in english).

## 7.11 Layout Templates

# You will find a sample Layout Template in the installation folder of Mnova (under the examples/datasets folder)

This feature will allow you to create templates for your NMR and MS spectra (including processing) with the location of the spectrum, spectral width, molecular structure, images, tables and multiplet reports. To create a template with Mnova, open a document and select the desired location and properties for the different objects present in it. The picture below shows a 1H-NMR spectrum, with the

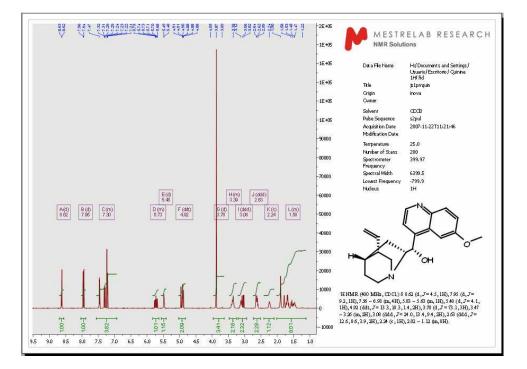


applicable molecular structure, multiplet report, images and the Parameters table:

To save the created layout as a template, just follow the menu 'View/Layout Templates/Create Template Document' and select the location of the new template.

View Database Processing	Analys	is A	Advanced Stack Mass Analysis Predi
Layout Templates	×		Lay out in Template Document
Manage User Interfaces Customize User Interface	×	~	Apply Processing Template Layout Template Options
Pages Page Notes Previous Page	Page Notes		1 C:/Users/Usuario/Desktop/layout_pag 2 C:/Users/Usuario/Desktop/Layout.mn 3 C:/Users/Usuario/Desktop/Mis docum
Next Page			Create Layout Template Document

You can also use the 'New Blank Document' scroll down menu from the toolbar:



Once saved, a template can be easily opened by double clicking on the .mnova file. Please note that drag and drop also works in this instance.



#### ATTENTION

The layout template will keep all the properties of the objects (draws, annotations, spectra and molecules), the processing (optional) and the analysis features used in the original spectrum ('peak picking', 'integrals', 'multiplets' or 'cuttings'). Double click on each item to check the embedded properties.


The picture below shows the layout created previously:

	Image
NMR Spectrum: 1D, [1H]	Text: NMR Table, [Parameters]
	Molecule
	Text: Report Special, [Multiplets]


also the processing us	<b>ply Processing Template'</b> option, the layout templa used in the original spectrum. If this option is not s nly keep the properties:	
Layout Template Options     Policy     Apply Single Page Template to C     NMR     Apply Processing Template     Apply Zoom     OK	o Current Page	

The policy option is only valid for layout templates containing just one page. If a layout template with more than one page is selected, the layout template will be applied to the whole document, no matter the selection of the option.

If the user opens a different 1D-NMR spectrum over this layout, it will be obtained in the applicable location, with the corresponding processing and analysis features (multiplet analysis in this case) and also with the applicable object properties, including all the relevant tables and reports:

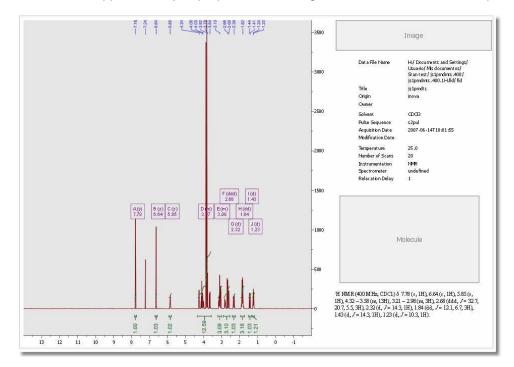


In the same way, when the user opens or pastes a molecule and an image, they will also be automatically displayed in the corresponding location (with the original properties).

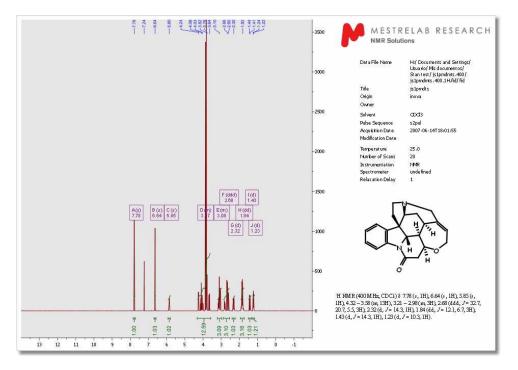

Also note that our concept is designed to be extended to reports with more than one page, to allow for the placing of several spectra on the report (in this case 1H, 13C and HSQC):


M Mes	tReNova - [H:Wocuments and SettingsWsuario\Escri	rioV.ayout 1H,13C,HSQC.mnova]	
	Edit View Processing Analysis Tools Annotate Mo	cule Scripts Windows Help	_ 8 ×
	💋 🔜 🚑 🔀 🦄 🎢 👔 🕈 🥐 Entire	∞ 💌 ▶ f1 f2 ፣ ାରେ 😽 🧠 🌾 🥂 🖉 🖉 🐨	<u>-</u> 十 に 九 山 國 4 名 国 2 3
	Pages & X		<u></u>
10	L. Proceeding of the second se		
- 88			
$[\mathbf{X}]$ -			
	At 1	You can write any annotation here!	MESTRELAB RESEARCH NMR Solutions
	- Constant of the Constant of		
	2.		
M	- An inger fanse genet		
赵三			
×10	and the second		Text: NMR Table, [Parameters]
14	14 million 11 million		
I			
			e
		NMR Spectrum: 1D, [1H]	
	3.		
	- seat to prove		
			Molecule
	197. Annual (1) (111)		
	inter a second se		
			Text: Report Special, [Multiplets]
			2.
T	dark blue - 🗆 black - 📃 - 🖪 - 🗙	<ul> <li>A black - MS Shell Dig 2</li> <li>I4 </li> </ul>	
	- 1.2		

Of course you can use layout templates with your MS documents (or combined with NMR spectra). Here you can see an example of a layout template for MS spectra:

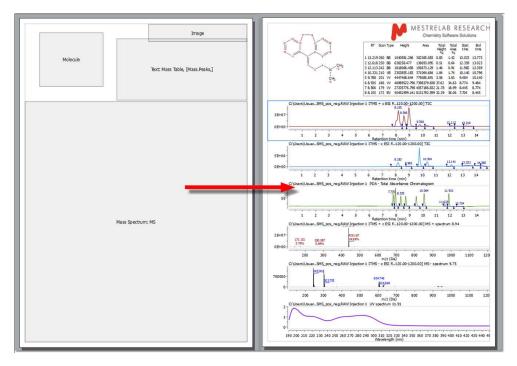

You can modify any layout template. For example in the template above we have added an annotation and a logo and then clicked in the 'Save' button. If you open again the template you will have by default the annotation and the logo on your screen. You can also double click on any item to change any property and then save the changes.


It is also possible to apply a layout template to any opened spectrum, just by following the menu 'View /Layout Templates/Lay Out in Template Document':

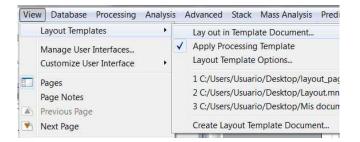

There is a script to load a layout template (see the script called 'applyLayoutTemplateAndPrint.qs' under the examples/scripts installation folder). You will find another example under the 'Scripts/Report' menu, to apply a **'Smart Reporting'** which will load a layout template, with the option to include applicable processing template embedded in the layout or to load other processing templates. The script will allow you also to select 'Spectral Widths' for each nuclei:

Help				
<u>大·筑· ≲· ⊮· 쌨·</u> 4···5···6···7···8···9·	Layout Template File:			
	Processing Templat 1H File: 13C File:	tes		
Peaks	Spectral Widths			
All Multiplets in Document	Spectra	From	То	
Chemic Chromatogram Subtraction	2 C1			
		2000 <del>-</del>		date Table
	Help           人、く気、く気、水、、、、、、、、、、、、、、、、、、、、、、、、、、、、、、、	Help Layout Template File: Layout Template File: File: Processing Templat HFile: Spectral Widthsets Main Multiplets Assignments Assignments Chromatogram Subtraction With UV Subtraction	Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton service       Image: Crypton service       Image: Crypton service         Image: Crypton servi	Help       Image: Circlest of the start of

Here you can see an example:

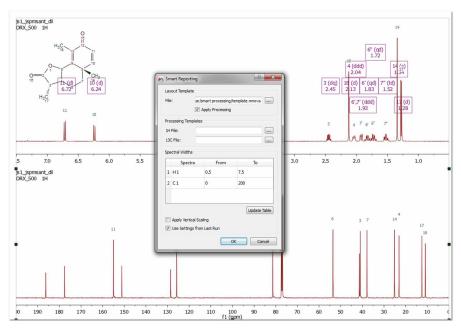

To use a layout template by default for all of your experiments follow the menu 'Edit/Preferences/Scripting/Events/nmrSpectrumImported' and add the function onSpectrumImportedDemo.applyLayoutTemplate.

	•	r 🎁	2	-	40	<u></u>	8
General	Plug-ins	Database	NMR	Mass	Molecule	Scripting	Drawing Tools
User Interface	e Visibility						
Directories	Events						
Event: nmrSp	ectrumImport	ed 🔹					
*							
		ed. <mark>openSam</mark> edDemo.app		alata			
iv onspec	uummporu	euvenio.app	lycayoutien	piace			
		w Event Han	dler			? ×	
	m Ne						
		ion Name:	nSpectrumIm	portedDemo.a	pplyLayoutTem	plate	
		ion Name: o	nSpectrumIm	portedDemo.a	opplyLayoutTem	plate Cancel	
		ion Name:	nSpectrumIm	portedDemo.a		100 C	
		ion Name: d	nSpectrumIm	portedDemo.a		100 C	
		ion Name: d	inSpectrumIm	portedDemo.a		100 C	
		ion Name: o	nSpectrumIm	portedDemo.a		100 C	
		ion Name: d	nSpectrumIm	portedDemo.a		100 C	


Next, select the Directories tab in the 'Edit/Preferences/Scripting' dialog and copy the script " onSpectrumImportedDemo.qs" to a script directory of Mnova. Finally, save a layout template document (called 'test.mnova') into "C:\temp\' and restart Mnova. Load your NMR spectra and the layout template will be applied automatically.

## 7.12 How to measure coupling constants? The Crosshair Tool

**The Crosshair**: These two orthogonal lines forming a crosshair are available on the 'View' menu (or by pressing the <c> key) for reporting positional information, and for help in visualizing peak alignments. This tool can also be found on the 'Zoom' toolbar.

#### How to measure coupling constants?

The crosshair includes information about the chemical shift and the intensity of the peak (as you can see in the picture below) and also allows the user to measure distance between peaks (or **coupling constants**) by clicking on the left mouse button and dragging to the desired peak. Activating the crosshair tool will open a 'Cursor Info' dialog box, where the user will be able to see the units distance expressed in ppm, Hz or points. This dialog box will also display the distance between the desired peaks, as well as the intensity ratio. The info View window also contains information about the Spectrum Resolution.

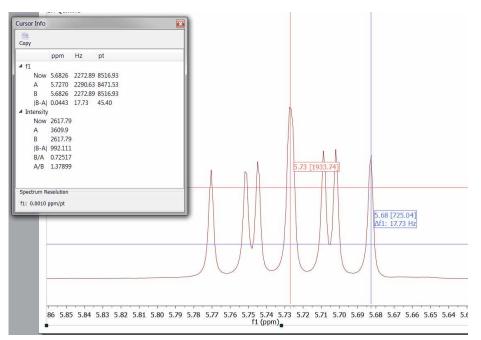


Click on the 'Copy' button to copy to clipboard the information displayed in the 'Cursor Info'.


The cursor will "ride" along the 1D-NMR spectrum simplifying the location of peak maxima and minima by pressing the 'Shift' key.

#### 7.12.1 Multiple Crosshair for 2D analysis


**Double Crosshair:** If you are working with COSY-like spectra (homonuclear spectra), you will obtain the **double crosshair** tool just by pressing the 'Shift' key, as you can see in the picture below:

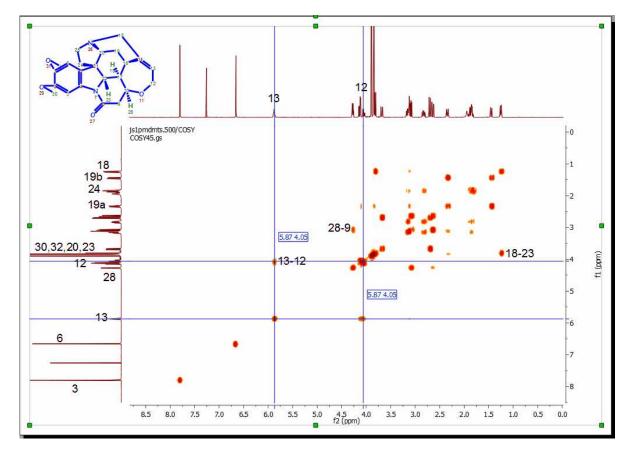


**Multiple Crosshair:** If you have several spectra displayed on the same page, you can tie the crosshair cursors together over all the experiments by selecting the crosshair feature in one of them. In the example below you can see how the multiple crosshair works in a HSQC, COSY and a 1H spectrum.

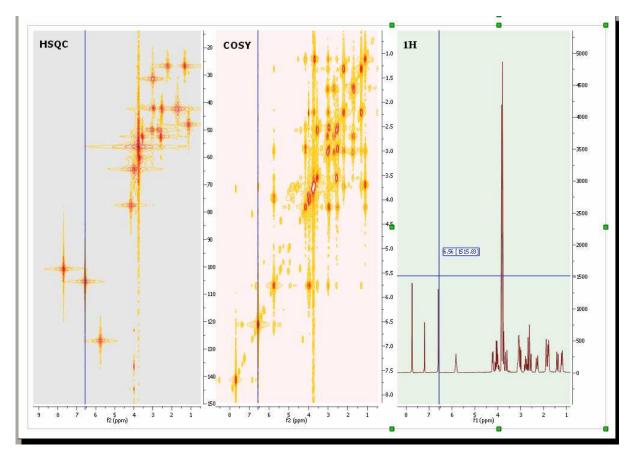

Here you can see a COSY, HMQC and HMBC (with the multiplet crosshair):

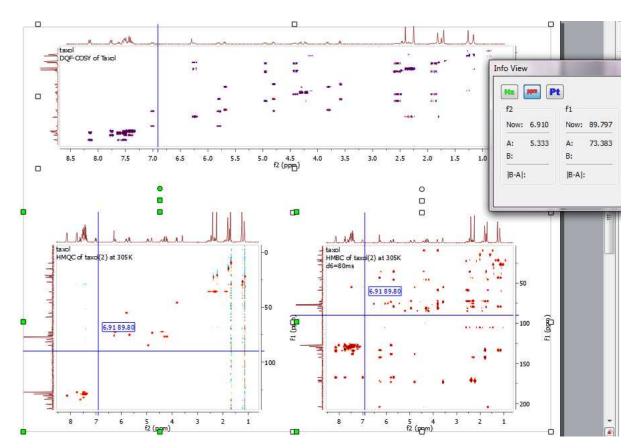

You can get correlated cursors in stacked mode. To disable/enable the correlated cursor, just press the 'C' key:

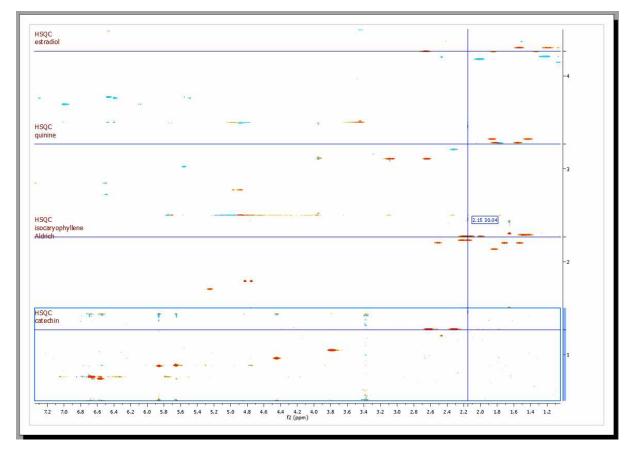

## 7.13 Zooming


A number of ways of zooming are available in **Mnova**.

The most common type of zooming in spectroscopy applications is the 'Zoom In' mode. This mode can be entered by following the menu 'View/Zoom/Zoom In' or by using the 'Zoom In' icon on the toolbar.

In this area, Mnova presents a significant innovation, allowing the user to apply 'horizontal', 'vertical' and 'box' zooms, as illustrated by the figures below.


**HORIZONTAL ZOOM.** Click the **'Zoom In'** icon Son the toolbar (or press **<Z**> key), hold down the left mouse button on the spectrum display and drag the *magnifying glass cursor* (with a red horizontal segment) across the area you want to zoom in to; a highlighted rectangle indicating the new spectral region to be displayed once the mouse is released, will follow the cursor. Use 'Undo' to revert to the previous display. A zoom lens of a 20% will be obtained by clicking on the left mouse button.

The zoom cursor shows information about the position (same units as in spectrum scales). Once the starting position is selected, only the values for the ending position (f1, f2 or both dimensions, depending on the type of the zoom applied) are displayed.

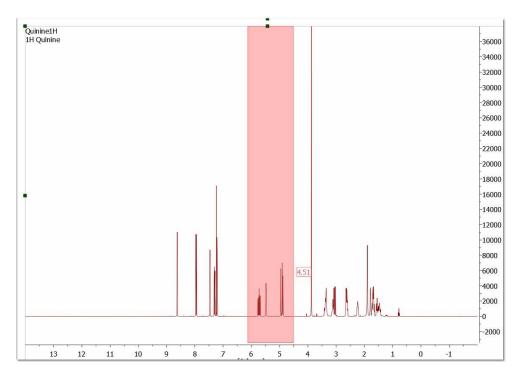


Please note that holding down 'Ctrl+Space bar' (in Mac: 'Space+Cmd') will activate the zoom in temporarily.

**VERTICAL ZOOM.** Click the **'Zoom In'** icon so on the toolbar and then press the **<Z>** key (or just press twice the 'Z' key). You will see a red vertical line segment beside the mouse pointer) while the cursor is located on the spectrum display and then click and drag the cursor vertically over the area you want to zoom in on; once again you will see highlighted red rectangle.

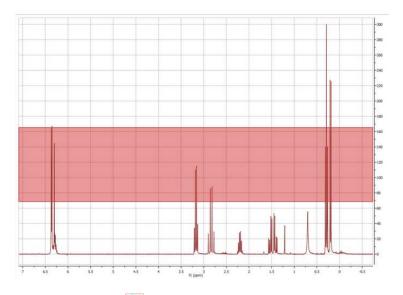

**BOX ZOOM.** Click the **'Zoom In'** icon so on the toolbar and then press **<Z>** key twice with the mouse pointer on the spectrum display (or just press three times the 'Z' key), then click and drag the cursor diagonally over the area you want to zoom in (highlighted rectangle in red). This zoom is very useful for 2D-NMR.

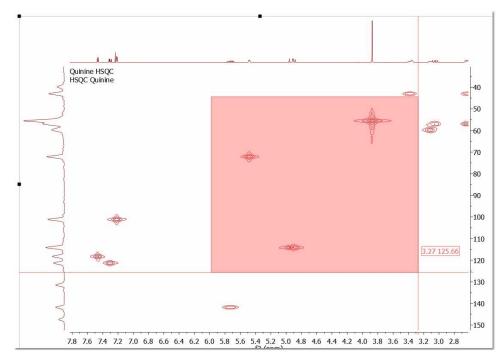

In order to switch between these three types of zoom, just press the **<Z>** key whilst in the **'Zoom In'** mode.

**ZOOM OUT:** Click the **'Zoom Out'** icon on the toolbar s and click on the left mouse button to obtain a zoom lens out of a 20%.

MANUAL ZOOM: Click 'Manual Zoom' on the toolbar, as you can see below:

i.i. · K + D IL 🗉 🕄 🔊

Manual zooming is also available from the menu 'View/Zoom/Manual Zoom'. The manual zoom is slightly different in 1D to that in 2D NMR spectra where you may select spectral spectral limits for both dimensions.

1. If you are working on a 1D-NMR spectrum, a dialog box like this will open:

Manual Zoom	2
Horizontal	OK
From: -4,2668 🗢 To: 16,3000 🤤	Cancel
ppm     Hz     Points     sec	

You can select the limits of the spectral region of interest in ppm, Hz, points or sec and then click 'OK'.

2. If you are working on a 2D-NMR spectrum, the dialog box will look like this:



Select the horizontal and vertical limits of the region of the spectrum that you want to zoom in on, and click 'OK'.

#### OTHER ZOOMING MODES

**1. FULL SPECTRUM:** This tool may be used to revert to a full spectrum from a zoomed view. This may be done from the menu 'View/Zoom/Full Spectrum' or by using the **'Full Spectrum'** icon **I** on the toolbar.


**2. FIT TO HIGH:** The Fit to High function adjusts the display of spectral intensity in both 1D and 2D spectra so that the strongest signal is optimally displayed.

**3. FIT TO HIGHEST COMPOUND:** The Fit to Highest function adjusts the display of spectral intensity in both 1D and 2D spectra so that the strongest compound signal is optimally displayed (discarding solvent or impurity peaks). You can select this mode by default from the 'Edit/Preferences/NMR/Import' menu.

**4. PANNING:** While the spectrum is in a zoomed state, click on the **'PAN'** icon . on the toolbar (or hold down the space bar, or hover the mouse over an axis), hold down the left mouse button and drag the *hand cursor* in any direction to navigate throughout the spectrum. In order to select vertical or horizontal panning only, press the <P> key whilst in the **'Panning'** mode.

You will be able to toggle the Full View window by using the F2 key. This will allow you to get a 'Super Fast' panning by using the Full View window..

**4. ZOOMING COMBO BOX:** In addition to the traditional **'Zoom In'** mode, **Mnova** also allows the user to apply different zooms, including Zoom Out (from a zoomed state), by using the zooming combo box.




These zooming modes are:

- ✓ <u>Percentage zooms</u>: These allow different size views of the object, by selecting the different percentages available (from 400 to 25%).
- ✓ Entire Page: This is the standard view, which can be seen in all the figures above.
- ✓ Page Width: In this view, the program will fit the size of the paper to the window width, whilst


preserving the original paper proportions.

✓ <u>Entire Window</u>: This is a special view within Mnova. It will fit the size of the paper to the size of the available window, to optimize the available screen area. This view represents an exception to the WYSIWYG concept, since in this case the proportions of the screen paper may differ from the proportions of the printer paper and therefore of what you will get when printing the page.

The **Entire Window** concept deserves further comments. For example, consider the following scenario in which the page zooming mode is set to **Entire Page**:

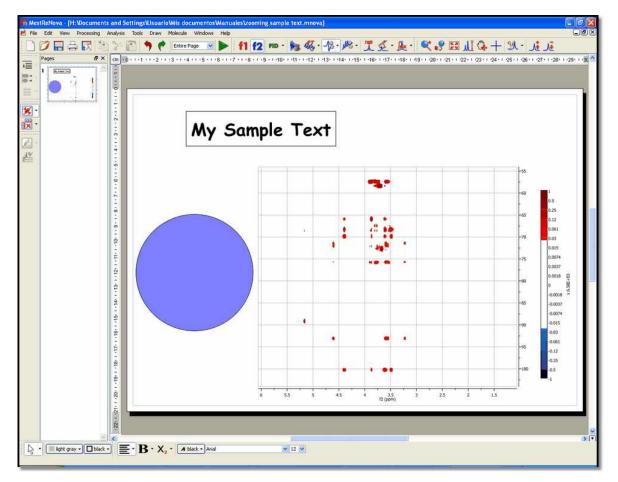

As seen in the figure above, Mnova is a fully **WYSIWYG** application. This can be appreciated in the blue circle which was created with the **ellipse** tool and then its dimensions set to form an actual circle. However, in this case there is a significant space of the window which is not covered by the page (see gray regions surrounding the page) which can be considered as wasted space. In order to make the most of the available space, we can use the so-called **Entire Window** zooming mode. In this mode, the page stretches to fit all the available space. Of course, this means that paper proportions (i.e., width/height ratio) have to be changed and thus the WYSIWYG principle is broken. As always, a picture is worth a thousand words:

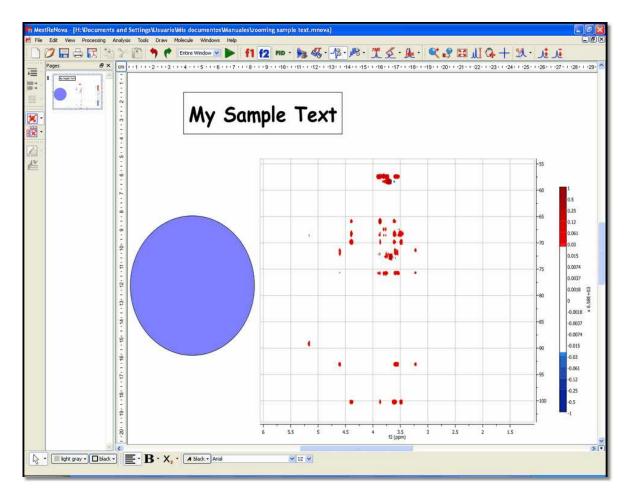


Note that all the objects are now distorted. However, this mode is very convenient to work with spectra on the screen as the graphical spectral proportions are rarely an issue. Nevertheless, if you print a document in this non WYSIWYG mode, you will get exactly the same results as when working on real WYSIWYG modes.

Please bear in mind that you can copy the zoom areas from one spectrum to another just by doing Ctrl/Cmd+C in the first one and 'Edit/Paste Properties/NMR View Options':

Edit	View Database	Processing	Analysis Advanced Stack Ma
•	Undo	Ctrl+Z	🥐 Entire Page 💌 📐 🔳
4	Redo	Ctrl+Y	8×
*	Cut	Ctrl+X	
3	Сору	Ctrl+C	
	Copy Special	•	
-	Paste	Ctrl+V	-
-	Insert Object		E
?	Paste Special		- Number δ (ppm)
7	Paste Properties	•	NMR Graphic Properties
×	Delete	Del	NMR Integrals
-	Select All	Ctrl+A	NMR Peaks
	Alignment	۲	NMR Peaks & Snap NMR View Options
-	Description		


### 7.13.1 Full View

**'Full View'**: (Not to be confused with 'Full Spectrum) will bring up a miniature view of the entire working document with the active area of the spectrum highlighted in blue, as you can see in the picture below:

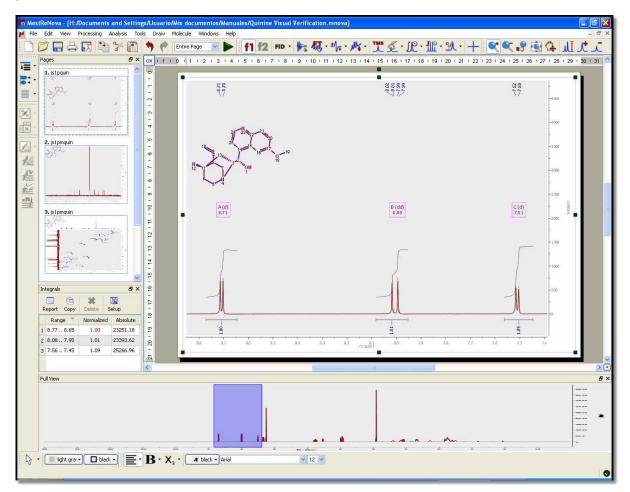


You will be able to toggle the Full View window by using the F2 key. This will allow you to get a 'Super Fast' panning.

If **'Apodization'** is selected from the Processing menu (or from the toolbar icon **Full**) then the **'Full View'** switches to show the FID and the effective window function. This allows you to manipulate the FID (using apodization for example) and observe the effect on both the FID and the spectrum.

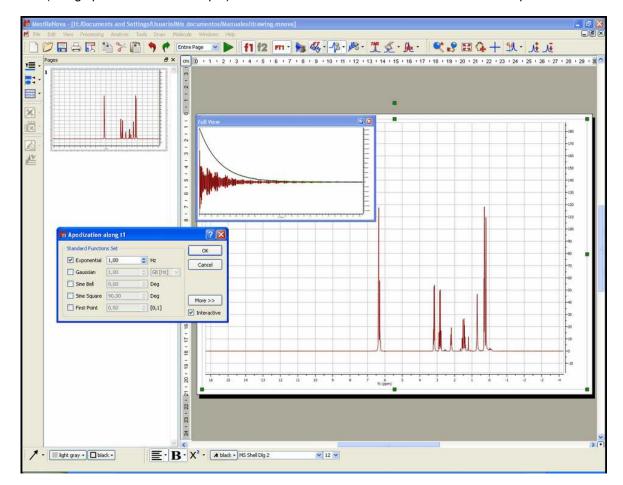

### 7.13.2 Create Expansions

You can create expansions with Mnova by clicking on the corresponding icon of the toolbar [] (or by pressing the  $\langle E \rangle$  key) and then holding down the left mouse button and dragging the *magnifying glass cursor* (with a red horizontal segment) over the area of interest. A highlighted rectangle indicating the new spectral region to be expanded once the mouse is released, will follow the cursor. You can see in the picture below an example of this feature:

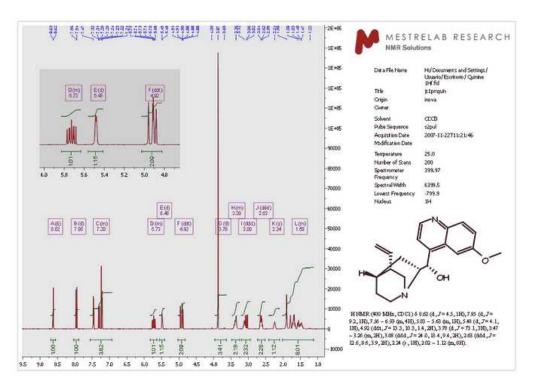

# 7.14 Cutting Spectra

THE SPECTRUM CUTTING TOOL

This is a tool that most **Mnova** users will not have seen before (with the notable exception of **iNMR** users). It is important to note that this tool is in no way related to the "copy", "cut" and "Paste" object manipulating tools found in this and most Windows programs as Icons and in the Edit drop-down window. The **'Cutting'** tool allows the user to create **dark** regions, i.e., to hide areas of the spectrum the user is not interested in seeing (these could be noise regions or other regions which are of no interest at a specific time). By hiding these regions, areas of interest become larger on the screen without a need to create numerous expansion windows. The Cutting Tool is basically a way of split zooming, as opposed to the more limited traditional zooming in a single block. The hidden areas are shown on the scale and on the grid. The software also implements an **Auto Cut tool**, which will hide all noise-only regions of the spectrum at the click of one button.


It is important to stress that this tool is not eliminating the information, but simply not displaying it. The 'Cut' and 'Auto Cut' options are available from following the menu item 'View/Cuts/Cut' or 'View/Cuts/Auto Cut'. Manual cutting can also be accessed by clicking on the **'Cut'** icon (or simply, by pressing the <X> key) as can be seen in the figure below. Auto Cut can be accessed via the drop-down menu which can be displayed by clicking on the side-bar of the Cutting Icon.



You can **restore** one specific region ('Restore', or <V> key), a limited region ('Manual Restore') or all regions ('Restore All'). These options can be selected from the menu 'View/Cuts/Restore',

'View/Cuts/Manual Restore' and 'View/Cuts/Restore All' or by selecting 'Restore', 'Manual Restore' or 'Restore All' in the scroll menu shown in the figure below.

By the way, you should also note that the 'Cut' mode is available in 2D, along direct, indirect or both dimensions. Once again, switching between modes is achieved by simply pressing the <X> key.

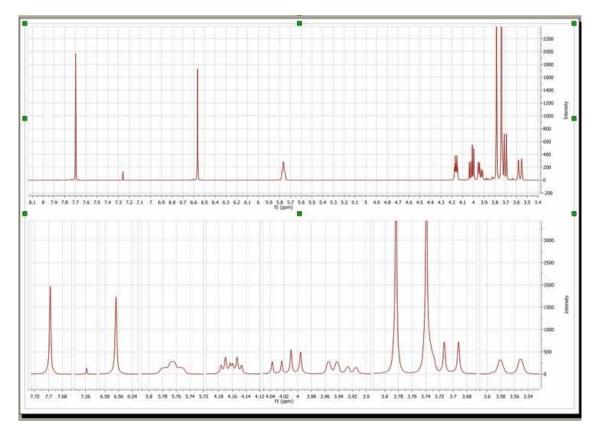

#### **Manual Cutting**

The user will be also able to use the 'Manual Cut' to select the limits of the dark regions.

8.600	
7.900	
7,100	
0.000	
	7.900

The user will be able to predefine the cuts ranges to automate the cutting analysis. Clicking on OK, will cut the current spectrum with the desired ranges and keep the regions to apply further cuts to additional spectra.


The user will be able to save these regions for later uses, by clicking on the **'Save Cuts'** icon which will be loaded by clicking on the **'Load Cuts'** icon

## 7.15 Blind Regions


This feature will be used to select regions from your spectra which will skipped by the automatic phase correction algorithm and analysis algorithms such as integration, peak picking or multiplet analysis. Conversely, blind regions will not be saved or searched in the Database. This will allow users to ignore areas of the spectrum which present particular challenges, whilst still being able to use the rest of the information in the spectrum (for example, ignore non-phasable signals in solvent suppressed spectra when doing quantitation).

You will be able to select the Blind Regions by following the menu 'View/Blind Regions/Add Blind Region' and clicking&dragging on the regions of interest.

In the example below, you can see how we have added a blind region to the dispersive signal of the water in order to apply an automatic phase correction to the spectrum without taking into account that signal. We can get similar result by using the <u>cutting tool</u> (to hide the solvent signal):

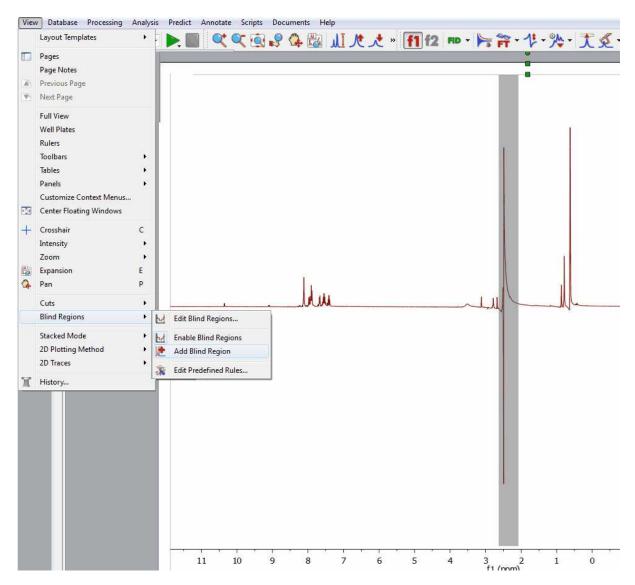


Selecting the 'Edit Blind Regions' will display a dialog box which will allow you to save the regions, to load another 'blind regions' file, to enable/disable the highlight of the blind regions will additional blind regions will display a dialog box which will allow you to save the regions, to load another 'blind regions' file, to enable/disable the highlight of the blind regions will additional blind regions.

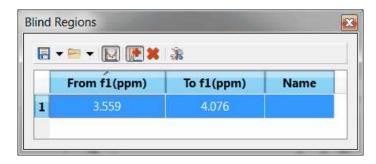

Right clicking on any cell of the table will allow you to delete or disable the applicable blind region. You can also delete them by clicking on the red cross button

If you have previously saved any blind regions, you can use it as 'Predefined Rule'



Clicking on the 'Open scroll down menu, you will be able to open any saved regions (including some templates for the common solvents by default).

Dimethyl Sulfoxide-d6	
Acetic Acid-d4	Na
Acetone-d6 Acetonitrile-d3	
Benzene-d6 Chloroform-d Cydohexane-d12 Deuterium Oxide	<b>*</b>
4 ( m	

Selecting the 'Import' option in the 'Open' scroll down menu, will allow you to load XML files containing the blind region limits.

### 7.16 Increasing and Decreasing Intensity

The two icons ICOC towards the right of the standard toolbar allow the user to interactively scale the data of the NMR spectrum. This operation does not modify the acquisition or the MestreNova data file; it only magnifies or diminishes the representation of the data which you see on your screen. You can also find these options via the 'View/Increase Intensity' and 'View/Decrease Intensity' menus. Additionally, you can use the '+ key' to increase or the '- key' to decrease the intensity and the same effects may be obtained by rotating the scroll wheel of the mouse.

The intensity increases/decreases 10 times slower if the user press the Ctrl/Cmd key while moving the mouse wheel.

# 7.17 Undo & Redo

### 7 🥐 🛛


**Undo** is a very useful command; it erases the last change made to the document, causing the document to revert to an earlier state. The **Redo** command reverses the undo.

**Mnova** has very powerful **Undo** and **Redo** capabilities. These can be applied to virtually any operations carried out by Mnova, from creation of pages and opening of documents through zooming, panning, and annotating, to any processing or analysis operations. Undo & Redo in Mnova are virtually unlimited (RAM memory limitations may apply). These options can be found as the toolbar icons shown above or via the 'Edit/Undo' and 'Edit/Redo' menus. Additionally, there are keyboard shortcuts for these operations, <Ctrl+Z> (or Cmd+Z for Mac) for Undo and <Ctrl+Y> (or Cmd+Y for Mac) for Redo.


## 7.18 Graphics and Annotations

**Mnova** has the most powerful graphics and annotation capabilities available in any NMR software. Most of the annotations and drawing available in MS Powerpoint are available in Mnova via the graphics toolbar placed by default at the bottom of the screen, below the page navigator and the document area. The software supports Rich Text and so a wide range of fonts and font embellishments (sub- and superscript, bold, italic etc) are available.

Mnova can import objects such as **molecular structures** using Edit/Insert Object while **images** may be embedded using the standard Windows Copy and Paste tools.

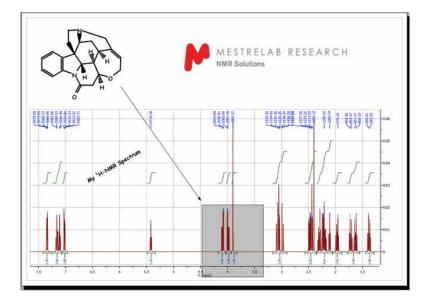

You can draw a curved arrow, line, a rectangle, an ellipse or a polygon by following the menu 'Edit/ Annotate' or by using the graphic toolbar, as you can see below. Once you have selected the object you want to draw, hold down the left mouse button in the spectrum display and drag the cursor over the area where the line or shape is to be drawn. Once created the line/shape may be moved, rotated and resized by selecting it and using the object's moving, sizing and rotating "tabs". You can also choose the fill color (light grey as default) as well as the colour and linewidth of the border of the object (black as default). Text may be added to the document in much the same way (T is the shortcut). The text can be aligned (right or left justified or centred) and you can select the text features **Bold**, *Italic* and <u>Underline</u>, sub-and superscript and the font (color, type and point size).

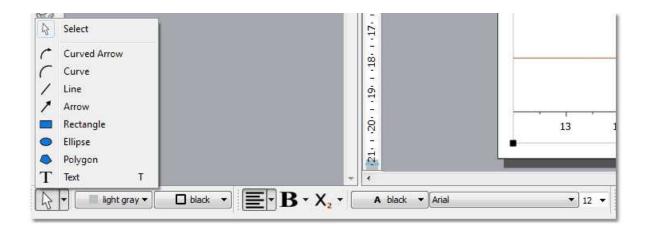




# 8 **Processing Basics**

Our aim in developing Mnova has been to make the opening, processing, handling, analysis, saving and printing of NMR data simpler than it has ever been before, so that even the NMR novice can enjoy the software and obtain excellent results from the very start.

Mnova introduces a brand new NMR data processing paradigm; when a raw, unprocessed spectrum (FID) is opened, you will get the fully processed spectrum instantaneously.

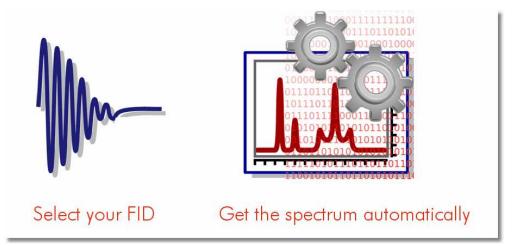

This new concept consists of two fundamental points:

- 1. <u>Automatic File Format Recognition:</u> Once you select the FID, Mnova will automatically identify its origin (e.g. Varian, Bruker, Jeol, etc).
- 2. **Fully Automatic Processing:** Once the FID is opened Mnova will automatically and optimally process it using the information it discovered in Part 1, so you do not need to bother with processing details.

The two steps outlined above will successfully process most NMR data. However, if you are not completely satisfied with the result you can, at anytime, reprocess using your own choice of processing parameters, changing or adjusting the window function, the FT, the phasing and baseline correction to meet your requirements.


With this scheme, processing of 1D and 2D spectra is essentially identical as you will see in the following two tutorials:

1D NMR Processing 2D NMR Processing

### 8.1 1D NMR Processing Tour

#### Opening the data set

In pulsed NMR spectroscopy we obtain what is called a *time-domain signal* since the measured signal is a function of time; all the nuclear resonances decay from the same starting time to form the Free Induction Decay or FID. This kind of signal is not readily interpretable by the human eye, and so it is necessary to transform it (into the frequency domain) using a Fourier transformation (FT) to display the separate nuclear resonances as a frequency spectrum.

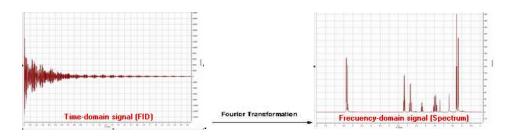


There is one single command for opening all types of files in **Mnova**. It is not necessary for the user to have any knowledge about the way in which the experiment has been acquired. **Mnova** will automatically recognize most common spectrometer file formats and acquisition modes and will apply the necessary processing operations.

To open your data (including mol files and graphics files), just go to '*File/Open'* menu, use the keyboard shortcut <**Ctrl+O**> (or Cmd+O for Mac) or click on the '**Open'** icon on the toolbar (note that this is exactly the same for 1D and 2D data). You can also drag&drop into Mnova, the folder containing the FID (the FID must be in the first level of folders)




Once this command has been issued, navigate through your disk to find the NMR experiment of interest and select the desired FID file which is normally named **fid**; however in Bruker 2D experiments the time domain data is named ser (serial fid). After selecting this file, the first thing you will notice is that the spectrum will open **already processed**, despite the fact that you are opening raw data (FID). When opening files, Mnova will apply the necessary processing operations, selecting the correct processing parameters from the spectrometer files. If these parameters are not available (e.g. phase parameters are not available), Mnova will use automatic algorithms (e.g. automatic phase correction) and will apply them to the data set. Thus, even a completely inexperienced chemist, working with NMR for the first time, should be able to get good results when processing both 1D and 2D spectra.

In the figure below you will see what happens when the FID is opened:

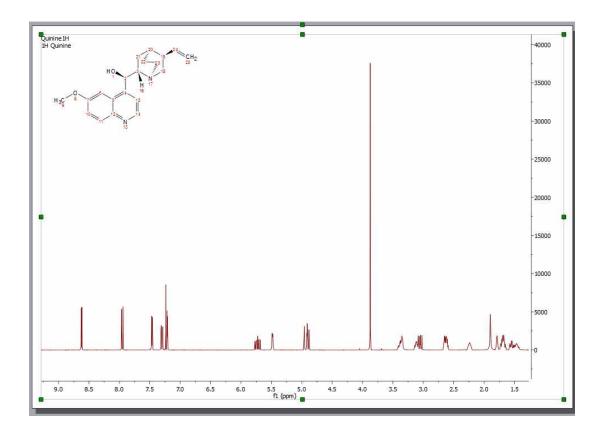

As explained above, the FID is automatically processed. In this case, the native files contained values for phase correction and thus Mnova utilized them for phasing. However, as you can appreciate, the result is not good enough (most likely because the spectrum was processed in the spectrometer computer using an inefficient automatic phase correction algorithm). Later we will show how to improve the phase of this spectrum by applying first the automatic phase correction algorithm implemented in Mnova and finally using manual phase correction. Remember that if the native files do not contain values for phase correction, Mnova will apply an automatic phase correction.

Even though you have opened a FID and you see only the processed spectrum in Mnova, you can see the **original FID and the processed FID** (Processed FID or **FID'**). When we process the raw data on-the-fly, we do not discard these data, we just do not display them. The user can view the FID by just clicking on the '**FID'** icon on the toolbar:




There are several options in the scroll down menu:


- **Original FID**: Clicking on this option will show the original *time-domain signal* (FID) as it was when ported from the spectrometer.
- **Processed FID**: Clicking on this option will show the FID after time-domain processing functions have been applied (i.e., immediately prior to FT)

- FT1: Clicking on this option will show the data after FT along the direct dimension (spectrum for 1D data, interferogram in 2D data)
- FT1': it will display the processed fid before the second FT (in t1):
- FT2: Clicking on this option will show the data after FT along two dimensions (2D spectrum)

For example, this is the original FID of our test spectrum:

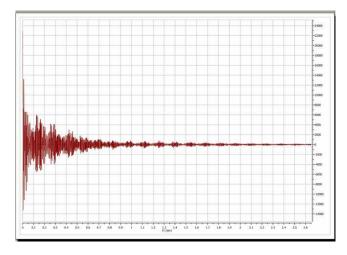

And this is the so-called **FID'**. In this case, prior to FT, Mnova applies a zero filling operation as can be appreciated in the FID' below. A zero fill increases the digital resolution by adding null data to the FID, increasing the size of the data array.

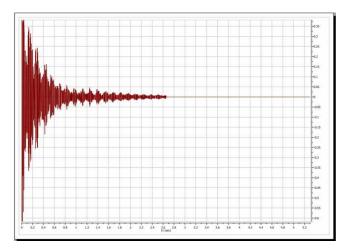

You can switch at any time between any of the displays (FID, FID' and processed spectrum).


#### Interactive Processing: Real Time Frequency Domain Processing

As we saw in the previous section, Mnova will keep all pre, during and post processing information together with the spectrum we can see on the screen. This fact, combined with the extremely fast and optimized processing algorithms implemented in Mnova, allows us to introduce to NMR processing the concept of **'Real Time Frequency Domain Processing'**, designed to greatly simplify processing for the user and to ensure faster and better results even when complicated operations are applied to the data.

The way this concept works is very simple: Reprocessing of the spectrum is possible at any time, independently of the time domain and frequency domain operations which may have been applied to

the data set (for example, to change the window function after having applied a FT, phase and baseline correction). This is possible because, in the background, Mnova is going back to the FID and reprocessing the spectrum by applying the new functions or parameters as well as all the other functions applied ad posteriori on the previous processing. The very important advantage for the user is that he can see, in **real time**, the effect of any processing operation (including time domain operations) on the resulting frequency domain spectrum (for example, you can apply a more drastic exponential apodization function and see in real time, on screen, what effect this is having on the resolution and sensitivity of the frequency domain spectrum).

In the figure below, you can see the frequency domain 1D spectrum, the FID with the window function which is being applied interactively (which is shown graphically in the 'Full View' window (go to the 'View/Full View' menu to activate), and also the Apodization dialog box - note that the 'Interactive' box is ticked). The user can follow the exact effect of the function s/he is applying on the frequency domain spectrum. This can avoid repeated transformation and reloading of the data while the optimum processing parameters are sought and, of course, act as an excellent teaching and self-teaching tool for those who are not conversant with the effects of different processing parameters.

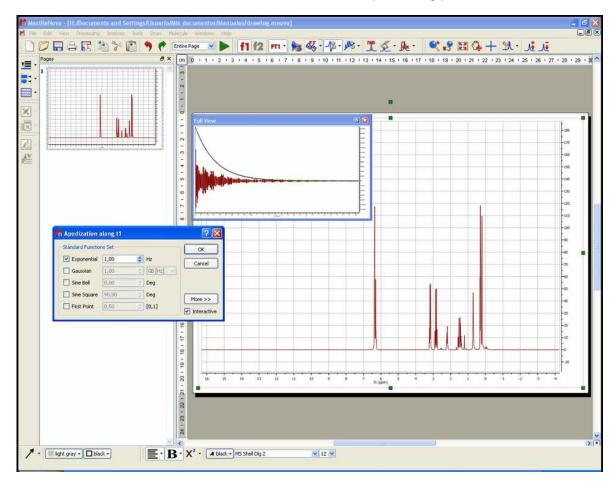

This same principle can be applied to all other processing operations, such as Zero Filling, Linear Prediction, Signal Suppression, etc. For example, if we want to increase the digital resolution of the spectrum, we can increase the number of points used in the FT operation by selecting **Zero Filling**.

Of course, standard frequency domain operations such as <u>phase correction</u> or <u>baseline correction</u> can be applied in the traditional way.

#### See also:


Phase Correction Baseline Correction

## 8.2 2D NMR Processing Tour

(Not available in Mnova Lite)

1D experiments contain a wealth of information but this information is often obscured due to signal overlap. Homonuclear couplings are often more readily and rapidly determined by extension into a second dimension. Heteronuclear couplings (1H-13C for example) are much easier to determine using two frequency dimensions. 2D experiments which use one frequency dimension and some other variable on the other axis (the DOSY processed STE experiment for example with diffusion coefficient on one axis) exist but this tour will concern two frequency (chemical shift) dimensions.

These 2D spectra are collected as time domain data dependant upon two time variables ( $t_1$  and  $t_2$ ) and after two orthogonal Fourier transformations a frequency spectrum which is a function of two frequency variables results. The general scheme for these **two** dimensional experiments is shown in the pulse sequence below:



In the *Preparation Time*, the sample is excited by one or more pulses and the spin system is placed in a non-equilibrium state which will evolve later. During the *evolution* period, the resulting magnetization evolves freely. Each signal will evolve with its characteristic frequency. Then follows the *Mixing Time* containing a further pulse or pulses; it is in this period that, for example, magnetization, may be transferred from proton to 13C during indirect detection. Finally the signal is recorded (detected) as a function of the second time variable,  $t_2$ ; the signal has, however, been frequency-labelled as a function of  $t_1$ .

After acquiring a bidimensional experiment, you will have a matrix of data; the rows contain data collected at fixed values of  $t_1$  with  $t_2$  varying; they are, in fact, normal 1D data FIDs. The columns contain data collected at fixed values of  $t_2$  with  $t_1$  varying and are "synthetic" 1D FIDs. This matrix will be fourier transformed twice, once for the rows and again for the columns. In this way, the time dimensions ( $t_1$  and  $t_2$ ) are converted into frequency dimensions ( $f_1$  and  $f_2$ ).


In a 2D-NMR experiment we can find any nucleus represented on either of the dimensions of the spectrum, so the spectrum can show correlations between the same nuclei (<sup>1</sup>H/<sup>1</sup>H) or different nuclei (such as <sup>1</sup>H/<sup>13</sup>C, <sup>1</sup>H/<sup>15</sup>N, <sup>1</sup>H/<sup>31</sup>P, etc...). In a 2D-NMR spectrum, the acquisition dimension ( $t_2$ ) is the dimension in which we can obtain the greater number of data points without a considerable increase of the acquisition time. On the other hand, each point acquired in dimension  $t_1$ , multiplies the necessary number of scans, considerably increasing the total acquisition time. For this reason, in many cases the number of data points must always be must always be sufficient to provide adequate  $f_1$  resolution. The "synthetic"  $f_1$  FIDs are generally truncated and may benefit from forward linear prediction.

Processing of 2D NMR data sets with Mnova is almost as easy as processing 1D NMR data. You simply select the FID file (or SER file in Bruker) and the 2D spectrum appears on your screen without the need to touch a single button.

In this tutorial we will show how to process a 2D experiment. This tour will guide you through all the necessary steps to process, display, and print out two dimensional spectra with Mnova. Before you attempt to process a 2D spectrum, please read the <u>1D NMR Processing Tour</u> since you need to be able to process 1D spectra also.

Multidimensional (or bidimensional) data processing requires only a few new concepts when compared with 1D NMR data processing. A 1D-NMR spectrum can be considered as a single vector of data points and its transformation into the frequency domain only requires only one FT. In the case of 2D spectra we have a two dimensional matrix of points and it is necessary to Fourier transform both rows and columns.


In 2D homo- and heteronuclear NMR the matrix of points results from an array of 1D FIDs which are functions of  $t_2$  due to their detection (sampling of the FID at intervals of delta- $t_2$ ) and  $t_1$  since each successive FID the value of  $t_1$  which determined the evolution time, is incremented. The first row has  $t_1 = 0$ , the second row has  $t_1 = \Delta_1$ , the third row has  $t_1 = 2\Delta_1$  and so on. The same happens with the data columns, although in this case the sample interval is different ( $\Delta_2$ ).

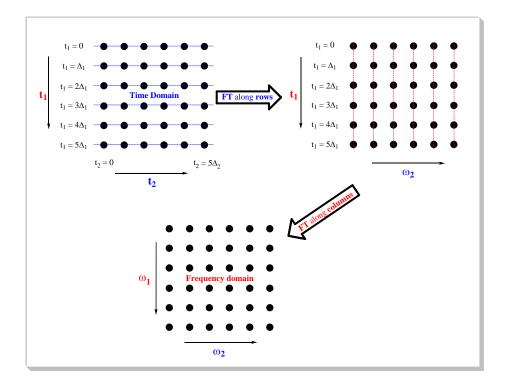

As you can see in the picture above, the first step is the application of the FT along the rows of the matrix; to obtain a new matrix (*interferogram*) where each row corresponds to an increasing value of  $t_1$  and each column to a running frequency variable  $\omega_2$ . Next the columns are subjected to a FT to obtain the final matrix (2D spectrum) where the frequency axes ( $\omega_1$ ) corresponds to the evolution in  $t_1$ , while  $\omega_2$  corresponds to the evolution in  $t_2$ .

This 2D data can be processed using apodization functions and once you obtain the 2D spectrum, you can apply a phase or a baseline correction as with 1D processing. One important point is that processing operations need to be performed along each dimension. In Mnova, the processing is always started along the acquisition dimension, and finished along the indirect dimension.


In this example we will use a Bruker spectrum so you will need to select the **ser** file. Once you do so, you will immediately obtain the processed spectrum:

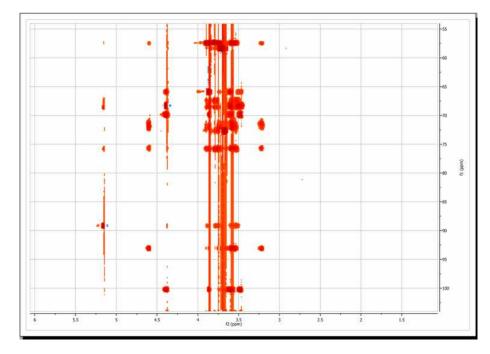

The program has performed the following set of operations on the fly:

- 1. Automatic file format recognition: The program identifies this file as a Bruker file and uses the corresponding filter to decipher the data
- 2. For each dimension:
  - <u>Weighting</u>
  - Zero filling
  - Fourier Transform
  - Phase Correction

The user can break the processing after the first FT along the direct dimension and also before the second FT (in t1)

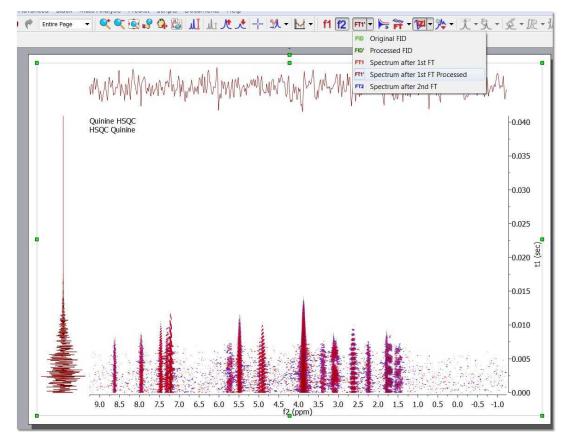

#### **Baseline Correction**

From the figure above, baseline artifacts along the indirect (f1) dimension are apparent. They can be easily removed by the <u>baseline correction</u> procedure. Select this option by clicking on the **'Baseline Correction'** icon to obtain an automatic **'Baseline Correction'** or by choosing 'Baseline Correction' in the scroll bar menu:



so that you get the following dialog box:

Method			Qk	ŝ
Whittaker Smoot	her	•	Cano	el :
Whittaker Smoot Polynomial Fit Bernstein Polyno Ablative Splines			Autodei	tect
-0	3 0	1 I	1 1	Ţ
Smooth Factor:	20000	* V	Autodet	tect


Baseline correction will be applied to the currently **active dimension** unless the Apply to All Dimensions option is checked. What does **active dimension** mean? The active dimension is the dimension highlighted on the toolbar and is generally the direct dimension. With the exception of <u>phase</u> <u>correction</u>, processing operations in Mnova default to the active dimension only. For example, if we want to process along columns (f1) you just need to set the processing dimension to f1 as depicted below:



As a shortcut, you can use the corresponding toolbar buttons:



In our present situation, as the current processing dimension is **f2**, baseline correction will take place only along this dimension. This is not appropriate for our case as it is evident that baseline distortions are present mainly along the indirect **(f1)** dimension. We can simply set the processing dimension to **f1** , but it is even simpler to check the Apply to All Dimensions option in the **baseline correction dialog box**. After applying the correction using default values, this is the resulting spectrum:

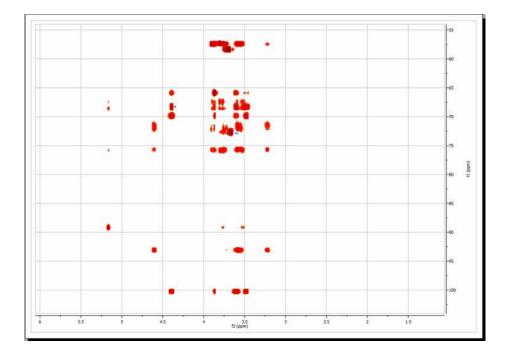


The user can show the traces of the 2D-NMR spectrum, just by clicking on **'Show Traces'** icon **I** In the same icon, you will find a scroll bar menu to setup the vertical and horizontal traces of a bidimensional spectrum. You can show the traces by default, by selecting the applicable option on the 'Properties dialog box and clicking on the 'Set as default' buton.

See also 'Show traces in 2D-NMR'

#### More on real time frequency domain processing

In the <u>1D NMR Processing</u> section, we described the real-time frequency domain processing concept. **Diagonal Suppression** of homonuclear 2D experiments represents another example of this concept. This technique is typically carried out in the mixed time-frequency domain (interferogram). However, this is something you do not need to know in Mnova. You can suppress the diagonal while the transformed spectrum is on the screen.

For example, the figure below shows a 2D magnitude spectrum:

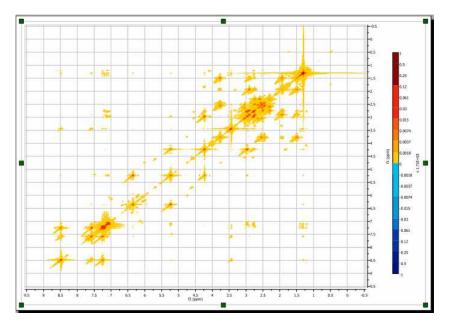


To suppress the diagonal, just click on the small arrow at the right-hand side of the FT toolbar button (see below) and select the **Diagonal Suppression** command:



Mnova provides different algorithms for this task. In this example we will select the Wavelet method

Method Wavelet		
Parameters		
Dyadic Levels:	4	**
Daubechies Coefficients:	12	Y

And this is the resulting diagonal-free spectrum.

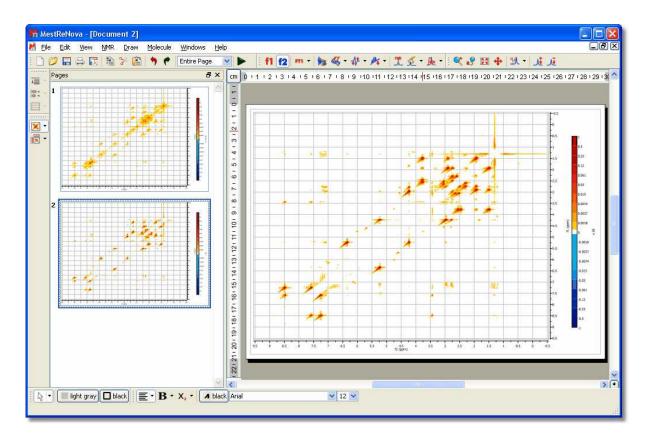

Note that in the figure above there are two pages, the first one containing the 2D spectrum with its original diagonal, and the second one after the diagonal has been removed.


#### See also

Phase Correction Baseline Correction


## 8.3 Stacked NMR Processing

Many types of experiments require obtaining a series of FIDs, related to each other through the variation of one or more parameters (temperature, concentration, solvent...). The user, for example, may need to run several spectra at different temperatures: 270K, 300K, 330K, 360K and 390K. Instead of acquiring five different sets of data, the user is able to create an array in which the temp parameter is given for successively different values.


Creating a stacked (or pseudo 2D) spectrum with Mnova is very easy; just by **dragging** one spectrum from the 'Page Navigator' to another spectral window. In the example below we are dragging the first page into the second spectrum to generate a stack plot:

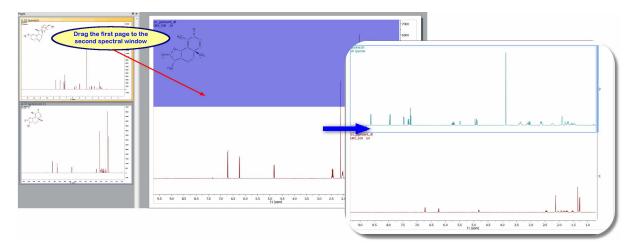

You can use this method to add a spectrum to an existing stack. In the example below we are adding the spectrum in the second page as the trace 19th of the stacked plot:

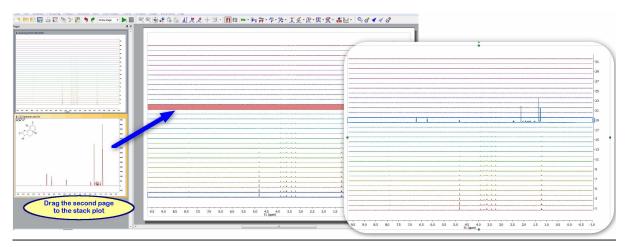


You can also create a stack plot by selecting the desired spectra in the page navigator (by holding down 'CTRL/Cmd key' while clicking on each spectrum) and then issue the command 'Stack/Stack Items' (or by pressing the applicable button in the left-vertical toolbar):

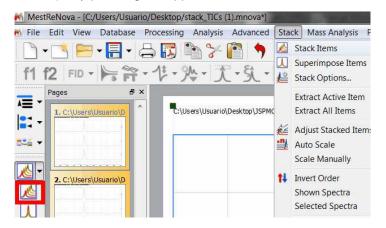



By default Mnova will not delete the 1D spectra after having stacked them. If you want to modify this default, you will need to follow the menu 'Stack/Stack Options' and uncheck the applicable box.

Additionally, Mnova can detect spectra which have been acquired in the so-called arrayed-mode (or pseudo 2D), typically used in relaxation, kinetics or diffusion experiments. For all these cases, Mnova will only process the acquired dimension (t2). Basically, Mnova will process only the rows of the data matrix and, by default, will display the spectrum as a stacked plot (see below):

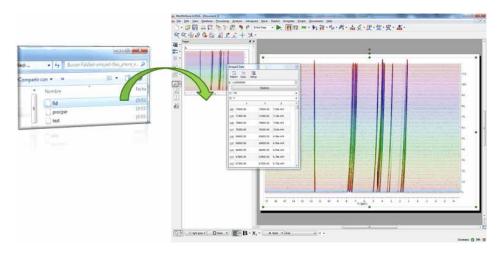

#### A few tips on Stacked Spectra

- Change the stacked angle to zero (15° by default) in the properties dialog box (by double clicking on the spectral window).
- Normalize the spectra (if they have different intensities) by using the command: 'Processing/Normalize'.
- Highlight the desired trace of the stack plot just by clicking on it.
- Create a stack spectrum just by dragging one spectrum to another.

### **Display Modes:**

The main features to handle arrayed spectra will be described below:


- Multiple display modes: Stacked, superimposed, active, bitmap
- · Ability to select multiple spectra and apply processing only to those selected spectra
- · Ability to hide any number of spectra
- Multiple selection can be done either graphically in the stacked plot mode or by means of a table
- · New powerful algorithm for the automatic alignment of arrayed spectra
- Ability to automatically import any number of spectra and automatically stack them
- New selection mode to extract NMR descriptors (e.g. integrals) with the ability to adapt its shape to any profile (useful when peaks are not aligned)

As you well know there are several display modes of arrayed datasets, as stacked, superimpose,


active or bitmap. You can select the mode by using the scroll down menu of the vertical toolbar:




**'Active Spectrum':** to see only the highlighted spectrum. Within this mode, you can navigate along all spectra in this stack by using Shift+Mouse wheel (or arrow keys up&down).

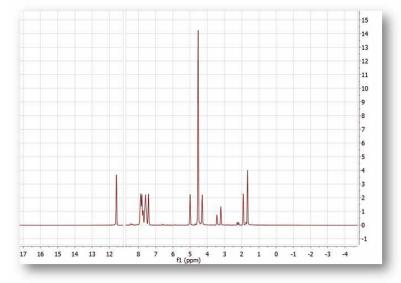


'Stacked': to see all the spectra in arrayed mode. You can change the angle from the Properties dialog box.

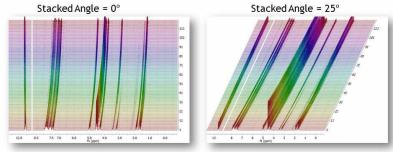

'Superimposed': to see all the spectra overlayed (one over another).

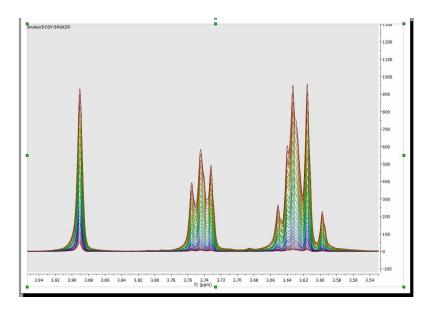


For metabolomics studies it is important to superimpose multiple spectra and compare their shape, e.g. to identify which ones are outliers. In such a mode, when the user sets a spectrum as the Active spectrum, that spectral curve will be displayed with a thicker curve:

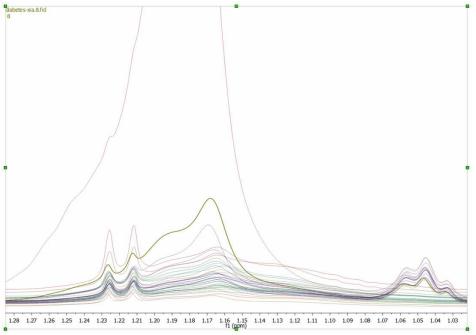

Follow the menu 'Edit/Properties/Stack' to customize 'Active pen width factor' (2.00 by default) and 'Secondary Transparency:

▼ ■ ometry NMR Spectrum			
General Grid	Stacked Stacked Angle:	0.00	-
🗼 1D	Top Margin:	5.00 %	*
Kacked	Bottom Margin:	5.00 %	
<ul> <li>Scales</li> <li>Horizontal</li> <li>Stacked</li> <li>Peaks</li> <li>Integrals</li> </ul>	Clipped Vertically	Hue Color marcon	*
	Superimposed		
M Integrals	Active Pen Width Factor:	2.00	*
Fitting	Secondary Transparency:	0.50	A

'Bitmap': too see all spectra in a bitmap mode.

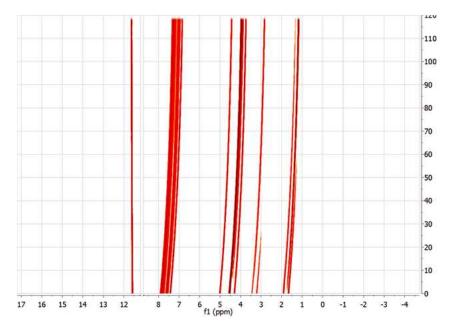

## **Multiple Spectra Selection**

Mnova includes a powerful, yet easy to use *multiple spectral selection* mode, which allows the user to optimize the processing of groups of spectra by selecting a bunch of spectra and applying any processing (e.g. manual phase correction to the selected group)

Multiple spectra selection can be done either graphically from the stack or directly from a table

In addition, Mnova offers the ability to hide any number of spectra in an arrayed item.

## **Graphical selection of spectra**

In order to be able to select a bunch of spectra graphically with the mouse, it is necessary to display

the spectra in the stacked plot mode

To select a single spectrum, **left click** on the spectrum trace while keeping pressed the **Alt key** To deselect a spectrum: **left click + Ctrl + Alt** 


In order to select multiple spectra, follow the same operation as above while keeping pressed Alt and/or Shift keys.

The following slide will show how to select several groups of spectra


### Some important concepts: Active spectrum vs Selected spectrum/spectra

**Selected spectra:** when the spectra are selected, they are highlighted with a light blue background. Any processing operation will take place only for those selected spectra

Active Spectrum: active spectrum is marked with a blue box and it indicates the spectrum which will be displayed in the *active spectrum* display mode. It's also the reference spectrum used in some processing operations (e.g. alignment)

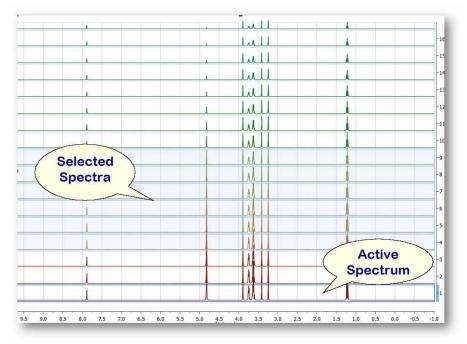

You can also **select** several slides by using the check boxes on the right of the 'Stacked Items Table'. When the spectra are selected, they are highlighted with a light blue background. Any processing operation will take place only for those selected spectra.

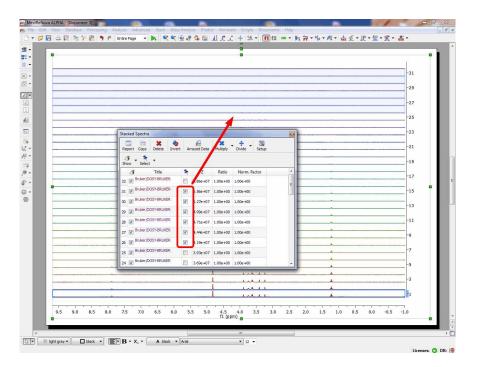


#### Example #1:

If there are no spectra selected and the active spectrum is not either selected (i.e. no spectra have a blue background) then **any processing operations will be applied to ALL spectra (**Active spectrum is not selected)

	<u></u>		_
	iii	1	
*			
i	1		
		<u> </u>	
		<b>1</b>	
i			
<u>↓</u>			
Î.			
	· · · · · · · · · · · · · · · · · · ·		
	<u>────</u> ╊───┼╂╫┼┼		
1			


#### Example #2:

If only the active spectrum is selected, *any processing operations will be applied ONLY to the active spectrum.* (Remember, to select a spectrum: left click + Alt)

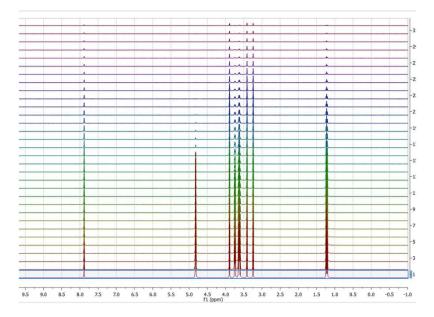

#### Example #3:


In general, *any processing operation will be applied only to the selected spectra* (and remember that if no spectra are selected, All spectra will be processed):

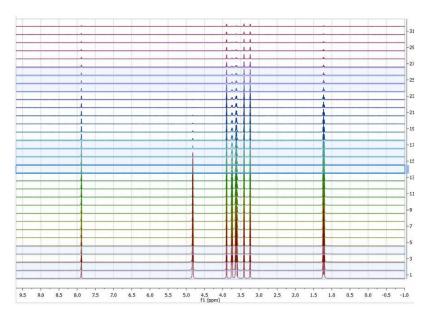

### See also 'Table of stacked items'


To navigate through the traces in the stack plot, press and hold down **SHIFT** and use the up or down arrow key (or use the mouse scroll wheel). The **active trace** will be highlighted by default with a blue rectangle, whilst **selected traces** will be highlighted with a light blue background (those marks will not be exported whit the stack plot). Any processing operation will take place only for those selected spectra.

Please note that in strange cases, Mnova shows some arrayed datasets as 2D plots. In those cases just follow the menu 'Stack/2D to 1D stack':



### Scripts to autophase importing autophase stacked spectra when importing.


Following the menu 'Scripts/NMR Tools', you will find a couple of scripts to apply automatic phase correction to a stacked plot:




- Auto-Phase Current, Same Phase Rest: the active spectrum is automatically phase corrected, and the resulting values of PH0 and PH1 are applied to the other spectra in the stacked.
- Same Phase as Current: PH0 and PH1 values of the active spectrum are applied to the other spectra in the stacked.

## 8.3.1 How to apply a peak picking or an integration analysis in stacked mode?

It is very easy to apply a peak picking or an integration analysis to a stacked spectra, just by clicking on the corresponding icon (or selecting the desired analysis function). In the picture below, we have applied an automatic peak picking and a manual integration of several areas of interest:

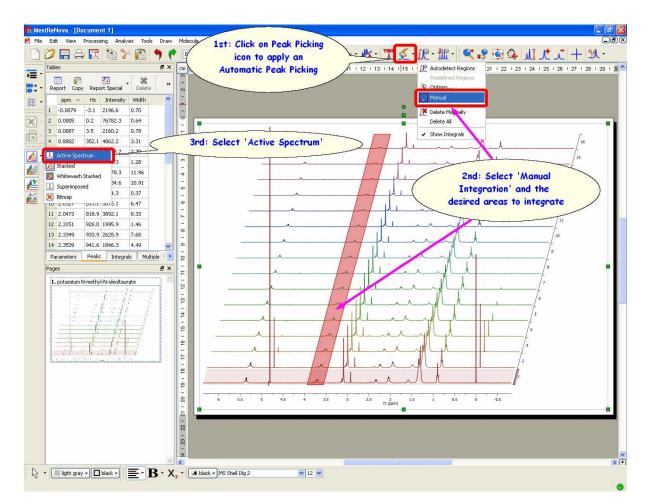


Then, just select 'Active Spectrum' in the vertical toolbar to obtain only the highlighted spectrum and you will be able to see the integrals and the peak picking. To navigate through the traces, press and hold down **SHIFT** and use the up or down arrow keys (or the mouse scroll wheel):

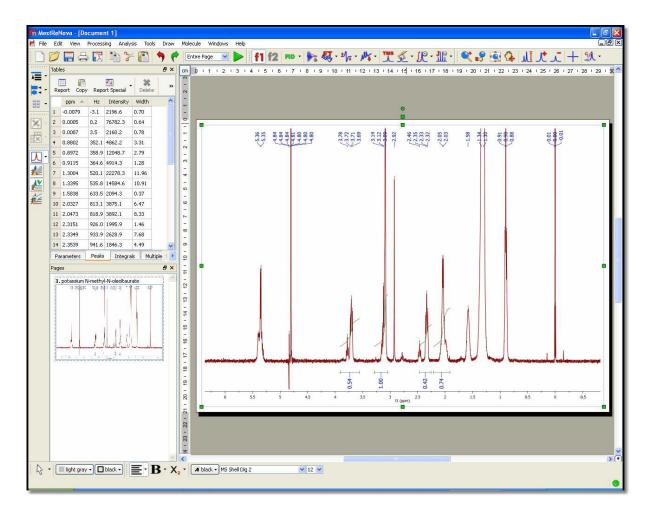

Finally you can export the peak picking or the integration analysis to a text file by following the menu File/Save as/Script:ASCII Matrix or 1D Integral Series (\*.txt). This will generate a text file which can be loaded into Excel (for example). Saving as "Script: NMR CSV Matrix (.txt)" you will get the zoomed area of all spectra distributed in columns (blind region and cut areas will be filled with zeroes). If you save it as "Script: NMR CSV Matrix (Transposed) (.txt)" you will get them in rows.


The user can apply the same integral normalization to all the spectra (in the current document) or to all the traces of a stack plot by selecting the applicable option:

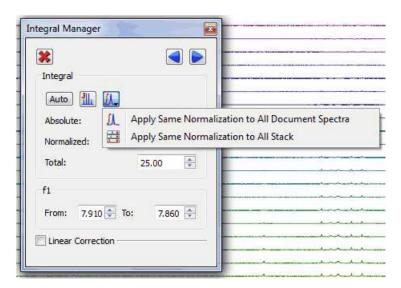

This is very useful if you need for example to determine relaxation times from a series of 1D spectra, to be able to compare the integral values between the different traces.

## 8.3.2 Setup Arrayed Spectra

This feature for the vertical & horizontal alignment of stacked spectra is contained within a panel which is available from the left-vertical toolbar or by following the menu 'Stack/Setup Spectra':

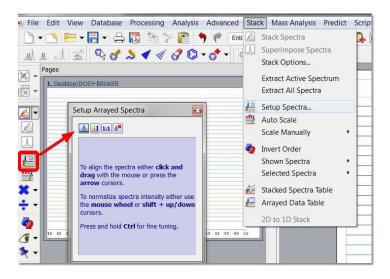

The way in which this control works is explained directly in the panel, in the same manner as with the phase correction panel:

Horizontal shifting: To align the spectra just click&grag to right or left. When the spectrum is shifted to the left or to the right, its chemical shift reference is adjusted to reflect that horizontal move.

**Vertical scaling:** This consists in changing the internal data points in the spectrum array by multiplying each point by a scaling factor. Note that this will have implications in the quantitation results.

Reset Intensities: this button will restore the intensity changes

Reset Shifts: this button will restore the shift changes.

Every change carried out during this process will be reflected in the stacked table. For example, if you move one spectrum 15 Hz to the right, that result will be shown in that table, so that it will be possible to use that value to measure, for example, a coupling constant or the amount by which a spectrum was shifted so that it perfectly overlaps with another spectrum.

Report	Сору	XX Delete	invert Order		2 tup			
X Multiply		de 🖌 S	🔏 🚽 🗙 Show Selec	• •[	Le Setup Spectr	a		
1				4		2010		
4			2	*	T/G	Ratio	Norm. Factor	Δ (Hz)
2 🔽 E	stradiol <u>.</u>			*	T/G 1.00e+00		Norm. Factor 8.65e+01	∆ (Hz) 0.00

## 8.3.3 Table of stacked items

This table (View/Tables/Stacked Items) makes it possible to select spectra as an alternative way to the graphical method but it offers more features, including the ability to **delete**, **hide** or **change the relative intensities** of any spectra:

Repo	ort Copy	Delete Invert	t Arrayed Data	Multiply		etup
Show	v Select	•				
	1	Title	*	T/G	Ratio	lorm. Facto
190	66353L	illy/190		6.64e+04	1.00e+00	1.00e+00
189	66002L	illy/189	E	6.60e+04	1.00e+00	1.00e+00
188	65650L	illy/188		6.56e+04	1.00e+00	1.00e+00
187	65296L	illy/187		6.53e+04	1.00e+00	1.00e+00
186	64945L	illy/186		6.49e+04	1.00e+00	1.00e+00
185	64593L	illy/185		6.46e+04	1.00e+00	1.00e+00
184	64241L	illy/184		6.42e+04	1.00e+00	1.00e+00
183	63890L	illy/183		6.39e+04	1.00e+00	1.00e+00
182	🔲 63538L	illy/182		6.35e+04	1.00e+00	1.00e+00
181	63187	illy/181		6.32e+04	1.00e+00	1.00e+00
180	62835L	illy/180	<b></b>	6.28e+04	1.00e+00	1.00e+00

T/G column: 'T' stands for Time whereas 'G' stands for Gradient. The underlying idea is that the Data Analysis module is intended mostly to analyse (1) Reaction monitoring and relaxation experiments in which case the independent variable would be expressed in seconds and (2) Pulse field gradient (aca DOSY) experiments where the independent variable would correspond to field gradients strength.

## Sorting traces:

The user can easily sort the traces of the arrayed spectrum by clicking on the 'Stacked Items Table'

E	to display the dialog box below:
icon 🖳	to display the dialog box below:

Repo	ort	Copy	X Delete	🧑 Invert	Arrayed Data	ML	🗙 🗸 🖡	ride Se	tup
	0	N.		Title		*	T/G	Ratio	Norm. Facto
700					-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
699	7				-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
698	mix of phenethylamine in 2methoxy phen						4.00e+00	1.00e+00	1.00e+00
697	V	Array-phenethyl_ester_TSP-300-18March mix of phenethylamine in 2methoxy phen					4.00e+00	1.00e+00	1.00e+00
696	V				-300-18March ethoxy phen		4.00e+00	1.00e+00	1,00e+00
695	7				-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
694	J				-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
693	V				-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
692	V				-300-18March ethoxy phen		4.00e+00	1.00e+00	1.00e+00
691	7	Array-p	henethyl_	ester_TSP	-300-18March	m	4.00e+00	1.00e+00	1.00e+00

Once there, **click on the number of the spectrum** for which you want to change the location and drag to the desired location. Clicking on the title header will sort the spectra in descending/ascending order by title.

# How to hide several spectra?

- It is really easy to hide slides, just:
- Select in the table all those rows corresponding to the spectra you want to hide

1.1	port	Сору	* Delete	Mart Invert	Arrayed	Sec. 24	X Multiply	Divide +	Setup	
	0		т	itle		*	T/G	Ratio	orm. Facto	
32		32 -> 5.	81326e+0	6			5.81e+06	1.00e+00	1.00e+00	
31		31 -> 5.	51645e+0	6		<b>P</b>	5.52e+06	1.00e+00	1.00e+00	
30		30 -> 5.	22873e+0	6			5.23e+06	1.00e+00	1.00e+00	
29		29 -> 4.	9474 <del>4e</del> +0	6			4.95e+06	1.00e+00	1.00e+00	
28		28 -> 4.	67516e+0	6			4.68e+06	1.00e+00	1.00e+00	
27		27 -> 4.	40939e+0	6			4.41e+06	1.00e+00	1.00e+00	
26	V	26 -> 4.	15256e+0	6		7	4.15e+06	1.00e+00	1.00e+00	
25		25 -> 3.	9023e+06				3.90e+06	1.00e+00	1.00e+00	
24		24 -> 3.	66092e+0	6			3.66e+06	1.00e+00	1.00e+00	

• and uncheck the boxes of selected rows:

	port	Copy	* Delete	Mart Invert	Arrayed	Data	Multiply	Divide •	Setup	
	4		т	itle		*	T/G	Ratio	orm. Facto	
32		32 -> 5.	81326e+0	6			5.81e+06	1.00e+00	1.00e+00	
31		31 -> 5.	51645e+0	6			5.52e+06	1.00e+00	1.00e+00	L
3		0 -> 5.	22873e+0	6			5.23e+06	1.00e+00	1.00e+00	
2		9 -> 4.	9474 <del>1e</del> +0	6			4.95e+06	1.00e+00	1.00e+00	
2		8 -> 4.	-> 4.67516e+06			4.68e+06	1.00e+00	1.00e+00		
2		7 -> 4.	-> 4.40939e+06				4.41e+06	1.00e+00	1.00e+00	
26	V	26 -> 4.	-> 4.15256e+06			V	4.15e+06	1.00e+00	1.00e+00	
25		25 -> 3.	9023e+06				3.90e+06	1.00e+00	1.00e+00	
24		24 -> 3.	66092e+0	6			3.66e+06	1.00e+00	1.00e+00	

You can follow the same operations to restore those spectra.

This table provides new options to easily hide or select any number of spectra

Stacked Spectra						Stacked Spectra					-
Report Copy Delete Inve		X Multiply	t Divide	Setup		Report Copy Delete Invert A	/ rrayed Data	× Multiply •	Divide	Setup	
Show Select						Show Select					
Show All	*	T/G	Ratio	lorm. Facto	-	Select All	*	T/G	Ratio	Iorm. Facto	*
Invert Shown	23	5.81e+06	1.00e+00	1.00e+00		32 📝 5. Invert Selection	13	5.81e+06	1.00e+00	1.00e+00	
Show Active Only Show Selected	E	5.52e+06	1.00e+00	1.00e+00	#	31 V 5. Clear Selection	1	5.52e+06	1.00e+00	1.00e+00	Ξ.
Decimation	83	5.23e+06	1.00e+00	1.00e+00		30 ♥ 5.22873e+06		5.23e+06	1.00e+00	1.00e+00	
29 V 4.94744c+06	6	4.95e+06	1.00e+00	1.00e+00		29 📝 4.94744e+06	83	4.95e+06	1.00e+00	1.00e+00	
28 📝 4,67516e+06	13	4.68e+06	1.00e+00	1.00e+00		28 🛛 4.67516e+06	0	4.68e+06	1.00e+00	1.00e+00	
27 📝 4.40939e+06	2	4.41e+06	1.00e+00	1.00e+00		27 📝 4.40939e+06	8	4.41e+06	1.00e+00	1.00e+00	
26 📝 4.15256e+06	<b>m</b>	4.15e+06	1.00e+00	1.00e+00		26 📝 4.15256e+06	8	4.15e+06	1.00e+00	1.00e+00	
25 💟 3.9023e+06	0	3.90e+06	1.00e+00	1.00e+00		25 📝 3.9023e+06		3.90e+06	1.00e+00	1.00e+00	
24 🕅 3.66092e+06	2	3.66e+06	1.00e+	1.00e+		24 📝 3.66092e+06		3.66e+06	1.00e+	1.00e+	
23 📝 3.42618e+06	5	3.43e+06	1.00e+00	1.00e+00		23 📝 3.42618e+06	<u>111</u>	3.43e+06	1.00e+00	1.00e+00	
22 🛛 3.20025e+06	0	3.20e+06	1.00e+00	1.00e+00	- 1	22 👿 3.20025e+06	23	3.20e+06	1.00e+00	1.00e+00	

# How to scale the traces of the stacked spectra?


The user can also change the intensity of the traces from the Stacked items table; which can be

displayed by clicking on the applicable icon of the toolbar (or by following the menu 'Stack/Stacked items table'). Once there, just check the box of the trace that you want to modify and click on the 'Multiply' or Divide' buttons of the dialog box (as it is shown in the picture below).

Report Cop	The second s	Markert 🖉	Arrayed Data	× Multiply	÷ • Divide	Setup
1	Tit	le	*	T/G	Ratio	Norm. Factor
4 📝 1H en js1pm1	300Mgz 1211			0.00e+00	1.00e+00	2.00e+00
3 🔽 jspm10	jspm1052/1			1.00e+05	1.00e+00	2.00e+00
2 🔽 <sup>jsav3F</sup>	ftalcara			1.00e+00	1.00e+00	2.00e+00
1 V Quinin			E	1.00e+00	1.00e+00	2.00e+00

Clicking on the scroll down menu of the multiply or divide buttons will allow you to select the factor value .

Please bear in mind that you can also use the buttons of the Stacked NMR toolbar to multiply/divide the intensity of your traces (or follow the menu 'Stack/Scale Manually'):




You can also 'Auto Scale' the traces of your spectrum, just by clicking on this button et also 'Auto Scale'.

The user is also able to extract the 'Active Spectrum' or 'All Spectra' together by following the 'Stack menu':

	Stack Spectra
A.	Superimpose Spectra
	Extract Active Spectrum Extract All Spectra
Ň	Setup Stacked Spectra
	Show Arrayed Data Table


## **Decimation**

Worth mentioning is the 'Decimation' option:



This option is very useful when the number of stacked spectra is very large, slowing down the plotting and not showing relevant information

This shows the result of a R-M experiment consisting of 700 spectra. After selecting **the decimation option**, a new dialog shows up where you can select the first and last spectrum to be displayed and the step or decimation factor. In the picture below you can see how the dataset will look like after decimation:

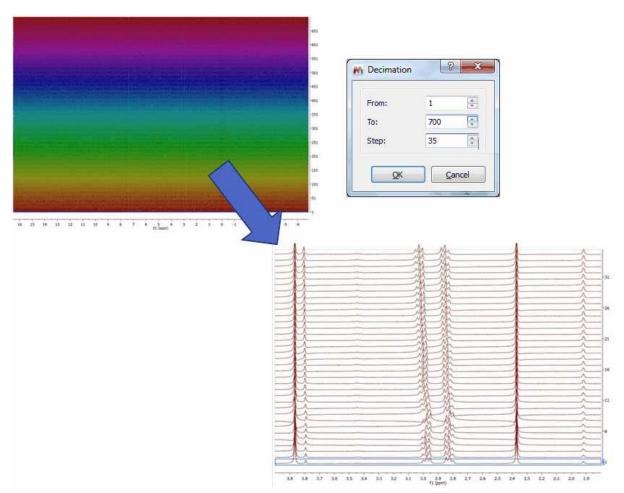

In the context of metabolomics, you would need to classify the stacked spectra by specifying a class.

To do that, you can add an editable column to the Stacked Items table in order to input there a short text. You can show the 'Class' parameter by clicking on the 'Setup' button of the Stacked Items table (or on the Customize button of the 'Parameters Table'):

	Title		T/G	Ratio	Norm. Factor	Class
/isible Name	Title		T/G	Ratio	Norm. Factor	Class
Visible					<b>V</b>	
Decimals	0	0	2	2	2	0
Horizontal Alignment	Left	Left	Left	Left	Left	Left
Font MS Shell	Dig 2					

This parameter will be editable just with one click (double-click is used to change the active spectrum):

1.80	port Copy Delete	🍫 inve	Setup				
Mu	iltiply Divide Shov	v <b>•</b>	💐 🚽				
	/ Title	*	T/G	Ratio	Norm. Factor	Class	1.5
14	Proton-T1/10 Ref. Sample, T1IR		1.00e+01	1.00e+00	1.00e+00	T2R	
13	Proton-T1/10 Ref. Sample, T1IR		<mark>5.00e+</mark>	1.00e+	1.00e+00	T2R4	
12	Proton-T1/10 Ref. Sample, T1IR		4.50e+00	1.00e+00	1.00e+00	T2RX	-
11	Proton-T1/10 Ref. Sample, T1IR		4.00e+00	1.00e+00	1.00e+00	T2RZ	
10	Proton-T1/10 Ref. Sample, T1IR		3.50e+00	1.00e+00	1.00e+00	T2R	
9	Proton-T1/10 Ref. Sample, T1IR		3.00e+00	1.00e+00	1.00e+00	T2R1	

## 8.3.4 Stacked Options and Properties

### Options

By default Mnova will delete the 1D spectra after having stacked them without autoscaling them. If you want to modify these defaults, you will need to follow the menu 'Stack/Stack Options' and uncheck the applicable box. From here, you will be able to change also the stacked angle and to select different palettes for your superimposed 2D experiments.

2	o scale the intensities w ked Angle:	0.00	
2D Pa			
	Experiment	Palette	
1 0	OSY	Red-Orange (Gradient)	
2 H	12BC	Green-Blue (Gradient)	
3 ⊦	ІМВС	Green-Blue (Gradient)	
4 +	łsąc	Red-Orange (Gradient)	
•	ш	ł	


## **Properties**

The user can change the Stacked Items properties by double clicking on the spectrum window; this will display the Properties dialog box, where the user can modify the Style (lines, crosses or circles), the Line Width, the Stacking Angle and the color of the current slice as well as that of the spectrum (single color, gradient or hue color). From here you can change the colour of the background or show the title of the spectrum and the title of each slide of the stacked plot, by checking the corresponding boxes:


·			
MMR Spectrum           Title         General           Grid         Grid	Stacked Stacked Angle:	0.00	A V
1D 1D	Top Margin:	5.00 %	*
Kacked	Bottom Margin:	5.00 %	
Scales Horizontal Stacked Peaks Integrals	<ul> <li>Clipped Vertically</li> <li>Current:</li> <li>All:</li> </ul>	Hue Color marcon	*
Multiplets	Superimposed Active Pen Width Factor:	2.00	×
Fitting	Secondary Transparency:	0.50	X A V

You can change the top and bottom margins of the stack plot, which is really useful in to avoid clipping a stacked plot at the spectrum border. With this property you will be able to adjust the distance between the top of the spectrum object and the baseline of the uppermost spectrum.


Here you can see an example with a top margin of 5%:

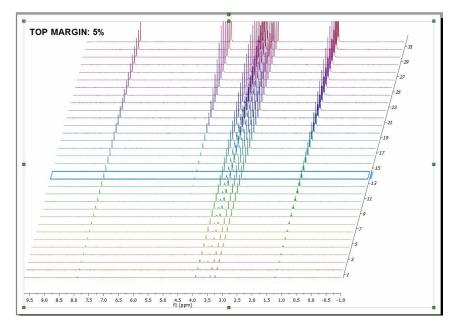


And the applicable result after having selected a top margin of 35%:

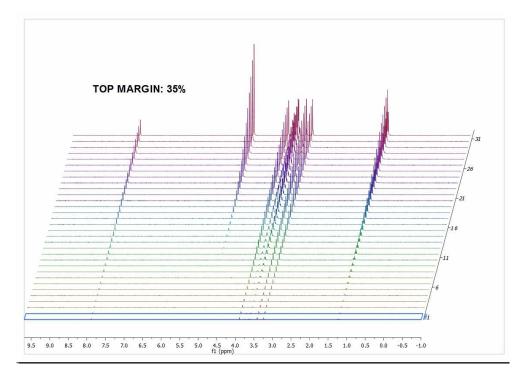

You can cut off the peaks to avoid overlapping just by checking the 'Clipped Vertically' option:

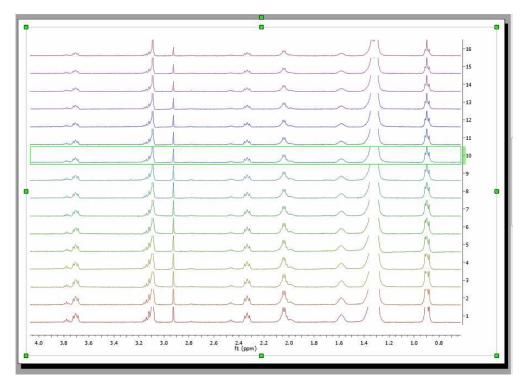

Here you can see an example of a stacked plot with the title of the different traces:

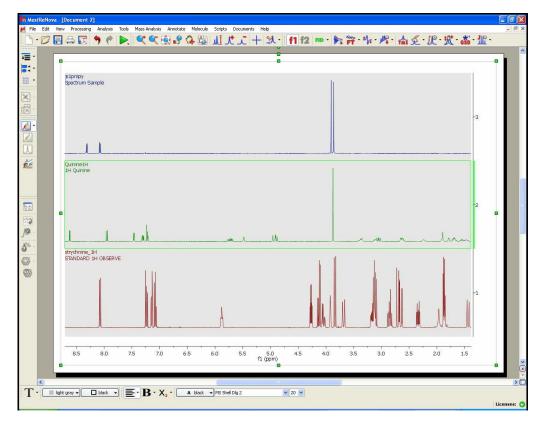

For metabolomics studies it is important to superimpose multiple spectra and compare their shape,

e.g. to identify which ones are outliers. In such a mode, when the user sets a spectrum as the Active spectrum, that spectral curve will be displayed with a thicker curve. Follow the 'Edit/Properties/Stack' menu to customize the 'Active pen width factor' (2.00 by default) and 'Secondary Transparency'.

Selecting 'Scales' in the left-vertical tabbed menu, will allow you to change the color of the scale, the font, add labels and also show/hide the horizontal and the stacked axes. From the Stacked menu, you can also change the label and the content (arrayed data or just numbers) of the stacked scale or the minimum width of the scale.


- 📑			
ometry NMR Spectrum			
General	Stacked		
Grid Grid	V Label:	.0.	
1D	Category names		
🔀 Stacked	Arrayed Data Value	25	
Scales	Numbering		
Horizontal	Minimum Width:	18.00 mm	×.
Stacked			

# 8.4 Fourier Transform

### **Basic concepts on FT**

Modern **NMR** involves pulse RF energy to excite all frequencies at once. Immediately after the pulse, the signal is detected as a time domain interferogram which contains the sum of all the damped-sinusoid signals emitted by the sample at the various nuclear resonance frequencies.

The signal will decay with time as various relaxation mechanisms either dephase the magnetization in the X-Y plane or return the magnetization to the Z axis. The resulting interferogram is called the *free induction decay* (FID, see figure below)

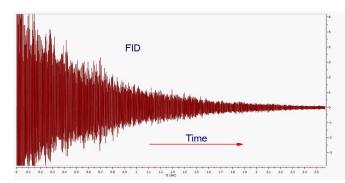


If you pay close attention to the FID shown in the figure above you can appreciate that it is composed of several frequencies. Moreover, if you were able to count the number of peaks and valleys in a given period of time (e.g. 1 second), you might be able to measure the periods and calculate the frequencies of some of the signals composing the FID.

In 'real' life, you don't need to do this conversion by hand. Fortunately, **Jean-Baptiste Joseph Fourier** suggested, while working a study of heat flow, that any function of a variable, can be represented by a

sum of multiples of sinusoidal harmonics of that variable. This work was later developed into the Fourier Series.

Fourier's proposals led, in part, to the development of a linear mapping operator which maps a given function to other functions and in our particular case, functions of time to functions of frequency. The operator was named the Fourier Transform in Fourier's honour. In short (math details are beyond the scope of these documents), the Fourier Transform or FT is the mathematical process that converts the time domain function (the **FID**) into a frequency domain function (the spectrum) as illustrated below:



Thus, FT is a mathematical procedure which generates the spectrum from the FID. It searches through the FID for frequency information and allows a plot of signal intensity versus frequency to be generated. When the frequency information is well defined, the peaks will be sharp, but if the information is not precise, the peaks will be broader.

The Continuous Fourier Transform nitty-gritty involves the equation:

$$A(w) = \int_{-\infty}^{+\infty} A(t) [\cos(wt) - i\sin(wt)] dt$$

where A(w) is the intensity of the signal as a function of frequency, A(t) is signal intensity of the FID as a function of time and *i* is (-1)<sup>1/2</sup>.

Separating the real from the imaginary part, we have:

$$A(w) = \int_{-\infty}^{+\infty} A(t) \cos(wt) dt - i \int_{-\infty}^{+\infty} A(t) \sin(wt) dt$$

The real part can be taken as the signal component which starts off in phase with the receiver reference oscillator, while the imaginary part is that which starts off 90 degrees out of phase with the receiver reference.

The original Fourier Transform is defined for functions of a continuous variable: To meet the needs of pulse NMR where the FID is sampled at short but discreet intervals, the so called **Discrete Fourier Transform** (**DFT**) is used. When the signal strength has been measured with discrete time-interval sampling, the Fourier integral is replaced by:

$$x(n) = \frac{1}{N} \sum_{n=0}^{N-1} \left[ A(n) \frac{\cos(2\pi kn)}{N} - iA(n) \frac{\sin(2\pi kn)}{N} \right]$$

where *N* is the number of samples, *n* is the *n*<sup>th</sup> sample and  $2\pi k$  is a multiplier which converts point *n*, into the value corresponding to *wt* (in rad/s). If we have a collection (named *A*) of *N* signal points as a function of time, the calculation of the applicable arrays of real and imaginary frequency points is quite straightforward and can be easily carried out with a computer.

The calculations with many points are obviously slow (though with current computers, they are extremely fast), but the more points, the smoother the plots will be. In order to reduce the computation time we can use the **Cooley-Tukey fast-Fourier algorithm** (**FFT**), reducing the number of calculations from  $N^*N$  for the **DFT** to  $Nlog_2N$  for the **FFT**. If N is 1024 samples the reduction is from 1048576 to 7098, a 93% time reduction. This algorithm has the special restriction that N must be a power of 2. (In cases where the number of points is not a power of 2, Mnova will extend the size of the FID by adding zeros to the next higher power of 2).

The Cooley-Tukey algorithm for the **FFT** achieves this stunning reduction in computation time in part by a process called "bit reversal" which avoids repetitions of internal vector component calculations. The algorithm also saves time by recognizing the orthogonality of certain calculations, allowing the one vector to be calculated from another just by changing an algebraic sign, or reversing sine and cosine terms. This process is an example of the general technique of *divide and conquer* algorithms apparent in many traditional implementations, in which the FT is divided in other more and more small FTs.

Although, as explained in the items dedicated to 1D and 2D NMR Processing, all processing parameters are applied by default by Mnova, prior to Fourier Transform and for Fourier Transform, the software also incorporates a significant number of algorithms which can be applied by the user to try to optimize the results obtained. Thus, on the scroll menu applicable to the '**FT'** icon the user can find the following options to apply:



The shortcut for the FT will be the 'Shift+F'.

### FT and Mnova

At first sight it might seem that a plain FFT would suffice to obtain the desired spectrum. However, this is not so in many cases. Although Mnova will adjust the number of samples by zero-filling to obtain a power of 2, the user may elect to increase the zero filling further to double the acquisition power of 2 value to obtain optimum 'frequency' resolution, or even further to improve the 'digital' resolution.

Other operations closely related to the FFT algorithm include:

- Quadrature Detection
- Drift Correction
- Digital Filtering
- Phase-sensitive Protocols


## 8.4.1 Group Delay

Most of NMR has finally gone totally digital and is now routinely resorting to high-frequency ADC sampling at rates of several tens of MHz, with a tendency to ever higher sampling frequencies. Such a drastic oversampling has clear advantages in simplifying the front-end electronics. It has also many


side benefits due to the fact that the subsequent down-conversion to low frequency range is done digitally and therefore theoretically artefact free. This includes perfect, calibration-free quadrature detection and drastic reduction of quantization noise. By the way, such techniques are routine in other areas of electronics (military, astronomy, audio, ...); NMR is just a latecomer to this world.

High-frequency (HF) oversampling, however, has also some problems of its own. The digital decimation from the HF range to the audio range and the contextual digital filtering (a combination of CIC and FIR filters) need to be properly implemented in the hardware in order to be completely transparent to the User.

However, in the case of Bruker and Jeol spectra a death time or group delay can be observed in the FID: it starts with very small values and then, after some points (usually between 60-80 points) the normal FID starts.

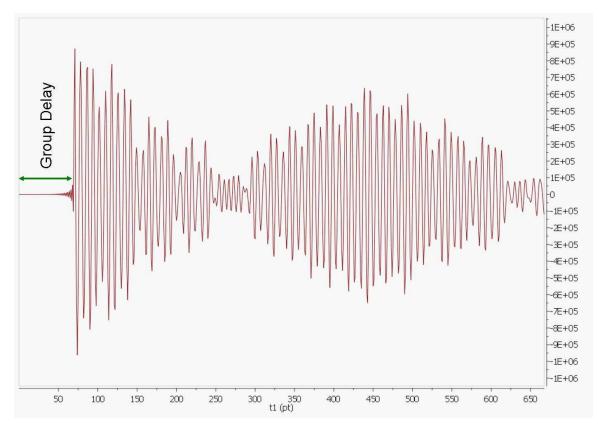


If a plain FT is applied to this FID, we will get a spectrum with a lot of wiggles in the baseline analogous to the convolution with a sinc function centred in the middle of the spectral window. This can be explained by recalling the time shift theorem of the Fourier Transform which says that if the time domain signal is shifted by n points, the frequency domain spectrum corresponds to the standard spectrum (when the FID has not been shifted) multiplied by  $\exp(-i2*pi*w*n)$ . In other words, we have introduced a very large first order phase correction in the spectrum. For example, if the FID is right shifted by 60 points (death time = 60 points), f-spectrum will exhibit a first order phase distortion of 60 \* 360 = 21600 degrees.

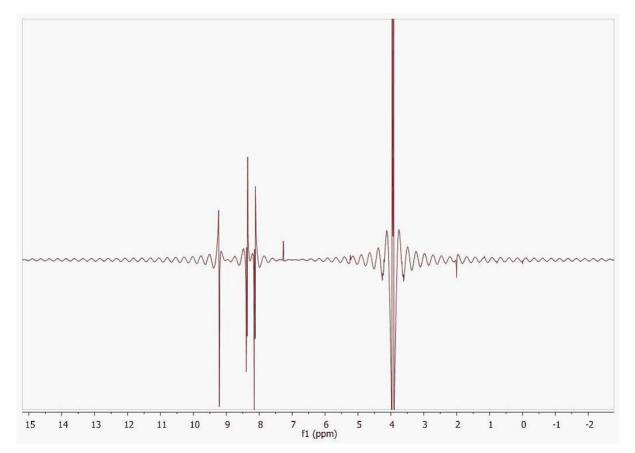


In order to work around this problem, Mnova reads the length of the group delay to be able to calculate the actual beginning of the FID to apply the required correction.

Former versions of Mnova applied a linear phase shift after FT calculated as the product of the group delay length by 360. The problem with this approach is that the resulting spectrum usually shows the so-called smiles at both edges of the spectral width (see figure below)

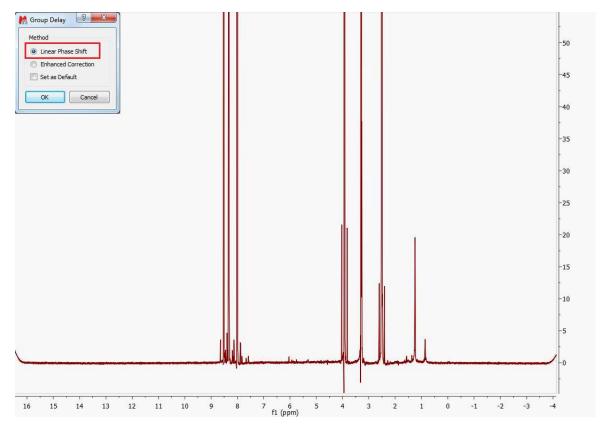

From version 6.1.0 onwards, Mnova includes a new correction algorithm (Enhanced Correction) which produces a normal and physically correct FID in such a way that the smiles/brownies will not be seen in the f-domain spectrum.

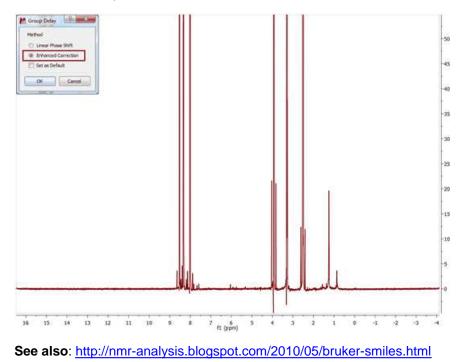

© 2017 MESTRELAB RESEARCH

## 8.4.2 FID Shift

Use this command located under the Processing menu of Mnova to right or left shift the FID.

Shifting the FID to the left or to the right is equivalent to shift the phase of the frequency domain spectrum by  $-wt_0$ .

From a practical point of view this means that if the FID is shifted by one point to the right, the resulting f-domain spectrum will have a linear phase correction of -360°. The same effect, but with the opposite sign occurs if the FID is shifted to the right.

This phenomenon is very easy to understand by considering the well-known property of the **Fourier Transform of a Time Shifted Signal which can be stated as**:

The Fourier transform of a signal which has a simple time shift is:

$$F\{x(t-t_0)\} = e^{-j\omega t_0}X(j\omega)$$


i.e. the original Fourier transform but shifted in phase by  $-wt_0$ 

For example: if you type -10 in the edit box, this will be equivalent to apply a linear phase correction of  $+10^{*}360^{\circ}$ .

👫 FID S	hift	? 🛛
Shift:	-10 pts 💲	Cyclic
	ок	Cancel

Basically, in this example, Mnova will not take into account the first 10 complex points of the original FID; shifting the origin of the new FID 10 points to the left and adding 10 zeroes to the end (i.e., left shift 10 points). Clicking on the Cyclic check box will add the original first points to the end of the FID (instead of zeroes).

Here you can see an example of a FID which needs to be shifted +11 points:

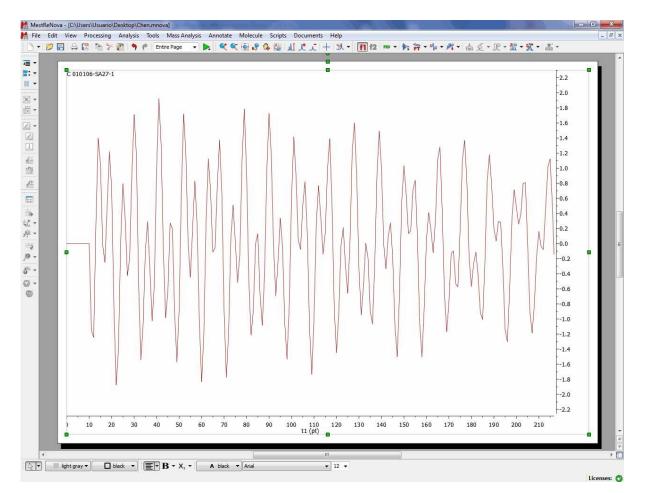


## 8.4.3 Diagonal Suppresion


**Diagonal Suppression** (Not available in Mnova Lite):

In the <u>1D NMR Processing</u> section, we described the real-time frequency domain processing concept. **Diagonal Suppression** of homonuclear 2D experiments represents another example of this concept. This technique is typically carried out in the mixed time-frequency domain (interferogram). However, this is something you do not need to know in Mnova. You can suppress the diagonal while the transformed spectrum is on the screen.

For example, the figure below shows a 2D magnitude spectrum:

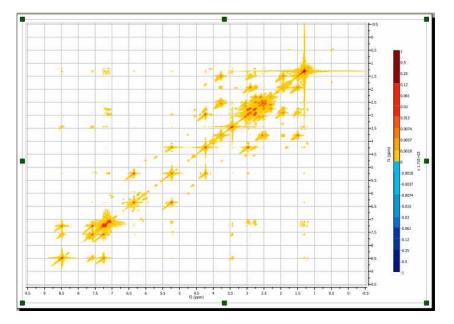

To suppress the diagonal, just click on the small arrow at the right-hand side of the FT toolbar button (see below) and select the **Diagonal Suppression** command:




This option offers a couple of well known traditional algorithms (Convolution and Shifted Convolution) as well as a new, in-house developed algorithm based on Wavelets to remove the diagonal from homonuclear spectra. Once you select the 'diagonal suppression' on the FT scroll menu, a dialog box like this will open:

Convolution Shifted Convolution
Wavelets
Selectivity (464): 24

As you can see, you can select the desired algorithm and also the selectivity of the diagonal supression. In the case where you choose the in-house algorithm based on Wavelets, you will be able to set the 'Dyadic Levels' and the 'Daubechies Coefficients'.

In this example we will select the Wavelet method; and this is the resulting diagonal-free spectrum.

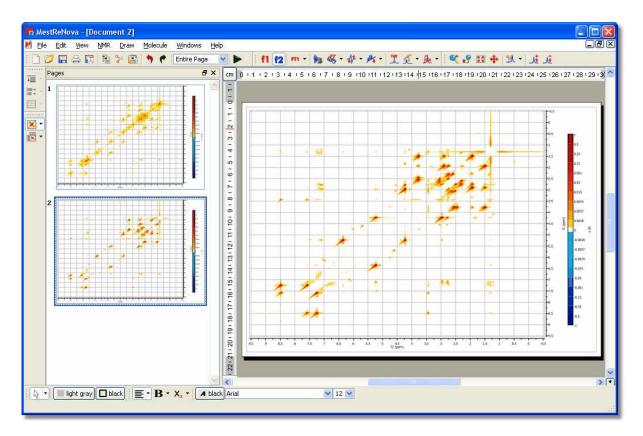


Note that in the figure above there are two pages, the first one containing the 2D spectrum with its original diagonal, and the second one after the diagonal has been removed.

## 8.4.4 Signal Suppresion


**Signal Suppression** (Not available in Mnova Lite): Strong solvent resonances with solutes of low concentration can result in a lot of problems relating to spectrum quality. One of the primary challenges in obtaining High resolution NMR spectra of biological samples is the suppression of the water resonance to prevent it from overwhelming the signals of interest.

This option is intended to suppress the solvent signal but can also be used to remove any other signal from the spectrum. To suppress the signal, you can select the method (algorithm) of the suppression and the selectivity (or width of the filter; a higher value of selectivity will suppress a narrower band). You can choose the signal, or signals, by double clicking on the applicable table titled 'Signals to Suppress'.

Method		Sign	als to Suppress	
Convolution	*		Position (ppm)	^
Convolution Shifted Convolution Wavelets		1	6.02	
Selectivity (464):	24 🧔	2		
		3		
		4		×




#### Here you can see an example:

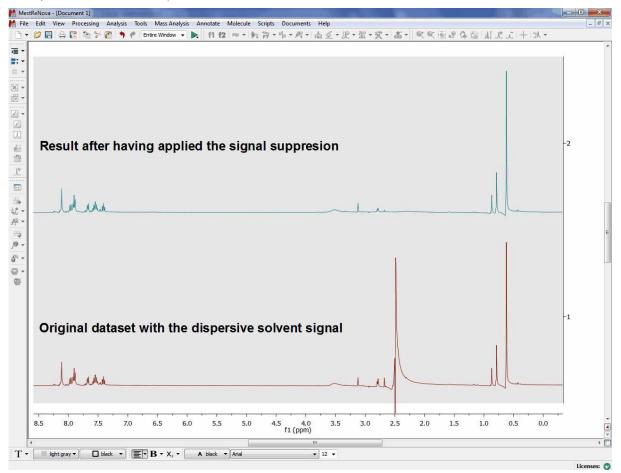

## 8.4.5 Apodization

**Apodization** (or Weighting or Windowing): literally, apodization means 'cutting off the feet' in the original Greek. In this case, the feet are the *leakage or wiggles* which appear when the signal decays rapidly to zero producing an abrupt truncation of the FID, as can happen for example when zero filling. Apodization is a very useful approach to enhance the S/N ratio (sensitivity) or the resolution, or even to remove truncation artefacts, after data has been collected.

The most commonly used apodization function is a decaying single-exponential curve. The magnitude of the decay constant determines how quickly the curve decays. In a regular FID, the resonances due to the sample are found in the earlier parts of the signal. When you multiply the FID by a decaying-exponential function, you favour the early parts of the time domain and attenuate the data at the end of the acquisition period, which is essentially all noise. A single exponential apodization function does not significantly affect the signal at short times, but it greatly reduces the noise at later times; at the expense of an increase in linewidth, that is to say, a decrease in the resolution. On the other hand, if you use an *increasing exponential curve* as apodization, you will obtain finer lines (increased resolution) but amplifying the noise (decreased sensitivity).

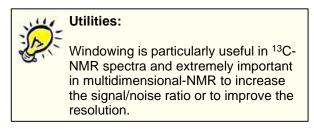


The Window function is applied by multiplying the data vector d, element by element, by a vector a. Thus element k of vector d is multiplied by element k of vector a to yield element k of vector d'.

$$d'_{\mathbf{k}} = a_{\mathbf{k}} d_{\mathbf{k}}$$

The challenge lies in finding a vector a, such that the noise in the tail of the FID is attenuated without excessive line broadening or, in the case of apodization, to smooth the truncated data exponentially towards zero, again without excessive line broadening. Theory shows that this is attained when the decay of vector a matches the decay of vector d; in this case we have what is known as a *matched filter*. Mnova makes this particularly easy by allowing the final spectrum to be observed while the decay parameter of the window function is adjusted.

Mnova incorporates many window functions (Exponential, Gaussian, Sine Bell, Sine Bell Square, TRAF, Trapezoidal, Parabolic, Hanning, Convolution Difference and Linear Ramp), which can be combined and can be used interactively (while viewing the FID as well as the resulting spectrum) to improve the sensitivity or the resolution. Unfortunately, it is very difficult to find a function which improves sensitivity and resolution simultaneously (an exception could be the Traficante function, as we will see later).

You can find this tool in the toolbar (see the button highlighted in red in the picture below), in the FT scroll menu on the toolbar or by following the menu 'Processing/Apodization' (shortcut: W):

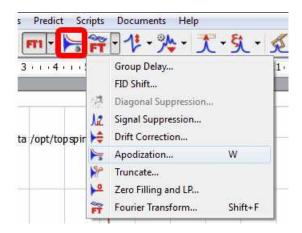

Once you have selected 'Apodization', a modeless dialog box will be displayed:

Average T2* = 0.247 Integral-to-noise effe			- 1.205	112			Reference
Functions							
Show advanced							
Z Exponential	0.00			(A) (V)	Hz		
Caussian	1.00			- A.   W	GB [Hz]	*	
🔲 Sine Bell	0.00	*	۰				
📃 Sine Square	90.00	(A) (F)	•				
📃 Sine Bell II	0.0	*	%		100.0	A. W	%
📄 Sine Square II	0.0	*	%		100.0	A. ¥	%
🔲 First Point	0.50			a T			

As it is a modeless dialog, you can change the intensity of the spectrum while the dialog is open. In 2D-NMR spectra, you will be allowed to switch from F1 to F2 to select the desired apodization function:


verage T2* = 0.056	ős, Line W	/idth :	= 5.7071	Hz			1	Referen
unctions								
Show advanced	-							
Exponential	1.00		4	≜ ¥ Hz				
💟 Gaussian	8.95		_	*	GB [Hz]	•		
📃 Sine Bell	0.00	A W	•					
📰 Sine Square	90.00	Å	•					
📃 Sine Bell II	0.0	A.	%		100.0	A. Y	%	
💟 Sine Square II	-66.4	A	%		167.1	*	%	
🔲 First Point	0.50			A. -9				

In this dialog box you will find the type of window function which Mnova has applied prior to FT, as well as other Standard Functions (Gaussian, Sine Bell, Sine Square and First Point). If you check the 'Show Advanced' box', you can set other apodization functions, as shown below:

Average T2* = 0.247 s Integral-to-noise effec		51120	Reference
Functions			
Show advanced			
	1.00	₩. Hz	-
📃 Trapezoidal	1.00	\$	
🕅 Parabolic	1.00	* %	
🛄 Hanning	0.50	(0,1]	E
🕅 Stanning	4.0	* •	
📃 Linear Ramp			
📃 Sinc	1.900		-

In order to assist in the process of finding the most suitable window function and its parameters, Mnova allows the user to interactively adjust the parameters of window functions, and to view the effect directly on the frequency spectrum. For this purpose, make sure the 'Interactive' box is ticked (highlighted in red in the figure), you can then follow the exact effect of the function you are applying on

the frequency domain spectrum (or on the FID, if you are on the FID' view) by using the buttons to change the desired parameter. If you have activated the 'Full View' window you will be able to see the window function displayed along with the FID.

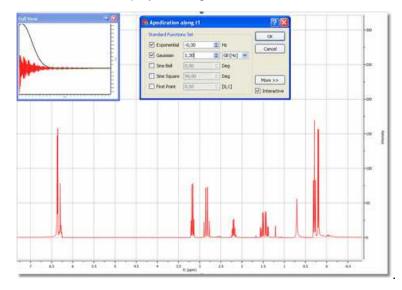


We will try to explain in a brief and easy way the applications and the effects of these functions:

Exponential: A exponential apodization function is defined as:

$$a_k = e^{-\pi W k \Delta t}$$

where W (the parameter to adjust) represents the the line broadening factor expressed in Hz. So, if the original width of the signal is 'L', the final width of the signal after applying this window function would be 'L+W'. If W is positive we will have a *decaying exponential curve* (and we are giving more weight to the points at the beginning of the FID and suppressing the data at the end of the time series, which is essentially all noise). As we explained previously, this will increase the **'sensitivity'** (Signal to Noise Ratio) of the spectrum at the expense of an increase in linewidth (decreased resolution).

The figure below shows the effect of *W* on the linewidth. The black trace has no window function applied. The red trace shows a taller signal due to application of an **Exponential Function** and also an increase of the Signal to Noise Ratio (matched filter), while the blue trace shows that if the **Exponential Function** is too severe the broadening of the lines reduces the signal size again.

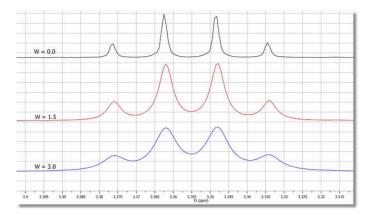

If *W* is negative, we will have an *increasing exponential curve*, thus obtaining the opposite effect (increased **resolution**, with finer lines, and a decrease in sensitivity, i.e., a lower S/N ratio). You can see below the graphical difference between an *increasing and a decaying exponential curve* over the FID (shown in the 'Full View' window). Note that in this case an *increasing exponential curve* will not be a good choice (it is normally used in combination with other functions, such as Gaussian).

all View 🗈 🚨
Increasing Exponential Curve

In most of the literature this parameter is symbolized by LB (Line Broadening).


**Gaussian:** In Gaussian window function resembles the Gaussian Probability Distribution function used in statistical analysis. The gaussian function rises quasi exponentially to its single maximum and then falls back to zero in the same manner and so may be regarded as almost two back-to-back exponentials.

In Gaussian apodization, each data point of the FID is multiplied by the vector:


$$a_k = e^{-W(k\Delta t)^2}$$

where W is the same widening factor used in exponential apodization. This function is similar to the

exponential but decays comparatively slowly at the beginning of the FID and then quite rapidly at the end. For this reason, it causes less line broadening than the exponential multiplication.



In the next picture, you can see the influence of *W* over the linewidth:

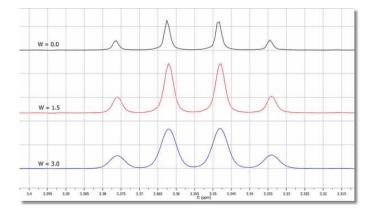

**Gaussian plus Exponential:** This function is also known as Lorentz-to-Gauss Transformation and is not directly implemented in Mnova, but you can apply it by ticking both exponential and Gaussian multiplication functions and introducing a negative value for the exponential line broadening (W) and a positive value for the Gaussian parameter (GB). The spectrum can be optimized for resolution by suitably adjusting these parameters.

Thus, this weighting function combines a rising exponential function with a decreasing Gaussian function; then, the resulting vector will be:

 $a_k = e^{\pi W k \Delta t} e^{W(k \Delta t)}$ 

To perform Exponential/Gaussian apodization with Mnova, select the Apodization option in the FT scroll menu on the toolbar, then click on the Exponential as well as on the Gaussian resolution enhancement option and finally enter the appropriate values of W (or LB) and GB and click OK.

Usually, a process of trial and error is adopted with the parameters being adjusted until the best result is obtained. You can follow (by ticking on the 'Interactive' box) the exact effect of the function you are applying on the frequency domain spectrum or on the FID window (shown graphically in the 'Full View' window), as you can see in the screenshot below.

off View	0 2	Apodization a	along t1			20
1	E	Standard Functio	ns Set			ОК
1	E	Exponential	-0,80	\$	Hz	Cancel
	H.	Gaussian	2,10	\$	GB [Hz] 💌	Contor
1 Allan	-	🔲 Sine Bell	0,00		Deg	
	E	Sine Square	90,00	13	Deg	More >>
	-	First Point	0,50	9	[0,1]	Interactive

GF (Gaussian Factor) is a number between 0 and 1 and defines where the maximum of the function will be, as a fraction of the acquisition time.

**Sine Bell** (Not available in Mnova Lite): This function is very useful in those NMR experiments where the signals of interest are not maximal at the beginning of the FID and very convenient for magnitude spectra because it reduces the dispersive part of the line shape.

In COSY experiments the cross peaks are sine modulated while the diagonal peaks are cosine modulated. Sine bell windowing thus emphasizes the cross peaks and attenuates the diagonal signals. Unfortunately due to differing relaxation times for some signals possibly not all cross-peaks will be maximal at the same time; in this case the sine-bell may be shifted to yield the best compromise spectrum. The unshifted sine-bell also removes dispersive signals from the absolute value COSY, providing the sought for absorption line shape.

# Utilities:


The **Sine Bell** window function is very useful for **COSY** experiments because it emphasizes the sine-modulated cross peaks compared with cosine-modulated diagonal peaks.

Avoid using this function with 1D spectra since it decrease the spectral intensity. If used with phase sensitive experiments the sine bell can result in signals with negative side lobes and near zero integrals.


This function consists in the multiplication of each data point of the FID by the next vector:

$$d_k = \sin \left(\beta + \frac{(\pi - \beta)t}{t_{sq}}\right)$$

Mnova requires you to enter the  $\beta$  parameter, whose input is expressed in degrees. When  $\beta = 0$ ; the equivalent function is a sine-bell, while when  $\beta = 90$  the equivalent function is a cosine-bell. In the pictures below you can see the representations of the sine bell functions resulting from different values for  $\beta$ :

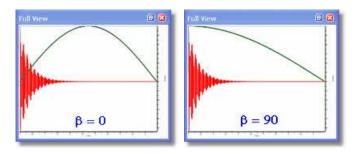

The cosine-bell apodization ( $\beta$  = 90) is very convenient in 2D-HSQC experiments:



You can use the "VNMR-like version of sinebell apodization" which uses % of acquisition time (instead of seconds) in order to make the parameters applicable to other spectra with the saved processing template.

The full formula for the shifted Sine II is sin(((t - sbs)\*pi)/(2\*sb)).


Where sbs = sbs Mnova /100\*T AQ; sb = sb Mnova/100\*T AQ

For function values less than zero, the function is truncated (i.e., only the first set of positive values are used).

As you can see you can also adjust the time-period of the SineBell (like the "sb" parameter in VNMR)

Average T2* = 0.6 Integral-to-noise e	10	0.463 Hz <u>Reference</u>	<u>Q</u> K Cancel
Standard Functions	Set		Gauce
Exponential	1.42	Hz	
Caussian	0.10	GB [Hz] 🐨	
📃 Sine Bell	0.00	•	
Sine Square	90,00	•	
🔽 Sine Bell II	0.0 🗘 %	100.0 🔹 %	
Sine Square II	-7.0 💠 %	17.7 🔷 %	More >>

**Sine Square** (Not available in Mnova Lite): The shape of the Sine Bell weighting function is altered by squaring it, resulting on the **Sine Bell Squared** function, which is more concentrated over the maximum. It is very useful to use a 90° shifted sine-bell squared to apodize 2D phase-sensitive experiments.



**First Point Correction:** There is an important difference between the *discreet* FT and the *continuous* FT. The *discreet* FT generates a constant vertical displacement of the baseline, which can be due to a

distortion of the first point of the FID. It treats the FID as a function which is repeated periodically, thus the ordinate at t=0 would represent the algebraic average of the first and the last point. In most FIDs, the value of the last point is very close to zero, and thus the first real point would have to be divided by two, before introducing it in the FT algorithm. It is often necessary to multiply the first point of the FID by 0.5 before FT in order to ensure that the value of the integral over the spectrum is equal to the value of the first point of the FID.

You can alter this multiplication parameter by entering the desired value (it should be 0.5 by default, as you can see in the FT dialog box below).

Apodization	along t1			2
Standard Functio	ns Set			OK.
Exponential	1,00	2	Hz	Cancel
🛄 Gaussian	1,00	14	GB [Hz] 💉	<u>C</u>
Sine Bell	0,00	9	Deg	
Sine Square	90,00		Deg	More >>
First Point	0,50		[0,1]	Interaction

The functions which follow are accessed via the [More >>] button in the Apodization dialog box.

**Traficante** (Not available in Mnova Lite): The Exponential Multiplication Gaussian and the combination of both can improve spectral resolution at the expense of some loss in SNR. The Traficante window function endeavours to improve resolution without noticeable loss in SNR. Traficante enhances the middle part of the FID and then uses a matched filter to attenuate noise in the latter part of the time-series. The process involves the division of the FID by the sum of the squares of the FID and its reverse. If there are N data points, the k<sup>th</sup> point in the original FID is point k while the applicable point in the reversed FID is point (N-k). As the resulting FID is symmetrical (with respect to the midpoint), we can multiply it by a function to obtain a new desired FID which does not decrease.

So, if we named the original FID *E*, and the reversed FID  $\varepsilon$ , we would get:

$$E \cdot g(t) + \varepsilon \cdot h(t) = 1$$

And Traficante apodization will consist of the multiplication of the FID by the following vector:

$$a_k = \frac{e^{-\pi W k \Delta t}}{\left(e^{-\pi W k \Delta t}\right)^2 + \left(e^{-\pi W (N-k)\Delta t}\right)^2}$$

In the picture below, we can see a Traficante function represented (with W = 2) applied to the FID

full View	0 8	Advanced Functions S	et		
٨	1	TRAF	2,00	0	Hz
. 1		Trapezoidal	1,00	1	%
1		Parabolic	1,00	- 2	%
		Hanning	0,50	0	[0,1]
the second se			1,00		Hz
1.0.0		Convolution Diff.	1,00		C Hz
			0,00		[-10,10]
A CONTRACTOR AND	J	🔲 Linear Ramp			



**IMPORTANT: Traficante apodization** will be only useful if the FID decays exponentially and, moreover, the value of W must be chosen with care.

**Trapezoidal** (Not available in Mnova Lite): This function multiplies the FID by a trapezoidal shaped function;

 $f(t) = 1 \cdots when t \le k$ 

$$f(t) = 1 - \frac{t-k}{T-k} \cdots \text{when } t > k$$

where T is the acquisition time and k is the percentage of the total length of data

This option is useful to avoid the "sinc" artifacts resulting from truncation of the FID. You can select the percentage of the total length of data between 0% and 100% (k), in the advanced functions of the FT menu:


TRAF	1,00	Hz
Trapezoidal	12,00	
Parabolic	1,00	: %
Hanning	0,50	0,1]
	1,00	÷ Hz
Convolution Diff.	1,00	C HE
	0,00	0 [-10,10]

**Parabolic** (Not available in Mnova Lite): This function multiplies the FID by a parabola shaped function, where

$$f(t) = 1 \cdots when t < b$$

$$f(t) = 1 - \frac{t - b}{\left[t(\max) - b\right]^2} \dots \text{ when } t > b$$


You can also set the length of the parabola by selecting (on the FT scroll menu) Apodization, click "More", select parabolic and then choose the desired value for the parameter (*b*, expressed as the total length of data). Again, you can see the exact effect of the function you are applying on the frequency domain spectrum or the effect on the the FID by (pre-)selecting the Full View" window:



Hanning (Not available in Mnova Lite): Mnova adopts the following generalized equation:

$$f(t) = p + (1 - p)\cos\left(\frac{\pi t}{2T}\right)$$

where *T* is the acquisition time, and P can be a value from 0 to 1. You can set this parameter on the advanced Functions set of the FT dialog box. If P = 0.5 we will have a Hanning function and if P = 0.54 we will apply a Hanning function, producing 10 and 20% line broadening respectively. The Hanning window, more correctly called the Hann window and the Hamming window are part of a family of functions known as "Raised Cosines" and also includes the Gaussian Window. These functions, like a cosine bell, have a maximum value; Mnova generally implements these functions with their maxima at zero time. The Hanning Function is sometimes used to reduce aliasing. Aliasing arises when signals are insufficiently sampled (violating the Nyquist Criterion), resulting in spectral folding. It results in peaks appearing at incorrect positions and generally not phasing along with the authentic signals. This arises due to incorrect experimental set up (signals beyond the high frequency end of the spectral width), and the ability to correct for it after acquisition is useful indeed.



Convolution Difference (Not available in Mnova Lite): This weighting function multiplies the FID by :

$$W(t) = 1 - e^{\left(-0.5t\pi \frac{LB}{SW}\right)}$$

where *LB* is the line broadening and *SW* is the spectral width in Hz. You can also access this function from the scroll menu of the FT icon where you will be able to set the value of LB.

**Linear Ramp** (Not available in Mnova Lite): This command is used to multiply the data points of the FID by an increasing linear ramp, resulting in the first derivative of the Fourier transformed spectrum { d(intensity)/d(frequency) }. This emphasizes the faster rising parts of the spectrum at the expense of SNR. If the initial spectrum had an excellent SNR this function can dramatically improve resolution. Mnova will soon offer derivative performed using wavelet processing which produces even better spectra.

This weighting function gives *more weight* to the end of the FID, amplifying the noise (decreasing the sensitivity), and for that reason we recommend its use only in combination with another function which gives more weight to the beginning of the FID (increasing sensitivity). In practical terms, add the ramp function to a spectrum that has already been windowed by, for example the EM function for 1D or the sine-bell function for a 2D in order to improve the selectivity.


### 8.4.6 Truncation

**Truncation:** This technique causes part of the time series, from a given time onward to be set to zero. For convenience Mnova truncates the time series after a given number of acquired points. The user may access this function either via the menu Processing/Apodization etc or via the FT icon scroll menu in the same manner.

cquired Number of Poini	ts: 16384	
uncabe FID After:	8192 pt	13

This technique may be used to shorten the acquisition data time series. If the FID, for example, decays to zero in 0.5 seconds and the acquisition time was 2 seconds, the FID consists of 25% signal and 75% noise. Since both 0 and a 90 degrees phase shifted spectra are collected a time series data length of twice the FID time is required for maximum information content. Truncating the FID at about 1.0 second will reduce the amount of storage required with no data loss. At a later time Zero Filling may be used to cosmetically adjust the spectrum's appearance.

This tool is used when the acquisition time has been set much longer than the FID, resulting in the acquisition of a long period of signal-free noise. Truncation sets the signal free latter region of the time-series to zero. This does NOT amount to zero-filling, and the appending of zero-s to twice the original number of acquisition points will still reveal the intrinsic resolution.

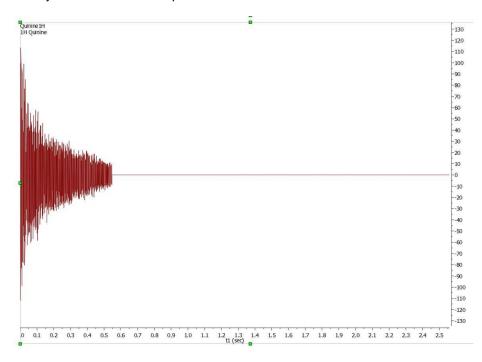

Here you can see an example of truncated FID:

# 8.4.7 Frequency Shift

Follow the menu ""Processing/Frequency Shift" to shift the frequency in f1 and f2.

Along f2:	100.000 Hz	×
Along f1:	100.000 Hz	

When applying for example 100 Hz in f2 or f1, a shift is applied in f2 or f1 dimension, respectively.

### 8.4.8 Zero Filling and Linear Prediction

**Zero Filling:** This option can be used to set the size of the Fourier Transform. It can be used either to increase the digital resolution or to truncate the FID. When the time-domain signal is subject to a FT, the resulting spectrum is represented by a set of data points (by joining the points to plot the spectrum as a smooth line). As a Fourier transformation preserves the number of data points, if we take the original FID and add an equal number of zeroes to the end of it, the applicable spectrum will have double the number of points, increasing therefore the 'apparent' digital resolution of the spectrum. The zero filling process is equivalent to a frequency-domain interpolation. This command is available in the **'FT'** icon scroll down menu, as shown below.



Just select the required number of points (only powers of 2 are allowed) and click 'OK':

From FID Size	To Spectr	um Size	
	65536 (6	i4K)	•
Original: 8959	LP Fill	ling	
inear Prediction			
Backward		Forward	
Erom: 0		From:	8959 🚔
<u>T</u> o: 0	*	To:	65536 🌘
Method: Toe	plitz 🔹	Method:	Zhu-Bax 🔹
Options		Options	
Basis Points: 89	934 🌻	Basis Point	s: 8943 🜲
Coefficients: 24	ŧ	Coefficient	s: 15 🌲

Mnova will be able to import the Zero Filling and Linear Prediction from the spectrometer by following the menu 'Edit/<u>Preferences</u>/NMR/Import' and checking the applicable box.

In some cases, the FID does not fulfil the requirement of the number of data points corresponding to an entire power of 2. In these cases, Zero Filling must be applied to the immediately higher entire power of 2 for FT to be possible. Mnova will automatically carry out this Zero Filling when the number of data points is not an entire power of 2. By default, Mnova proposes a duplication of the original number of FID data points. For example, if the FID has 16384 data points (or a number of data points between 16385 and 32768), the Zero Filling open dialog would show us the value of 32768 (32K) data points, which indicates that Mnova will add up to 16384 data points at the end of the FID.

**Linear Prediction** (Not available in Mnova Lite): Linear prediction is a mathematical procedure where a missing part of a FID can be constructed in order to increase the digital resolution of the spectrum; it is a tool which examines the free induction decay, extracts a set of coefficients, and extrapolates, either forward or backward, to predict what the data would have been had it been collected. This is a potentially valuable technique for extraction of useful information from marginal data.

Linear prediction is based in this fundamental principle: each value in the time series can be represented as a linear combination of the immediately preceding values. Mathematically, the basic LP equation postulates:

$$d_m = \sum_{p=1}^{p} a_p d_{m-p}, m = p, \dots, N-1$$

where  $a_p$  are the LP Coefficients and the number 'p' corresponds to the order of the prediction. Thus, you can extrapolate the series beyond the point *N*. This equation is known as *Forward Linear Prediction* (extrapolates forward, predicting the new values from the older ones).

Backward Linear Prediction will be represented in the following equation:

$$dm = \sum_{p=1}^{P} b_p d_{m+p}, m = 0, \dots, N - P - 1$$

This command is available in the same menu as zero filling. If you need to repair the baseline distortions (due generally to the first points of the FID) you have to tick Backward LP and select the limits; this will predict the first points of the FID.

Forward Linear Prediction is a better alternative to correct the last part of the FID than *zero filling;* this will extrapolate the FID in the direction of the advance, predicting the new data points from the older. If you select 'Linear Filling', a Forward LP from the end of the original FID up to the number of points defined in the 'Spectrum size' combo box, will be executed. You can also set the number of Basis Points and Coefficients of the algorithm that you want to use for Linear Prediction.

From FID Size Original: 895	To Spectru 65536 (64 LP Filli	4K)	•
near Prediction		Forward	
Erom:	0	From:	8959
<u>⊺</u> o:	0	To:	65536 🔶
Method:	Toeplitz 🔹	Method:	Zhu-Bax 🔹
Options		Options	Toeplitz Zhu-Bax
Basis Points:		Basis Points	Burg MIST
Coefficients:	24 🚔	Coefficients:	15 🌲

**Method:** Linear Prediction is extremely useful in 2D NMR as a way of reducing the acquisition time or increasing the quality of already existing data sets. Also, in 1D NMR it is useful when the FID has not decayed to zero before experiment completion. This often happens when working with slowly relaxing nuclei (such as quaternary carbons, in <sup>13</sup>C-NMR) and in experiments with a wide ppm area (spectral width).

One of the most common causes of the corruption of the first data points of the FID is the security time or *pre-scan delay* (time which exists between the pulse and the beginning of the acquisition) which in many cases may not be enough to allow the detector to recover fully from the effect of the pulse.

Our LP implementation is based in a very fast orthogonalization of Toeplitz matrices which is one of the fastest implementation of LP algorithms used in NMR. It gives very good results with phase sensitive data, in particular with HSQC and related spectra. However, it does not work very well with spectra in magnitude (or non phase sensitive) mode. In fact, Toeplitz method does not make it possible to reflect the roots of the LP coefficients within the unit circle because the resulting new LP coefficients get worse.

With such problems in mind, we decided to try the well known Zhu-Bax approach. In short, the algorithm calculates the forward and backward LP because in theory they should be identical. However, in presence of noise they are different. Zhu and Bax proposed to reduce the contribution of the random errors induced by noise by simply averaging the two sets of coefficients (fwd & bwd). Finally new roots are computed based on the average coefficients.

**Zhu-Bax** LP algorithm has been speeded up and it will be the default algorithm for forward LP as it is numerically much more stable and produces more artifacts-free spectra.

The Burg method is probably the first implementation of Linear Prediction developed by John Burg many years ago and it was extensively used in geophysics, but in general, should not be used with NMR data.

**Coefficients:** number of theoretical sinusoids. The number of the coefficients should be equal to the number of points in the FID in an ideal case. By default Mnova sets the number of coefficients according to:

#### Number Of Coefficients = points in the spectrum/16

**Basis Points:** they are the number of 'good' experimental points to be entered in the calculations. The number of basis points should be at least twice or three times greater than the number of coefficients.

**MIST:** This option is aimed at extending the FID using a modified Iterative Thresholding algorithm. Its performance has not been studied thoroughly so its application must be used with caution.

If some LP parameters don't match the sizes of the FID and spectrum then instead of auto-fitting them, a message box with the suggested corrections will be appear:

61	MestReNova	×
<u> </u>	The following corrections of the parameters will be made in order to of the FID and spectrum: Forward 'To': 65536 → 32769	fit the sizes
	ОК	Cancel

### 8.4.9 Drift Correction

**Drift Correction:** The DC (Drift Current) component is the zero frequency ( $F_0$ ) of the spectrum, which is proportional to the sum of all data points in the FID; if  $F_0$  is different to zero; a glitch signal (spurious peak) will appear in the centre of the spectral window. Both real and imaginary parts of the FID should decay to zero at the end of acquisition, but sometimes this "zero" is different and the offset may not be the same for both channels. Mnova corrects this spurious peak by default prior to Fourier Transform, although you can find and customize this tool (by selecting the number of tail points of the FID to determine the mean DC level) in the open dialog of 'Fourier Transform'; as you can see below:



You can also find this option by following the menu item 'Processing/Drift Correction':



You can automatically apply a drift correction when loading your NMR datasets by following the menu 'Edit/Preferences/NMR/Import' and checking the applicable box.

### 8.4.10 The FT Command

**Fourier Transform:** The FT command transforms the acquired data of the current data set, which may already have been processed using a filter function. Depending on the way a spectrum was recorded (e.g. simultaneous vs sequential sampling, quadrature settings, etc) the FT can be real or complex and some additional pre-processing may be required. All these options can be set in the

Fourier Transform dialog box, which will appear by clicking on the '**Fourier Transform'** icon <sup>4</sup> or by following the main menu item 'Processing/Fourier Transform'.

If you click on the F1 icon 1 (to select the indirect dimension) and then on the FT icon 4, you will obtain the following dialog box:

Fourier T	ransform along t	1 ? 🛛
Protocol:	Phasesensitive	~
Swap Ha	lves (Quadrature) 🛛 💽	Mirror Image (Invert)
		OK Cancel

**Protocol:** This option corresponds to the data shuffling algorithm required to process phase sensitive 2D spectra

**None:** If your spectrum is not phase sensitive, then the correct choice is: **none** protocol. (i.e. when only the

magnitude or power spectrum is to be obtained). It corresponds to the simpler 2D experiment in which a scan is collected with a 0° pulse of the mixing pulse, and then another is collected with a phase of 90° and finally combined before to storage in memory.

Bruker: QF mode Varian: p-type: f1coef='1 0 0 -1 ' n-type: f1coef='1 0 0 1 '

**Phase sensitive:** this kind of experiments are used to get higher resolution and more information out of a 2D dataset. You can obtain better resolution and better S/N ratio by generating quadrature phase detection in the second dimension, but at the expense of longer acquisition times and larger datasets.

Echo-antiecho: You should select this option for phase modulated experiments with

gradient pulses (used for coherence pathway selection), where pairs of slices are added and subtracted to generate complex "fids" in the indirect dimension. Each slice contains both sine and cosine terms in  $t_1$ . This means that the data must be handled differently from hypercomplex data, in which odd numbered slices contain only cosine  $t_1$  terms, and even numbered slices contain only sin  $t_1$  terms.

Bruker: ECHO-ANTIECHO Varian: f1coef='1 0 -1 0 0 1 0 1' f1coef='1 0 -1 0 0 -1 0 -1'

**Swap Halves (Quadrature):** the negative frequencies are distinguished from the positive ones by the detection and summation of the in-phase and 90° out-of-phase magnetizations (two-channel mode).

**Mirror Image (Invert):** this command performs a complex-conjugate of the data before the protocol and FT is aplied. It is used to generate a mirror image of both the real and the imaginary parts of the spectrum, with respect to a vertical line positioned in the middle of the spectrum; i.e., the spectrum is reversed.

You will need to check/uncheck this option when you get the mirror image of your expected spectrum along any dimension.


Most Varian spectra will require this option to be checked whilst most Bruker spectra will not except those experiments acquired using the TPPI scheme.

**Real FT:** it allows to execute a real Fourier Transform as opposed to the conventional Discreet Fourier Transform (normally, this is only necessary for Bruker spectra acquired by sequential mode). Modern spectrometers acquire spectra in a way which avoids the use of this option.

Typically, quadrature detection involves the use of two digitizers (ADCs) to sample at the same time the real and imaginary components of the signal. However, quadrature detection can also be done with a single digitizer using the Redfield trick in which the real and imaginary parts are sampled sequentially in time but doubling the sampling rate in order to get the same spectral with. In this case, a Real Fourier Transform is needed. This option is typically used in 1D Bruker spectra acquired in sequential mode (QSEQ) and also it is also necessary along f1 for 2D spectra acquired in TPPI mode.

### 8.4.11 NUS Processing

Mnova is able to process 2D data that has been acquired using Non Uniform Sampling (NUS). Under the Processing menu, you will be allowed to select the settings (Max iterations and Threshold level) for the MIST algorithm (Modified Iterative Soft Thresholding):

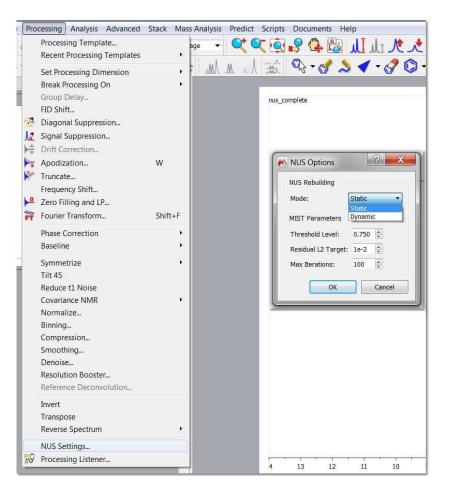

Generally speaking, NUS processing is fully automatic and there is no need to touch any parameter. The most critical one is the processing mode, Static vs dynamic. The static mode is the one that should always be used for performance considerations, otherwise everytime any processing in Mnova is issued, it will try to reconstruct the missing data points. The other parameters are related to the way in which IST works.

For further information about NUS and IST, please visit this link, this paper and also this post.

# 8.5 Phase Correction with Mnova

NMR spectra are usually represented in absorption mode, which offers a greater resolution and proportionality between the integral of peaks and the number of nuclei which cause the signal, in comparison with other representations such as dispersion mode, magnitude or power of the spectrum. Nevertheless, the absorption and dispersion curves are often mixed, giving rise to curves which lose the original symmetry. This problem, combined with other deficiencies, such as delays between the initial pulse and the beginning of data acquisition, cause a phase shift which varies linearly with frequency. This phase errors can be easily rectified in software by applying a lineal combination of the real and imaginary components of the spectrum in order to obtain pure phase lineshapes.

This correction is composed by a *frequency independent* parameter, or zero phase correction ( $\alpha$ ) and a first order phase correction ( $\beta$ ) or *linear dependent* on the frequency parameter:

$$\operatorname{Re'}_{k} = \operatorname{Re}_{k} \cos(\alpha + \frac{k}{N}\beta) - \operatorname{Im}_{k} \sin(\alpha + \frac{k}{N}\beta)$$

$$\operatorname{Im'}_{k} = \operatorname{Re}_{k} \sin(\alpha + \frac{k}{N}\beta) + \operatorname{Im}_{k} \cos(\alpha + \frac{k}{N}\beta)$$

where k = 0,...,N-1; Re<sub>k</sub> and Im<sub>k</sub> are the real and imaginary components of the data points (*k*), Re'<sub>k</sub> and Im'<sub>k</sub> are the new components after correction and *N* is the total number of points.

Mnova implements both manual and automatic Phase Correction algorithms.

The Phase Correction scroll menu is located on the arrow immediately to the right of the **'Phase Correction'** icon.



The software implements three algorithms for automatic phase correction, which can be applied both to 1D or to 2D data sets, and a manual algorithm, which allows for very easy, eye driven, real time zero order and first order phase correction. Once the user selects a Phase Correction method, Mnova will store it for future uses, highlighted with a black square.

#### **Automatic Phase Correction**

Mnova gives the user the choice between four auto-phasing algorithms for higher flexibility. Indeed you can select more than one algorithm at the same time and the algorithms will be applied consecutively:


Algorithms		
🔽 Global	Min. Entropy	
Selective	🔲 Baseline Optim	ization
Vetabonomics	Regions Analys	sis
Whitening		
Initial Phase:	Imported	2
Use only ranges highlig	ited for analysis, if any present.	

The user will be able to select the initial phase correction to run the Automatic Phase Correction algorithm (Zero,Imported, Current). By default is the imported phase from the spectrometer (you can change the default Phase Correction from the 'Edit/Preferences/NMR/Import' menu):

	🛷 💩 🕖 🚜
General Plug-ins Database NMR	Mass Molecule Scripting Drawing Tools
Drawing Import Save DataProc	
Parameters	
Apodization	
😨 Zero Filling	
Linear Prediction	
Apply	
	Automatic Apodization
Automatic Phase Correction	
	Fit to Highest Compound
Automatic Phase Correction	Fit to Highest Compound

**Global method:** This method automatically finds phasing parameters ( $\alpha$  and  $\beta$  or PH0 and PH1) using an iterative process in which the intensity of the lowest point in the spectrum is optimized. This method is not appropriate for experiments like DEPT or APT, where we can find both positive and negative peaks, but is highly efficient for most <sup>1</sup>H spectra. However, it is sensitive to bad baselines and low Signal/Noise ratios. Mnova will automatically execute this Phase Correction.

You can see below the effect of an automatic phase correction on a <sup>1</sup>H-NMR spectrum with a very bad phase:

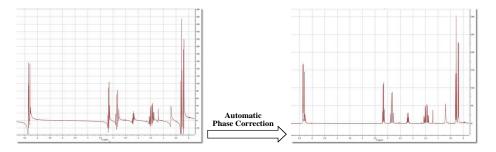


**Selective Method** (Not available in Mnova Lite): This automatic method is intended for spectra containing negative and positive peaks (e.g. DEPT, APT, etc) or in the presence of baseline distortions. Mnova creates a list of the highest peaks in the spectrum and then uses symmetrization criteria to obtain the optimal phasing parameters ( $\alpha$  and  $\beta$ ).

Mnova will automatically execute the better Phase Correction in each case prior FT.


# Metabonomics. A new Automatic phase correction algorithm optimized for biofluid-like spectra (Not available in Mnova Lite).

This algorithm is an extension of the standard automatic phase correction algorithm optimized to deal with Metabonomics-like spectra in which most of the signals are concentrated towards the center of the spectral width. In addition, it can also efficiently deal with situations in which a dispersive peak is present in the center of the spectrum, as is usually the case with water in urine samples. It is also tolerant to small first order baseline distortions (including V-shaped baselines).

The figure below shows a spectrum of rat urine with the standard automatic phase correction algorithm applied to the top spectrum and with the new automatic phase correction algorithm applied to the bottom spectrum.

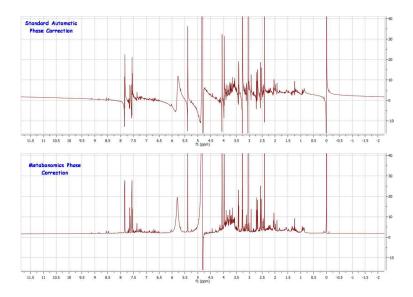


This algorithm is not restricted to Metabonomics spectra, as it is also good for any other spectra satisfying the two conditions outlined above. For example, the figure below shows the difference in performance between the standard automatic phase correction algorithm (top) and the new one (bottom). In this case, the water signal cannot be perfectly phased and thus a standard automatic phase correction fails. The new method yields a much better result as can be seen in the figure.

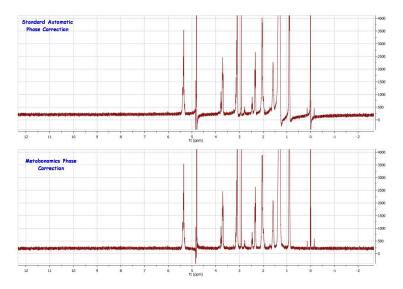

Whitening (only for 1D): A method for fully automated phasing of Fourier transform NMR spectra based on a combination of the whitening and the metabonomics method. First of all, the whitening method is applied in order to get good starting phase correction parameters even in spectra that have both positive and negative peaks. Then the most negative peaks are removed and a simple baseline correction is applied. Finally, the metabonomics method is applied.

The new phase correction algorithms will exclude all the regions in the spectra which are not part of the user selected region in the data analysis module. So for example, if the user has selected 3 regions in a spectrum for data analysis, auto phase correction should work exclusively in those 3 regions and discard all the other parts of the spectrum (If the applicable box is checked):

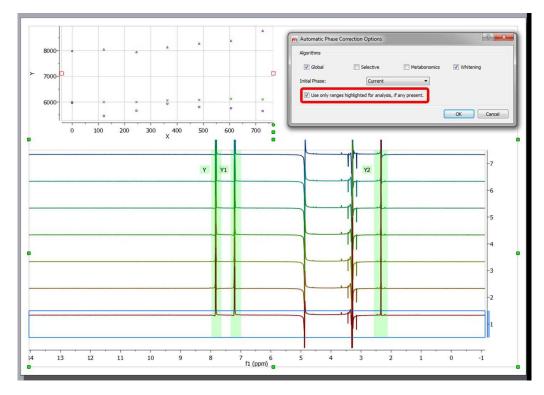

**Min. entropy:** An algorithm for automatic phase correction of NMR spectra based on entropy minimization. See <u>this paper</u> for further info

**Baseline optimization**: A method for fully automated phasing of Fourier transform NMR spectra based on a baseline optimization technique. See <u>this paper</u> for further info.

Regions Analysis: An autophasing routine which uses complex fit with phase on the peak regions.


**Manual Phase Correction (shortcut: Shift+P):** The manual phase correction is based in finding the appropriate  $\alpha$  and  $\beta$  phase correction parameters. This option is very easy to use. Just select 'Manual

Correction' in the 'Phase Correction' scroll down menu via the menu 'Processing/Phase Correction/Manual Correction'.

up or do		frag mouse			
		10 correction of	r		
		PH1 correction.			
(hold Ctrl	key for	fine tune)			
Como oro	coccina	ctope (o a ba	calina ca	reaction larg	nat
applied du	uring int	i steps (e.g. ba: teractive phasin the provisional i	g. The fi	inal spectrum	
applied du	uring int r from t	teractive phasin	g. The fi	inal spectrum tation.	
applied du may diffei	uring int r from t 1.00	teractive phasin the provisional i	ig. The fi represent	inal spectrum tation.	m
applied du may diffei PH0: -141	uring int r from t 1.00	teractive phasin the provisional i	ig. The fi represent	inal spectrum tation.	m

Once the dialog box is open, establish a pivot for the adjustment by just using the scrolling bar


provided. The pivot will maintain an invariable phase in the peak where it is located, while a first order correction is carried out. Click on the *Biggest* button to put the pivot point on the biggest peak of the currently displayed spectrum region. You can also place it in a position of your choosing by clicking and dragging the pivot point marker or by selecting the desired position in the edit box:

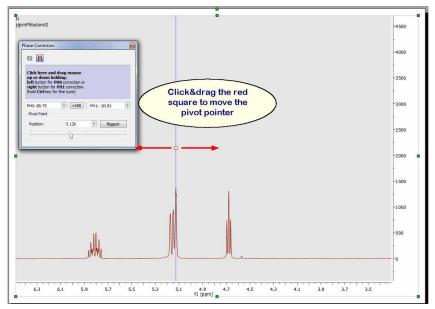

Next, correct the zero order phase (by clicking with the left mouse button anywhere on the *Phase Correction* dialog box and dragging the mouse up or down without releasing to correct the phase of the reference peak) and finally do exactly the same whilst right clicking to correct the phase of the remaining peaks (*First Order Phase Correction*). For a fine tuning, hold the 'Ctrl' (or cmd key in Mac) key while dragging the mouse.

You can use the 'Ctrl' key in a Mac machine to simulate the right mouse button in order to phase PH1.

The Phase Correction dialog box incorporates two edit boxes to introduce the values of  $\alpha$  (PH0) and (PH1)  $\beta$  for the correction and a button to apply +180° to PH0



The power and speed of the manual phase correction algorithm implemented in Mnova becomes obvious when correcting the phase of 2D experiments. This can be done directly on the 2D matrix, and the phase can be quickly corrected along one and then the other dimension (Note that for all operations in 2D NMR, the active dimension is indicated by the 'f1' and 'f2' icons in the upper toolbar).

### Phase Correction for 2D-NMR spectra

The phase correction feature for 2D NMR spectra includes in addition two powerful algorithms which can be accessed via the 'phase correction scroll down' menu:



Clicking on 'Options' will display a dialog box which will allow you to select the desired algorithm:

f2: 🔽 Projecti	one 🔽 Whi	
1: 🔽 Projecti	ons 🔽 Whi	tening
nitial Phase:	Imported	-
	7	
	Zero	
	Imported Current	
	Imported	

The **Projections** algorithm will calculate the 1D projections of the 2D-NMR spectrum and will apply a 1D automatic phase correction over both projections. These values will be used as initial values for the 2D adjustment when you have selected also the **Whitening** algorithm. If you only select the Projections algorithm, only 1D phase corrections values (of the projections) will be used for the 2D correction.

This method involves the calculation of the internal projection as the sum of all columns (or rows) in the 2D matrix. In the case of homonuclear correlation spectra, the projection is analogous to the diagonal. The phase correction calculated by an automatic 1D algorithm can be used as a rough estimate of the phase correction of the whole 2D matrix. This method is satisfactory in the case of homonuclear correlation, but inapplicable in the case of an edited HSQC (with both positive and negative peaks and much more noise).


The **Whitening** algorithm is based on the *whitening* concept formulated as the 'maximization of the number of white pixels into a bitmap that corresponds to the spectrum'. This process of maximization can be factorized along the individual axes of the spectrum and this property makes the method robust and fast. It employs a statistic measure based on a large number of spectral data points and, for this reason, is very tolerant to low SNR and local artifacts. The algorithm can efficiently phase either homonuclear or heteronuclear experiments and, unlike other previous methods, it can also process automatically spectra containing positive or negative peaks so that it is not necessary to deal with individual or special cases.

NOTE: After having applied a baseline correction in a 2D dataset, the manual phasing will be grayed out. To undo the baseline correction, follow the menu "Processing/Processing Template' and turn off the Baseline Correction for either dimension, click on OK and you will be able to correct the phase manually.

Alternatives to Phase Correction. Magnitude and Power.

There are other easier alternatives if you only need positive peaks: representations in 'Magnitude' or in 'Power'.

**Magnitude:** It determines the representation of the final spectrum. If this option is checked you will see the absolute part of the spectrum; if it is unchecked you will only see the real part. As a spectrum is composed of complex vectors, its magnitude or module M can be calculated by the following expression:



To represent the spectrum in *Magnitude* with Mnova, just open the 'Phase Correction' dialog box by clicking on the 'Phase Correction' scroll menu and then select 'Magnitude' (as you can see in the capture below) or via the 'Processing/Phase Correction/Magnitude' menu.

1	· M. T. L .
2/2	Auto (Global Method)
シン学	Auto (Metabonomics)
1000	Auto (Selective Method)
2/15	Manual Correction
)æ	Magnitude
Jy2	Power
-	T I

**Mnova** will replace the real part of the spectrum by the magnitude (*M*) of each complex vector and the imaginary one by the phase angle of the vector  $\phi$ , thus allowing reversal of this option. That is to say:


$$\operatorname{Re'}_{i} = M = \sqrt{\operatorname{Re}_{i}^{2} + \operatorname{Im}_{i}^{2}}$$
$$\operatorname{Im'}_{i} = \arctan\left(\frac{\operatorname{Im}}{\operatorname{Re}}\right)$$

**Power:** the power of the spectrum (*P*) is defined as the square of the magnitude:

$$P = M^2 = \text{Re}_i^2 + \text{Im}_i^2$$


To represent the power of the spectrum, open the **'Phase Correction'** dialog box by clicking on the **'Phase Correction'** scroll menu and then selecting **'Power'** or via the 'Processing/Phase Correction/Power' menu. The **'Power'** as well as the representation of the **'Magnitude'** are reversible options.

The 'Magnitude' representation produces an increase in linewidth, whilst the 'Power' representation distorts the intensities of the peaks:

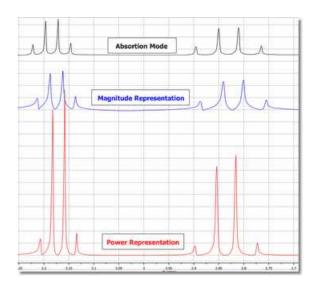

### Scripts to autophase importing autophase stacked spectra when importing.

Following the menu 'Scripts/NMR Tools', you will find a couple of scripts to apply automatic phase correction to a stacked plot:

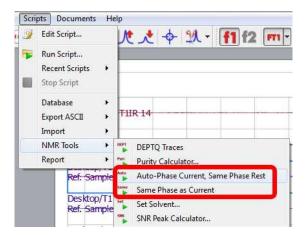

- Auto-Phase Current, Same Phase Rest: the active spectrum is automatically phase corrected, and the resulting values of PH0 and PH1 are applied to the other spectra in the stacked.
- Same Phase as Current: PH0 and PH1 values of the active spectrum are applied to the other spectra in the stacked.

# 8.6 Baseline Correction with Mnova

The baseline of a monodimensional spectrum is the theoretical line which connects the spectrum points which are not peaks (nor artefacts). When this baseline is not flat and/or it is offset from zero, many problems arise. Quantitative measuring of high resolution NMR demands a precise signal integration. These integrals are very sensitive to slight deviations of the spectrum baseline. The deviations are often due to a distortion of the first points of the FID (see First Point Correction and Linear Prediction). The origin of this kind of distortion is often the *transmitter breakthrough* effect (the detector needs a period to recover from the pulse effect in spite of being switched off when the pulse is applied). This could distort the first points of the FID producing a vertical displacement of the baseline, or even undulations, and, consequently, errors in the signal integrations. You can use a ' Backward Linear Prediction' to solve this problem on the time domain, or a 'Baseline Correction' as a better

alternative.

Modern spectrometer hardware uses oversampling and digital signal processing to improve the baseline, but some undesirable broad signals arise from real sources. Thus, a more general solution would employ an efficient post processing baseline correction in the frequency domain. In fact, this is the most common approach found in NMR literature.

2D spectra suffer from baseline problems which may cause difficulties in the visualization of the full data set at once, since the signals of interest may be smaller than the baseline distortions; specially for phase-sensitive experiments and when a large residual solvent signal distorts the baseline. Thus, it turns out that baseline correction is a very important processing step to obtain good quality spectra.

Baseline correction is an area in which Mnova is particularly strong. The software implements Manual Baseline Correction and several automatic Baseline Correction algorithms (Polynomial Fit, Bernstein Polynomial Fit and our in-house developed algorithm, the Whittaker Smoother, which gives exceptional results in 1D and 2D data sets, is extremely fast and in the vast majority of cases fully automatic and is tolerant to varying linewidths along the same spectrum and to poor signal to noise ratios).

The Baseline Correction interface is also very simple. Just click on the 'Baseline Correction' icon Met and this will execute a 'Full Auto' Baseline Correction, if you click on the scroll menu, the Baseline Correction dialog box will open and give the user a choice between the algorithms available, allowing control of certain parameters depending on the algorithm.





Novelty:


Using **Mnova**, you will able to adjust the phase after baseline correction, because Mnova will not discard the imaginary part of the spectrum after a baseline correction.

Mnova will be able to import the baseline correction from the spectrometer by following the menu 'Edit/ Preferences/NMR/Import' and checking the applicable box.


### THE BASELINE CORRECTION DIALOG BOX

Method			Qk	
Whittaker Smo	other	•	Cance	el
Whittaker Smo Polynomial Fit Bernstein Polyn Ablative Splines			Autodete	
<u>, , , , , , , , , , , , , , , , , , , </u>	0.01.01	1.1	1 1	1
Smooth Factor:	20000	*	Autodete	ect
				1.5

As a simple example of baseline correction, in the figure below we show a 1D spectrum in which the baseline distortions are evident. Note that the baseline not only deviates from the 0 level (represented by the gray dotted line), but it does also contain a significant rolling. You can choose the parameters of the baseline correction by dragging the parameter control (in the red circle in the 'Baseline Correction' dialog box above) or by introducing the values of the parameters directly into the edit boxes. You can also select 'Autodetect' if you prefer Mnova to calculate the best parameters for your spectrum.

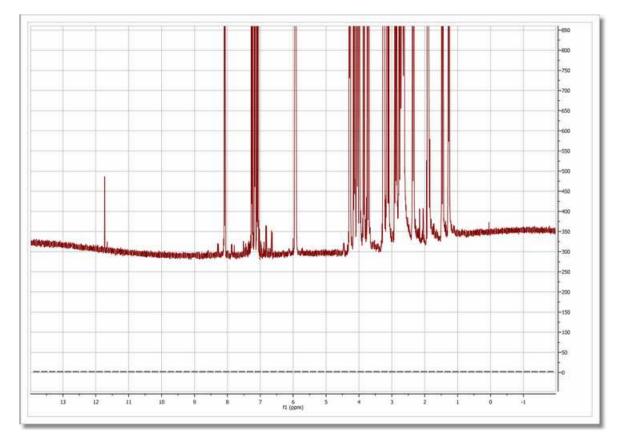

After baseline correction (fully automatic), using the **Whittaker Smoother** algorithm, the baseline becomes perfectly flat as depicted in the figure below

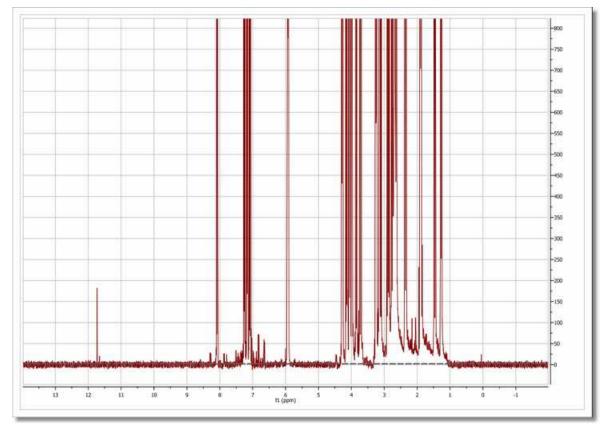

NOTE: Follow the menu 'Properties/Grid' to draw the baseline by selecting the applicable option (very useful if you have removed the vertical scale):

roperties		
eometry NMR Spectrum		
General Grid	Show Horizontal	Show Over
ID ▲ X Scales	Show Frame	Show Baseline
Horizontal	Line Width:	2.5

**Whittaker Smoother Algorithm:** it is a new procedure for automatic baseline correction of frequency-domain NMR data sets which we show to be highly effective on 1D and 2D spectral datasets, and which preserves the range of component line widths which are present in the sample.

The algorithm consists of two independent processes:

1. Automatic baseline recognition (signal-free regions) based on a Continuous Wavelet Derivative transform (CWT) followed by iterative threshold detection in the Power mode domain.

2. A baseline modelling procedure based on the Whittaker smoother algorithm.

Overall, the algorithm has been designed to afford perfect baselines in NMR data sets spanning a wide range of possible baseline topographies and signal-to-noise ratio (SNR) conditions. In most cases, it can be applied successfully without any operator interaction, but further versatility is assured by two parameters which could be adjusted to guarantee an optimum outcome. The procedure can therefore be "tuned" to achieve more accurate baseline recognition of signal-free regions, or to increase smoothness at the expense of spectral fidelity, or vice versa.


You can find more information about this 'in-house' developed algorithm in this reference: Cobas, J.C. *et al. J. Mag. Res. 183*, **2006**, 145.

**Polynomial Fit:** In some cases, the employment of polynomial interpolations offers the advantage of smoothing the corners of each section. The user can adjust the polynomial from first to 20th order as well as the so-called 'Median Filter' (the user can see in **real time** the exact effect of the algorithm by a green line drawn on the spectrum display).

The polynomial used in this interpolation is:

 $Y = a_1 + a_2 x + a_3 x^2 + a_4 x^3 + \dots + a_N x^{N-1}$ 


where  $a_1$ - $a_N$  are the coefficients to be fitted to the baseline and x the coordinates along the spectral axis.

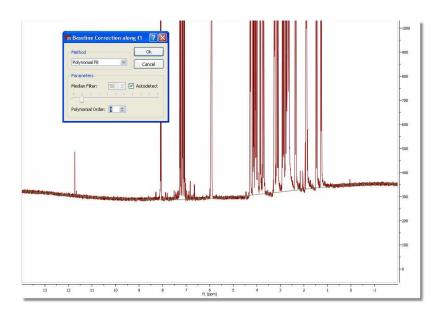

Bersntein Polynomial Fit: This interpolation is defined by the following polynomial:

 $Y = a_1(1-x)^{N-1} + a_2x(1-x)^{N-2} + a_3x^2(1-x)^{N-3} + \dots + a_Nx^{N-1}(1-x)^1$ 

The user only needs to select the order of the polynomial  $(a_I - a_N)$  and then click 'Ok', as shown in the capture below:



For a 2D example, see the <u>2D NMR Processing</u> Tutorial.

Please bear in mind that you can extract the baseline correction when you are working with 1D-NMR spectra by just clicking on the 'Extract' button CENTRAL. Once the baseline correction has been extracted, you can use it to correct the baseline of any other spectrum by using the 'Arithmetic' feature. You can see in the picture below that we have applied the previously extracted baseline correction of the sample 'js1pmquin' to the sample named 'STANDARD 1H OBSERVE' by applying a subtraction of the spectrum minus the baseline (Spectrum-Baseline=Spectrum with Baseline Correction).

1	rithme 7 + G ectra		?
1	Label	Title	Formula
1	A	STANDARD 1H OBSERVE	A - B
2	В	Baseline for js1pmquin	В

Ablative Baseline Correction: powerful algorithm for 1D-NMR spectra without negative peaks

Method				<u> </u>	<u>)</u> k
Ablative			•	Car	ncel
				r E	xtract
Paramete	rs				
Points:	5	¢	Passes:	10	

The ablative baseline correction works in frequency domain on NMR spectra which do not have negative peaks, nor prominent negative artifacts. It works best on spectra with relatively sharp peaks (though typical "broad" labile peaks are generally not affected).

It works, basically, by repeatedly "shaving off" positive peaks. Since it does it by alternating up- and

down- sweeps, it is reminiscent of the carpenter's ablative tool used to produce smooth surfaces (which is where it takes its name).

The algorithm gets negatively affected by negative-pointing peaks, including artifacts (like those from saturated water). In both cases the result is an improperly handled area extending over a significant portion of the spectrum. In many cases there is nothing of interest in that area, so the result is still perfectly usable. But sometimes it disturbs, in which case one should first get rid of the undesired features.


The algorithm gets also affected badly by Bruker smileys. Because of that, 2% of the spectrum on both ends are always set apart and considered as their own baseline. The result is that in the final spectrum, they get cut off.

Splines: it uses smooth curves to link the points.

**Multipoint Baseline Correction:** This method provides a way of modeling the baseline by selecting a well-distributed set of points that fall on the baseline and then interpolating between those points to complete the model. Please keep in mind that this method is not scriptable and can not be included in the Processing templates.


The following spectrum shows significant baseline distortion:

Next, select the 'Manual Multipoint Baseline Correction' in the 'Baseline Correction' scroll down menu:




This will display the 'Multipoint Baseline Correction' dialog box which will allow you to put down points along the baseline (by clicking on the 'Pick Baseline points' button ) to help the program to find the correct coefficients for the baseline correction equation that it will subtract from the spectrum. If you want to remove any undesired pick, just double click on it (click and drag if you want to change the

location of the point).

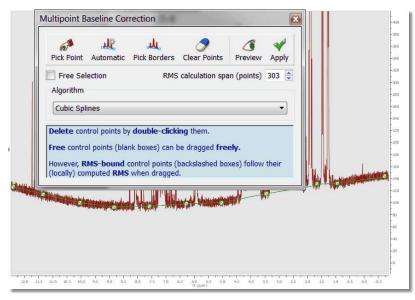

After subtracting the estimated baseline model, this is the resulting spectrum:

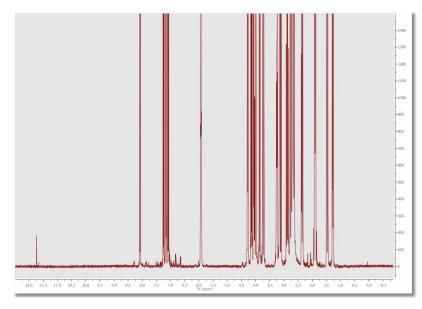

Let's see the functionality of each button of the "Multipoint Baseline Correction' dialog box:

**'Pick Baseline points'** allows the user to pick the points. To remove any selected point (highlighted in green), just double click on it.

'Automatic' automatically add points for the baseline correction

**'Pick Borders'** allows the user to pick the first and the latest points.

**'Clear all baseline'** Click on this button to delete all the selected points.

'Show/Hide Settings Controls' 🔤 click on this button to select the baseline correction algorithm and

the corresponding parameters.

**'Toggles Preview Showing' (**: to see a preview of the baseline correction.

**'Apply Baseline Correction' W**: to apply the correction.

'Free Selection' Free Selection : to pick a point anywhere.


**'RMS Calculation span (points):** The multipoint baseline algorithm builds a baseline model using the points selected; but if you select this option; instead of use the specific points selected in the spectrum when clicked, it uses an average value calculated from the point and the surrounded points given by the "average window" value. For example, and average window of 0 will use exactly the clicked/selected point, and a average window of 2 will use the average of the clicked/selected point and 2 point from the left and 2 points from the right, ie, in total it will use 2\*n+1 points where n is the average window

'Algorithm': from this drop down menu, we can select the algorithm for the baseline correction:

Segments: it simply connects the points with flat lines. This baseline will not be smooth, it just abruptly links the points with segments.

13	Multipoint Baseline Correction	-71
	Pick Point Automatic Pick Borders Clear Points Preview Apply	-61
	Free Selection RMS calculation span (points) 303 🖨	-5
	Algorithm Segments	-41
	Delete control points by double-clicking them.	-31
	Free control points (blank boxes) can be dragged freely. However, RMS-bound control points (backslashed boxes) follow their (locally) computed RMS when dragged.	-2
		-0
- Lealing and the second s		1

Cubic Splines: it uses smooth curves to link the points

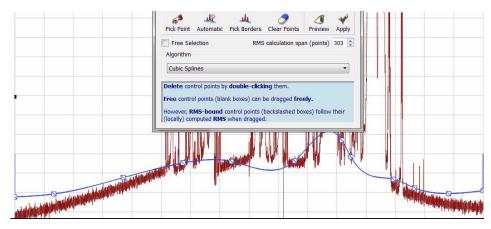

With segments and splines the baseline go thorough all the points defined by the user. This will not happen with the remaining algorithms:

Polynomial: the baseline will be adjusted to a polynomial function

13	Pick Point Automatic Pick Borders Clear Points Preview Apply
	Free Selection RMS calculation span (points) 303 🚖
	Polynomial
	Params Order: 8 🚖
	Delete control points by double-clicking them.           Free control points (blank boxes) can be dragged freely.           However, RMS-bound control points (backslashed boxes) follow their (locally) computed RMS when dragged.
A statistical of the statistical processing to state of the state of t	and manufacture and a second se

Witthaker: it will use the Witthaker Smoother algorithm to fit the baseline.

13	
	Free Selection RMS calculation span (points) 303
	Whittaker
	Params
	Smooth:
•	
	Delete control points by double-clicking them.
	Free control points (blank boxes) can be dragged freely.
	However, RMS-bound control points (backslashed boxes) follow their (locally) computed RMS when dragged.
	T(locally) compared which when dragged.
and and dealed and the state of	
	A STATE OF A
a had a later to be a start of the start of	

NOTE: After having applied a baseline correction in a 2D dataset, the manual phasing could be greyed out. To undo the baseline correction, follow the menu "Processing/Processing Template' and turn off the Baseline Correction for either dimension, click on OK and you will be able to correct the phase manually.

# 8.7 Symmetrization

Symmetrize (Not available in Mnova Lite):

This function, used in homonuclear correlation spectroscopy, replaces all signals which are symmetrically positioned about the diagonal by the smaller of the two signals. In this way unsymmetrically positioned noise and artifacts are removed. This technique should be used with caution since any symmetrical noise or artifacts will be preserved and may be mistaken for genuine signals. The data can be cleaned up considerably by using this tool in square data sets (homonuclear experiments). There are two modes available:


### Cosy-like mode

The most common type of symmetrization is performed on COSY type data where cross-peaks are symmetric on either side of a diagonal. This type of symmetrization is performed by following the menu

'Processing/Symmetrize/Cosy-like'. The command replaces the larger of two symmetrical points with a point that has the same magnitude as the smaller one. The user must know that this kind of symmetrization must not be used on phase sensitive data (because of the potential introduction of distortions to the cross peaks).

#### J-Resolved mode

For J-Resolved type data where the spectrum is symmetric on both sides of a horizontal line running through the middle of the matrix. The data point with the larger magnitude is replaced by one which has a magnitude equal to that of the smaller data point. This command is available by following the menu 'Processing/Symmetrize/J-Resolved'.



# 8.8 Tilt 45

Tilt 45 and Homonuclear J-resolved 2D-NMR spectroscopy (Not available in Mnova Lite):

Homonuclear *J*-resolved two-dimensional NMR spectroscopy is used to generate one frequency dimension representing chemical shifts and another with coupling constant information. This technique is most frequently used with homonuclear J-resolved spectra where the effect of couplings in the f2 dimension is not required.

The sequence:

$$d1\cdots90^{\circ}\cdots\frac{t_1}{2}\cdots180^{\circ}\cdots\frac{t_1}{2}\cdots t_2$$

(where d1 is for relaxation and  $t_1/2$  and  $t_2$  are the two time dimensions for the two-dimensional experiment) uses the 180° pulse to refocus chemical shifts during  $t_1$ .

In a *J*-resolved spectrum, the <sup>1</sup>H frequencies are found on the horizontal axis (f2) with the normal 1D spectrum displayed at the top while the vertical axis (f1) contains only proton-proton coupled multiplets, each centered about a zero frequency point. Then, the 2D *J*-resolved spectrum may be 'tilted 45°' (a projection at an angle of 45°) along a horizontal line through the center of the matrix, so that all the lines of each multiplet line up in the f1 dimension. Each row of the 2D matrix is shifted by an amount proportional to its distance from the middle of the spectrum. If all the individual spectra are now added together, the result is a <sup>1</sup>H decoupled NMR spectrum which is normally shown above the 2D spectrum.

Finally, the user could clean up the spectrum by symmetrizing it about the f1 = 0 Hz row. As it is explained in the previous chapter, this consists of comparing the intensities in the spectra equally spaced above and below the f1 = 0 Hz row and taking the smallest value.

This command is available by following the menu 'Processing/Tilt 45'.

# 8.9 Reducing t1 Noise


Reduce t<sub>1</sub> noise (Not available in Mnova Lite):

 $t_1$  noise is a particularly troublesome type of artifact which appears as streams of signals or ridges. The ridges (which are associated with strong signals in a contour plot), run parallel to the f1 axis and are found at their chemical shifts along the f2 axis. They can seriously interfere with the observation of real cross peaks from the signals.

The t1 command allows the user to clean up the spectrum along the f1 dimension by a factor proportional to the r.m.s. noise of that trace. It takes advantage of the fact that t1 noise is normally associated with the intense peaks which can be reduced without a significant loss of information.

The algorithm for t1-noise reduction has been designed to work with HSQC-like spectra.

This command is available by following the menu 'Processing/Reduce t<sub>1</sub> noise'.

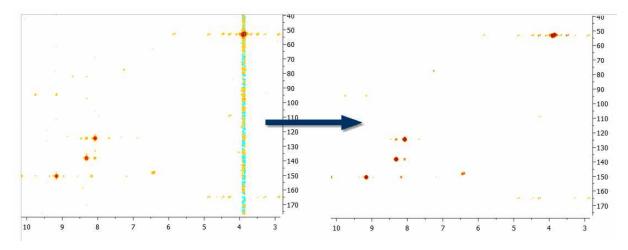

# 8.10 Covariance NMR


### (Not available in Mnova Lite)

Resolution and sensitivity are two key factors in NMR spectroscopy. In the case of 2D NMR, the resolution of direct dimension (f2) depends, among other things, on the number of acquired complex points whilst the resolution of the indirect dimension (f1) is directly proportional to the number of increments (or number of acquired FIDs). In general, it could be said that the resolution along the direct dimension comes *for free* in a sense that increasing the number of data points does not augment the acquisition time of the experiment significantly. However, increasing the number of t1 data points (increments) has a direct impact in the length of the experiment as can be seen from the Total acquisition time for a 2D NMR spectrum:

# T = n\*N1\*Tav


Where **n** is the number of scans per t1 increment, **N1** is the number of T1 increments and **Tav** is the average length of one scan. This usually means the resolution of the indirect dimension f1 is kept lower than that of f2.

You can easily apply the Covariance NMR tool just by following the menu 'Processing/Covariance NMR/Direct Covariance'. This will display the 'Covariance NMR' dialog box which will allows you to select the 'Regularization Factor', the 'Filter' and an 'Indirect Covariance NMR'. For further information about the CoNMR options, please check this paper: <u>JBiomolNMR (2007) 38, 73–77</u>

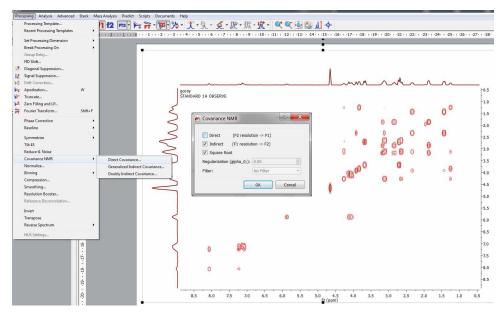


For example, let's consider the COSY spectrum (magnitude mode) of Strychnine which has been acquired with 1024 data points in the direct dimension and with 128 t1 increments. It's clearly appreciated that the resolution along F2 is much higher than the one along F1.

You can easily see that doublets corresponding to protons H20a and H23 are resolved in F2 but not in F1.

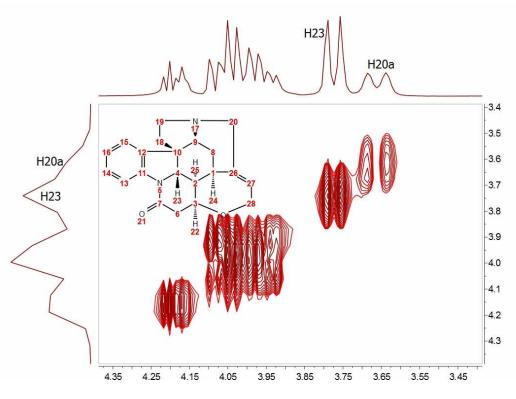


**How could this be improved?** We could try to extrapolate the FID (somehow) along the columns (F1) to a higher number of points (e.g. 1024). A well known technique is simply to add zeros, a process

called <u>zero-filling</u> which basically is equivalent to a kind of interpolation in the frequency domain. For example, in this particular case we could try to extrapolate the FID along t1) from 128 to 1024 points in order to match the number of points along f2. The figure below shows the results:

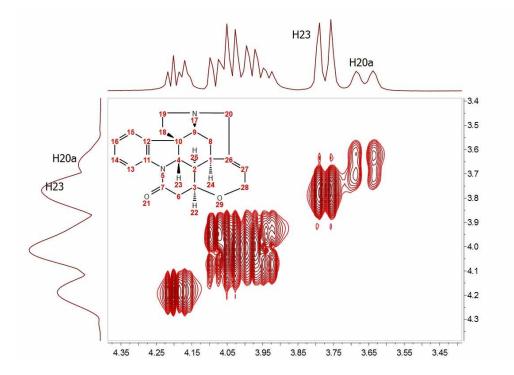

It can be observed now that the resolution along f1 is slightly higher than in the previous case but we cannot still appreciate the inner structure of the multiplets (e.g. H20a and H23). Zero Filling is certainly a good technique to improve resolution but of course, it cannot invent new information from where it does not exist. In this case we have zero filled from 128 to 1024 data points (e.g. 4 fold). In theory, zero filling by at least a factor of two is highly recommended because it enforces causality but beyond that, the gain in resolution is purely cosmetic. We might get more data point per hertz, but no new information is achieved as it's shown in the figure above.


**Is there a better way to extrapolate the FID?** Yes, and the answer is very evident: <u>Linear</u> <u>Prediction</u>. In few words, Forward Linear Prediction uses the information contained in the acquired FID to predict new data points so that we are artificially extending the FID in a more natural way than with Zero Filling. Of course, we cannot create new information with this process but the resulting spectrum will look better. This is illustrated in the next figure:

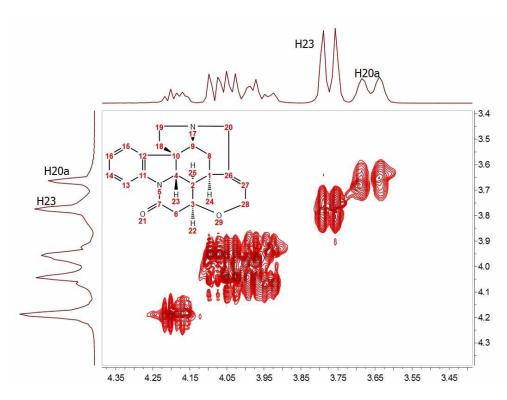

In this case, we have extended the t1-FID from 128 to 512 data points and then zero-filled up to 1024. Now we can see that the f1-lines are narrower but the couplings cannot be resolved yet.

In recent years there has been a great interest in the development of new methods for the time-efficient and processing of 2D (nD in general) NMR data. One of the more exciting methods is the so-called Covariance NMR, a technique developed by Brüschweiler et al. In fact, there are several types of Covariance NMR: Direct, Indirect Covariance NMR (there is a third method, Unsymmetrical Indirect Covariance which can be considered as a subtype of Indirect Covariance NMR). In this manual we will cover only the first type, Direct Covariance NMR leaving the other 2 types for future tutorials.

Before going any further with Covariance NMR, let's see the results of applying this technique to the same spectrum. This is what we get:

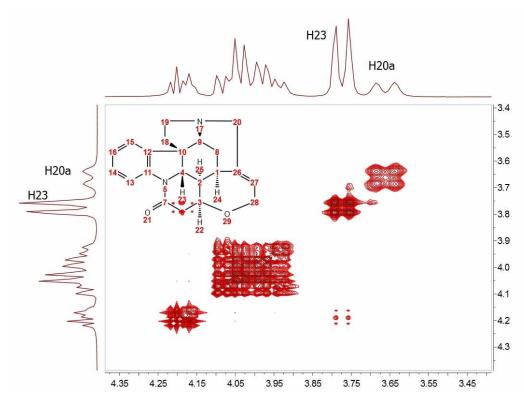

At first glance, this result looks like a kind of magic: Now the splitting of H20a and H23 are clearly resolved in both dimensions. Actually, the resolution along F1 is virtually analogous to that of the F2 dimension.

**How did we arrive to such a good result?** From an intuitive stand point, what we have attained here was a transfer of the resolution of F2 to the F1 dimension. In other words, we have applied a mathematical process which takes advantage of the higher spectral resolution in the F2 dimension to transfer it to the F1 one.


Mathematically, direct Covariance NMR is extremely straightforward as defined by the following equation:



Where C is the symmetric covariance matrix, F is the real part of the regular 2D FT spectrum and  $F^{T}$  its transpose (NOTE: direct covariance NMR can also be applied in the mixed frequency-time domain, that's, when the spectrum has been transformed along F2. In this case, a second FT will not be required – neither apodization or phase correction along the indirect dimension).


In order to approximate the intensities of the covariance spectrum to those of the idealized 2D FT spectrum, the square root of C should be taken. Root squaring may also suppress false correlations that many be present in  $F^{T}F$  due to resonance overlaps. Taking the square root of C matrix is in practice done using standard linear algebra methods (in short, diagonalizing the matrix and then reconstruct  $C^{1/2}$  using eigenvectors and square root of eigenvalues).

So direct Covariance NMR is able to produce a 2D spectrum in which the resolution in both dimensions is determined by that resolution of the spectrum in the direct dimension.

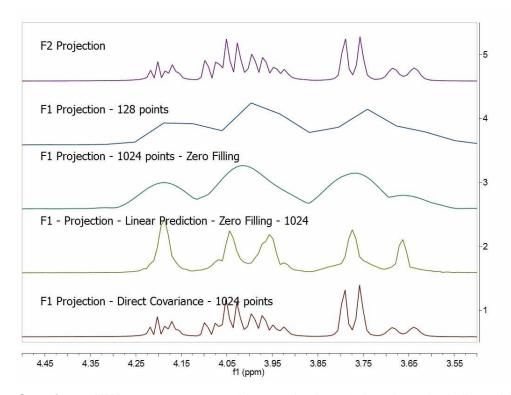


Let's see a stacked plot representation with the 1D projections obtained from the different processing methods described here (Zero-Filling, Linear Prediction and Direct Covariance NMR). You can see in the picture below the power of the Covariance NMR method.

**Covariance NMR** spectroscopy provides maximal resolution along the indirect dimension, but when the number of acquired data points is too small, the covariances exhibit poor statistics that manifest themselves as spurious cross-peaks. For example, in this case we can see some unexpected cross peaks (e.g correlation H27 and H23 which in principle should not appear in a GCOSY spectrum, but rather in a TOCSY spectrum). Some other artefacts might also arise when protons of different spin systems are coupled to resonances with overlapping proton multiplets.

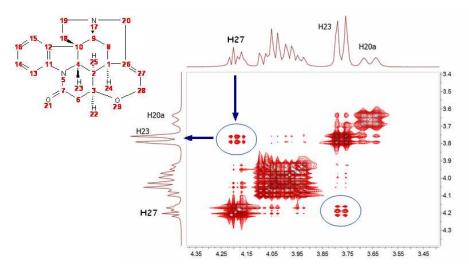


Mnova includes a novel filter which addresses this situation. This filter combines the standard 2D FFT

spectrum with the CoNMR version in such a way that the resulting spectrum, while keeping the high spectral resolution along F1, it's free of artefacts:

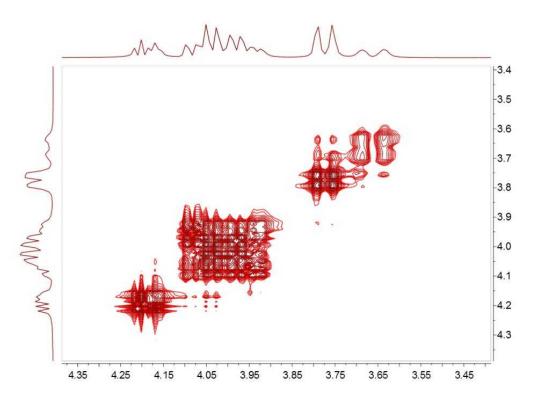


### **INDIRECT COVARIANCE NMR**

Interestingly, if we have a heteronuclear spectrum, we can transfer the correlation information from the indirect dimension to the direct one by simply changing the order in which the multiplication is carried out:



For example, the spectrum below shows the HSQC-TOCSY spectrum of sucrose (left) and its resulting indirect covariance counterpart (right) which contains essentially the same spin-connectivity information as a 13C-13C TOCSY with direct 13C detection:

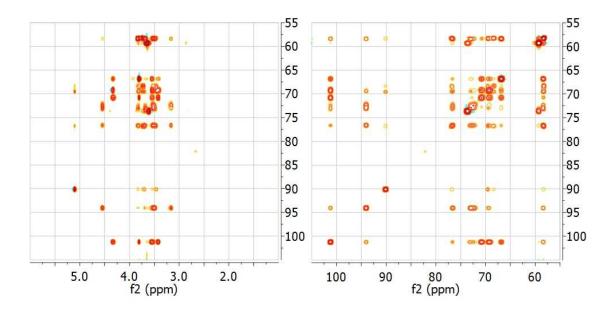

The advantage is obvious: Indirect Covariance NMR yields a 13C-13C TOCSY correlation without having to detect the 13C nucleus. In other words, it brings in a sensitivity increase of 8 over a 13C detected experiment. Of course, in indirect covariance NMR spectroscopy, the spectral resolution along both frequency axes is determined by the sampling along the evolution t1 time.

## **UNSYMMETRICAL COVARIANCE NMR**

You can also carry out **unsymmetrical Covariance NMR** with Mnova. However, as opposed to direct/indirect covariance NMR where one needs to deal with just one single spectrum, unsymmetrical NMR processing is probably not as intuitive as it's necessary to use 2 independent spectra and we have decided to implement it using a very open and flexible approach, that is, by using the spectral arithmetic module.

There two ways to apply an 'Unsymmetrical CoNMR' with Mnova:

1. Using the Arithmetic feature

### 2. Using the Generalized Indirect Covariance NMR

As you can see above, Covariance NMR is all about matrices operations. When you use direct/indirect CoNMR you simply multiply the spectrum matrix by its transpose where the order of the multiplication depends upon the CoNMR technique (direct vs indirect). The same concept applies to unsymmetrical CoNMR where you just need to multiply one spectrum by the transpose of another one.

Let's see an example to apply an unsymmetrical CoNMR by using the **'Arithmetic'** feature of Mnova, assuming that matrix A corresponds to an HSQC spectrum and matrix B corresponds to a COSY (or TOCSY) spectrum, unsymmetrical CoNMR can be achieved by the following matrix operation:

### C = A \* TRANS(B)

Where TRANS denotes matrix transposition.


It's important to bear in mind that with any algebraic matrix operation, it's necessary that matrices A & B are compatible according to their row/column dimensions.

To carry out unsymmetrical CoNMR, just open the 2 individual spectra in Mnova, process then as usual (making sure that the sizes are compatible) and finally go to Processing/Arithmetic to enter the

desire equation (e.g. A \* TRANS(B) )


Let's see step by step, how to generate a HSQC-COSY from separate HSQC and COSY spectra with Mnova

- 1. Import the HSQC and COSY spectra into Mnova
- 2. Select both spectra in the page navigator and follow the menu 'Processing/Arithmetic'

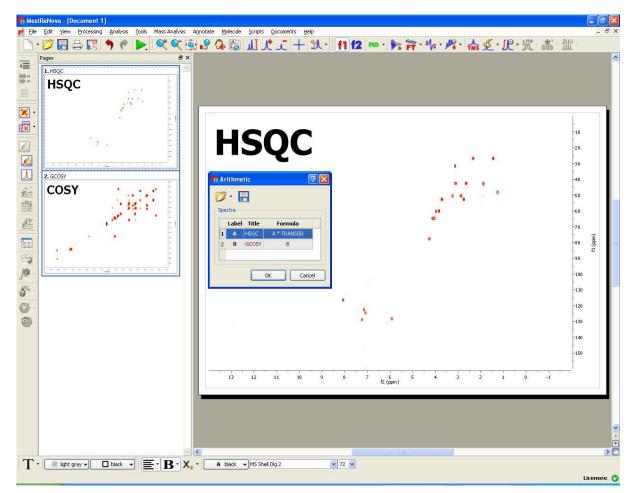

Finally enter the equation as depicted above "A\*TRANS(B)".In this case A corresponds with the HSQC spectrum whereas B is the COSY experiment. TRANS means the transpose operation.

Once the operation has been applied, click on the fit to height button  $\cancel{1}$ . You should get something like this:

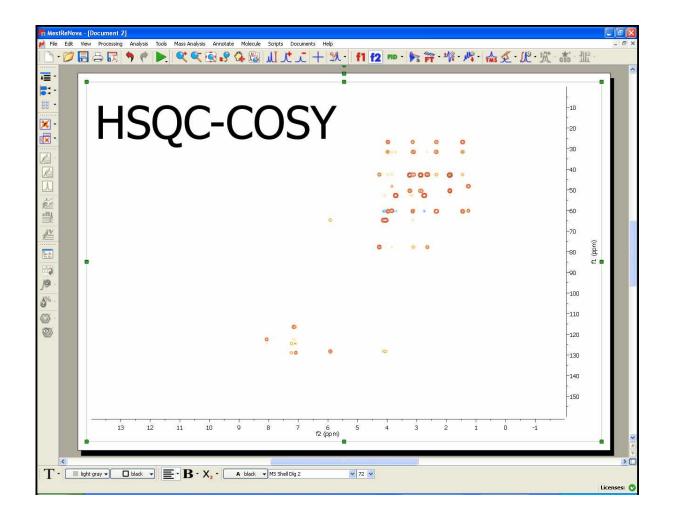


### Generalized Indirect Covariance NMR (GIC)

Multidimensional nuclear magnetic resonance (NMR) experiments measure spin-spin correlations, which provide important information about bond connectivities and molecular structure. However, direct observation of certain kinds of correlations can be every time-consuming due to limitations in sensitivity and resolution.

Covariance NMR derives correlations between spins via the calculation of a symmetric covariance matrix, from which a matrix-square root produces a spectrum with enhanced resolution. The covariance concept has also been adopted to the reconstruction of non symmetric spectra from pairs of 2D spectra that have a frequency dimension in common. Since the unsymmetric covariance NMR procedure lacks the matrix square root step, it does not suppress relay effects and thereby may generate false positive signals due to chemical shift degeneracy. This generalized covariance formalism permits the construction of unsymmetric covariance NMR spectra subjected to arbitrary matrix functions, such as the square root, with improved spectral properties.

This method is basically the same as the above one (Arithmetic) but using a more rigorous mathematic formalism which allows to minimize the number of false positive peaks, because now the user will be able to do the square of the two matrix product (or any other values of the lambda parameter; ie: 0.25)

To use this method, just load your datasets and follow the menu 'Processing/Covariance NMR/Generalized Indirect Covariance'. Finally select the spectra that you want to use and enter the value for the lambda parameter.

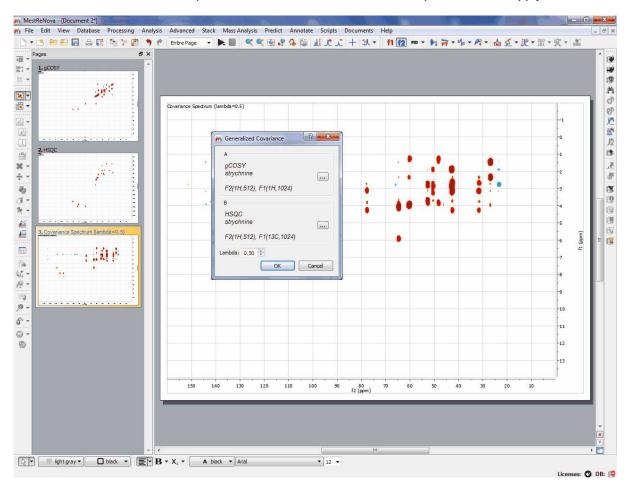


Please bear in mind that both spectra must have the same number of points in F2 to apply GIC


### **Doubly Covariance NMR**

The Double Covariance NMR spectroscopy, is extremely useful for structure elucidation as resulting spectrum is actually a carbon-connectivity map that can be directly analyzed with basic graph theory to obtain the skeletal structure of a molecule or even of individual mixture components or their fragments.

In the example shown below, we have a COSY and a HSQC loaded in the the same document.

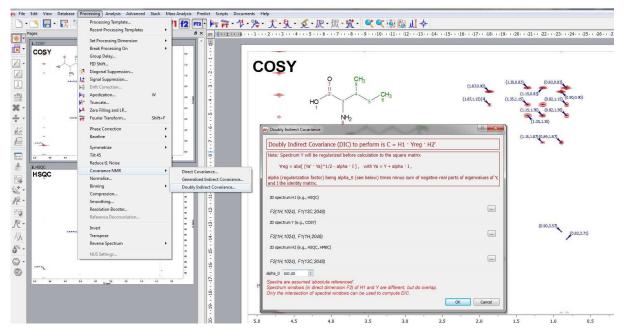

After having followed the menu 'Processing/covariance NMR/Doubly Indirect Covariance', we will get a synthetic spectrum (HSQC,HMBC) with the carbon-connectivity map:

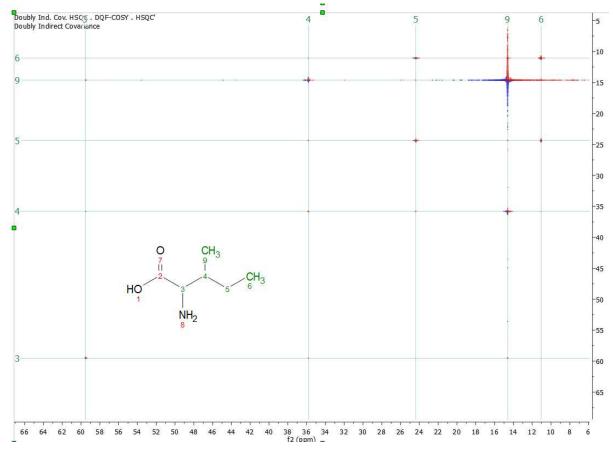

For further information about CoNMR, please read our blog:

http://nmr-analysis.blogspot.com/2008/10/introduction-to-covariance-nmr.html

http://nmr-analysis.blogspot.com/2008/11/indirect-covariance-nmr-fast-square.html http://nmr-analysis.blogspot.com/2008/11/removal-of-artifacts-in-direct.html

An this review: <u>http://www.ebyte.it/library/docs/nmr14/2014\_NMR\_Cobas\_Covariance.pdf</u> and this paper: <u>JBiomolNMR (2007) 38, 73–77</u>

For further information about Doubly Indirect CoNMR: J.Am.Chem.Soc. 2010, 132,16922

### 8.11 Normalization

#### Normalization:

The user is able to normalize the intensity of the spectrum by using this tool located in the 'Processing Menu'. The user can normalize the spectrum (or the spectra) by six different methods: total area, largest peak, largest peak range, a desired peak, a peak range or the 'manual normalization':

Normalize	2 ×
Normalize By:	Largest Peak 👻
Value:	Total Area Largest Peak
	Largest Peak Range
	Peak Peak Range Manual

- Total Area: Set the total area of each spectra to a specified value. Note you can use Cut or Blind Regions tools to exclude regions (such as residual water peaks).

- Largest Peak: Set the height of the highest peaks to the specified value. Again you can use the Cut or Blind Regions tools to exclude some peaks.

- Largest Peak Range: Set the height of the highest peaks within a range (default: the current zoom in region) to the specified value.

- Peak: Set the height of the specified ppm point to a specified value.

- Peak Range: Set the sum-integral of a specified range (default: the current zoom in region) to a specified value.

- Manual: Multiply all points of the spectrum by the specified value. (100 in the example below):

Normalize By:	Manual	
Value:	100.000	B

4	Utilities:

This tool is extremely useful when the user wants to stack spectra with different relative intensities and also after applying a binning.

# 8.12 Binning

Spectral binning is a widely-used technique where the spectrum is subdivided into several regions (bins), and the total area within each bin is used as an abstracted representation of the original spectrum. The area encapsulated by a bin would ideally capture all of the area associated with a given resonance across all spectra in the dataset, thereby mitigating the effect of minor peak shift and line width variations for a compound across samples.

This command is available by following the menu 'Processing/Binning'. Then, the 'Binning' dialog box will open and the user can choose the desired limits of the spectrum to apply the binning (or select Full Spectrum). The user can also select the width of each integral region. A typical 64k point NMR spectrum would be reduced using bin widths of 0.04 ppm, resulting in ~250 bin integral values.

Apply To		
📝 Full Spectrum		
From: -1.29 p	opm 🛓 To: 10,70 ppm	A Y
Width of Each Integral R	Region Method	
0.040000 ppm 🚔	Average Sum	•
	Sum	
V Save	Average Sum Center	
C:/Users/Usuario/Deskt		_
Тір		
Use <b>Cuts</b> view command (such as water region).	d if you want to exclude any regions	1
Include Class definition	into Stacked Spectra Table.	
	14 UEV	

The 'Sum' method will sum all the points of the bucket, the 'Average Sum' will divide the sum by the number of points on the bin, the 'Center' method will only return the value found in the middle of the bin. For example if the bin has 5 points it will return the value for 3rd point. The 'Peaks' method will use GSD for the peak picking.

There will be an option to save the matrix as CSV. The file generated is the same as the one obtained when saving as "Script: NMR CSV Matrix (Transposed).

Binning (also called bucketing) is a tool used in the multivariate analysis of NMR-based metabonomics data to address the NMR peak misalignment issue. In NMR metabonomics, small variations in the resonance position of the individual peaks caused by experimental and instrumental variations can adversely impact PCA results.

Fixed-width binning (usually at 0.04 ppm) is commonly used to alleviate the impact of the peak misalignment by averaging up the data points falling inside the bin width. However, since it drastically reduces the data resolution, it makes it more difficult to interpret the PCA results such as identifying the changed metabolites from the loadings plot.

The goal of binning a spectrum is to produce a new spectrum in which each new spectral data point corresponds to the integral of a bucket with a given width (e.g. 0.04 ppm). In other words, this is simply a data reduction operation analogous to bucketing integration. Once the spectrum has been binned, you can export it in ASCII format in order to use it for further PCA analysis.

It is often convenient to use the <u>Normalize</u> processing command to normalize the spectrum after applying a binning.

See also here an practical example of this feature

### 8.13 Compression

Compression (Not available in Mnova Lite):

A typical 2D experiment could be as large as 64Mb, whereas the final size of a processed 4D spectrum reaches easily the gigabyte range, resulting in a considerable burden on the data storage and backup systems and in low processing efficiency. Furthermore, these data must be transmitted and stored on computer networks. It is clear that advances in technology for transmission or storage are not sufficient to solve this problem. These considerations clearly raise the issue of efficient data compression.

Mnova incorporates a fast in-house developed wavelet-based compression algorithm, which is generally applicable to 2D NMR data sets (obtaining high compression rates; up to 800:1). We have tested this compression methodology with some examples of 2D spectra focusing on keeping the NMR signal information intact either on cases of qualitative purposes of signal assignment or on quantitative analysis as commonly required for solution structure calculations derived from nuclear Overhauser effects.

This command is available by following the menu 'Processing/Compression'. Then an 'Open' dialog will be shown:



The user can select the Compression Ratio or select 'Type:Lossless'. Lossless data compression allows the exact original data to be reconstructed from the compressed data.

# 8.14 Smoothing

**Smoothing** (Not available in Mnova Lite):

The signal to noise ratio (S/N) of a spectrum can be enhanced by smoothing (or filtering) techniques. This technique is used to reduce the effect of noise on a spectrum and possibly reveal signals embedded in, or distorted by, noise. Noise contains rapid fluctuations which are are generally faster than the rates of change of genuine signals. Smoothing applies a low-pass filter to the spectral data to remove these rapid fluctuations while having minimal effect on signals.

Mnova incorporates some of the more used signal smoothing algorithms.

This command is available by following the menu 'Processing/Smoothing. Then, a dialog box will open:

Apply	to All Dimensions	ОК
Method		-
Moving A	werage Filter 👱	Cancel
Paramete	rs	
Span:	2	0

The user can select the smoothing algorithm (Moving Average Filter, Whittaker Smoother, Savitzky-Golay or Wavelets) in the Method scroll bar. The user can also apply the smoothing to All Dimensions (by ticking the applicable box).

**'Moving average algorithm'**: The simpler software technique for smoothing signals consisting of equidistant points is the moving average. An array of raw (noisy) data  $(y_1, y_2, ..., y_N)$  can be converted to a new array of smoothed data. The "smoothed point"  $(y_k)_s$  is the average of an odd number of consecutive 2n+1 (n = 1, 2, 3, ..) points of the raw data  $y_{k-n}$ ,  $y_{k-n+1}$ , ...,  $y_{k-1}$ ,  $y_k$ ,  $y_{k+1}$ , ...,  $y_{k+n-1}$ ,  $y_{k+n}$ , i.e.

$$(y_k)_s = \sum_{i=-n}^{i=n} \frac{y_{k+i}}{2n+1}$$

The odd number 2n+1 is usually named filter width (or span in Mnova). The greater the filter width the more intense the smoothing effect.

The moving average algorithm is particularly damaging when the filter passes through peaks which are narrow compared to the filter width.

The user can select the desired filter width (Span) in the dialog box.

Whittaker Smoother: A smoothing algorithm is proposed by Whittaker in1923. If y is a series of m data points and z is the smooth series which should approximate y, we minimize:

$$Q_2 = \sum_{i=1}^{m} (y_i - z_i)^2 + \lambda \sum_{i=2}^{m} (z_i - z_{i-1})^2$$

The first term measures the fit of z to y, the second term is a so-called penalty: it discourages changes in z. The influence of the penalty is tuned by the parameter  $\lambda$ ; the larger a  $\lambda$  is chosen, the smoother z will be, at the cost of a worse fit to the data.

The user can select the Smooth Factor in the dialog box or let Mnova detect the best one automatically.

Smoothing along f2	?
Apply to All Dimensions	OK
Method	-
Whittaker Smoother 🛛 👻	Cancel
Parameters	
Smooth Factor:	2
Autodetect	

'Savitzky-Golay algorithm' : A much better procedure than simply averaging points is to perform a

least squares fit of a small set of consecutive data points to a polynomial and take the calculated central point of the fitted polynomial curve as the new smoothed data point.

Savitzky and Golay showed that a set of integers  $(A_{-n}, A_{-(n-1)}, ..., A_{n-1}, A_n)$  could be derived and used as weighting coefficients to carry out the smoothing operation. The use of these weighting coefficients, known as convolution integers, turns out to be exactly equivalent to fitting the data to a polynomial, as just described, and it is computationally more effective and much faster. Therefore, the smoothed data point  $(y_k)_s$  by the Savitzky-Golay algorithm is given by the following equation:

$$(y_k)_s = \frac{\sum_{i=-n}^n A_i y_{k+i}}{\sum_{i=-n}^n A_i}$$

Sets of convolution integers, instead of the smoothed signal, can be used to obtain directly, instead, its  $1^{st}$ ,  $2^{nd}$ , ..., m<sup>th</sup> order derivative, therefore the Savitzky-Golay algorithm is very useful for calculation of the derivatives of noisy signals consisting of discrete and equidistant points.

The smoothing effect of the Savitzky-Golay algorithm is not as aggressive as in the case of the moving average and the loss and/or distortion to vital information is comparatively limited. However, it should be stressed that both algorithms are "lossy", i.e. part of the original information is lost or distorted. This type of smoothing has only cosmetic value.

The user can select the 'order' and the 'Width' as the dialog box below shows:



**Wavelets:** Wavelet thresholding is the basis of wavelet based noise reduction. For a function *f* with Gaussian noise

 $y_i = f(t_i) + \sigma \varepsilon_i \cdots (i \in \mathbb{N})$ 

this means that the function *f* is restored.

Hard thresholding is a simple "keep or kill" selection. All wavelet coefficients below a threshold  $\lambda$  are zeroed.

$$c_{j,k}^{hard} = \begin{cases} 0, & \left| d_{j,k} \right| \leq \lambda \\ \\ \\ c_{j,k} & \left| c_{j,k} \right| > \lambda \end{cases}$$

Soft thresholding shrinks the coefficients towards zero:

$$c_{j,k}^{soft} = \begin{cases} c_{j,k} - \lambda, & c_{j,k} > \lambda \\ 0, & \left| c_{j,k} \right| \leq \lambda \\ c_{j,k} + \lambda & c_{j,k} < -\lambda \end{cases}$$

The most important step is now a proper choice of the threshold  $\lambda$ .

A universal threshold consists of:

$$\lambda = \frac{\sigma \sqrt{2\log n}}{\sqrt{n}}$$

where *n* is the sample size and  $\sigma$  the scale of the noise on a standard deviation scale.

The overall procedure of noise suppression consists of a wavelet transform (WT), which yields the wavelet coefficients cj;k, followed by thresholding of these coefficients and by an inverse wavelet transform (IWT), which restores the original spectrum.


The user can select the scale ( $\sigma$ ) and the fraction threshold ( $\lambda$ %) or also the soft or the Universal Threshold (by ticking the applicable box).

Apply to All C	Vimensions	OK
Method	(	
Wavelets	I	Cancel
Parameters		
Scales:	4	
	And and a second second	

## 8.15 Denoise

In any experimental technique, the distinction between signals and noise is a real factor, and this is particularly the case with NMR because of its low inherent sensitivity. The application of the so-called ' spatial filters' has been proposed for the efficient denoising of images as well as for 1D and 2D NMR data sets.

Mnova includes a number of those filters aimed at reducing the noise level while maintaining the original spectral resolution.

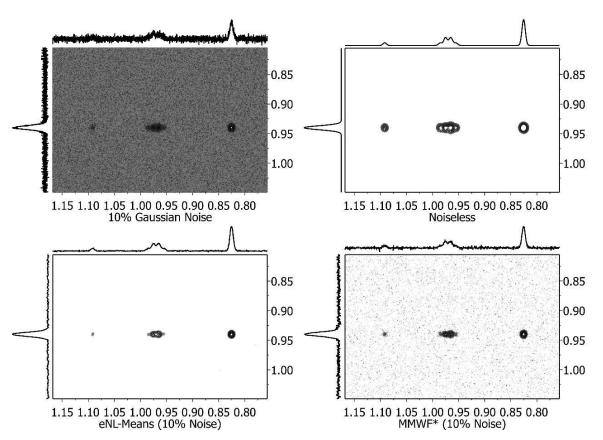

Comparison of the MMWF\* and eNL-means filter with a synthetic 2D spectrum 10% Gaussian noise (top-left). Top-right spectrum is the original noiseless spectrum whilst the two spectra at the bottom of the figure are the denoised spectra using MMWF\* (bottom-right) and eNL-Means (bottom-left)

### Enhanced Non-Local Means

This is an algorithm based on the Non-Local Means denoised procedure which exploits the property that many structural similarities are present in different parts of the spectrum and that are not necessarily located in a local neighborhood. This algorithm is complemented by the application of a hybrid median algorithm used to remove potential spikes in the resulting NL-means denoised algorithm.

The **blocksize** is the default mode as it gives the highest denoising power. As a drawback, it is much slower than the other two modes (pixelwise and fast pixelwise).

Method: Non-Local I	Means
Noise Factor:	1.00
Mode:	Blocksize

# 8.16 Resolution Booster

**Resolution Booster** (Not available in Mnova Lite):


Resolution is a key concept in high resolution NMR and considerable effort (e.g. shimming) is usually devoted to ensure optimum resolution. High spectral resolution is important for the measurement of NMR parameters, especially for signal intensities, chemical shifts, and coupling constants. However, in many areas of high-resolution NMR the observed resonance lines are broadened in some undesirable way that may complicate, if not preclude, the accurate analysis of e.g. scalar couplings. Moreover, you can directly measure accurate values of *J* only when the splitting is much larger than the linewidth. The classical solution to the line broadening problem, other than using higher magnetic fields and assuming proper shimming, is multiplication of the FID by a resolution-enhancement function. More sophisticated procedures involve nonlinear data-processing methods such as the much-discussed maximum entropy method. The Filter Diagonalization Method (FDM) and Reference Deconvolution are other well known processing procedures that can be used for resolution enhancement.

The most frequently used methods for resolution enhancement are those which involve appropriate mathematical treatment of the FID (weighting). For example, one popular, routinely used weighting function is the Lorentzian/Gaussian transformation. Other well-known weighting functions include the TRAF, convolution difference, and sine-bell functions. Most of these methods have in common that they alter the FID such that its beginning is deemphasized, relative to the latter parts. Although these methods can improve resolution significantly, caution must be taken because information can be destroyed or artefacts created by extreme enhancement, such as that which results in large negative lobes on both sides of a signal.

The **Resolution Booster** is a new frequency domain post processing method which yields a considerable resolution enhancement with a fast calculation, while avoiding the negative artefacts of the other resolution enhancement functions.

#### **Real Example:**

In order to illustrate the power of our Resolution Booster method, we will use as an example the spectrum of *dimethyl pyridine-2,5-dicarboxylat*e acquired at 250 MHz:

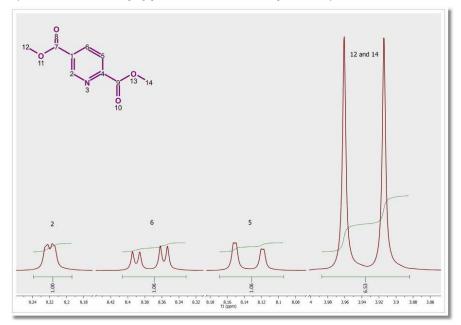

This spectrum has been processed without applying any weighting function and the resolution is **0.13 Hz/pt**. If we look at the signals corresponding to proton 2 in the structure, we can appreciate a small splitting due to 4 bond coupling with proton 6. Proton 6 shows a large splitting due to 3 bond coupling

with proton 5 and a small splitting due to the 4 bond coupling with proton 2. Proton 5 appears as a double doublet because of the 3 bond coupling with proton 6 and a small 5 bond coupling with proton 2. The latter is barely appreciated in the figure because of the lack of resolution. In fact, the same splitting should show in proton 2 but this can not be seen at this resolution level. It is important to remember that you can measure couplings constants accurately when the splitting is much larger than the line width.


Following the menu 'Processing/Resolution Booster' will display the 'Resolution Booster' dialog box, where the user will be able to select the resolution degree of the algorithm:



Resolution Booster is sensitive to the line width of the signals. If a spectrum contains both narrow and broad lines, the algorithm could try to enhance the resolution of the sharp lines, but the negative side effect would be a potential removal of the broad lines.

Likewise, if we want the keep the broad lines, the resolution power of Resolution Booster should have to be reduced.

In the picture below you will be able to see the result of applying the **Resolution Booster** method by using the Normal Resolution:

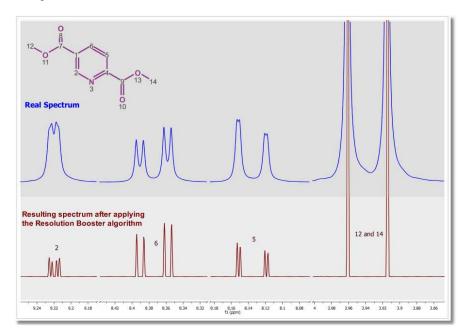

In this case, resolution has been increased by ~230% making possible the calculation of the weak, long range coupling constants.



It is important to notice that this procedure may change relative intensities. On isolated lines, in principle, it is approximately proportional to the second derivative which, when all lines have the same line width (as they often do) is proportional to the line height. However, broad lines can get suppressed and unresolved humps and shoulders get resolved (+) but their intensities and, to some extent, positions can not be trusted (-).

Please bear in mind that we can not integrate the spectrum after having applied Resolution Booster as this algorithm is sensitive to the signals linewidths. If all the lines in the spectrum would have exactly the same line width, Resolution Booster could also be considered a valid tool for qNMR analysys. But in real life, this is never true.

Thus, RB should be considered as a Resolution Enhancement tool which you can use for any of the following purposes:

- to measure chemical shifts & coupling constants more accurately
- to reveal signals which could otherwise be hidden and badly resolved because of spectral overlap

The Resolution Booster can also be used with 2D-NMR spectra.

#### See also:


http://nmr-analysis.blogspot.com/2007/11/resolution-booster.html http://nmr-analysis.blogspot.com/2007/11/selective-resoluton-booster.html http://nmr-analysis.blogspot.com/2007/12/introducing-2d-resolution-booster-rb.html

# 8.17 Reference Deconvolution


Reference Deconvolution is a signal processing method to remove experimental effects that broaden lines. Reference deconvolution is a technique which uses the shape of a single resonance line to measure the actual frequency distribution produced by the local magnetic field in homogeneity and then deconvolves that distribution from the whole spectrum. It is a simple linear process which requires no prior knowledge of the number of lines, their intensities, or their relaxation characteristics. No fitting procedures are used.

This ability to generate sharp line spectra is very important for DOSY measurements, improving t1 noise in 2D spectra, qNMR (through reducing truncation effects), and we can expect it to also add robustness to Verification, metabolomics, and in many more real-life situations.

Here you can see an example of the NMR spectrum which has been folded several times to optimize digitization. To correct the severe lineshape problems and spinning sidebands, we will apply 'reference deconvolution' by following the menu 'Processing/Reference Deconvolution'. After that you will notice that the mouse cursor will change to an integral curve; the next step will be to click&drag over the region of interest (which must be always a singlet) to display the Reference Deconvolution dialog box, from where additional settings can be applied:

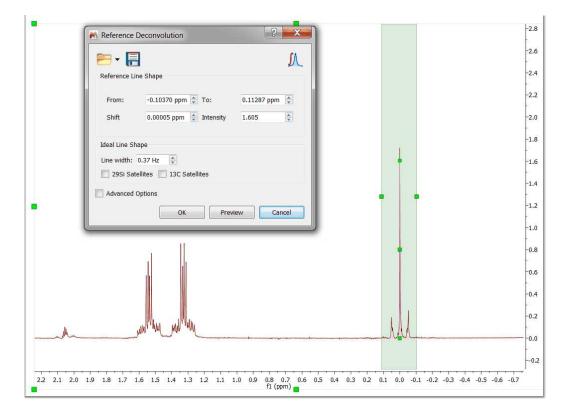

After having clicked on the OK button, you will get the result:

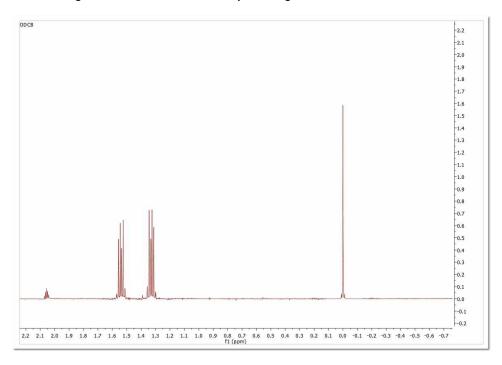

Checking the 'Advanced' box will display additional tabs with settings for the 13C and 28Si satellites; to minimize the artifacts and to select the peaks of interest for the reference deconvolution model:

Deconvolutio	on		2	X
				<b>M</b>
e Shape				
-0.10370 p	ppm 🏮 <u>T</u> o:	0.	11287 ppm 🚦	
0.00005 p	pm 🍃 Intens	ity 1.	605	
0.37 Hz 🌻	*)			
	*)	del		
illites 🔲 13	9 <u>C</u> Satellites	-		
Illites 13	9⊆ Satellites Peaks for Mo Right		10000	
	e Shape -0.10370	e Shape -0.10370 ppm 🖨 To: 0.00005 ppm 🌲 Intens	e Shape -0.10370 ppm 🔶 To: 0. 0.00005 ppm 🔶 Intensity 1.	e Shape -0.10370 ppm 🖨 To: 0.11287 ppm 🖨 0.00005 ppm 🌲 Intensity 1.605

The model settings can be saved to be used with other datasets by clicking on the 'Load/Save' buttons.Saving the model will store:

1. The experimental shape between specified limits.

2. The peaks found by peak picking in the same region, including info if the peaks are selected or deselected by the user.

3. The parameter which shows if user want to use experimental shape or the synthetic shape from the peaks.

Loading a settings file and clicking on the "Show Reference" button, will display all the GSD peaks in the reference region (the non-selected ones will appear in grey). You can switch to the experimental shape (by unchecking the option "Create shape from peaks"):

Reference Deconvolution		2	<b>x</b>	0.00			- F
₽- 🗐	1			0.00			-1.8
Reference Line Shape	ppm Ir	tensity	•				-1.6
External reference is loaded. Original file: C:/Users/Usuario/Desktop/testing.mnrd	0.042	0.06					-1.5
Show Reference	☑ 0.041	0.02					-1.4
Press and hold to view the loaded referen	nce shape 0.020	0.01					-1.3
Ideal Line Shape	☑ 0.011	0.04	E				-1.2
Line width: 0.37 Hz	☑ 0.009	0.01					-1.1
29Si Satellites 📝 13C Satellites	0.006	0.03					-1.0
Advanced Options	0.004	0.05					-0.9
Satellites Artifacts Peaks for Model	0.000	1.60		4			-0.8
	-0.002	0.51					-0.7
Create Reference Shape from Peaks	-0.006	0.15					-0.5
			-				-0.4
OK Preview Car	ncel						-0.3
	<b>A</b>		)			$\wedge$	-0.2
h	him		1	///		mont 1	-0.1
			At	<u> </u>		An S	-0.0
				1			~0.1
0.060	0.050 0.040	0.030 0.020	0.010	0.000 -0.010 -0.02 f1 (ppm)	0 -0.030 -0.040	-0.050 -0.060	-0.070


See also this blog post

# 8.18 Inverting, Transposing and Reversing Spectra

**Invert:** The command 'Processing/Invert' multiplies all spectrum data points by -1. It is equivalent to applying a zero order phase correction of 180° It is very useful for DEPT spectra.

**Transpose** (Not available in Mnova Lite): This command allows the user to transpose (by interchanging the rows and columns of the matrix) a spectrum for more convenient representation. This command is available by following the menu 'Processing/Transpose'.

**Reverse Spectrum:** The commands ('Processing/Reverse Spectrum') on this submenu allow you to reverse the spectrum along **F1**, **F2**, (horizontally or vertically) or **both axes** to obtain a more convenient representation.

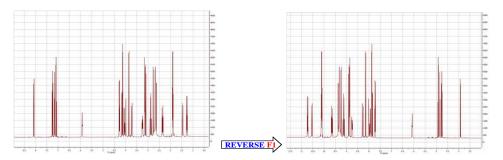

# 8.19 Processing Templates

**Mnova** includes a powerful and flexible feature which allows the user to easily automate the full processing of both 1D & 2D NMR data sets. This is ideal for the batch processing of spectra of the same type, and can also incorporate analysis operations.

For example, let's say you have acquired 20 proton spectra which you want to process using the same processing operations. The procedure is:

- 1. Load one spectrum and process it as desired.
- 2. Go to Processing/Processing Template. The following dialog appears:

F1			
	More Processing	Analysis	
Time	Domain	Frequency Domain	
<b>F</b>	ID Shift	Phase Correction	
		Method: Imported PHO: -141 PH1: -4.39315	
	Drift Correction	Baseline Correction	
<u> </u>		Method: Whittaker Smoo	
۲ 📃	Truncate	Median Filter: Autodetec Smooth Factor: Autodet	
<b>F</b>	Frequency Shift	Smoothing	
V A	Apodization	Reverse	
Exp	ponential: 0.5 Hz	Reference	
Zero	Filling and LP	Absolute Reference	
Sp	ectrum Size: 65536		
Four	ier Transform	E Factor: : 100.000000	
	otocol: None	Cuts	
Sw	ap Halves: on	Number of Cuts: 0	
Mi	ror Image: on	number of cuts: 0	

This dialog includes all the processing and analysis features implemented in Mnova. You can choose the required options by selecting the check boxes and, if necessary, specify options by clicking the button  $\boxed{}$ ; next to the corresponding command.

3. Once you are happy with the result, save the script file to a Mnova Processing file (\*.mnp) by

clicking on the save button in the dialog box.

4. You can now apply this processing script file to any other spectrum/spectra by selecting the spectra you wish to process following this procedure (one or several spectra), and then opening the previously


saved file by using the open command in the Processing Template dialog box.



#### A few helpful tips ...

If you want to apply a processing script to all the spectra opened in one document, first select all the spectra in all the pages.
 Next you can simply go to *Processing/Recent Processing Templates* and select the appropriate processing file script.
 Remember that only spectra acquired using the same conditions should be processed using a processing script file. For example, if you have acquired a spectrum using a sequential mode and another one using simultaneous quadrature detection, you will get erroneous results.

You can report into Mnova the processing template you have created, just by clicking on the 'Report' button . From the scroll down menu, you will be able to 'copy the report to clipboard' and to customize it:

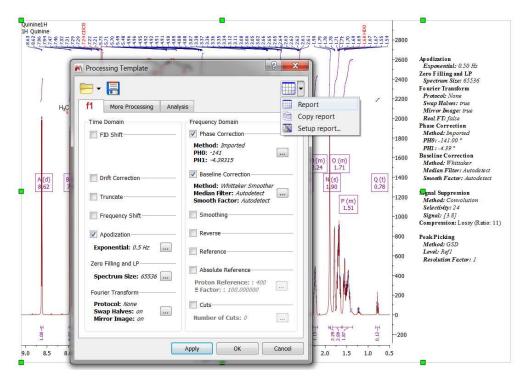

Use the script below to run a saved processing template:

```
//<GUI menuname="ApplyProcessingTemplate"shortcut="Ctrl+2"tooltip="Apply a saved processing tem
function ApplyProcessingTemplate()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    var processing = new String;
    if (!spec.isValid())
    return;
    processing = "C:\\ProcessingTemplate.mnp";
    nmr.processSpectrum(spec, processing);
    spec.process();
    mainWindow.activeWindow().update();
}</pre>
```



# 9 Analysis Tools

This section will give you an outline of the features already implemented, and which will have full or at least partial capabilities in this version:

Ana	lysis Advanced S	tack	٨
	Reference	•	
	Blind Regions	•	
	Peak Picking	•	
	Integration	•	
	Multiplets Analysis	•	l
	Assignments	•	
Ì	Clean Analysis		
	Predict & Highlight	•	
	Predict & Verify	•	
	Predict Compare		
	Spectral Moments		
	Verification		

Chemical Shift Referencing Peak Picking Integration Multiplet Analysis Molecular Structure Assignments Prediction of NMR Spectra

The 'Clean Analysis' tool will delete all analysis features (peaks, integrals, multiplets) for the selected spectra as well as all assignments of the molecules linked with that spectrum.

# 9.1 Chemical Shift Referencing


In NMR, the frequencies are usually measured relative to a frequency standard. As these frequencies are strictly measured relative to a frequency standard proportional to the magnetic field, it is convenient to define the chemical shift as:

$$\delta = 10^{6} \cdot \frac{(\nu - \nu_{ref})}{\nu_{ref}} = 10^{6} \cdot \frac{\sigma_{ref} - \sigma}{1 - \sigma_{ref}} \approx 10^{6} \cdot (\sigma_{ref} - \sigma)$$


Thus, in order to establish a chemical shift scale, it is necessary to choose some substance as a reference and define its chemical shift. In non-aqueous solvents, the most used reference substance is **TMS** (tetramethysilane) which is defined to have a chemical shift of **0.0 ppm**. For biomolecules, slightly different compounds (e.g. TSP,  $(CH_3)_2SiCD_3CD_2CO_2Na$ , Sodium-salt of trimethylsilyl-propionic acid) are used, since TMS is not soluble in water.

There are two way to reference your spectra, one graphically and another by using a dialog box.

The **Graphic Reference** (R as shortcut) will allow you to reference your spectra just with two clicks. Once click to select the position that you want to reference and another click to select the new chemical shift. This feature will be very useful to reference stacked spectra (for example):

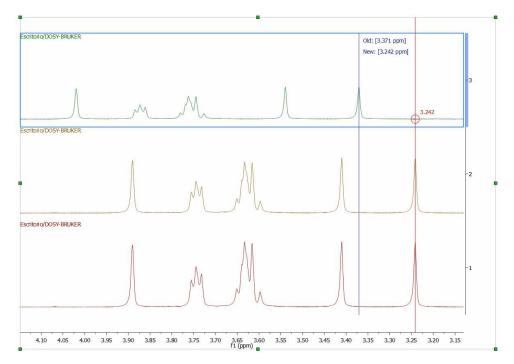

you can also use this tool to reference the 2D-NMR spectra directly with the 1D external trace. To do it just press the 'R' key, next click on the peak that you want to reference and finally click again on the new chemical shift (matching with the peaks of the external traces):

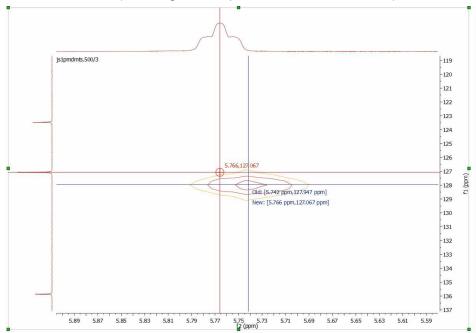

You can also calibrate your spectrum by selecting *Analysis/Reference/References* (L shortcut) on the main menu or by clicking on the toolbar button and then following this procedure:

1. Zoom-in on the spectrum region containing the reference peak

2. Select the peak you want to be a reference point. You will notice that the mouse cursor automatically *jumps* to the peaks maxima. To select a peak at an arbitrary position which is not a local extreme (e.g. the shoulder of a peak), press **SHIFT** key, move the mouse to the desired position and click. The **following** dialog box appears:

Old Shift:	7.25	2 ppm	4	Auto Tuning
New Shift:	7.26	0 ppm	٢	+/-: 0.100 ppm 🙄
🗹 Annota	tion	CDCl3		

You will be able to type any annotation after having referenced your signal.

The 'Auto Tuning' option finds the maximum peak inside a limit and references it. This is very useful for example if you need to reference automatically a large amount of metabonomic spectra, where the solvent peak could slightly change its shift with the pH of the sample.

Solvents >>

You can type the new value for that peak or you can click on the button to get a list of solvent chemical shifts.

	•			OK Cancel olvents <<
iolvent List <ul> <li>1H</li> </ul>	O 13C			or or the second
Name	Shift (ppm)	Multiplicity	J (Hz)	Desc 📤
Acetic Acid-d4	11.650	1		
	2.040	5	2.2	
Acetone-d6	2.050	5	2.2	
Acetonitrile-d3	1.940	5	2.5	
Benzene-d6	7.160	1		
e	107		1. <sub>1</sub> .	>

You can add new entries or edit the list of standard reference chemical shifts by using the buttons at the bottom of the dialog box.

### 9.1.1 Absolute Reference of x-Nuclei experiments

According to IUPAC, using a suitable secondary reference compound is no longer recommended. The unified scale is now the preferred method of referencing all spectra.

For example; in the past, the middle peak of the CDCl3 1:1:1 triplet at 77.0 ppm was often used to reference 13C-NMR spectra; but now the recommended method for 13C spectral referencing is the following:

1. Obtain a 1H spectrum of the same compound, and set 0 ppm using the TMS resonance.


- 2. Determine  $V_{TMS}^{obs}$  TMS from the 1H spectrum.
- 3. To determine the absolute frequency of the 0 ppm position in the 13C spectrum, use:

 $v_{C} = v_{TMS}^{obs} \frac{\Xi_{C}}{100}$ , where  $\Xi_{C} = 25.145020$ 

4. Finally use  $\nu_{\rm c}$  as shown below to reference the 13C spectrum.

Let's see how you can use the Absolute Reference in Mnova:

1st: Load into Mnova for example a 1H, 13C and HSQC experiments and reference the solvent in the 1H dataset:

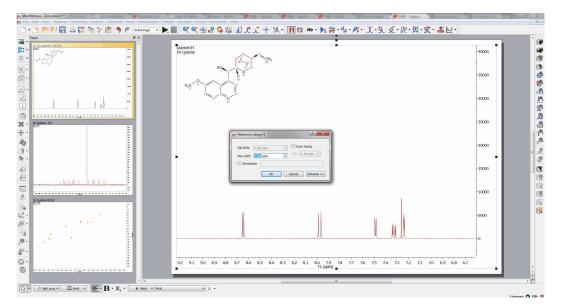

2nd: Click on the 'Absolute Reference' button of the toolbar  $\frac{5}{2}$  (or follow the menu 'Analysis/Absolute Reference') to display the applicable dialog box. Once there, select the 1H experiment as reference and check the boxes of the other experiments that you want to reference


Jse as Reference: Quinine1H: 399.972 MH	z ·
Spectra	Ξ
Quinine1H: 1H, 399.972 MHz 2D-HSQC-EDITED: Quinine HSQC	
📝 🕃 13C, 100.583 MHz	Ξ=25.145020 (Me4Si CDCI3, φ
🔽 🙀 1H, 399.971 MHz	Ξ=100.000000 (Me4Si CDCl3, φ
🔽 🕃 Quinine 13C: 13C, 100.582 MH	z Ξ=25.145020 (Me4Si CDCl3, φ
	= Values

If the document contains assignments, check the applicable box to update them.

The user can add any custom Xi value for any nucleus, using the "Xi values" table:

Absolute Reference		8 23	M E Values			8 23	
Jse as Reference:	SN0010378303.610.fid: 500	.453 MHz 🔹	Nucleus	E Value	Description		
Spectra		:	M 1H	100.000000	Description Me4Si CDCl3, φ = 1%	Ξ	
		E=100.000000 (Me4Si CDCI3, φ = 1%) E=25.145020 (Me4Si CDCI3, φ = 1%)	2H	15.350609	(CD3)4Si neat	MestReN	Nova 8
2D-COSY: SN001037 (1) 1H, 500.453		Ξ=100.000000 (Me4Si CDCl3, φ = 1%)	3H	106.663974	Me 4Si-t1	Nucleus	(й) IH
<ul> <li>IH, 500.453</li> <li>2D-HSQC-EDITED:</li> </ul>	MHz	Ξ=100.000000 (Me4Si CDCl3, φ = 1%)	3He	76.178976	He gas	Value	100.000000
V 313C, 125.85	MHz	Ξ=25.145020 (Me4Si CDCl3, φ = 1%)	6Li	14.716086	LiCI D20, 9.7 mol/kg	Description	Custom Value
🔽 🗎 1H, 500.453	MHz	Ξ=100.000000 (Me4Si CDCl3, φ = 1%)	7Li	38.863797	LiCI D2O, 9.7 mol/kg		OK Cancel
			9Be	14.051813	BeSO4 D2O, 0.43 mol/kg		1
		≣ ⊻alues	108	10.743658	BF3.Et20 CDCI3, φ = 15%		
Show in spectrum title	Show in parameters ta	ble Vpdate Assignments	118	32.083974	BF3.Et2O CDCI3, $\phi = 15\%$		
		Concer	G 130	25 144953	DSS methyl cignal D20	-	


Select 'Save Reference' from the 'Analysis/Reference' menu to save the Absolute Reference that you have applied:

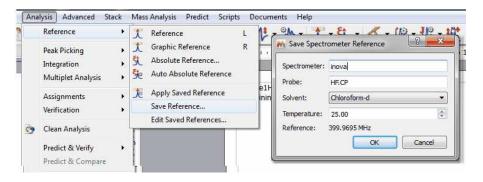

This will be useful for subsequent 1H spectra on the same spectrometer and in the same solvent. The user will be able to use this saved value to reference his/her 1H spectra. Since this value may change slowly with time, the user must be able to update the stored value at a later time (by selecting 'Edit Saved References'). By default the saved values will be valid for 30 days.

Date	Spectrometer	Probe	Solvent	Temperature	Reference (MHz)	
Thursday, 10 October 2013	av600	5 mm CPTCI1H-13C/15N Z-GRD Z44896/0009	DMSO-d6	300.00	600.12999	1
Tuesday, 3 September 2013	spect	5 mm CPTCI1H-13C/15N/D Z-GRD Z44896/0008	DMSO-d6	300,00	599.69951	
Tuesday, 13 August 2013	av700_33b193	5 mm CPTCI1H-13C/15N/D Z-GRD Z44908/0024	DMSO-d6	303.10	700.03001	
Tuesday, 6 August 2013	inova	5mmID	Methanol-d4	25.00	399.72814	

Selecting 'Auto Absolute Reference' will reference automatically the spectra (according to the know references from the list above):




Following the menu 'Edit/Preferences/NMR/Import', the user can select to automatically apply the known references when importing.


See also this blog post

### 9.1.2 Reference of 2D-NMR spectra with the 1D external trace


Press the 'R' key (or follow the menu 'Analysis/Reference/Graphic Reference') to activate the **Graphic Reference** feature. Next click on the peak that you want to reference and finally click again on the new chemical shift (matching with the peaks of the external traces):

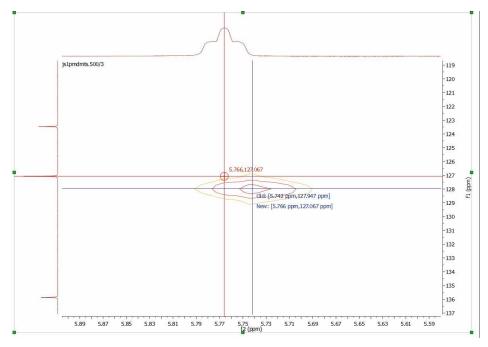

To apply an automatic referencing, right click over one of the traces and select 'Setup' to display the 'Setup Traces' dialog box. Once there click on the 'Use External 1H Trace as Reference' box':



Let's see how this feature work with a unreferenced HSQC spectrum (with a 1H and 13C datasets as <u>external traces</u>):

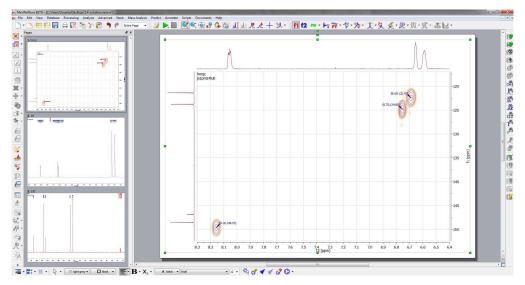


As you can see, this spectrum is not referenced. To apply an automatic referencing, just right click over one of the traces and select 'Setup' to display the 'Setup Traces' dialog box. Once there, check on the 'Use External 1H Trace as Reference' **box** (highlighted in red in the picture below):

vailable 1D Spectra:	V Horizontal Trace
🔒 1H js1pm24luti	1H
13C js1pm24luti	
	Internal Trace: 0
	Vertical Trace
	13C
	<ul><li>✓ ×</li><li></li></ul>
	Internal Trace: 0
	Vuse External 1H Trace as Reference


Automatically, you will obtain your HSQC spectrum referenced, as you can see in the screenshot



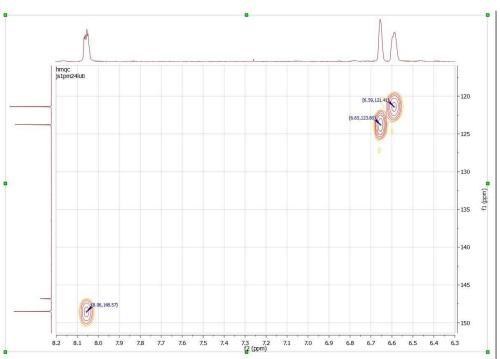

# 9.2 Peak Picking

**Mnova** implements a series of peak picking algorithms for 1D and 2D. These algorithms can be accessed via the menu item 'Analysis/Peak Picking' or via the scroll menu immediately to the right of the '**Peak Picking'** icon for the toolbar. This scroll menu will allow you to use **Automatic** Peak Picking, **Manual** Peak Picking (Manual Threshold), **Peak by Peak** Peak Picking, Move Peaks, Auto Classify Peaks (it will classify peaks as compound, impurity, solvent, artifact, etc by using the molecular structure of the document), create a new synthesized spectrum, to show or not show peaks on screen, to delete all peaks or delete peaks one by one, to set Peak Picking Options and to report the peak list, etc.

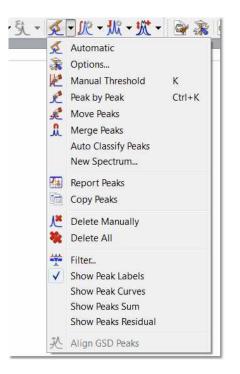


Move the peaks labels up and down just by clicking and dragging them.

#### **Automatic Peak Picking**

The Automatic Peak Picking option can be launched by simply clicking on the **'Peak Picking'** icon on the toolbar. This algorithm will peak all the peaks in the spectrum, and, by default, show **them** on screen with automatic recognition of the solvent lines. This algorithm can be applied indistinctively to both 1D and 2D spectra.


#### Example 1: 1D Peak Picking

This is a major change to Mnova NMR functionality. The default automatic Peak Picking algorithm is now based on **GSD**, rendering enhanced resolution, identification of overlapped peaks and also including autodetection of solvent and impurities (this algorithm is slower than the Standard, so if you are not interested in the deconvolution, you may prefer to use the Standard algorithm. See <u>options</u> below)

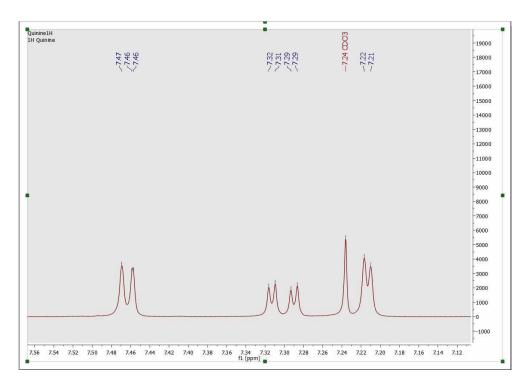


You can see above an example of the autoediting capabilities in the new algorithm, which automatically identifies solvents (as well as impurities, reference peaks, etc).

You can see below another example of the enhanced resolution achieved by the new Peak picking algorithm, now capable of identifying shoulders on large peaks as smaller peaks and of labelling and include them in multiplet analysis.

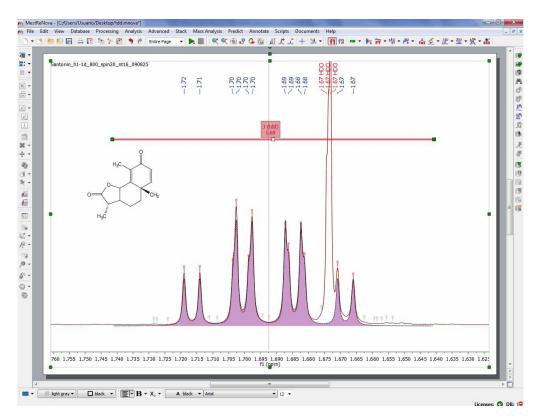


Peak curves are now active objects which can be interacted with, and three-way highlighting of peaks table, peak labels and the peak themselves has been implemented. For example, double cliking on any peak lable will display the 'Peaks Table', hovering the mouse over the peak label (or on any table) will highlight the peak in the spectrum and allow the user to interact directly with that peak. Clicking on any peak of the spectrum will automatically **scroll up/down the table** to the position of currently highlighted peak in the spectrum. **Right clicking** on any peak, will allow you to change the 'Peak **Type'** from the 'Peaks context' menu (and to set peak compound, use curve color, report, copy and delete peaks).

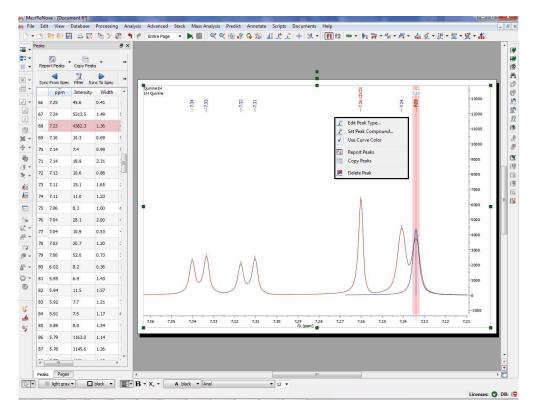

If your document contains more than one compounds, you will be able to select the applicable compound for each peak by right clicking on the peak label (or by selecting the peak(s) from the Peaks Table) and selecting 'Set Peak Compound':


Set Compound	2
Compound:	
EtOAc	
	OK Cancel

Example 2: 2D Peak Picking

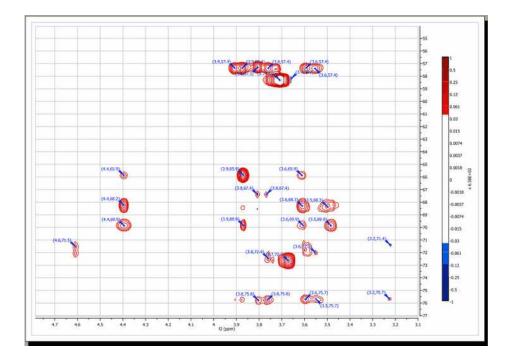

### Manual Threshold (shortcut: k)

Click and drag with the mouse to select the area to be picked

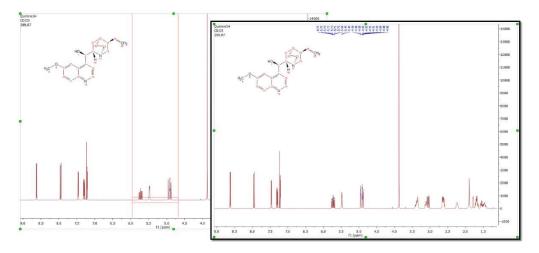


#### Peak by Peak (shortcut: Ctrl+k or Cmd+k in Mac)

Click on the peaks in the spectrum that you wish to identify and their chemical shifts will be marked on the spectrum. You will notice that the mouse cursor automatically *jumps* to the peaks maxima. To select a peak at an arbitrary position which is not a local extreme (e.g. the shoulder of a peak), press **SHIFT** key, move the mouse to the desired position and click.

#### Merge Peaks

Use this mode to merge more than one peak labels into a new one:

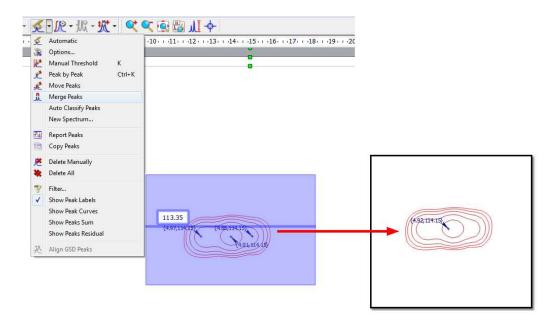

The peak list of a spectrum can be exported via File/Save As and selecting "Script: NMR 1D Peak List". It includes values of ppm and intensity for each peak. Follow the menu 'File/Save As/Script: NMR Peaks Table' to export the peaks in a table (only the fields set as 'Visible' in Setup Table get exported).

### 9.2.1 Peak Picking Options

Mnova has two Peak Picking algorithms: GSD (by default, with global spectral deconvolution and slower than the Std) and Standard (without deconvolution, faster than GSD).

#### **GSD Peak Picking options:**

The Peak Picking based on GSD (Global Spectral Deconvolution) will have these options:

Method:	GSD
Peaks Type	
Only Positive	
Settings	
Refinement Level	Optimized for Peaks:
Ref. 1 ( 2 fitting cycles )	Narrow
<u> </u>	Average
	Broad
Use Parallel Processing	Custom 1.00
Auto Classify	Impurities/Compounds
	Defaults

GSD has different operational levels, ranging from a very fast but inaccurate method to slower but much more accurate levels. In addition, GSD makes it possible the automatic recognition of solvent

peaks, impurities, etc. We recommend to use a GSD level of 1 (flash) or 2.

From this menu we can set the Refinement Level (number of cycles), the Resolution and the 'Auto Classify' of the GSD peaks. Clicking on the 'Defaults' button will restore the default settings from the registry.

The 'Refinement Level' will be the number of GSD fitting cycles applied over the spectrum. For example if you select 2 cycles, that means that the program will apply a GSD to your original spectrum and then another to the deconvoluted spectrum. GSD has different operational levels, ranging from a very fast but inaccurate method to slower but much more accurate levels. We recommend to use a GSD level of 1 (flash) or 2.

Resolution (Optimized for Peaks): GSD is sensitive to the line width of the signals. If a spectrum contains both narrow and broad lines, the algorithm could try to enhance the resolution of the sharp lines, but the negative side effect would be a potential removal of the broad lines. Likewise, if we want the keep the broad lines, the resolution power of GSD should have to be reduced.

'Auto Classify': the program will try to identify the type of each signal of the spectrum (compound, solvent, impurity, etc). This information will appear in the 'Type' column of the Peaks table. This feature should be used only with GSD (and not with the Standard method).

#### Standard Peak Picking options:


This algorithm is much faster than GSD, but it does not include deconvolution.

h Peak Picking Options	? <mark>.</mark>			
Method:	Standard 💌			
Peak Picking Options				
Noise Factor:	10.00			
Peaks <u>T</u> ype:	Positive and Negative 💌			
Sensitivity:	10.00			
Maximum Number of Peaks	1000			
Vse Parabolic Interpola	tion			
Auto Classify	[Impurities/Compounds]			
WARNING: Peaks a not be used with Standa GSD method instead to a Interactive	rd method. Please, use			
E fueracave				
	OK Cancel			

A series of options can be controlled on the 'Peak Picking Options' dialog box, which can be accessed via the Peak Picking scroll menu. The user can choose the 'Noise Factor' (intensity threshold) and the 'peaks type'. Clicking on the 'Advanced' button, you will be able to change the 'sensitivity' factor (the higher the value, the less peaks will be picked), maximum number of peaks, whether to 'use parabolic interpolation', merging options for 2D multiplets. All these options can be evaluated interactively, so that their results can be viewed on screen in **real time**, by making sure the **'Interactive'** box is selected.


- **Sensitivity:** it is basically a kind of smoothing parameter. For example, in noisy spectra, large values of this parameter will smooth the spectrum in the background so that less peaks will be detected. By default, this value will be 1 which means that the program will try to find the maximum number of peaks in the spectrum. This is the recommended value for routine 1D spectra.

The sensitivity factor is indeed being used by the program and its main application is to avoid the detection of too many peaks in noise spectra. As we said above, this option can be considered as a smoothing parameter which is somehow applied before the peak picking algorithm is applied. For instance, if you have a very noise peak with a lot of local extrema caused by the random fluctuations of the noise, the peak picking algorithm could find just too many peaks which do not correspond to real peaks, just noise local maxima/minima. In order to avoid that situation, the sensitivity factor can be increased in such a way that the peak is smoothed on the fly and ideally, only the real peak would be detected.

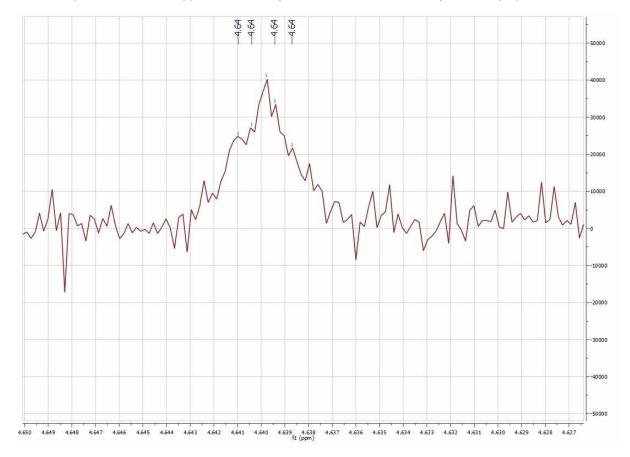



For example, this is what happens with a very low value for the sensitivity in a noisy spectrum:

And this is the result when a higher value is used:

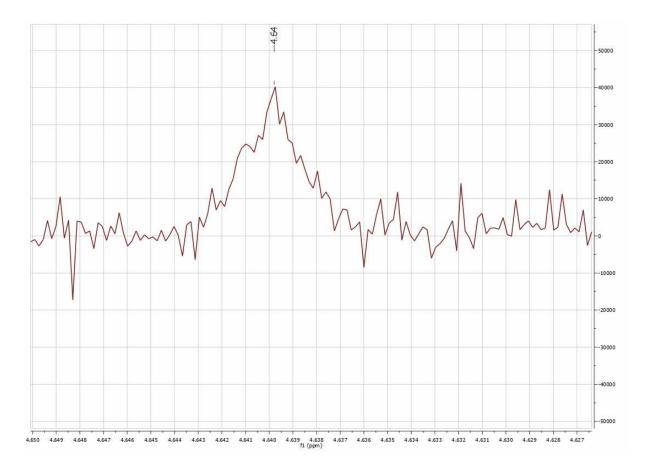

It is shown below, how this sensitivity factor is being used by the program by opening a 1H-NMR spectrum of strychnine. First you will see the result with sensitivity = 1 (BTW, it's important to realize that the sensitivity factor can be lower than 1. The lower the value, the higher the resolving power of the algorithm):

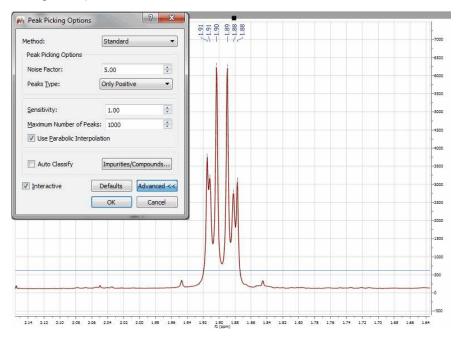


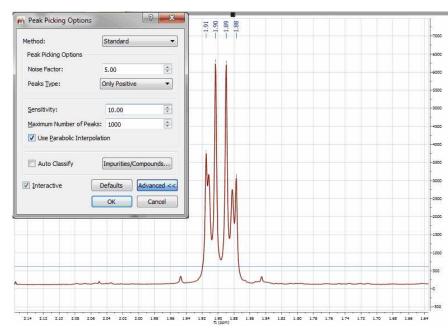

So you can appreciate that with sensitivity =1 all peaks have been detected. Now let's increase the value to 10. This is the result:


You can see that only 4 peaks have been detected whilst 2 less resolved peaks are missing now.

- **Noise Factor:** it is a kind of intensity threshold. The program will automatically calculate the noise value of the spectrum. This noise value is then multiplied by the noise factor. After running the peak picking algorithm, peaks smaller than the noise value multiplied by the noise factor will be rejected. The program shows this vertical threshold as two horizontal lines in the spectrum, as you can see in the picture below:

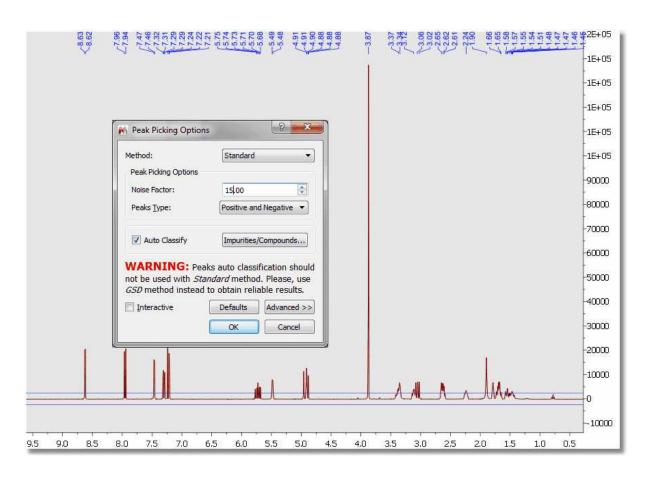


### **Manual Peak Picking**

The Manual Peak Picking option allows the user to set an area of the spectrum where the software will carry out the Peak Picking, by simply left clicking and dragging the mouse over the area.

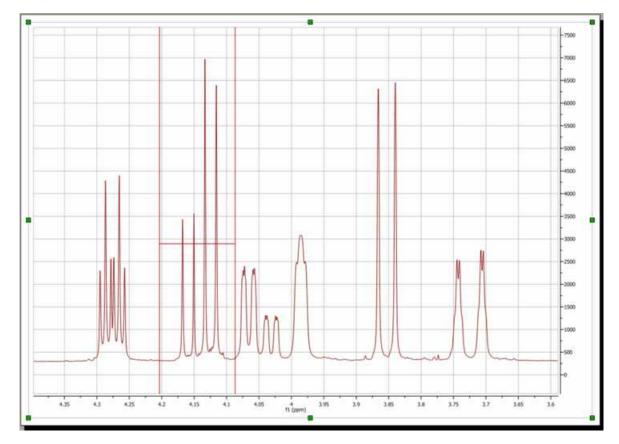


This will generate a bucket, and all peaks with chemical shifts between the left and right hand sides of the bucket and with intensities above the bottom of the bucket will be picked.

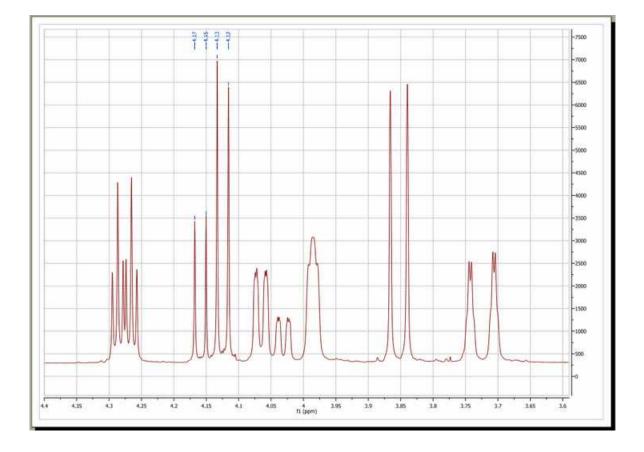


### Peak by Peak

The Peak by Peak option will allow you to hover the mouse over specific peaks of interest and to only select those for the peak picking output, by just left clicking on each one at a time. The procedure is very simple: just point to the peak you want to pick so that it is highlighted and then left click on the mouse.

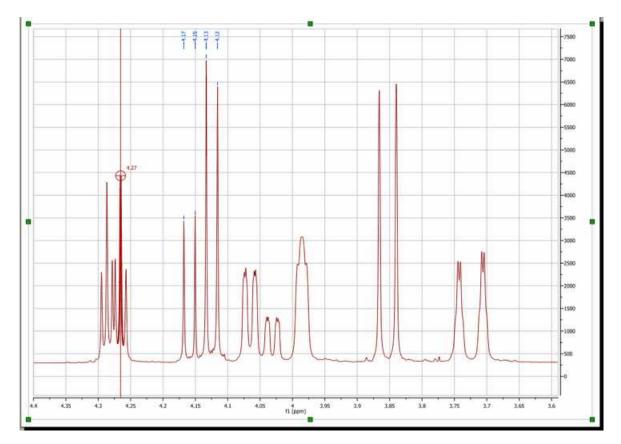


Note that, by default, Mnova will find the peak top by using parabolic interpolation. To pick a peak at an arbitrary position (e.g. not at a local extreme), press <Shift> and click.

Mnova also allows the user to **move a peak label** to a new location, by using the 'Move Peaks' tool under the Peak Picking scroll down menu.



**Note**: When a peak is moved its Annotation information remains unchanged, although other info such as peak widths and intensities are updated.

**Merge peaks** (very useful for 2D) just by selecting the applicable option in the Peak Picking scroll down menu and clicking and dragging on your spectrum:

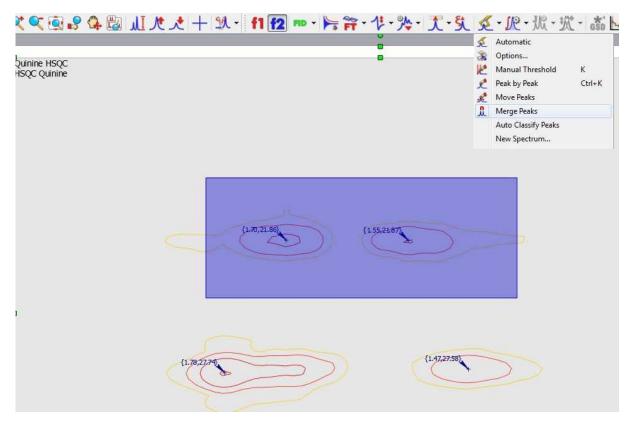

Once you have finished with the 'Peak Picking', select the 'Report' option in the Peak Picking scroll down menu.



Select 'Copy Peaks' in the scroll down menu to copy the report to the clipboard.

Choose the peak report template for the 'Peak List' just by selecting 'Setup' in the 'Report Special' scroll down menu of the 'Peaks Table'.

#### **Filter Peaks**

You can apply some filters (to show for example only Compounds Peaks) from the Peak Picking scroll down menu (or from the Peaks table). If the spectrum contains peaks belonging to more than one compound, you can show only the peaks assigned to one of them:


Including: All   Excluding: None  Peaks Assigned To:  None EtOAc Outprine	Filter	
Peaks Assigned To:  None EtOAc	Including:	Ali 🔻
None EtOAc	Excluding:	None 🔻
Quinne	EtOAc Quinine	

You can also synchronize the type of the peaks in the <u>table</u> (i.e. only Compounds peaks) with the peaks showed in the spectrum (by using the button 'Sync from Item') or viceversa, to synchronize the spectrum peaks with the peaks showed in the table ('Sync to Item' button).

#### 9.2.1.1 Impurities Auto detection

This novel algorithm will be used to detect the solvents as impurities in your samples. Please bear in mind that this is the first version and will be improved in the oncoming versions of the software.

The first version of the algorithm will detect MeOH, EtOH, iPrOH and EtOAc in deuterated DMSO. Here you can see an example containing several solvents.

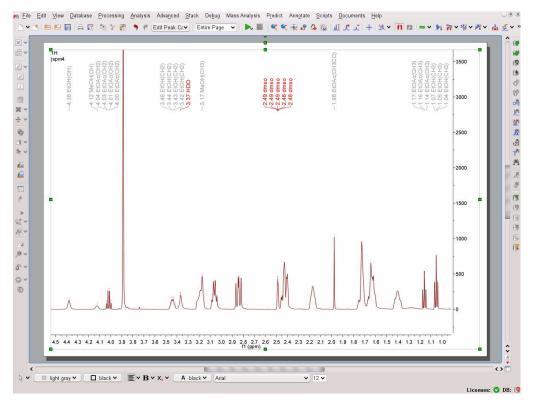


In the Peak Picking options, you will be able to select what solvents you want to be detected and you will be able to edit this table and to include additional solvents:


Enabled	Label	Description	Nucleus	Solvent	Priority	Multiplets	Peaks
<b>7</b>	iPrOH	Isopropanol (Form 1: Resolved CH2-OH coupling)	1H	DMSO-d6	0	4	18
<b>V</b>	iPrOH	Isopropanol (Form 0: no CH2-OH coupling)	1H	DMSO-d6	0	3	10
7	EtOH	Ethanol	1H	DMSO-d6	0	3	8
7	EtOAc	Ethyl Acetate	1H	DMSO-d6	0	3	8
V	MeOH	Methanol	1H	DMSO-d6	0	2	2

Clicking on the Advanced button, will allow you to add further impurities or to edit the existing ones:

	E	kport			Im Im	port				D	efault			*	Clear
npurities															
Enabled	Label	()		Desc	ription			Nucleu	is So	lvent	Priority	Multi	plets I	eaks	Add
1	iPrOH	Isopro	opanol	(Form 1: Re	solved CH2-	OH coupl	ing)	1H	DN	ISO-d6	0	4		18	X Delete
~	iPrOH	Isopro	opanol	(Form 0: no	CH2-OH co	oupling)		1H	DN	ISO-d6	0	3		10	
<b>v</b>	EtOH	Ethan	ol					1H	DN	ISO-d6	0	3		8	
1	EtOAc	Ethyl	Acetat	e				1H	DN	ISO-d6	0	3		8	
<b>v</b>	MeOH	Meth	anol					1H	DN	ISO-d6	0	2		2	
ultiplets															
	ahel N	Peaks	Shift	Shift Min	Shift May	Weight	ä	Delta	Flags	Sat W	leight l	Sat S	at Shif	t Hetero Inde	ex Add
		1	3.16	3.06	3.26	3	0	1	No	0.0	-	0	0	0	2 Delete
2 (	ЮН	1	4.01	3	5	1	0	0	No	(	)	0	0	0	

For example let's add CH3CN as a new solvent impurity. As CH3CN only has one multiplet visible in the 1H spectrum (the Me group), you can enter for the label CH3 and 1 for the number of peaks (Npeaks). For the base chemical shift, we have used a value of 2.08 and a minimum and maximum shift values of 2.04 and 2.10 respectively. This is the interval in which the CH3 resonance will be searched for.

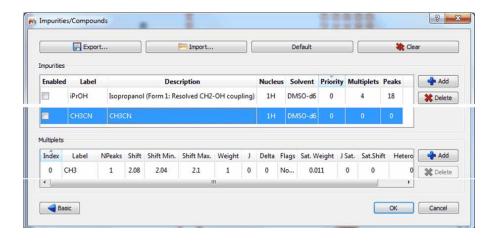

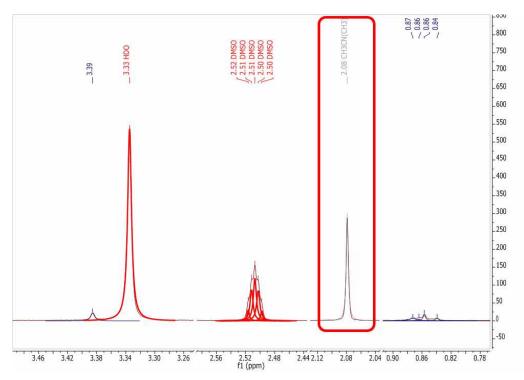

This is it! Now, when a Pick Picking with Auto Classify option enabled will be run, the CH3CN peak will be automatically detected, as illustrated in the spectrum below:

## 9.2.2 GSD (Global Spectral Deconvolution)

1H NMR is for sure the most powerful technique for structure elucidation, especially for small organic molecules. Typically, an organic chemist uses the chemical shift, coupling constants and integration information contained in an 1H-NMR spectrum to either verify or elucidate an unknown compound. Of course, it's quite common that a simple 1H-NMR spectrum is not enough to unambiguously confirm a structure and thus other NMR experiments (e.g. 13C-NMR, HSQC, COSY, etc) are used to get more structural information.

Nevertheless, we have often found that many organic chemists do not always try to get the most out of 1H-NMR spectra (which is the cheapest experiment), in particular when some multiplets are complex to interpret (due to the strong coupling) or when peaks overlap prevents valuable information to be detected in some multiplets.


As it is well known, there are two principal factors limiting the resolution power in a spectrum. First, we have the natural line width limitation imposed by the T2 (spin-spin relaxation). For example, if T2 is about 1 second, the peak linewidth at half height cannot be less than 0.32 Hz (remember, line width at half height = 1 / (pi \* T2) = 1 / 3.1415 = 0.32) no matter how powerful is our NMR instrument or the field homogeneity. On the other hand, there are instrumental shortcomings (e.g. spatial uniformity of the applied magnetic field, etc).

Nonetheless, there is an additional limiting factor, and whose importance is generally underestimated which has to do with the generally large number of transitions in 1H-NMR spectra. In short, the peaks we can observe in a 1H-NMR are just a small fraction of the actual transition resonances which are not observable because of the limited digital resolution. In fact, every peak in an 1H-NMR spectrum is basically an envelope of a large number of transitions and its shape is dominated by the coupling pattern of the spin system. Even in molecules of modest size the number of distinct peaks is tens to thousands times smaller than that of quantum transitions.

These problems have been the motivation of the development of a brand new peak analysis algorithm,

the so-called GSD (Global Spectral Deconvolution); which applies automatically a deconvolution of the whole spectrum in a few seconds and does not require that the user set a starting point for the fitting of each multiplet.

Let's see the GSD in action. Just open a 1H-NMR spectrum:

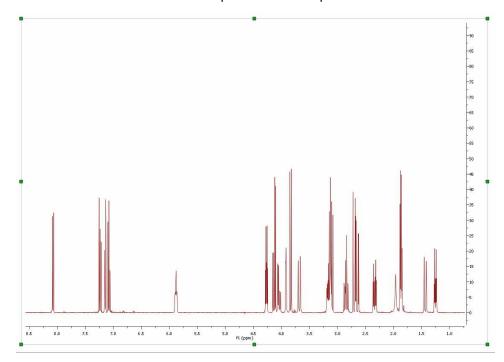


Select GSD as the Peak Picking method (in the Peak Picking Options) and apply a Peak Picking which will to carry out the deconvolution of the whole spectrum. See also: "Using GSD for multiplets analysis"


Nethod:	GSD
Peaks Type	
Only Positive	
Settings	
Refinement Level	Optimized for Peaks:
Ref. 1 ( 2 fitting cycles )	Narrow
<u>, i i j i i i</u>	Average
	🔘 Broad
Use Parallel Processing	🔘 Custom 1.00 🐳
24 mil 1	
V Auto Classify	Impurities/Compounds
	Defaults
	OK Cancel

Automatic multiplet deconvolution will be applied to the whole spectrum without asking the user to select multiplets, specify number of lines and their approximate locations, etc ... Everything is

automatic! (Ideally, data would be zero filled to 64K points and line broadening functions would not be used.).

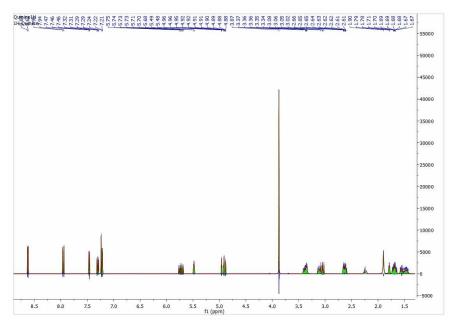

Let's expand an area to see how the algorithm works:

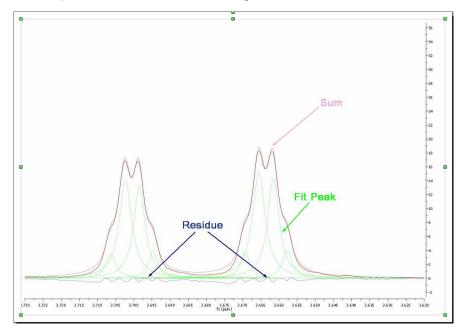


As you can see in the picture above you will obtain a green line to show the fit peaks, a blue line to show the residue and red line to show the sum.


It's very important to realize that the result of GSD is just a list of peaks, but each peak is fully characterized (chemical shift, Peak Width, Height, Phase, Area, etc). To see the list of the GSD peaks just follow the menu 'View/Tables/Peaks' (or right click on any toolbar and select 'Tables/Peaks'):

Rep	ort Peaks	Copy Pea		Report -	.) Delete Se	lect Peaks		
Syn	C From Spec	Filter Sy	/nc To Spec	犬 Set Flags	L Set Compou	ind New Spe		
	ppm	Hz	Intensity	Width	Area	Туре	Flags	*
1	8.85	3539.1	29.2	1.32	294.19	Compound	Weak + C13_Sat	
2	8.84	3534.6	29.3	1.22	270.32	Compound	Weak + C13_Sat	
3	8.78	3512.9	21.9	0.92	153.96	Impurity	Weak	
4	8.77	3508.4	23.6	0.85	162.98	Impurity	Weak	
5	8.64	3456.9	40.6	1.42	500.00	Compound	Weak	
6	8.64	3455.5	28.4	0.19	48,33	Compound	Weak	
7	8.64	3454.5	37.3	3.14	955. <u>5</u> 6	Compound	Weak	
8	8.63	3451.0	6203.9	1.00	46415.96	Compound	None	
9	8.62	3446.6	6622.7	0.82	44958.30	Compound	None	
10	8.60	3440.5	27.3	0.91	147.13	Compound	Weak	
11	8.52	3406.5	7.0	0.86	46.67	Impurity	Weak	
12	8.40	3361.2	26.8	1.32	252,49	Compound	Weak + C13 Sat	

This table contains information about the chemical shift, width, height, Area, Type and Flags. Select 'Auto Classify Peaks' in the Peak Picking scroll down menu to edit automatically the Type and Flags of each signal:




Follow the menu 'Scripts/Export ASCII/GSD Spectra' to export the GSD peaks as ASCII.

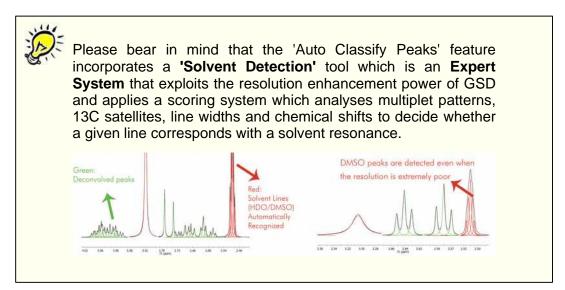


You can display the 1D spectrum with 'All Peaks' (default view) and also to decompose the spectrum into 3-sub-spectra:

- 1. Containing only the 'compound peaks'.
- 2. Containing only 'solvent+impurity' peaks.
- 3. A stack plot with the different views (all, compounds and solvent+impurities):




Here you can find an example of the stacked sub-spectra view obtained from a 1H-NMR spectrum:

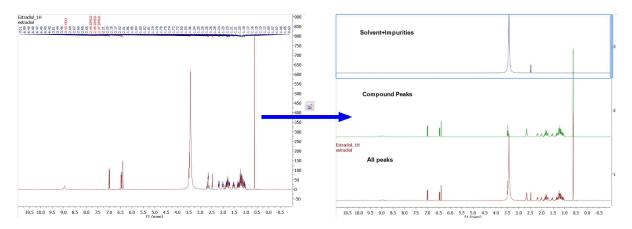

Double click on the applicable cell (or on the 'Set Flags' button) to manually edit the 'Type' and the 'Flags' table. To change the flag to several peaks at the same time just hold down the Ctrl/Cmd key and click.

	oort Peaks	Copy Pea	~	145				
Syn	The From Spec	Filter S	ync To Spec	K Set Flags	Set Compo	und New Spect	trum	
	ppm	Hz	Intensity	Width	Area	Туре	Flags	
1	8.85	3539.1	29.2	1.32	294.19	Compound 🔻	Weak + C13_Sat	2
2	8.84	3534.6	29.3	1,22	270.32	Compound	Weak + C13_Sat	
3	8.78	3512.9	21.9	0.92	153.96	Impurity Solvent CS Reference	Weak	
4	8.77	3508.4	23.6	0.85	162.98	Quantrence	Weak	
5	8.64	3456.9	40.6	1.42	500.00	Compound	Weak	
6	8.64	3455.5	28,4	0.19	48.33	Compound	Weak	

Once you have edited your GSD spectrum, you can generate a new spectrum with the fit peaks, just by selecting 'New Spectrum' in the Peak Picking scroll down menu:




This will display a dialog box from where you will be able to select the mode of the new spectrum (Synthetic, Sticks, Uniform Line Width or Proportional Line Width). From here you can also excludes the peaks with a specific 'Type or Flag' and you can get the spectrum a new item or stacked with the original one.


We will generate a new spectrum with a proportional Line Width of 0.3, including only the peaks marked as compound (without artifacts, solvents, impurities, etc.)

Mode	
Proportional Line Wi	dth 🔻
f1 Line Width <mark>f</mark> actor:	0.30
Options	
Including: Comp	ound 🔻
Excluding: Defau	lt 👻
Output	
New Item	
Stack in current i	tem

Here is the result of the New spectrum from GSD:

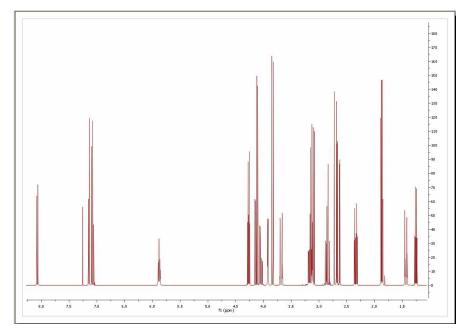

You will see in the picture below an expanded region of the original spectrum and the GSD one in stacked one. As you can see, now you will be able to measure the coupling constants more accurately, as only the compound peaks are displayed and they are displayed at an artificially increased higher resolution

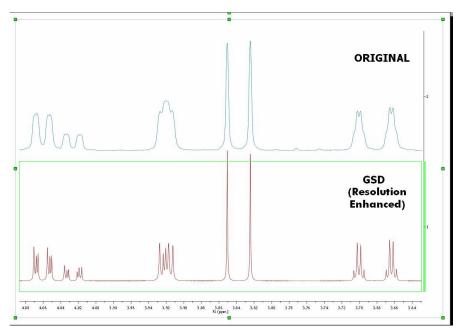


## Improving GSD with Line Fitting

After the GSD peak picking, allow the user to define a line fitting region, and it uses all the GSD-peaks in that region as the starting peaks. The user changes the peaks and then re-fit the peaks as usual,


until satisfied. The Peaks table gets automatically updated every time a peak is modified in the Line Fitting panel.

#### 9.2.2.1 What else can I do with GSD?


As you have seen above, from the GSD list of peaks you could create a mocked spectrum with enhanced resolution; but in addition you can use GSD for example to **remove solvent lines**. Consider the following spectrum containing solvent peaks (DMSO/Water):

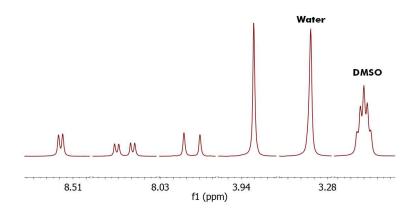


To remove the undesired peaks, just run a Peak Picking with GSD and with the 'Auto Classify Peaks' option enabled, in order to autodetect the solvent peaks (in yellow in the figure below):

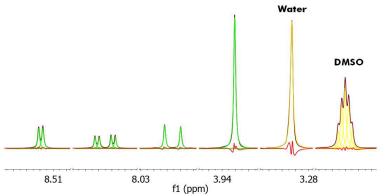

And finally we create a new synthetic spectrum *without* the solvent lines:

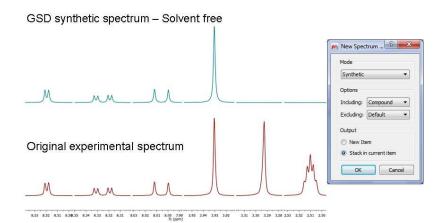


Here you can see another example where the solvent and compound signals are overlapped. Mnova's autoedit successfully separates a triplet signal sitting on the HDO signal. The approach of generating dark regions used by other software products would miss the triplet at 3.5 ppm and therefore any verification efforts would fail.

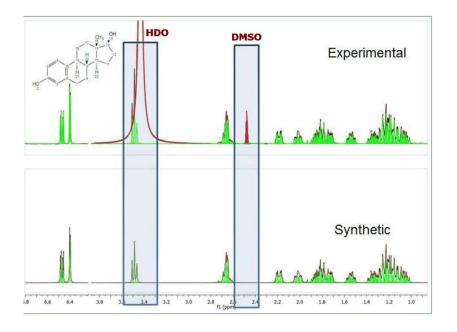


You can display the 1D spectrum with 'All Peaks' (default view) and also to decompose the spectrum into 3-sub-spectra:

- 1. Containing only the 'compound peaks'.
- 2. Containing only 'solvent+impurity' peaks.
- 3. A stack plot with the different views (all, compounds and solvent+impurities):



Here you can find an example of the stacked sub-spectra view obtained from a 1H-NMR spectrum:

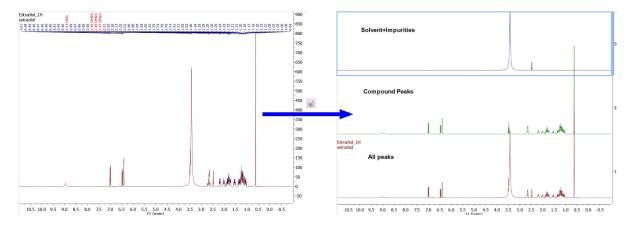

### 9.2.3 Peaks Table and Reports

**Peak Table:** The user will obtain the peak table by following the menu 'View/Tables/Peaks'. Clicking on any peak of the spectrum will automatically scroll up/down the table to the position of currently highlighted peak in the spectrum,

Please note that **hovering** the mouse over the peak label will **highlight** the applicable **peak** shape in the spectrum. The same effect you will obtain if you hover the applicable cell in the Peaks Table. Double clicking on a row in Peaks table will *zoom in* that peak in the spectrum. Move the peaks labels up and down just by clicking and dragging them.

Rep	ort Peaks	Copy Pea		Report 🔻	Delete Se	lect Peaks		
Syn	c From Spec	Filter St	ync To Spec	犬 Set Flags	Compou	und New Spe		
	ppm	Hz	Intensity	Width	Area	Туре	Flags	1
1	8.85	3539.1	29.2	1.32	294.19	Compound	Weak + C13_Sat	-
2	8.84	3534.6	29.3	1.22	270.32	Compound	Weak + C13_Sat	
3	8.78	3512.9	21.9	0.92	153.96	Impurity	Weak	
4	8.77	3508.4	23.6	0.85	162.98	Impurity	Weak	
5	8.64	3456.9	40.6	1.42	500.00	Compound	Weak	
6	8.64	3455.5	28.4	0.19	48,33	Compound	Weak	
7	8.64	3454.5	37.3	3.14	955. <u>5</u> 6	Compound	Weak	
8	8.63	3451.0	6203.9	1.00	46415.96	Compound	None	
9	8.62	3446.6	6622.7	0.82	44958.30	Compound	None	
10	8.60	3440.5	27.3	0.91	147.13	Compound	Weak	
11	8.52	3406.5	7.0	0.86	46.67	Impurity	Weak	
12	8,40	3361.2	26.8	1.32	252,49	Compound	Weak + C13 Sat	

The Peaks table displays the list of peaks, including the following information: chemical shift in ppm and Hz, Intensity (height), Width (in Hz, at half maximum of the peak), Type (compound, solvent, impurity, etc), Flags, Multiplicity (for the carbons) and 'Annotations'.

The user can report the Peak table directly on the spectrum by clicking on the **'Report Table'** icon under the 'Report Text' scroll down menu. To delete an undesired peak, click on the **'Delete'** icon of the Peak List, or select 'Delete Manually' on the Peak Picking scroll bar icon:


2	⑦伬・Ⅲ・斑・	
R	Automatic	
*	Options	
10.3	Manual Threshold	К
J.	Peak by Peak	Ctrl+K
	Move Peaks	
	Auto Classify Peaks	
	New Spectrum	
2	Report Peaks	
	Copy Peaks	
×	Delete Manually	
*	Delete All	
•	Show Peaks	
永	Align GSD Peaks	

By default, peak frequencies are listed directly on the spectrum but they can also be accessed via the *Peak Picking table* and also as a **'Peak List'** by clicking on the **'Report Peaks'** icon. The user will be able to select the 'Peak Report' Template between several journal formats by selecting 'Setup Report' in the 'Peaks table'.

R	eport Peaks	<ul> <li>Copy Peak</li> </ul>	s Setu	ip Report	· /	ct Peaks		Setup Peak Report
S	ync From Spe	ec Filter S	ync To Spe	c Set Flag	ی s Set Compour	nd New Spectrun	n	JACS  Ascending order shifts
10 39	0), 44.19 (d 9.38 (d, 9),	, 19), 43.48	3 (s, 15), 7), 30.54	40.73, 40.	52, 40.3 <mark>1, 4</mark> 0.	0.75 (d, 13), 50.2 10, 39.89, 39.68 51 (t, 8), 26.76 (t	, 39.47,	Only report compound peaks  C Report 13C assignments  Report 13C multiplicity
	ppm	Intensity	Width	Area	Туре	Flags	'ity/Com	
1	218.04	7.2	1.93	49.91	Artifact	None		2D
+			1.31	481.51	Compound	None		Report as points
_	155.50	90.1	1.31					
2	155.50 137.81	90.1 88.1	1.08	368.83	Compound	None		Report f1
2				368.83 396.33	Compound Compound	None None		Report f2
2 3 4	137.81 131.15	88.1	1.08	2.0 PC 025		100000		Report f2
2 3	137.81 131.15	88.1 74.8	1.08 1.26	396.33	Compound	None		


From here you can select the order of the report (ascending or descending), the option to only report the compounds peaks, to report the 13C assignment and to select the number of decimals. For 2D experiments, you will have the choice to report a list of F1, F2 peaks or both. This option will be remembered when creating a reporting template.

After making assignments to the 13C peaks the multiplicity gets automatically filled in Peaks table. This multiplicity information can be included in the Peaks Report by selecting it in Setup Report.

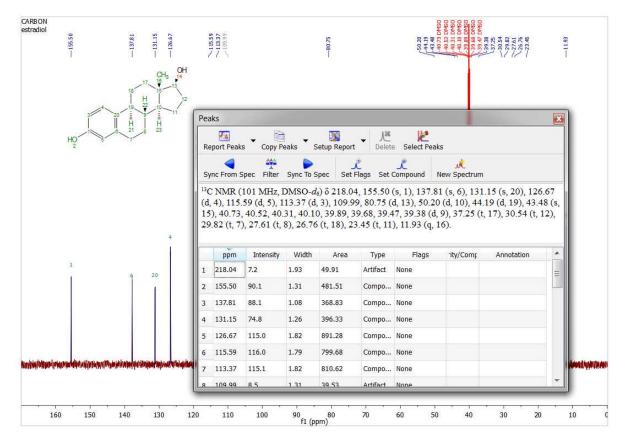

The user will be able to copy the 'Peak List' report to the clipboard by selecting 'Copy Peaks' on the

'Peaks Table'.



The peak list can also be exported as an ASCII file by following the menu 'File/Save as' and selecting Script: NMR 1D Peak List (\*.csv, \*.txt):


	is documentos 🕨 (				- 44	Buscar Assignments	
Organizar 🔹 N	lueva carpeta					⊟ <b>•</b>	(
	*	Nombre	*	Fecha de modifica	Tipo	Tamaño	
			Ningún	elemento coincide con el criteri	o de búsq	ueda.	
	=						
UULSE	+						
	codeine_ManualAssigned.cs	/					
Nombre		v * tut)					
	Script: NMR 1D Peak List (*.cs						
	Script: NMR 1D Peak List (*.cs Script: Assignments (*.txt) Script: Multiplet Integral Serie Script: NMR 1D Custom CSV	is (*.bit)					

You can export NMR spectra via 'File/Save As/NMR Custom CSV File' with options to export PPM+Re+Im, Hz+Re, PPM+Re or Hz+Re+Im, either from right to left or from left to right.


	The second se	(14) (14) (14) (14) (14) (14) (14) (14)	
Format:	{ppm}{tab}{real}{t	ab}{imag}	*
Decimal Places:	-	Expected	column name
Decimal Places:	6		z], (pts), (real
			pe (tab) for

Follow the menu 'File/Save As/Script: NMR Peaks Table' to export the peaks in a table (only the fields set as 'Visible' in 'Setup Table' will be exported).

To copy&paste the peaks from one spectrum to another, just press 'Ctrl/Cmd+C' in the original spectrum and then follow the menu 'Edit/Paste Properties/Paste NMR Peaks in the other spectrum (or spectra, if you have previously selected them in the page navigator):



If your document contains more than one compounds, you will be able to select the compound for each peak from the Peaks Table (by clicking on the 'Set Compound' button or by double clicking on the 'Impurity/Compound' cell). The same effect will be obtained by right clicking on the Peak label and selecting 'Set Peak Compound':

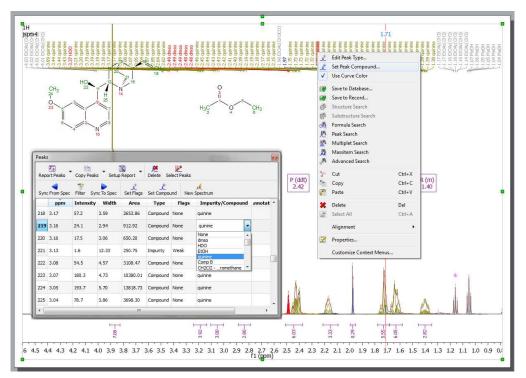


You can apply some filters to show for example only Compounds Peaks. If the spectrum contains peaks belonging to more than one compound, you can show only the peaks assigned to one of them (by using the 'Filter' button):

Rep	ort Peaks	Copy Pe	aks Setu	p Report	)) Delete Se	lect Peaks		
Syno	From Spe	Filter S	Sync To Spec	<del>گر</del> Set Flags	Set Compou	und New	,) Spectrum	
	ppm	Intensity	/ Width	Area	Туре	Flags	Impurity/Compound	11
339	M Pea	ks Filter	+48	8 8	×rity	Weak		
340	Filte	r			irity	Weak		
341	Ind	uding:	All	•	] arity	Weak		
342	Exd	uding:	None	•	] rity	Weak		
343		Peaks Assig	gned To:		rity	Weak		
344	1	None EtOAc			irity	Weak		
345		Quinine	ŝ		arity	Weak		
346					rity	Weak		
347			ОК	Cancel	pound	Weak + C13_Sat		
348	1.17	131.4	1.19	2019/03	Compound	None	EtOAc	
349	1.17	80.5	1.25	1191.49	Compound	None	EtOAc	
350	1.16	268.5	1.15	4274.61	Compound	None	EtOAc	
351	1.16	159,3	1.23	2448.77	Compound	None	EtOAc	
252	1.15	4.0	0.21	10.49	Impurity	Weak		

You can synchronize the type of the peaks in the table (i.e: only Compounds peaks) with the peaks showed in the spectrum (by using the button 'Sync from Item') or viceversa, synchronize the spectrum peaks with the peaks showed in the table ('Sync to Item' button).

M.

The 'New spectrum' button New Spectrum' will generate a synthetic spectrum from the selected peaks in the table or for all the peaks shown in the table if there is no selection. Here you can see an example, showing a mixture of two compounds on top and the synthetic spectra (geenrated with the 'New Spectrum' feature) of each compound at the bottom:

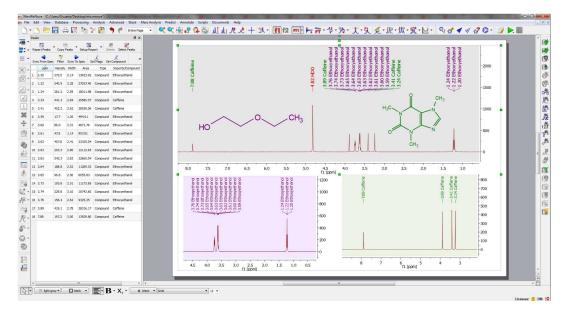

Select 'Auto Classify Peaks' in the Peak Picking scroll down menu to edit automatically the Type and Flags of each signal:

\$	Automatic	
R	Options	
12ª	Manual Threshold	к
P.ª	Peak by Peak	Ctrl+K
3ª	Move Peaks	
	Auto Classify Peaks	
	New Spectrum	
6	Report Peaks	
h	Copy Peaks	


You can also manually edit the 'Type' and the 'Flags' table just by double clicking on the applicable cell:

	4	-		P	P			
Syn	nc From Spec	Filter S	nc To Spec	Set Flags	Set Compo		rum	
	ppm	Hz	Intensity	Width	Area	Туре	Flags	
1	8.85	3539.1	29.2	1.32	294.19	Compound -	Weak + C13_Sat	
2	8.84	3534.6	29.3	1.22	270.32	Compound	Weak + C13_Sat	
3	8.78	3512.9	21.9	0.92	153.96	Impurity Solvent CS Reference	Weak	
4	8.77	3508.4	23.6	0.85	162.98	Quantrence	Weak	
5	8.64	3456.9	40.6	1.42	500.00	Compound	Weak	
6	8.64	3455.5	28,4	0,19	48.33	Compound	Weak	

You can also select several cells and click on the 'Set Flags' button to change the Type or the Flags of several peaks at the same time:

Re	port Peaks	Copy P	eaks Setu	Report -	Delete S	elect Peaks	
Sy	nc From Spe	Tilter	Sync To Spec	犬 Set Flags	犬 Set Compo		<del>)(</del> ipectrum
_	ppm	Hz	Intensity	Width	Area	Туре	1
1	8.63	3451.0	5611.9	1.15	52127.17	Compound	Non
2	8.62	3446.5	5678.3	1.13	51807.32	Compound	Non
3	7.96	3185.3	M GSD Peak	r Flags	1911.00	8	× n
4	7.94	3176.1	Peak			ОК	- 0
5	7.47	2987.5	V Type:	Compou	und 🔻	Cancel	n
6	7.46	2982.9	V Flags:	None	•	L	
-	7 22	2025 2	1			-11	

Right click on any peak and select 'Edit Peak Type' to change the Peak type:

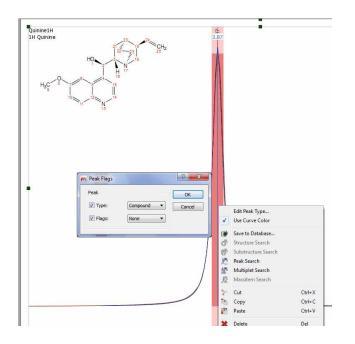

The user will be able to highlight in the table any desired peak just by clicking on the 'Select Peaks' button and then selecting the peaks in the spectrum (by clicking and dragging). Those peaks will be highlighted in the table and the user will be able to modified their flags (or Type) by clicking on the 'Set Flags' button. In the example below, we have changed the type of two peaks (from compound to impurity):

Rep	ort Peaks	Copy Peak		Report	Nelete Se	Nelect Peaks			
Syna	From Spec	Tilter Syr	C To Spec	犬 Set Flags	L Set Compo		elect Peaks Spectrum		
	ppm	Intensity	Width	Area	Туре	Flags	rity/Comj	*	
131	5.68	690.8	1.23	12966.51	Compound				
132	5.55	3.0	1.73	83.72	Compound	Weak + C13_Sat			
133	5.54	5.6	2.21	179.35	Compound	Weak + C13_Sat			
134	5.49	1004.9	4.22	62045.74	Impurity	None			
135						None			
136	5.30	6.3	10.66	932.44	Impurity	Weak			
137	5.15	8.0	1.69	223.08	Impurity	Weak			
138	5.14	3.3	0.74	37.02	Impurity	Weak			
139	5.10	12.8	2.64	505.30	Impurity	Weak			
•			u.	1			,		

You can customize the appearance of the table by clicking on the 'Setup Table' button:

Rep	Paks	Copy Peak	s * Setur	Report	)進 Delete Se	Hect P	Customize Table - Peak	3								100				2
	4	59		Setup Rep				ppm	Hz	Intensity	Width	Area	Туре	Flags	Max/Min	Multiplicity	J(CH)	Kurtosis	Impurity/Compound	Annotation
Syn	c From Spec	Filter Sy	nc T 🙀	Setup Table	e	nd	Visible Name	ppm	Hz	Intensity	Width	Area	Туре	Flags	Max/Min	Multiplicity	J(CH)	Kurtosis	Impurity/Compou	Annotation
	ppm	Intensity	Width	Area	Туре	F	Visible	1		V	V	7	1	2		8	8	1	<b>V</b>	7
1	8.85	12.2	1.21	236.63	Compound	Wea C13	Decimals	2	1	1	2	2	0	0	0	0	2	2	0	0
2	8.84	11.7	1.21	226.78	Compound	Wea C13	Horizontal Alignment	Left	Left	Left	Left	Left	Left	Left	Left	Left	Left	Left	Left	Left
3	8.78	8.0	0.98	125.83	Impurity	Wea														
4	8.77	8.5	0.97	131.67	Impurity	Wea	Font MS Shell D	olg 2												
5	8.63	2810.6	1.14	51659.03	Compound	None	Report												-	
6	8.62	2840.8	1.12	51397.20	Compound	None	V Frame	1	Borde	rs		V	Numbe	ring		Title			Bold Header	
7	8.60	22.4	1.35	485.99	Impurity	Wea	Show Purity Label													
8	8.40	11.2	1.29	232.28	Compound	Wea C13												_	OK Cancel	Apply
9	8.39	12.3	1.14	226.96	Compound	Wea C13							_							J Copped
9	8.39		1.14	226.96	Compound	C13		-	-		1	_	-	-			_	_	1.000	-


Purity (as a ratio of Compounds Vs (Impurity+Artifacts) peaks) can be displayed in Peaks table by selecting the checkbox "Show Purity Label" in Setup Table (disabled by default).

To export the peaks in a table, follow the menu 'File/Save As/Script: NMR Peaks Table'; (only the fields set as 'Visible' in Setup Table get exported).

See also Tables.

# **Customizing Peak Reports**

You can add additional report templates by creating new scripts. You will find an example of a script (customPeakReporter.qs) with a different 'Peak Report Template' in the 'examples/scripts' folder of Mnova. To see how to customize this script, take a look at the <u>'Multiplet Analysis'</u> chapter. The concept will be the same.

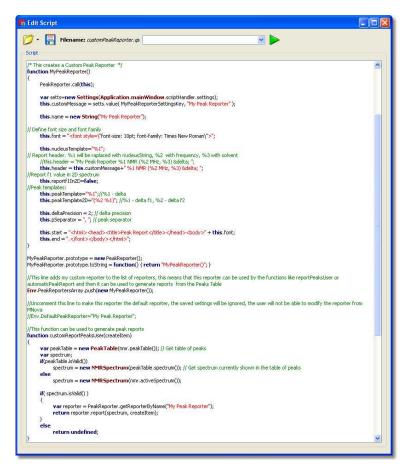

For 2D. you can modify the 'PeakReporter.qs' script (which is located in the scripts folder of Mnova) by just changing the **false** with **true** in this line:

//Report f1 value in 2D
spectrum
this.reportf1In2D=false;

with: this.reportf1In2D=true;

and you will get a report like this:

NMR (400 MHz, CDCl3)  $\delta$  (8.62 147.34), (7.97 131.35), (7.94 131.37), (7.46 118.14), (7.32 121.23), (7.28 121.24), (7.21 101.03), (5.48 71.99), (4.91 114.03), (3.87 55.34), (3.11 59.66), (3.05 56.77), (2.65 56.82), (2.62 42.87), (1.78 27.53), (1.54 21.65).

See also: Peak Picking Properties

### 9.2.4 Peak Picking Properties

The user can modify the properties of the **Peak Picking** by following the menu 'Edit/Properties/Peak Picking' or by double clicking the left mouse (or pressing the right mouse) button on the spectrum display and selecting *Properties/Peak Picking* from the *pop-up* menu.

eometry MMR Spectrum General Grid JD Scales Horizontal Vertical Peaks Integrals Kultiplets Fitting Xassignments	Peaks	Imaxy     Font 2.5 ppm 2 Top All Default V Show Annotations V Show Assignments	
--	-------	--	--

Then, the user can display or hide the peaks (according the peak type by selecting the applicable option in the scroll down menus) and to show/hide the Position, Annotations, Ticks or Assignments by checking (or unchecking) the applicable check box. You can select the color, the font and the units (ppm or Hz) of the 'peak picking label'; the number of decimal figures to be shown on screen and the position of the 'peak labels'.

Clicking on the 'Curve' tab, you will be able to customize the color of peak curves (Peaks, Sum or Residual):

Ceometry NMR Spectrum  General  Grid  ID  Certical  Peaks  Multiplets  Kitting  Assignments	Peaks Label Curve Peaks Edit Coloring Rules Sum Maroon  Residual Navy
---	---

Clicking on the 'Edit Coloring Rules', will display a dialog box to allow you to create different colours rules depending on the peak type and flag:

	Туре	Flags	Color	
1	Compound	Labile	1	
2	Compound	Unused		
3	Solvent	Unused		
4	Impurity	Labile		
)ef	ault Color:			
-	duit Color,	Dark Gray 🔻		


Let's see an example with different peak curve colours:

metry NMR Spectrum	Peaks		Coloring Rules:			
Grid	Label Curve	,	Туре	Flags	Color	
1D Scales	Peaks		1 Artifact	Unused		
Horizontal	Edit Coloring Rules		2 Impurity	Unused		*
Vertical	Maroon v		3 Compound	Labile		*
Peaks	Residual		4 Compound	Unused		
Multiplets	Navy *		5 Solvent	Unused		
Fitting						
Assignments						
s Default Restore	OK Cancel A	PY	Default Color:	Dark Gray 🔻		Cancel
$\wedge$	$\wedge \wedge$			Á	$\wedge$	$\checkmark$
			-		1	X

## 9.3 Integration

Spectral integration can provide invaluable quantitative information about a molecule as the integral of a spectrum indicates the number of nuclei which contribute to a given line (or set of lines).

**Mnova** implements a series of integration algorithms for both 1D and 2D data sets. These algorithms can be accessed via the menu item 'Analysis/Integration' or via the scroll menu immediately to the right of the **'Integration'** icon  $\mathscr{R}$  on the toolbar. This scroll menu will allow you to use Automatic, Predefined or Manual Integration:



# **Autodetect Integration**

# 1D spectra

The program automatically determines the regions containing signals. The algorithm uses the following **options**:

Integral Calculation		<u>O</u> K
Calculation Method:	:	Cancel
Sum	7.	<u>.                                    </u>
Integral Regions		
Source:	Autodetect 🔹	
Parameters		
Algorithm:	Peak Picking 💌	
Minimum Area:	5.00 %	
	Defaults	

• Calculation Method: you can select between 'Sum' (classical integration, faster than 'Peaks' but without deconvolution), 'Edited Sum' or 'Peaks' (it takes into account only the integrals of the GSD spectrum and because of the deconvolution applied, it is slower than the 'Sum' algorithm). In the Peaks calculation method, you can select what peaks will be taken into account for the integration (for example, only compounds peaks and not solvent or impurity peaks, etc...)

Integration Op	otions	8
General		ОК
Calculation Met		Cancel
Peaks Method	d Parameters	Apply
Including:	Compound + ( 💌	
Excluding:	Default 💌	

Edited Sum: in this integration method, the values from Sum method are corrected using a correction factor:

### Sum(Ps\_i)/Sum(P\_i)

where "Ps\_i" are the selected peaks (by default, including Compound peaks and excluding Hidden, C13\_Sat and Rotational); "P\_i" are all peaks in the integration range. Int (Edited Sum) = Int (Sum)\* (Sum(Ps\_i)/Sum(P\_i))

- Algorithm: you can select between the regular algorithm which is called 'Derivative' and the new algorithm based in the 'Peak Picking'.
- Minimum Area: Integrals with a value smaller than a given percentage of the largest integral will be discarded
- Peak Picking algorithm: this integral algorithm is based in the peak picking analysis. The user will

be able to set the maximum value of the coupling constants (J Max), the **Peak Width Factor** and also the **Minimum Area** of an integral (integrals with a value smaller than a given percentage of the largest integral will be discarded)

Peaks	•	Cancel
Calculation Method Peaks Method Pa		
Including: Excluding:	Default	
ntegral Regions		
Source:	Autodetect 🔹	
Parameters		
Algorithm:	Peak Picking 💌	
Minimum Area:	3.00 % 🜩 	

Bear in mind that this algorithm is based on the peak picking results. If no peak picking has been applied, the program applies one on the fly automatically but the best way to proceed will be by first applying a peak picking to make sure that all the real peaks have been detected and, more importantly, artifacts and very small peaks (e.g. impurities) have not.

So as always, it will be a good idea to apply a baseline correction, followed by peak picking – In this case, it's important to ensure that the noise factor is right.

Once you're happy with the peak picking results, it's time to apply integration algorithm. The critical parameter is the 'peak width factor'; the larger this parameter, the wider will be the integral segments.

## 2D spectra

Automatic integration of 2D spectra is based on the <u>2D peak picking</u> algorithm. If no peak picking has been applied when the automatic integration command is issued, **Mnova** will automatically apply a 2D peak picking on the background and then, for every peak detected, it will find the applicable volumes. Thus, the options that control the <u>2D peak picking</u> procedure also apply to the 2D automatic integration algorithm.

A series of Automatic Peak Picking Options can be controlled on the 'Peak Picking Options' dialog box, which can be accessed via the Peak Picking scroll menu (see the 'Peak Picking' section of this guide). The user can choose the noise factor (the higher the factor the less peaks will be picked), the peak type, whether to use parabolic interpolation, merging options for 2D multiplets, maximum number of peaks, etc. All these options can be evaluated interactively, so that their results can be viewed on screen in **real time**, by making sure the **'Interactive'** box is selected.

Peaks Type: Positive and Negative  Use Parabolic Interpolation Maximum Number of Peaks: 1000	Peaks Type: Positive and Negative  Use Parabolic Interpolation Maximum Number of Peaks: 1000 Merge 2D Multiplets Maximum Distance: 15.00 Hz	Sensitivity:	4.00		¢
Maximum Number of Peaks: 1000	Maximum Number of Peaks: 1000	Peaks Type:	Lores.		~
Merge 2D Multiplets	Merge 2D Multiplets	🔽 Use Paraboli	ic Interp	polation	
		Merge 2D Mi	ultiplets		
		Merge 2D Mi	ultiplets		
F2 Maximum Distance: 15.00 Hz	F1 Maximum Distance: 15.00 Hz		ance:	15.00 Hz	0
F1 Maximum Distance: 15,00 Hz		F2 Maximum Dist			

Peak volume integration in Mnova is measured as the sum of all digital intensities within the integration area (footprint). This footprint can be of 2 shapes: rectangular or ellipsoid footprints. In low resolution spectra with no significant fine structure, the ellipsoids footprints fit well, whereas higher resolution spectra tend to show rectangular patterns according to the projections of the correlated individual multiplets.

The default setting is with ellipsoids. But you can change it to rectangular in the integration options.

Seneral	<u>O</u> K
Calculation Method: Sum	<u>C</u> ancel
Integration Shape: Elliptical 👻	Apply
Automatic Integration	1
Method	
Autodetect Regions	

By the way, you can also manually change the size of a footprint by click-and-drag on one of the edges of the footprint.

#### See Integral Properties

# **Predefined Regions Integration**

The user will be able to predefine the integral ranges to automate the integral analysis. Just go through the following procedure:


1. Open the 'Integral Option' dialog box (by clicking on 'Options' in the 'Integration' scroll down menu) and select the Method: **'Predefined Regions'** as is shown in the picture below:

Method		ОК
Autodetect Regions		
Autodetect Regions		
Predefined Regions		Apply
Algorithm:	Derivative	~
Sensitivity:	6 🗘 🗸	utoDetect
Merging Distance:	0.030 ppm	٠
Minimum Area:	1.10 %	\$
Interactive	Defaults	

2. This will display a new dialog box, where the user will be able to select the desired ranges to apply the integration. If you have already integrated the spectrum you can click on the 'Use Current' button to import the integral ranges:

re	defined Regions		~	Cancel
				Cancel
egi	ons			Apply
Z	7 - 🔚			
_	f1 From (ppm)	f1 To (ppm)	~	
l.	8,490	8.784		
2	7,788	8.088	1 E I	
3	7.368	7.615		
1	7.037	7.367		
5	5.571	5.879		
5	5.313	5.570		
7	4.677	5.066	-	
3	3.642	3.971	~	
	Delete D	elete All		

Clicking on OK, will apply the integrations to the current spectrum and keep the regions to apply further integrations to additional spectra by just clicking on 'Predefined Regions' in the Integral scroll down menu:

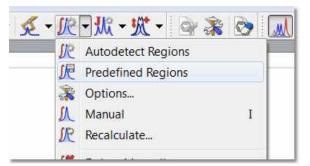


The user will be able to save these regions for later uses, by clicking on the 'Save Integral Regions'

icon which will be loaded by clicking on the 'Load Integral Regions' icon . To save the integral regions, follow the menu 'File/Save as' and select 'MestReNova Integral Regions'.

You will also be able to use the original Bruker integrals by using the 'Use Imported' button. Please bear in mind that if you import a Bruker file with MNova, the integrals will appear automatically, however if you open and old Mnova-document with Bruker data then this button is the way to use Bruker ranges. With the 'Use Imported' button you will be able to reload the original Bruker integrals.

To copy&paste the spectral regions from one spectrum to another, just press 'Ctrl/Cmd+C' in the original spectrum and then follow the menu 'Edit/Paste Properties/Paste NMR Integrals' in the other spectrum (or spectra, if you have previously selected them in the page navigator):

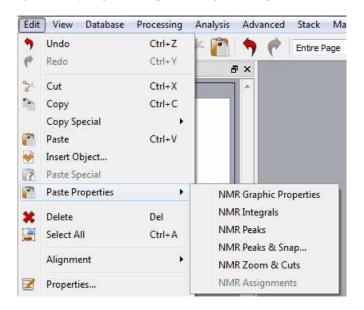


The integral list can also be exported as an ASCII file by following the menu 'File/Save as' and selecting 'Script: Integrals 1D (\*.txt)' (or 2D depending on the dataset). You can also export the integral series and tables:

Nombre:	Document 1.mnova	
Tipo:	MestReNova Document (*.mnova)	
Ocultar carpetas	MestReNova Document (*.mnova) MestReNova Customization (*.mncs) ASCII Text File (*.txt) Adobe PDF Files (*.pdf)	
	BMP Image (*.bmp) Encapsulated PostScript (*.eps) Enhanced Metafile (*.emf) JCAMP-DX (*.jcamp) JPEG Image (*.jpeg)	
	MestReC (*.mrc) MestReNova Integral Regions (*.txt) MestReNova Peaks (*.txt) PNG Image (*.png) PPM Image (*.pnm) PostScript (*.ps)	
-	SDFile (".sdf) SVG Image (*.svg) TIFF Image (*.tiff) XBM Image (*.tbm)	
-	Script: 1D Integral Series (*.bd) Script: Integral Table (*.bd) Script: Integrals 1D (*.txt)	

# Manual Integration (shortcut: I)

First, select integration mode by clicking on the Manual integration command as depicted below:




- Next, click and drag with the mouse to select the area to be integrated
- The first integral will be normalized to 1.0. All following integrals will be referenced relative to the first integral.

Follow the menu 'File/Save as' and select 'MestReNova Integrals (\*.txt)' to save the integrals list as a 'text file'


# **Integral Settings:**

All the integral curves are mouse-sensitive and they respond to usual mouse operations. If you want to move up or down all the integrals, just click and drag (with the left mouse button) over anyone of the integrals (notice that hovering the mouse over the integral will highlight it in red). If you keep pressed the SHIFT key at the same time, the height of the integral curves will be changed.


The same effect will be obtained if you hover the mouse over integral curve, click on one of the green squares and drag the mouse up or down. If you want to change the range of the integral, do the same with the integral label (notice that once you hover the mouse over the green squares of the integral curve or label, the mouse pointer turns to vertical or horizontal arrows, respectively).

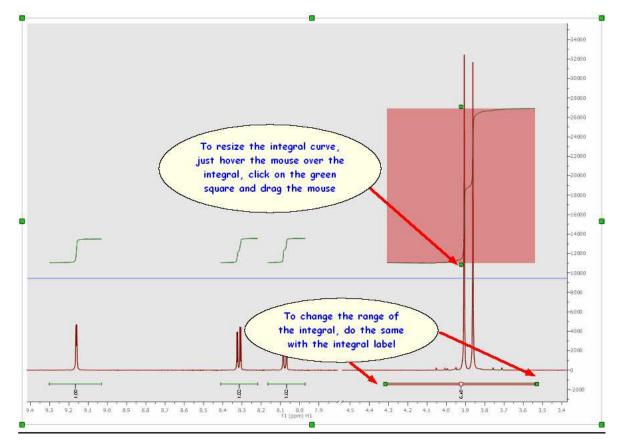

**Cutting Integrals:** to divide any integral just by clicking on the red square of the integral label and dragging the mouse:

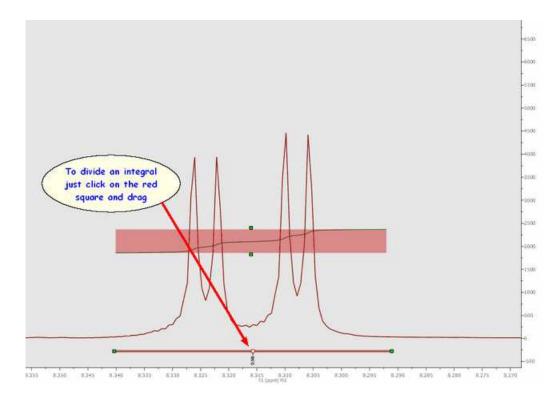

**Integration Manager (shortcut: Shift+I):** The integral editor will be displayed by double clicking on any integral curve, as you can see in the figure above. From there, you can change the integral range, normalize the integral to a specific integral, navigate through them and also to reference integrals to the total integral value for the spectrum.

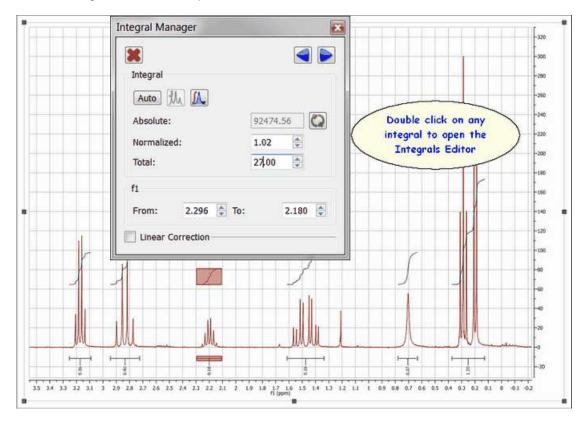

You can manually add integrals and multiplets using different integration calculation methods (Sum, Edited Sum and Peaks). To avoid missunderstandings in the integration results, you can track the method used in each integral/multiplet. This will be displayed in the Integral/Multiplet Manager, where there is an option to recalculate each integral/multiplet with ability to choose the integration method in each case.

tegral Manager		🕅 Integral Calculation 💡 🔜 🗙
Integral Auto M. M. Absolute: Normalized: Total:	92474.56 1.02 - 27.00 -	Integral Calculation Calculation Method: Sum Peaks Edited Sum
f1 From: 2.296 💽 To	: 2.180	

A similar option can be found under the Analysis/Integrals menu.



The user can resize the limits of the integral by using the arrow buttons 🗟 or entering the desired value on the applicable edit box:

From:	2.273	\$ To:	2.105 😂

Bear in mind that you are able to navigate over the integrals by using the 'Previous or Next' icons.

If you want to resize the height of the integral curve, just hover the mouse over one of the integral curves and hold down SHIFT, click on left mouse button and drag up or down (to increase or decrease the height).

If you want to normalize the integrals, just overwrite the desired value on the 'Reference edit box' (on the Integrals Editor') and press OK, all integrals will update with reference to the chosen one. The user can also delete an integral one by one by clicking on the 'Delete' button.

You can apply the same integral normalization to all the spectra (in the current document) or to all the traces of a stack plot by selecting the applicable option, as you can see below. This is very useful if you need for example to determine relaxation times from a series of 1D spectra, to be able to compare the integral values between the different traces.

Integral Manager		]
Integral		
Absolute: Normalized:	and the second second	ization to All Document Spectra ization to All Stack
Total:	25.00	
f1 From: 7.910	🔹 To: 7.860 🐳	
Linear Correcti	on	

**Linear Correction:** Linear correction is basically a straight line built connecting the left and right boundaries of every integral in such a way that the final area will include only the integral above that line. In other words, if A is the total area under the peak(s) and B is the area under that straight line, the reported integral R will be:

R = A - B

Mnova has an option to automatically calculate this straight line. In order this to work properly, it's recommended to have a good digital resolution (e.g. by applying ZF), as the program utilizes 3 points at both edges of the integral to build the straight line.

If you want to apply an integral correction or rather, a linear baseline correction just on the integral

region, just click on 'More >>' button, this will display the 'Linear Correction' dialog box, where you will able to adjust the *Bias* and *Slope* parameters.

Bias:	0.000	\$
Slope:	0.000%	\$
🗌 Au	to	
Appl	y to All Reset All	


Use the controls for *Bias* and *Slope* correction as follows:

- Adjust the Bias parameter until the initial (left) part of the integral is flat.
- Adjust the Slope parameter to flatten the top (right) part of the integral curve.

The *Auto* box computes the *Bias* and *Slope* values automatically. The button *Apply to All* is used to correct all the integrals simultaneously.


We strongly recommend to correct the baseline prior integration using any of the baseline correction algorithms.

Likewise, if you press the right mouse button on an integral, you will get a pop-up menu with the following options:



Edit Integral: displays the Integration Manager dialog box. Show Table of Integrals: to show the integrals table Delete Integral: deletes the current integral. Delete All: deletes all integrals.

Autodetect Nuclides Count: this command will be very useful to count the nuclides present in any spectrum. In this case, it is shown the 1H-NMR spectrum of the quinine. We have applied the 'Nuclides Count' algorithm after the integration and the result is that the number of protons is 24 (which is consequent with the molecule).

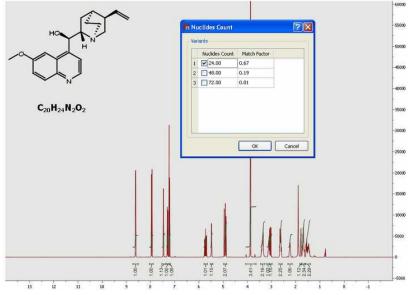


Integration only gives information on the relative number of different nuclides. From a practical stand point, first the absolute integral values are computed and then the integrals are normalized (referenced).

For example, if we know that a given integral corresponds to a CH3 group, we can set it to a value of 3 so that all other integrals will be scaled accordingly. Note that these values are not exact integers and need to be rounded to the nearest integer to obtain the significant value. But that means that the reference should have correct intensity to start with, which is not guaranteed.


Our goal is to automate this process, that is, starting from the absolute integral values, automatically select the reference group and scale the remaining values in order to obtain the correct number of nuclides.

It is a simple algorithm to auto normalize the 1H NMR integrals without prior-knowledge. It will be useful especially for auto batch processing using the scripts of Mnova.

Starting from this situation:

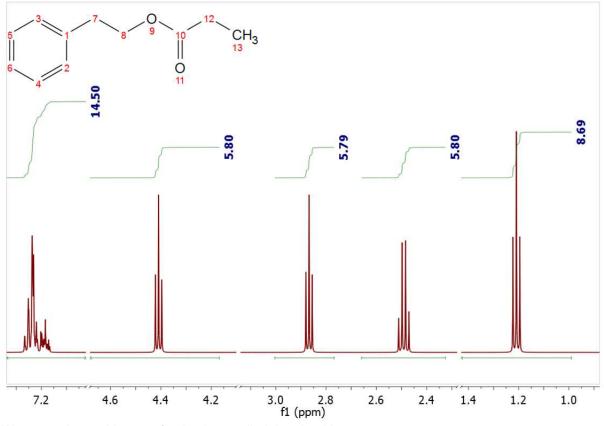

We can arrive to this one after having applied the algorithm:

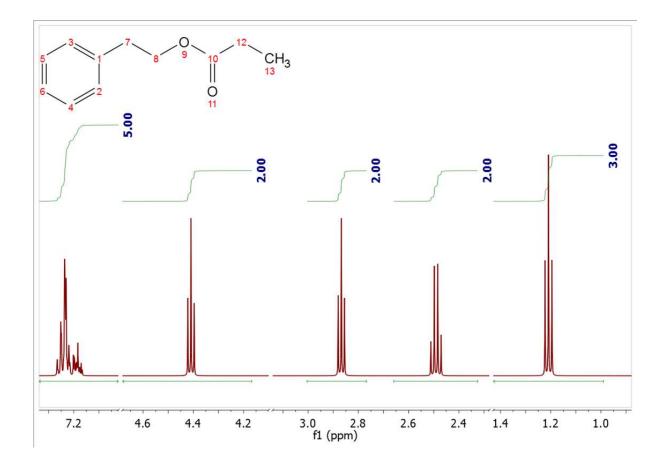

#### See also:

#### **Integral Properties**

#### 9.3.1 Integrals Table


The Integrals Table (by following the menu: 'View/Tables and then select: Integrals') includes information about the integral range (in ppm) and the normalized and absolute values of each integral.

In this table the user can delete a desired integral by clicking on the **'Delete'** icon **\***. The user can also normalize the integrals by double clicking on the normalized value of the integral which the user would like to set (in the red square on the capture below). Once it is highlighted, the user has to overwrite the desired value, press return, and all integrals will update with reference to the chosen one.

This method is an alternative way to normalize integrals. The user can obtain the same result by double clicking directly on the integral curve on the spectrum, as we have explained in the chapter above.

R	eport Copy	X Delete Set	up
	Range	Normalized	Absolute
1	9.21 9.11	1	26356.88
2	8.37 8.26	0.93	28021.56
3	8.13 <mark>8</mark> .03	0.98	29299.02
4	3.95 3.89	2.98	89550.74
5	3.89 3.82	3.23	97200.39

You can normalize on the sum of several integrals, by highlighting the applicable integrals (from the Integrals table) and right clicking and selecting "Normalize" from the context menu. Finally type the total value to normalize:

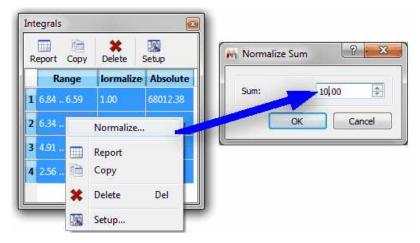

Double clicking on any cell of the 'range' or 'absolute' columns will display the 'Integral Manager', which will allow you to normalize or change the integral range:

				Integral Manager		
inte	grals					
200	port Copy Dele	CLED		Integral		
	Range	lormalize	Absolute	Auto the Ma		
1	8.67 8.58	0.92	84736.61	Absolute:	84736.61	
2	7.99 7.92	9.91	84299.52	Normalized:	0.92	A Y
3	7.50 7.43	1.03	94664.84	Total (24 in molecule)	; 25.00	A V
4	7.34 7.26	0.94	86584.13	f1		
5	7.25 7.18	1.54	141809.61	From: 8.668 🚔	To: 8.57	7 🜲
6	5.80 5.66	0.94	86507.62			
7	5.51 5.45	1.06	97207.07	Linear Correction -		
8	4.99 4,85	1.92	177354. <mark>3</mark> 1	Bias:	0.000	* *
9	<mark>3,90 3,84</mark>	3.11	286086.42	Slope:	0.0000°	(A) (V)
10	3.44 3.31	1.97	181648.81	Apply to All R	eset All	

You can also display the integral calculation method (Peaks, Sum or Edited Sum) by clicking on the 'Setup' button:

R	eport Copy	X Delete	Setup	D	
	Range	Norm	alized	Absolute	Method
1	7.93 7.89	0.95		33691.34	EditedSum
2	7.78 7.73	0.87		31017.26	Sum
3	7.73 7.66	1.97		70167.37	Sum
4	7.60 7.53	1.10		39288.38	Peaks
5	3.41 3.36	5.39		19211	Peaks
6	1.57 1.48	6.00		21379	Sum

# 9.3.2 Integral Properties

The user can modify the properties of the integrals by following the menu 'Edit/Properties/Integrals' or by double clicking the left mouse (or pressing the right mouse) button on the spectrum display and selecting *Properties/Integrals* from the *pop-up* menu.

The options are different in 1D and 2D-NMR:

#### 1D Spectra

General	Integrals				
🔣 1D 4 🚧 Scales	Font:			MS Shell Dlg 2	•
Horizontal	Decimals:			2	*
Uertical	Position:			On Segment	•
Peaks	Margin:			8 %	*
🍌 Integrals	Orientation:			Vertical	*
Multiplets Integrals Itting Assignments	Color:	ion Methoo	i Symbo	green	•
Section Prediction	Line Width:	2.5			
10000					
	Position:	56 %	*		
	Maximum Height:	40 %	*		

**Integrals**: Check/Uncheck this option if you want to display/hide the integrals (labels + curves) **Label**: Check/Uncheck this option if you want to display/hide the integral labels

Font: Select the font type

Decimals: Select the number of decimal figures to be shown on screen

**Position**: Use this option to show the integral label on the curve or on the integral segment **Margin**: distance (in % with respect to the spectrum item height) from the top

#### Orientation: vertical/horizontal

**Show Calculation Method Symbol:** it will display and S (Sum); E (Edited Sum) or P (Peaks) in the integral label; depending on the integral calculation method used.

Curve: Check/uncheck this option to show/hide the integral curves

Color: Select the curve color

Line Width: to select the width of the line of the integral curve **Position:** distance (in % with respect to the spectrum item height) from the top **Maximum height** of the integral curve.

-

2D Spectra

General Grid Grid 1D 2D Traces Stacked Stacked Scales Horizontal Vertical	✓ Integrals ✓ Label Font: Decimals: Curve Color: Line Width:	MS Shell Dig 2 2 green 2.5	•
Assignments as Default Restore		OK Cancel	Appl

Integrals: Check/Uncheck this option if you want to display/hide the integrals (labels + curves) Label: Check/Uncheck this option if you want to display/hide the integral labels Color: Select the integral label color

Font: Select the font type

Decimals: Select the number of decimal figures to be shown on screen

Curve: Check/Uncheck this option to show/hide the integral curves

Color: Select the integral color

Line Width: Select the with of the line of integral curve

# 9.4 Multiplets analysis

(Not available in Mnova Lite)

You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder)

Mnova incorporates a powerful multiplet analyzer. The user will carry out an automatic multiplet analysis by clicking on its respective icon, placed on the analysis toolbar menu International sis/Multiplets Analysis/Automatic'.




Bear in mind that when you select an automatic multiplet analysis, Mnova will take into account the <u>Multiplet Analysis</u> options

See also this <u>chapter</u> about using GSD for multiplets analysis.

The user can also apply a manual integration followed by an automatic multiplet analysis (to obtain the same ranges in both cases), but please bear in mind that **integrals and multiplets are two independent lists**, so you will be able to have different ranges in both. In that case where the multiplets are made from integrals, MNova visualizes only multiplet integrals.

In the picture below, you will see the result of having applied an automatic multiplet analysis and selected **'Report Multiplets'** in the context menu of the multiplet box (which can be accessed by right clicking on it). The same result will be obtained by selecting 'Report Multiplets' in the multiplets scroll down menu.

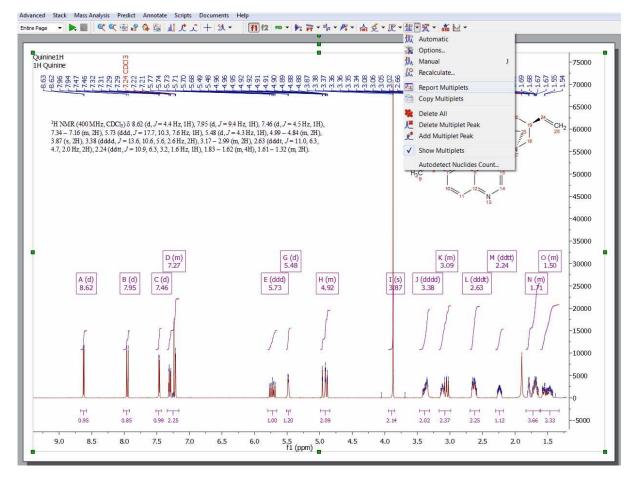


Another valid workflow would be to press the 'J' key to activate the manual multiplet analysis and click&drag on the regions that you want to analyze. You will not need to use the integration at all. If you want to show the integral curves of your multiplets, just double click on the spectral window to display the 'Properties' dialog box and check the applicable box:

Metadata     Geometry     NMR Spectru       Image: General     Grid       Grid     Integrals       Integrals	Multiplets Labels Font: Line Width: Label: Shift Decimals: Js Decimals: Margin: Follow Peak Visibility Rules J's Tree Show Label	MS Shell Dig 2 2.5 2 2 50 % V Show Label Box	
--	---	---	--

You can export the multiplet integrals list by following the menu: 'File/Save As:/Script: Multiplet Integral' or 'Script: Multiplet Integrals Series' if you work with arrayed spectra.

## 9.4.1 Multiplet Manager

The user will be able to set the multiplet parameters by double clicking on the magenta square ( shortcut: Shift+J) containing the multiplet information.

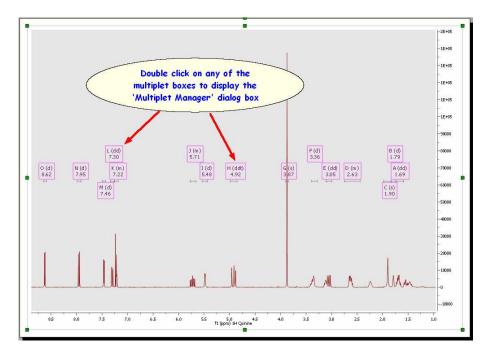

This will display the 'Multiplet Manager' dialog box, where you will be able to modify the multiplet limits as well as to normalize the values or report the multiplets just by clicking on the applicable button .

Aultiplet	Manager	×
5.73 (0	ldd, J = 17.7, 10.3, 7.6 Hz, 1H)	
Name:	F Class: ddd 🔻	
δ:	5.727 ppm V Middle	
J-List:	17.70, 10.30, 7.59	
	Discard Peaks	
Color:	Purple 🔻	
Total Nu	clides = 27	
Nuclide	s: 1 😫 Auto	
Integral	: 0.95 🔮 🗼	
Absolut	e: 86500.5	
From:	5.796 📮 To: 5.658 🌻	
	A DEVELOPMENT AND A DEVELOPMENT	

You can manually add multiplets using different integration calculation methods (Sum, Edited Sum and Peaks). To avoid missunderstandings in the integration results, you can track the method used in each multiplet. This will be displayed in the Multiplet Manager, where there is an option to recalculate each integral/multiplet with ability to choose the integration method in each case.

5.73 (ddd, J = 17.7, 10.3, 7	.6 Hz, 1H)		
		Integral Calculation Setting	gs ? X
Name: F 5: 5.727 ppm V Mid 17.70, 10.30, 7.59	Class: ddd 👻	Integral Calculation Calculation Method: Edited Sum Sum Peaks Edited Sum	OK Cancel
Color: Purple	•	Periodenings (excess	
Nuclides: 1	Auto		
Integral: 0.95			
Absolute: 86500.5			

A similar option can be found under the Analysis/Multiplets menu.

From the multiplet manager, you will be able to change the name, class (you can add new classes to the drop down menu just by typing the name and pushing Enter key), the coupling constant tolerance, limit and the color of the multiplet box. Please bear in mind that if the class of the multiplet is called 'mx' (being x any letter); the multiplet will be reported as a chemical shift instead of the multiplet range.

Here you can see the difference:

Multiplet	Manager		Multiplet	Manager	
<b>X</b>	2 🛃 🗷			2 🗹 🛛	
1.69 -	- <mark>0.96 (</mark> m, 1H)		1.29 (	m, 1H)	
Name:	A	Class: m	Name:	A	Class: mx
ō.	1.203.000	1 Middle	5.	1 293 000	Middle

The number of hydrogens (Nuclides) will be rounded (up or down) by default with respect to the multiplet integral value (which in this case corresponds with the area under the multiplet range, not with the area under the integral curve).

Bear in mind that, integrals and multiplets are two independent lists, so you can change the nuclides (or multiplet) value, without affecting to the integration.

Click on the applicable icon III of the 'Multiplet Manager' dialog box to import the integral normalization values.

Clicking on the 'Auto' button is of the 'Multiplet Manager' dialog box will display the 'Nuclides Count dialog box'. From this window, you will be able to select the total number of nuclides of the spectrum (nine hydrogens in the example below) and apply it to the spectrum.




The user will also be able to add or delete couplings constant by clicking on . After that, the 'J's Editor' dialog box will be displayed:

<b>J-List Edito</b> I-List		
Manual		~
1.45 1.45 10.33 13.25		
ſ	ок	Cancel

From the multiplet manager dialog box, you can delete a multiplet by clicking on the 'Delete' button or navigate through the multiplets by using the 'Previous' or 'Next' buttons

From this dialog box, you can also "add multiplet peak" 📝 (if you pick a peak twice with this feature, the peak will be removed) or delete undesired peaks 🗷 by using the applicable icons.

Once you click on this icon *I*, you will see the applicable label above each peak of the multiplet, indicating the name of the multiplet:

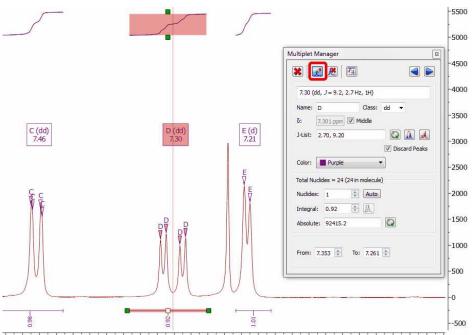


50 7.48 7.46 7.44 7.42 7.40 7.38 7.36 7.34 7.32 7.30 7.28 7.26 7.24 7.22 7.20 7.18 7.16 7.14 7.12 7.10 7.08 7.06 7.04 7.02 7.00 6.98

Please note that the 'Multiplet Manager' dialog is **modeless**, so you will be able to use any other tool (i.e. zooming) whilst you are applying the analysis.

Clicking on this button will allow you to select two points in the spectrum and the difference between them in Hz will be added to the J list.

Mnova offers the possibility of displaying the corresponding synthetic multiplet built using these calculated *J* couplings. This is a useful tool to check whether the values calculated by Mnova using first order rules actually match the experimental multiplet. In order to show the synthetic multiplet, just check the button highlighted in red in the figure below. The program will automatically create a synthetic multiplet with a light red color as background.

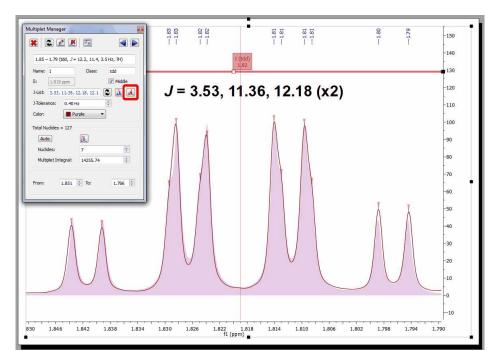


# 9.4.2 Using GSD for multiplets analysis

### Exploiting the power of GSD for an improved Multiplet Analysis

By default Mnova uses Global Spectral Deconvolution (GSD) algorithm for automatic peak picking and multiplet analysis.

Multiplet Analysis benefit directly from the exploitation of GSD capabilities to carry out the automatic analysis, with the enhanced peak picking capabilities resulting in much more reliable automatic multiplicity identification and labeling.

Here you can see an example of a triplet which is hidden under the solvent signal:

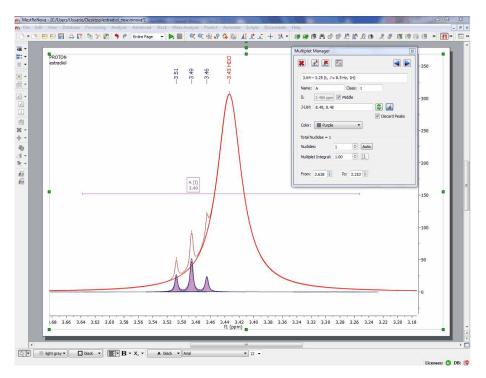

In order to use this algorithm, make sure that you have the following default options in Mnova.

#### 1 – Defining the GSD level

GSD has different operational levels, ranging from a very fast but inaccurate method to slower but much more accurate levels. In addition, GSD allows the automatic recognition of solvent peaks, impurities, etc. We recommend to use a GSD level of 1 (flash) or 2. This level can be set from Peak Picking/Options as depicted below:

1ethod:	GSD
Peaks Type	
Only Positive	
Settings	
Refinement Level	Optimized for Peaks:
Ref. 1 ( 2 fitting cycles )	Narrow
<u>, i i j i i i</u>	Average
Use Parallel Processing	🔘 Broad
	Custom 1.00
V Auto Classify	Impurities/Compounds
	Defaults
	OK Cancel

Also, make sure that the Auto Edit option is checked.

From now on Mnova will use GSD when automatic peak picking algorithm is issued (which is the default setting).

#### 2 – Set the Automatic Integration method to GSD

Finally, for Mnova to be able to detect the multiplets regions automatically using GSD, it's necessary to define the **'peaks'** as integral calculation method under the 'multiplet options' (this should be the default setting).

General	ОК
Minimum Area: 3.00 % 🚔	Cancel
Integral Calculation	Restore Defaults
Calculation Method:	
Peaks 🔹	
Method Parameters	
Excluding: Default	

### First Order Multiplet Analysis with GSD with Resolution Enhancement

(click here to download the spectrum used chapter)

 Bit-MMS-Sattonin
 150

 Sattonin
 130

 130
 120

 130
 120

 130
 120

 130
 120

 130
 100

 90
 60

 70
 60

 50
 60

 50
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100

 90
 100


 90
 1

Consider the following multiplet:


At first sight, this looks like a doublet quadruplet ( $J = 12.2 \times 3, 3.6 \text{ Hz}$ ) and in fact, this is what some NMR software packages would report if this multiplet were analyzed using based on traditional peak picking algorithms.

Now Mnova Multiplet Analysis is armed with GSD, making the analysis of NMR spectra a more

efficient process. Assuming that all Mnova options have been set properly in order to use GSD for multiplet analysis, this is what Mnova would report for this multiplet:

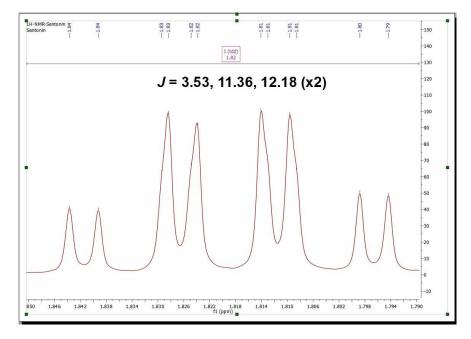

As it can be noticed, Mnova now finds an extra coupling of 11.4 Hz. If we take a closer look at the fine structure of the multiplet once GSD has been applied, we can observe that the 4 peaks in the center of the multiplet are actually split into 8 peaks as illustrated in the figure below:

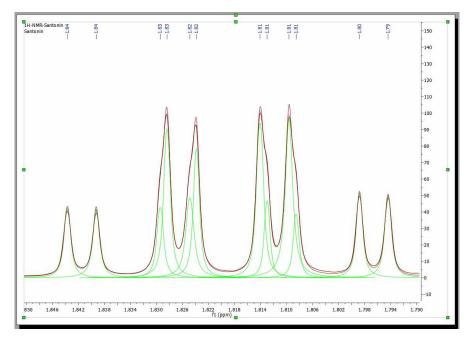


### 9.4.3 Setting multiplets

All the multiplet boxes are mouse-sensitive and they respond to usual mouse operations. If you want to move up or down all the multiplet boxes, just click and drag (with the left mouse button) over anyone of the boxes (notice that hovering the mouse over the box will highlight it in red).


To change the range of the multiplets, hover the mouse over the multiplet box, click on one of the green squares and drag the mouse to the left or right (notice that once you hover the mouse over the green squares of the multiplet label, the mouse pointer turns to horizontal arrow).



**Cutting Multiplets:** to divide any multiplet just by clicking on the red square of the multiplet label and dragging the mouse:

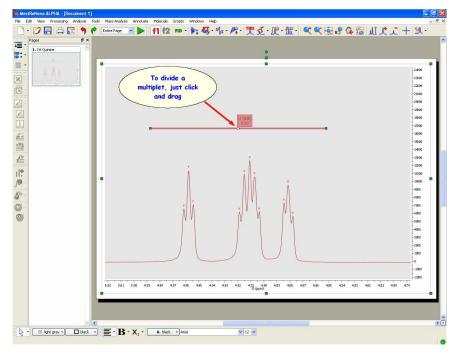

Right clicking on the multiplet box, will display the applicable context menu:




From here you will be able to display the 'Multiplet Manager' or the 'Table of Multiplets'. You can also change the 'Peaks Type' (from compound to impurity, solvent, artifact, etc) or to assign the peaks inside the multiplet to a specific compound. You can generate a 'multiplet report', copy the multiplets to


the clipboard, delete and add multiplet peaks, etc as you can see in the picture above.

### 9.4.4 How to resolve overlapped multiplets?

It is really easy to resolve overlapped multiplets. Imagine the below overlapped doublets:

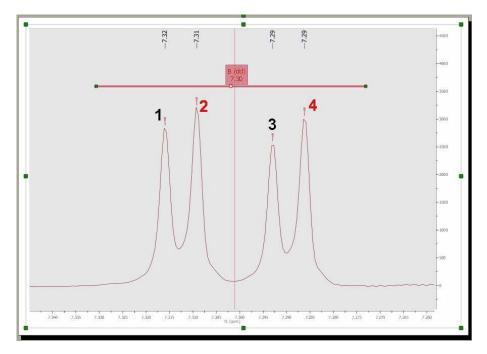

where the peaks 1 and 3 correspond to one doublet and the other peaks (2 and 4) to the second doublet. First of all, divide the multiplet just by clicking on the red square of the multiplet label (to obtain two overlapped multiplets):

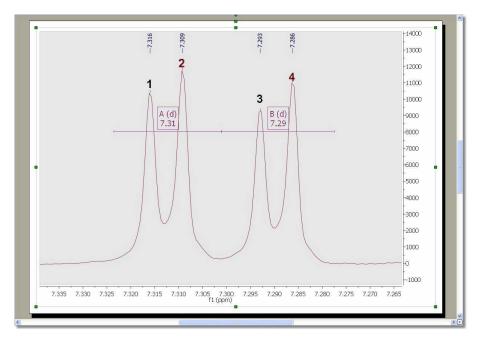


Next, double click on any of the multiplet boxes to launch the 'Multiplet Manager' dialog box. Once there, click on the 'Add multiplet peak' button (red square in the picture below). With this tool you can


also remove peaks from the multiplet, by picking over a previously picked peak. Use this button Let to delete undesired peaks.

	l, J= 2.7 Hz,	-5	
Name:	A	Class:	d
δ:	7.313 ppm		Middle Middle
J-List:	2.71		
J-Tolera	ance:	0.40 Hz	÷
Color:		Dark magenta	~
Total N	uclides = 55		
C	Auto	A	
N	uclides:	1	\$
	t Integral:	1.00	(4)


This will add a peak label with the multiplet name (A and B) over each peak, as you can see below:

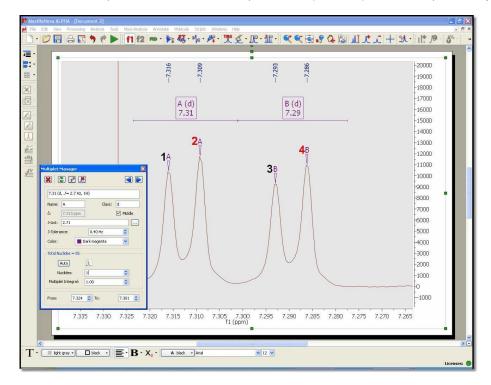


Finally, hover the mouse over the multiplet box A, click and drag to the the label (**B**) of the peak **3**, or vice versa, hover the mouse over the label of the peak 3, click and drag it to the multiplet box A (as it is shown in the picture below):

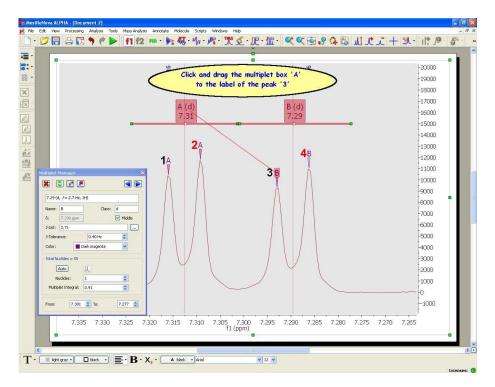

After that, the peak **3** will be a part of the multiplet **A**; (at this moment the multiplet A contains the peaks 1, 2 and 3):

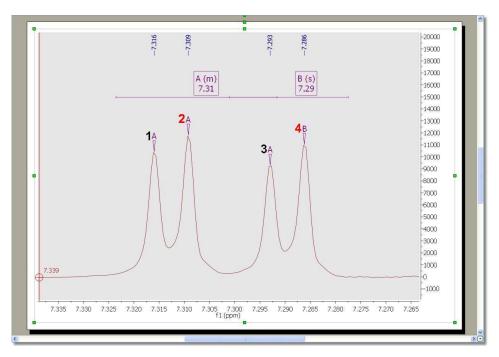

Finally, do the same procedure with the peak **2** and the multiplet box **B** (click and drag the peak label to the multiplet box or vice versa), in order to include the peak 2 into the multiplet B:

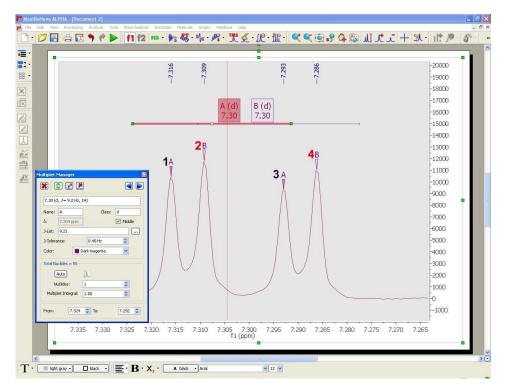

As you can see in the picture above the multiplet A contains the peaks 1 and 3 and the multiplet B contains the peaks 2 and 4.

## 9.4.5 Multiplets Table and Reports

## **Multiplets Table**

The user will be able to get the 'Multiplets' table by following the menu 'View/Tables'. The 'Multiplets' table includes information about the name (by default Mnova will have named the multiplets in alphabetical order, but the user is able to change this order in the 'Multiplet Manager'), the chemical shift (ppm), the range (ppm), number of hydrogens, integral value, type of multiplet and coupling constant values (Hz).


Re	eport Multip	lets 🝷	Copy Multiplets	s * Se	etup Report	• Delete			
1H 5.4 2H	I), 7.30 (dd 18 (d, $J = 4$	, <i>J</i> = 9.3 .3 Hz, 11 .99 (m, 2	, 2.7 Hz, 1H), 7 H), 4.99 – 4.84 H), 2.63 (dddt	.21 (d, (m, 2H	J = 2.7 Hz, ), 3.87 (s, 31	1H), 5.73 (dd H), 3.38 (ddd	$\frac{\mathrm{dd}}{\mathrm{dd}}, J = 1$ $\mathrm{dd}, J = 1$	1H), 7.46 (d, <i>J</i> = 4.5 7.5, 10.3, 7.6 Hz, 1H 3.4, 10.5, 5.6, 2.5 Hz .18 (m, 1H), 1.83 – 1	),
	Name	Shift	Range	H's	Integral	Absolute	Class	J's	1
1	C (d)	7.46	7.517.43	1	0.86	92585.19	d	4.51	
2	A (d)	8.62	8.67 8.58	1	0.80	86101.39	d	4.39	111
3	N (m)	1.71	1.83 1.62	3	3.29	352791.56	m		
4	M (m)	2.24	2.30 2.18	1	0.96	103210.06	m		
	L (dddt)	2.63	2. <mark>6</mark> 9 2.55	2	1.97	211502.68	dddt	2.01, 2.01, 4.29, 6.03, 10.73	
5	K (m)	3.09	3.17 2.99	2	2.31	247987.14	m		
	ic (m)							2.54, 5.56, 10.50,	
5 6 7	J (dddd)	<mark>3.3</mark> 8	3.46 3.31	2	1,90	203318.84	0000	13.36	

You can add/remove columns by selecting 'Setup table' in the Setup Report scroll down menu.

Double clicking on any cell of the multiplet table will display the <u>'Integral Manager'</u>, which will allow you to edit the applicable multiplet information:


ult	iplets					1		Multiplet Manager
Re	eport Multiple	ets Čop	y Multiplets	Setup Report	t Delete			
(d 	d, J = 9.2, 2 4.85 (m, 2H) I), 2.63 (ddo	.7 Hz, 1H), , 3.87 (s, 3H id, J = 13.6,	7.21 (d, J = 2.8 H I), 3.38 (ddq, J	Hz, 2H), 5.73 = 13.3, 8.2, 2	6 (ddd, J = 17 2.6 Hz, 2H), 3	.1, 10.3, 7.6 .17 – 3.09 (	), 7.46 (dd, <i>J</i> = 4.5, 0.7 Hz, 1H), 7.30 5 Hz, 1H), 5.48 (d, <i>J</i> = 4.4 Hz, 1H), 4 m, 1H), 3.05 (dd, <i>J</i> = 13.8, 10.2 Hz, = 3.2 Hz, 1H), 1.69 (dddd, <i>J</i> = 13.9,	.99 Name: O Class: p 🔻
	Name	Shift	Range	H's	Integral	Class	J's	▲ Discard Peaks
1	Q (m)	1.51	1,61 ., 1,36	2	2.18	m		Color: Purple
2	P (dddd)	1.69	1.75 1.62	2	2.19	dddd	2.65, 4.51, 8.25, 13.90	Total Nuclides = 25 (24 in molecule)
3	O (p)	1.78	1.83 1.75	1	1.05	р	3.20, 3.20, 3.08, 3.08	Nuclides: 1
4	N (m)	2.24	2.29 2.18	1	1.00	m		Integral: 1.05 🚖 🛴
	M (dddd)	2.63	2,69 ., 2,56	2	2.10	dddd	2.11, 5.09, 6.33, 13.60	Absolute: 96423.8
5				-		dd	10.17.10.00	
8	L (dd)	3.05	3.09 3.00	1	1.16	ad	10.17, 13.83	From: 1.825 🐳 To: 1.751 🜩

The user can paste the 'Multiplets' table on the spectrum by clicking on the **'Report table'** option (under the 'Report Multiplets scroll down menu) and also can delete a multiplet from this table by using the **'Delete'** icon **\*** when the undesired multiplet is highlighted.

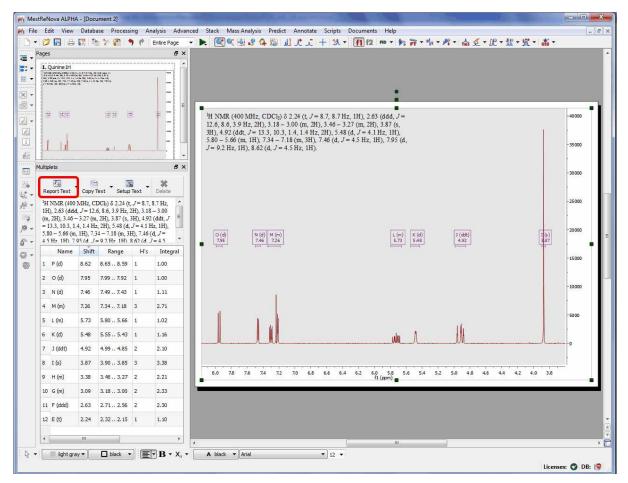

Finally, the user will be able to obtain the multiplet report list by clicking on the 'Report Multiplets' button:

The same result will be obtained by right clicking on the multiplet box and selecting 'Report Multiplets' or by selecting 'Report Multiplets' in the 'Multiplet Analysis' scroll down menu (highlighted in red in the picture below). Of course, the user will be able to add an icon for this feature (highlighted in green in the picture below) into the toolbar. See the chapter <u>'Toolbars Customization'</u> for further information about it.

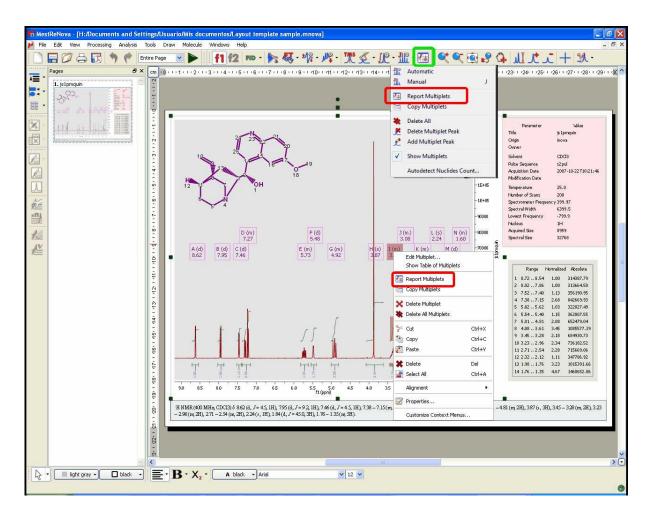

# How can I select the Journal template for my multiplet reports?

The format of the Multiplet Report can be selected just by selecting 'Setup' (in the 'Setup Text' scroll down menu of the Multiplet Table). This will display the 'Multiplet Report' dialog box with a scroll down menu, which will allow the user to select the desired template (JACS, Royal Society of Chemistry, Angewandte or any other Custom Report).


JACS
🔲 All as Ranges
👿 m's as Ranges
Ascending Order of Shifts
Report Js
V Reduce J List
🔲 Use Extended Solvent Names
Report Assignments
Shift Number of Decimals: 2

From here you can also report your multiplets as ranges or even combine the report of the multiplets (some as ranges and other as chemical shifts). To do that, please rename the class of the multiplet (from the multiplet manager dialog box) as 'mx' (being x any letter) and this specific multiplet will be reported as a chemical shift instead of the multiplet range.


Uncheck the option 'Reduce J List' to show all degenerated coupling constants.

You can also sort the multiplets in ascending order, report assignments, or use extended solvent names just by checking the applicable boxes. You can also select the number of decimals for the chemical shift values.


The user will be able to copy the multiplet report to the clipboard by selecting 'Copy Text' on the Multiplets table:



And then paste the multiplet report on another document just by using Ctrl+V or Cmd+V.

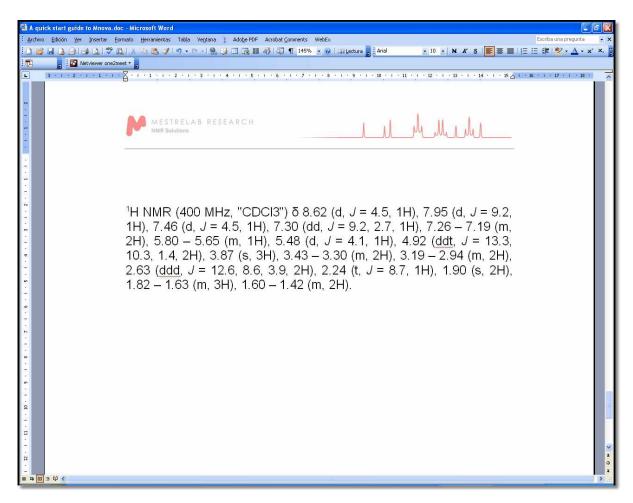

Follow the menu 'Scripts/Report/All Multiplets in Document' to generate multiplet reports in each spectral page of a document.

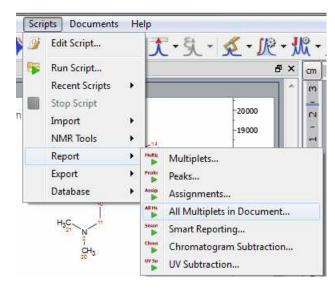

# How can I create a new 'Multiplet Report' format?

The user will be able to change or create his own multiplet report templates; by following the menu 'Script/Edit Script'.

You can see below how to add a new multiplet reporter to the Mnova GUI.

1. Follow the menu 'Script/Edit Script' to launch the 'Script editor'.

📅 Edit Script	
Script	
Script	
Output	
Output	

2. Write your own script or edit the example 'customMultipletReporter.qs' under the script folder of Mnova (Mnova\examples\scripts). Do not forget to include the below sentence in the script; in order to add the reporter to the program:


Env.MultipletReportersArray.push(new MyMultipletReporter());

We have created a variable in the scripts which saves a list of the known reporters. To see the list, just type in the editor:

print(Env.MultipletReportersArray)

1ultipletReporter()
1ultipletR

See below how to edit this script.

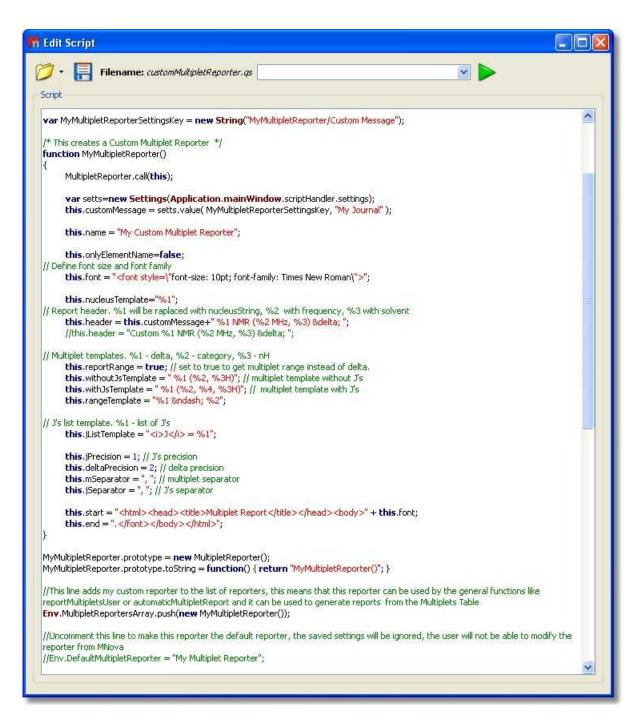

**3.** Save the resulting script (for example 'My Multiplet Reporter') in a directory where Mnova will be able to find it and restart Mnova. To add new script directories follow the menu 'Edit/Preferences/Scripts/Directories':

		35	1	2	-	1	15
General	Plug-ins	Scripts	Database	NMR	Mass	Molecule	Drawing Tools
irectories	Events						
C:\Prog	ramData/Mes	trelab Resear	lesearch/MestR ch S.L./MestRe ng/Mestrelab R	Nova ALPHA	Vscripts	AI DHA/cerin	ts 🕷
	s\Usuario\App s\Usuario\Des		ig/ Mestrelab N	esearch S.L.	MESLACIADA	MERTIN/SCOP	

**4.** The script will be automatically added to the Mnova GUI (for example, to the 'Multiplet Table/Report Special/Setup' menu). This will allow you to select the 'Multiplet Report' format for your analysis. Of course, you can add as many different scripts as you need.

🖁 Multiplet Report 🛛 🕐	
O JACS	1
O RSC	
O Angewandte	
💿 My Multiplet Reporter	
O My Custom Multiplet Reporter	
🗹 m's as Ranges	1
Ok Cancel	

Please bear in mind that the multiplet format that you select on this dialog box, will be applied always when you select the 'Multiplet Report' option; however you can select any other formats for individual reports (without changing the default one) just by following the menu 'Scripts/Report/Multiplets' and selecting the desired format for that report.

Let's see how to create a new multiplet reporter script from the example 'customMultipletReporter.qs' (stored at the 'example/scripts' folder of Mnova) :

```
/* This creates a Custom Multiplet Reporter */
function MyMultipletReporter()
{
      MultipletReporter.call(this);
      var setts=new Settings(Application.mainWindow.scriptHandler.settings);
      this.customMessage = setts.value( MyMultipletReporterSettingsKey, "My Multiplet
Reporter" );
      this.name = "My Multiplet Reporter";
      this.onlvElementName=false;
// Define font size and font family
      this.font = "<font style=\"font-size: 10pt; font-family: Times New Roman\">";
      this.nucleusTemplate="%1";
// Report header. %1 will be raplaced with nucleusString, %2 with frequency, %3 with
solvent
      this.header = this.customMessage+" %1 NMR (%2 MHz, %3) δ ";
      //this.header = "Custom %1 NMR (%2 MHz, %3) δ ";
// Multiplet templates. %1 - delta, %2 - category, %3 - nH
      this.reportRange = true; // set to true to get multiplet range instead of delta.
      this.withoutJsTemplate = " %1 (%2, %3H)"; // multiplet template without J's
this.withJsTemplate = " %1 (%2, %4, %3H)"; // multiplet template with J's
      this.rangeTemplate = "%1 – %2";
// J's list template. %1 - list of J's
      this.jListTemplate = "<i>J</i> = %1";
      this.jPrecision = 1; // J's precision
      this.deltaPrecision = 2; // delta precision
      this.mSeparator = ", "; // multiplet separator
      this.jSeparator = ", "; // J's separator
      this.start = "<html><head><title>Multiplet Report</title></head><body>" + this.font;
      this.end = ".</font></body></html>";
MyMultipletReporter.prototype = new MultipletReporter();
MyMultipletReporter.prototype.toString = function() { return "MyMultipletReporter()"; }
//This line adds my custom reporter to the list of reporters, this means that this reporter
can be used by the general functions like reportMultipletsUser or automaticMultipletReport
and it can be used to generate reports from the Multiplets Table
Env.MultipletReportersArray.push(new MyMultipletReporter());
//Uncomment this line to make this reporter the default reporter, the saved settings will be
ignored, the user will not be able to modify the reporter from MNova
//Env.DefaultMultipletReporter = "My Multiplet Reporter";
//This function can be used to generate multiplet reports
function customReportMultipletsUser(createItem)
      var multipletTable = new MultipletTable(nmr.multipletTable()); // Get table of
multiplets
      var spectrum;
      if(multipletTable.isValid())
            spectrum = new NMRSpectrum(multipletTable.spectrum()); // Get spectrum currently
shown in the table of multiplets
      else
            spectrum = new NMRSpectrum(nmr.activeSpectrum());
      if( spectrum.isValid() )
            var reporter = MultipletReporter.getReporterByName("My Multiplet Reporter");
            return reporter.report(spectrum, createItem);
      else
            return undefined;
```

```
//Uncomment this line to use the previous function to report multiplets instead of the
default one
//Env.ReportMultipletsUser = customReportMultipletsUser;
//Function to setup my reporter
function customReportMultipletsUserSetup()
      var rep = MultipletReporter.getReporterByName("My Multiplet Reporter");
      var diag = new Dialog();
      diag.title = "Custom Setup";
      var lEdit = new LineEdit();
      lEdit.text = rep.customMessage;
      diag.add(lEdit);
      if(diag.exec())
            rep.customMessage = lEdit.text;
            settings.setValue( MyMultipletReporterSettingsKey, rep.customMessage );
      }
//Uncomment this line to use the previous function to setup the report multiplets
//Env.ReportMultipletsUserSetup = customReportMultipletsUserSetup;
```

Firstly, we are going to change the name of the 'Multiplet Reporter' and the message which appears at the beginning of the Multiplet Report (customMessage) to 'My Report' and 'My Journal' respectively' (see the text below highlighted in yellow)

```
/* This creates a Custom Multiplet Reporter */
function MyMultipletReporter()
{
    MultipletReporter.call(this);
    var setts=new Settings(Application.mainWindow
.scriptHandler.settings);
    this.customMessage = setts.value( MyMultipletReporterSettingsKey,
    "My Journal" );
    this.name = "My Report";
    this.onlyElementName=false;
```

**this**.onlyElementName=false; changing false with true, we will obtain only the element name without the atomic mass (For example: H, C instead of <sup>1</sup>H, <sup>13</sup>C).

The function: **this**.font = "<font style=\"font-size: 10pt; font-family: Times New Roman\">"; will define the font size and the font family of the multiplet report.

We are going to change the font of the multiplet report to 14pt and Arial:

```
// Define font size and font family
    this.font = "<font style=\"font-size: 14pt; font-family: Arial\">";
```

The line: this.header = this.customMessage+ "%1 NMR (%2 MHz, %3) δ "; is used to print the header of the report, where %1 will be the nucleus (H or C), %2 the frequency of the spectrometer (in MHz), and %3 the solvent, followed by a delta symbol ( $\delta$ ). For example: "1H NMR (500 MHz, CDCl<sub>3</sub>) ".

Let's modify the header of the report by putting the 'delta' symbol in italic:

```
// Report header. %1 will be replaced with nucleusString, %2 with
frequency, %3 with solvent
    this.header = this.customMessage+" %1 NMR (%2 MHz, %3) <i>&delta;</i>
";
```

We can also modify the way to report the multiplet infomration

```
// Multiplet templates. %1 - delta, %2 - category, %3 - nH
this.reportRange = true; // set to true to get multiplet range
instead of delta.
this.withoutJsTemplate = " %1 (%2, %3H)"; // multiplet template
without J's
this.withJsTemplate = " %1 (%2, %4, %3H)"; // multiplet template
with J's
this.rangeTemplate = "%1 – %2";
```

The sentence: **this**.reportRange = true is used to obtain the multiplet range instead of the chemical shift.

The functions: **this**.withoutJsTemplate = "%1 (%2, %3H)" and **this**.withJsTemplate = "%1 (%2, %4, %3H)" are used to customize the appearance of the multiplet report by changing the positions of %1, %2, %3H, or %4 (where, %1 means: chemical shift; %2 means: type of multiplet (s, d, t, etc); %3H means: number of hydrogens and %4 means the coupling constant value). As you can see, the first line shows a multiplet without coupling constants, (while the last line shows a multiplet with coupling constants).

So, if you need to obtain something like this (japanese format):

1H NMR (300 MHz, Solvent) δ ppm 6.43-6.22 (1 H, m), 3.17 (1 H, q, J = 7.15 Hz) etc...

You should modify both lines, as you can see below:

this.withoutJsTemplate = %1 (%3H, %2)"; this.withJsTemplate = " %1 (%3H, %2, %4 Hz)";

If you prefer to obtain something like this:

1H NMR (300 MHz, Solvent)  $\delta$  ppm 1.23 (d, J = 1.2 Hz, 3 H), etc...

Just replace the original lines with:

this.withoutJsTemplate = %1 (%2, %3H)"; this.withJsTemplate = " %1 (%2, %4 Hz, %3H)";

You can also customize the coupling constant format:

```
// J's list template. %1 - list of J's
    this.jListTemplate = "<i>J</i> = %1";
    this.jPrecision = 1; // J's precision
    this.deltaPrecision = 2; // delta precision
    this.mSeparator = ", "; // multiplet separator
    this.jSeparator = ", "; // J's separator
    this.start = "<html><head><title>Multiplet Report</title></head><body>"
+ this.font;
    this.end = ".</font></body></html>";
}
```

To obtain the coupling constant symbol in normal instead of *'italic'*, just modify the script by removing the italic format (<i>J</i>). If you prefer to obtain it in **"bold**" just type:

```
this.jListTemplate = "<b>J</b> = %1";
```

```
To add a superscript to get for example: <sup>3</sup>J:
this.jListTemplate = "<sup>3</sup><i>J</i> = %1";
```

The following paragraph will be used to customize the appearance of the coupling constants list:

The second line is used for the precision of the coupling constants values, the next will be used for the precision of the chemical shift and the remaining two lines will print the separation (coma, colon, dots, etc.) between the multiplets and the coupling constants values.

If you need to obtain the coupling constants in descending order, replace 'true' with 'false' in the following line:

var jList = new JList(multiplet.jList());
jList.sort(true);


To obtain the multiplet range in ascending order, just replace the rangeMin with rangeMax in the below line of the script:

shiftStr = **this**.rangeTemplate.argDec(multiplet.rangeMax, 0, 'f', **this**.deltaPrecision).argDec(multiplet. rangeMin, 0, 'f', **this**.deltaPrecision);

You can select a multiplet report format as the default one, without allowing the user to modify it, just by removing the two slash symbols (before this sentence: **Env**.DefaultMultipletReporter = "My Multiplet Reporter";). Please bear in mind that if you do that, you will not obtain any dialog box when you follow the Menu 'Multiplets Table/Report Special/Setup'.

```
//Uncomment this line to make this reporter the default reporter, the
saved settings will be ignored, the user will not be able to modify the
reporter from MNova
Env.DefaultMultipletReporter = "My Multiplet Reporter";
```

Indeed, the variable **'Env'** contains several environment variables which can be used to customize the Mnova behaviour. Typing print(Env) in the Script editor, you will get the list of the available variables. In the example below, we have only defined the 'Setup' of the 'Multiplet Reports'. All the remaining variables are 'undefined'.

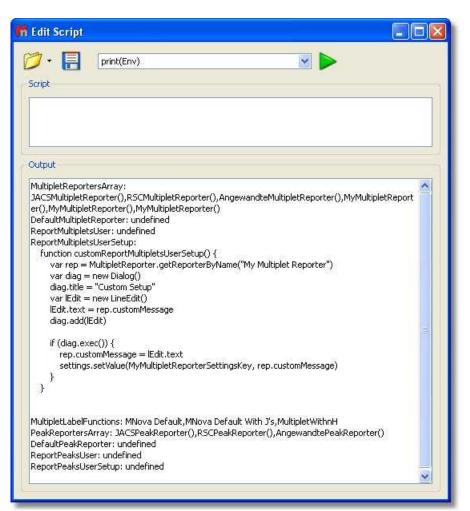

You can define the 'DefaultMultipletReport' variable by uncomment this line in the script: Env.DefaultMultipletReporter = "My Multiplet Reporter";

Doing that, the user will not be able to modify the multiplet report.

You can define the '*ReportMultipletUser*' variable by uncomment this line of the script: **Env**.ReportMultipletsUser = customReportMultipletsUser;

Defining this variable, you will have a format for the 'multiplet report' and the 'copy special' and another different (the default one) for the report which appears on top of the 'multiplets table'.

The '*ReportMultipletUserSetup*' is the variable defined in the menu 'Multiplet Table/Report Special/Setup' for the 'Multiplet Report'.

The 'MultipletLabelFunctions' are different options (showed in the <u>'Multiplet Properties'</u> dialog box) which allow the user to customize the information which appears in the multiplet boxes.

## 9.4.6 Multiplet Analysis options

Follwing the menu 'Analysis/Multiplet Analysis/Options' will display the applicable dialog box:

General	ОК
Minimum Area: 3.00 % 🚔	Cancel
Integral Calculation Calculation Method:	Restore Defaults
Peaks 🔹	
Method Parameters	
Excluding: Default	

From here you can select the minimum area and the integration calculation method (Peaks, which uses GSD, Sum, which is the classical integration method and 'Edited Sum' which uses the traditional integration and the peak classification from GSD, discarding impurities and solvents from the area calculation) and also to select what kind of peaks will be take into account for the multiplet analysis. By default **only compounds peaks** will be, so the solvent peaks will not affect to the multiplet analysis (very useful for example if a solvent signal overlaps with a compound peak).

When running automatic multiplet analysis using Sum or Edited Sum methods the multiplet ranges will not overlap.

## 9.4.7 Multiplets Properties

The user can modify the properties of the **Multiplet Analysis** by following the menu 'Edit/Properties/ Multiplet Analysis' or by double clicking the left mouse (or pressing the right mouse) button on the spectrum display and selecting *Properties/Multiplets* from the *pop-up* menu.


Then, the user can choose the color, line width, decimals for the shifts and coupling constants, the font and the margin of the 'Multiplet' boxes.

Integrals     Multiplets       Multiplets     Fitting       Assignments     Prediction	<ul> <li>Multiplets Labels</li> <li>Font:</li> <li>Line Width:</li> <li>Label:</li> <li>Shift Decimals:</li> <li>Js Decimals:</li> <li>Margin:</li> <li>Follow Peak Visibility Rules</li> <li>J's Tree</li> <li>Show Label</li> </ul>	MS Shell Dig 2 2.5 2 2 50 % V Show Label Box	
--	---	---	--


If the spectrum contains peaks belonging to more than one compound, we can show only the peaks assigned to one of them by <u>filtering</u> the desired peaks in the Peaks Table. Checking the 'Follow Peak Visibility rules' box will allow you to show only the multiplet boxes applicable to those visible peaks.

You can also hide the multiplet square box by unchecking the applicable box.

The user will be able to display the coupling constant tree just by checking the applicable option. Here you can see an example:

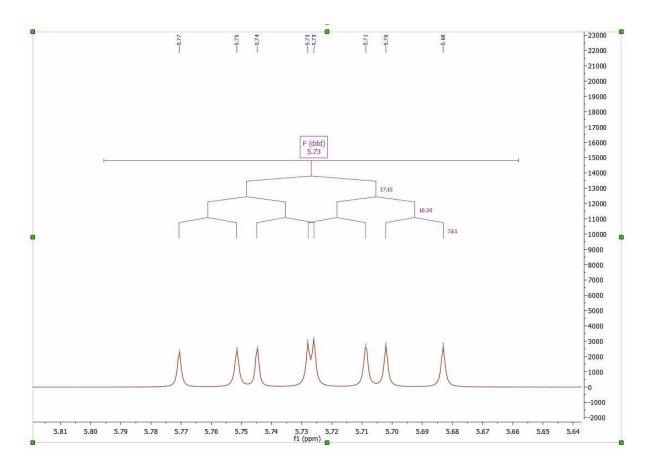

These objects are mouse sensitive in the case of predicted spectra, making possible the graphical edition of both the chemical shift and couplings by using drag & drop.

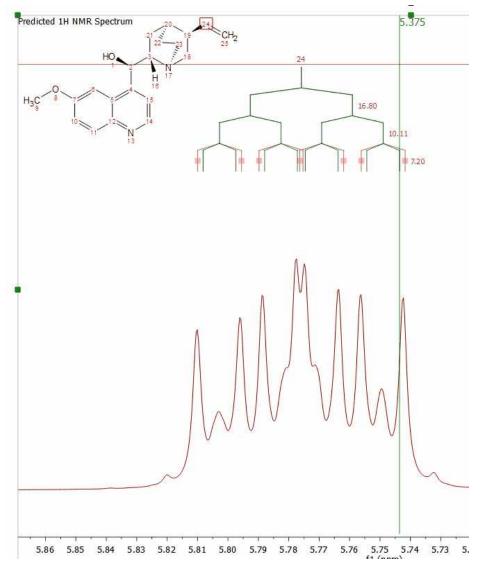

You can modify the information of the multiplet label by selecting the desired option in the scroll down menu:

idth: 2.5
idth: 2.5
Name (Category) / Shift / NN / Integral
Name (Category) / Shift Name (Category) / Shift / Nuclides Name (Category) / Shift / Integral
Name (Category) / Shift / NN / Integral Name (Category) / Shift / J's
ì


You can also add new labels by using the scripting feature. You will see below a script to show multiplet labels with the number of Hydrogens. You will find another example in the 'Examples/Scripts' folder of Mnova.

Filename: MultipletLabel with nH.qs         Script         function customMultipletLabel()         {         MultipletLabelReporter.call(this);         this.name = "Multiplet Label with nH";	-
{ MultipletLabelReporter.call(this);	^
this.name = "Multiplet Label with nH"; }	
customMultipletLabel.prototype = <b>new</b> MultipletLabelReporter(); customMultipletLabel.prototype.report = <b>function</b> (aMultiplet) {	
<pre>var multLabel = new String("%1(n%4"); multLabel = multLabel.replace("%1",aMultiplet.name).replace("%2",aMultiplet.category).replace("%3",aMultiplet.delta.toFixed(2)).replace("%4",aMultiplet.nH); return multLabel;</pre>	100
} Env.MultipletLabelFunctions.push( new customMultipletLabel() );	*

You will only need to save this script in a folder where Mnova can find it ('Edit/Preferences/Scripting/Scripts Directories) and after having restarted the software, you will get the new entry in the 'Multiplet Label' scroll down menu of the 'Properties' dialog box.

You can see in this <u>Scripts chapter</u>, all the multiplet properties which you can include in the 'multiplet label'.

Adding the above script to the Mnova scripts directories, you will obtain your multiplet labels as you can see in the picture below:

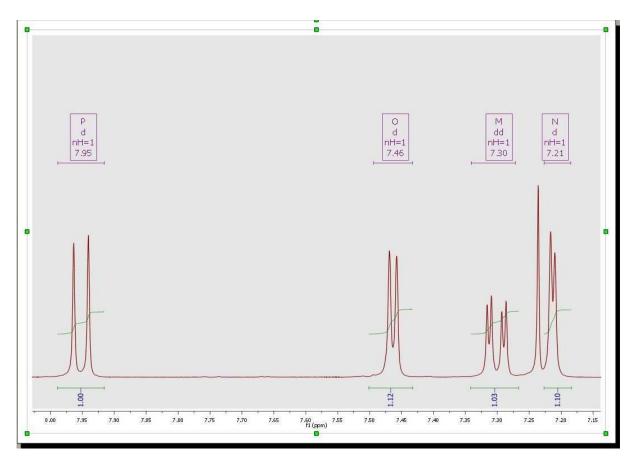


The user can also show the Multiplet Integrals Curves and customize the appearance. Please bear in mind that integrals and multiplets are two different list, so you can select what integrals you want to show (the 'pure integrals' or the integrals existing under the multiplet ranges):

1D Scales Horizontal Vertical Peaks Multiplets Multiplets Fitting Assignments	Decimals: Position: Margin: Curve Color: Line Width: Position: Maximum Height:	2 ★ On Segment ★ 2 % ★ 2 % ★ 2.5 ★ 86 % ★ 40 % ★
---	---	--

## 9.4.8 Importing spectral data from literature to synthesize a spectrum

To synthesize a spectrum from a multiplet report (copied from a paper); you will only need to copy to clipboard the multiplet report and follow the menu 'Scripts/NMR Tools/Multiplet Report to Spectrum':

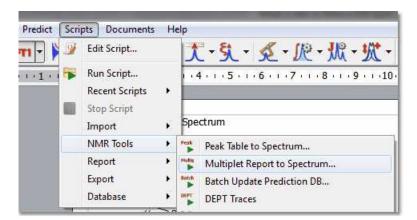


This will display a dialog box to paste your multiplet report. For example, let's paste the report below:

1H NMR (400 MHz, CDCl3) 6.65 (d, J = 8.2 Hz, 1H), 6.56 (dt, J = 8.2, 1.0 Hz, 1H), 5.70 (dddd, J = 9.9, 3.2, 1.9, 1.3 Hz, 1H), 5.33 - 5.24 (m, 1H), 4.88 (dd, J = 6.6, 1.3 Hz, 1H), 4.17 (s, 1H), 3.84 (s, 2H), 3.84 (s, 2

3.34 (dd, J = 6.3, 3.2 Hz, 1H), 3.04 (d, J = 18.7 Hz, 1H), 2.90 (d, J = 10.0 Hz, 1H), 2.66 (p, J = 2.9 Hz, 1H), 2.62 – 2.53 (m, 1H), 2.43 (s, 3H), 2.44 – 2.33 (m, 1H), 2.34 – 2.23 (m, 1H), 2.05 (td, J = 12.4, 5.1 Hz, 1H), 1.87 (ddd, J = 12.6, 3.7, 1.8 Hz, 1H).

5.7 Hz 1H 3H	70 (dddd, J = 9. , 1H), 4.17 (s, 1 ), 2.90 (d, J = 1	9, 3.2, IH), 3.8 10.0 Hz m, 1H),	1.9, 1.3 H 4 (s, 2H), 1 , 1H), 2.66 2.34 - 2.2	, J = 8.2 Hz, 1H), 6 z, 1H), 5.33 – 5.24 3.34 (dd, J = 6.3, 3 (p, J = 2.9 Hz, 1H 23 (m, 1H), 2.05 (to	(m, 1H), 3.2 Hz, 1H ), 2.62 – 2	4.88 (dd, J = I), 3.04 (d, J 2.53 (m, 1H),	6.6, 1.3 = 18.7 Hz, 2.43 (s,
ars	ed Multiplets						
_	Shift (ppm)	NN	Class	jList	Atom	Line Widt	th (Hz)
1	6.65	1	d	8.2		0.75	
2	6.56	1	dt	8.2,1.0,1.0		0.75	
3	5.70	1	dddd	9.9,3.2,1.9 <mark>,1.3</mark>		0.75	,
۲	Ú		.11	Ľ.			•
iuc iolv ipe	ed Parameters leus: 1H vent: CDCl3 ctrum Simulation ctrum Size: 32 olfile			-2.00 ppm	Freque	ency: 400.0	0 MHz 🌻 0 ppm 🌻
	] Use Prediction	n to Sim	ulate m's				


After having clicked on the OK button, we will get the synthetic spectrum:

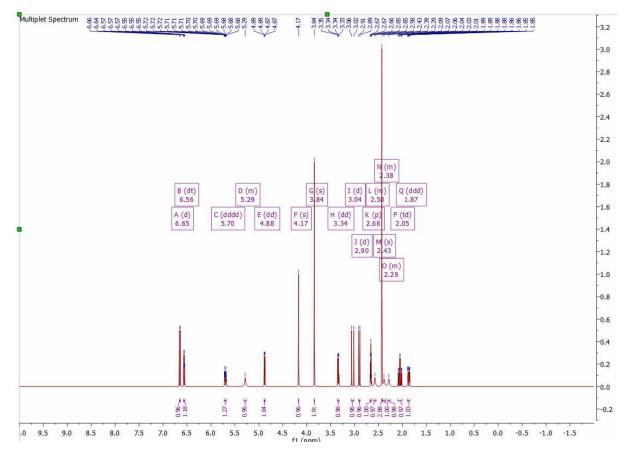

By the default the 'not defined multiplets' (labelled as 'm') will appear as 'broad singlets', however you can predict the multiplet shapes by loading a mol file and selecting the atom numbers for each multiplet (labelled as 'm') in the table:

	, 1H'), 1.87 (ddd, J sed Multiplets	- 12.3, 3,	7, 1.7 (12,	шŋ.			
	Shift (ppm)	NN	Class	jList	Atom	Line Width (Hz)	
4	5.285	1	m		14	9.00	_
5	4.88	1	dd	6.6,1.3		0.75	E
6	4.17	1	s			0.75	
7	3.84	3	s			0.75	
8	3.34	1	dd	6.3,3.3		0.75	
Nuc Solv Spe	sed Parameters deus: 1H vent: CDCl3 ctrum Simulation Par actrum Size: 32768 olfile		From:	-2.00 ppm	F	requency: 400.00 MH; 10.00 ppm	


In the example above, we have assigned the multiplet at 5.29 ppm to the H-14 (and also the multiplets belonging to H-20' and H-20''), we loaded the mol file and checked the option to 'predict' the shape for those assigned multiplets. Here you can see the result:

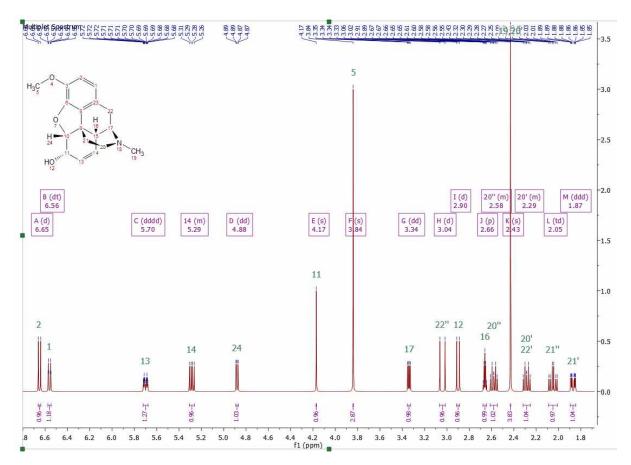

For further information, please see this video and take a look at this post

# 9.5 Automatic Analysis

This feature runs a multiplet analysis in 1D spectra and peak picking in 2D spectra using all the context information (molecule item, other NMR items...):

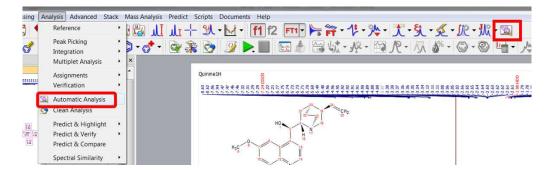

## 9.6 How to carry out assignments?


You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder)

You can carry out automatic assignments and atom to peak assignments both to 1H, 13C and HSQC spectra.

Automatic Assignment of NMR spectra has been a pipedream for many years, especially in the organic chemistry community. In spite of successful applications of computer algorithms for the automation of the processing and analysis of NMR spectra, fast and robust unsupervised assignment of NMR spectra of small molecules has so far been a discouraging endeavor.


See this **publication** for further information.

**Mnova** provides a very simple interface to automatically assign your molecule. Just load your NMR spectrum (1H, 13C and HSQC; alone or combined) with the applicable molecular structure and follow the menu 'Analysis/Auto Assignments':

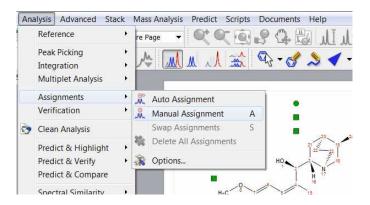


Mnova will automatically run a multiplet analysis and will fully assign your spectrum with the applicable molecular structure. If you have a license of the <u>prediction plugin</u>, the assignments will be more accurate.

The multiplet boxes will be renamed with the corresponding atom number of the molecule and you will get an assignment label with the atom number over the applicable peak (including a colour quality coding). In addition, hovering the mouse over the atom will highlight the applicable signal in the spectrum:

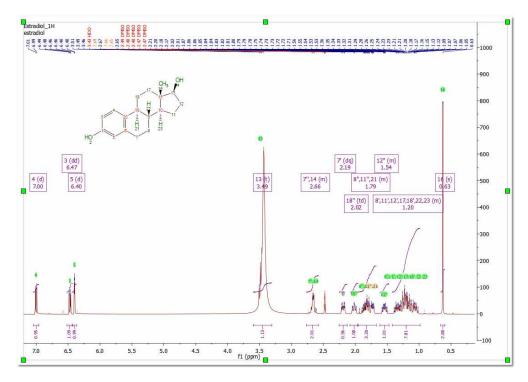

This algorithm for automatic assignment of NMR spectra has to be understood as a quick method to generate an initial 'rough' assignment that in some cases will require manual intervention from the user to easily amend any potential incorrect auto-assignment.

The auto-assignments could assign, for example, all the protons properly except two which are swapped (as illustrated in the figure below) where assignments (3) and (6) must be swapped.

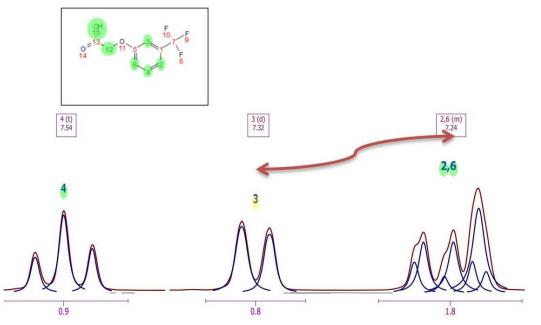


You can **swap assignments** by following the menu 'Analysis/Assignments/Swap Assignments' (shortcut: S). Then you will only need to click on one assignment label (or multiplet box) and drag and drop it to the target assignment label (or multiplet box).

If the target multiplet has more than one assignment, you will be asked for which assignment must be

used for swapping.


### MANUAL ASSIGNMENTS

**Mnova** provides a very simple interface to manually assign your molecule. Open your NMR spectra in the same document and load/draw the molecule structure. Next, follow the menu 'Analysis/Assignments/Manual Assignments' (or use the shortcut 'A').




Finally, click on an atom in the molecular structure (or a spectrum region) and then release the mouse and drag it to your desired peak, peak range, multiplet box or integral curve. We recommend you to assign your atoms to your multiplet boxes in order to <u>transfer assignments through datasets</u>.

With the 'Assisted Assignment mode' (which works for 1H and 13C spectra having a multiplet analysis) , a 1H and 13C predictions are made in the background. When hovering the mouse over the atoms of the molecule, the suggested multiplets in the spectrum will be highlighted (following a color code: green, yellow, red, gray- depending on the quality: grey: -1 to -0.5; red: -0.5 to -0.25; yellow: -0.25 to 0.25; green: 0.25 to 1) and viceversa if you hover the mouse over the multiplet boxes, the suggested atoms in molecule and compounds table will be also highlighted. This feature can be disabled from the 'Assignments options'.

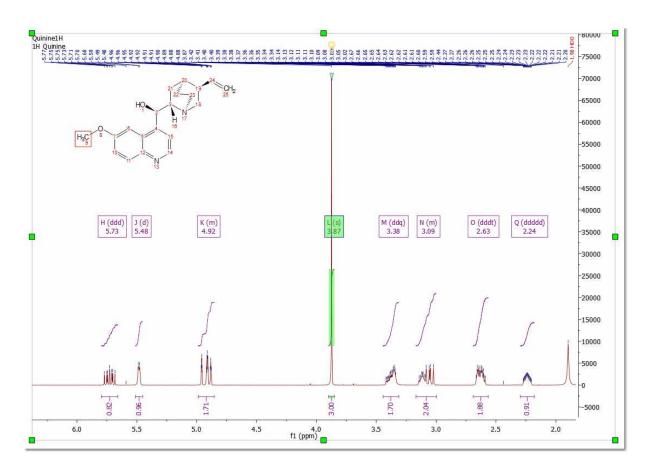

Note: Hold down the 'Ctrl' key and click, to select several atoms at a time.


This multiplet will now be assigned to the atom (which will turn to green). Once the assignment has been made, you will get an atom number label on the chemical shift (with quality colour coding). Hovering the mouse over the atom will highlight the applicable peak in the spectrum and hovering the mouse over the peak will highlight the corresponding atom on the molecular structure. To customize the assignments labels, click <u>here</u>.

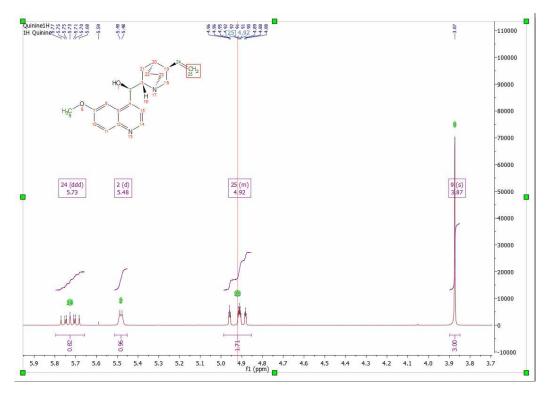

If you do not want to show the assignments labels or the quality colour coding; just uncheck the applicable option from the <u>'Assignments Properties'</u> dialog box


The user can also assign a region of the spectrum just by clicking, dragging and releasing the mouse over the desired region. In the example below, we have assigned a  $-CH_2$  group, so a new window will

be displayed to allow us to select which atom we want to assign, 18, 18', both (in blank) or even we can select any other annotation: 18a, 18b, cis/trans, ax/eq,  $\alpha/\beta$ :




You can assign a 13C-NMR spectrum of the same molecule in the same document. To do that, select the atoms from the 'Molecule Window' panel by following the menu 'View/Panels/Molecule Window' (or from the Compounds Table; from 'View/Tables')


To keep the assignments propagation, follow the menu <u>'View/Tables/Assignments'</u> and make sure that the desired are linked (in the example below, we have selected the 1H, 13C and HSQC).

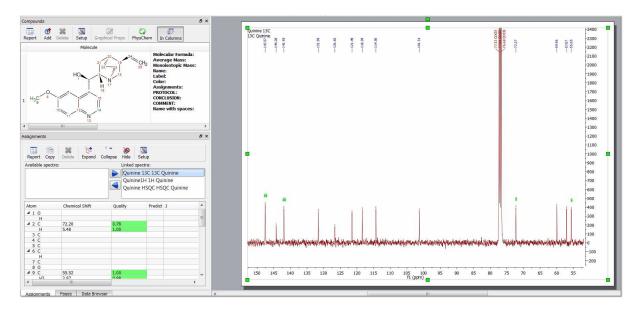

If your document has more than one molecule (see also this tutorial), use the compounds table to select a different colour for the assignments of each compound. In the example below the assignments labels of the quinine appears in blue and the assignments labels of the EtOAc are green (make sure that 'Use Compound color' is checked in the Assignment Properties):

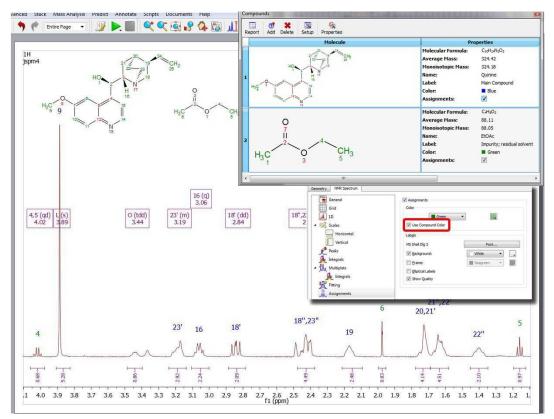

If your document contains more than one compound, you can select the compound for each peak from the Peaks Table (by clicking on the 'Set Compound' button or by double clicking on the 'Impurity/Compound' cell). The same effect will be obtained by right clicking on the Peak label and selecting 'Set Peak Compound' (please make sure that the 'Use Curve Color' box is checked in the 'Peaks Properties'):

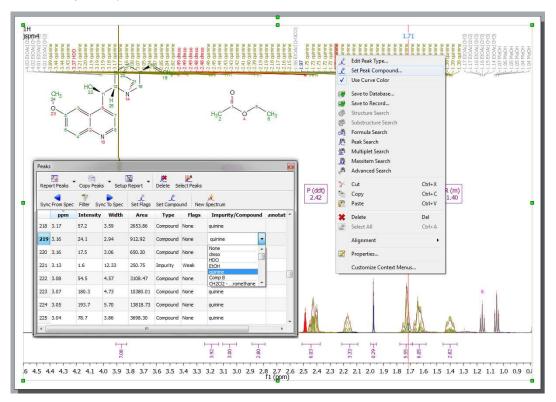

#### **Rules for 1D assignments:**

#### For 1H assignments:

-CH2 atoms with diastereotopic protons: assign the not assigned proton first.

-Show the Assign dialog (automatically) when both protons are assigned and the user wants to assign again the same atom. (Options Add/Replace/Keep Original)

-Other atoms: assign all protons to the same chemical shift. Replace the chemical shift when the user wants to assign again the same atom.

#### -Other nucleus:


Assign to the selected chemical shift. Replace the shift value when the user wants to assign again the same atom.

Note: when the user assigns a diastereotopic proton, the notation is ', " by default. It can be changed in the Assignments Table, if the user doesn't want to use the dialog.

The user can force the visualization of the Assign Dialog pressing the Alt key together with the second click of the mouse (when assigning).

# Assignments in 2D


Once you have assigned the 1H and the 13C spectra, if you jump to a 2D-NMR spectrum (in the same Mnova document) you will see the assignments graphically on the screen. In the example below, you can see the correlation between the two hydrogens and the C-12 in a HSQC:

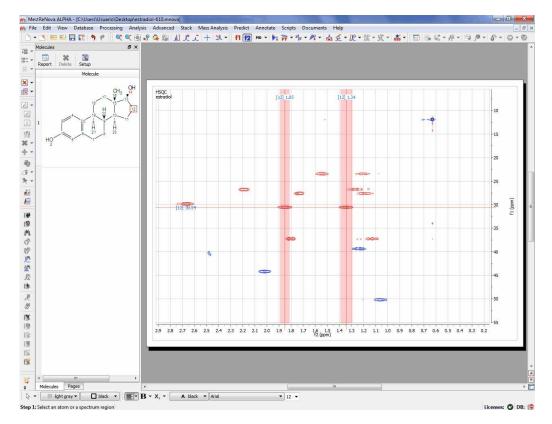

From the Assignments options, you can use the 1H multiplet shift when you assign a 2D spectrum:

<ul> <li>Show the suggested assignments</li> <li>Always use the 1H multiplet shift when adding 2D assignment</li> </ul>	Manual Assignment	
Always use the 1H multiplet shift when adding 2D assignment	Show the suggested assignments	
		ding 2D assignment

To carry out assignments to 2D spectra, type the applicable number of the atom in the 'Assignments Table' or **graphically** select the atom in the molecule structure and the applicable signal (peak label or chemical shift) in the 2D:

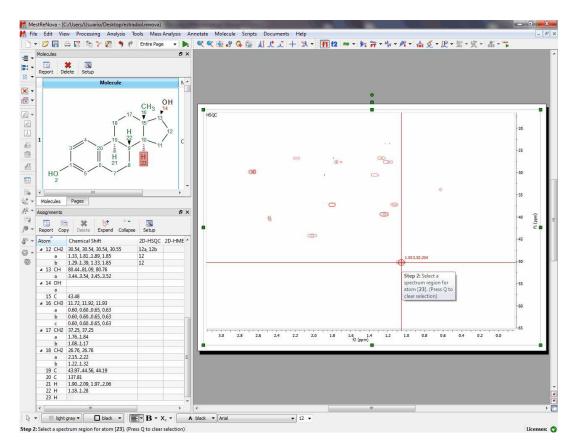


Once an assignment is made in a 2D spectrum, this assignment will be **transferred** to the applicable **multiplet** box in the 1H spectrum:

If you had already assigned the atoms in the 1D datasets and you assign in the 2D, the assignment will be replaced. You can force the visualization of the Assign Dialog pressing the Alt key together with the second click of the mouse (when assigning); so you will be allowed to keep the assignments from the 1D, replace or add new assignments:

<ul> <li>Assign f2</li> <li>Single Peak,</li> </ul>	/Range	
Atom: 9	- δ	i(1H): [f2=3.88 ppm 🔹
Already ass	igned (9):3.71	🔘 Keep Original
问 Multiple Pea	ks	
Shift (	1H) Atom	
1 3.876	9	

Finally click on OK and hover the mouse over the atom to see the result (please notice how the

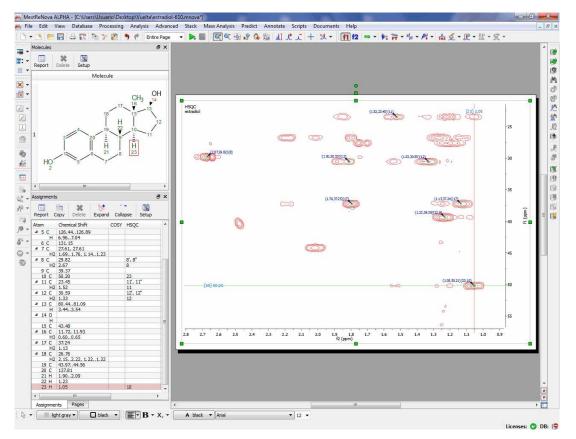

assignment table has been automatically filled with the number '10' in the HSQC column, in order to show the correlation between the C-10 and the H-23)

If you are working with a HMBC, you could assign one of the protons and then all the 13C in the same step (by selecting 'Multiple Peaks' from the panel):

	im 24: 💽 🔹	δ(1H): f2=4.8	83 ppm		_
	1 - Tel - St. 4	🔘 Add	0	Keep Origina	al I
0	Assign f1 Single Peak/Range tom: Select In Mo	elecule *	δ(13C):	f1=35.8 ppm	
)	Multiple Peaks				
)	Multiple Peaks Shift (13C)	Atom			
1		<b>Atom</b>	I IIII		
1	Shift (13C)				
1	Shift (13C) 36.031	21			

Alternatively, you could assign only one of the carbons and the next times that you need to assign carbons to the same proton, you will not need to select again the applicable proton (as it is already assigned). If you have overlapping in the proton dimension, you could hold down the Alt key and click to get the 'Assign' dialog displayed which will allow you to select any other proton.

#### **Rules for 2D assignments:**

<u>HSQC C-H (HSQC, HSQC EDITED, HMQC, HETCOR)</u>: Assign the dimension/s not assigned to the 2D position (or the 1H multiplet shift if the user has the option "Always use the 1H multiplet shift when adding 2D Assignments" selected). When the Carbon/Protons/both of the selected atom are already assigned, the current chemical shift is replaced by the new value. (correlations, Js, NOEs, RDCs change according with the new shifts).

The Assign Dialog is only shown (automatically) when the user wants to assign a CH2 atom with diastereotopic protons and the carbon and the two protons are already assigned.

#### HMBC C-H (HMBC, H2BC): Two ways of assigning:

#### -selecting only one atom in the molecule

-selecting two atoms in the molecule, the ones of the correlation. It works selecting first the spectrum, second a first atom in the molecule, and then, a second atom. And also selecting first one atom, then the spectrum, and then the molecule again.

When the user selects a 2D position in the spectrum already assigned to the f2 dimension, the program expects only one click on an atom. The f1-element of the selected atom is assigned to the f1 value. The correlation is added.

Same behaviour when the selected 2D position is already assigned in the f1 dimension.

When the 2D position is not assigned in f2 nor in f1, the program expects two clicks in the molecule. The assignment (and the correlation) are made to the f2-element of the first atom and the f1-element of the second atom.

The same rules are applied when assigning NH or OH groups.

Assign Dialog is shown (automatically) in this cases:

-The 2D position is assigned in both dimensions.

-The 2D position is not assigned in any dimension and the first atom doesn't contain f2-elements. -The 2D position is assigned only in f1 (not assigned in f2) and the selected atom doesn't contain f2-elements.

-The 2D position is assigned only in f2 (not assigned in f1) and the selected atom doesn't contain f1-elements.

COSY (COSY, DQF\_COSY, NOESY, ROESY, TOCSY):

Same identical rules described in the first 4 points of the HMBC case Assign Dialog is shown (automatically) when:

-The 2D position is assigned in both dimensions.

When assigning a NH2 to a proton, COSY, TOCSY or HMBC spectrum, both proton are assigned to the selected position.

-If you want to assign only one of the two protons of the NH2, you need to press Alt+the second click when assigning. The Assign Dialog is shown and you can choose '-", a-b, cis-trans, etc.

- Once you have one of the NH2 protons assigned, the corresponding partner is chosen by default when selecting the same atom to assign the other proton.

In the three cases (HSQC, HMBC, COSY) when the user selects a CH2 atom with diastereotopic protons, the assignment is produced always to the first not assigned proton.


General behaviour for all 2D spectra: in the case the Assign Dialog is shown and the user chooses the option "Select in molecule", if the user selects a CH2 atom with diastereotopic protons, only the first not assigned proton is assigned.

So the assignments behavior is different depending on the assignments that you have in F1 and F2: - If you do not have any assignment; the first assignment that you will make will go to F2 and the next for F1.

- If the peak is already assigned in one of the dimensions, when you make the assignment, Mnova waits only for the selection of one atom (in the dimension which is not assigned) in order to complete the information. If you do not want to do it, you would need to do 'ALT+clic' to launch the 'Assign dialog '


- If the peak is already assigned in both dimensions and you try to assign it to another atom; the 'Assign dialog' will appear (as Mnova does not know what you need to do).

You can graphically visualize (by arrows between the coupling groups) the HMBC, ROESY, NOESY, COSY, TOCSY, H2BC and connectivity in the structure. To do it, double click on the molecular structure to display the 'Properties' and select the 'Arrows' tab to check the desired correlation arrows:

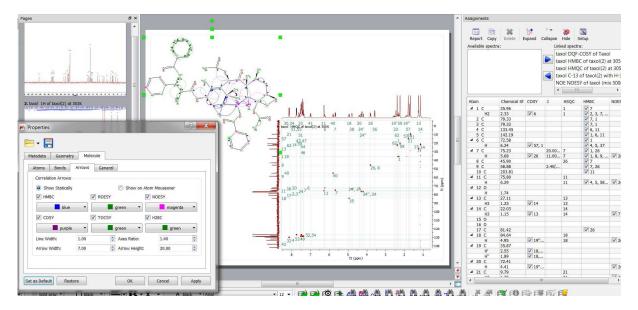


The Assignments table shows checkboxes for each row in the correlations that can be displayed as arrows in the molecule. Checking/unchecking these checkboxes will change the visibility of the correlations for each atom.

Right clicking on the atom will allow you also to 'Hide Correlations'; you can show them again by using the command 'Display Hidden Correlations'.

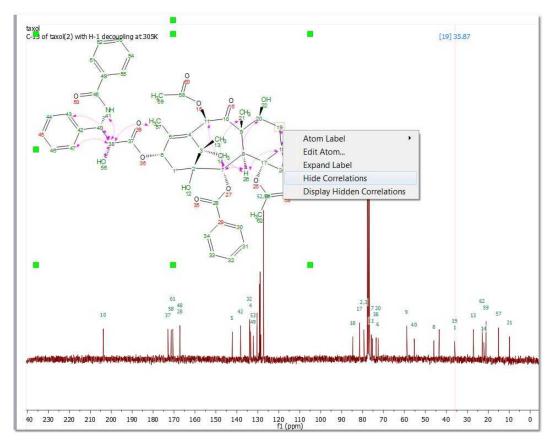


You can also copy several datasets in the same page (and after having resized them) to make the

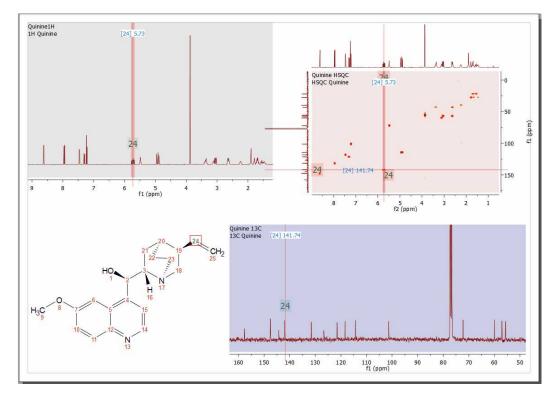


assignments. Here you can see a page which contains a 1H, 13C and HSQC datasets with an assignment in the molecular structure:

Follow the menu 'Scripts/Report/Assignments' to **export your assignments** in journal format. Then, a new dialog will appear, to allow you to report the 2D correlations and the chemical shifts or to copy only the report to the clipboard (to paste it to another document) or export it as CSV or HTML file. From here you can also order by chemical shift, include 13C and X-nuclei assignments or multiplicity. When no chemical shift is included, the correlations get ordered according to the atom number. When chemical shifts are included, the correlations get ordered according to the chemical shifts values.

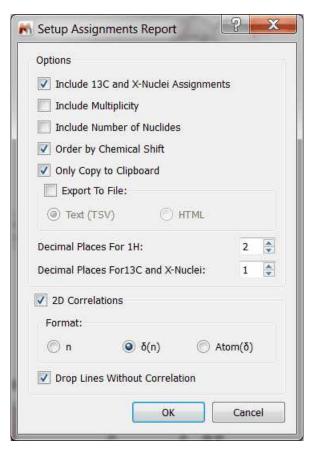

It is required at least a 1H spectrum. The table only will include columns for the spectra present in the document containing assignments. It generates a table in which each row corresponds to each non-equivalent proton.

Finally, you will get the report of the assignments pasted on the spectral window:

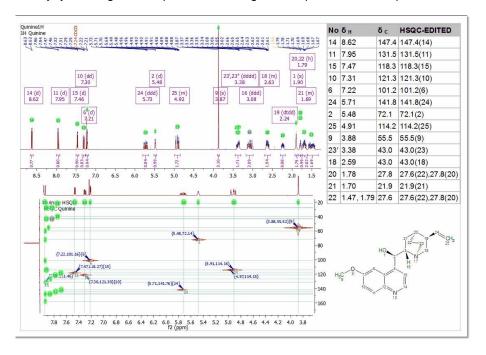


You can export the assignments as an ASCII file by following the menu 'File/Save As/Script:Assignments' or <u>copy the assignments</u> from one molecule to another (with the same numbering of the common parts).

### See also this post

### 9.6.1 Assignments Table


Once you have finished with the assignment, you can visualize the assignment list by following the menu 'View/Tables/Assignments'. From here, you can edit any entry by double clicking on it and overwriting the new value. Hovering the mouse over any cell of the table, will highlight the signals on the spectrum and the atom on the molecular structure.

Bear in mind that you can carry out the peak assignment directly from this table by typing the applicable chemical shift in the edit box.

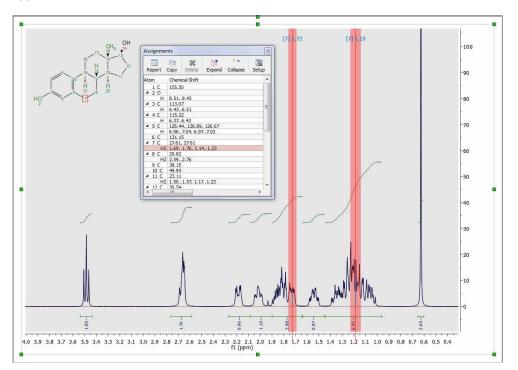

If you use the Assignment table to type directly the assignment of a  $CH_2$  you would need add the prime marks if you want to assign only any of the two protons. If you do not type the prime marks, the assignment will be applied to both protons.

For example; typing this in a CH2 row: **3.0**, **3.5'**,**3.7''** means that 3.0 ppm is the chemical shift of both protons and in addition the H' has a signal at 3.5 ppm, whilst H'' appears also at 3.7 ppm. The assignments table will automatically refresh showing something like this (after having typed: **3.0**, **3.5'**,**3.7''**):



Double click on the applicable 'atom cell' to change the label of a -CH2 group. You can also change the atom number by double clicking on the applicable atom cell:

Report	Сору	Delete	Expand	o 🖕	Setup	
Available	spectra:			Linked spec	tra:	
				codeine_	(3.3mg)_in_	CDCI3
Atom	~		Chemical	SI Predicte	ed S COSY	т
	H3		Chemical 2.43	SI Predicte	ed S COSY	T
	H3		2.43	SI Predicte	ed S COSY	T
	H3		2.43	SI Predicte	ed S COSY	T
<b>4</b> 20	нз С		2.43	SI Predicte	ed S COSY	T
<ul><li>20</li><li>21</li></ul>	H3 C		2.43 2.58 2.39	SI Predicte	ed S COSY	
<ul><li>20</li><li>21</li></ul>	нз С		2.43	SI Predicte	ed S COSY	T

You can do **ambiguous assignments** in a -CH2, just by typing both values in the chemical shift cell (both chemical shifts are assigned to both protons)

	FF 44	FF 65
4 8 C	55.41	55.65
H2	2.66, 3.06	3.15, 3.40
4 9 C	31,45	37.62
н	2.26	2.40
4 10 C	40.78	40.80
н	2.95	3.01
4 11 C	28.82	28.90
H2	1.27, 2.00	1.37, 1.49
4 12 C	23.30	23.10
H2	1.56, 1.65	1.78, 1.66
4 13 C	34.09	33.90
H2	1.35, 2.20	1.68, 1.93
4 14 C	48.91	51.34
H2	4.06, 4.19	4.07
4 15 C	51.93	55.80
H2	3.13, 3.41	3.40

If you want to do **unambiguous assignments** (one chemical shift belongs to proton a and the other to proton b), you will need to assign each proton:

4 8 C	55.41	55.0
Ha	2.66	3.1
Hb	3.06	3.1
4 9 C	31.45	37.0
Н	2.26	2.40
4 10 C	40.78	40.8
н	2.95	3.01
4 11 C	28.82	28.9
Ha	1.27	1.3
Hb	2.00	1.3
⊿ 12 C	23.30	23.
Ha	1.56	1.78
Hb	1.65	1.78
▲ 13 C	34.09	33.9
Ha	1.35	1.68
Hb	2.20	1.68
⊿ 14 C	48.91	51.3
Ha	4.06	4.0
Hb	4.19	4.01

Type the value of the coupling followed by the atom number involved, to include coupling constants in the assignment table. If you want to add an *ambiguous assignments*, type the coupling constant value and press the 'enter key' (a question mark will be added between brackets):

Report Copy	v Delete	Expand Collapse Hide	»
Available spect	ra:	Linked spectra:	
Atom	Chemical	S J (Hz)	RD
1 N			
2 N			
3 C			
4 C			
5 C			
46 C			
H	7.74	8.24(7), 0.80(?)	
47C			
Н	7.48	7.00(8), 8.24(6), 0.80(?)	
4 8 C			
Н	7.32	8.20(9), 7.00(7)	
⊿ 9 C			
Н	8.10	8.20(8)	
4 10 C	4.16		
H3			
H3 11 C			
H3 11 C 12 O			
H3 11 C	12.92		

The couplings will be added by pairs, in the same way as in the correlations columns, i.e., when the J(2-3) is created, the coupling J(3-2) is also automatically added, with the same value.

The table will give priority to the homonuclear couplings. Thus, when the user writes in a H row the atom number (without specify a proton), the coupling will be done between the protons. To add a coupling H-C, the user will have to write the *atomsymbol*, for example, "C". The same for the cases in which the user writes in a C row, the coupling will be done between the carbons, by default.

In the case of CH2 with no equivalent protons: the user should type the correct proton notation in the coupling. If we want to add a coupling with the first proton of  $13CH_2$ , and the notation is cis/trans, the text should be "1.20(13cis)". If we type "1.20(13')", we will get a message saying "the atom 13' doesn't


exist in the molecule".

Report Copy	X Delete	Expand Collapse Hide	,
Available spectra:		Linked spectra:	
Atom	Chemical	5 J (Hz)	
н			
5 C			
4 6 C			
Н			
47C			_
Н			1
4 8 C			
H	-		
9 C			
10 N	-		
▲ 11 C			_
Н			
12 C			_
▲ 13 C	5.00	1 20(12)	
Hcis	5.80	1.20(13trans)	
Htrans	6.03	1.20(13cis)	_
14 N 15 C			

Click on the 'Delete' button to delete any assignment selected on the table. To delete 'All the assignments', do 'Ctrl/Cmd+A' to select all the assignments and click on the Delete button. The same effect will happen if you follow the menu Analysis/Assignments/Delete All Assignments or if you right click on the molecule to display the context menu:

Ana	alysis Advanced Stack	Mass Analysis Predict Annotate Scripts	*	Delete All Assignments
↑ TMS	Reference     L       Peak Picking     D       Integration     D       Multiplets Analysis     D		Ĥ Q	1H Spectrum 13C Spectrum HSQC Spectrum X-Nuclei Prediction
	Assignments Predict & Highlight Predict & Verify	Lelete All Assignments		Update 1H User DB Update 13C User DB To X-Nuclei Database
	Predict & Compare Spectral Moments	HO 3 18	1 🕉 🗎 🕑	Browse User DB Use Substructure Search Structure Search in 1H User DB Structure Search in 13C User DB
		10 12 N 14	đ	Structure Search in X-Nuclei Us Tag Search


You can add (or replace) a second chemical shift assignment to a single nucleus. This feature will be very useful if you need to assign rotamers or for ambiguous assignments.




From the assignments table, you can hide "no protonated heteroatoms" or the the assignments of any specific spectrum:

signments	;	_			Sec. 1	
Report (	Copy D	* elete	Expand	Collapse	100 Hide	Setup
Available sp	ectra:					inked constrained Heteroatoms
						Gammerit zu Kamme
Atom	Chemica	ISI Pred	licted Shif	t		
4 5 C						
signments	207	2 10	6			
Report Copy			ollapse Hide d spectra:	Setup		
			adiol_1H			
			1.2	ide Assignme now Assignme	8403 - C	
Atom Chi	emical SI Pred	icted Shift			E	
1 C 4 2 O H 7.0 4 3 C					E (1 3.4	
H 4C H						

It is possible to display the 1H and 13C assignments in the molecule by right clicking on it and selecting 'Atom Label/Show Assignment'

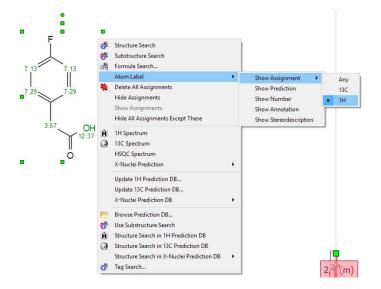

The Assignments table shows checkboxes for each row in the correlations that can be displayed as arrows in the molecule. Checking/unchecking these checkboxes will change the visibility of the correlations for each atom:

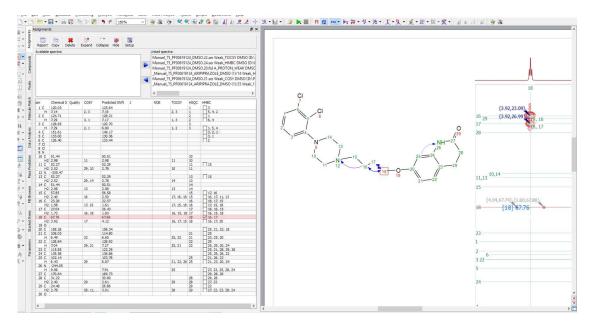


## 9.6.2 Transfering assignments through datasets


The **automatic assignment deduction** from 2D spectra are applied only when the user makes a manual assignment to a multiplet box in the 1H spectrum and 2D peaks have been picked in 2D spectra. The automatic deductions are made only when there are no other peaks very close, so that correlations are clear. In those cases where there is more than one peak peak label per signal, you would need to delete the extra peak labels or use the 'Merge Peaks' feature (under the 'Peak Picking' scroll down menu) and re-do the assignment to the multiplet box in the 1H-NMR spectrum (to get the deduction).

Let's see how it works:


1st: Open for example a 1H, 13C and HSQC datasets and the applicable molecular structure in the same document.

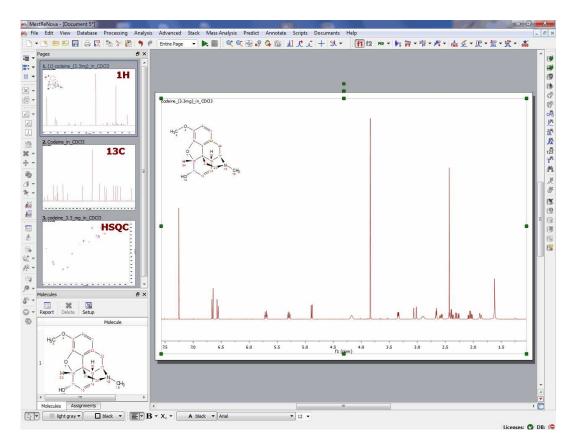

2nd: Apply a Peak Picking in all the datasets and a Multiplet Analysis in the 1H-NMR spectrum:

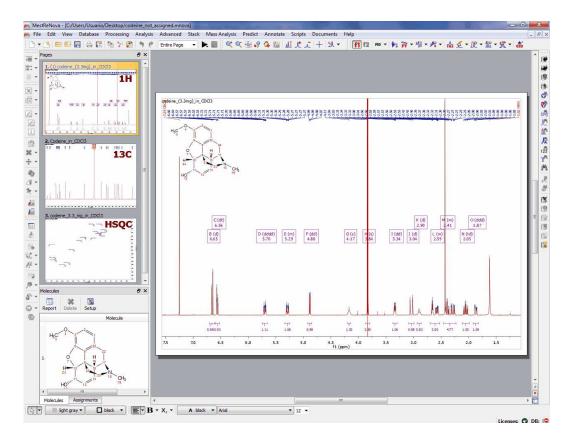


3rd: Make sure that you link all the spectra of the document from the Assignments table:




When adding or deleting spectra to the assignments linked spectra; the columns of the assignments table will be updated.


4th: Make an assignment to a multiplet box in the 1H-NMR spectrum. In that case we have assigned the atom 2 to the multiplet box at 6.65 ppm:

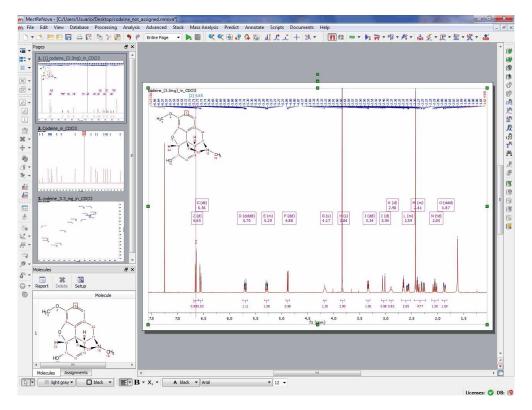

5th: And that's all! Jump to the 13C and automatically you will find the applicable assignment:

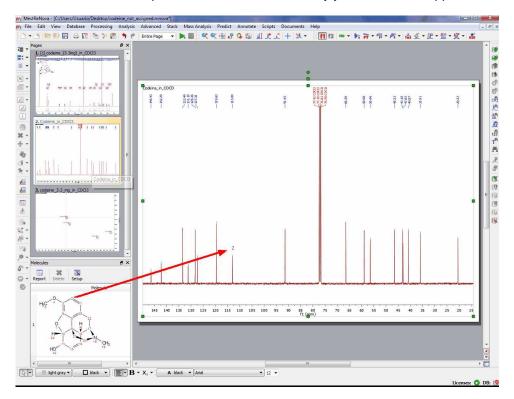

....and the same with the HSQC as you can see below:

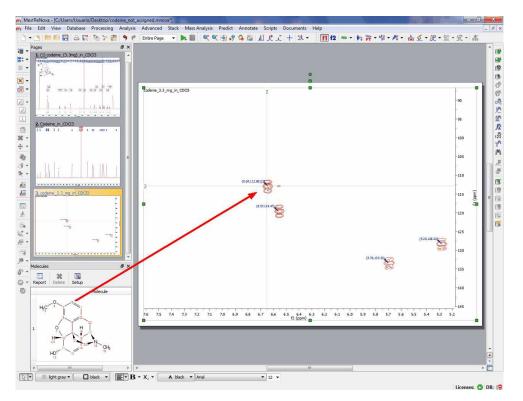


### 9.6.3 Assisted assignment by using the predictions


You can use Predict&Compare (or Predict&Verify) to make your assignments.

Just open a 1D-NMR dataset with a molecular structure and follow the menu 'Analysis/ Predict&Compare'. After the prediction is run, Mnova synthesizes the corresponding 1H-NMR spectrum using a rigorous full quantum mechanics method taking into account any second order effect present in the predicted spin(s) systems(s).


For example, in the figure below, you can see the results of running a prediction and comparing the resulting 1H spectrum with its experimental counterpart and the applicable assignments for the predicted spectrum:

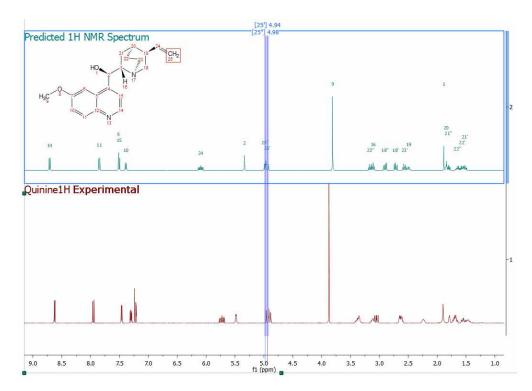

Next, you will only need to press the 'A' key to activate the assignment mode and select the atom and the applicable region of the experimental spectrum to be assigned (following the assignments of the predicted spectrum):

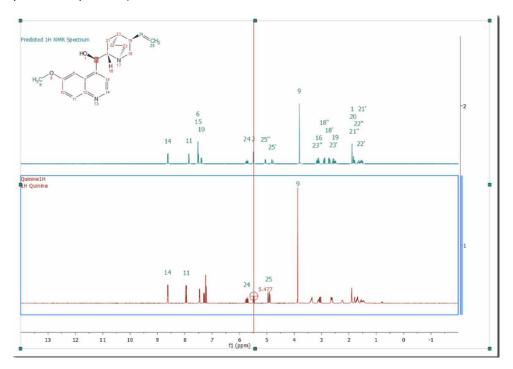


If you load a 1H-NMR spectrum with a multiplet analysis and run Predict and Compare; you will get a stack plot with the multiplet boxes displayed in the experimental spectrum, so you can easily assign those multiplets to the molecular structure and finally update the 'Prediction DB' if you wish:

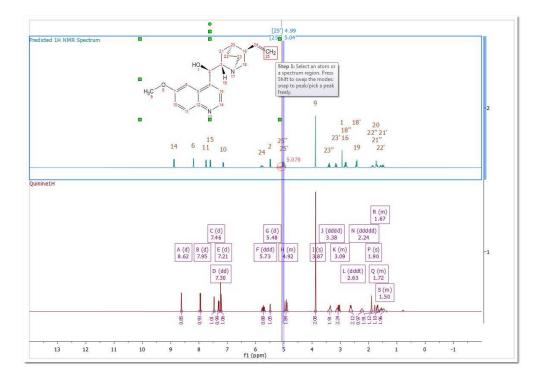


### 9.6.4 Copy assignments from one molecule to another

You can **copy assignments** from one molecule to another (the numbering of the common atoms must be the same) by selecting the first molecular structure with the assignments and doing 'Ctrl/Cmd+C'. Finally, select the second molecular structure and follow the menu 'Edit/Paste Properties/NMR assignments'. Please bear in mind that the numbering of the common parts of both molecules must be the same.

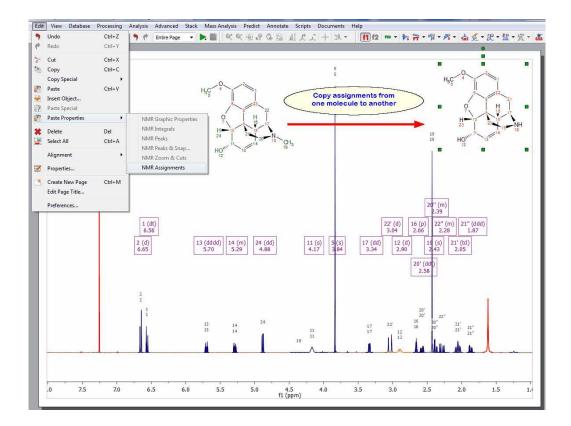

Another way would be to copy&paste the molecular structure with the assignments and make the structural changes in one of the molecules. You could renumber the resulting molecules by selecting 'Concatenate Numbering' from the 'Molecular Drawing Toolbar':

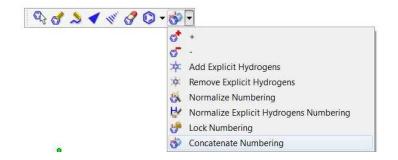


### 9.6.5 Assignments Properties

To change the properties of the Assignments labels, double click on the spectral window and select 'Assignments' in the left tabbed menu. Once there you will be able to select the font, background, frame and form of the labels:

Title General	Assignments
Grid Grid 2D Traces Stacked Scales	Color  Color  Seagreen  Color  Clues  Horizontal  Clue  Line  Color  Col
Horizontal Vertical Peaks Integrals	Vertical Ver

If you have several compounds in your document, you can use the same color compound for the assignments labels (green and blue in the example below) by checking the applicable box:

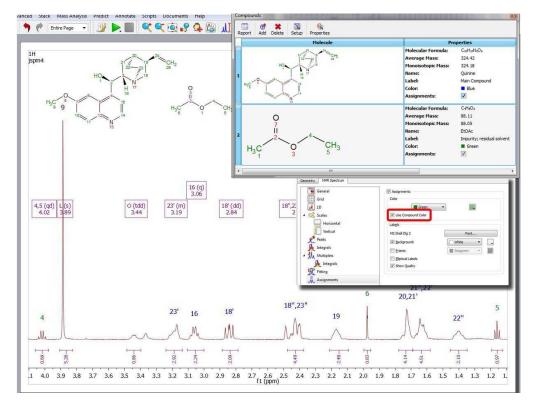

You can hide the assignments in a spectrum by unchecking the 'Assignments' box (or lines boxes for 2D) in the Assignments Properties. You can also do the same by right clicking on the molecule and selecting the applicable option:



The same effect will be obtained by right clicking on the 'Linked Spectrum' from the Assignments table and selecting 'Disable Link':

Report	Copy Dele	te Expand	d Collap:	se Setup	
Available s	pectra:	Lir	ked spect	ra:	
			luini	Disable I	
				Endure L	
Atom	Chemical SI	Predicted S	COSY	TOCSY	
4 1 0			COSY		
	Chemical SI 3.08	Predicted S 1.65	COSY		

# 9.7 Mnova Verify

Mnova Verify is a new developing approach for structure verification by NMR and MS.

The pharmaceutical and biotechnology industries are currently facing very significant challenges which are resulting on major organizational and operational changes. The trend is for pharmaceutical companies to outsource many of their Research and Development operations to third parties with specific specialties and areas of expertise, in order to focus their own resources on areas where they are in a position to maximize value.

As a result, where many operations such as data mining, information sharing and decisions on chemical entities used to have to be carried out at an internal company level, now these same functions need to encompass the entirety of the supply chain and all partners involved in the company's R&D effort. In addition, it is desirable to standardize data formats and data handling as much as possible, to keep tight controls on quality, particularly when compounds are being transferred between organizations and to optimize the sharing of information to maximize productivity.

A further challenge, which affects, among others, the domain of Analytical Data, is the reduction in the resourcing of internal support teams. In the case of Analytical Data, this means that, whilst progress in hardware capabilities and huge steps forward in automation allow us to generate very large amounts of analytical data in high throughput, a bottleneck is being created by the capability of Analytical Departments to get eyes on data. In this situation, overseeing also the data and proposed chemical structures proposed by partners outside the organization, and typically received in large numbers, is becoming harder and in most cases has been abandoned as an achievable objective.

Mnova Verify evaluates a series of elements (GSD, solvent recognition, novel similarity measure, multiplets and chemical shift predictions) and applies a scoring system to return a Yes/No/I don't know answer. This makes it a very powerful screening system useful for chemists who need to validate decisions as to the structure corresponding to their experiments, either in single or batch mode.




### 9.7.1 Single Mode

To run a verification in single mode, import into Mnova (by using the File/Open dialog or by dragging and dropping from the OS browser) a set of spectra (any combination of one 1H spectrum, one HSQC, 13C and one LCMS or GCMS) and a single structure (.mol or .sdf).


Please note that our preference is to work with fid and ser files as opposed to processed data, as the optimal processing for the verification may differ from processing used for visualization, etc.

Optimally, prior to running the verification, 1H NMR should be zero filled to 64K or 128K points and should have no line broadening applied.

Once the data have been imported, invoke the 'Analysis/Verification' menu.

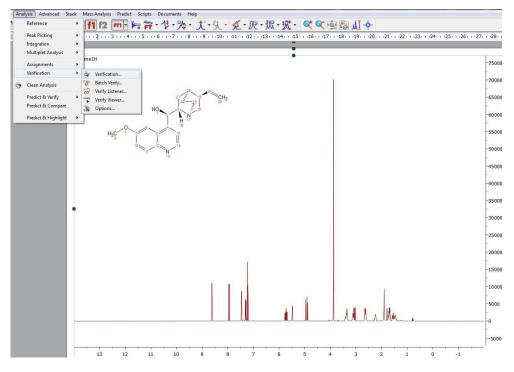

Once you have selected 'Verification'; the 'verification setup' dialog box will be displayed:

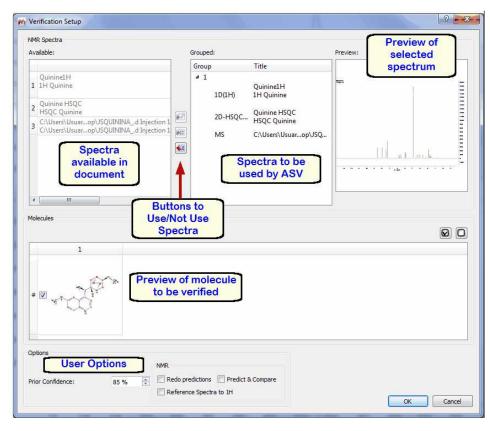

The document spectra panel displays the spectra which are available in the document.

The verification spectra panel displays the spectra which will be used for the verification (you could have some more spectra in the document which you do not want to use for verification, so this allow you to use only those which are relevant to you at that stage)

The spectral preview just shows you an image of the spectrum you have selected in the verification spectra panel (this could be handy when you are trying to decide maybe between 2 different 1H spectra to do the verification on)

The buttons to Use/Not Use spectra allow you to move spectra which are available on the document to the list of spectra to be used for verification or viceversa. To do so, just select the relevant spectrum and click on the relevant arrow to move from the list on the left to the list on the right or from the list on the right to the list on the left.

The molecule panel allows you to visualize the molecules you have available in the document and to select the one you want to verify by ticking it.


The User Options do the following:

**Prior Confidence**: If the prior probability is 0.5, that means that we don't have any prior knowledge about the quality of our structures so that the new score will be exactly the same as if the prior probability concept is not applied.


On the other hand, higher values of the prior confidence (i.e. 0.95) will result in higher scores (the significances are untouched). This is like saying: I know that 95% of my molecules are always correct, so please use this prior knowledge to scale the scores. Values of prior confidence below 0.5 will drop the scores (I know that most of my molecules are wrong, so take this into account).

**Redo Predictions:** to be used in cases where the prediction failed and the user manually corrected the values. See this <u>chapter</u> (example 2) for further information

**Predict and Compare** tick box allows you to select how you want the spectra to be presented after verification. If you tick the box, you will be presented with the experimental and predicted spectra in a stack:

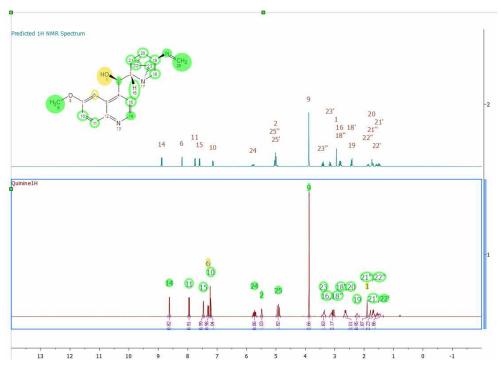

If you untick the Predict & Compare box, then you will be presented with just the Experimental spectrum:

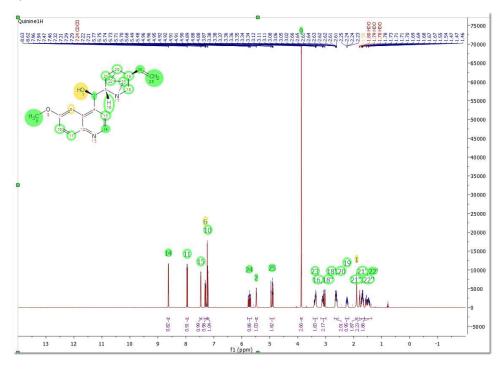


#### Reference Spectra to 1H: to apply Absolute Reference to the document

Once you have selected the desired options, click OK and the verification will run.


Once you have run verification, you will be presented with the following:

- 1. Spectrum/spectra, in your chosen view mode (Predict & Compare or Active)
- 2. A table of verification results which should appear after you run. If not, turn it on by using the View/Tables/Verification Results' menu.
- The structure, annotated with colour coded assignments. The color coding of the elementary assignments is made according to their quality (Green = High Quality; Yellow = Medium quality; Red = bad quality; Gray = worse quality).

However, this quality parameter is not the only descriptor that we can use to show the outcome of a given assignment. There is another very useful parameter that is called 'Stability'. A stable elementary assignment means that this remains stable in all the assignments solutions whose score is higher than a given positive threshold, that is, that assignment is found in all the assignments solutions. This is another way to say that such assignment is very likely to be correct. So the stable assignments are displayed as filled disks, whilst normal assignments are displayed with unfilled disks.

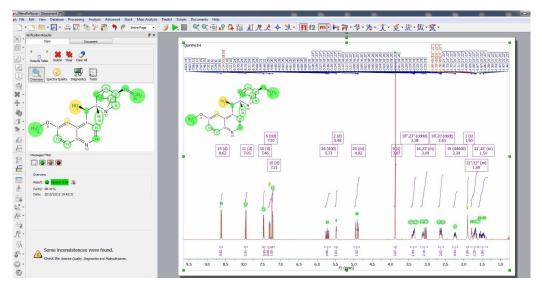


The paper area will present the spectra annotated with the assignments the software has made to the molecule and the molecule with each atom colour coded by quality of assignment (green is a good assignment, yellow is poorer assignment and red is a bad assignment but which still allows the software to make a total assignment of the structure).

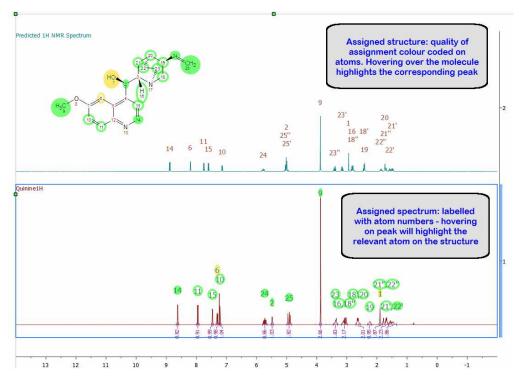

In the case of HSQC, the software will present you with the assigned molecule and assigned HSQC spectrum, with the assignment labels for the spectrum placed at the top of the paper. In addition, the spectrum is marked with colour coded rectangles as follows:

- A green rectangle represents a predicted 2D range for a peak, which does have a real peak within it, therefore indicating a good match between experimental and predicted peaks.
- A yellow rectangle represents a predicted 2D range for a peak, which has a real peak very close to its edge, therefore indicating an acceptable but less reliable match between experimental and predicted peaks.
- A red rectangle represents a predicted 2D range for a peak, which does not coincide with any experimental peaks, and therefore indicates a significant difference between a predicted and experimental peak or the complete lack of an experimental peak.
- A peak without a rectangle means that there is an experimental peak present where the prediction does not expect any peaks

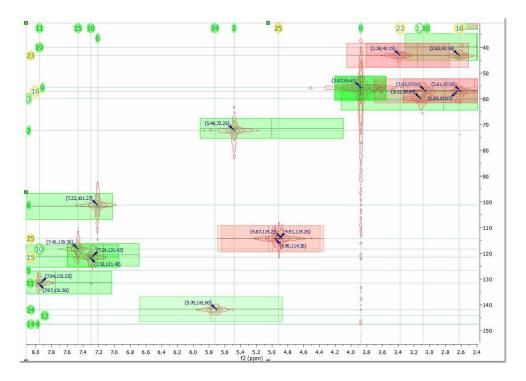


## 9.7.2 Verification Results panel

In the Verification Results panel (under the 'View/Panels' menu), the information is distributed in different pages (Overview, Spectra Quality, Diagnostics and Tests). The messages can be filtered depending on the type of inconsistency:




In the **Overview** mode, we will get the result, purity value, date and the verification results options. From that dialog, you can change the 'prior confidence' to one spectrum or to all in the document (which can be useful for example if you had run a Verification with 100 spectra and then you want to see how the results would be with different prior confidence value, without needing to re-run the Verification) and also the quality format:

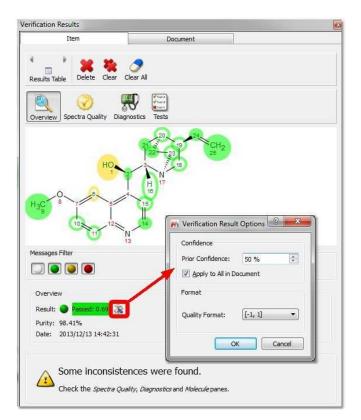


If the document contains more than on molecule, you can use the 'Result Table' arrows to navigate through the results:




Clicking on the 'Results Table' button will display the verification results in a table:

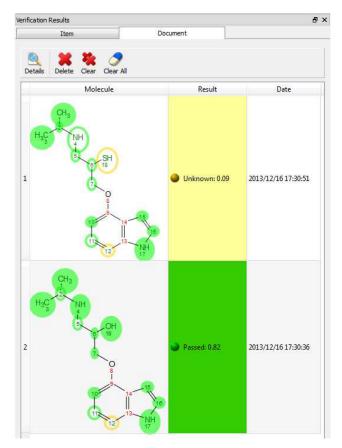


Clicking on the Spectral Quality button, will display the report any problem detected concerning the quality of the experimental data, which you can filter with the coloured buttons:

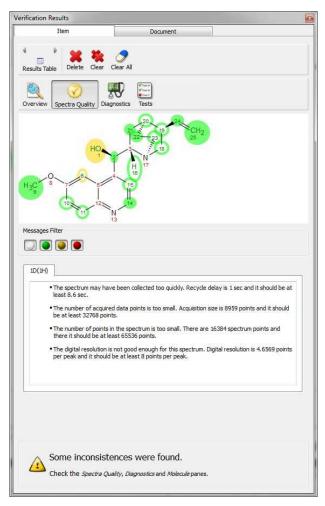

Clicking on the 'Diagnostics' button, will display some warning messages:



Clicking on the 'Tests button', will display the Score, Significance and Quality values for each individual test, which is designed to help you identify quickly possible reasons for a failure:

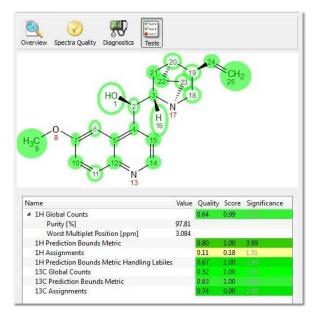

#### Global Counts:

**Purity:** this is an estimation of the purity of the sample calculated by NMR. Basically, it is the ratio of Compounds Vs (Impurity+Artifacts) peaks. Purity can be displayed in Peaks table by selecting the checkbox "Show Purity Label" in Setup Table (disabled by default).

Worst Multiplet position: this is the location of the real multiplet which is furthest away on the chemical shift scale from its predicted counterpart

- Prediction Bounds Metrics: this is the location of the predicted multiplet which is furthest away on the chemical shift scale from its experimental counterpart. Each atom in the molecular structure is given a chemical shift and an allowable range based on the quality of the prediction for its specific environment. The software then checks whether a multiplet with the right number of nuclides is present within that allowable range. There will be a specific test for multiplet labeled as labiles by the Autoedit analysis step.
- Assignments Test: Effective number of missing peaks and effective number of extra peaks (1H, 13C and HSQC). The full spin system for the proposed molecular structure is built and compared to the experimental data. Every possible assignment of the multiplets in the spectrum to the spin system (and through it to the atoms) is enumerated and its likeability calculated by a merit function. The highest positive result of the merit function will be reported as both as verification test result and as automatic assignments made on the structure/spectrum pair. In the case of HSQC, the 2D spectrum for the structure is predicted and each predicted peak is given a 2 dimensional allowable range. Each of these ranges is then evaluated as to whether a real peak in present within them, and whether there are ranges with missing peaks or real peaks which do not correspond to allowable predicted ranges.


When running the verification of a HSQC against several molecules, the user has the ability to show the rectangles in the HSQC for each molecule, by selecting the molecule from the ASV Results table and checking/unchecking the 'Highlight' box for the HSQC assignments in the table:

Name V	alue Quality	Score	Significance
1H Nuclides Count	0.65	0.98	20
1H Prediction Bounds Metric	0.80	1.00	3.99
1H Assignments	-0.33	-0.39	5.65
1H Prediction Bounds Metric Handling Labiles	0.67	1.00	
13C Nuclides Count	0.51	0.95	
13C Prediction Bounds Metric	0.63	1,00	
13C Assignments	0.47	0.63	
<ul> <li>HSQC Assignments</li> </ul>	0.75	0.97	3.44
Image: Highlighting			

• MS Molecule Match Score: For each proposed structure's molecular formula, with the given ionization mode (such as protonation), a molecular ion cluster spectrum is computed. Each molecular ion cluster spectrum is then compared to every spectrum in the LC- or GC- MS run, and ranked according to spectral similarity, where 1.0 is identical within the m/z region of the molecular ion cluster. This ranking is further refined by taking into account the response of a molecular ion chromatogram (or chemical chromatogram), which also has a maximum value of 1.0. The final match score is the product of the two metrics. The MS Molecule Match similarity measurements are derived from traditional dot product calculations and take into account a user specified m/z accuracy, to make full use of accurately mass measured mass spectral data. If MS/MS spectra are also present in the data set, the structures are used to predict fragment spectra, and these predicted fragment spectra are compared with the acquired MS/MS spectra.

Once the data is processed and made ready for the verification, a series of tests of the hypothesis that the proposed structure is the major component of the sample are carried out. For an effective automatic structure verification system when many of the parameters being considered by it may well be imperfect (integration, spectral analysis, predicted chemical shifts, etc.) it is fundamental that the system has the capability to weigh different results in different ways and to auto-evaluate the importance of specific tests in specific conditions. This allows the system to become robust to a level of uncertainty in the quality of the inputs. Therefore, the single tests may have not only a score but a different significance which, in addition, may correlate with the principle outcome. Each test generates a [quality, score, significance] result:

 Quality: The Quality Score corresponding to each individual test is generated by combining the Score and the Significance for that test. The objective of this Quality Score is to generate one single number to allow easy comparison when handling large volumes of data. The format of Quality values can be selected from 'Verification Results table' after having clicked on the 'Options' button:

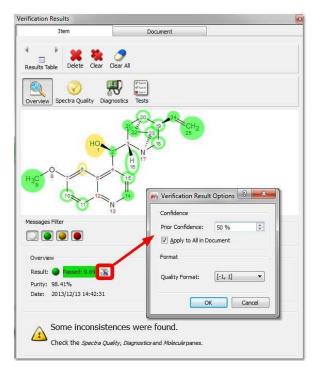

- Score: This is the result of the test, where a value of 1 means that the hypothesis fits perfectly with the experimental data, whilst a score of -1 means that the hypothesis is a perfect failure and therefore definitely wrong. The score value will include three digits (Score taking into account the prior confidence, verification score (without taking into account the prior confidence) and 'prior confidence')
- Significance: Each test, depending on the characteristics of the data, the proposed molecular structure, the prediction quality for the given HOSE codes or chemical environments present on the molecule, etc., gets given a significance. Thus, a high level of impurities in the spectrum may reduce the significance of tests which rely heavily on integration, whilst a poorly predicted chemical environment may reduce the significance of a test relying heavily on chemical shift prediction. Significances of 0-2 are low, 3-5 are medium and >5 are highly significant. There is no theoretical limit to the value of significance, if a test could be devised which was fully deterministic and completely infallible, this could have infinite significant within this concept.

### 9.7.3 Options

Following the menu 'Analysis/Verification/Options' will display the dialog box below:

General Traces Peak Detection	Mass NMR Prediction Error Factor:
Major Peak's Minimum Area Ratio: 0.50	1H: 1.000 🗘 13C: 1.000
	Integral Values Error: 20.00% Expected Sample Purity: Normal Purity "Bad" Water Known 1H Impurities DMSO CDCl3 EtOH DMSO-d6 Acetone-d5 MeOH IPA Acetone MeOH-d4

From here, you will be allowed to change the some setting for the MS and NMR verifications (i.e prediction error factors, to select a threshold for the integration values, the percentage of impurities, etc).


NOTE: The option to <u>'clean analysis'</u> (under the Analysis menu) could be useful to rerun a verification after having changed the options.

### 9.7.4 Troubleshooting a negative result

#### What happens if I get a negative verification result?

There are several reasons to get negative results in the verification. Let's take a look at some of them


 All or most of the NMR tests fail with bad scores: this could be an indication of either the wrong structure, a very poor quality spectrum or solvent misrecognition, which will affect most tests very significantly. The recommended Operating Procedure is to check the solvent recognition first. To do so, make sure you are in 'Active Spectrum' mode and that your graphical properties (Edit/Properties/NMRSpectrum/Peaks/Curve) has the 'Peaks' box ticked. This will display colour coding for the autoediting carried out by the software on the spectra. You may identify this way that a solute peak has been considered as solvent or viceversa.

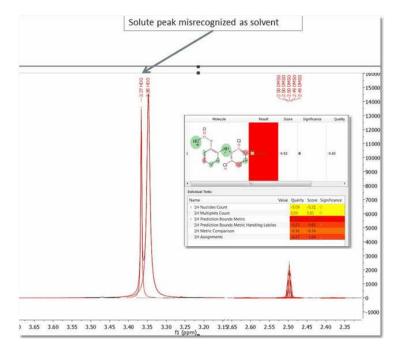


In a case in which this happens, this can be corrected by right clicking on the peak label (pointed at by the arrow on the figure) and selecting Edit Peak Type, then marking this peak correctly (in the case above would be marked as compound and with the Flags unticked...)

Peak			ОК
V Type:	Compound	•	Cancel
Flags:	2ary_Solvent	¥	


Once GSD/AutoEdit has been modified, you can just re-run Verification and your GSD modifications will be respected. In this case, after running again, the result is totally different, as can be appreciated in the figure below:

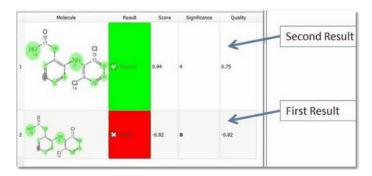

2. Should you find that the score is reasonable but that some atoms are showing assigned in red and that either the PBM or NN tests have low values, then this could be due to an *inaccurate prediction* or to an atom which is not where it is supposed to be (in the latter case this would be a true negative result). In this case, check the 'Worst Multiplet' and 'Worst Location' feedback, as this might indicate where you should look first. In the case of the figure below, 'Worst Location' is 9.49 ppm, and there we can see that there is a peak, which is being assigned to atom number 11, but the predicted value for atom number 11 is at 8.75 ppm. The user can decide here whether it is reasonable that the prediction is poor and that the real value of atom 11 could indeed be 9.49.

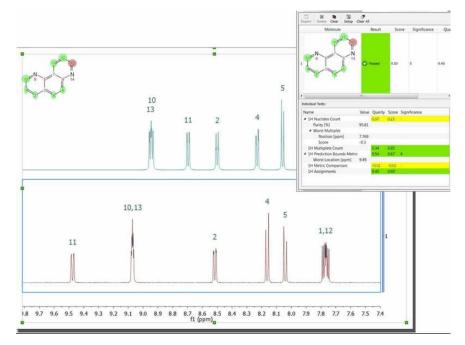

In this case, the user can grab the prediction label (the same could be done with the rectangles in a HSQC) by clicking on it (the number 11 label on the blue spectrum) and moving it to the 9.49 ppm position. Once this has been done, the verification can be carried out again, making sure that the **'Redo Predictions**' tickbox in the verification dialog is unticked. This will allow the user to see what the result of the verification would be in case the prediction was being made at 9.49 ppm, rather than 8.75 ppm. In this case, as the figure below shows, the verification 'Score' has improved from 0.56 to 0.82 and the atom which was badly assigned (colour coded in red on the molecule previously) is now well assigned. Should the user decide that the presence of atom 11 at 9.49 ppm is possible given its chemical environment, then this is a likely indication that the reason for the previous lower score was simply a poor prediction.




3. A low result in 1H Nuclides Count could also be indicative of poor integration due to either impurities or a very short relaxation time. It is to be noted that a very short relaxation time can affect integration and that poor integrals will have a negative impact on the verification result. This can be thought of as a false positive but in fact the software is reporting a problem or

incompatibility in the data with the proposed molecule.

### 9.7.5 Rank potential molecular candidates


Mnova Verify can also be used to run one set of spectra against more than one potential structural candidate (or viceversa). Taking as an example a situation where we have one single spectra set (1H only, for example), as we can see in the figure below:

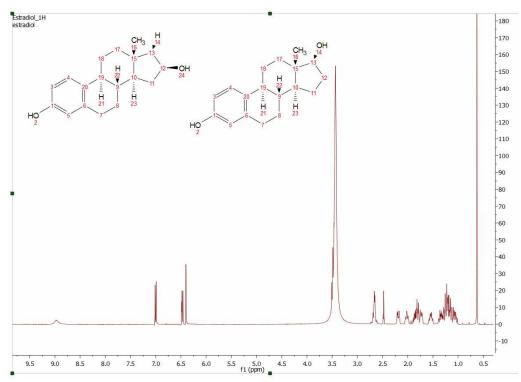

Mnova Verify will be able to rank these 2 structural candidates on the basis of their NMR. To do so, we would need to duplicate the NMR datasets inside the same document and run the Verification against the two molecules:


	R Spectra					
4va	ailable:		1	Grouped:	and and	Preview:
	Title	Туре		Group	Title	A
1	CARBON estradiol	1D(13C)		▲ 1 10	PROTON (1H) estradiol	
2	CARBON estradiol	1D(13C)	== <b></b>		CARBON (13C) estradiol	
3	PROTON estradiol	1D(1H)			PROTON	
1	PROTON estradiol	1D(1H)	+	10	(1H) estradiol	•
1		1	2			
#	R.					
	tions					
pt			NMR			
20	or Confidenc	e: 99 % 葦				

The software will run the spectral set against both structures and present the user with a score for each structural proposal, which may in many cases allow the user to differentiate between 2 possible candidate structures.




This is one of the areas where having the ability to combine NMR and MS data can prove very powerful. In the following example, 1H NMR alone does not distinguish between the structures on the

total score, as the only difference is in a different nuclei (S or O) (although there are already some indications that one structural proposal has greater merit than the alternative in the quality of the assignments made by the verification module and reflected in the colour coding).

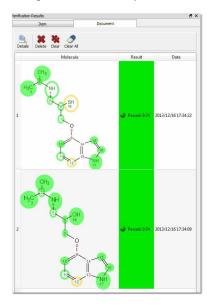

Should the user have MS data in this example, however, the difference between both proposals would be immediately obvious:

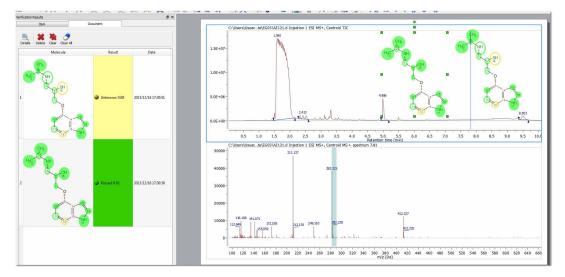


### 9.7.6 Verification in batch mode

Mnova Batch Verify evaluates analytical data and makes a judgment as to whether they are compatible with the structures proposed by the user in full automation mode (from libraries or at the point of data acquisition by using the Listener). This plugin is sold apart and an specific license is needed. You will need to install the Batch Verify plugin by following the menu 'Edit/Advanced Plugins' and clicking on the 'blue plus' button or just by dragging&dropping the XML file in Mnova

With this plugin licensed, you can run verifications in Mnova in batch mode by following the menu

'Analysis/Verification/Batch Verify':



This script will run a set of spectra against a set of molecules. Once the user has invoked the script, a dialogue will be presented, where a set of information can be entered.

Save To DB	🖻 🖪 🕨			
NMR       Mass       Structures         1H Path Mask:       28cpds_NMR/*/1/fid <ul> <li>Image: Structures</li> <li>Image</li></ul>	Data Location Main Directory:		b\Desktop\download	
13C Path Mask:       28cpds_NMR/*/2/fid       ●         HSQC Path Mask:       ●       ●         Other Files Mask:       ●       ●         Results       ●       ●         Directory:       C:\Users\Usuario\Desktop\download       ●         I Save To DB       Image: Create Extended Results       Image: Create Extended Results	100000	Structures	20-onde NMD/#/1/6/4	
Directory: C:\Users\Usuario\Desktop\download	13C Path Mask: HSQC Path Mask		Accession of the second se	•
Results Ordered by Quality				
	Directory: 📝 Save To DB		op\download	

**Main directory** for the location of experimental files: The directory containing all the experimental data should be entered here.

**Expert:** it will allow the user to use masks for NMR, MS and molecules.

**1H Path Mask:** Should the user desire to use 1H spectra as part of the verification, a file mask describing how to open each of the spectra should be entered here. All Operating System standard conventions apply (\*, ?, !, etc.).

In the example above the 1H datasets are in stored in C:\Users\Usuario\Desktop\Batch Verification TEST\spec\Paper\_01 (Paper\_02, Paper\_03 and so on):

Organizar 🔻 🛛 Incluir en l	biblioted	a 👻 Compartir con 🔻	»	₩. •	
🔆 Favoritos	* I	lombre	^		
Escritorio		Paper_01			
Sitios recientes		Paper_02			
🗘 Dropbox		Paper_03			
퉳 Descargas		Paper_04			
		Paper_05			
🧊 Bibliotecas		📙 Paper_06			
Documentos		Ш			,

13C and HSQC Path Mask: Same for 13C and HSQC.

MS Path Mask: Same for MS data.

The scroll down menu of the Masks will hold the last 5 used masks. Please bear in mind that you can use more than one mask at a time by separating the masks with the character |. This separator will be inserted automatically if the mask is chosen from the list.

**Structure File Location:** The location of the .mol (or .sdf) files to verify against can be entered here, as well as the File Mask to each one of the individual files. The script has the options (see the options tab) to run spectra and molecules with the same name (therefore user should rename the mol or sdf files to the same name as the spectra) or in the same order (in which case user should make sure that the spectra and the molfiles are in the same order in their respective locations). If you are working directly with Mnova documents (instead of raw data) containing the molecular structure inside, you will not need to fill the molecule file location.

**Files Associated by name:** The script has the options to run spectra and molecules with the same name (therefore user should rename the mol or sdf files to the same name as the spectra) or in the same order (in which case user should make sure that the spectra and the molfiles are in the same order in their respective locations).

The user can enter a folder location where results should be saved and decide whether, in addition to standard output, Mnova files and PDFs should also be saved (this will be an Mnova file and a PDF for each verification set).

Results order by quality will order the results from best verification quality to worse, whilst if this box is unticked, the results will list spectra/molecule pairs in the same order as they are in the folders they are being picked up from to run the verification.


The **'Create Main Parameters Report'** box; will generate a .txt report for each group. The reports are named as its corresponding group and will contain the following fields: Title, Comments, Date, Time, Verification Quality, Verification Score, Verification Significance, Purity and Compound peaks.

The verification script will also generate a log file with some basic information about the verification that has been run (time it was run, number of datasets, etc.) and a summary html file which can be opened in any web browser and which will contain a table showing all the verification results for all the sets, as well as links to the documents in case the user needs to interrogate the data further or look at the detail behind, for example, unexpected failures.

Drganizar 🔻 🦪 Abriz 🔻	Compartir con 👻 Grabar Nueva carpet	ta		
🛠 Favoritos	Nombre	Fecha de modifica	Tipo.	Tamaño
Escritorio	😹 data	04/12/2012 12:45	Carpeta de archivos	
3 Sitios recientes	🕌 images	04/12/2012 12:45	Carpeta de archivos	
👽 Dropbox	E log.bt	04/12/2012 12:45	Documento de tex	2 KB
Descargas	H Paper_01_20_fid.mnova	04/12/2012 12:44	Archivo MNOVA	37.825 KB
	Paper_01_20_fid.pdf	04/12/2012 12:44	Archivo PDF	70 KB
Bibliotecas	Paper_03_20_fid.mnova	04/12/2012 12:44	Archivo MNOVA	37,829 KB
Documentos	Paper_03_20_fid.pdf	04/12/2012 12:44	Archive PDF	69 KB
Se Imágenes	Paper_04_20_fid.mnova	04/12/2012 12:45	Archivo MNOVA	37.878 KB
a Música	Paper_04_20_fid.pdf	04/12/2012 12:45	Archieg PDF	100 KB
Videos	Paper_05_20_fid.mnova	04/12/2012 12:45	Archivo MNOVA	37,863 KB
	Paper_05_20_fid.pdf	04/12/2012 12:45	Archivo PDF	94 KE
🀺 Pablo	Reper_06_20_fid.mnova	04/12/2012 12:45	Archive MNOVA	37,828 K8
Disco local (C:)	Paper_06_20_fid.pdf	04/12/2012 12:45	Archivo PDF	66 KB
	i result.html	04/12/2012 12:45	Chrome HTML Do	8 KB
🗣 Red	esults.dat	04/12/2012 12:45	Archivo DAT	1 KB
MESTRECRIS	, DEPARTON MULTIN		need and an inter	

For results interrogation and to gain understanding of the results, user should open the 'result' html file, with any web browser. This file will present, in one single view:

- Some basic verification parameters (time run, type of data)
- A well plate with the summary results for all datasets
- An extended table with the final result for each dataset as well as all the individual test results for each individual dataset
- Links to the .mnova and .pdf files generated, as well as to original files (fid, mol, etc.) to allow user to quickly drill into specific results which need to be check or looked at further.

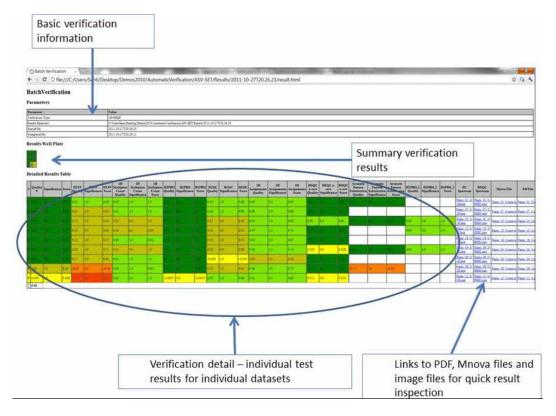

Selecting the 'Pre&Post' label, a new dialog will be displayed:

Main Pre&Post DB Op	ions	
Solvent		
Replace Default With:		
Pre Verification		
1H Processing Template:		
13C Processing Template:		(***)
HSQC Processing Template:		
Post Verification		
Layout Template:		
✓ Advanced		
Pre Verification Function:	pre()	
Pre Verification Script:	C:\pre.qs	
Post Verification Function:	post()	
Post Verification Script:	C:\post.qs	

**Solvent/Replace Default With:** This allows users to handle situations in which the solvent may be wrong in the parameters. It can be the case that a certain batch has been run on a specific solvent but that the user left the default solvent on the spectrometer data entry and therefore the solvent could be wrongly entered. Since the target solvents will affect the performance of the Autoedit function in Mnova Verify, it is important to be able to correct for this at the script level.

**Pre-Verification:** This allows the user to select a <u>processing template</u> for the 1H and HSQC and a script or function the user would like to run prior to each verification being performed. There could be many examples of this. One obvious example would be a script to remove from the GSD input peaks belonging to a known impurity (THF, iPrOH, etc.)

**Post-Verification:** This allows the user to select a <u>layout template</u> for the result and a script or function the user would like to run after each verification is performed. Again, there could be many examples of this. One obvious example would be a script to perform and report qNMR on the data being verified, or a script to apply a specific reporting template, or to save the results to an ELN or other external database.

Clicking on the 'DB' tab, will allow you to save your results into the Database:

Batch Verify	? ×
= 🖪 🕨	
tain Pre&Post DB Options	1
Connection	
Server:	localhost
Port:	5504
User:	Test
Password:	*****
V Save Password	Disconnect
Database	
Selected Database:	test

Selecting the 'options' tab will allow you to 'Predict&Compare', as with the single mode verification, this just sets the way in which the data are presented to the user after the verification has been completed. If the option is selected, the user will be presented with a stack of the experimental and the predicted 1H spectrum, if the option is unselected the user will get presented with just the experimental spectrum.

You can also Absolute Reference the spectra to the 1H-NMR spectrum.

Batch Verify	2
😑 📑 🕪	
Main Pre&Post DB Options	
Basic Options	
V Predict & Compare	
Reference Spectra to 1H	
qNMR	
qNMR     qNMR Settings       Report qNMR Results in Documents	
Advanced Options	
General Resume Automatic Detection Subtraction	
Debug Mode (Execute All Process in Foreground)     Matrix Mode	
Prior Confidence: 99%	
13.1	
<u></u>	

qNMR: Do quantitation as well when running the verification:

	otions					
Concentration Meth	od					
Internal Refer	ence		Concentr	ation Conv	ersion	Factor
From:	-1.10	🔷 To:	-0.90		Â	ppm
Reference F	eak is a Solve	nt				
Apply Line F	Fitting to the Re	eference Peak				
Reference Cond	centration:	100.00		\$ M	•	
Nuclides of Refe	erence:	1		*		
	ithm					
Autoselection Algor						
Autoselection Algor Load Concentratio	ii butu					
Autoselection Algor Load Concentratio Files Directory:						
Load Concentratio	*.txt					-

See <u>qNMR chapter</u> for further information.

**Matrix Mode:** Running in this mode will verify every spectral set against every available molecule, generating a matrix like output with number of rows and columns equal to the number of spectral sets/molecular structures, and with each cell corresponding to a verification result.

**Prior Confidence**: If the prior probability is 0.5, that means that we don't have any prior knowledge about the quality of our structures so that the new score will be exactly the same as if the prior probability concept is not applied.

On the other hand, higher values of the prior confidence (i.e. 0.95) will result in higher scores (the significances are untouched). This is like saying: I know that 95% of my molecules are always correct, so please use this prior knowledge to scale the scores. Values of prior confidence below 0.5 will drop the scores (I know that most of my molecules are wrong, so take this into account).

Automatic Detection tab: to add the masks for the NMR, MS and structures files:

9 📑 🕅	
in Pre&Po	ost DB Options
Basic Options	
Predict & Co	ompare
Reference S	Spectra to 1H
NMR	
/ qNMR	qNMR Settings
Report qNM	R Results in Documents
Advanced Or	itions
Advanced Op	
General R	tions Automatic Detection Subtraction
General R	
General R Masks:	Automatic Detection Subtraction
General R Masks: NMR: Mass:	fid,ser
General R Masks: NMR: Mass:	fid,ser _FUNC001.DAT,MSD1.MS,analysis.baf
General R Masks: NMR: Mass: Structures: Options	fid,ser _FUNC001.DAT,MSD1.MS,analysis.baf

You can work with clusters of NMR+MS spectra and *n* molecules per cluster by checking the "Cluster Size" box. It works only in 'Automatic detection mode' (no clustering is possible in Expert mode).

Resuming a batch job is possible via the "Resume" tab. It allows you to load a .resume file from a batch job that has been stopped.

If you have not displayed the 'Expert mode', you will find a button on the 'Main' tab to inspect the folders and find what experiments and molecules will be used for the verification:

R Batch Verify	
😑 🗐 🕪	R
Main Pre&Post DB Options	
Data Location	Experiments Found: 3
Main Directory: C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_NMRandMS	Experiment: MOXIFLOXACIN 11: C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_INRandMS/Moxifloxacin/1H/fid
Expert Select Experiments	HSQC: C://Jeers/Usuario/Desktop/Batch/verify testing/Celebrities_INRRandMS/Moxifiloxacin/HSQC/ser Mass: C:/Users/Usuario/Desktop/Batch/verify testing/Celebrities_INRRandMS/Moxifiloxacin/HSQC/ser Mass: C:/Users/Usuario/Desktop/Batch/verify testing/Celebrities_INRRandMS/Moxifiloxacin/Moxifiloxacin.mol, Structureg3): C:/Users/Usuario/Desktop/Batch/verify testing/Celebrities_INRRandMS/Moxifiloxacin/Moxifiloxacin.mol,
Results Directory: C:/Users/Usuario/Desktop/Listener_results  Seve to DB  Advanced Options	Experiment: ONDANSETRON 11t: C:/Users/Usuario/Desktop/Batch/Verify testing/Celebrities_NMRandMS/Ondansetron/1H/fid HSQC: C:/Users/Usuario/Desktop/Batch/Verify testing/Celebrities_NMRandMS/Ondansetron/HSQC/ser. Mass: C:/Users/Usuario/Desktop/Batch/Verify testing/Celebrities_NMRandMS/Ondansetron/HSQC/ser. Structureg3): C:/Users/Usuario/Desktop/Batch/Verify testing/Celebrities_NMRandMS/Ondansetron/HSQC/ser.
Create Single Mnova and PDF Files Create Main Parameters Report	Experiment: VORICON4ZOLE 111: C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_NMRandMS/Voriconazole/1H/fid HSQC: C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_NMRandMS/Voriconazole/HSQC/ser Mass: C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_NMRandMS/Voriconazole/HSQC/ser Structures(3): C:/Users/Usuario/Desktop/BatchVerify testing/Celebrities_NMRandMS/Noriconazole/MGNOroicon/Modiform/_FUNC
	۲ H
	OK Cancel
OK Cancel	

Clicking on the 'Subtraction' tab, will display the dialog box below:

ain Pre&Post DB Options Basic Options           Image: Predict & Compare	
Reference Spectra to 1H	
qNMR	
Advanced Options General Resume Automatic Detection Subtract	ion
Chromatogram Subtraction	UV Subtraction
Background MS Folder: 28cpds_UPLC_M\$_ACII	Background MS Folder: .C_MS_ACID_MODE/UV/
Background MS Mask: */_FUNC001.IDX •	Background MS Mask: */_FUNC001.IDX

The script to subtract chromatograms will subtract a blank background run from the run of interest, for example to ensure a good baseline for quantitation purposes, or to accurately measure differences between two or more runs.

You will need to select the folder containing the datasets (background) and the applicable path masks.

Similarly to chromatogram subtraction, there is another option for UV subtraction. So you will subtract a background UV chromatogram from the foreground one.

#### 9.7.6.1 Verify Viewer

After having run a Batch Verification, you will also obtain a results.dat file which can be opened with the Verify viewer (Analysis/Verification/Verify Viewer). Clicking on any row or any cell of the well plate will display the applicable dataset in your spectral window:

E Load		tings R	eport	Save to DB	Show Active			
#	Title	Qu	ality	Significance	Score	Purity	Molecule	
	LS00027756.10.fid LS00027756.11.ser	0.20	1	111	0.97(50%)	95.50	Q N H C L BE	
2	LS00012648.10.fid LS00012648.21.ser	0.27	g	0.50	0.90(50%)	94.28	of the of	
3	LS00021274.10.fid LS00021274.21.ser	0.77	8	.90	0.86(50%)	91.00	CH-CH-CH-CH-CH-CH-CH-CH-CH-CH-CH-CH-CH-C	
Indivic	dual Tests				Results Well F	late		-
	Name	Quality	Score	nifica	A	В	C D E	
1H F	Prediction Bounds	0.80	1.00	3.99	1 0.89 2 0.78	0.86 0.82		
14 1	Nuclides Count	0.68	1.00	2.10	2 0.70	0.77		
1H A	Assignments	0.81	0.93	6.97				
HSQ	C Assignments	0.73	0.94	3.42	Woll Plate 9	Showing: Verif	ication Quality	•

Clicking on any of the rows of the viewer (or well plate) will load the applicable document in Mnova in order to allow you make changes if necessary. Redoing manually the verification (after those changes) will automatically refresh the result in the Viewer.

Save those results to your <u>Mnova Database</u>, just by clicking on the applicable button of the viewer.

If you have run the Verification together with qNMR, both results will appear in the Viewer and you will have options to show the well plates with the purity/concentration results:

oad Save	e Clear	Settings	Report	Save to DB	Show A	ctive				
#	Title	Qu	ality	Significance	Score	Pu	ity q	NMR	Molecul	le
	LS000277	'5 <mark>0.91</mark>		10.20	1.00	95.2661	1201	9,7184 g <sub>~1</sub>		2
Individual Te	sts					Results W	ell Plate			
Name	Quality	Score	1	Significance			В	с	D	E
1H Metr	0.50	1.00	1.00			1 0.91	0.90	0.87	0.49 0	0.45
1H Nucl	0.49	0.95	1.05							
1H Assi	0.83	1.00	5.22							
1H Assi 1H Pred		1.00 1.00	5.22 4.23							
-	0.81									
1H Pred HSQC A	0.81	1.00	4.23			Well Pla		Verification Qua Verification Qua Purity		*
1H Pred	0.81	1.00	4.23			Well Pla		Verification Qua		
1H Pred HSQC A	0.81	1.00	4.23			Well Pla		Verification Qua Purity		
1H Pred HSQC A	0.81	1.00	4.23		Aultiplet	Well Pla		Verification Qua Purity		SNR
1H Pred HSQC A	0.81	1.00	4.23	4(c				Verification Qua Purity Concentration	lity	SNR 10456.8774
1H Pred HSQC A qNMR Report Concentratio	0.81	1.00	4.23		ł)	NN	Range	Verification Que Purity Concentration Abs. Int,	lity Conc.	

Clicking on the 'Settings' button will allow you to customize the fields that appears in the table, to save automatically the results to the Database and to create single Mnova and PDF documents with or without extended results:

Settings		? ×
Customize Table	Fields	
V Position		
🔽 Title		
Document		
<b>Quality</b>		
Significance		
Score		
V Purity		
Molecular We	eight	
Molecule		
🔽 qNMR		
DB		
Save Results	s to Database whe	en Reporting
Results		
Extended Re	esults	
Create Single	e Mnova and PD <mark>F</mark>	Files
	ОК	Cancel

The Show Active button of the Verify Viewer will be very useful in those cases where you are working with a lot of opened documents in Mnova and you want to highlight in the Verify Viewer the current

one.

#### 9.7.6.2 Verify Listener

You can automatically run Batch Verify as a **listener**. Mnova can 'listen' on a series of folders or drives and can grab data as is acquired and run the verification analysis automatically, saving the result in the selected folder. The settings for the Verify listener can be selected under the 'Analysis/Verification/Verify Listener menu:

Reference	×	re Page 🔻 🔍 🔍				
Peak Picking	×					
Integration	×		Main Pre&Post Subtraction	Notification	ns Options	
Multiplets Analys	s 🕨					
Assignments	•		Files Location			
Verification	Þ	🔬 Verification	Listened Base P	ath	Grouping Level	2
S Clean Analysis		Batch Verify	C:/Users/Usuario/Desktop/M	olecules	1	8
Predict & Highlig	ht ▶	Verify Listener	C:/Users/Usuario/Desktop/Li	stener	1	
Predict & Highing Predict & Verify	nt P	Verify Viewer				
Predict Compare		🔉 Options				
Spectral Moment				1.4	- 10	
		-	Molecule Mask:	*.mol]*.	sdt	*
			1H File Mask:	fid		•
			13C File Mask:	fid		<b>*</b>
			HSQC File Mask:	ser		•
			Mass File Mask:	-		¥
			Other Files Mask:	-		
						•
			Results			
			Directory:	C:\Users\Us	suario\Desktop\Listener\Results	
			Create Extended Results			
			Send Result to Printer			
			Create Main Parameters Repo	rt		

In that case, we will only need to select the path of the datasets folder (and click on the 'blue plus button' to add it to the list of 'Listened Folders'), the file name that we want to import (fid, ser, etc..) and the path folder of the molecules (with the applicable path mask). Please bear in mind that if you only use one listened folder; the **name of the each spectral folder** must be the **same** with the name of the applicable **molecule file** and the molecules folder must be loaded previously in the listener folder (before running the listener).

If you select a specific listener folder for the spectra and another for molecules; then molecules and spectra will get grouped according to the name of the mol files and the first level folder where the spectra are transferred. When spectra matching the mask of "Other files" are added, the files generated get an additional ' to distinguish them from the previously obtained.

In that dialog box, we will find the same options for the 'Pre&Post, Subtraction and Results'that we have for the <u>Batch Verify</u> feature. In addition in the last tab (called Options/Listener), we will find an option to select the number of listener folder levels (default value: 2 folders). So by default, the listener will search for the 'File Names' (fid, ser in the example above) in the first two folders of your datasets.

Main Pre&Post Not	fications DB Opt	ions			
Basic Options           Basic Options           Reference Spectra to 1H           Multipe Spectra per Stru	cture 🔽 1H 📃 H		13C	1	
		IZBC NOESY	TOCSY		
Listener Options V Process Old Files					
qNMR Options qNMR qNMR s qNMR qNMR s qNMR results in					
Advanced Options					
General Subtraction	Listener				
		2			
Listened Folder Levels:					
Listened Folder Levels: Delay:	1 s				
	1 s 1 min				

There is also an option to skip files with a modification date older than the days selected.

When the listener is working, Mnova will display a dialog box like this:

S. S.
sktop/Listener
Finish


Finally, load the results (in .dat format) with the Verify Viewer.

## 9.8 Molecules Editor

Mnova incorporates a basic 'Molecules Editor' which will be improved in the forthcoming versions of the software. This editor includes a powerful toolbar to draw your molecules:



The Drawing mode will allow you to draw a Carbon on your spectral window just by clicking on any empty field. Clicking on any existing atom will add an additional carbon. If you click on a single bond, you will get a double bond (clicking on a double bond will draw a triple bond).




The same result can be obtained from the bond context menu (by right clicking on the bond). The 'Edit Bond' dialog will allow you to change the bond type (single, double, triple, up, down) or to set a label for the bond (to add stereochemistry notation, for example):

•	•		💏 Edit Bo	ond 2 X
<b>•</b> њ.с´	2-2-2-21	OH 4	Symbol Bond In	odex: 2
130		Edit Bond	Prop	perty Value
			1 Labe	E
	•		2 Type	Double


You can **change the atom** just by hovering the mouse over the atom and typing the applicable letter (i. e 'o' for Oxygen, 'n' for Nitrogen, "b" for Boron, 'b' plus 'r' for Bromine, or more complex labels, such as Me, Ph, COOH, etc). You can also change the atom by double clicking on it to display the 'Edit Atom' dialog. From here you will be able to change the name (from C to F, for example).

If you have any spectrum loaded together with a molecule; you will need to select any molecular drawing tool (from the molecular sketcher toolbar) before typing the applicable letter (unless you activate a 'Molecule preference" to have the "keyboard editing" always available). See more <u>here</u>.


From the 'Edit Atom' dialog, you can add greek letters to the number by typing the \$ prefix; for example \$a, 4\$b, 22\$g\$d21 will be converted into , 4 , 22 21.

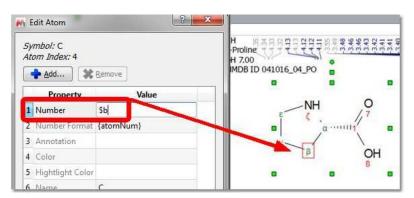


You can **draw salts** from the 'Molecular window' panel (View/Panels/Molecule Windows'), just by drawing both components there. To draw the NH4+ component, you will need to draw a CH4 and then hover the mouse to type the **N** followed by the **+** (to add the positive charge):



You will obtain the same result by drawing both components, selecting them, right clicking on any of the molecules and choosing 'Merge selected Molecules':

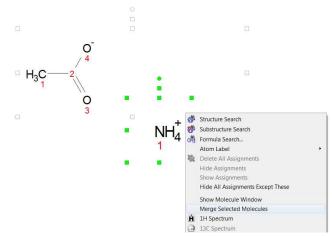


Mnova will not allow to add new atom (clicking on existing one) or change the bond type if that leads to atom valence exceeding, but it will allow you to create a new atom by stretching the bond from existing one. In this case the old atom will be marked with invalid valence cross:



Mnova will also automatically change the atom valence (e.g. 3-5-3 for Nitrogen) when adding/deleting new atoms or changing the bonds type.


This mode will allow you to move an atom or a bond just by clicking&dragging.

In this mode you can also use the lasso mode (by clicking and dragging the mouse around the desired part of the molecule) to select several atoms (to delete them, for example):

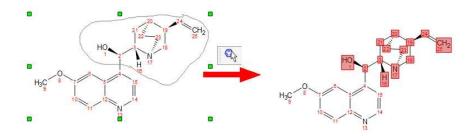

When you select an atom, move it over another one and release the mouse button, only the last atom will stay (except when the first selected atom is non-carbon and the second atom is carbon).

to draw chains by clicking, holding and dragging after having clicked on this button:




Use these buttons to draw stereobonds.

Use this button to delete an atom. An atom, a bond or multiple atoms can be also deleted by selecting them and pressing the Delete key.

You can delete the bonds keeping the atoms (by holding down the Ctrl/Cmd key). Deleting several atoms selected with lasso while pressing Ctrl/Cmd key allows to keep neighbor terminal atoms.


1	0	
	0	Benzene
	Δ	Cyclopropane
	0	Cyclobutane
	0	Cyclopentane
	0	Cyclohexane
	0	Cycloheptane
	0	Cyclooctane

This scroll down menu, will allow you to draw cycles. Spiro atoms can be drawn by adding cyclic templates while pressing 'Shift key'.

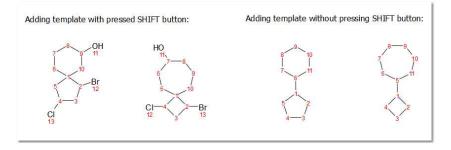

**Increment atom change:** This button includes a scroll down menu with several features to add positive/negative charges (you can set a charge on any atom just by pressing + or - keys), add/remove


explicit H and to normalize, lock or concatenate the numbering, expand labels of compacted groups or clean molecules.

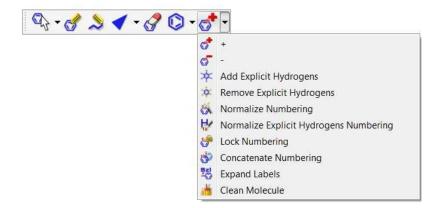


The **Normalize Numbering** button applies re-numbering of the whole selected molecule. From the <u>Preferences</u> you can select if you want to auto-renumber the imported (or pasted) mol files (and also when joining fragments); very useful if you have two equal molecules drawn in different applications or in different order, and you want to normalize the numbering.

Preferences			? ×
General Plug-ins Database	NMR Mass Molecule	Scripting Drawing Tools	Publications
Save Numbering to Molfiles	🔽 Import Mole	ecule Styles	
Auto-renumbering			
On Importing	🔽 On Joining F	Fragments	
Expand Labels On Importing     Automatically Open Table Of Compounds V	Vhen Importing A Molecule		
PhysChem Properties			
Update When Editing			
Open Babel Folder			
<ul> <li>Autodetect</li> </ul>			
Select			<b></b>
Keyboard Editing Always Available			
		DK <u>S</u> ave Loa	d Cancel


The tool "**Normalize Explicit Hydrogen Numbering**" renumbers only the explicit Hs to match with the heavy atom number (with appended a, b, c... letters):




The **Lock numbering** tool will fix the numbering for the selected part of the structure (using lasso). The fixed atoms will have a yellow background:

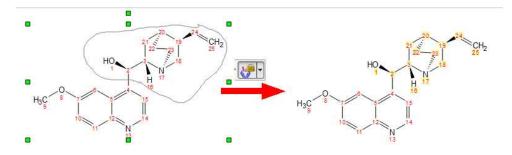

Clicking the '**Concatenate Numbering'** button, will de-duplicate the atom numbers of all the molecules in the document. The highlighted molecules will be renumbered so that the atom numbers are not repeated (leaving a gap from one molecule to another). The order in which molecules get renumbered will depend on the size of the molecule (the biggest molecule will keep its numbering).

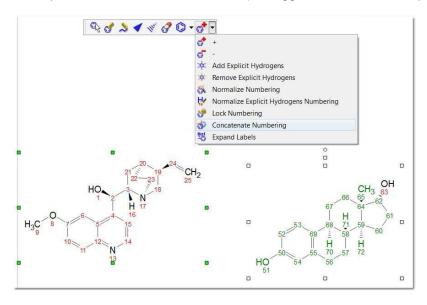

**Expand Labels:** to draw molecules with compacted groups and expand them by right clicking on the applicable group:

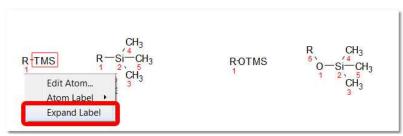

You can expand them by enabling the "Expand labels on importing" option in 'Preferences/Molecule' and also by clicking on the button "Expand Labels" in the Molecule toolbar.

Use the macro editor (under the General tab) to add free text labels and several parameters from the Molecule Properties:

20. 31	👩 Properties
Ho C Ho Ho C Ho Ho C Ho Ho C Ho Ho C Ho Ho Ho Ho Ho Ho Ho Ho Ho Ho Ho Ho Ho H	Additata Georetty, Molecular      Mannel, Bondis, General      Suber      Purnat: Free too(by)-to-Henris      Purnat: Arial
Time Stamp: jue 5. nov 17.12:00 1908	
Time Stamp: Jue 5. nov 17 12:00 1908 Macro Editor	
Macro Editor lat. (b:Malcole Label - (b- (indicabel)(br)-to-Time Stang (b- (indiferentiany))	OK Set as Default Restore OK Cancel Apply Cancel
Macro Editor	OK Genoel Apply

The molecule label is stored in a layout template and also gets applied when applying the template. See also the <u>Properties</u> chapter (for further information about the macro editor)

## 9.8.1 Molecular Structure

Mnova allows the user to import Molecular Structures, and to interact with them.

Currently, molecular structures can be imported as a **.mol**, **.cdx or .sdf** files by simply using the Open command (or by dragging & dropping the file to the Mnova icon or interface) exactly in the same way as this would be applied to a spectrum. Support to 'drag & drop' operations are currently limited to **ACD ChemSketch and ChemDraw**.


If you have OpenBabel installed, you will also be able to load (or copy&paste) molecular structures in INCHI and SMILE formats. For example you can copy to clipboard each line above (molecules in SMILE and INCHI formats) and then run Mnova and paste them as molecular structures: COc1cc(ccc1)C#NInChI=1S/C9H7F3O2/c10-6-2-1-5(7(11)8(6)12)9-13-3-4-14-9/h1-2,9H,3-4H2

You can also copy structures as MDL SK format (with abbreviated groups), to do that just copy the molecular structure to the clipboard (from ChemDraw for example) and follow the menu 'Edit/Paste Special':

Paste Special		
Source: CS Ch	emDraw Drawing	
	As:	
<u> <u> P</u>aste: </u>	CS ChemDraw Drawing	
Paste: Paste link:	CS ChemDraw Drawing MDL CT File MDL SK File	


You can keep the numbering from ChemDraw or the abbreviated structures by using the 'ChemDraw Exchage file' from the dialog box above.

If you are using IsisDraw, please keep in mind that you will need to select the capability to copy your molecules as mol files in the 'Options/General Settings' menu.

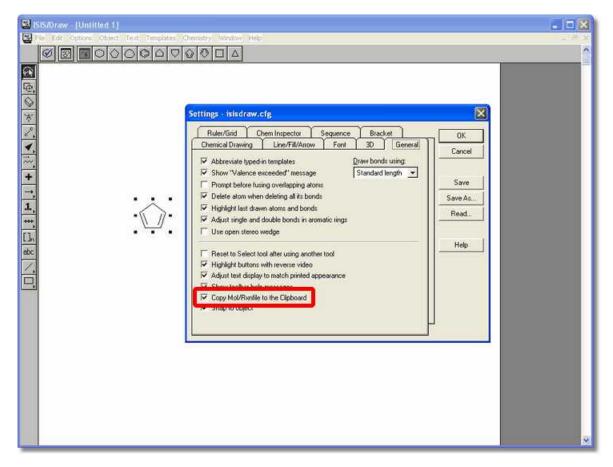

The molecular structure can be handled (resized, moved, aligned, copied, pasted, etc) exactly in the same way as all other Mnova objects. Molecular structures can be imported in a separate page or into a page already occupied by another object, such as for example its applicable spectrum.

The first thing you will notice when interacting with molecular structures, is the fact that atoms will become highlighted in a red transparent box when the mouse hovers over them. Clicking on an specific atom will make it the active atom and highlight in a red box with pink background, as can be seen in the figure below. This atom selection will become essential when interacting with the molecule, as will be explained in the following chapters.

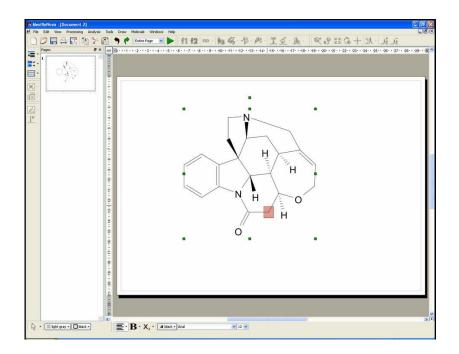


**Mnova** will allow you to customize the appearance of the molecule, by using the object 'Properties' dialog box. This box can be accessed by double clicking on the molecule, or by right clicking and then scrolling down to 'Properties'.

Atoms Bonds	Arrows General	
Rotate with Molect Symbols Show Carbons: Show Others: Font:	All 📝 Terminals	✓ Resize Fonts with Molecule         ✓ Label         Format: {atomNum}         Font:         Arial         Assignments         Color:         ✓ Show Quality

The 'Properties' dialog box will allow you to customize the size of the molecule, its angle with respect to the paper (geometry properties) and all representation properties, such as whether or not to show explicit carbon and hydrogen atoms, whether to show atom numbers, the length and spacing of bonds, etc. It is therefore possible to achieve many different representations of the same molecule, as the


## figure below shows.

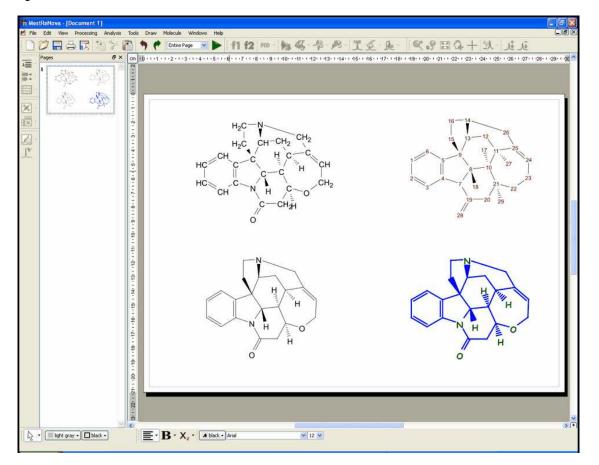

To customize the appearance of all the atom labels of the molecule, just double click on this button . From the 'Macro Editor' dialog box, you can add information about 'annotations', 'atom number', 'assignments', 'predicted chemical shift', etc.

Macro Editor			
Text			<u>O</u> K
{atomNum}, {stereo}			<u>C</u> ancel
Add Macro			
Available Macros:	Parameters:		
Annotation	1	1012	
Atom Index	Name	Value	
Atom Number			
Custom			
Custom			
6.52 (MAR) 1 (2 (MAR) 10 (M)			

In the example below, it is shown an atom label which contains information about the 'atom number'

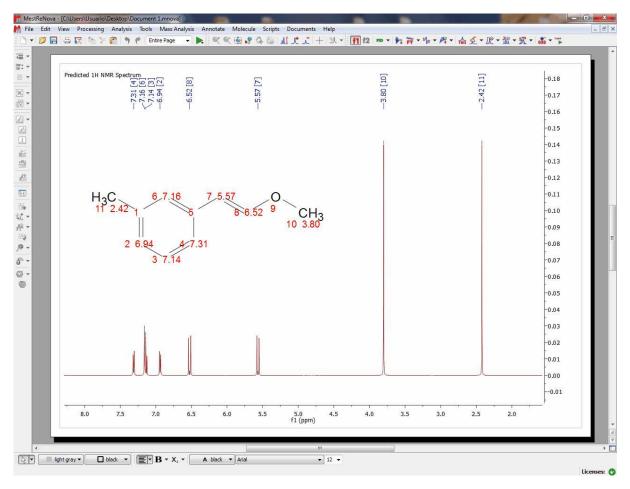


and the 'predicted chemical shift':

Double clicking on the applicable atom to edit its label:


	om Index: 25	Remove
	Property	Value
1	Number	25
2	Number Format	{atomNum}
3	Annotation	My atom
4	Color	Green
5	Hightlight Color	Orchid
5	Name	N
7	Charge	1
B	Isotope	15
9	Label	Nonamed

You can add a macro for the atom label (as it is shown a few lines above) in order to include information such as 'annotations', 'atom number', 'assignments', 'predicted chemical shifts' etc...

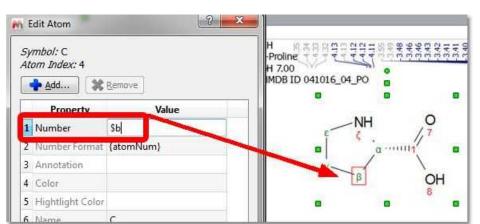


Typing the \$ prefix to add greek letters to the number; for example \$a, 4\$b, 22\$g\$d21 will be converted into , 4 , 22 21:

To define an isotope, you only need to enter the value of the mass number in the "Isotope" field. For example, in case of a C atom you can type 12, 13 and 14. The isotope number (and the charge) of an atom can be deleted by typing 0 or by deleting the number of the field.

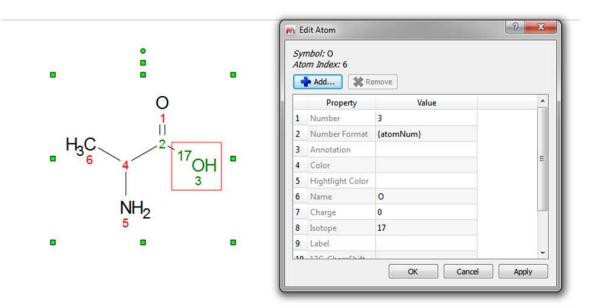

You can type any annotation, such a comment or a different numbering (just by changing the value of the 'Number' cell). You can change the color of the atom or of the highlight or even to add any property just by clicking on the this button Add...

In that case we have changed the number to the atom 25 (the new number is 99) and added a macro to show the 'Atom Number', the 'Annotation' (Test) and the 'Custom Property' (Vinyl), changing the color to green with a yellow highlight:

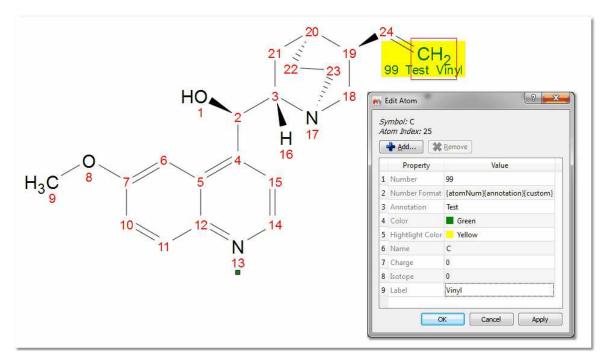


Highlight an atom and type the desired number to renumber it. If the new number already exists, the symbols # will appear on the duplicated numbers.

The new numbering can be exported in a mol file and you can 'import molecule styles' (for the 'Edit/ Paste Special' feature) by selecting the applicable option in the <u>Edit/Preferences/Molecules</u> menu.

🗌 🕐 📫 🧈	<b>%</b>	<b>1</b>	The second
General Plug-ins Database NMR	Mass Molecule	Scripting Drawing Tools	Publications
Save Numbering to Molfiles	📝 Import Molecu	ule Styles	
Auto-renumbering			
On Importing	On Joining Fragments		
Expand Labels On Importing     Automatically Open Table Of Compounds When Imp	orting A Molecule		
PhysChem Properties			
Update When Editing			
Open Babel Folder			
Autodetect			
Select			<b>E</b>
Keyboard Editing Always Available			


The "*keyboard editing always available*" preference, will allow you to type any letter when hovering the mouse over an atom.

Right clicking on any atom number of the molecular structure will display a context menu which will allow you to show the assignments, prediction, number, annotations or stereodescriptors as atom labels:

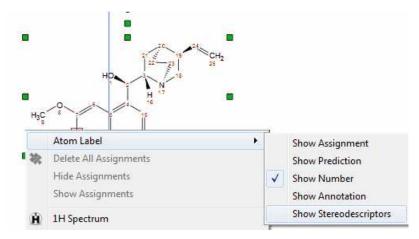

## 9.8.1.1 Compounds Table

This table will show all the molecules present in the document, with information about the chemical formula and molecular weight, name, label, description, color, etc.

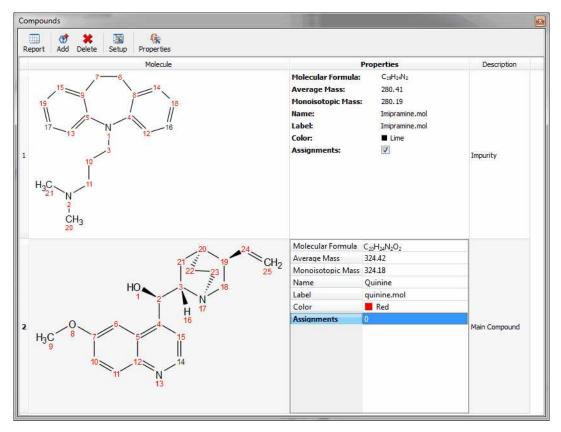

You can copy any molecule from this table to another page just by selecting it and clicking on the 'Report' button. Please bear in mind that the information about predictions and assignments is linked to the molecule and will be kept after having pasted it to another slide.

Clicking on the 'Add' button of the table, will allow you to add a new 'unknown structure', very useful to start assignments of unknown compounds.


Compounds	1.14			É
Report Add Delete Setup Properties				
Molecule	Pr	operties	Description	
	Molecular Formula: Average Mass: Monoisotopic Mass: Name: Label: Color: Assignments:	C <sub>19</sub> H <sub>24</sub> N <sub>2</sub> 280.41 280.19 Imipramine.mol Imipramine.mol Imipramine.mol	Impurity	E
2 Ho Ho S S HO HO HO HO HO HO HO HO HO HO HO HO HO	Molecular Formula: Average Mass: Monoisotopic Mass: Name: Label: Color: Assignments:	C2dH24N2O2 324.42 324.18 Untitled 2col_StyleSheet-1 Untitled 2col_StyleSheet-1 Red	Main Compound	
Unknown	Molecular Formula: Average Mass: Monoisotopic Mass: Name: Label: Color: Assignments:	C₂sH₂cO3 368.42 368.14 Unknown Unknown ⊠ None		

The user can type the name, label (to be displayed in the assignments) and molecular formula when creating a new unknown compound from the Compounds Table:


Name:	
abel:	
Molecular Formula:	

This compound can be assigned in the same way as a molecule, but it's represented as a text item, only the label is shown (the molecular structure is not shown).

By default, all the assignments (of all compounds) will be displayed on your spectral window, however you can use the toggle of the 'Assignment' check box for each compound of the table to show only the applicable assignments for that compound. When the user checks the checkBox, Mnova hides the assignments of all the molecules except the assignments of the current molecule. When the user unchecks the checkBox, Mnova hides all the assignments of the current molecule. (The same behaviour as in the molecule context menu: Hide Assignments).

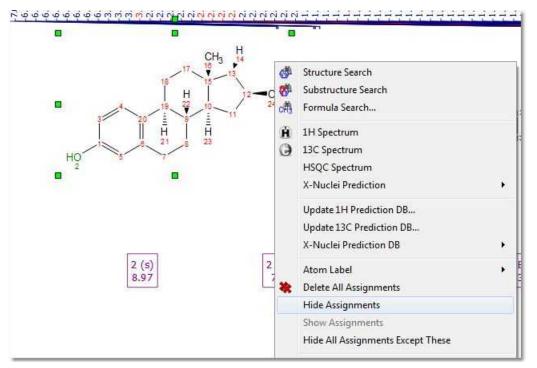

Add a property by right-clicking on the 'Properties' column and selecting 'Add Property':

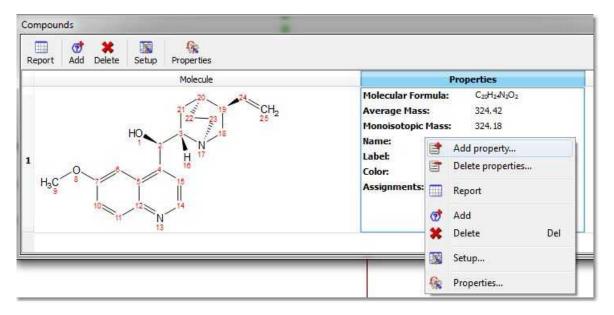

The added properties can be deleted in the same way, by selecting 'Delete Properties'. The visibility of these properties can be also customized via Properties button. By default the visibility is setup as automatic.

If you import a SDF file with several tags, you can display them by checking the applicable boxes:


	Visible Name	Visible	Decimals	*
ID	ID		0	
INPUTDATA	INPUTDATA		0	
MSD	MSD		0	
NMR-Nr.	NMR-Nr.		0	
NMR_CONSTANTS	NMR_CONSTANTS		0	
ORGFILENAME	ORGFILENAME		0	
REMARKS	REMARKS		0	
SOLVENT	SOLVENT		0	
VU	VU	1	0	=
Parameter: Acquisition Time (sec)	Parameter: Acquisition Time (sec)		0	1
Parameter: Comment	Parameter: Comment		0	-
Parameter: Date	Parameter: Date	1	0	
Parameter: Date Stamp	Parameter: Date Stamp		0	
Parameter: File Name	Parameter: File Name		0	
Parameter: Frequency (MHz)	Parameter: Frequency (MHz)		0	
Parameter: Nucleus	Parameter: Nucleus		0	
Parameter: Number of Transients	Parameter: Number of Transients		0	
		2 million (	-	+

There will be three type of boxes (empty, blue filled and checked): Empty: the parameter will not be visible Filled: the parameter will be visible only if it the filed is not empty Checked: the parameter will be always visible (even when the field is empty)

You can edit any of the properties from the table, by double clicking on it, typing the new value and **pressing the 'enter' key** to update the changes.

# 9.9 NMR Prediction

**NMR Prediction:** The handling of molecular structures within **Mnova** also allows the user to carry out **spectral predictions**. Although the process described here could be applied to predictions by means of any commercially available or in-house prediction package, currently **Mnova** will carry out predictions by using the prediction application **NMRPredict**, by **Modgraph Consultants Ltd**.

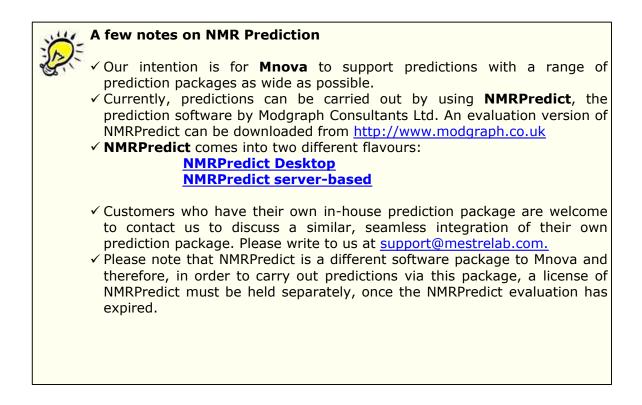

Mnova incorporates a fast simulation mode of <sup>1</sup>H, <sup>13</sup>C and X-nuclei (<sup>11</sup>B, <sup>15</sup>N, <sup>17</sup>O, <sup>19</sup>F, <sup>29</sup>Si, <sup>31</sup>P) NMR spectra, called **NMRPredict Desktop.** 

Pred	dict Scripts Documents Help		
A O	1H Spectrum 13C Spectrum HSQC Spectrum	μ	大九山
	X-Nuclei Prediction	B	11B Spectrum
22	Prediction Options		15N Spectrum
	Update 1H Prediction DB Update 13C Prediction DB X-Nuclei Prediction DB		170 Spectrum 19F Spectrum 29Si Spectrum 31P Spectrum
-	Rrowse Prediction DR	10	STA Shecting

The reference used for the prediction are listed below:

<sup>1</sup>H, <sup>13</sup>C and <sup>29</sup>Si (0.00 ppm, TMS); <sup>11</sup>B (0.00 ppm, BF<sub>3</sub>.Et<sub>2</sub>O); <sup>15</sup>N (0.00 ppm, NH<sub>3</sub>); <sup>17</sup>O (0.00 ppm, Water); <sup>19</sup>F (0.00 ppm CF<sub>3</sub>COOH); <sup>31</sup>P (0.00 ppm, H<sub>3</sub>PO<sub>4</sub>),

You can change the references by editing the file named "CSEARCH.REF" stored in the Mnova installation folder:

C:\Program Files (x86)\Mestrelab Research S.L\MestReNova\NMRPredict\csearchho3abhijmab

The path to the file in Mac is

/Applications/MestReNova.app/Contents/MacOS/NMRPredict/csearchho3abfhijkmab/CSEARCH.REF

For example, The F19 is referenced CF3COOH. To change the reference, you will need

This application does not need to connect itself to a server for the spectra prediction. Besides, it makes uses of the fastest prediction algorithms (**Neural Network, Charge, Increments** and **Best**) implemented into **NMRPredict**.

Watch a miniclip on this functionality here

## 9.9.1 Random Forest prediction

Mnova Lite SE come with a new module for the fast and accurate prediction of 1H and 13C NMR spectra. It consists of a novel proprietary algorithm based on a *machine learning* algorithm (Random Forests) which has been training with a large database of experimental assigned 1H and 13C chemical shifts as well as proton scalar coupling constants.

#### Running a Prediction

Once a molecule is available in Mnova, predicting a 1H or 13C spectrum can be done by simple selecting that option either from the *Predict* menu or by right clicking on the molecule and selecting the prediction from corresponding contextual menu.

First time a prediction is run, it can take a few seconds for the mathematical prediction model to be loaded in memory. This is done only once, so subsequent predictions will be extremely fast, although the model will be unloaded from memory if no predictions are run during five minutes.

#### **Prediction options**

From:	-2.00 ppm	*
To:	10.00 ppm	Å
Number of Points:	32 K	•
Frequency:	500.13 MHz	*
Line Width:	0.75 Hz	-
Solvent:	Chloroform-d	-

From/To: Lower and upper limits for the chemical shift scale

**Number of Points**: Number of points used to build the predicted spectrum. Actually, Mnova predicts a time domain signal (FID) which is automatically Fourier Transformed to yield the final predicted frequency domain spectrum.

Line Width: Line width at half height of all peaks in the predicted spectrum.

Solvent: Prediction solvent.

## 9.9.2 Modgraph NMR Predict Desktop

**Mnova** integrates a fast simulation module of <sup>1</sup>H and <sup>13</sup>C-NMR spectra, called **Modgraph NMRPredict Desktop**.

See also <u>'How to predict a spectrum with NMRPredict Desktop?</u>

NMRPredict Desktop is faster than NMRPredict server-based, because it does not need to log in to a server to predict a spectrum. Besides, it makes use of the fastest prediction algorithms (Neural Network, Charge, Increments and Best) implemented into NMRPredict. Other very significant advantages are that the software can be used without an internet connection, there are no access issues with firewalls, and no risk to confidential data being sent over the internet.

**NMRPredict Desktop** uses a Neural Network system for the prediction of <sup>13</sup>C-NMR spectra, and the NMR tables (**increments** methodology) of Professor Ernö Pretsch (ETH, Zürich) for a fast simulation mode of <sup>1</sup>H and **X-nuclei:** <sup>11</sup>B, <sup>15</sup>N, <sup>17</sup>O, <sup>19</sup>F, <sup>29</sup>Si, <sup>31</sup>P NMR spectra, as well as the **CHARGE** program which offers <sup>1</sup>H-NMR prediction based upon partial atomic charges and steric interactions.

NMR Predict Desktop also includes the calculation of heteronuclear (HF, HP, CF and CP) couplings.

**CHARGE** offers the **first** quantitative prediction of the proton chemical shifts of a variety of organic compounds. It works by first generating 3D conformers from a 2D structure through a choice of *force fields* and then predicting proton spectra for all the conformers. The program works by looking at functional groups which have been parametrised by Professor Abraham.

To read more about the scientific theory behind CHARGE, please visit the following link:

http://www.modgraph.co.uk/product\_nmr\_proton.htm

The **CHARGE** and the **Increment** algorithms included in **NMRPredict Desktop** are the same as used in the Server-based version to predict <sup>1</sup>H-NMR spectra, whereas for the prediction of <sup>13</sup>C-NMR spectra; **NMRPredict Desktop** uses a **Neural Network** system, but not the HOSE database methodology implemented additionally in the server-based application.

The **Best** algorithm is the combined approach between the Increments and the Conformers algorithm that is capable of producing significantly improved proton NMR predictions for the data set upon which it has been tested down to below the 0.2 ppm target error.

You will find further information about this feature in:

http://www.modgraph.co.uk/best\_proton\_press\_release.htm

Please bear in mind that we are not giving any guarantees that the "Best" will always give prediction accuracy as low as 0.18 ppm. Statistically this is what we got against the 1.1 million shift values in the 90,000 data we used. This may or may not be the case with user data.


The **Neural Network algorithm** is much more general and error tolerant than the HOSE code approach (based on a reference spectra database) and is much more accurate at predicting shifts not found in the database.

The Neural Network prediction method in **NMRPredict Desktop** was developed during the mid 1990s in the group of Professor Robien at the University of Vienna. It was developed by V Purtuc and gave a very broad application range to cover general organic chemistry.

The basic design principles as defined in 1995 were:

- to be general enough and be able to handle problems from basic organic chemistry to complex natural products.
- to be able to handle "unusual" organic chemistry like organometallics.
- to be solvent specific during prediction.
- to be able to use stereochemical information not restricted by ring size, in the same way as could be done within the HOSE code technology.
- to make sure that only interpolation and not extrapolation occured when making predictions.

The Neural Network implemented into **NMRPredict Desktop** has been thoroughly tested and proved to be both reliable and accurate. The 4,000,000 assigned chemical shift values of the available 345,000 reference spectra can be predicted with an average deviation between experimental versus calculated of below 2.00 ppm. This includes compounds which are not well handled by traditional prediction programs, such as ferrocenes and chromium complexes.




## ATTENTION


Bear in mind that, in terms of stereochemistry, drawing a structure as a chair or as a boat means nothing to the .mol file and the computer. In those cases the user must draw all the corresponding bonds to show the stereochemistry of the molecule, i.e., you must explicitly draw up and down bonds using wedges.

#### 9.9.2.1 Running predictions


Carrying out of predictions in Mnova with **NMRPredict Desktop** is very easy. Just load a molecule into Mnova and right click on it to select the desired prediction (or follow the 'Predict' menu):

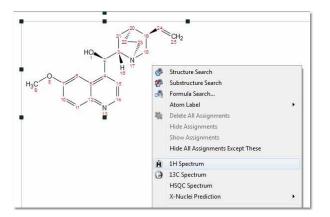


After that, you will obtain the desired predicted spectrum using a rigorous full quantum mechanics method taking into account any second order effect present in the predicted spin(s) systems(s):

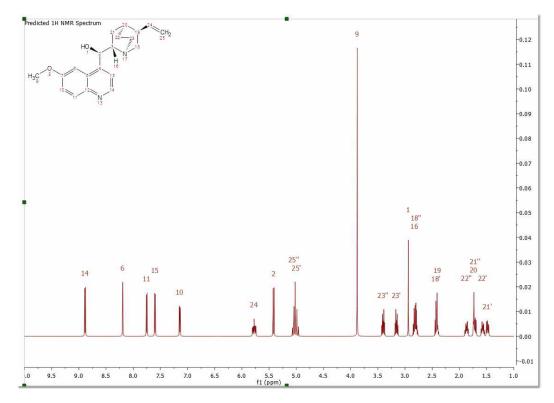


This predicted spectrum can be analyzed as a real one (e.g. it can be integrated, etc). The user can also visualize and edit the chemical shift and coupling constants values from the tables of the predicted spectrum by following the menu 'View/Table/1H Prediction'. Please bear in mind that the peak labels and the multiplet boxes will show the applicable atom numbers of the prediction.

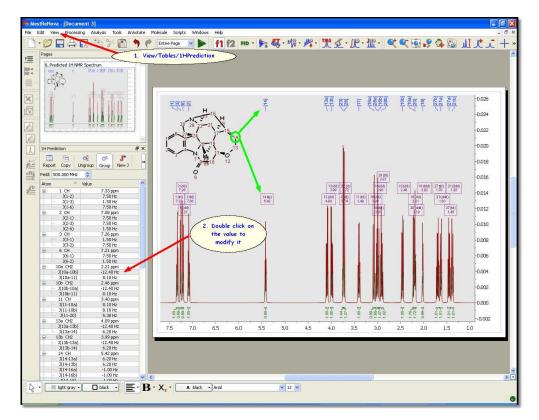

Click&drag over the prediction label to graphically modify the chemical shift of the predicted signals:

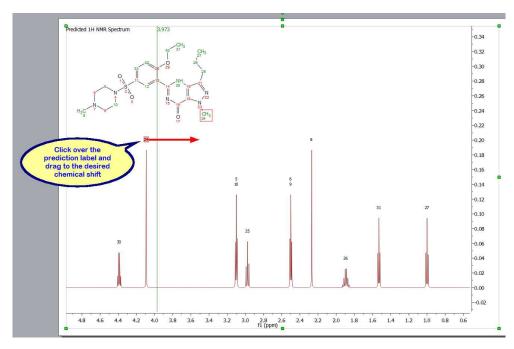

You can change the predicted coupling constants by showing the multipet tree from the <u>Prediction</u> <u>Properties'</u> dialog box and clicking&dragging:

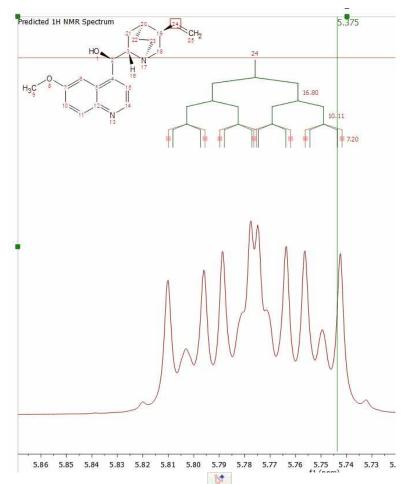


Click on the on the 'New J' button was to introduce new coupling constants:


Report Copy	Ungroup	Group New J Expand Collapse Setup	
Field: 500.13 MHz	<b>A</b>		
Atom	Value	Error	-
3(11-6)	0.50 Hz	0.5 Hz	
J(11-10)	7.50 Hz	-1 Hz	
4 14 CH	8.88 ppm	0.35 ppm	
J(14-15)	7.50 Hz	-1 Hz	
4 15 CH	7.60 ppm	0.5 ppm	in.
J(15-6)	0.50 Hz	0.5 Hz	
J(15-14)	7.50 Hz	-1 Hz	
4 16 611	New J	? ×	=
J(10-			-
J(16-	;		-
J(16-1			
J(16-2 18' CH2	Atom 1: 1	▼ Atom 2: 1 ▼ Value: 1.00 +	
J(16- J(16- J(16- J(18- J(18-	Atom 1: 1	▼ Atom 2: 1 ▼ Value: 1.00 💠	
J(16-; 4 18' CH2 J(18'- J(18'-	Atom 1: 1		
J(16- 18' CH2 J(18'- J(18'- J(18'- 4 18" CH2	Atom 1: 1	Atom 2: 1  Value: 1.00  OK Cancel	
J(16- ▲ 18' CH2 J(18'- J(18'- ▲ 18" CH2 J(18"-	Atom 1: 1		
J(16- 18' CH2 J(18'- J(18'- 18" CH2 J(18"- J(18"- J(18"-		OK Cancel	
J(16- 18' CH2 J(18'- J(18'- 18" CH2 J(18"- J(18"- J(18"- J(18"- J(18"- J(18"- J(18"- J(18"- J(18"- J(18)'-	2.41 ppm	OK Cancel	
J(16- J(18') J(18' J(18') J(18' J(18') J(18' J(18') J(18') J(18') J(18') J(18') J(18') J(19'	2.41 ppm 7.90 Hz	OK Cancel	
J(16- J(18' CH2 J(18'- J(18'- J(18'- J(18'' J(18'' J(18'' J(19'- J(19-18'') J(19-18'')	2.41 ppm 7.90 Hz 7.90 Hz	0.7 ppm -1hz -1hz	
J(16- J(18' CH2 J(18'- J(18') J(18') J(18') J(19') J(19-18') J(19-18') J(19-20)	2.41 ppm 7.90 Hz 7.90 Hz 1.80 Hz	0.7 ppm -1 hz -1 hz -1 hz	
J(16- J(18' CH2 J(18'- J(18'- J(18'- J(18'' J(18'' J(18'' J(19'- J(19-18'') J(19-18'')	2.41 ppm 7.90 Hz 7.90 Hz	0.7 ppm -1hz -1hz	
J(16- J(18') J(18') J(18') J(18') J(18') J(19') J(19') J(19-18') J(19-20) J(19-24)	2.41 ppm 7.90 Hz 7.90 Hz 1.80 Hz 6.20 Hz	0.7 ppm -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz	
3(16- 4 18' CH2 3(18'- 3(18'- 1(18''- 1(18''- 4 19' CH2 3(18''- 4 19 CH 3(19-18'') 3(19-20') 3(19-24') 3(19-25')	2.41 ppm 7.90 Hz 7.90 Hz 1.80 Hz 6.20 Hz -1.00 Hz	OK Cancel	
J(16- J(18' CH2 J(18' J(18' J(19'	2.41 ppm 7.90 Hz 7.90 Hz 1.80 Hz 6.20 Hz -1.00 Hz -1.00 Hz	0.7 ppm -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz -1 Hz	
3(16- ▲ 18' CH2 J(18' J(18' J(19' 18' J(18' 18' 18' J(18' 18' J(18' 18' 18' J(18' 1	2.41 ppm 7.90 Hz 7.90 Hz 1.80 Hz 6.20 Hz -1.00 Hz 1.74 ppm	OK Cancel	

After that, the 'New J' dialog box will be displayed and you will only need to select the atoms involved in the coupling and the value of the new coupling constant. Click on OK and the new coupling constant will be added to the spectrum and also to the prediction table.

Finally, to know the "predicted assignment", just hover the mouse over the desired atom, (so that it becomes highlighted in a red box) and the corresponding signal in the spectrum will automatically be highlighted in blue; or vice versa (hovering the mouse over the peak will highlight the applicable atom on the molecular structure). You will also get highlights in the applicable row of the 'Prediction table':

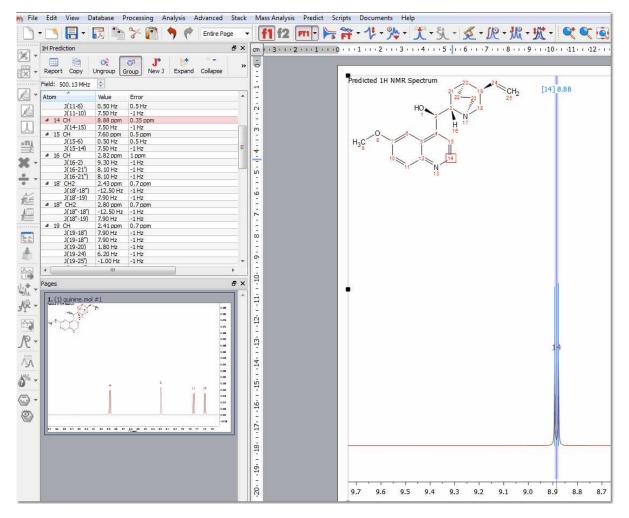


Please bear in mind that NMR Predict Desktop also includes the calculation of heteronuclear (HF, HP, CF and CP) couplings:

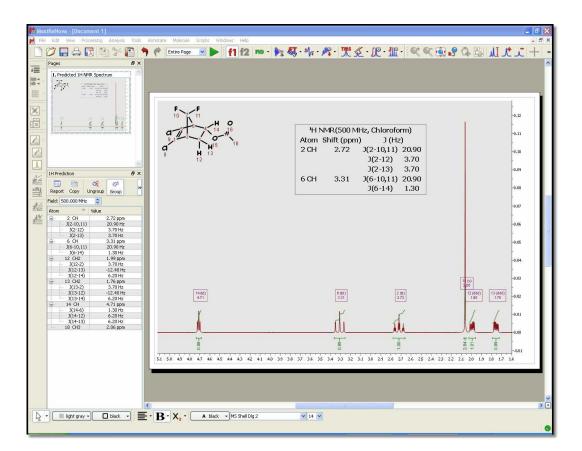


If you need the <sup>13</sup>C-NMR predicted spectrum, follow the same instructions but selecting the options for '13C' (be sure that you select the correct tab for 13C in the 'NMR Predictor Box' dialog, red square in the figure below). As you can see in the 'NMR Predictor Option' box below, you can select the limits, the number of points, the frequency and the line width of the spectrum. You can predict 'DEPT' (CH and CH3 up and CH2 and Quaternary carbons down) and spectra with only protonated carbons (DEPT 45) by checking the applicable boxes. If you want to get a DEPT 135, you must check both boxes.

H 13C HSQC	31P 19F 15N 11	B   17∛
From:	-20,00 ppm	\$
To:	230.00 ppm	*. *
Number of Points:	32 K	•
Frequency:	125.03 MHz	
Line Width:	1.50 Hz	
Solvent:	Common NMR Solvents	
DEPT	Protonated Carbons O	nly
Predictor:	Modgraph NMRPredict De	sktop 🔻


Here you can see an example of a DEPT 135 prediction:

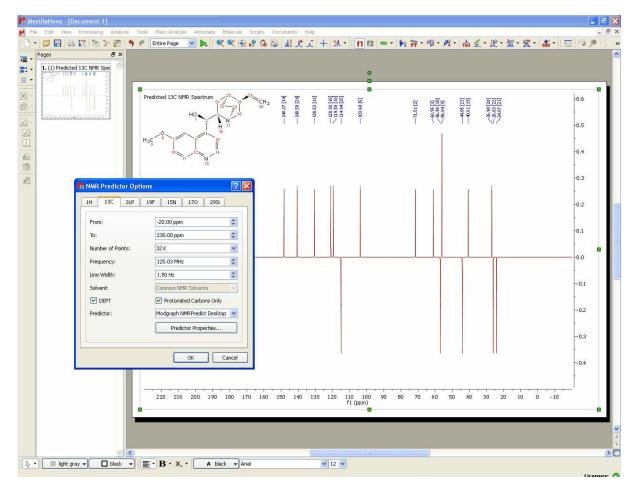


Follow the menu 'Scripts/NMR Tools/Predict 1H and 13C' to get both predictions in the same page:

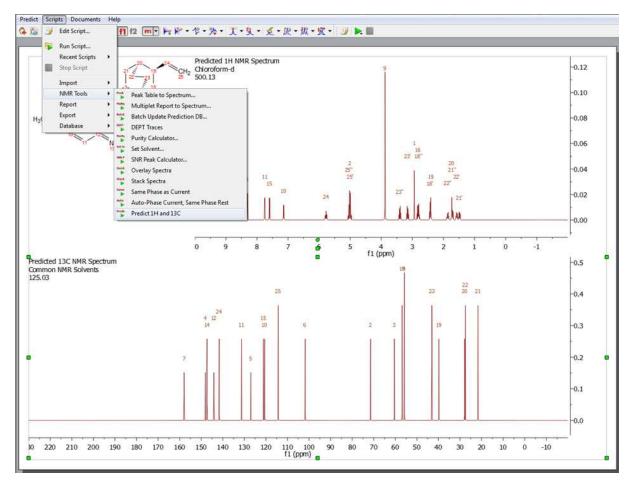

Follow the menu 'Predict/HSQC Spectra' to predict a HSQC spectra from a given molecule:

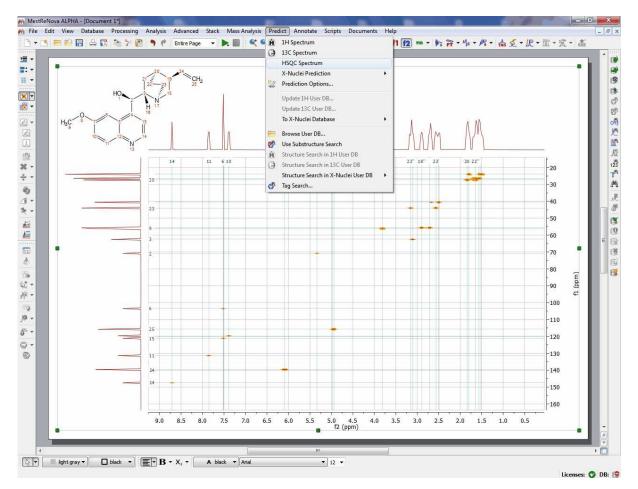


You can modify the predicted chemical shifts either graphically, by clicking&dragging any prediction label, or by typing the new values in the prediction tables:

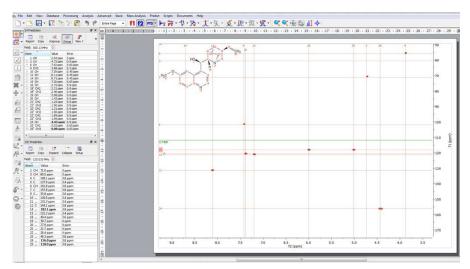


The same procedure will be followed to run X-Nuclei predictions <sup>11</sup>B, <sup>15</sup>N, <sup>17</sup>O, <sup>19</sup>F, <sup>29</sup>Si, <sup>31</sup>P (under the menu 'Predict/X-Nuclei Predictions'):


Å O	1H Spectrum 13C Spectrum HSQC Spectrum		μ	大九山
	X-Nuclei Prediction	•	8	11B Spectrum
22	Prediction Options			15N Spectrum
	Update 1H Prediction DB		0	170 Spectrum
	Update 13C Prediction DB		Ð	19F Spectrum
	X-Nuclei Prediction DB		S	29Si Spectrum
-	Browce Prediction DR		Ð	31P Spectrum

And here you can see an example:

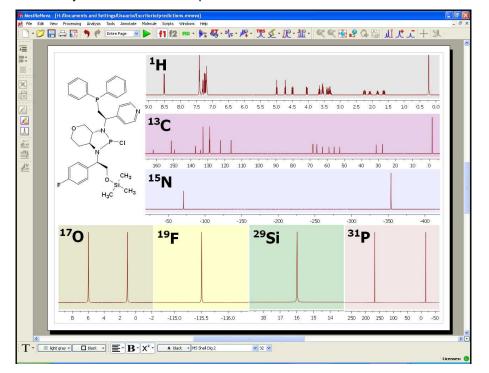




You can see (in the picture below) the higher order effects observed in the 1H predicted spectrum of the cholesterol:

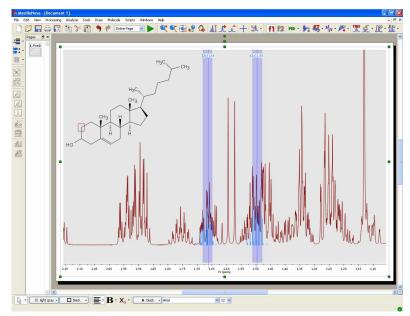

After having run an NMR prediction, the <u>Spin Simulation</u> panel will be automatically populated with the predicted values:

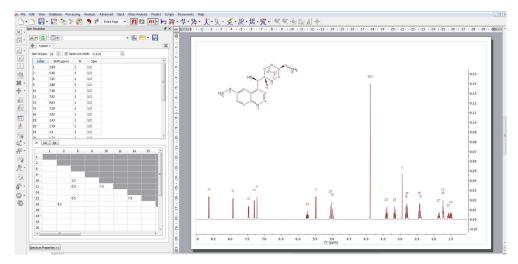

Modifications done in the spin simulation panel will be reflected in the 1H Prediction table (an vice versa); those changes will be graphically updated in the applicable synthetic spectrum.


#### See also: How to predict a spectrum with NMRPredict Desktop?

#### 9.9.2.2 Automatic Assignments

#### (NMR plugin is needed)

Mnova automatically does atom to peak assignments to 1H, 13C and HSQC spectra.

Just load your NMR spectrum (1H, 13C and HSQC; alone or combined) with the applicable molecular structure and follow the menu 'Analysis/Auto Assignments':

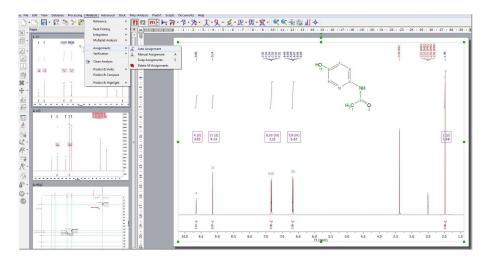

Mnova will automatically run a multiplet analysis and will fully assign your spectra with the applicable molecular structure. The multiplet boxes will be renamed with the corresponding atom number of the molecule and you will get an assignment label with the atom number over the applicable peak. In addition, hovering the mouse over the atom will highlight the applicable signal in the spectrum.


See also 'How to carry out assignments?'

#### 9.9.2.3 Predict & Highlight

You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder). NMR plugin is needed.

This feature will calculate in the background a simulation of the spectrum of the molecular structure present in the spectral window, highlighting the expected chemical shifts when the user hover the mouse over a proton or a carbon. This tool will be very useful to help the user in the process of assigning of NMR spectra.


The user will be able to use this tool with 1D and HSQC NMR spectra just by pasting the applicable molecular structure (quinine, in this example) over the spectrum and following the menu 'Analysis/ Predict & Highlight', as is shown in the picture below:

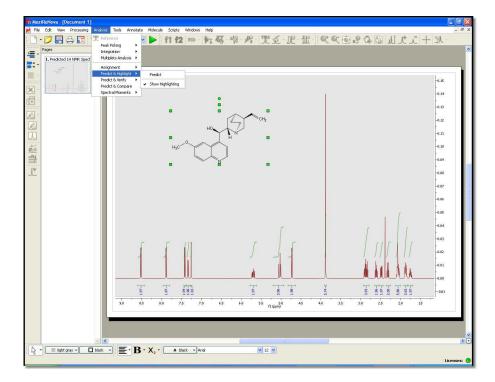


The algorithm of the simulation carried out in the background will be the selected in the 'Predict/ Prediction Options' menu.

The same feature can be applied by selecting the molecule on the Compounds Table.


After having applied this feature, the user will be able to notice that hovering the mouse over the atom will highlight the applicable simulated area in the spectrum. So the user will know that this signal will correspond with the proton of the carbon number 9 in the quinine.

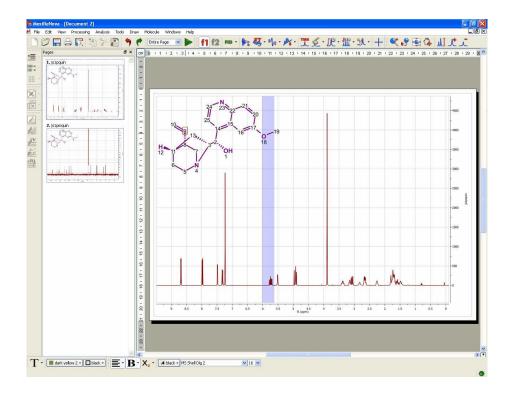

The user will be able to apply the same feature with the <sup>13</sup>C NMR spectra, as is shown in the picture below:

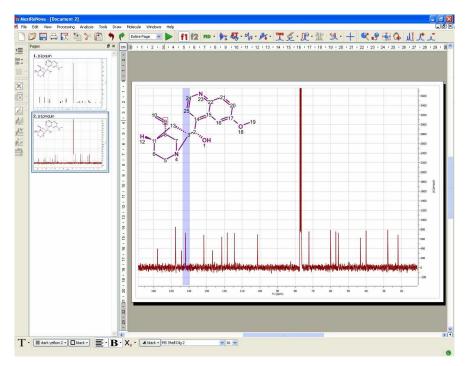

Here you can see an example with a HSQC:

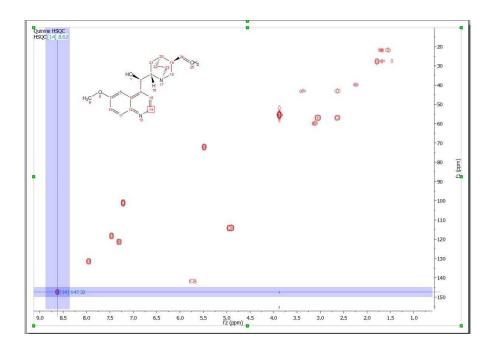

## 9.9.2.4 Predict & Compare


### (NMR plugin is needed)

This feature will display in stacked mode, the experimental dataset and a simulation of the spectrum of the molecular structure present in the spectral window, highlighting the expected chemical shifts when the user hovers the mouse over a proton or a carbon. This tool can be used of assistance in the process of assigning <sup>1</sup>H and <sup>13</sup>C NMR spectra.


The user will be able to use this tool with <sup>1</sup>H and <sup>13</sup>C NMR spectra just by pasting the applicable molecular structure (quinine, in this example) over the spectrum and following the menu 'Analysis/ Predict & Compare'. The same feature can be applied by selecting the molecule from the Compounds Table (without a need for having the molecule pasted on the relevant page, affording users the flexibility to run different predictions without having to generate many instances of the molecule on their report).

After the prediction is run, Mnova synthesizes the corresponding 1H-NMR spectrum using a rigorous full quantum mechanics method taking into account any second order effect present in the predicted spin(s) systems(s).


For example, in the figure below, you can see the results of running a prediction and comparing the resulting 1H spectrum with its experimental counterpart:

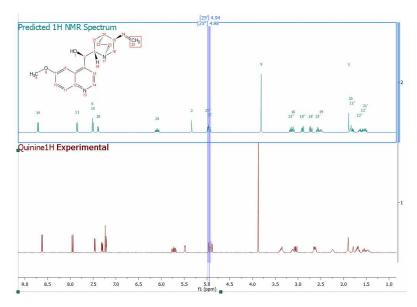


As you can see, you will get the predicted spectrum on top with the proton assignments labels. You can draw (or load) a second molecule over the 'Predict&Compare' result, in order to get a new prediction in the stack:

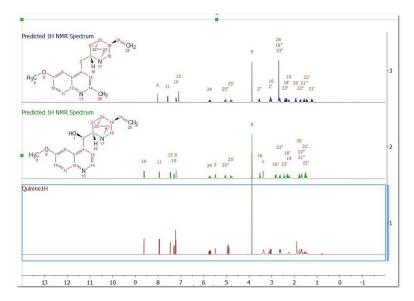


Hovering the mouse over the assignment labels and clicking&dragging will change the chemical shift in in real time:

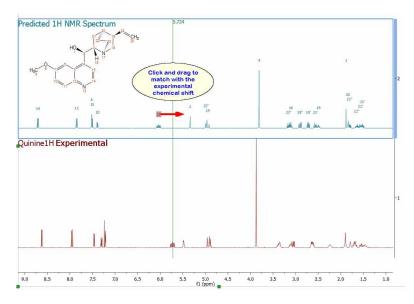


Even you can graphically modified the predited coupling constants (just by clicking&dragging) if you have selected the option to show the coupling tree in the Multiplet properties

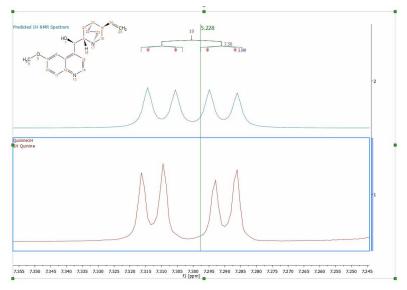

Once you have modified the prediction, you can update those changes to the <u>prediction Database</u> to enhance the prediction results of similar structures. To do it, just right click on the molecular structure and select 'Update Prediction DB':



If you load a 1H-NMR spectrum with a multiplet analysis and run Predict and Compare; you will get a stack plot with the multiplet boxes displayed in the experimental spectrum, so you can easily assign

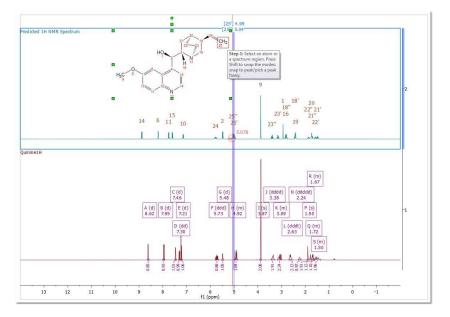


those multiplets to the molecular structure and finally update the 'Prediction DB' if you wish:

## 9.9.2.5 Predict & Verify


This chapter describes a new feature to validate molecular structures, which is based on the concurrent analysis of two simulated 1D (<sup>1</sup>H and <sup>13</sup>C) NMR spectra and a real 2D NMR one-bond correlation spectrum, such as HMQC or HSQC (experiments which correlate the chemical shift of the proton with the chemical shift of the directly bonded carbon).

The procedure to apply a **Visual Verification** with Mnova is very easy, just load your HSQC or HMQC spectrum, and follow the menu: 'Analysis/Predict & verify/HSQC' with the applicable molecular structure pasted on the spectral window as is shown in the pictures below:


1<sup>st</sup>: Load the HSQC or the HMQC spectrum in Mnova:

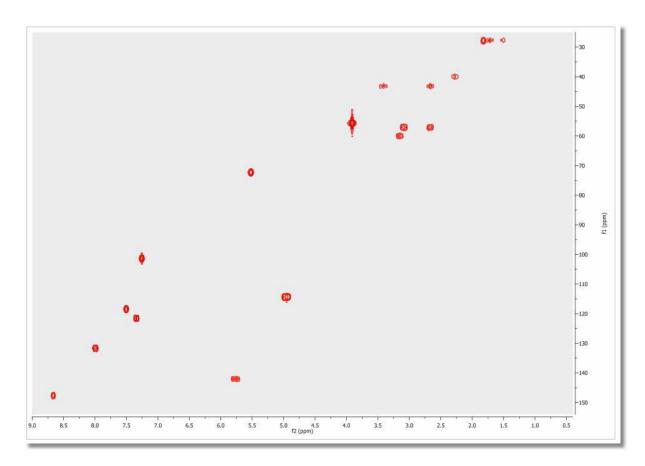

2<sup>nd</sup>: Paste (or load) the applicable molecular structure. Bear in mind that molecular structures can be imported as a **.mol** file by simply using the 'Open' command exactly in the same way as this would be applied to a spectrum. Keep in mind that you are also able to copy & paste structures from **ChemDraw, ChemSketch** and **IsisDraw**.

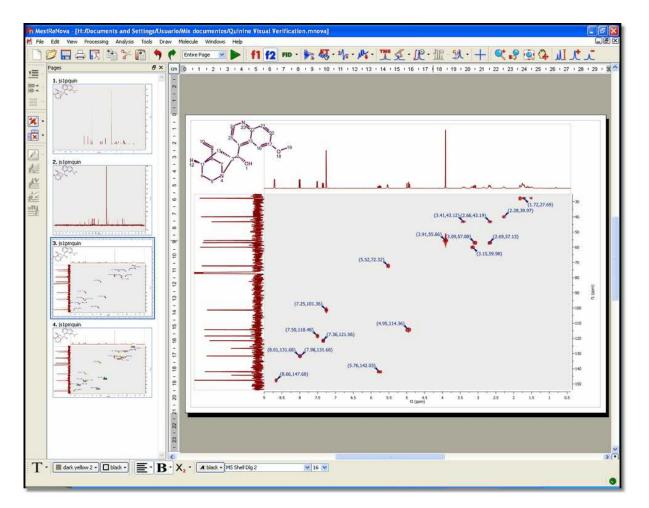


3<sup>rd</sup>: Follow the menu: 'Analysis/Predict & Verify/HSQC' to obtain the corresponding analysis:

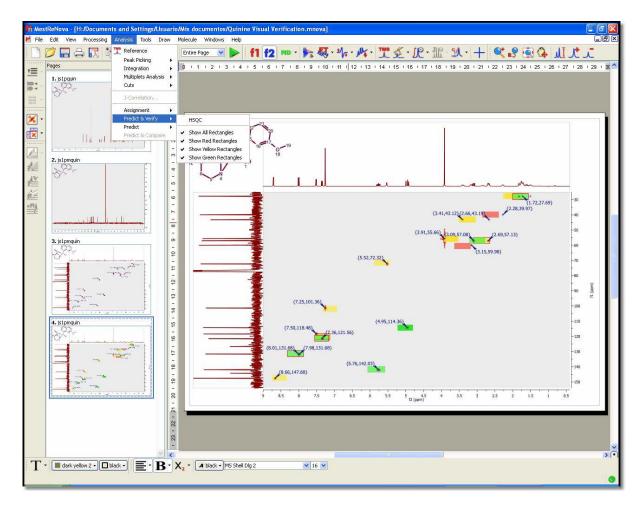

The same feature can be applied by selecting the molecule in the Compounds Table.


As you can see in the picture above, green, yellow and red rectangles will be obtained in the analysis.

A green rectangle will appear when the simulated value fits with the experimental one (the experimental value falls within a rectangular window, drawn around the simulated value, with dimensions of 0.2 ppm along the proton dimension and 2 ppm along the carbon dimension). A yellow rectangle will be displayed when an experimental peak falls within a window which is between 0.2 and 0.4 ppm along the proton dimension and 2 and 4 ppm along the carbon dimension. Finally, the red rectangles are displayed when no experimental peak is found within the latter rectangle, with the simulated value at its center and dimensions of 0.4 ppm along the proton dimension and 4 ppm along the carbon dimension.

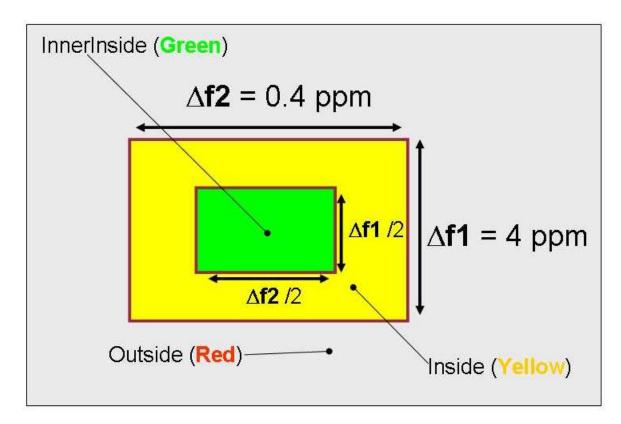


For example, if we have a real cross peak in the HSQC spectrum at (1.00, 10.0) ppm and a simulated value of (1.05, 10.2) ppm, then we shall obtain a green rectangle, because there is a experimental peak within the rectangle with a predicted peak at its center and sides of 0.2 ppm along the proton and 2 ppm along the carbon dimensions, which we will call 'inner inside'. If we would have a simulated value of (1.25, 11.0) ppm, then we would get a yellow rectangle drawn around the simulated value, as the experimental peak values would fall outside the 'inner inside' but within the area, drawn around the predicted peak, with sides of 0.4 ppm along the proton dimension. In this case the carbon simulation would be fine, but we would get a yellow rectangle due to the deviation in the proton prediction. If the simulated value for this cross peak was (1.41, 15.0) ppm, then we would obtain a red rectangle.

Finally, we shall get a rectangle with a red border when more than one experimental cross peak falls within the green or yellow rectangles drawn around a predicted peak, as is shown in the picture below:

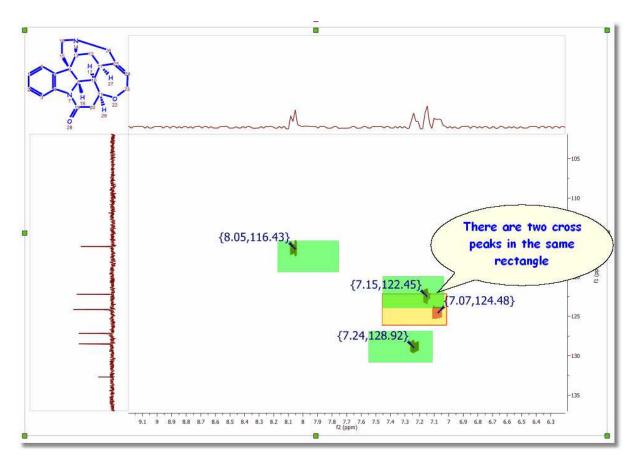

The user also has the ability to display any combination of rectangles, such as only red rectangles or green and yellow rectangles, for example. These options are available from the 'Analysis/Predict & Verify' menu.

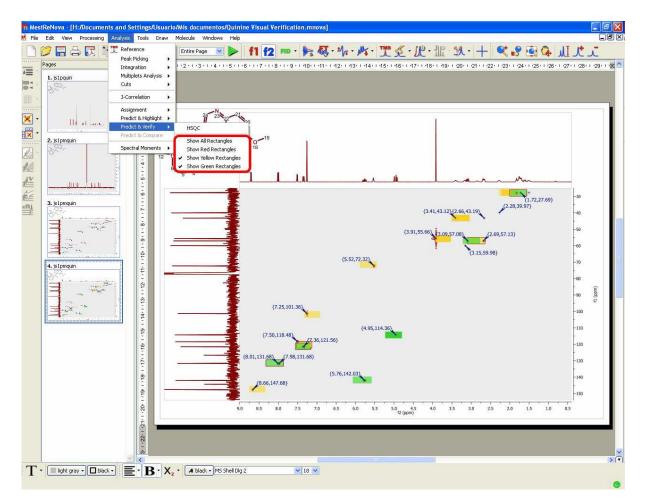


Bear in mind that the results reported by visual verification will depend on the prediction algorithm used in the spectral simulation. The user will be able to change this algorithm by following the menu: ' Predict/Prediction Options/Predictor Properties'.

### 9.9.2.6 Prediction Database


This feature will allow the user to build databases with experimental assigned spectra which can be used to enhance the prediction results of similar structures.

You can build <sup>1</sup>H, <sup>13</sup>C and X nuclei (<sup>11</sup>B, <sup>15</sup>N, <sup>17</sup>O, <sup>19</sup>F, <sup>29</sup>Si, <sup>31</sup>P) NMR databases from any Mnova document containing a molecular structure with the resulting assignments.


Building the database is really easy, just open your NMR dataset with the molecular structure; make the <u>assignments</u> and follow the menu 'Predict/Update 1H Prediction DB' (you can also update the prediction database from the Well Plates view of the DB plugin by right clicking on any of the plates, or even directly from a predicted spectrum).

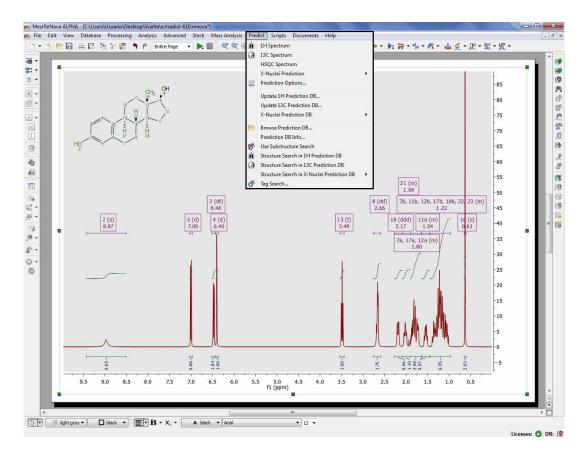


This will display a new dialog box, with information about the molecular structure and the assignments. From here, you can select the DB Letter to save your assignments (from 'N' to 'Z'; the database letter chosen represents the unit which can be excluded from any subsequent prediction or search. Thus, the database letter should be carefully selected on an organization wide basis).

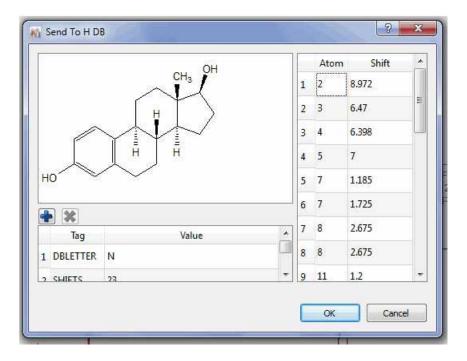

Here we can see the effect of having updated the prediction database. The blue spectrum corresponds with the original dataset, the green one with the original prediction (prior to the update of the Database) and the red one corresponds with the resulting predicted spectrum after having updated the database with the assigned experimental dataset. As you can see, now the prediction is even more accurate!

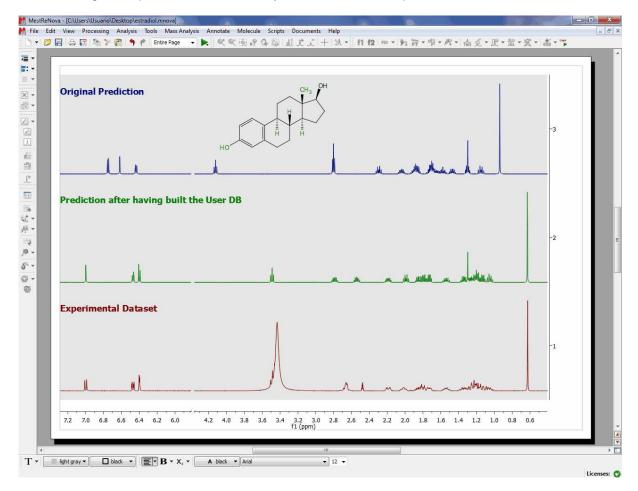

Once you have built your assignments database, load a molecular structure with assignments and select any structure search option under the 'Predict' menu to search for structures and substructures in the DB:



You can also Search for Tags:

SOURCEID	1 120
	13C -
STRUCTUREID	
CHEMISTID	Second 1
SPECTRUMID	Cancel
SOURCEID	
Molecular Formula Lower	
Molecular Formula Upper	-
Molecular Weight Lower	
Molecular Weight Upper	
Source Number Lower	
Source Number Upper	

Selecting 'Prediction DB Info' will show you the number of records for each nucleus in each prediction DB:

DB	Min	Max	Total	Copyright	
N	1	2	2		
0	0	0	0		
Р	1	2	2		
Q	0	0	0		-
R	0	0	0		
s	0	0	0		
т	0	0	0		
U	0	0	0		
v	0	0	0		
w	1	28	27		
х	0	0	0		

Min and Max values correspond to the number of entries in each database, where the deleted entries are also counted.

Follow the menu 'Predict/Browse Prediction DB' or 'View/Panels/Prediction DB Browser' to navigate through the database:

263	Structures Found in 1H d						
	2	.46.			Atom	Shift	-
	HO 3			1	1	4.29	
	1	7		2	2	4.29	
				3	3	3.38	
+				3 4	3	3.38 3.38	
+	Tag	Value	*				
<b>-</b>		Value		4	3	3.38	
	Tag	Value		4	3	3.38 1.41	
3	Tag CHEMISTID	Value		4 5 6	3 4 4	3.38 1.41 1.41	Ē

From this browser, you will be able to navigate through the different compounds in the DB by using the 'blue arrows'. You can paste the assigned molecular structure into Mnova by clicking on this button

You can edit any assignment by double clicking on the cell and typing the new value. Once you have changed the value, click on this icon is to update the changes in the DB. Click on this button to remove any molecule from the DB.

Nucleus: IH DB Letter: All Databases  IH 13C	14				
13C	13C 11B 15N Cancel	Nucleus:	1H	DB Letter:	All Databases 👻
	11B OK Cancel		2H		·
	15N				
110					OK Cancel
	170				
					10.0
19F			29Si 31P		8

Select another DB letter (from 'N' to 'Z') by clicking on this button  $\textcircled{\sc l}$  :

From the Prediction DB Browser you can also run substructures searches, by clicking on the resulting icon for each nuclei:



The location of the prediction database can be selected from the 'Prediction Options' menu, after having clicked on the 'Predictor Properties' button.

	version 4.94
1H	
Shifts Algorithm:	Best
Js Algorithm:	Increments 💌
Prediction Data	base
BETA WMRPred	lict'\VMR 1HDatabase  📖 🦄
Number of GMMX	Cydes: 5
13C and X-Nuclei	Prediction Database
C: \Users \Usuario	o'Desktop (VIMRPredict 🛄 🦄
Databases	
	es:

Please make sure that you have rights to write in the folders above (if not, you will need to change the paths):

1H		
Shifts Algorithm:	Best	•
Js Algorithm:	Increments	•
Prediction Data	base	
BETAWMRPred	lictWMR 1HDatabase	) 🧑
Number of GMMX	Cycles: 5	×
13C and X-Nudei	Prediction Database	
/lestReNova\NMR	Predict\csearchdb2nz	🧖
Databases		
Selected Databas	200	[]


Prediction DBs are stored by default in the following locations (with writable permissions).

- 1H: C:\Users\*Username*\AppData\Roaming\Mestrelab Research S.L.\MestReNova\NMRPredict\NMR1HDatabase

- 13C and X-nuclei: C:\Users\Username\AppData\Roaming\Mestrelab Research S.L.\MestReNova\NMRPredict\csearchdb2nz

However, if you are getting a red path, please try to find the "*13C and X-nuclei folder*" called " **csearchdb2nz**". Then copy the "**csearchdb2nz**" folder to any other location where you have writing privileges (for example to your 'My documents' folder or directly to your 'desktop'). Finally select the path in the 'Prediction Databases Setup' dialog box and try to update the prediction.

If you have loaded a molecule in Mnova (or a SDF containing several molecules) with assignments, you can update the prediction Database by following the menu 'Scripts/NMR Tools/Batch Update Prediction DB':

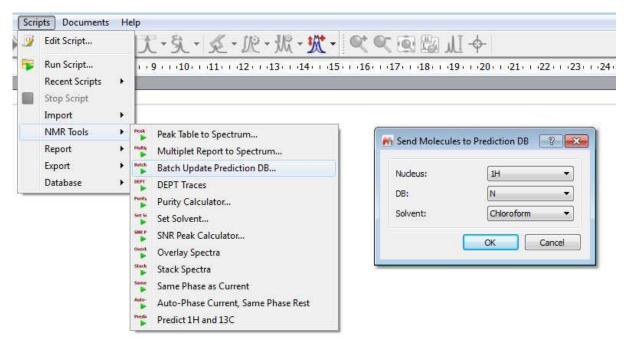

Follow the menu 'Scripts/Database/Batch Update Prediction DB' to export the assignments that you have in your <u>Mnova Database</u> into the <u>Prediction Database</u>:


				n DB	diction	To Predic	nments To	Assign	Export As	Me	(10) THO +M+	SA I I		Help	> +	-	Script
Destination Database Existing: Saving Options Verify Score Rar	Da Ex Sa	- 12					localhost 5504	lo 5	Source Connect Host: Port:		<u>爬 - 侃 - ़∭</u> 2+++13+++14++				•	dit Script un Script ecent Scripts top Script nport MR Tools	
Store Only S			-	•••	•••••		Pablo		User: Passwor					2	+	eport «port	
To: Prediction DB's t V 1H V 13C 15N 170 19F 29Si 31P	F [ [ [ [ [		*	Cor		0	ssword	ase ase: ds	V Save Databas Databas Records From: To:	4) 4)	) o Prediction DB	oort Documents oort Pages oort Files (by locatic oort Files (pairwise) oort SDFile ort Documents ort Assignments to oy Database rch MS in Chromat ille to Definition	Im Im Im Im Exp Exp Co Se SD	in i	•	atabase	
21P												ile to Definition y MNSR File	> 50	SE PL			

This script will be useful for example to import external prediction Databases into a Mnova Database

and from here export the assignments to the Mnova prediction DB (in combination with other scripts as it is described in this <u>chapter</u>)

#### 9.9.2.7 3D Molecule Viewer

You can activate the 3D molecule viewer after having running a prediction which involves more than one conformer. In that case, just highlight the molecular structure and follow the menu 'View/ Panels/3D Molecular Viewer':

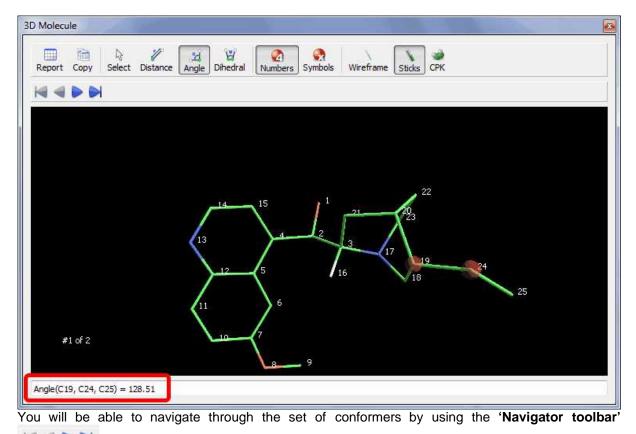

Molecular 3D structures can be managed by:

- Clicking on the right mouse button and dragging (or scrolling up or down the mouse wheel) to zoom in/out the molecule structure.
- Clicking on the left mouse button and dragging to apply a *TrackBall Rotation* (the user is able to control the movement of a ball which contains the molecule).

From this panel, the user will also be able to select the rendering mode (Wireframe, Sticks and Ball Sticks).

The user will be able to measure the bond distance, the angles and the dihedrals by just clicking on

the corresponding buttons of the toolbar and next selecting the desired atoms to analyze. As you can see in the screenshot above, we have measured the angle between the atoms C19-C24-C25.

## 9.9.2.8 Prediction Options and Properties

Following the menu Predict/Prediction Option will display a dialog box from where you will be able to select the chemical shift limits of the spectral window, as well as other parameters, such as number of points, frequency, Line Width, solvent and minimum coupling constant value. If you are going to predict a <sup>1</sup>H-NMR spectrum, you can also exclude the 'Labile Protons' from this window

From:     -2.00 ppm       To:     10.00 ppm       Number of Points:     32 K       Frequency:     500.13 MHz       Line Width:     0.75 Hz       Solvent:     Chloroform-d       Exclude Labile Protons			17 1					
Number of Points:     32 K       Frequency:     500.13 MHz       Line Width:     0.75 Hz       Solvent:     Chloroform-d	i l	-2.00 ppm						
Frequency: 500.13 MHz Line Width: 0.75 Hz Solvent: Chloroform-d		10.00 ppm						
Line Width: 0.75 Hz Solvent: Chloroform-d	oints:	32 K 👻						
Solvent: Chloroform-d		500.13 MHz						
		0.75 Hz						
Exclude Labile Protons	(	Chloroform-d 💌						
	Labile Protons							
Predictor: Modgraph NMRPredict Desktop	[	Modgraph NMRPredict Desktop 💌						
Predictor Properties	[	Predictor Properties						

Clicking on the 'Predictor Properties' button will display a dialog box to allow you to select the location of the prediction <u>Databases</u> and also the algorithms to use (Best, Increments or Conformers) for the shifts and Js in the 1H prediction:

	10	rsion 4.9
1H		
Shifts Algorithm:	Best	•
Js Algorithm:	Increments	•
Prediction Data	base	
BETA WMRPred	lict WMR 1HDatabase	)
Number of GMMX	Cycles: 5	\$
13C and X-Nuclei	Prediction Database	
C: \Users \Usuario	DVDesktop WMRPredict	. 🤊
Databases		
Selected Databas	ies:	

The 2D mol file representation of the structure is converted by <u>GMMX</u> into a 3D structure and then this structrure is repeatedly minimised to produce a series of conformers. The parameter "Number of

GMMX Cycles" affect the number of conformers produced by GMMX. There is, however, no simple relationship between this value and the actual number of conformers.

Clicking on the 'Selected Database' will allow you to select the 'Prediction Databases' that you want to use for your predictions:


ludeus: 1H	•
<b>V</b>	
Select All	-
Only System Dbs	
Only User Dbs	E
V E	
🕼 F	
☑ G	
▼ H	
V J	
K K	
V L	

## **Properties**

Double clicking on the predicted spectrum will display the 'Properties' dialog box:

Ietadata Geometry NMR Spectrum	Prediction	
Grid Grid	<u>C</u> olor:	Sienna 👻
1D	MS Shell Dlg 2	Font
4 🧏 Scales	Show J Tree	
Horizontal	Show Errors	
Vertical		
Peaks		
🍌 Integrals		
Multiplets		
M Integrals		
Fitting		
Assignments		
Prediction		

Selecting 'Prediction' from the left tabbed menu will allow you to change the color and font of the prediction labels and also to display graphically the J Tree and the prediction errors:

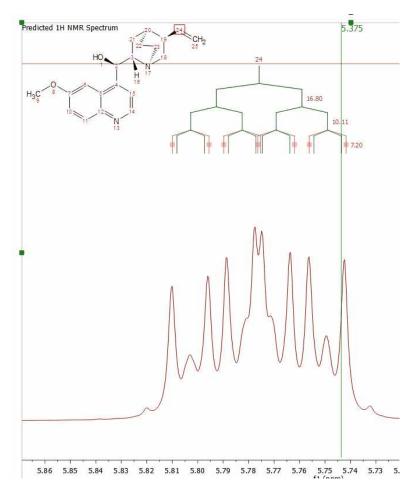

## 9.9.3 NMRPredict Server-Based

**NMR Prediction:** The handling of molecular structures within Mnova also allows the user to carry out **spectral predictions**. Although the process described here could be applied to predictions by means of any commercially available or in-house prediction package, currently Mnova will carry out predictions by using the prediction application **NMRPredict**, by Modgraph Consultants Ltd. Please note that this is a separate plugin which must be licensed in addition to Mnova.



## A few notes on NMR Prediction Server-based

- ✓ As opposed to NMRPredict Desktop, NMRPredict server-based is a client-server application, so to carry out the predictions you will have to log in to the server via a dialog box shown by Mnova. Log in details will be provided to you when downloading NMRPredict. This login will only have to be carried out the first time you run a prediction with Mnova. After that, the software should remember your login details and do the log in in the background.
- ✓ Because it is a client-server application and the data are being sent over the internet to the server, industrial testers may wish to have an inhouse installation of NMRPredict for security reasons. If this is the case, just write to us with your request at <u>nmrpredict@mestrelab.com</u>.
- Customers who have their own in-house prediction package are welcome to contact us to discuss a similar, seamless integration of their own prediction package. Please write to us at <u>support@mestrelab.com</u>.
- ✓ Please note that NMRPredict is a different software package to Mnova and therefore, in order to carry out predictions via this package, a license of NMRPredict must be held separately, once the NMRPredict evaluation has expired.

Carrying out of predictions in Mnova is very simple. With a molecular structure open in the active page of Mnova, just go to the 'Predict' menu and select Prediction Options; then a dialog box will open.

н	13C	HSQC	31P	19F	15N	11B	17			
Fro	m:		-2	-2.00 ppm						
To:			10	10.00 ppm						
Nur	mber of P	oints:	32	<b>32 K</b>						
Frequency:				500.13 MHz						
Line Width:				0.75 Hz						
Solvent:				Chloroform-d >						
	Exclude	Labile Prote	ons							
Predictor:			Mo	Modgraph NMRPredict Server 💌						
				Predi	ctor Prop	erties				
	: Use 3I	D Molecu	le pane	to see	all predi	cted				

This open dialog allows the user to set a series of prediction parameters before carrying out the prediction: limits, number of points, frequency of the spectrometer, line width, solvent and the Predictor methodology. To carry out a server-based NMR prediction the user has to select 'Modgraph NMRPredict Server' in the 'Predictor' edit box.

Clicking on the 'Predictor Properties' (red square in the capture above), the user will be able to select

the algorithm for the <sup>1</sup>H-NMR prediction (Increment or Charge):

Connect	on	
Server:	localhost	
Port:	9300	
Algorithr	n	
Increme	ents	
Increme CHARG	ents E (Conformers)	

The Increment algorithm (based in Ernö Pretsch's NMR tables) is the same as NMRPredict Desktop uses to predict NMR spectra

The CHARGE program offers <sup>1</sup>H-NMR prediction based upon partial atomic charges and steric interactions. This program offers the **first** quantitative prediction of the proton chemical shifts of a variety of organic compounds.

The program works by first generating 3D conformers from a 2D structure through a choice of *force fields* and then predicting proton spectra for all the conformers. The program works by looking at functional groups which have parametrised by Professor Abraham.


To read more about the CHARGE theory, please visit the following link:

http://www.modgraph.co.uk/product\_nmr\_proton.htm




**NMRPredict** is a **client-server** application, so to carry out the predictions you will have to log in to the server via a dialog box shown by Mnova. Log in details will be provided to you when downloading **NMRPredict**. This login will only have to be carried out the first time you run a prediction with Mnova. After that, the software should remember your login details and do the log in in the background.

Finally, just go to the 'Predict' menu and select the desired prediction.

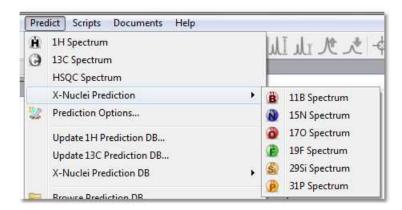

This will send a request to the server, which will run a prediction and return a set of values which Mnova will display as a spectrum on the screen. You will immediately notice that this will be an assigned spectrum, and therefore hovering of the mouse over the atoms will highlight the applicable peak on the spectrum and viceversa.

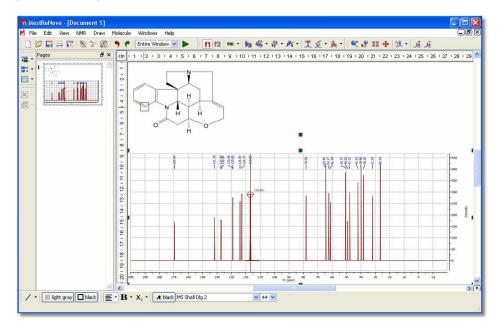


## A few notes on the synthetization of NMR 1H spectra

✓ It is important to note that the simulation carried out by Mnova when displaying the predicted values as a spectrum is not first order. The software is carrying out the full quantum-mechanics calculations to arrive at the displayed spectrum. This is very computationally intensive and results in such simulation module having a limitation, for 1H spectra, which prevents it from simulating spin systems larger than 13 spins. However, we have developed a new algorithm to overcome this problem.

The prediction of the 13C-NMR is based on the HOSE code approach. The **HOSE** (Hierarchical **O** rganisation of **S**pherical Environments) code approach starts at the carbon atom whose shift is to be

predicted, looks one bond away from the carbon and tries to find this same environment in its database. If it is successful it moves two bonds away and tries again and so on until it either comes across something not represented in the database or it reaches the boundary of the molecule.

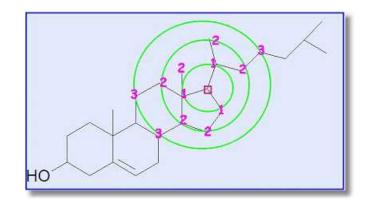

The HOSE code approach works very well for query structures which are well represented in the reference collection. If atoms can be predicted to three spheres or more (NMRPredict goes to a maximum of five spheres) the prediction can be considered to be very reliable.

However, if the query structure is not well represented in the database and the atom can only be predicted to one or two spheres the prediction cannot be relied upon at all. Also the HOSE code approach exactly reproduces the contents of the reference database – including every error within the reference database.

If atoms can only be predicted to one or two spheres the only solution traditionally was to add your own similar data and use that for prediction. NMRPredict also uses a unique Neural Network algorithm, which is much more general and error tolerant than the HOSE code approach and is much more accurate at predicting atoms it has not seen in its database.

## 9.10 Tables

**Mnova** groups all spectra relevant information into the so-called **Tables window**, available from the *View* menu or by right clicking on any toolbar.

	Tables					6
ASV Results		t 🔉				
	Range	<ul> <li>Normalized</li> </ul>	Absolute			
Elemental Composition	1 7.85 7	7.72 1.00	43685.19			
Molecule Match	2 6.736	5.56 1.03	45026.66			
Mass Peaks	3 5.91 5	5.84 1.02	44492.10			
1033 1 COKS	4 4.30 4	1.24 1.03	44850.78			
Compounds	5 4.17 4	1.04	45349.12			
	6 4.08.,4	1.05	45707.23			
Arrayed Data	7 3.92 3	3.87 3.11	135900.60			
ssignments	8 3.87 3	8.83 4.12	180070.53			
	9 3.83 3	3.78 1.22	53170.47			
ntegrals	10 3.72 3	3.64 1.13	49431.41			
Aultiplets	11 3.20 3	3.01 3.22	140585.40			
arameters	12 2.88 2	2.77 1.07	46792.28			
	13 2.74 2	2.67 1.05	45756.58			
leaks	14 2.67 2	2.60 1.10	48210.60			
tacked Spectra	15 2.38 2	2.29 1.06	46387.96			
llind Regions	16 2.01 ., 1	.92 0.90	39331.89			
	17 1.92 1	.77 2.26	98611.68			
3C Prediction	18 1.49 1	.41 1.06	46151.39			
H Prediction	19 1.291	.19 1.25	54462.08			
(-Nuclei Prediction	Parameters	Peaks Inte	egrais Multiplet	s Assignments	1H Prediction	13C Prediction

From this set of tabbed pages, the user can find information, about:

- Elemental Composition (Mass plugin)
- Molecule Match (Mass Plugin)
- Mass Peaks (Mass plugin)
- Compounds
- GSD Peaks
- Arrayed Data (DOSY, T1/T2, etc... processing)
- Assignments
- Integrals
- Multiplets
- Parameters
- Peaks
- <sup>1</sup>H Prediction (Prediction plugin)
- <sup>13</sup>C Prediction (Prediction plugin)
- X-Nuclei Prediction (Prediction plugin)

Spectral Parameters: This table shows information about:

- Experiment Title
- Data File Name
- Origin of the Experiment (type of spectrometer used)
- The Owner
- Solvent Used (CDCl<sub>3</sub> in the example below)
- The Frequency of the Spectrometer Used to Carry Out the Experiment
- Number of Acquired Data Points
- Spectral Width
- Spectrum Size After FT
- Lowest Frequency (in Hz) Used for Referencing Purposes, etc.

# Please note that Mnova includes the ability to add more parameters into this list and customize the way it is displayed on the screen. See also: <u>Parameters Table</u>

The user can directly paste the spectral parameters table on the spectrum by clicking on the **'Report'** icon (red square in the capture below). You can also export the table to another document by clicking on the **'Copy to Clipboard'** icon in the screenshot below).

Re	port Copy Col. Setus	Row Setup				
	Parameter	Value (f2; f1)				
1	Origin	UXNMR, Bruker Analytische Messtechnik GmbH				
2	Owner	root				
3	Solvent	020				
4	Temperature 300.00					
5	Pulse Sequence	mm_invigsmitp				
6	Number of Scans	16				
7	Acquisition Date	Wed 24. Jul 22:19:15 2002				
8	Spectrometer Frequency	(500.13; 125.77)				
9	Acquired Size	(1024; 256)				
10	Spectral Width	(2500.00; 6289.31)				
11	Data File Name	H:/Documents and Settings/Usuario/Mis documentos/Manuales/HMQCT_TOCSY/80/set				
12	Spectral Size	(512; 512)				
13	Lowest Frequency	(529.73; 6796.97)				
14	Nucleus	(1H; 13C)				


The user will be able to modify some of the parameters (Spectrometer frequency, Spectral Width, Lowest Frequency, Nucleus...) by just double clicking on the value as is shown in the picture below:

Re	eport Copy Col. Setup	) Row Setup				
	Parameter	Value (f2, f1)				
1	Data File Name	H:/Documents and Settings/Usuario/Escritorio/js1pmftalato/js1				
2	Title	js1pmftalato				
3	Origin	inova				
4	Owner					
5	Solvent	CDCl3				
6	Temperature	25.00				
7	Pulse Sequence	gHSQC				
8	Number of Scans	16				
9	Acquisition Date	20071020T003052				
10	Spectrometer Frequency	(399.97, 100.57)				
11	Spectral Width	(3668.04, 25000.00)				
12	Lowest Frequency	(-233.13, -1917.94)				
13	Nucleus	f1: 1H 👿 f2: 13C 👿				
14	Spectral Size					
15	Acquired Size	19F 19F 19F 14N 2H 35Cl 10B ▼				

You can customize the table, by clicking on the **'Column or Row Setup'** icon **S**. The 'Customize Table' dialog box will be displayed and will allow you to change the name of the columns, hide them, change the number of decimals as well as the horizontal alignment.

	Parameter	f1
Visible Name	Parameter	f2
Visible		
Decimals	0	2
Horizontal Alignment	Left	Left

Once any table has been reported, you can change its properties (position, size, fill and border) just by double clicking on it:

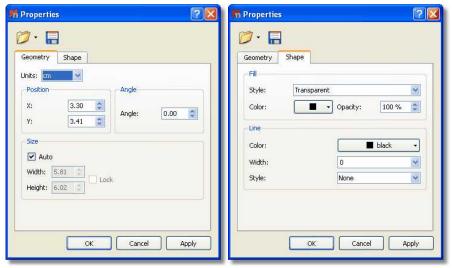

See also: Parameters Table

**<u>Peak Table</u>**: By default, peak frequencies are listed directly on the spectrum but they can also be accessed via the *Peak Picking table* by following the menu 'View/Tables/Peaks'.

Rep	ort Peaks	Copy Pea		Report 🔹	)應 Delete Se	lect Peaks		
Syn	c From Spec	Filter Sy	ync To Spec	ال Set Flags	اللہ Set Compou	ind New Spe		
	ppm	Hz	Intensity	Width	Area	Туре	Flags	*
1	8.85	3539.1	29.2	1.32	294.19	Compound	Weak + C13_Sat	-
2	8.84	3534.6	29.3	1.22	270.32	Compound	Weak + C13_Sat	
3	8.78	3512.9	21.9	0.92	153.96	Impurity	Weak	
4	8.77	3508.4	23.6	0.85	162.98	Impurity	Weak	
5	8.64	3456.9	40.6	1.42	500.00	Compound	Weak	
6	8.64	3455.5	28.4	0.19	48,33	Compound	Weak	
7	8.64	3454.5	37.3	3.14	955.56	Compound	Weak	
8	8.63	3451.0	6203.9	1.00	46415.96	Compound	None	
9	8.62	3446.6	6622.7	0.82	44958.30	Compound	None	
10	8.60	3440.5	27.3	0.91	147.13	Compound	Weak	
11	8.52	3406.5	7.0	0.86	46.67	Impurity	Weak	
12	8.40	3361.2	26.8	1.32	252.49	Compound	Weak + C13_Sat	

This table displays the list of peaks, including the following information: chemical shift in ppm and Hz, intensity (height), width (width, in Hz, at half maximum of the peak), type (the user can select between 'Compound', Artifact', Impurity' or 'Solvent') and 'Annotations'.

The user can report the Peak table directly on the spectrum by clicking on the **'Report Table'** icon (under the Report Text scroll down menu) You can customize the appearance of this report (an also of

the table), by clicking on the 'Setup Table' button (under the Setup Text scroll down menu) to display the 'Customize Table-Peaks' dialog box:


	ppm	Hz	Intensity	Width	Туре	Max/Min
Visible Name	ppm	Hz	Intensity	Width	Туре	Max/Min
Visible	~	~	~	~		
Decimals	2	1	1	2	0	0
Horizontal Alignment	Left	Left	Left	Left	Left	Left
<						)
Font M5 She Report	ell Dig 2					
Frame	Borders	F	Numbering	Title		Bold Headers

This dialog box will allow the user to change the name of the columns, hide them, change the number of decimals as well as the horizontal alignment. You can change the Font Family and also to customize the appearance of the table report (Frame, Borders, Numbering, Title and Bold Headers).

The user will also be able to select the multiplicity of the carbon signals, just by double clicking in the applicable cell, as you can see in the picture below:

	ppm 🎽	Hz	Intensity	Width	Multiplicity
1	164.59	20700.3	14829.9	3.63	c
2	164.51	20691.3	15192.3	3.46	с
3	150.55	18935.1	17656.2	3.74	с
4	150.44	18920.5	58586.9	3.49	сн
5	138.03	17360.2	58763.0	3.36	СН
6	128.32	16138.7	18100.4	3.51	с
7	124.40	15646.3	60696.7	3.41	СН
8	52.91	6654.4	55386.2	3.30	СНЗ
9	52.48	6600.8	55978.5	3.29	снз 📘
		10	Unknown		
	Para	Inte	Multi	Assi	Сн

To delete an undesired peak, click on the **'Delete'** icon **\*** of the Peak List, or select 'Delete Manually' on the Peak Picking scroll bar icon

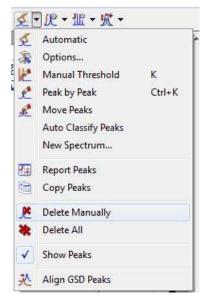

By default, peak frequencies are listed directly on the spectrum but they can also be accessed via the

*Peak Picking table* and also as a **'Peak List'** by clicking on the **'Report Text'** icon Report Text'. The user will be able to select the 'Peak Report Template' between several journal formats by selecting 'Setup Text' in the 'Report Special' scroll down menu.

JACS		•
Ascending order s		
Only report compound in the second compound in the second composite of the second component is a second compound in the second compound in the second component is a second component in the second component in the second component is a second component in the second component in the second component is a second component in the second component in the second component in the second component is a second component in the se	en la construction de la	
Number of decimals:	2	\$
2D		
Report as point:	S	
👿 Report f1		
🔽 Report f2		

From here you can select the order of the report or only report the compounds peaks.

From the Peaks table, you can apply some filter (by clicking on the applicable button) to show for example only Compounds Peaks:

	-			11 (65)			1.	
Sync	From Spe	Filter S	Sync To Spec	Set Flags	Set Compou	und New	<u>M</u> Spectrum	
2010	ppm	Intensit	y Width	Area	Туре	Flags	Impurity/Compound	t.
339	M Pea	aks Filter	-	8 5	X Irity	Weak		
340	Filte	r			urity	Weak		
341	Ind	uding:	All	•	] wity	Weak		
342	Exc	luding:	None	•	]   irity	Weak		
343		Peaks Assig	gned To:	_	arity	Weak		
344		None EtOAc			irity	Weak		
345		✓ Quinine	ŝ		urity	Weak		
346					rity	Weak		
347			ОК	Cancel	pound	Weak + C13_Sat		
348	1.17	131.4	1.19	2013/03	Compound	None	EtOAc	
349	1.17	80.5	1.25	1191.49	Compound	None	EtOAc	
350	1.16	268.5	1.15	4274.61	Compound	None	EtOAc	C
				2448.77	Compound		EtOAc	

You can synchronize the type of the peaks in the table (i.e. only Compounds peaks) with the peaks showed in the spectrum (by using the button 'Sync from Item') or viceversa, synchronize the spectrum peaks with the peaks showed in the table ('Sync to Item' button).

**Integral List:** The Integrals Table includes information about the integral range (in ppm) and the normalized and absolute values of each integral. In this table the user can normalize the integrals by double clicking on the normalized value of the integral which the user would like to set (in the red

square on the capture below). Once it is highlighted, the user has to overwrite the desired value, press return, and all integrals will update with reference to the chosen one. You will obtain the same effect by double clicking directly on the integral label on the spectrum.

The user can also delete an integral from this table by clicking on the **'Delete'** icon **\*** when the undesired integral is highlighted. To paste the integral list on the spectrum, just click on the **'Report'** icon .

R	eport Copy	X Delete Set	up
U	Range	Normalized	Absolute
1	9.21 9.11	1	26356.88
2	8.37 8.26	0.93	28021.56
3	8.13 <mark>8</mark> .03	0.98	29299.02
4	3.95 3.89	2.98	89550.74
5	3.89 3.82	3.23	97200.39


**Multiplets:** The multiplet table includes information about the name (by default Mnova named the multiplets following the alphabetical order, but the user is able to change it in the multiplet manager), the chemical shift (ppm), the range (ppm), number of hydrogens, integral value, type of multiplet and coupling constant values (Hz).

Re	eport Multip	lets 📩	Copy Multiplets	s * Se	etup Report	- X Delete			
1H 5.4 2H	I), 7.30 (dd 18 (d, $J = 4$	, J = 9.3 .3 Hz, 11 .99 (m, 2	, 2.7 Hz, 1H), 7 H), 4.99 – 4.84 H), 2.63 (dddt	7.21 (d, (m, 2H	J = 2.7 Hz, ), 3.87 (s, 31	1H), 5.73 (dd H), 3.38 (ddd	$\frac{\mathrm{dd}}{\mathrm{dd}}, J = 1$ $\mathrm{dd}, J = 1$	1H), 7.46 (d, <i>J</i> = 4.5 ) 7.5, 10.3, 7.6 Hz, 1H 3.4, 10.5, 5.6, 2.5 Hz, .18 (m, 1H), 1.83 – 1	),
	Name	Shift	Range	H's	Integral	Absolute	Class	J's	
1	C (d)	7.46	7.517.43	1	0.86	92585.19	d	4.51	
2	A (d)	8.62	8.67 8.58	1	0.80	86101.39	d	4.39	11
3	N (m)	1.71	1.83 1.62	3	3.29	352791.56	m		
4	M (m)	2.24	2.30 2.18	1	0.96	103210.06	m		
5	L (dddt)	2.63	2.69 2.55	2	1.97	211502.68	dddt	2.01, 2.01, 4.29, 6.03, 10.73	
6	K (m)	3.09	3.172.99	2	2.31	247987.14	m		
	J (dddd)	<mark>3.3</mark> 8	3.46 3.31	2	1.90	203318.84	dddd	2.54, 5.56, 10.50, 13.36	
7									

See also <u>'Multiplets Table.</u>

**<u>1H Prediction</u>**: In this table, the user can visualize the <sup>1</sup>H assignments of the predicted shifts (in NMR Predict mode). As you can see in the picture below, the carbon atoms are labeled to make easy the proton assignment. The user can also select the frequency of the desired predicted spectrum (on the frequency edit box) as well as do (or not) groups magnetically equivalents (by clicking on the

suitable icons: (and also expand or collapse the predicted values by clicking on the applicable buttons

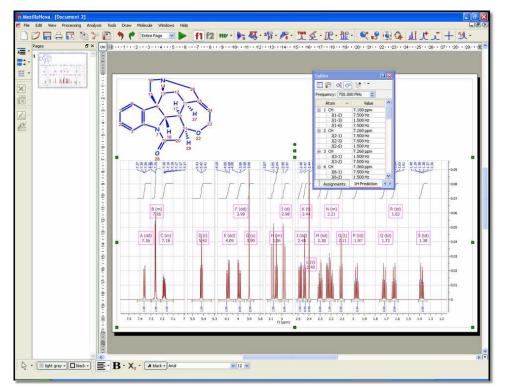

You can also modify the chemical shift and coupling constant values directly from this tables, just by double clicking on the applicable box and entering the desired value.

re	quency: 300.00	10 MHz 😂	
	Atom 🔺	Value	^
۵	1a CH2	3.960 ppm	
1	J(1a-1b)	-12.400 Hz	
100	J(1a-6)	7 Hz	
ė	1b CH2	3.710 ppm	
	J(1b-1a)	-12.4 Hz	
	J(1b-6)	7 Hz	
(a)	3 CH	4.500 ppm 🔄	
-	J(3-4)	7.000 Hz	
1	J(3-21)	7.000 Hz	
É	4 CH	4.65 ppm	
1	J(4-3)	7.000 Hz	
	J(4-5)	7.000 Hz	
😑 5 CH		5.250 ppm	
J(5-4)		7.000 Hz	
	J(5-6)	7.000 Hz	
ė	6 CH	4.660 ppm	v
	Assignments	1H Prediction	( ) ( )


Please bear in mind that you can also put the table on the 'Page Navigator' just by clicking on the table and dragging it to the 'Page Navigator', as you can see in the picture below:

Rej	oort Text	Copy Text	🔹 🔛	ext 🕶 De	<b>X</b> elete		
121	.49, 118.39					141.93, 131.59, 12 , 57.07, 55.66, 43.1	
	ppm	Hz	Intensity	Width	Туре	Annotation	
5	141.93	14275.41	194.0	3.77	Compound		
6	131.59	13235.55	177.8	4.39	Compound		
7	126.65	12738.65	93.0	4.31	Compound		
8	121.49	12219.60	174.0	4.60	Compound		
9	118.39	11907.57	187.3	4.26	Compound		
10	114.30	11496. <mark>1</mark> 9	195.2	4.62	Compound		
11	101.31	10189 <mark>.</mark> 51	186.2	4.71	Compound		1
12	77.32	7776.84	4410.5	5.05	Solvent		
13	77.00	7744.89	4496.6	5.04	Solvent	CDCl3	
14	76.68	7712.95	4450.2	5.09	Solvent		
	72.27	7269.40	198.9	4.58	Compound		

<sup>13</sup>C Prediction: In this table, the user can visualize the <sup>13</sup>C assignments of the predicted shifts (in NMR Predict mode). You can also select the frequency of the desired predicted spectrum (on the frequency edit box). The user can paste the <sup>13</sup>C Prediction table directly on the spectrum by clicking on the **'Report'** icon is or copy it to the clipboard by clicking on the applicable icon is. You can also customize this table by clicking on is.


Frequency: 205.00	io MHz 🛫		
Atom 🔺	Value	^	
-1 C	144.91 ppm		
-2 C	147.95 ppm 101.52 ppm 142.32 ppm 124.140 ppm 110.00 ppm 170.12 ppm 38.16 ppm 78.08 ppm 64.08 ppm 126.59 ppm		
- 3 CH			
-4 C			
5 C			
-6 CH			
-8 C			
- 9 CH2			
- 10 CH			
-12 CH2			
-13 CH			
-14 C	138.68 ppm		
- 15 CH2	54.58 ppm		
- 16 CH	31.36 ppm 49.89 ppm		
- 17 CH			
- 19 CH2	27.40 ppm	v	
1H Prediction	13C Prediction	•	


**Compounds:** This table will show all the molecules present in the document, with information about the chemical formula and molecular weight, name.

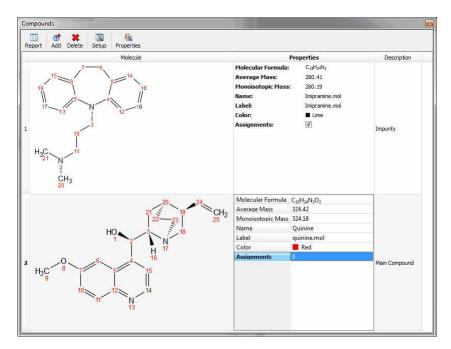

You can copy any molecule from this table to another page just by selecting it and clicking on the 'Report' button. Please bear in mind that the information about predictions and assignments is linked to the molecule and will be kept after having pasted it to another slide.

You will be able to dock any table to the right or left side of the spectrum just by clicking on it and dragging to the desired place:

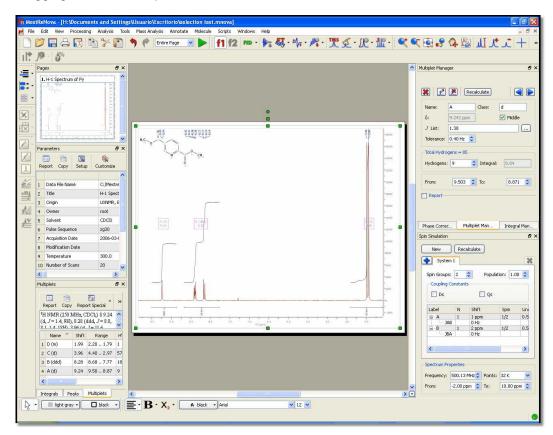

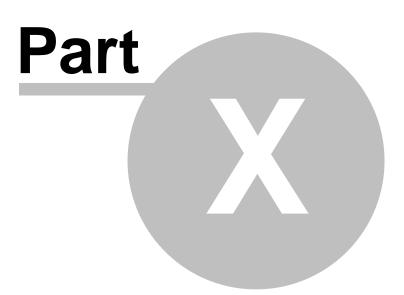

# 10 Advanced Menu

You will find under this menu some advanced tools for the more expert users, such as GSD, Line Fitting, Data Analysis, DOSY transform, Arithmetics, Verification, qNMR etc...

## **10.1** Line Fitting (Deconvolution)

When the spectrum is crowded with peaks, or affected by excessive noise, deconvolution may be the only way to measure the compounds ratio; but please bear in mid that this feature does not make miracles and it can not be a substitute for higher magnetic fields, more concentrated samples or longer acquisitions.


The name "deconvolution" means (more or less): "removing the shape". The theoretical shape of an NMR peak is given by the Lorentzian equation. Field inhomogeneity and weighting functions can however yield partial Gaussian line-shapes. From a merely graphical (and practical) point of view, they are two complementary shapes, in the sense that most symmetrical peaks can be approximated with suitable combinations of Lorentzian and Gaussian components. For your convenience, Mnova defines a mixed function, for which you can vary at will the percentages of Lorentzian and Gaussian character.

MestReNova includes a fully interactive interface for the deconvolution of experimental spectra into individual lines.


This module includes options for locking any of the parameters during optimization and the ability to compare the resulting calculated spectrum, as a sum of the individual components, with the experimental spectrum.

It is really easy to run the Line Fitting feature. Just click on the 'New Fit Region' icon 2000 (or follow the menu 'Advanced/Line Fitting/New Fit Region') and next click and drag over the desired region of the spectrum. (Please make sure that you have corrected the baseline of the experiment).

NOTE: It you prefer, you could apply a previous peak picking before selecting the Line Fitting region. To have a better control over the peak picking, you could use the 'Peak by Peak' mode or the 'Manual Threshold'.

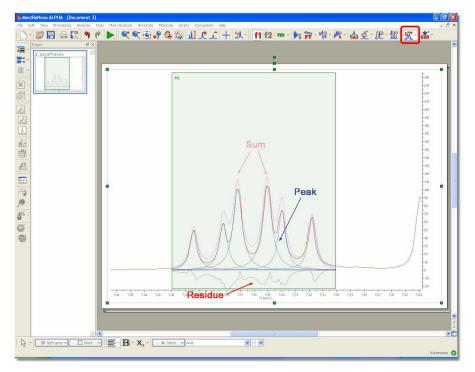

You can see in the picture above a blue line which corresponds with the fit peak, a red line which corresponds which the fitting residue and a magenta line which corresponds with the sum.

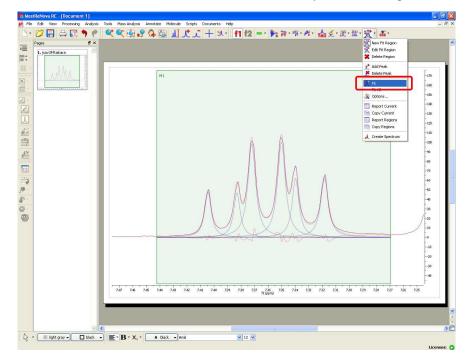


Next, select Fit under the scroll down menu to carry out the Fitting:

You will notice that the residue, the fit peak and the sum lines have changed. They constitute a starting point for the fitting (unless you are happy with the first fitting). If you are not happy with the initial fitting; you can add/remove components and change their parameters, just by selecting 'Edit Fit Region' in the 'Line Fitting' scroll down menu. This will display the 'Line Fitting' panel, where you will find information about the peaks of interest (the chemical shift, in ppm; the Height, the Width, in Hz; the Lorentzian /Gaussian ratio and the Area).


la	me: M1					
rc	m: 7.269	ppm 📚		To:	7.442 ppm	5.2
£	· <u>*</u> ·				👯 Fit 🔹 [	, H
	ppm	Height	Width (Hz)	L/G	Area	
1	7.4044	48.18	1.46	🔒 1.00	798.960	
2	7.3829	47.00	1.44	â 1.00	774.239	
3	7.3719	98.85	1.70	â 1.00	1927.260	
4	7.3504	100.35	1.75	🔒 1.00	2008.002	
5	7.3399	62.13	1.51	🔒 1.00	1075.534	
6	7.3184	61.84	1.71	🔒 1.00	1207.914	

These parameters can be changed interactively over the spectrum (just by clicking and dragging over the green little squares) or by double clicking on each cell of the Line Fitting panel. Changes on any parameter will obviously affect to the 'Residual Error' (the smaller error, the better). For each point of the region, Mnova calculates the difference between the experimental and theoretical points, this value

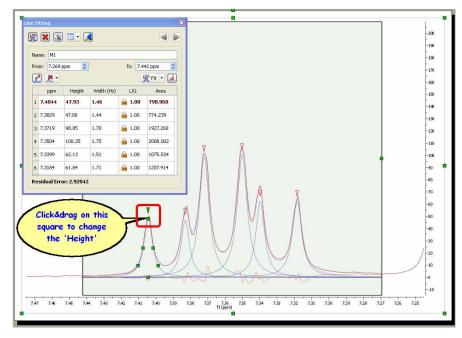


is powered by two and Mnova calculates the average of all the errors in the region of interest.

Clicking and dragging the green square at the top of the peak, will change the Height of the peak. The squares at the mid-height of the peak can be used to modify the Width of the peak:

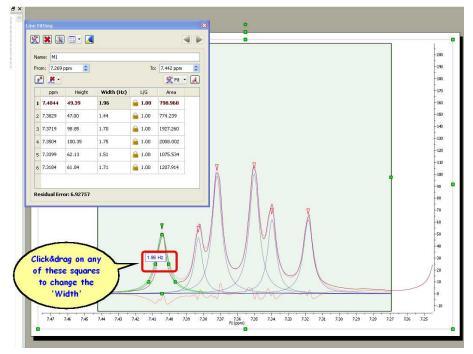


Clicking and dragging on the next two squares will modify the Lorentzian/Gaussian ratio of the signal and finally the last square will be used to modify the chemical shift of the signal.

Clicking on the red triangles will set the active peak:

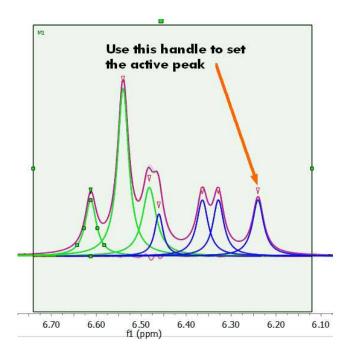


Any of these parameters can be locked for the Fit, just by double clicking on the applicable cell of the panel and closing the lock which appears. In the picture below it is shown how we have locked the width parameter of the peak 1 and also the L/G ratio of all the peaks, so these parameters will not change when the fitting will be applied. So a lock in front of a value indicates that it will not be optimized in the fitting.

**L/G ratio:** it does not pretend to be a mathematic representation. It is like a ratio between L and G. The value of the function to be fit would be:  $LG(x) = LGFactor^*L(x) + (1-LGFactor)^*G(x)$ 

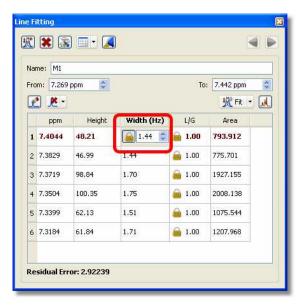


Of course you can fit several regions within a single spectrum, just by selecting a 'New Fit Region':

© 2017 MESTRELAB RESEARCH

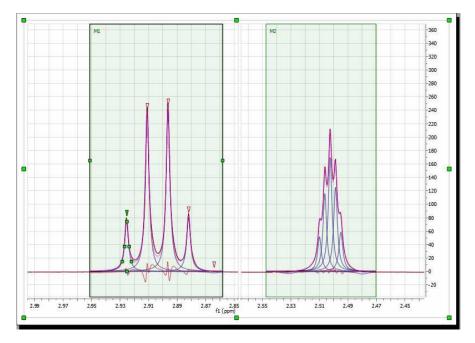

Once you are happy with all the parameters, you will only need to apply a new Fit, just by clicking on this icon this icon this icon the fit v. If you have several regions, you will need to select 'Fit All' in the Fir scroll down menu. Once the fitting has been made, if you want to get the Fitted spectrum just click on the 'Create spectrum' icon

You can also use the Line Fitting feature for the simultaneous fitting across arrayed spectra. Just select the region and the fitting will will take place along all the arrayed spectra:

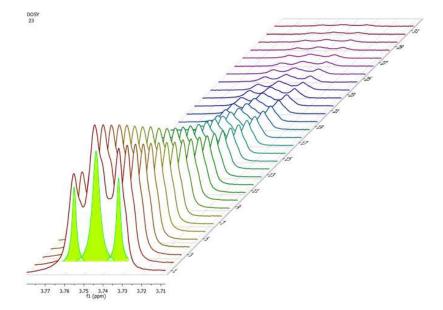

You can apply line fitting options and parameters for all stacked spectra.

Name: M1	E.C.			and a second second	
From: 0.779 ppn				To: 2.240 pp	
Shift(p	Lock all shifts	Width(Hz)	L/G	Area	
1 1.6699	Lock all heights Unlock all widths	i 34.5	Ø.21	69.857	
2 1.2015	Unlock all L/G	≥ 84.7	≥ 1.00	52.667	

Follow the menu 'Scripts/Export ASCII/Fit Regions' to export the results in a .txt file.

<u>Other Options of the Line Fitting panel</u> The Line Fitting panel includes other tools, let's see the meaning of them:

New Fit region: use this icon to create another region to be fit.

**Delete region: \*** to delete the current region.

**Fitting Options:** Is to display the Fitting Options window where the user will be able to establish some constraints for the fitting. Line Widths and Chemical Shift parameters can be constrained within user-defined values:

Width Cons	traint			
Lower:	0. 10 Hz	Upper:	100.00	Hz
Position Cor	nstraint			
Within ±:		5.00 %		
Shape Type				
Generalize	d Lorentzian			•
				•
Generalize				•
Generalizer Default Lock None Advanced				
Generalizer Default Lock None Advanced	3		0	-
Generalizer Default Lock None Advanced Use Sim Maximum N	ulated Annealing	Iterations: 50		49

If the spectrum contains broad signals, just increase the Width Constraint to get good results. In the example below the Upper width constraint has been increased to 100 Hz:

Name: M1 From: 7.175 (				To: 8.547 ppm	Lower: 0.10 Hz	Upper: 100.00 F	tz 💿	-75 -70 -65
ppm	Height	: Width (Hz	z) L/G	Area	Within ±:	13.00 %	-	-60
1 7.9330	38.91	1.8		445.048				-55
2 7.8630	9.69	33.4	🔒 1.00	2075.983	Shape Type			-
100 Contraction of					Generalized Lorentzian		-	-50
Residual Erro	or: 0.17047	1						100
					Default Locks			-45
•					e None		-	-45 -40 -35
•					None Advanced	Inn	-	-40
•					e None			-40 -35 -30
					None Advanced Use Simulated Anneal	rse Iterations: 500		-40 -35
					None Advanced Dise Simulated Anneal Maximum Number of Coar	rse Iterations: 500		-40 -35 -30
					None Advanced I Wes Smulated Arneal Measure Number of Fire Local Minima Filter:	Iterations: 500 5		-40 -35 -30 -25
•					None     Advanced     Use Smulated Anneal     Meanimm Number of Fire	Iterations: 500 500 5	* *	-40 -35 -30 -25 -20
					None Advanced I Wes Smulated Arneal Measure Number of Fire Local Minima Filter:	Iterations: 500 500 5	* *	-40 -35 -30 -25 -20 -15
					None Advanced I Wes Smulated Arneal Measure Number of Fire Local Minima Filter:	se Iterations: 500 Iterations: 100 5 OK	* *	-40 -35 -25 -20 -15 -10 -5

**Position Constraint:** it takes into account the values outside the range (p=shift) p\*(1-pos\_constraint\*p). A big value of the algorithm will 'shift' the peak far. Normally, you will not need to change the default value, because the peak should be close to the original position.

Shape Type: you can select between 'Generalized Lorentzian' or 'Lorentzian-Gaussian'.

'Generalized Lorentzian': The new generalized NMR peak shape profile proposed (which is a lorentzian plus a factor by another function), generalizes the ubiquitous Lorentzian shape. The mathematical expression (to be published) for the profile function contains only one extra parameter in addition to the three parameters of the Lorentzian line (location, height, and width). The new parameter does not interfere with any of the three 'classical' parameters (orthogonality) but affects the peak's kurtosis (for this reason we call it the kurtosis parameter). It is a-dimensional and has a 'natural' physical range of -1.0 to 2.0 (beyond these limits the formula is still operative but the peak profile starts splitting into a doublet or triplet). There are strong physical and conceptual reasons to expect that the new family of shape profiles will be much more useful in NMR spectroscopy than any of the often-used mixtures of Lorentzian and Gaussian shapes. In particular, we expect it to improve the quality of quantitative assays through NMR spectra and help the process of automatic editing of NMR peaks prior to structure verification.

NOTE: When a GSD peak picking is done the assumed peak shape is the Generalized Lorentzian.

Default Locks: you can select from here what parameters you want to lock by default.

**Use Simulated Annealing:** coarse fitting algorithm which will look for random solutions, keeping the best one as starting point for the *Fine Line Fitting* in order to get a better solution. The user will need to select the Maximum Number or coarse iterations (to find the initial starting point). This algorithm will be faster but less precise than the Fine Line Fitting.

**Local Minima Filter:** the algorithm uses a variation method to find the solution. With the initial parameters, it calculates the difference between the result and the real curve; after that, it modifies a little these parameters to achieve the real curve.

The iterations stop when you reach the maximum number of iterations, when the difference with the real curve is too small (this is not customizable), or when after several iterations, the variation of the parameters does not improve the fitting result. This parameter controls how much the parameters vary


on each iteration. A high value means that the parameters change a lot on each iteration, which will be very useful in those cases where the initial curve is really different with the real curve. The user should not need to change this value.

**Report Current:** to report the Line Fitting panel. This icon includes a scroll down menu to copy the report to the clipboard, report or copy the fit regions or customize the format of the report.

Μ	nov	78		)	(e + ) =	Libro1 - Mi			
e Fitting				Inicio I	nsertar Diseño	de página Fo	irmulas Dato	s Revisar Vis	a 🎯 – 🗂
Name: M1	Report Current		R	egar 👌	N K § -	A A A Aline	ación Número	Estilos Čeldas	Σ - 27- 
From: 2.858 pp		÷		G7	• (*	$f_{\mathbf{x}}$			
	Copy Regions	M		A	В	С	D	E	F
ppm	Setup Report	Widt	1	Name: M1					
The second			2	From: 6, 125 pp	m				
1 2.9255	74.36	1.62	3	To: 6.773 ppm					
2 2.9110	233.66	1.62	4	Residual Error:	7/555.05				
3 2.8964	240.25	1.62	5	#	2. AD111	Height	Width(Hz)	58.5	Area
5 2.0304	240.25	1.02	6		1 6.6122	31.63	15		4070.436
4 2.8819	79.51	1.65	7	-	2 6.5402	94.9	15		12211.314
5 2.8640	-2.26	5.00	8		3 6.4852 4 6.4632	31.63	15		4070.433
			9		4 6.4632 5 6.364	31.63	15	(TE)	4070.439
4	-1		11	2	5 6.3286	31.63	15		4070,44
Residual Error:	12.3484		11	2	7 6.2399	31.63	15		4070.435
			13   4    13	< → → Hoja	- a	ioja3 🦯 🖏 🖊	14	100% (=)	

Follow the menu 'Scripts/Export ASCII/Fit Regions' to export the results in a .txt file.

The format of this report can be also customized by following the menu 'Advanced/Line Fitting/Setup Report'. You can also create reports by using the 'Line Fitting' scroll down menu:

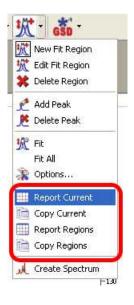

Select Lines to Show: toggle button to show or hide the fitting lines (peaks, sums or residues) Previous/Next Region : to navigate through the fit regions. Name: to change the name of the fit region. From/To: to change the rang of the fit region.

Add Peak: 12 to add a new peak to the region

Delete Peak: Method to delete the current peak of the region (or all peaks at the same time)

**Create spectrum:** To generate a new spectrum from the fit regions.

### **10.1.1 Line Fitting Properties**

You can customize the colours (and transparency) of the Fit regions, label and lines (Peaks, Sum and residue) from the 'Properties' dialog box, which can be accessed by double clicking on the spectral window and selecting 'Fitting' in the left tabbed menu


R Properties		?
Ø · 🗐		
	MR Spectrum	
Geometry Spectrum Scales Cales Peaks Integrals Integrals Multiplets GSD SD	Region  Region  Dark green  Label  MS Shell Dlg 2  Peak  Sum  Region  Region  Region  Magenta  Region  Region Region Region  Region Region Region  Region Region Region  Region Region Region Region	
Fitting	Restore	OK Cancel Apply

### **10.2 TD Quantitation**

This feature will be used for the processing and analysis of low-field, time domain data acquired in Oxford Instruments.

See this paper for further information.


First of all, you will need to load the NMR spectra which will be automatically displayed as an overlaid plot of FIDs. It is recommended to start with the datasets which belong to samples of known concentration, in order to build a calibration curve:

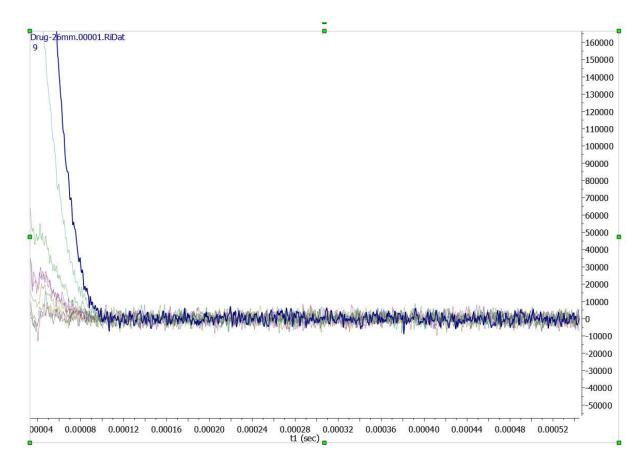

Next follow the menu 'Advanced/Quantiation":

; [	Advanced Stack Predict M	ass Ai	nalysis Documents Scri
nt	Line Fitting	•	- MIM -
	Data Analysis Reaction Monitoring	*	Drug-26mm.00001.RiD
	Time Domain	•	Quantitation
	Bayesian DOSY Transform Align Spectra Reference Alignment PCA		

That will display the TD Quantitation window. Clicking on the 'blue plus button' 💽 will allow you to select the integration region (by clciking&dragging):

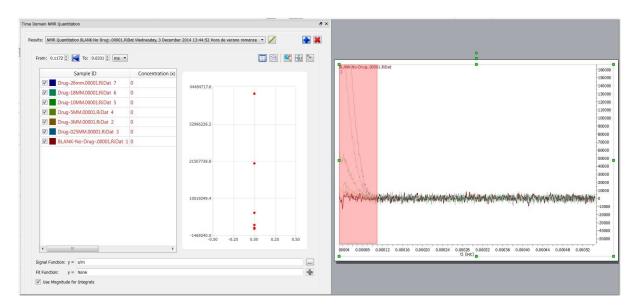

The next step will be fill the concentration and mass columns with the known values (for each of the samples used as reference):

				_					
Sample ID	Concentration (x)	Theor. Concentration (Diff)	Value (y)	Mass (m)	Signal (s)	Theor. Value (Diff)			
Drug-26mm.00001.RiDat 9	100	00.303 (-0.303166)	3.41017e+06	7.51	.56104e+07	1.33126e+07 (-9.90241e+06)	3579181.7		
I Drug-18MM.00001.RiDat 8	49.91	4 <mark>9.395 (0.514961)</mark>	1.68761e+06	7.51	.26739e+07	3.39992e+06 (-1.71231e+06)	5575101.7	1	(*100*0#) (#
Drug-10MM.00001.RiDat 7	12.86	2.4606 (0.399363)	437868	7.51	.28839e+06	1.70503e+06 (-1.26716e+06)			4
Drug-5MM.00001.RiDat 4	3.29	43514 (-0.145139)	132475	7.51	94887	127564 (4911.04)		/	Newman
Drug-3MM.00001.RiDat 2	1.1	10354 (-0.00353526)	53581.1	7.51	02394	53461.5 (119.622)	2649636.3		
Drug-025MM.00001.RiDat 3	0.71	765608 (-0.055608)	42146.8	7.51	16522	40265.2 (1881.59)			
BLANK-No-Drug00001.RiDat 1	0	406876 (-0.406876)	30008.4	7.51	25363	16241.1 (13767.3)		/	
							-138999.8 -0. 22.5	50.0 77.5 105 50.0 77.5 100 50.0 77.5 100	

Automatically, we will get a calibration curve with a fit function which will be used to calculate the concentration of unknown samples. Statistic information can be displayed by clicking on the plus button besides the Fit Function.

The next step will be to load the datasets of the unknown samples and enter the mass values for each of the samples. Automatically, we will get the applicable concentration values (according to the calibration curve):

Sample ID           2         Drug-26mm.00001.RiDat 9           2         Drug-18MM.00001.RiDat 8           2         Drug-10MM.00001.RiDat 7           3         Tablets-400MG-Drug-278KN.00001.RiDat 7           4         Drug-3MM.00001.RiDat 2	6 16.6954	Theor Concentration (Diff) 100.303 (-0.303166) 49.395 (0.514961) 12.4606 (0.399363)	Value (y) 3.41017e+06 1.68761e+06 437868	Mass (m) 7.51 7.51 7.51	Signal (s) 2.56104e+07 1.26739e+07	Theor. Value 1.33126e+07 (-9.9 3.39992e+06 (-1.7	3579181.7	
Z         Drug-18MM.00001.RiDat 8           Z         Drug-10MM.00001.RiDat 7           Tablets-400MG-Drug-278KN.00001.RiDat           Tablets-400MG-Drug-75KN.00001.RiDat           Drug-5MM.00001.RiDat 4	49.91 12.86 t 5 16.6414 16.6954	49.395 (0.514961)	1.68761e+06 437868	7.51			3579181.7	
Image: 10MM.00001.RiDat         7           Image: 10MM.00001.RiDat         7           Image: 10MM.00001.RiDat         7           Image: 10MM.00001.RiDat         4	12.86 5 16.6414 6 16.6954		437868		1.26739e+07	3.39992e+06 (-1.7	33/9101./	1
Tablets-400MG-Drug-278KN.00001.RiDat Tablets-400MG-Drug-75KN.00001.RiDat Drug-5MM.00001.RiDat 4	t 5 16.6414 6 16.6954	12.4606 (0.399363)		7.54				
Tablets-400MG-Drug-75KN.00001.RiDat	6 16.6954			7.51	3.28839e+06	1.70503e+06 (-1.2		
Drug-5MM.00001.RiDat 4			579331	2.86	1.65689e+06			
			581160	2.8274	1.64317e+06		2649636.3	
Drug-3MM.00001.RiDat 2	3.29	3.43514 (-0.145139)	132475	7.51	994887	127564 (4911.04)		
	1.1	1.10354 (-0.00353526)	53581.1	7.51	402394	53461.5 (119.622)		
Drug-025MM.00001.RiDat 3	0.71	0.765608 (-0.055608)	42146.8	7.51	316522	40265.2 (1881.59)		
BLANK-No-Drug00001.RiDat 1	0	0.406876 (-0.406876)	30008.4	7.51	225363	16241.1 (13767.3)	1720090.9	
		ш					790545.6 -138999.8 -5.0 2	22.5 50.0 77.5 105.0

As you can see in the screenshot above, the known references used for the calibration curve appear in red and with the check box selected, whilst the samples to analyze appear in blue and unchecked.

#### 10.2.1 TD Quantitation panel

Let's describe some of the features that appear in the TD quantitation panel:

im: 0.0350 🏚 📢 To: 0.0553 🛊 ms 🔹								🔲 🖻 🛯 🖬 🖬
Sample ID	Concentration (x)	Theor Concentration (Diff)	Value (y)	Mass (m)	Signal (s)	Theor. Value		
Drug-26mm.00001.RiDat 9	100	100.303 (-0.303166)	3.41017e+06	7.51	2.56104e+07	1.33126e+07 (-9.9	3579181.7	
Drug-18MM.00001.RiDat 8	49.91	49.395 (0.514961)	1.68761e+06	7.51	1.26739e+07	3.39992e+06 (-1.7		/
Drug-10MM.00001.RiDat 7	12.86	12.4606 (0.399363)	437868	7.51	3.28839e+06	1.70503e+06 (-1.2		/
Tablets-400MG-Drug-278KN.00001.RiDat	5 16.6414		579331	2.86	1.65689e+06			
Tablets-400MG-Drug-75KN.00001.RiDat 6	16.6954		581160	2.8274	1.64317e+06		2649636.3	
Drug-5MM.00001.RiDat 4	3.29	3.43514 (-0.145139)	132475	7.51	994887	127564 (4911.04)		
Drug-3MM.00001.RiDat 2	1.1	1.10354 (-0.00353526)	53581.1	7.51	402394	53461.5 (119.622)		
Drug-025MM.00001.RiDat 3	0.71	0.765608 (-0.055608)	42146.8	7.51	316522	40265.2 (1881.59)		
BLANK-No-Drug00001.RiDat 1	0	0.406876 (-0.406876)	30008.4	7.51	225363	16241.1 (13767.3)	1720090.9	
		m					790545.6 -138999.8 -5.0 2	2.5 50.0 77.5 105.0
•								

This feature will allow you to rename the experiment.

Enter the desired values in the boxes below to change the ranges. Additionally, you can select the first point in the spectrum as start point of the region. From here you can also change the units (seconds, milliseconds or  $\mu$ s)

From:	0.0000 😩 [	🚽 То:	0.0553 🤤	ms 🔹
		Use	first point	]

From the panel we can also 'show/hide' the table, copy the table to the clipboard, zoom in the graph, restore the zoom and copy the graph to the clipboard:



# **10.3 DOSY Transform**

(Not available in Mnova Lite)

**NMR diffusion** experiments provide a way to separate the different compounds in a mixture based on the differing translation diffusion coefficients (and therefore differences in the size and shape of the molecule, as well as physical properties of the surrounding environment such as viscosity, temperature, etc) of each chemical species in solution. In a certain way, it can be regarded as a special chromatographic method for physical component separation, but unlike those techniques, it does not require any particular sample preparation or chromatographic method optimization and maintains the innate chemical environment of the sample during analysis.

The measurement of diffusion is carried out by observing the attenuation of the NMR signals during a pulsed field gradient experiment. The degree of attenuation is a function of the magnetic gradient pulse amplitude (G) and occurs at a rate proportional to the diffusion coefficient (D) of the molecule. Assuming that a line at a given (fixed) chemical shift f belongs to a single sample component A with a diffusion constant  $D_A$ , we have

$$\mathbf{S}(\mathbf{f},\mathbf{z}) = \mathbf{S}_{A}(\mathbf{f}) \exp(-\mathbf{D}_{A}\mathbf{Z})$$
(1)


where  $S_A(f)$  is the spectral intensity of component A in zero gradient ('normal' spectrum of A),  $D_A$  is its diffusion coefficient and Z encodes the different gradient amplitudes used in the experiment.

Depending on the type of experiment, there are various formulae for **Z** in terms of the amplitude **G** of the applied gradient and one or more timing parameters such as (time between two pulse gradients, related to echo time) and (gradient pulse width). In the original Tanner-Stejskal method using two rectangular gradient pulses, for example,

# $Z = 2G2 \ 2(-/3)$ (2)

The above equation holds strictly for simple PFG-NMR experiments, and is modified slightly to accommodate more complicated pulse sequences.


In practice, a series of NMR diffusion spectra are acquired as a function of the gradient strength. For example, the figure below shows the results of a series of 1H-NMR diffusion experiments for a mixture containing caffeine, 2-Ethoxyethanol and water.

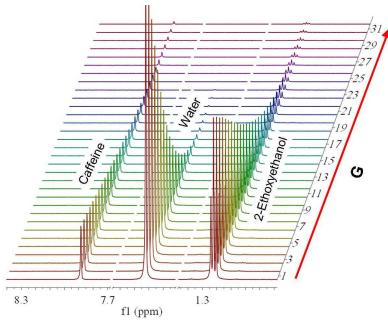

It can be observed that the intensities of the resonances follow an exponential decay. The slope of this decay is proportional to the diffusion coefficient according to equation (1). All signals corresponding to the same molecular species will decay at the same rate. For example, peaks applicable to water decay faster than the peaks of caffeine and 2-Ethoxyethanol

# The DOSY transformation

As far as data processing of raw PFG-NMR spectra is concerned, the goal is to transform the NxM data matrix S into an NxR matrix (2D DOSY spectrum) as follows:

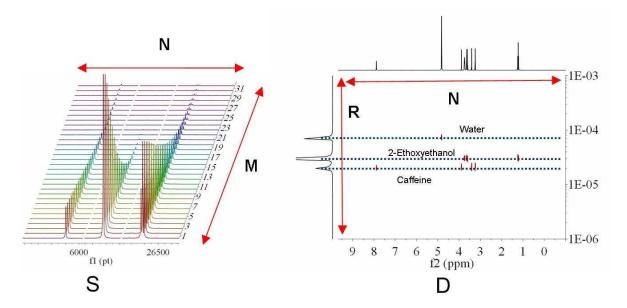

The horizontal axis of the DOSY map D is identical to that of S and encodes the chemical shift of the nucleus observed (general 1H). The vertical dimension, however, encodes the diffusion constant D. This is termed **Diffusion Ordered Spectroscopy** (DOSY) NMR. In the ideal case of non-overlapping component lines and no chemical exchange, the 2D peaks align themselves along horizontal lines,

each corresponding to one sample component (molecule).


The horizontal cut along such a line should show that component's 'normal' spectrum. Vertical cuts show the diffusion peaks at positions defining the corresponding diffusion constants.

The **mapping S=>D** will be henceforth called the DOSY transformation. This transformation is, unfortunately, far from straightforward. Practical implementations include mono and biexponential fitting, Maximum Entropy, and multivariate methods such as DECRA.

We have recently developed a brand new method for DOSY processing which has been included in <u>Mnova</u>.

# **Bayesian DOSY Transform**

Let's see how this feature works step by step:

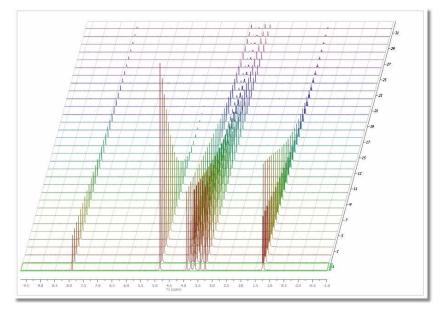

1. **Import your raw data:** for example by dragging the spectrum folder into Mnova:

2. **Process the spectrum:** Mnova processes the spectrum automatically for you. However, it might be necessary to apply some further processing, usually manual phase and baseline correction

You can do that directly on the stacked plot mode, but it's recommended to use the 'Active Spectrum' mode as depicted below:



Within the 'Active Spectrum' mode, correct any phase distortion and apply an automatic baseline correction (use Berstein polynomials). These corrections will be applied to the whole dataset. You can also apply the <u>Align</u> tool (under the Advanced menu) if the traces are not aligned.

3. Setup Diffusion-related exp. values: Make sure that the big and little delta values have been correctly read from the experiment files by following the menu 'View/Tables/Arrayed Data' (or Stack 'Show Arrayed Data Table').

# **NOTE** The gradient values are read from the difflist, whilst the small delta values are taken from Pulse Width (from P30 and PULPROG) in acqus file. A formula has to be used to calculate the value: p30\*1.0e-6. When the pulprog is bipolar (pulse sequence containing 'bp'), the value is multiplied by 2.

These values should be entered in seconds:

ØE,	-	Layout Templates	•	Page 👻 📐 🔍 🔍 🛞 🖉 🖌 🔛 川	犬 犬 十 圦 ▼   12 / 10 ▼   約 斧 ▼ 塩 ▼ 輝 ▼ 歯 爻 ▼ 沢 ▼ 雅 ▼ 扨	
1. Bruk		Pages Full View				
L. DEUK		Rulers			Arrayed Data	
		Toolbars				
		Tables	÷	Close All		-2600
		Panels		Close All	γ (G <sup>-1</sup> s <sup>-1</sup> ): 26752.2212	
	-	Center Floating Windows		Elemental Composition	Δ (s): 1.2000 Φ δ (s): 0.0031 Φ	-2400
	-	Customize Context Menus		Molecule Match	Restore	
				Mass Peaks	G': G"k	-2200
2	H.	History		Molecules	Z: pow(g*G*d,2)*(D-d/3)	
	R)	Previous Page		GSD Peaks	G G' Z	-2000
	Ψ.	Next Page		Arrayed Data	1 1.69 16.86 2.34e+06	
	II	Fit to Height	н	Assignments	2 1.90 19.03 2.99=+06	-1800
	t	Increase Intensity	+	Integrals	2 1.90 19:05 2.99=+06 3 2.12 21:21 3.71e+06	
	ĩ	Decrease Intensity		Multiplets		-1600
				Parameters	4 2.34 23.38 4.51e+06	
	+	Crosshair	С	Peaks	5 2.56 25.56 5.39e+06	-1400
		Zoom	1	Verification Results	6 2.77 27.73 6.34e+06	
		Expansion Pan	E	Well Plates	7 2.99 29.91 7.38e+06	-1200
3	*	Pan	P		8 3.21 32.08 8.49e+06	-1000
		Cuts	•	13C Prediction	9 3.43 34.26 9.68e+06	1000
		Stacked Mode	•	1H Prediction X-Nuclei Prediction	10 3.64 36.43 1.09e+07	-800
		2D Plotting Method	•	X-Nuclei Prediction	11 3.86 38.61 1.23e+07	
		2D Traces	•		12 4.08 40.79 1.37e+07	-600
					13 4.30 42.96 1.52e+07	
					14 4.51 45.14 1.68e+07	-400
					15 4.73 47.31 1.85e+07	
					16 4.95 49.49 2.02e+07	-200
					17 5.17 51.66 2.20e+07	
				A	18 5.38 53.84 2.39e+07	-0
					19 5.60 56.01 2.59e+07	1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
					20 5.82 58.19 2.79e+07	200
			9.5	9.0 8.5 8.0 7.5 7.0 6.5 6.0	0 55 50 05 0	1.0 -0.5 -1.0
					fi (ppm)	

By means of the bayDOSY transform (BDT) we are fitting a model of the type

 $S(f,z) = S_A(f) \exp(-d_A z)$ 

where  $S_A(f)$  is the spectral intensity of component A in zero gradient ('normal' spectrum of A) and  $d_A$  is its diffusion coefficient. Z values corresponding to the expression above are displayed in the third column which are calculated according to the formula highlighted in the figure.

It's assumed that the gradient strength comes in G/cm. Note that the values used by the algorithm are those listed in the G' column which are in turn obtained from G column after multiplying these values by the k factor.

#### ΝΟΤΕ

Mnova will read the arrayed parameter directly from the metadata. However, in some cases, the units are not in the correct format and thus Mnova gives the user the opportunity to scale the values parsed from the metadata by simply scaling those values by a factor k. So what Mnova reads directly from the metadata is column G (or t in the case of Reaction-Monitoring or metabonomics examples), whilst column G' is the result of scaling G by the scaling factor k. Column Z is the final arrayed parameter, parameter which will be used in several other places such as DOSY transform, Data Analysis, etc.

4. Run the Bayesian DOSY Transform: Just by following the menu 'Advanced/DOSY Transform'


Method:	Bayesian		-	ок
Method Options				Cancel
Resolution Factor:	1.00		-	Restore
Repetitions:	1			More >>
DOSY spectrum				
Minimum: 1.00e-06	Maximum:	1.00e-04	-	
Points in diffusion dime	nsion:	128		

a) Enter the minimum and maximum expected diffusion values. If the gradient strengths have been introduced in G/cm, the resulting diffusion coefficients will be in cm^2/s


b) To start with, use a resolution factor of 1 (or 0.1). Higher values will increase the resolution along the diffusion dimension (vertical). However, small peaks can be missed when the resolution factor is too high

c) The number of repetitions should be kept to 0 for the first try. Next, if you want to further increase the vertical resolution, set this value to 1 or 2. This should drastically increase the resolution, though some artifacts might appear.


This is the result obtained. As you can see the 3 compounds (water, ethoxyethanol and caffeine) are perfectly separated.

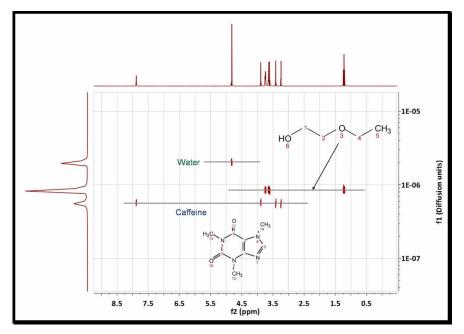


You can use the 'Crosshair' to measure the Difussion values.

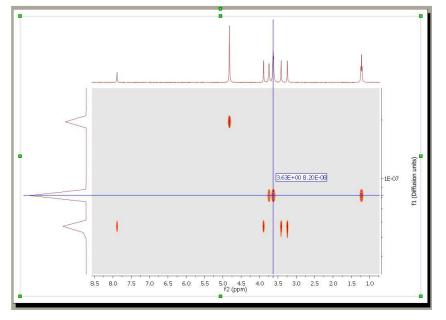

Non-uniform gradient (NUG) correction can be applied by checking the option "Correct for non-uniform gradients" in Bayesian DOSY Transform dialog (the options only appear if the dataset requires them):

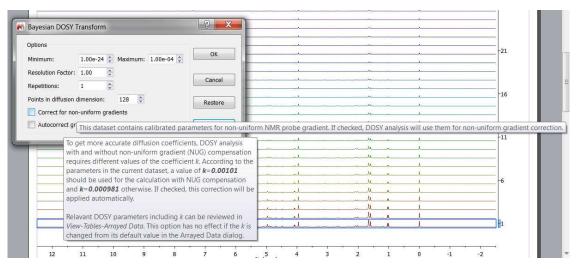

You can also use the <u>'Data Analysis'</u> feature to get your **Diffusion coefficient** in the traditional way (given by the value of the parameter G):

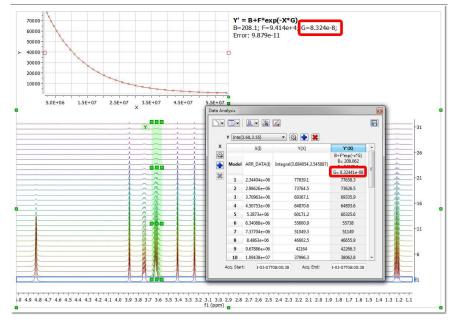

#### **Peaks Heights Fit**

A new "Peak Heights Fit" method is added to DOSY processing capabilities. The existing Bayesian DOSY routine provides a full continuous map of diffusion coefficients found in the system. To provide a more "filtered" DOSY 2D output and improve consistency with other spectrometer software a new DOSY processing technique is implemented.

Method:	Peak Heig	hts Fit	•	ОК
Method Options	aks			Cancel
Autocorrect pea				Restore
Voerlapped pea	ıks analysis			<< Less
DOSY spectrum				
Minimum: 1.00e-0	6 🍦 Maximum:	1.00e-03		
Points in diffusion d	imension:	128		
Reduce Size in a Fa	ctor			

#### **Options:**

<u>Use existing peaks</u>: If there are user-defined peaks at the start-up of the procedure, these peaks can be used instead of applying a fresh peak picking.

<u>Autocorrect peak positions:</u> It could be a slight variation in the peak positions going from row to row of the arrayed DOSY experiment. The peak position can be adjusted to compensate the effect.

<u>Overlapped peaks analysis:</u> to resolve overlapped peaks and report independent diffusion coefficients for them.


The procedure support NUG correction. For data without NUG coefficient a highly efficient exponential fitting routines is used. If NUG calibration exists, then D values found in this procedure are used as starting points for non-linear Levenberg–Marquardt fitting using NUG-corrected decay model.

#### **Bayesian DOSY and quantification**


The Bayesian DOSY-data transform algorithm (BDT) in Mnova is inherently linear so amplitudes of "responses" are proportional to "inputs". However, that is not the whole story: The Bayesian approach always involves a final normalization which is pretty much a matter of choice and in BDT leaves a lot of degrees of freedom to play with. We normalize each column in the resulting 2D map so that it matches the point in what would be the 1D spectrum corresponding to zero gradient. Such column normalization might look as involving a series of integrals along the D-axis, but it is not, because an "integral along the D-scale" makes no sense (at best it might be viewed as a kind of Stieltjes integral, with properly defined D-scale interval weights). It is a trick, an intuitive hack, which however greatly alleviates the quantitation problem. Ratios of peak integrals in the projection therefore come quite close to ratios between component quantities. However, given the inherent impossibility to justify an "integral along D or logD", we tend to avoid the concept, at least for the time being, especially should somebody integrate over very broad intervals of D's, or compare two integrals around very different D values. From this point of view, given the kind of normalization we have adopted, peak heights are more rigorous quantities - unless the peaks of a component get misaligned on the D axis because of artifacts (for that reason a moderate integration including just very few D-scale points might be acceptable).

So, BDT will help you to obtain the relation of each compound by just integrating the diffusion trace. To do that, just right click on the trace and select 'Setup' in the contextual menu to display the 'Setup

Traces' dialog box. Once there click on the 'blue arrow icon to extract the 'Vertical Trace'. Please make sure that this trace is the 'Internal Projection' (Sum):

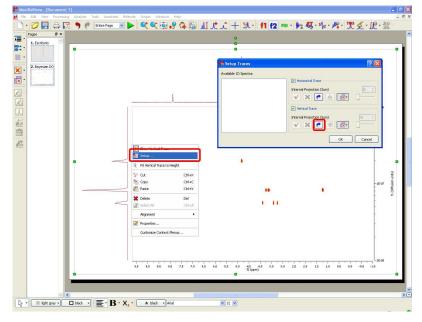


This will extract the trace to a new page. Finally integrate the signals of this trace to get the applicable ratio of the compounds:

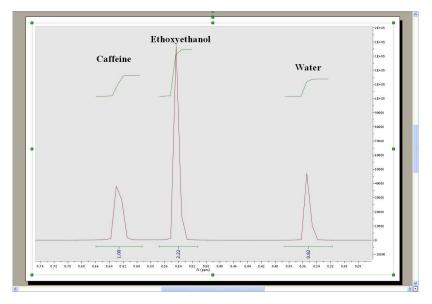

## **10.4 Data Analysis Quick Start Guide**

First of all, please make sure that you are familiar with stacked plots. Take a look at this <u>chapter</u> for further information.


Let's see how the Data Analysis feature works. Just load your experiment into Mnova:

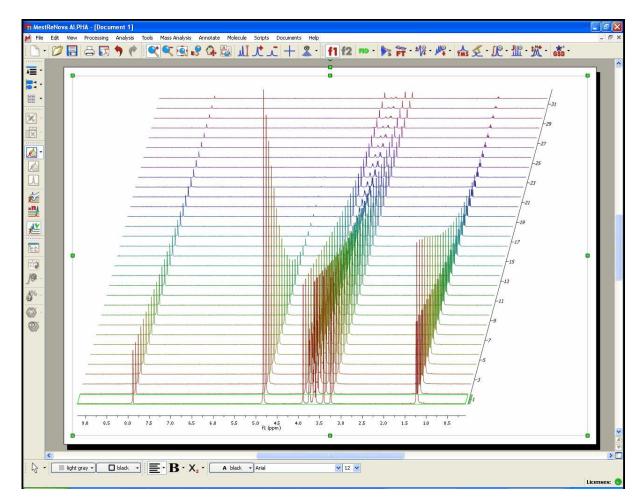

Follow the menu 'Advanced/Data Analysis/Create' and select the desired graphical representation. In that case 'Integrals Graph':

Line Fitting	*		१ 🔍 🧕	2	0	5 1 1 1 1 W	+
Data Analysis	•		Create	۲	n	Empty Graph	1
Reaction Monitoring	•		Report	1.	A	Integrals Graph	-
Bayesian DOSY Transform Align Spectra Reference Alignment	1		Import Export		▲ 火肥	Concentration Graph Peaks Graph Max. Peak Graph	
J-Correlator Filter False Positives			Pick Edit	•	12 L	Max. Peak Pos. Graph Alignment Shifts Graph	
Arithmetic		_	Show Table		+		
Spin Simulation							
qNMR	•			-			-
Mnova Screen							

You will notice how the cursor will change to a blue integral. Now you will only need to integrate the desired signal (in this case, we will select the signal at 1.20 ppm). Once you have integrated the

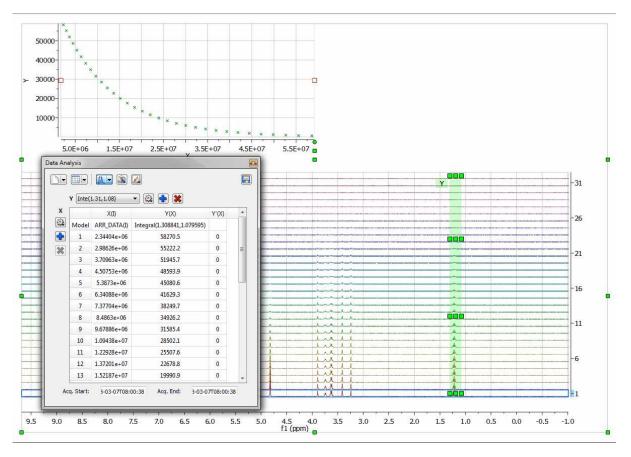

desired region, you will notice how the graphical will change according with the decay of the signal. Please bear in mind that all values will appear in a tabulated form in the <u>Data Analysis panel</u>

NOTE: the integration calculation method used in the Data Analysis will be the one selected under the 'Integral Options' (Analysis/Integration/Options).

Finally, allow Mnova to try to guess the order of the reaction, fitting the data to standard equations and comparing the mean square error. To do it just follow the menu ' Advanced/Data Analysis/Edit/Fit to Best'.

Advanced Stack Mass Analysis	Pre	edict Annotate Scripts	Documents Help
Line Fitting	11	잘 📐 🔲 🔍 🔍	NIL CO O SE
Data Analysis		Reaction Monitoring	1
Bayesian DOSY Transform		Create +	
Align Spectra Reference Alignment		Import Export	
J-Correlator Filter False Positives		Pick •	-
		Edit	🎖 Disable Points
Arithmetic		Show Table	Fit To Best
Spin Simulation	Γ		🛞 Edit Model Options
Verification +		100	

You can also set the 'Fit to Best' option by default by selecting 'Fit Function=Best Fit' on the 'Edit Model Options'

You will find the result of the fitting in the <u>'Data Analysis' panel</u> (View/Panels/Data Analysis). In that case, the best fit would be a 'Three Parameter Exponential'. If you are not happy with the fitting, just c lick on the first cell of the column Y'(X) to select any other function:

Ant	lysis		Y			Name	Function	Initialization Re	nort
I.		.31,1.08)		- 🗟 🖡 🗶		1 Linear Fit 2 Mono-exponential Fit 3 Three Parameter Exponential Fit	A+B*x B*exp(-x*F)	A= 0, B= 0	Zero Order R Exponential E Exponential E
x		X(I)	Y(X)	Y'(X)		4 Inverse Linear Fit	1/(A+B*x)	A= 1, B= 0	Second Order
	Model		Integral(1.308841,1.079595)	B+F*exp(-x*G) B=153.914 F= 70474.2 G= 8.31486e-08		5 			
×	1	2.34404e+06	58270.5	58148.2		Restore Defaults			
	2	2.98626e+06	55222.2	55132.5		Fitted Parameters			
	3	3.70963e+06	51945.7	51923.2		Calculate			
	4	4.50753e+06	48593.9	48600.1		Calculate			
	5	5.3873e+06	45080.6	45182.6		B= 153.914, F= 70474.2, G= 8.3148 rError = 9.32836e-11, probnotmono =			
	6	6.34088e+06	41629.3	41750.3		Torio - Statesse 11, prostronisto			
	7	7.37704e+06	38249.7	38316.5					
	8	8.4863e+06	34926.2	34954.1				[ c	K Cancel
	9	9.67886e+06	31585.4	31668.9	6				
	10	1.09438e+07	28502.1	28522.6			-		-6
	11	1.22928e+07	25507.6	25512.6					
	1.7	1 27201 - 07	27670.0	22674.0		*			

NOTE: The Probnotmono value is important to assess whether or not the model for the fit we are assuming, in this case, a three parameter-exponential model satisfies. For instance, if you assume a mono-exponential model but the experimental data follows a bi or multi-exponential behavior, then the analysis will not be fully correct.

On the other hand, if we assume that the model is mono-exponential, the 'rError' value gives the [absolute] probable error in the value of 'r', where 'r' is:

 $y = a^*exp(-r^*x)+b$ 


This error is calculated based on the assumption that the final residues correspond to the actual noise in the data.

#### 10.4.1 Data Analysis

Mnova incorporates a **'Data Analysis'** feature for the analysis of diffusion experiments. This feature covers also relaxation (T1/T2) experiments, kinetics, reactions monitoring, etc.

With this feature you will be able to extract the peak intensities and integrals in a tabular form from series of 1D NMR experiments and to draw graphical representations of the extracted values as well as any fit results.

Let's see how this feature works in the case of a diffusion sample. Just load your experiment into Mnova:

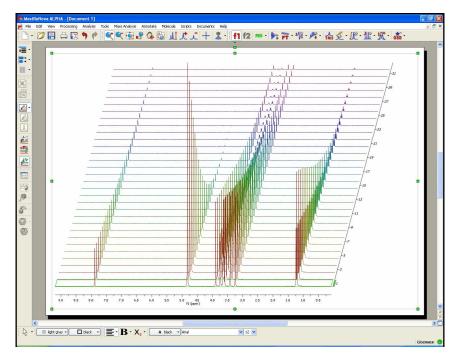

Follow the menu 'Advanced/Data Analysis/Create' and select the desired graphical representation


Data Analysis       Create       Empty Graph         Reaction Monitoring       Report       Integrals Graph         Bayesian DOSY Transform       Import       Concentration Graph         Align Spectra       Import       Peaks Graph         Reference Alignment       Pick       Max. Peak Graph         J-Correlator       Filter False Positives       Alignment Shifts Graph         Spin Simulation       Show Table       Show Table	Line Fitting	<b>)</b> E	0	र् 🔍 🧕 ।	8	0	<b>3</b>	L IL	1 K	×	+
Bayesian DOSY Transform     Import     Concentration Graph       Align Spectra     Import     Peaks Graph       Reference Alignment     Pick     Max. Peak Graph       J-Correlator     Filter False Positives     Alignment Shifts Graph       Spin Simulation     Show Table	Data Analysis					3	11.85	y Graph		1	
Bayesian DOSY Transform       Import       Concentration Graph         Align Spectra       Import       Peaks Graph         Reference Alignment       Export       Max. Peak Graph         J-Correlator       Filter False Positives       Max. Peak Pos. Graph         Arithmetic       Show Table       Show Table	Reaction Monitoring	•		Report		IL	Integ	als Graph	i		-
J-Correlator Filter False Positives Arithmetic Spin Simulation	Align Spectra			Import	•	ふとと	Peaks	ks Graph			
Spin Simulation	and realized an ever					-		and the second			
	Arithmetic		-	Show Table		ł	ACCESSION INTERACTOR			12-004	-
qNMR +	Spin Simulation					-					
	qNMR	٠		-	2010		_	1100000		1.5.00	

Let's select for example the 'Integrals Graph' option; you will notice how the cursor will change to a blue integral. Now you will only need to integrate the desired signal (in this case, we will select the signal at 1.20 ppm). Once you have integrate the desired region, you will notice how the graphical will change according with the decay of the signal. Please bear in mind that all values will appear in a tabulated form (in this case the integral values) and you will be able to export them to 3rd party apps


for further post-analysis or reporting (just by clicking on the 'Copy to Clipboard' button <sup>1</sup> of the table or by saving as XML files). Notice also that, if you integrate another region of the spectrum, the curve will be updated.

NOTE: the integration calculation method used in the Data Analysis will be the one selected under the 'Integral Options' (Analysis/Integration/Options).

Go to this chapter to see a fully description of the Data Analysis panel

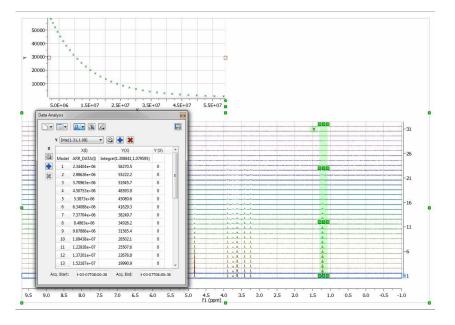



Please notice, that the integrated region will be highlighted in green and will contain several handlers to modify the ranges of the integration just by clicking&dragging them (which will be really useful for 'reaction monitoring' in order to account for peaks movements). Holding down the 'shift' key, whilst you click and drag on any of the handlers, will shift all the handlers together of the same vertical.

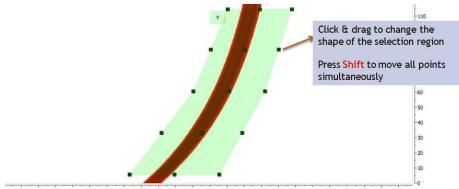

5.1 5.0 4.9 4.8 4.7 4.5 4.4 4.3 4.2 f1 (ppm) 4.1 4.0 3.9 3.8 3.7 3.6 3.5 3.4 3.3 3.2 3.1 5.3 5.2 4.6

This new selection method works with any displaying mode: bitmap, stacked, active spectrum ... The picture below shows this with the stack mode

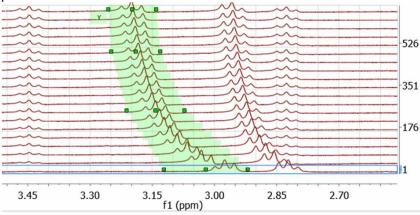

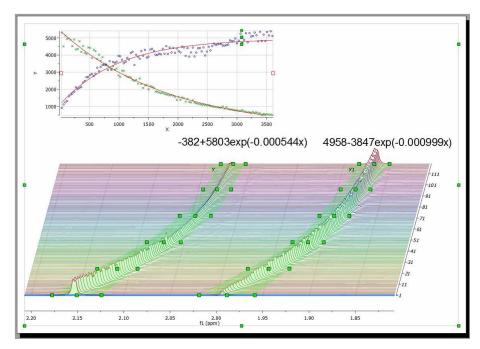

Here you can see another example, where the graphical tool can be very useful to follow the evolutions of the signals:

Clicking on the first cell of the column Y'(X) will allow you to fit the curve. In this case, we will fit it as a three parameter exponential curve.

5.	DE+06	1.5E+0	7 2.5E+07 3.5E+07	4.5E+07 5.5E+0		Functions			
ta Ana	lysis		191			Name	Function	Initialization	Report
1.						1 Linear Fit	A+B*x	A= 0, B= 0	Zero Order R
100	(000100)					2 Mono-exponential Fit	B*exp(-x*F)		Exponential E
	Y Inte(	1.31,1.08)		- 😫 🛖 😫		3 Three Parameter Exponential Fit	$B+F^{*}exp(-x^{*}G)$		Exponential E
x		X(I)	Y(X)	Y'(X)	1	4 Inverse Linear Fit	1/(A+B*x)	A= 1, B= 0	Second Orde
4 + *	Model	ARR_DATA(I)	Integral(1.308841,1.079595)	B+F*exp(-x*G) B=153.914 F=70474.2 G=8.31486e-08		5 • m			
*	1	2.34404e+06	58270.5	58148.2		Restore Defaults			
	2	2.98626e+06	55222.2	55132.5		Fitted Parameters			
	3	3.70963e+06	51945.7	51923.2		Calculate			
	4	4.50753e+06	48593.9	48600.1		(management)			
	5	5.3873e+06	45080.6	45182.6		B= 153.914, F= 70474.2, G= 8.31480 rError = 9.32836e-11, probnotmono =			
	6	6.34088e+06	41629.3	41750.3					
	7	7.37704e+06	38249.7	38316.5					
	8	8.4863e+06	34926.2	34954.1					OK Cancel
	9	9.67886e+06	31585.4	31668.9					

You can also select the 'Edit Fit' option below:

nalysis	<u>M</u> - 🔉 (	<b>a</b>				
Contraction Contraction	.34,3.08)	<u>.</u>		3200 W.	1	
	X(I)		Experimen	ital 🕨	ox	
	ARR_DATA(I)	Integral (8.19	Fit 20,7.0007017	• <del></del>	~	Visible
1	2.34404e+06	1398	7.2	14	1003	Edit
2	2.98626e+06	1344	4.7	13	497	.2


Next, click on the 'Calculate' button to generate the error and the parameters of the fitting and finally click on the OK button to draw the fitting curve.

**NOTE** 


Probnotmono parameter is very important and deserves some more information: it gives the probability (0-1) that the decay is NOT monoexponential. For example, probnotmono>0.7 can be read as 'this could be non-monoexponential' while 'this is almost certainly non-monoexponential' when probnotmono>0.95

The rError is the quadratic error of the fit.

Ref: Gianni Ferrante and Stanislav Sykora, Technical Aspects of Fast Field Cycling, in Advances in Inorganic Chemistry, Vol. 57, Relaxometry of water-metal ion interactions, Elsevier 2004 (ISBN 0-120-23657-5), pp.405-470.

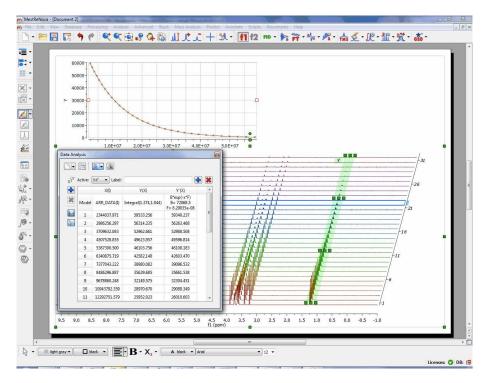


You can select other regions to be analyzed; each selected region will be colored differently (and the grab handle colors and graphical lines will have the same colors; which you can change by double clicking on the graph):

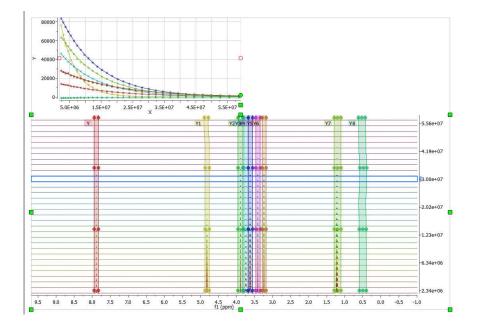


Follow the menu ' Advanced/Data Analysis/Edit/Fit to Best' to allow Mnova to guess the order of the reaction (by fitting the data to standard equations and comparing the mean square error):

Advanced Stack Mass Analysis	s Pre	edict Annotate Scripts	Documents Help
Line Fitting		🦻 📐 🔳 🔍 Q	NIL CO O SID
Data Analysis		Reaction Monitoring	-
Bayesian DOSY Transform		Create +	
Align Spectra Reference Alignment		Import Export	
J-Correlator Filter False Positives		Pick •	
Arithmetic		Edit •	Disable Points Fit To Best
Spin Simulation	T		Edit Model Options
Verification +	5	100	


From the menu above, you will also be able to disable points (either directly from the XY graph or from the table):

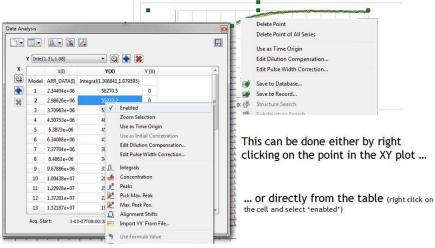

You can also disable points directly from your arrayed dataset, just by clicking on this button and then selecting the undesired signals on the dataset. You will notice how the applicable points in the XY graph will disappear and the signals on the stack plot will be highlighted in grey.

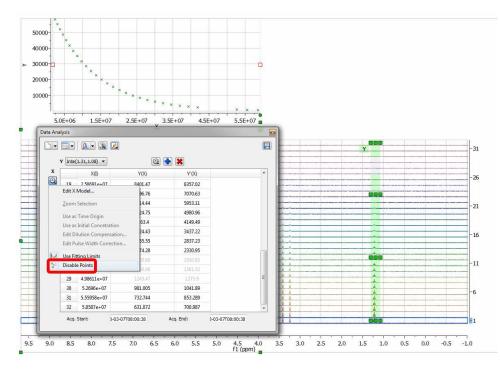

For convenience, you can **exclude points from the left and right** edges of the graph (by selecting 'Use Fitting Limits' on the Data analysis panel and highlighting the graph):

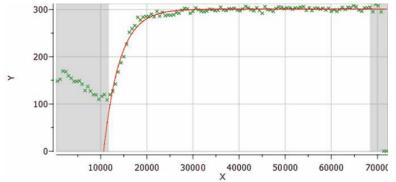

If you want to disable this option, just uncheck this button on the Data Analysis panel:



**IMPORTANT:** Every time a point is excluded, Mnova will *dynamically* recalculate the fitting function.

With the *Reaction Monitoring* plugin enabled, if you right click on any point of the Data Analysis Graph (or Table), you will be allowed to 'use that point as time origin', or to set the Dilution Compensation

Parameters' and 'Pulse Width Correction':

			🖌 Dilution Com	pensation	6	2 X
			Reagent Added: Volume		NaOH	*
	Delete Point Delete Point of All S	eries	Initial Volume:		0.50 ml	A V
	Use as Time Origin Use as Initial Conce	tration	Volume Added:	ł	0.15 ml	A v
	Edit Dilution Comp Edit Pulse Width Co		Time			T
R	C		Start Time:		2155.0 s	*
	Save to Record		End Time:		2185,0 s	A. Y
C.S.	Structure Search		<u>A</u> ddition Ra	ate:	0.300 ml/min	-
C.	Substructure Search	1				
0Å3	Formula Search				ОКСС	lancel
붠	Peak Search	🙀 Pulse Width Cor			-	? X
譜	Multiplet Search	Puise Width Col	rrection	-		9
殿美	Massitem Search Advanced Search	Start		End		
		Ţime: β1	76.00	Time:	3651.00	×
		pw90: 10	.00 µs	p <u>w</u> 90:	15.00 µs	<u>A</u> ¥
		Probe Retuned				
		Pulse Width Factor (	(pw/pw90):	1.00		×
					ок (	Cancel


Double click on the applicable cell to customize your NMR model by adding any other fitting formula:

	Name	Function	Initialization	Report	Description	Algorithm
1	Mono-exponential	B*exp(-x*F)			Exponential Decay (e.g DOSY)	monoExponentia
2	Three parameter exponential fit	B+F*exp(-x*G)		T1= 1/G;	Exponential Decay with Baseline Offset	monoExponential
3	User	A+Bx	A= 0, Bx= 0			general
4	Custom Exponential Fit	$B + 2F^{exp}(-x * F)$	B= 0, F= 0			general
5						
	ed Parameters Calculate					
- 8						

<u>Here</u> you can find a list of Mathematics javascript functions that you can use for your formulas (by using Math.sqrt(...))


# Crossing over of peaks

Crossing over of peaks is a very common event in Reaction Monitoring (RM) experiments. When this happens, the <u>automatic alignment algorithm</u> might not work properly. To illustrate this issue, we have simulated using Mnova a very simple data set comprised by a triplet and a singlet in such a way that the chemical shift of the triplet moves from 1.4 ppm to 0.7 ppm and having an exponential decay from spectrum to spectrum. This is depicted in the figure below, both as a stacked and a bitmap plot:

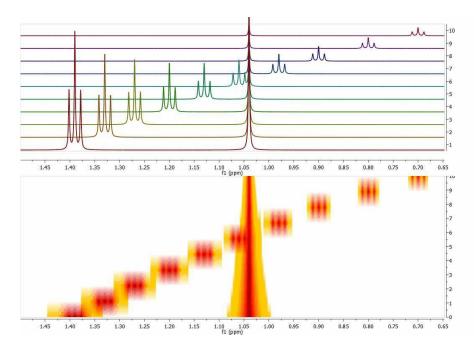


Now let's say you are interested in extracting the intensities of the triplet as the reaction progresses. There is actually no need to pre-align the spectra algorithmically; it is much simpler to have some kind of graphical tool to instruct the software which peaks (or multiplets) need to be used for the reaction monitoring analysis. Let me show you how this works in Mnova:

First of all, in the Data Analysis module you select the region to be analyzed. As a starting point, the region will have a rectangular shape (green rectangle in the figure below):

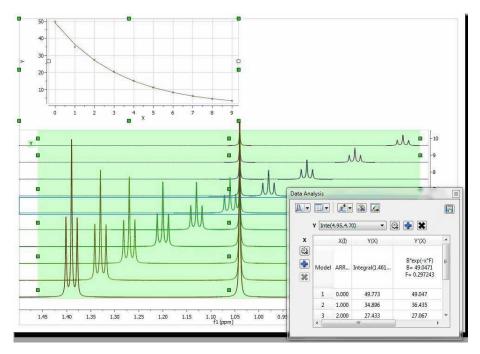


It can be noted that the graph shows an exponential decay, but the actual values must obviously be wrong as the values calculated, using the green rectangle as a boundary for the integration, include peaks from both the triplet and singlet, and we are interested in the analysis of the triplet resonances only.


The selection rectangle has a number of handlers (small green boxes). You can drag and move them freely so that you can adjust the selection feature to follow the triplet (the number of handlers can be adjusted in the Data Analysis options. In the figure below, the result of adjusting the handlers to follow the triplet is shown:

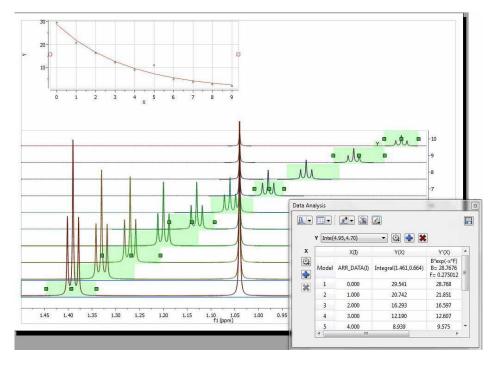


Now you can see that there is an outlier in the exponential curve which, obviously is caused by the singlet which overlaps with the triplet (spectrum number 6 which corresponds to data point #5, as in the graph the numbering starts from zero). Figure below shows that particular spectrum showing the singlet overlapping with the triplet:

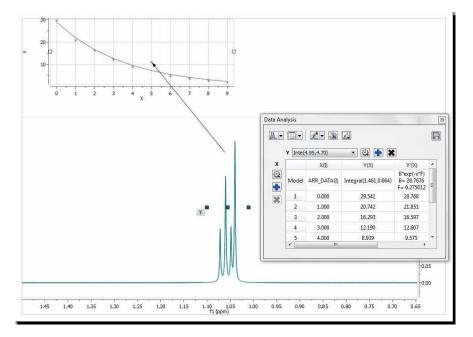

At this stage, there are several approaches. The simplest one is to just discard that point for the analysis, for example, by right clicking on that point in the graph and disabling it:

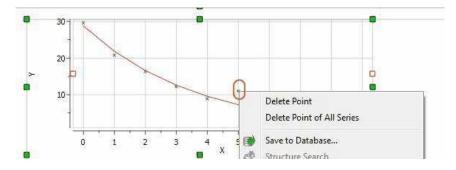

As soon as that point is deleted / disabled, Mnova will update the graph automatically. This is the new result:

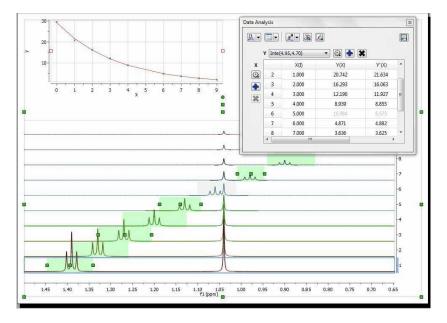

Another approach would involve using GSD to eliminate the singlet from the triplet so that it would not be necessary to discard the information from that particular spectrum.

Here you can watch a video about using Data Analysis for pKa calculation by NMR.

See this blog entry for the automatic peak tracking feature: http://mestrelab.com/blog/automatic-peak-tracking-in-arrayed-nmr-data/

#### 10.4.1.1 Data Analysis panel

The Data Analysis panel contains several options to create your graphs. You can import a .txt or .csv file (via File/Open dialog of Mnova) to fill the Data Analysis panel with X,Y values and generate the applicable graphical representation.

21-	Y Conct	(1.40, 1.33)		Properties selected co	
x		X(I)	YCO	Y'(X)	¥1 /
	Model	ARR_DATA(I)	Concentration(1.476624,1.413967)	B+F*exp(-x*G) B= 3.30766 F= 93.7625 G= 9.95856e-05	Concentration(1.
46	1	10	100	96.9768	3.75
	2	750	95.0064	90.3222	9.58
	3	1490	85,8131	84.1404	14.8
		2230	76.6458	78.3978	18.ć
rope	rties f	or rows	69.4157	73.0631	22.9
	6	3710	67.5465	68.1074	27.£
	7	4450	64,4336	63,5038	31.5
	<		M		>

You can select any graph from the scroll down menu below (and then a region of interest in the arrayed spectrum):

)	Empty (		R 🛃 🔛		
L	Concen	tration Graph	Y(X)	Y'(X)	*
1	Peaks Graph		ral(1.308841,1.079595)	B= 118.9/: F= 70079.8	
	Max. Pe	ak <mark>Grap</mark> h	58270.5	57864.9	
*	Max. Peak Pos. Graph		55222.2	54882	E
λ	Alignme	ent Shifts Graph	51945.7	51706.3	
E	Import		48593.9	48416.6	
	5	5.3873e+06	45080.6	45031.9	
	6	6.34088e+06	41629.3	41630.7	
	7	7.37704e+06	38249.7	38226.2	
	8	8.4863e+06	34926.2	34890.4	
	9	9.67886e+06	31585.4	31629.1	
	10	1.09438e+07	28502.1	28503.5	
	11	1.22928e+07	25507.6	25511.2	
	12	1.37201e+07	22678.8	22687.7	
	1	4.50407 07			2

If you select the Concentration Graph, a new dialog box will appear to ask you for the number of nuclides of the selected region

n Response Fac	8	ж
Number of Nuclides:	þ	<u>*</u>
$C(y,N,t) = \gamma^*M/(N)$	/*V) [	)
ОК	Cance	

Click on the 3 dots button to customize the formula:

Variable	Value	Description
v	100	Volume
w	255.65	Molecular Weight
м	7.3	Inital Amount
: Integral p Number o		<

The terms in the equation and table are as follows:

N=Number of nuclides

- W = molecular weight of chemical species (g/mole)
- M = initial amount, or mass


V = volume

So if M is in grams, and V is in litres, then the equation calculates concentration in Molar. (Obviously the user can introduce factors to convert this to mM or whatever is convenient).

With the 'Reaction Monitoring' plugin enabled you will be able to select 'PULCON' or 'Initial Concentration' modes:

Number of Nuclides: 1	Number of Nuclides: 1
PULCON 👻	Initial Concentration
Value: 1.000	Value: 1.000
Units: mM	Units: mM 🔻
OK Cancel	OK Cancel

NOTE: If the X column in Data Analysis is filled with zeros or you need to change the function, just double click on the model cell to derive t' not only from t but also from i-spectrum index:



From the same dialog (or by selecting 'Edit X Model'), you can also change the time units and setting the k and ARR\_DATA values:


ata Ana	lysis					đ×	
x	Y Inte(1.40,1.34)	•		×			
121	X(I)		Y(X)	X-Colu	ımn Func	? ×	
		(I) Integral(1	40235				
	Edit X Model Zoom Selection Use as Time Origin		63.2 V(D - APP DATA(D)				
			90.5	X(1) =	X(I) = ARR_DATA(I) Units: s		
New In			50.1	1			
	Use as Initial Conce	tration	11.8	k:	3600.0	000	
	Edit Dilution Compensation Edit Pulse Width Correction						
100.004			82.2 ARR_DATA = t/k			•	
	Eart raise what rec	arection	462.	_			
M	Use Fitting Limits		490.1 OK Cancel				
2º	Disable Points				11 85 T		
	0 1./ 32/4	i i i i i i i i i i i i i i i i i i i	10445.6		0		
	9 2.00274	0.00	11354.9		0		

Copy the values from an an Excel worksheet and paste them into the X(I) column by highlight the first cell (in the row 1) and doing 'Ctrl/Cmd+V' to paste the values.

Clicking on the Report scroll down menu, will paste the report or the table to your spectrum or to the clipboard:

	1	Report Report to Clipbo			
х		Report Table		Y'(X)	4
•	1000	Report Table to	Clipboard Integral(4.953175,4.696959)	B+F*exp(-x*G) B= -94.6772 F= 110204 G= 2.00294e-07	ш
*	1	2.34404e+06	68758.4	68817.5	
	2	2.98626e+06	60476.5	60499.6	
	3	3.70963e+06	52392.9	52326.6	
	4	4.50753e+06	44637.7	44584.1	
	5	5.3873e+06	37385.9	37365.7	
	6	6.34088e+06	30838.3	30852.7	
	7	7 37704e+06	25058 3	25052.6	
		m.		+	<u>.</u>

Clicking on the 'Interactive Y Filling' scroll down menu will allow you to select between different peaks selection modes (Peak Integrals, Concentrations, Intensities, or Maximum Peak Intensity, Alignment shifts or import YY' File), in order to generate the applicable plot.



Please note that you can also change those options by double clicking on the '...' button of the Model cell under the Y(X) header of the Data Analysis panel:


-	(4.95,4.70)	- 🙉 🛖 😹	V'(X)
Model	X(I) ARR_DATA(I)	Y(X) Integral(4.953175,4.696959)	V'(X) B+F*exp(-x B= -94.67 F= 11020 G= 2.00294
1	2.34404e+06	68758.4	68817.5
~	2.0962606	60476.5	2 50100 5
- Y-	Column Rule	And in case of the local division of the loc	
In	tegral(4.95,4.70)		ОК
I	ntegral	<b>•</b> ]	
	ntegral		Cancel

The 'Alignment shift' option will measure the change of chemical shift of the peak across the spectra, after having used the Alignment algorithm to align the peaks of interest.

Clicking on the 'Edit Model Options' button , will allow you to change some defaults, such as the capability to replace the active column (or to create a new one); number of handlers of the selected regions, the Fit function for the Y'-Filling column or use a 'Parabolic Interpolation for the 'Peak intensities'.

Y-Filling Policy	
Replace A	Active Column
🗸 Auto Adju	ist Regions
Number of Ha	andlers: 4
ric Function:	None
Fit Function:	Best Fit 👻
	Rost Eit
Peak Intensiti	
🔽 Parabolic	Mono-exponential Fit Three Parameter Exponential Fit
 f1 +/-:	Inverse Linear Fit

The 'auto adjust regions' option will automatically track the 'move' of the peaks/multiplets through the time course of a reaction.

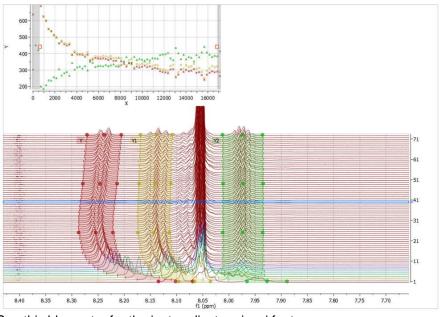


See this blog entry for the 'auto adjust regions' feature: http://mestrelab.com/blog/automatic-peak-tracking-in-arrayed-nmr-data/ In this panel; you will also find a button ("Reaction Monitoring") which contains all Show and Select options from Stacked Items table, and options to show/hide Stacked Spectra and Arrayed Data tables. The button is only visible when RM plugin is installed and licensed:


						E
¥ [	(1.40.1.24) -		View 🕨		Active Spectr	um
	(1.40,1.34) ▼ X(I)		Show Select	ACCOUNT.	Stacked Whitewash St	acked
Model		10 A	Stacked Spectra Table		Superimpose	d
1	10		2 12 224	×	Bitmap	
2	750	1	Arrayed Data Table	1	0.633412	
3	1490		0.894391		0.881752	
4	2230		1.12474		1.11448	
5	2970		1.33817		1.33259	
6	3710		1.53537		1.537	
7	4450		1.72298		1.72855	
8	5190		1.89733		1.90807	-

From the Data Analysis panel, you can select the region of interest of the Y axis or the properties for the rows and columns:

	<b>Y</b> Inte(4.95,4,70)		•] @		w			
x	Inte(4.95,4.70) Inte(1.33,1.09)		T	Experimental +	1	Visible	K)	
-			B+F*exp(-x*0	Fit 🕨		Edit	(-x*G)	
	Edit X Model Zoom Selection	3175,4.696959)	B= -94.6772 F= 110204 G= 2.00294e-07	Integral(1.325697,1.0	Label	G= 8.32	.122 57.5 339e-08	
	200m Selection	758.4	68817.5	58229.7		581	21	
	Use as Time Origin	476.5	60499.6	55185.5		5510	3.7	
	Use as Initial Concetration	392.9	52326.6	51912.2		5189	2.7	
	Edit Dilution Compensation	537.7	44584.1	48568.9 48568.1		8.1		
	Edit Pulse Width Correction	385.9	37365.7	45063.8		4514	19.5	

You can add additional curves to the representation by clicking on the 'Add New Data Serie' icon (of the 'Data Analysis' dialog box) and integrating (or applying any other analysis) the desired region of the spectrum:

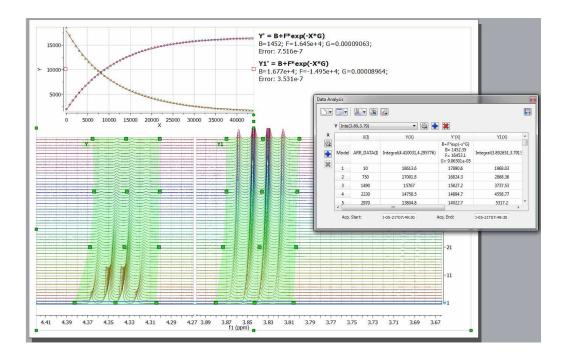



• Rows corresponding to spectra which have been removed from the dataset will be marked with **red** color in the Data Analysis table.

Right clicking on the Data Analysis Graphic, will allow you to update the graph after having made changes in the Stacked Items Table or directly on the stacked spectra (very useful, for example if you invert the order of the spectra). If you have more than one curve, you will be able to select/deselect available "series" (curves) on the plot.



Follow the menu 'Processing/Blind Regions/Add Blind Regions' to add <u>blind regions</u> to your arrayed experiment.

#### 10.4.1.2 Data Analysis Properties

Modify the properties of the graphic representation, just by double clicking on it to display the 'Properties dialog box' which contains three labels (Y/Y', Axes and Basic).

In the first label you will be able to change the style, color and width of the Experimental and Fitted lines

Y/Y' Y1/Y1'	Y2/Y2' Y3/Y	3,	
Z Experiment	ntal		
<u>S</u> tyle:	Line	•]	
<u>C</u> olor:	gree	n 👻	
Width:	3.00	Y	
Fitted			
<u>S</u> tyle:	Line	•	
<u>C</u> olor:	📕 gree	n 👻	
Width:	3.00	<b></b>	

Selecting the Axes label will allow you to change the color, font and margin of the axes and also to select the units scale (seconds, minutes, hours, points) and the capability to select Logarithmic values or to change the label of each axis:

Color:		
Line Width: MS Shell Dlg 2	2.5	
Margin:	1.27 mm	
Show Legend		
Horizontal Vertical		
V Label:	t(s)	
Units	s 🔹	
Max. Significant Digit		
Primary Tics: Secondary Tics:	✓ Auto         ▲           1         ★	
Logarithmic Scale		


Clicking on the Basic label will allow you to change the background, the grid and also to show the corresponding legend:

adata G	eometry	Graph		
Y7/Y7'	Y8/Y8'	Axes	Basic	
Backgroun	d			
Color:				•
Opacity:		0 %		A
Grid				
Show	Horizontal	Show	/ Over	
Show	Vertical	Shov	/ Frame	
Color:			ight gray	•
Line Widt	<b>1</b> '	2.5		4

# 10.4.1.3 T1 Analysis

Let's see how to use the Data Analysis feature to calculate the T1 value of a 1H-NMR dataset.

Firstly, load your dataset into Mnova and make sure that the phase is right (if not correct it by using the 'Manual Phase Correction tool):

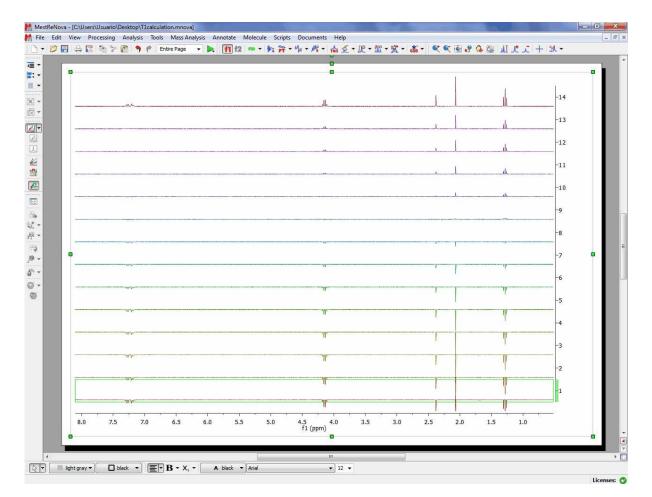


Follow the menu 'Advanced/Data Analysis/Create/Integrals Graph' and select the desired signal to analyze (i.e. the singlet at 2.38 ppm). You will notice how the graphical plot will be updated with the integral values:

dvanced Stack Mass Analysis	Predict Annotate Scripts Documents Help
Line Fitting	L + 5 9 11 11 12 40 2 10 20 1
Data Analysis	Create Find Create
Bayesian DOSY Transform	Import 🕅 Integrals Graph
Align Spectra	Export de Concentration Graph
Reference Alignment	Pick Peaks Graph
J-Correlator	Max. Peak Graph
Filter False Positives	Max. Peak Pos. Graph
	Reaction Monitoring 🕨 🚨 Alignment Shifts Graph
Arithmetic	Show Table

Finally double click on the Y'(X) cell, select the 'Three parameter exponential Fit' (**B+F\*exp(-x\*G)**) and click on the Calculate button

	Interact	ve Y Filling Options	Y-, Y'-Colu Active: Y				
	Rows		X(I)	Y(X)	Y'(X)		
3 4	5	Model AR	R_DATA(I)	Integral(2.29	4,2.428)		
	×	1	0.250	-54705.0	74		1
		2	0.300	-52173.3	28	-	
		3	0.500	-47078.6	99		
		4	0.800	-39973.5	12	- A	?
N: 1 Mono-expone	ime	Function	Initializati	ion Report	Descrip		Algorithm ^
2 Three parame		B*exp(-x*F) B+F*exp(-x*G)		71 1/6	Exponential Decay Exponential Decay		monoExpone +
2 Three parame	ter exponenti	b+r exp(-x G)	m	11= 1/0;	Exponential Decay	with paseline	monoexpone +

The T1 value will be the inverse of the G value, so in that case the T1 value for the proton at 2.38 ppm will be 4.87 seconds. Here you can see the result:

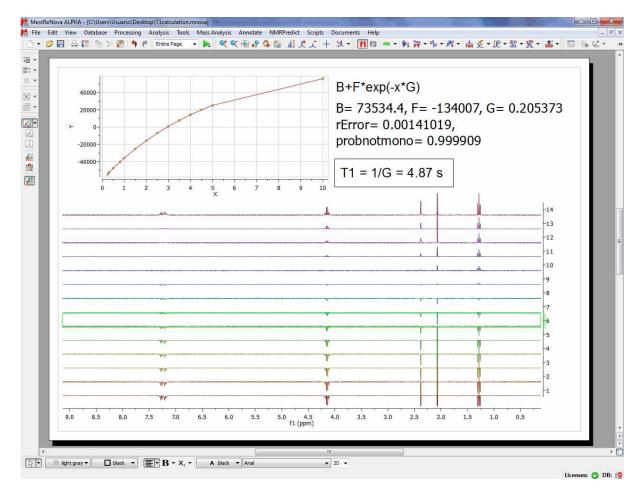

# 10.4.2 Reaction Monitoring (R-M)

You will need to install the RM plugin apart, by following the menu 'Edit/Advanced Plugins' and clicking on the 'blue plus' button or just by dragging&dropping the XML file in Mnova

Many experiments require obtaining a series of FIDs, related to each other through the variation of one or more parameters.

For example, in a kinetics or reaction monitoring (R-M) experiment, a series of spectra are recorded at predetermined time intervals to follow the progress of the reaction.

There are two ways to acquire these kind of experiments:

- · Acquiring all spectra at different times and storing those individual spectra
- Instead of acquiring separate data sets, it is very common to keep all acquired spectra into a single NMR experiment, the so-called **Arrayed mode**

In general, arrayed mode is the most commonly used, although sometimes, acquiring the spectra as individual spectra can offer more flexibility. Of course, **Mnova supports both modes**.


See this video for further information and also this post

#### 10.4.2.1 Importing Datasets


#### Importing of R-M data sets acquired in arrayed mode

If your dataset has been acquired in arrayed mode, it will be enough to drag&drop the FID (Varian) or SER file (Bruker) to Mnova.

Mnova supports, in addition to Reaction Monitoring, Relaxation (T1/T2) and PFG (DOSY) experiments (in other words, it will parse the arrayed parameter automatically).

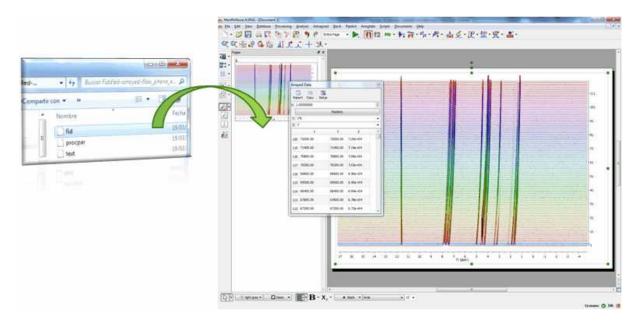


In either case, Mnova will automatically read the values of the arrayed parameter, e.g. time stamp and populate the corresponding arrayed data table

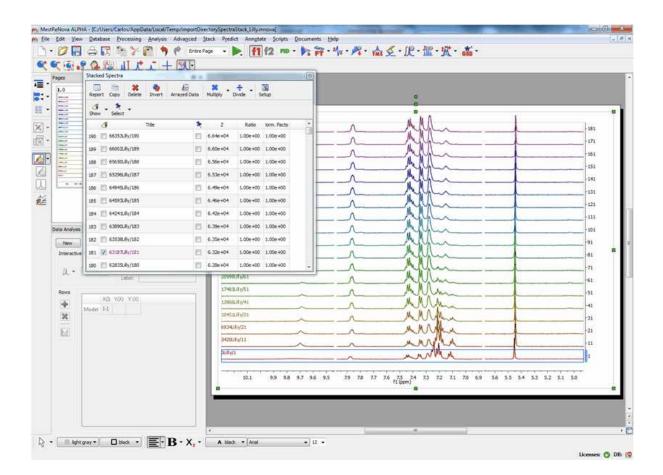

#### Importing of R-M data sets acquired on individual basis

Mnova includes a powerful script which makes it possible to import all spectra contained in a folder and automatically stack them for forthcoming R-M analysis. This script is under the Scripts menu and it is called 'Directory Spectra Stack'. It will allow the user to select the directory where the spectra are contained. Then Mnova will open and process all those spectra (FIDs) automatically in bunches of 20 spectra and finally will stack all of them.

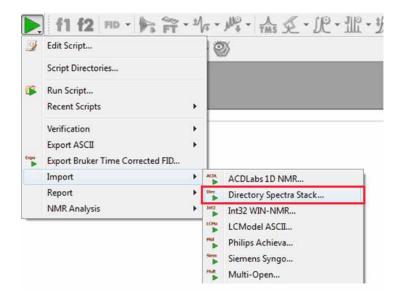

Note: This script has also the option to decimate the spectra while loading (i.e. the program can skip every 10 spectra in the data set) and to apply a processing template (or to load the 1r processed data):

import Sp	ectra Stack		2	CAD
Data Folder:	\rxnMon - neat-a	cetylacetone-42 2016-02-04	1 0442PM	1 [
Order:	By Name			3
File Path Fi	ltering			
File Name	Masks:	fid *.fid *.jdx		
Folder Nan	ne Masks:			•
		Preview Files		
Spectra	l Data Filtering			
Parameter		=		
Chunkin	g			
First Spect	rum: 1	Number of Chunks:	1	* ¥
Chunk Size	: 96	Step to Next Chunk:	97	×
Visualizatio	n			
View:	Kacked	Decimation Step:	10	*
Process	ing Template			
File:				
Backup				
Folder: C	/Users/Usuario/A	ppData/Local/Temp		
		ОК	Can	cel

# Reaction Monitoring Wizard 📒

This wizard is a simple way to quickly get Reaction Monitoring data into Mnova and analyse it. It will allow you the save and recall procedures in the future.

Line Fitting	トトロ・ヤ・ジャラ
Data Analysis	2.1.1.0.1.1.2.1.3
Reaction Monitoring	🖐 Use as Time Origin
Bayesian DOSY Transform	🐘 Use as Initial Concetration
Align Spectra	Edit Dilution Compensation
Reference Alignment	Mar Bedit Pulse Width Correction
PCA	🔝 Listener
J-Correlator	🚈 Wizard
Filter Falce Docitiver	

In the screenshot below you can see how to select the directory of your dataset, to sort the spectra by name or date, to display them in stack or superimposed mode and to use decimation.

Import	
Set the Import Options	
Import Directory:	C:\Users\Usuario\Desktop\test
Sorting:	By Name
Default View:	Kacked
Import Decimation:	1
Visual Decimation:	1
Nucleus:	[1H
Backup Directory:	C:/Users/Usuario/AppData/Local/Temp

You can also 'Save or Load Settings' from this dialog box. Clicking on the 'Next' button will display the dialog below:

Processing				
Select the Desired Processing O Default Mnova Processing				
Processing Template:	]	C:/Users/Usua	ario/Desktop/te	est/ProcTemplate.m
Advanced Processing:		// Custom Set	up Processing F	Function

This new window will allow you to apply <u>'processing templates'</u> to your datasets. Clicking on the 'Next' button will display the 'Extraction' dialog:

Extraction				
Spectrum Regions				
Select Graphically and Press New	ct	∬_ Integ	grals	
Use Last Selection		Contraction of Contra	centrations grals	
Import from File:		LUC Inte	yr ais	
Zero Time Index:	0	A		
Tip: Keep Pressed Space to Pan and	Ctrl+Space	to Zoom		

From the dialog above, you will be able to select graphically the regions (with concentrations or integrals), import a XML file with the regions of interest or use the latest selection. From here you can also select the Zero Time Index. Clicking on the 'Next' button will display the 'Fit Options' dialog:

Fit Options	
Select the Equation To Fit	
🔘 No Fit	
🔘 Use Last	
Select By Reaction Order	First Order
Import From File	Zero Order First Order
🔘 Fit To Best	Second Orden

Finally, click on the Next button to display the Report dialog box which will allow you to save the document in Mnova or PDF format:

Report	eaction Monito		-	-	-	
Select Report (	Ontions					
Text Report	- Franker					
🗹 Add Rep	ort					
Save						
🔽 Mnova	C:/Users/Usuari	o/Desktop/t	est mnova			

See also this video

**Reaction Monitoring Listener**: The listener will automatically import, stack and save any dataset that arrive to the selected folder

mport					
et the Import Op Directory:	C:/Users/	leuario			
Default View:					,
Max. Number o	f Spectra:	-1	*		
Max. Time:		60 min			
Log File:					
Save:					
Final Command					

You can use a final command to get whatever you want. For example, to receive an email when the listener stops completely, because all the conditions has reached. You can define a final command when an specific condition has reached (but not necessary all of them).


In the example below, we have used the application 'blat exe' to send an email when a condition in a serie has reached. The initial concentration was 5 mM. After the condition is reached (when concentration is lower than 4), the listener stops, shows a message of "Warning" and an email is sent. (the final command used was:

c:\temp\blat.exe -body "Condition reached" -to support@mestrelab.com -u guest@mestrec.com -pw \*\*\*\*\*\* -subject "Automatic message from RM Listener")


🖌 Reaction Monitori	na Listener	1.1	8 23	Label: Mode:	Product	ration		
		5.0	<u></u>	From:	0.500	To:	1,500	
Product (0.5,1.5), B+	F*exp(-x*G)		*	Number of Nu	udides:		1	4
Response Factor     Init Concentration:     Due contraction:	5.00			Equation: F		•		8134-012
	5.00         *           1.00         *           1.00         *					• :3.423678937042	3535e-308,"comm	ients":""]
<ul> <li>Init Concentration:</li> <li>PULCON:</li> </ul>	1,00	params":{"V":100,"W":2	55.65, "M": 7.3}}			• :3.423678937042	13535e-308, "comm	ients":"")
<ul> <li>Init Concentration:</li> <li>PULCON:</li> <li>Internal Reference:</li> </ul>	1.00 ÷	params":{"V":100,"W":2	55.65, <sup>*</sup> M*:7.3}}	a":"B+F*exp		▼ .3.423678937042	:3535e-308, "comm	ents":""]
<ul> <li>Init Concentration:</li> <li>PULCON:</li> <li>Internal Reference:</li> <li>Formula:</li> </ul>	1.00 ↔ 1.00 ↔ ("formula":"γ™/(W™/)"," mM	params": {"V": 100, "W": 2	55.65, 'M':7.3}}	a": "B+F*exp Trigger Condition: Message:	(-x*G)", "error Y < 4 Warning	• ::3,423678937042 ubject "Automatic m		

#### 10.4.2.2 Selecting Regions

Once you have imported your datasets, you can select the 'Reaction Monitoring' regions of interest by following the menu 'Advanced/Data Analysis/Create Concentration Graph' to select the desired regions:

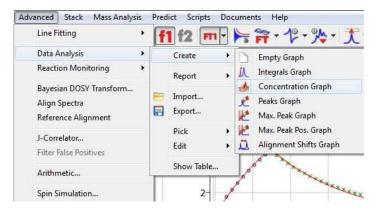

Once you have selected the first region in your stacked plot, you will be asked to type the number of nuclides and concentration value. Once you have typed the values, the Data Analysis panel will be filled.

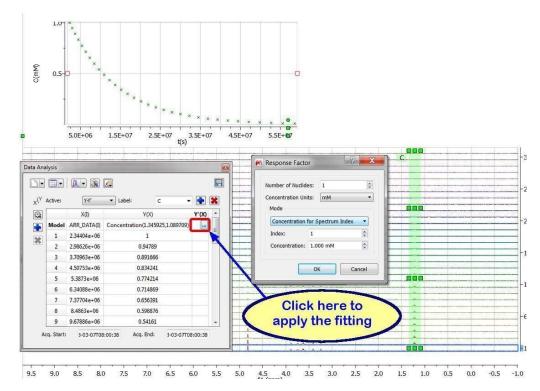


You can select different modes: Concentration for spectrum Index (by area of peak of the selected spectrum in the array), Concentration Conversion factor (CCF), Internal Reference (to include a reference compound of constant, known concentration) or to use a Formula:

Number of Nuclides:	1	A V
Concentration Units:	mM	•
Concentration for S	The set of	
Provide a state of the second s	Spectrum Index version Factor	
Internal Reference		


Next click on the '3 dots' button of the Y'(x) column to select the desired fitting (Mono-Exponential in the picture below). Next, click on the 'Calculate' button to generate the parameters of the fitting and finally click on the OK button to draw the fitting curve.

	0.5-0						a			
	alysis	5.0E+06	t(s)	3.5E+07	4.5E+07		FF 67	C		? ×
] .					_	Functions	25.00			
NY.	Active:	Y-Y	▼ Label: C	-			Name	Function	Initialization Re	1
		X(I)	Y(X)	Y'(X)			1 Linear Fit	A+B*x	A= 0, B= 0	Zero Order Rea
	Model	ARR_DATA(I)	Concentration(1.345925,1.089709)	B*exp(-x*F) B= 1.21044 F= 8.2637e-08	E		2 Mono-exponential Fit 3 Three Parameter Exponential Fit 4 Inverse Linear Fit	B*exp(-x*F) B+F*exp(-x*G) 1/(A+B*x)	A= 1, B= 0	Exponential De Exponential De Second Order f
1		2.34404e+06	1	0.997287			4 Inverse Linear Fit	I/ (ATD XJ	- 1, D= V	Second Order I
*	1		0.94789	0.945739			<u>×</u>			
1	1 2	2.98626e+06					۰ III			
1		2.98626e+06 3.70963e+06	0.891666	0.890862						
1	2		0.891666 0.834241	0.890862			Restore Defaults			
1	2 3	3.70963e+06								
1	2 3 4	3.70963e+06 4.50753e+06	0.834241	0.834017			Restore Defaults Fitted Parameters			
1	2 3 4 5	3.70963e+06 4.50753e+06 5.3873e+06	0.834241 0.774214	0.834017 0.775534						
1	2 3 4 5 6	3.70963e+06 4.50753e+06 5.3873e+06 6.34088e+06	0.834241 0.774214 0.714869	0.834017 0.775534 0.716768			Fitted Parameters			


Follow the menu ' Advanced/Data Analysis/Edit/Fit to Best' and Mnova will try to guess the order of the reaction; fitting the data to standard equations and comparing the mean square error:

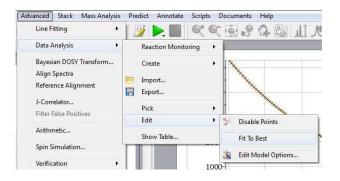

With the *Reaction Monitoring* plugin enabled, if you right click on any point of the Data Analysis Graph (or Table), you will be allowed to 'use that point as time origin or as 'Initial Concentration', or to set the Dilution Compensation Parameters' and 'Pulse Width Correction':

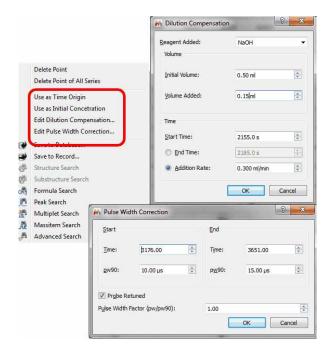


#### Here you can see an example following an enzymatic reaction:

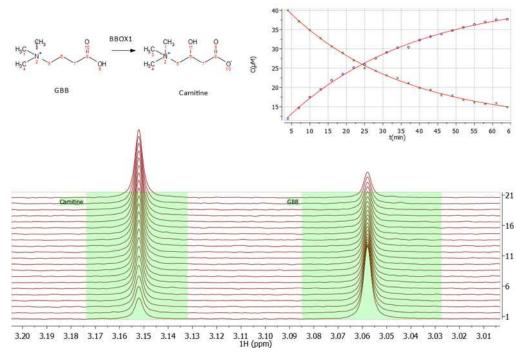

Data courtesy of Tim Claridge, Oxford

and here an ester hydrolysis:

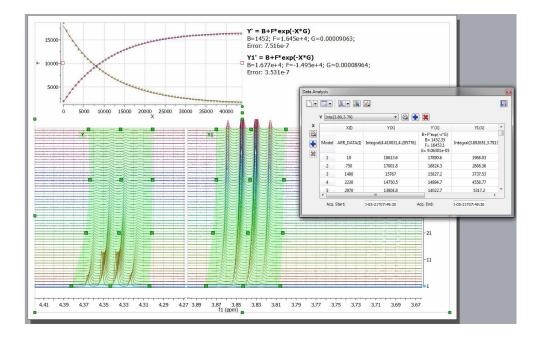

#### 10.4.2.3 Practical Example


This tutorial will show you how to use the Reaction Monitoring plugin for your spectra.

You will need to import your dataset into Mnova just by dragging and dropping the stacked spectra (if it has been acquired in arrayed mode) o by using the Reaction Monitoring Wizard (Advanced/Reaction Monitoring/Wizard) if the datasets have been acquired on individual basis (you can also use the Scripts/Import/Directory spectra Stack).

In this tutorial we will use the RM Wizard. You can download the dataset from this link.

Import			
Set the Import Options			
Import Directory:	E: \data\Reaction Monitoring \AZ\Ac2Ohydrolysis1in4		
Sorting:	By Name		
121			
Default View:	🔀 Stacked 👻		
Import Decimation:	1		
Visual Decimation:	1		
Nucleus:	1H 💌		
Backup Directory:	C:/Users/Mike/AppData/Local/Temp		
	Save Settings Load Settings Next Cancel	Ļ	
	Save Settings Load Settings Next Cancel	Date modified	Туре
		Date modified	
	Name		File fo
	Name 2	11/02/2013 12:03	File fo
	Name 2 6	11/02/2013 12:03 11/02/2013 12:03	Type File fo File fo File fo

Once Mnova has loaded all the individual spectra, it will show you the stacked plot. Zoom in (by using 'Ctrl+Space' (or Space+Cmd) to activate the zoom in mode temporarily) the spectral region of interest

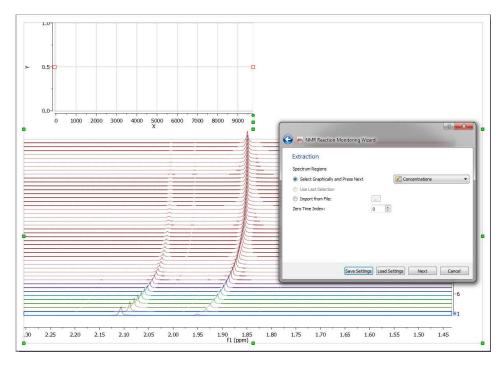


and select graphically the signals that you want to analyze


Once we have selected the first region (signal at around 2.10 ppm), a dialog box will be displayed to enter the 'response factor' values:

Number of Nuclides	6	4
Concentration Unit	s: mM	÷
Mode		
Initial Concentra	ation	•
Index:	2	A. 
Concentration:	10.000 mM	×


Clicking on OK, the graphic will appear on your spectral page and the 'Data Analysis' panel will be displayed:

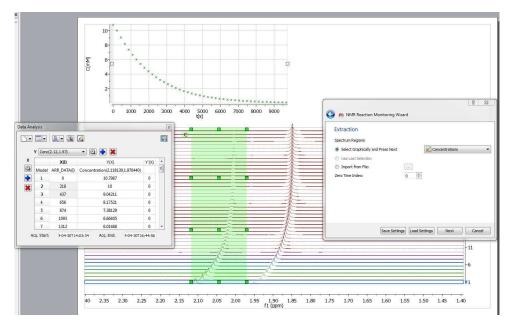

The next step will be to select the second region of interest (around 1.90 ppm) and the number of nuclides (6):

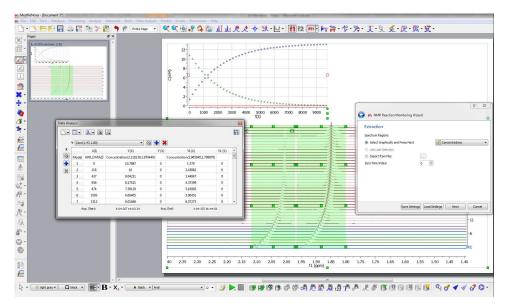

We can use the green square handlers to adjust the regions of interest with the deviation of the signals in the stacked (you could also use the 'Align Spectra' feature)

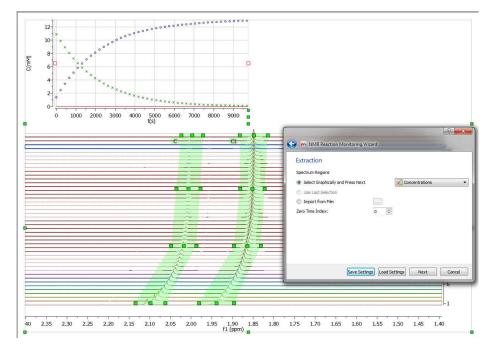


Clicking on the 'Next' button of the RM Wizard will allow us to select the equation for the fitting (or to ask to Mnova to search for the Best Fitting):

Fit Options		
Select the Equation To Fit		
🔘 No Fit		
🕐 Use Last		
Select By Reaction Order	First Order	3
Import From File		
Fit To Best		

Clicking on the 'Next' button again, we will be allowed to paste the report into the Mnova document and to save the result in Mnova and PDF documents:

Report Select Report	Ontions
Text Report	
Add Rep	port
Save	
Mnova	C:/Users/Usuario/Desktop/Test_RM.mnova
	C:/Users/Usuario/Desktop/Test_RM.pdf


Clicking on the 'Finish' button, will do the job. You can 'save the settings' to be used in the future with similar datasets.

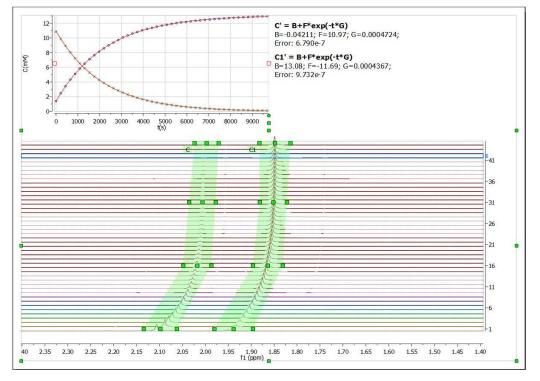

# **10.5** Reference Alignment

This feature will be used to manually align the chemical shift of 1D or 2D spectra (very helpful in Metabonomics), that is, to correlate signals of 1D or 2D spectra.

Just select, in the page navigator, the spectra that you want to align and follow the menu 'Advanced/Reference Alignment'. All the spectra will be aligned with the first one.



You can also use this feature to align stacked spectra. In that case, the method uses the active one and then aligns all remaining spectra by maximizing the cross-correlation between the reference spectrum and the spectra to be aligned:



The idea of global alignment is very simple and corresponds to the well-known chemical shift referencing method in which the user sets the internal reference peak (e.g. TMS, DSS, TSP, etc) of each spectrum to e.g. 0 ppm. In order to cope with small fluctuations in chemical shifts, this method seeks for the highest peak within a narrow (user-defined, auto-tuning option in Mnova) interval, as depicted in the figure above.


See also Align Spectra.

# 10.6 Align Spectra


The **chemical shift** is of great importance for NMR spectroscopy because it reflects the chemical environment of the nuclides under observation providing detailed information about the structure of a molecule.

Although the chemical shift of a nucleus in a molecule is generally assumed to be fairly stable, there are a number of experimental factors (pH, salt concentration, solvent, field inhomogeneity –bad shimming, etc) which might produce slight or even quite significant variations in chemical shifts.

This is particularly important in **metabonomics/metabolomics** NMR where shifts of NMR peaks due to differences in pH and other physico-chemical interactions are quite common in NMR spectra of biological samples. For example, some important metabolites, such as citrate or taurine, have peaks whose chemical shifts fluctuate in an uncontrolled way from sample to sample. These variations can cause spurious grouping of samples in chemometric models.

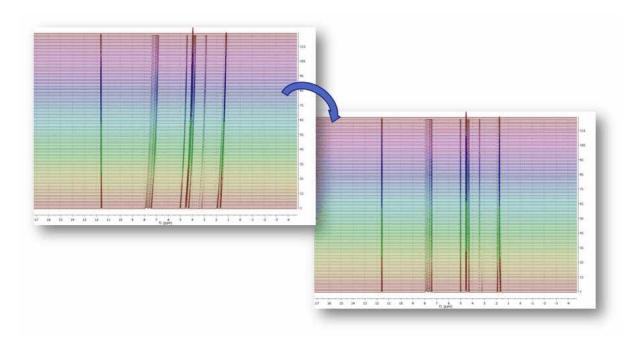

This problem is also very common in **kinetics** or **reaction monitoring** experiments by NMR. For example, consider the following reaction monitoring example:

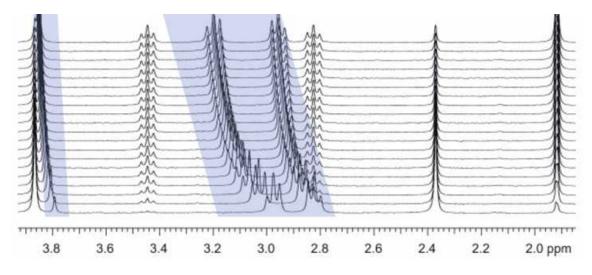

It can be appreciated that during the course of the reaction, the chemical shifts of highlighted signals change as a result of the change in pH (in this case, as a hydrolysis proceeds).

Although characterizing these chemical shifts fluctuations can be sometimes important (pH or drug binding-induced chemical shifts, for example) in general they obscure the process of pattern recognition and impede the performance of data analysis (e.g. selection of the peaks whose intensities/heights need to be monitored can be more difficult).

Whilst it is critical to setup the experimental conditions in the best way to minimize these chemical shift fluctuations (for example by using an appropriate buffer); spectral misalignments may still occur and special post-processing methods have to be employed.

In order to cope with this misalignment issue, Mnova includes several methods, namely:

- Manual (semi-automatic) global spectral referencing
- Fully automatic global spectral referencing
- Spectral alignment (including global and regional-wise spectral alignment)

The first two methods can be regarded as simple, global methods for peak alignment as they shift the entire spectrum by some constant amount, whilst the third method is much more sophisticated making possible both the global and local alignment of different spectral regions

These three methods are explained below:


#### 1) Manual (semi-automatic) spectral referencing

This method corresponds to the well-known chemical shift referencing method in which the user sets the internal reference peak (e.g. TMS, DSS, TSP etc) of each spectrum to e.g. 0 ppm. The particularity of Mnova is that it contains an **auto-tuning** parameter which makes it possible the automatic referencing of many spectra by simply seeking for the highest peak within a narrow (user-defined) interval.


The figure below (left) shows 26 superimposed misaligned peaks. <u>Manual Referencing</u> using an auto-tune parameter of 0.1 ppm yields the result depicted in the figure on the right:


Reference along f1	? <u>×</u>	100 900 800
New Shift: 0.000 ppm	Auto Tuning	700 600 400 300 300 200
Annotation OK Can	cel Solvents >>	100 10 20 30
		-36

Clearly, this method will not work properly in those data sets with local misalignments, that is, when signals of one metabolite fluctuates in one direction whilst the peaks of a different metabolite move differently). As an example, let's consider a simulated data set of Taurine:

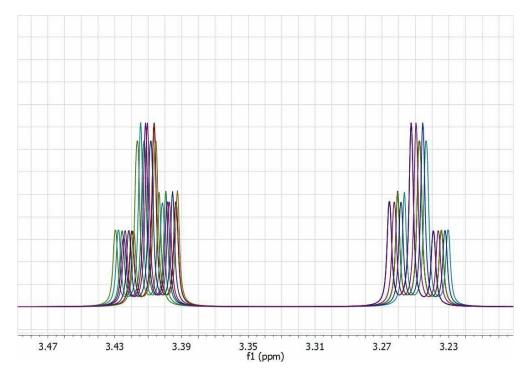

This data set has been generated by randomly changing the chemical shifts of the two CH2 groups. Now, let's apply the global alignment procedure using as chemical shift reference at a value of 3.25 ppm as shown in the picture below:

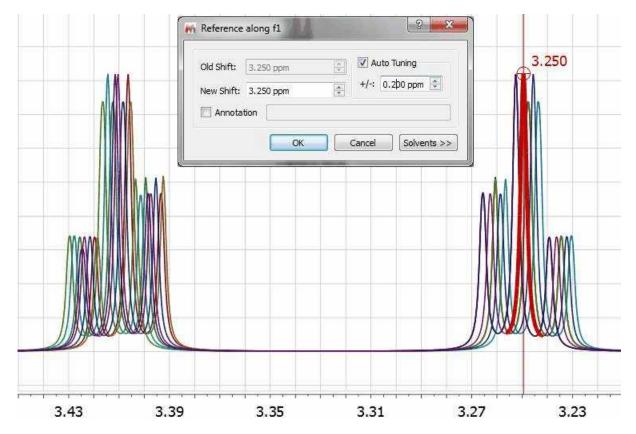

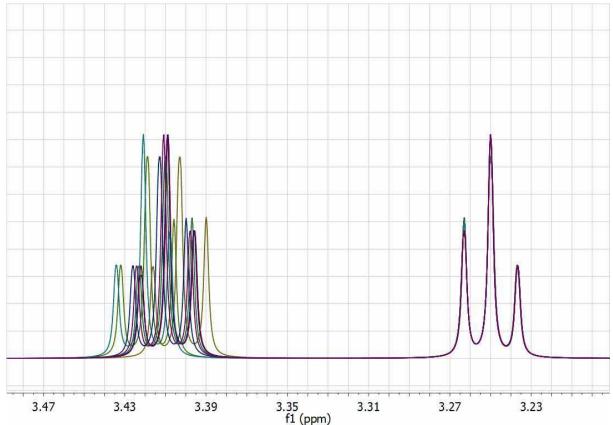


As expected, all peaks corresponding to the triplet at 3.25 get perfectly aligned, but the other multiplet remains misaligned:

One could devise an extension to this global alignment procedure in which the same procedure is applied to different segments of the spectrum. In this particular case, one could select two different windows, one for each triplet and apply the same algorithm locally to each segment. However, having to manually select the chemical shift reference for each segment is not very practical and, in addition, relying only on the simple search of the maximum peak within each segment is not a very robust method for automatic alignment.

#### 2) Fully automatic global spectral referencing

In the previous method, the user needs to select a peak as a reference for the alignment process, together with the window width for the auto-tuning parameter.

Mnova provides an alternative, fully automatic method which <u>aligns</u>, **globally**, all spectra in a stack. This method uses one spectrum as a reference (the active spectrum) and then aligns all remaining spectra by maximizing the cross-correlation between the reference spectrum and the spectra to be aligned:

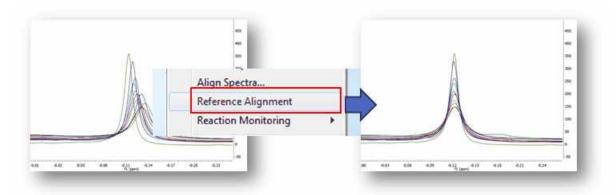


### 3) Spectral alignment (including global and regional-wise spectral alignment)


The magnitude of <u>misalignments</u> within a single sample may be <u>nonlinear</u>, making it challenging to apply a simple alignment correction across an entire spectrum.

An example of this nonlinear misalignment is shown in the spectrum below (intensity map or bitmap plotting mode). It can be noticed that the peaks at about ca 11.6 ppm do not move whilst the peaks at higher field move very significantly.

It's evident that correcting the data using a single reference peak (or a global shift) is not sufficient:

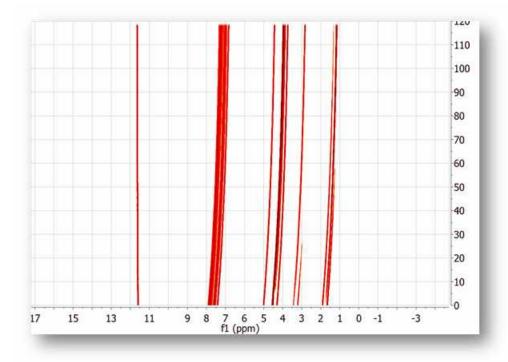

Resorting back to the synthetic data set used in the previous section, let's see a semi-automatic method designed specifically to align spectra having local chemical shift variations. From a practical point of view, the user needs to select the spectral regions to be aligned and then the program will automatically align those regions separately The picture below shows the spectrum before alignment and the two selected regions (top) and the result obtained after applying the alignment algorithm (bottom):

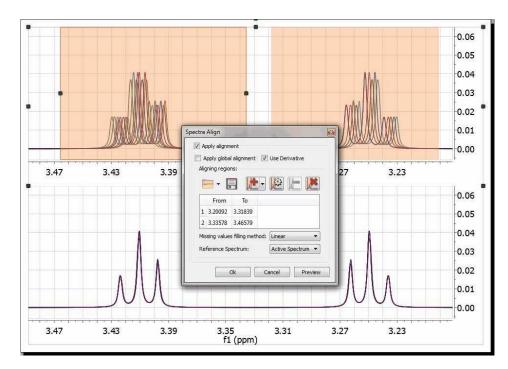

Mnova provides a powerful and flexible approach to dealing with misalignments based on a segment-wise peak alignment with the option to apply a global alignment as a pre-processing stage. The algorithm allows the user to select the boundary locations using an interactive display, but the process is also amenable to automation.


1000		l alignment	VL	lse Deriv	in the unit
Align				Se Den	auve
	ning region	ns:			
P	9 - 6		-	3	
	From	То			
1	3.20092	3.31839			
2	3.33578	3.46579			
Miss	ing value:	s filling meth	nod: []	inear	*
Refe	erence Sp	ectrum:	6	Active Sr	oectrum 🔻
1020	100000		6		1000

Use the applicable buttons to load and save alignment regions in XML format.

We have improved the traditional cross-correlation algorithm by working on the first **derivative** domain calculated using an improved Savtizky-Golay routine in which the order of the smoothing polynomial is automatically calculated. The idea is to minimize potential problems caused by baseline distortions or very broad peaks.

We have found this method to be very useful not only in the context of metabonomics, but also in the alignment of Reaction Monitoring data sets.


This comprehensive spectral alignment toolkit is available in Mnova in the Advance menu. It can work on the entire spectrum (Global Alignment) as well as on intervals of arbitrary length in sequence. Based on these options, different strategies can be employed.



Two examples (strategies) will be shown below:

#### Strategy 1

Starting with raw spectrum (1), to perform a full-spectrum correction before the single intervals are aligned

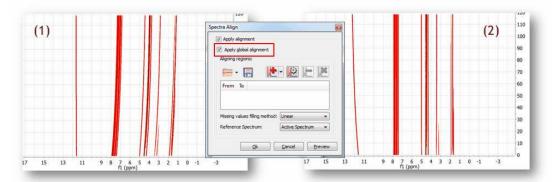

It can be appreciated that after applying the global alignment, most of the peaks in (2) are now properly aligned, except the peaks at the left which were previously aligned but after this operation get misaligned. This problem will be cured in the next step.

#### Strategy 2

A different, although analogous strategy, would consist in aligning two different spectral intervals separately without resorting to a global alignment as shown in (1). Note that the peaks in the interval in the left are already well aligned.

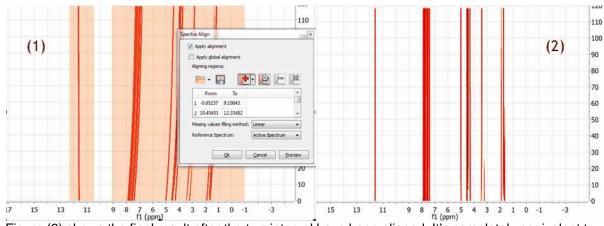


Figure (2) shows the final result after the two interval have been aligned. It's completely equivalent to the result obtained with Strategy 1

#### See also our blog

# 10.7 PCA

Principal Component Analysis (PCA) is a procedure which uses orthogonal transformation to convert a set of observations from correlated variables into a set of values of linearly uncorrelated variables (named principal components).

You can use Mnova for your PCA studies. You will only need to load your stacked spectra and follow the menu 'Advanced/Chemometrics/Data Processing'. That will display the 'Data Preparation' dialog box:

riginal Data		
Data	Processing	
Spectrum Class	Data Cleaning	
Bin	Data Integrity Check	
Bin Tag	Eilter	Standard deviation 👻 10.00 % 🎄
	Normalization	
	(@) Sum	
	O Median	
	C Reference Spectrum	No reference
	Reference Bin	0.000 ppm
	Scaling	
	Only Centering	
	Auto	
	🔘 Range	
	🔘 Pareto	
	🔘 Vast	
	🗇 Level	
		Process
	e e	

**Data Cleaning**: two options are available which could be used simultaneously.

- a. *Data Integrity Check* replaces negative bin values (negative integrals) with zeros.
- b. <u>Filter</u>. Filtering methods are used to remove bins that are null and do not displays any changes among spectra series. By default if a variable (bin) shows zeros among all rows (spectra) it is discarded. Five options are possible. In the first three options Standard Deviation, MAD and IQR a fixed fraction (default 10%) of the bins is discarded (e.g. if the matrix is composed by 100 bins it means that 10 bins are discarded, and the selection is based on the Filter method chosen). In practice Standard Deviation, Median Absolute Deviation and Interquartile Range are calculated for all bins. Furthermore an amount of bins (with the lowest SD, or MAD or IQR values) are discarded with respect a percentage value of the total bins.

In the case of Mean Value or Median Value, user is asked to input a value for the Mean or the Median. By doing, so only bins that display a lower value of the inputted one are discarded.

**Normalization**: it is an operation that is performed on the rows of the matrix. Four possible strategies could be selected:

- c. <u>Sum</u>: every element on a raw is divided by the sum of all elements of the same raw;
- d. <u>Median</u>: every element on a raw is reduced by the median value of all the bins that constitute the same raw;
- e. <u>Reference Spectrum (or reference series of spectra)</u>: upon normalization by the sum, every element of a raw is divided by the corresponding element of the raw of the selected reference spectrum (e.g. when you have a reference spectrum and you wish to compare all the other spectra relative to it). If you select a bundle of spectra (like all spectra belonging to the same class) normalization is performed on the calculated average spectrum.
- f. <u>Reference Bin</u>: user inputs chemical shift value (in ppm) of a reference peak of interest and automatically MNova identify the bin that comprises the selected peak. Furthermore every components of a raw are divided by the reference component of the corresponding raw.

**Scaling:** it is an operation that is performed on the columns of the matrix. Five different methods are implemented: Autoscaling, Range, Pareto, Vast and Level scaling. Mathematical operations applied are the follows:

Autoscaling	$\tilde{x}_{ij} = \frac{x_{ij} - \overline{x}_i}{s_i}$	Where $\overline{x}_i$ is the mean, $s_i$ is the standard deviation and $\tilde{x}$ represent data after scaling.
Range Scaling	$\tilde{x}_{ij} = \frac{x_{ij} - \overline{x}_i}{x_{i_{max}} - x_{i_{min}}}$	$\overline{x}_i = \frac{1}{J} \sum_{j=1}^{J} x_{ij}$
Pareto Scaling	$\widetilde{x}_{ij} = \frac{x_{ij} - \overline{x}_i}{\sqrt{s_i}}$	$s_i = \sqrt{\frac{\sum_{j=1}^J (x_{ij} - \overline{x}_i)^2}{J - 1}}$
Vast Scaling	$\widetilde{x}_{ij} = \frac{x_{ij} - \overline{x}_i}{s_i} \cdot \frac{\overline{x}_i}{s_i}$	
Level Scaling	$\widetilde{x}_{ij} = \frac{x_{ij} - \overline{x}_i}{\overline{x}_i}$	

For further information about the different scaling methods, please visit this link.

The next step would be to select 'New from from spectrum' (or 'new from file' if you have any saved 'preparation file' from other experiment):

rigina	al Data	
Data		
1		
M	New from spectrum	
	New from file	
Rin	Tag	

A new dialog will appear to select the <u>binning</u> options:

Bin width:	0.0\$0000 € ppm ▼
Method:	Average Sum 👻
) Regions	


There are four binning methods are available: Sum, Average Sum, Center and Peak. The 'Sum' method will sum all the points of a bucket, the 'Average Sum' will divide the sum by the number of points in the bin, the 'Center' method will only return the value found in the middle of the bin. For example if a bin has 5 points it will return the value for 3rd point. The 'Peaks' method will perform firstly the GSD (Global Spectral Deconvolution) and then will apply binning over the peak table. For large dataset (more than 50 stacked spectra, it advisable to perform GSD before executing PCA module).

Clicking on the 'Regions' radio button; will allow you to load any existing 'MestReNova Integral Regions file' (which you can obtain from any integrated spectrum and following the menu "File/Save As/ MestReNova Integral Regions (\*.txt)")


After having clicked on 'Process' button, you will get a new dialog summarizing the processing and allowing you to save the 'Data preparation file' or the 'Processing' file to be used in the future:

	2016-06-03T10:12:45						
ata					Processing		
-							
	Spectrum	Class	1		A Binning		
Bin			(-1.28924, -1.25924)	(-1 25924	Method	Average Sum	
			(-1.20524, -1.25524)	(-1.23524,	Bin width	0.03 ppm	
Bin Tag					Data integrity che	eck true	
	a_group/A2				Filtering		
	A2 polare	Α	1.31004	2.06	<ul> <li>Normalization</li> </ul>		
	7C_noesypr H2O+D2O /opt/topspin Metabolomic 2				Method	Sum	
	a_group/A6				<ul> <li>Scaling</li> </ul>		
2	A6 polare 7C_noesypr H2O+D2O /opt/topspin Metabolomic 6	A	1.12881	1.25	Method	Auto	
	a_group/A8						
3	A8 polare	A	0.541955	1.59			
	7C_noesypr H2O+D2O /opt/topspin Metabolomic 8						
	a_group/A12						
1	A12 polare	Α	0.840557	1.24			
	7C_noesypr H2O+D2O /opt/topspin Metabolomic 12						
	a_group/a3						
5	A3 polare 7C_noesypr H2O+D2O /opt/topspin Metabolomic 3	A	0.990225	1.59			
	/C_noesypr H2O+D2O /opt/topspin Metabolomic 3 b_group/B3						
5	B3 polar	в	-1.59915	-0.73			
	7C_noesypr meta /opt/topspin Metabolomic 3	3	1.53513	0.73			
	b group/b2			-			
				4			

Finally, click on the 'PCA button' to select the number of principal components (and to change the title):

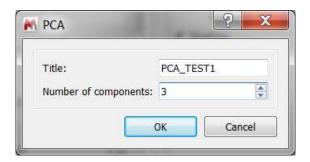

After having clicked on the 'OK' button; the 'PCA results panel' will be displayed. Right clicking (or Ctrl/Cmd+C) on any of the plots, will allow you to copy to clipboard:

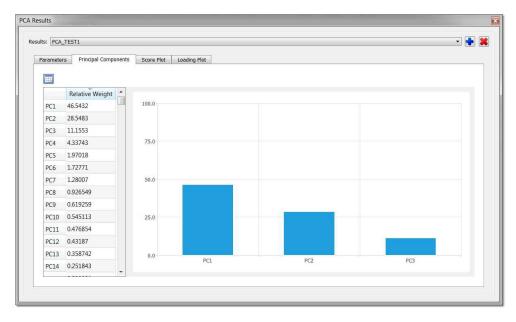


Clicking on the 'Show Table' button, will hide/display the applicable table with the relative weight for each component:

Right clicking on any table will allow you to copy to clipboard or to save as CSV:


	Relative Weigh		
PC1	98.5552	100.0	
PC2	1.30762	100.0	
PC3	0.0579155	75.0	
PC4	0.0286905		
PC5	0.024 Copy	50.0	
PC6	0.008 🛃 Save Table		
PC7	0.00605692	25.0	
PC8	0.00373003	0.0	
PC9	0.00296346	PC	1

Clicking on the 'header' of the column will sort the results in ascending/descending order.

Selecting the 'Score Plot' tab will display a window like this:

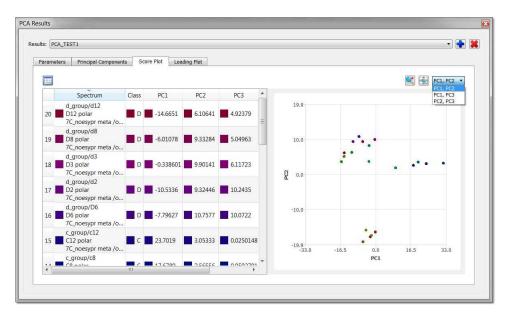


Each point of the 'Score Plot' is associated to a trace of the stack. If you are in the 'Active Spectrum' mode, you will get displayed the applicable spectrum when clicking on the point (of the Score Plot):

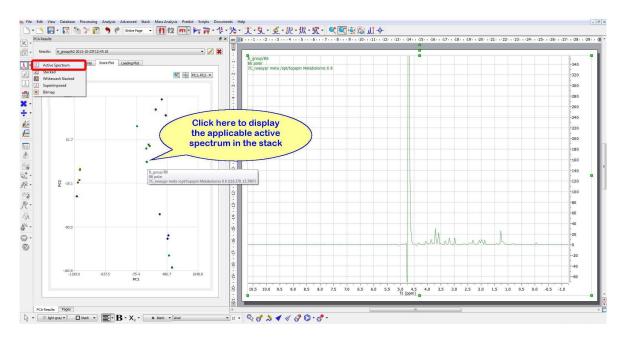


You can 'zoom in' and 'reset zoom' by using the applicable buttons. Use the combobox to switch between different PC comparisons:



Clicking on the 'Show Table' button is will display the results panel. From here you can select several rows and change the class or the color by right clicking on them:

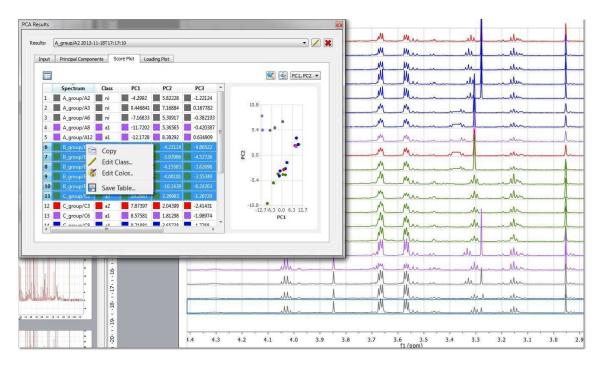


Select the applicable tab to display the 'Loading Plot'. In this plot, each point will be associated to each region of the stacked spectra. You can change the visibility and colors of the bins by right clicking on the applicable row:

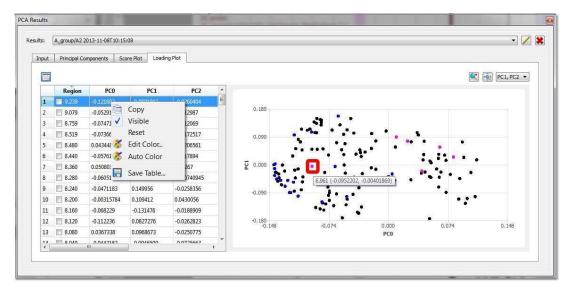

You can also change the color of all PCA regions on the spectrum based on the value of the loading plot for one component by selecting 'Auto Color' from the context menu above.

From the PCA dock widget, you can edit the parameters and run again the PCA algorithm in order to compare different results.

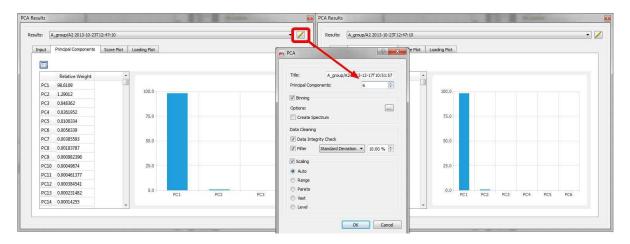

### See also this useful posts:

http://nmr-analysis.blogspot.com.es/2014/01/chemometrics-under-mnova-9-pca.html http://nmr-analysis.blogspot.com.es/2014/07/pca-and-nmr-practical-aspects.html http://mestrelab.com/blog/pca-of-nmr-data-advantages-of-an-integrated-approach/ And this video:

https://www.youtube.com/watch?v=kxVQKLY1KcU

# 10.8 J-Correlator


**J-Correlator** (Not available in Mnova Lite): is a new method for detecting spin connectivities in <sup>1</sup>H NMR spectra. The main goal of this method is to convert a 1D spectrum into a 2D-like plot in which it is easy to correlate multiplets containing the same **splitting**. Its main purpose is to rule out couplings between multiplets. It is suitable for human inspection.

The basic idea is to generate a 2D plot from a 1H NMR spectrum in such a way that the horizontal dimension conveys the chemical shifts whereas the vertical one represents the separation between peaks in the spectrum (*splittings* from now on). Basically, it is a special kind of 2D 1H - D experiment (where D = splitting).

Just load your <sup>1</sup>H NMR spectrum and follow the menu 'Advanced/J Correlator' to display the J Correlation dialog box to select the desired algorithm and display options:

Algorithm O	ptions				
PRF:	Doublet Picke	r 🛛 🗹 Use	Square Roo	t	
Threshold:	0.003	Max. Splitting:	25.00	\$	
Splitting Re:	solution: 0.12	255 👶			
Display Opti	ions				
Total Size:		65536 x 2	65536 x 200		
Size after S	caling Down:	21845 x 1	00		
Manu	al Adjustment				
Reduce H	orizontal Size I	by an Order of: 3	.00 0		
Reduce W	ertical Size by	an Order of: 2	.00 0		
Noduce n	arcicol bico by		.00		

As usual, a picture is worth a thousand words:

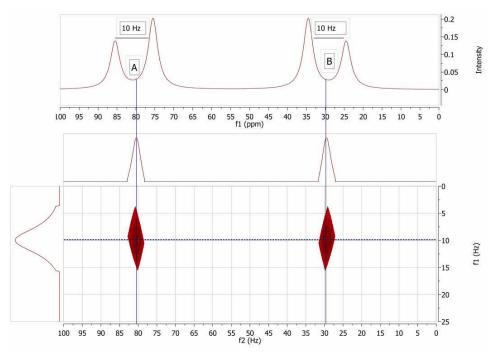

In this figure we have simulated 1D spectrum with two coupled spins, A = 80 Hz and B = 30 Hz. JAB = 10 Hz.

In the new 2D plot (JCorr from now on) we can see two cross peaks at the positions of A and B respectively and at the same d-trace (vertical dimension or splitting dimension).

It's very important to remember that what we see in the JCor plot are just splittings, not Coupling Constants, even though in some cases these splittings can coincide with coupling constants.

# 10.9 Arithmetic

Arithmetic (Not available in Mnova Lite):

This feature is used to carry out arithmetic operations with 'fid"s or processed spectra. Typically, you will use the arithmetic module implemented in MestReNova to sum 'fid"s acquired under the same measurement conditions in order to improve the signal-to-noise ratio.

This tool is also very useful to **remove impurities** or solvent signals from a spectrum, to **analize DEPT experiments**. This feature will be enhanced in the oncoming versions of the software to be able to **subtract FIDs of Selective Experiments** (such as NOE or ROE).

### How to sum or subtract spectra?

Application of Linear Combinations (sums, subtraction and multiplication) to spectra in the MestReNova interface is extremely simple. Just select the desired spectra (make sure they are acquired under same conditions) on the Page Navigator (by holding down 'CTRL key' or 'Cmd key' while clicking on each spectrum) and follow the menu 'Advanced/Arithmetic':


m File	Edit	View	Databas	e Proce	ssing	Analysis	Adv	anced	Stack	Mass Analysis	Predict
- 1	- 📑	8.		1000	1			Line Fi	tting		• • •
	Pages							Data A	nalysis		• 1 • •
<u></u> _	1.0	iinine 1H						Reacti	on Moni	toring	•
関・	Pres.				t:		2	Bayesi	an DOS\	Transform	
									Spectra		
19-									nce Alig	nment	
								PCA	1110-11-11-1 <b>1</b> 7		
								J-Corr	elator		
×111								Filter F	alse Pos	itives	
置			10.00	1			-	Arithm			
<b>X</b> -				1 al	11-1		-	Anthin	leuc		
- <b>*</b>	-	a 6	2 1 1	1	1 1	1 1 1		Spin S	imulatio	n	
	L. La	10.0		1941				qNMR			
赵王	Z.ES	tradiol_1	1					*****			
						Ť			a Screen		
*=							M.		a Screen		
Perch							View I	View N	Anova So	creen Result	
							1		7		
10									<u>б</u>		
								2	ġ		

This will display the 'Arithmetic' dialog box on screen. In this example, we want to add two times spectrum A to spectrum B, so we shall type the formula 'B+2A' in the applicable cell.


pe	ctra			
	Label	Title	Formula	
1	A	Quinine1H	A	
2	В	Estradiol_1H	В	
3	с	с	B+2A	

The 'Save Formulas' icon 🗐 will allow the user to save formulas, which can then be loaded by using the 'Load Formulas' icon 😰.


On pressing 'OK', the result is a new spectrum which will consist of the sum of spectrum B plus two times spectrum A.

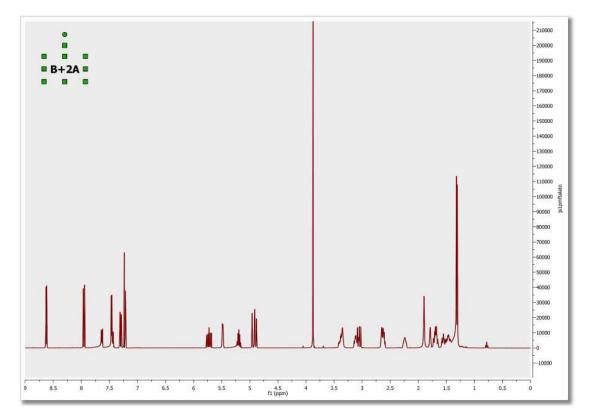

You can also subtract spectra, but in this case it is important that the user calculates the intensity ratio of both spectra. For example, in this spectrum we have a sample contaminated with a solvent.

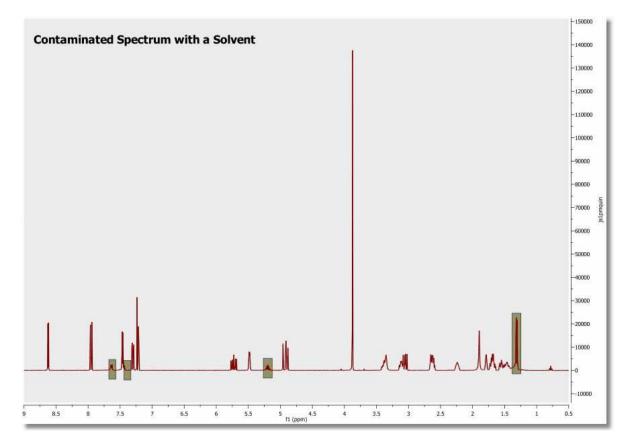


Whilst the spectrum below corresponds to the solvent which we need to eliminate from the sample.

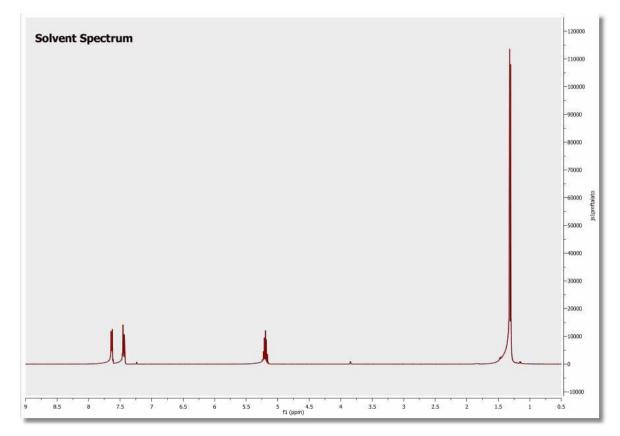


To successfully carry out the subtraction, we need to calculate the intensity ratio between the contaminated spectrum and the solvent spectrum. To obtain this ratio we can measure the intensity of a signal present in both spectra (by applying the command 'Peak by peak' and getting the result on the applicable table). For example, we measure the intensity of the singlet which appears at 1.32 ppm. For the first spectrum, we obtain an intensity of 22617 and for the second, 115031, indicating the the intensity ratio to be 1/5, or 0.2.

Typing the formula **'A-0.2B'** (or 'A-0.2\*B') in the 'Arithmetic' dialog box, we shall obtain the spectrum below, where the solvent signals have been removed:

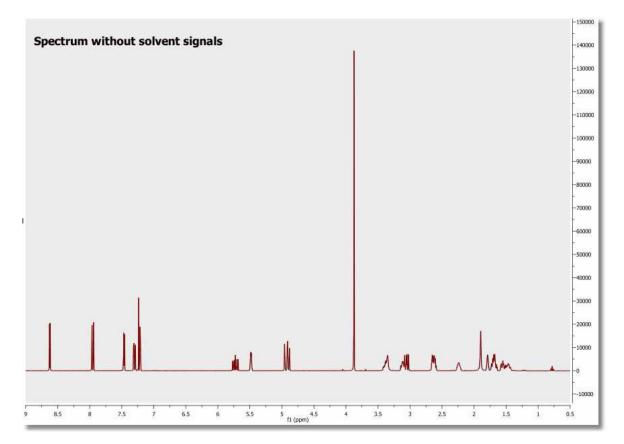

### Arithmetic and Covariance NMR

2D NMR spectra are simply 2D matrices (Note: these matrices can be real, complex or hypercomplex, but for the sake of simplicity, we will consider real matrices only) which can be subject to standard matrix algebra operations. You can read the <u>Covariance NMR</u> chapter where it is shown how Indirect and Direct Covariance NMR can be applied by proper matrix algebra. These methods are incorporated in Mnova as a dedicated module which also makes the filtering of spurious resonances possible . In order to show you that Covariance NMR actually involves these matrix operations, you can use Mnova's powerful Arithmetic module which we have recently completed. This module has been designed in such a way that it operates as a simple spectral calculator. You enter the equation which the program parses and produces the expected result. For example, if we have a HSQC-TOCSY spectrum (**A**), we can enter the Indirect Covariance formula like this:

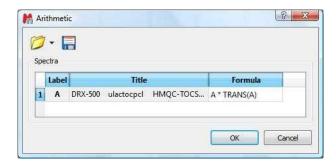

Where **A** corresponds to the real part of the original spectrum and **TRANS** indicates the transpose operation. This operation will produce the (unnormalized) Covariance NMR spectrum, in this case the 13C-13C correlation spectrum. Of course, in order to better approximate the covariance spectrum to

the applicable standard 2D FT counterpart, it's necessary to calculate the square-root using, once more, matrix algebra. This is again very simple with our arithmetic module by just adding the square root operation (**SQRT**) into the equation:

	Label		Title		Formula
E	Α	DRX-500	ulactocpcl	HMOC-TOCS	SQRT(A*TRANS(A))

This arithmetic module is not restricted to matrix operations within a single spectrum. We can freely combine as many spectra as we want. For instance, if we have, in the one hand a COSY spectrum and in the other a HSQC spectrum, we can combine both in an analogous way so that the indirect covariance NMR spectrum yields a HSQC-COSY 2D spectrum.

# 10.10 Spin Simulation


NOTE: The NMRpredict Desktop plugin must be installed (a license for this plugin is not needed).

This module of MestReNova is an efficient simulator for high resolution NMR spectra which can be used by following the menu 'View/Panels/Spin Simulation (or Advanced/Spin Simulation') which will display the applicable dialog box:

_	ew Sir	nulation	<u> </u>	ame Line		0.5 Hz	••••••••••••••••••••••••••••••••••••••
	bel	Arriter	t (ppm)	N		Spin	
A		1		1	1/2		
в		5		1	1/2	2	
С		7		1	1/2	2	
Js	Ds A	Qs	B	с			
A							
В	3						
C	3.4	5.5					
1							<u> </u>

Once there, we can easily simulate a spectrum by entering the desired values. For example, imagine 3 protons (3 spins Groups) called A, B and C, with chemical shifts 1, 5 and 7 ppm respectively. Their


coupling constants were J(AB) = 3Hz, J(BC) = 5.5Hz and J(CA) = 3.4Hz. Finally select the number of points and the spectral limits and click on the 'New Simulation' button to generate the corresponding spectrum:

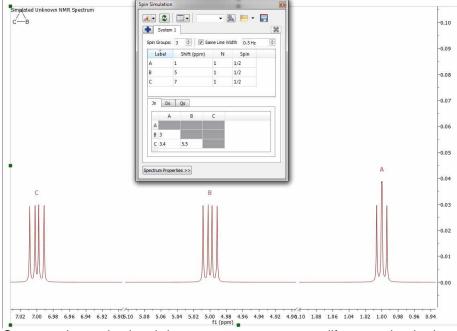

Once you have simulated the spectrum, you can modify any value in the table and obtain the new

spectrum by clicking on the 'Recalculate' button <sup>[S]</sup>. You can introduce 'Dipolar' or 'Quadrupolar' coupling constants and change the 'number of nuclei', 'Spin' and the 'Line Width' values by clicking and entering the desired values on the corresponding boxes. Finally, click on the 'Recalculate' button to update the changes in the spectrum.

Click&drag the assignment label to change the chemical shift of any signal of the spin-simulated spectrum:

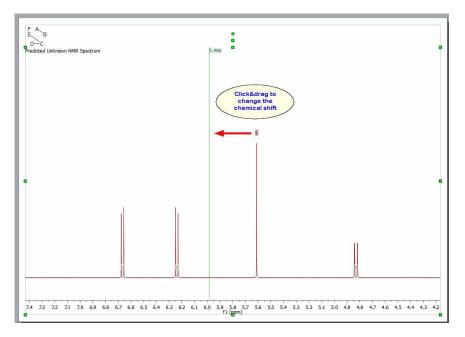

Traditionally, Spin Simulation algorithm were limited to 11-12 magnetic unequivalent coupled particles. However, this is completely insufficient to tackle the 'small molecules' of today. Consequently, simulation nowadays calls for brand new approximate algorithms involving, for example, fragmentation techniques.

Mnova SpinSimulation toolkit includes such sophisticated fragmentation algorithm which makes it possible the simulation of any spin system regardless of its size.


Select 'New as Superimposed' over an experimental spectrum to stack the synthetic spectrum with an experimental one:

k 🖬 🎑			- 🕺	N 🖻 - 🖪
🔬 New S	imulation			
Kew a	s Superimposed	me une W	/idth 0.75 Hz	<b></b>
Label	Shift (ppm)	N	Spin	
ANITO DETROMANDO		14777 14777	500 20 100 20 100 20 10 20 20 20 20 20 20 20 20 20 20 20 20 20	
ANITO DETROMANDO	Shift (ppm)	14777 14777	Spin	


If parameters of experimental spectrum and simulated spectrum are not the same, when you try to generate the calculated spectrum as superimposed a message will be displayed:

n Spin	Simulation	and the second second	
?	Predicted spectrum parar Do you want to use the ex	meters are not the same as the exp xperimental parameters?	perimental ones
		Yes	No


Clicking on Yes, the Spectrum Properties parameters will be modified to match with the experimental ones.

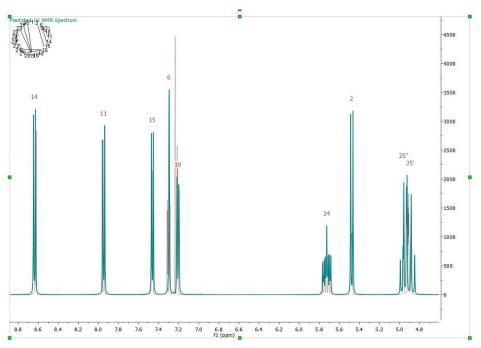

Here you can see another example comparing an experimental dataset with the simulated one:

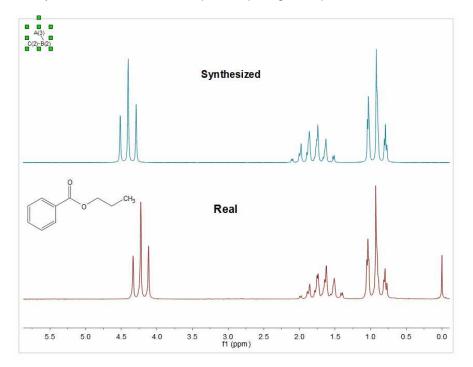

You can see below the simulated spectrum of the 'orto-dichlorobencene'; which is a AA'BB' system:

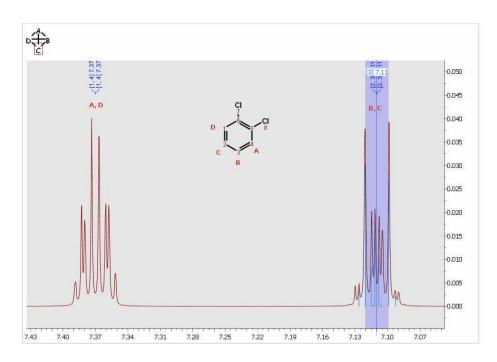

# How can I simulate an A3BXY system?

Here you can see an example of an A3BXY system:

L	abel		Shift (pp	m)	N	Spin	
A		1			3	1/2	
в		2			1	1/2	
с		5			1	1/2	
D		6			1	1/2	
A						-	
В	10						
C	4	12			14		
122			5				

To get the table above just follow this procedure:


1. Firstly, create a system with 4 spin groups. Please bear in mind that A3 is a unique spin group with 3 magnetic equivalent spins, so you will need to type N=3 in the label A..

2. Then, type the desired values for the other nuclei (B, C, D) with N = 1 for all of them (enter also the desired chemical shift value). Please bear in mind that Mnova does not need to know if the coupling is strong or weak, because Mnova makes the quantic calculations by using a rigorous method taking into account the chemical shift and the coupling constants

3. Once you have entered all the values and selected the Larmor Frequency and number of digital points, Linewidth for each nuclei, etc..., just click on the 'New Simulation' button to get the synthesized spectrum.

# How can I add new systems?

Click on the 'Add System' button 💽 to add several systems. A new system will be a fragment of the molecule that can be simulated separately since its protons do not interact with the rest. In other words, a set of nuclei that are related through their coupling constants. Once you have added a new system, you can change the population of the system by using the 'Population' edit box.

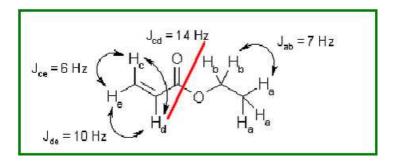


As an example, consider the case of a small molecule, ethyl acrylate CH2CHCOOC2H5

As you can see, a standard simulation of the 1H-NMR spectrum of this molecule would require eight frequencies to be introduced, one for each proton. Moreover, you should introduce nine coupling constants as well. However, even a brief study of this spin system suggests us a more elegant solution.

Why not treat this spin system as two 'subsystems'? One 'subsystem', corresponding to the ethyl group, is composed of five protons with only two distinctive frequencies labeled a (the methyl group) and b (the methylene group), and only one coupling constant, Jab. Other 'subsystem' is composed of the three remaining protons (those of the vinyl group), with three frequencies, c, d and e, and three coupling constants, Jcd, Jce and Jde. This decomposition of the spin system in two subsystems is possible because they are not connected in any way. The decomposition of a spin system into subsystems can be carried out in many molecules, and is, for example, the conceptual basis of the NMR spectroscopic data tables.

You can see below, the synthesized spectrum of the ethyl acrylate; after having created two different systems; system A (vinyl protons) in red, and system B (ethyl group) in green:

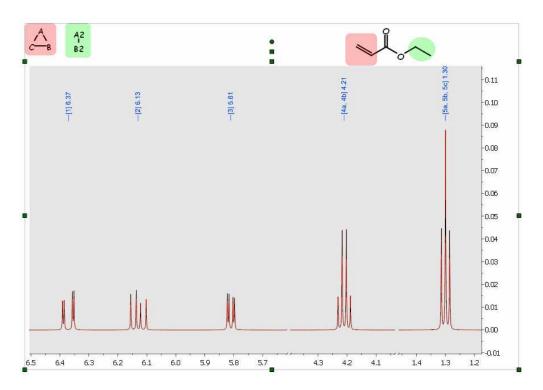

This decomposition method represents a great advance in terms of calculation speed, because the complexity of the calculation grows exponentially with the number of spins (nuclei) considered. However, we can perform even faster calculations and achieve greater flexibility going one step further.

Why not introduce only five frequencies, and tell the program how many protons correspond to each frequency? The introduction of magnetic equivalence allows the calculation to be performed using five spin groups, labeled from a to e, with their corresponding frequencies. The two first spin groups, a and b, have three and two protons respectively, while the other three spin groups have only one proton each. Of course, we need then only four coupling constants, Jab, Jcd, Jce and Jde. This process can be carried out in many molecules.

### 10.10.1 Spin Simulation panel

Click on the applicable buttons of the panel 📃 🗐 to 'Load/Save' the spin systems (in XML format).

You can sort by chemical shift, atom number, etc... by clicking on the applicable header (of the Spin Simulation panel). Right click on the applicable label to join/split magnetically equivalent multiplets:

- 2		• [	III 🖻 🕶	
System	n 1			
Spin Groups	: 4 🐳 🛛 🛛 Sa	ime Line W	/idth 0.5 Hz	
Label	Shift (ppm)	N	Spin	1
A	1	3	1/2	
в	Join Groups	1	1/2	
c	Split Group		1/2	
D	6	1	1/2	

Check the 'Same Line Width' box to change all the 'line width' values at once.

Spin Simulation - 風 😑 - 🖪 M - 2 **III -**Report Simulation System 1 + **Copy Simulation** Spin Groups: .5 Hz Setup Report 8 Label Shift (ppm) N Spin

You can report or copy to clipboard the Spin Simulation table:


### Command line for spin simulation

There is command line in the spin simulation panel to manually enter the values of interest. For example. when typing "A=1.2, B=2.3, AB.j=12, C=3.5, A.nn=3, C.nn=4, A.lw=1.2, B.sb2=2" the table in Spin Simulation panel will be filled as expected:

	Simulated	Unknor	wn NMR S	pedrum			C(4)			-0.2
es A(j)BC(i)	58(4)3°B						4.47			ŀ
.02										-0.1
.02										-0.13
mpound							-			-0.1
imulation	n				_					-0.16
- 2	A=1.3	2, B=2.3,	AB.j=12, C=	3.5, A.nn=3, C.nn=4, A.lw=	.2, 8.sb2=2 💌 🚻 🖡	🖹 • 🔚				-0.1
Syster	n 1					*				-
n Groups	: 3 💽 🗐 Sa	me Line V	ildth							-0.1
Label	Shift (ppm)	N	Spin	Line Width (Hz)						-0.1
	1.2	3	1/2	1.2						-0.12
	2.3	1	1	0.5				в		-0.1
	3.5	4	1/2	0.5						
										-0.10
ls Ds	Qs									-0.0
A	В	с							A(3)	-0.0
A									1	-0.0
B 12										-
с									1	-0.0
										-0.0
										-0.0
trum Prop	perties <<							1		
quency:	500. 13 MHz				Points:	32 K 💌				-0.0
n:	-2.00 ppm				To:	10.00 ppm				-0.0
_										-0.0
1										-0.0
										-
										0.0

### Simulating a spectrum by importing a XML file

Here you can see an example. Loading the XML file into Mnova, will generate the spectrum below:

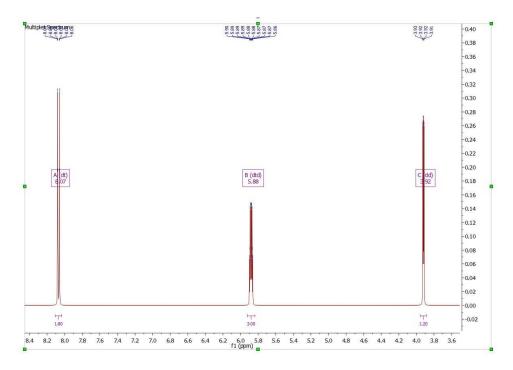


### Simulating a spectrum from the Multiplet Analysis

The table of multiplets can be used for the simulation of the synthetic spectrum. To do it just run a multiplet analysis on a experimental spectrum (make the necessary corrections if it is needed) and open the 'Spin Simulation' panel to click on the 'Get From Multiplets' button to populate the table with chemical shift and coupling constants values. Finally click on the 'New Simulation' button (or 'New as superimposed' if you want to get the experimental and the synthetic spectra overlaid).

pin Simulation	
🗶 🕒 🗐 📰 🗍	
System 1	Get From Multiplets 🕷

See also <u>"Importing spectral data from literature to synthesize a spectrum"</u>

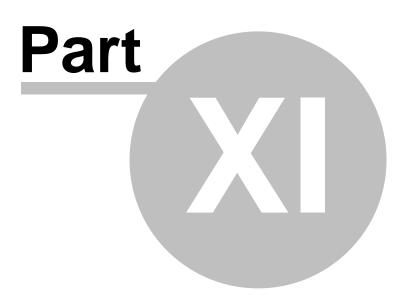

# 11 qNMR

qNMR is the "gold standard" of compound quantification and has found many uses and applications. qNMR stands for "quantitative NMR", and refers to the use of NMR to determine the concentration of one or more chemical species in solution.

# The area of an NMR signal is directly proportional to its concentration, and this "response" will be the same for all molecules.

And this is also what sets qNMR apart from almost all other metrological techniques used to quantify compounds. Each suffers with problems such as compound-specific response factors (UV), chemical considerations (NCLD), or relative volatility (ELSD). The qNMR method only requires that (a) the sample dissolves completely in a (normally fully deuterated) solvent, and (b) it contains NMR-active nuclides – and that some care and attention is paid to data collection and processing.


Our new module provides a mechanism to quantify compounds that is:

- Accurate
- Versatile
- Automatic

The basics of qNMR require simply the *Absolute Integral* per nuclide for one or more spectral regions, and a factor to *convert* this to concentration.

We have designed a competent, flexible, and sophisticated program for quantitation by NMR. It may be run fully automatically and is thereby incorporated into automated procedures and combined to streamline processes such as compound <u>Verification</u> and quantitation.

This new feature needs its own license and it is located under the Advanced menu of Mnova.

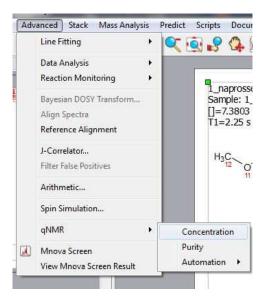

You will need to install the qNMR plugin separately, by following the menu 'Edit/Advanced Plugins' and clicking on the 'blue plus' button or just by dragging&dropping the XML file in Mnova. See <u>this video</u> for further information.

Once you have installed the advanced plugin, you can move the folder to a shared location and create a defaults.ini file (in the Mnova installation folder) pointing to it. After doing that, all users accounts will have the advanced plugin installed.

Here you can see an example of a.defaults.ini file:
[%General]
AdvancedPluginsDir=C:\Your\Path\To\Plugins\Here

For further information about qNMR, please visit our blog: http://mestrelab.com/blog/what-is-qnmr/ http://mestrelab.com/blog/edited-sum-integration-for-acquisition/ http://mestrelab.com/blog/determining-concentrations-when-using-nmr-to-model-chemical-reactions/ http://mestrelab.com/blog/automating-qnmr/ http://mestrelab.com/blog/qnmr-purity-recipe-book-i/ http://mestrelab.com/blog/qnmr-purity-recipe-book-ii/ http://mestrelab.com/blog/new-qnmr-experiments/ and download article: http://pubs.acs.org/doi/abs/10.1021/ac400411g

#### For Mixtures Analysis:

http://mestrelab.com/blog/biodiesel-level-determination-using-lf-nmr-data-experiment-validation-and-sma-implem entation/


# **11.1 Concentration Workflow**

Generally, the workflow will be:

- Determine multiplets
- Run the script and select the qNMR variables
- The software will choose the multiplets to include
- Report

So first of all, we will load a 1H NMR spectrum and apply the necessary processing. (Depending on the level of accuracy required, you must pay attention to the number of data points used for the FT (typically 64K) and to apply a phase correction. Sometimes a baseline correction could be also needed. If necessary (e.g., solvent saturation was used), <u>blind regions</u> should be used to mask these spectral regions).

In the example shown below (which you can download from <u>here</u>), we have just loaded the dataset and applied an 'automatic multiplet analysis':

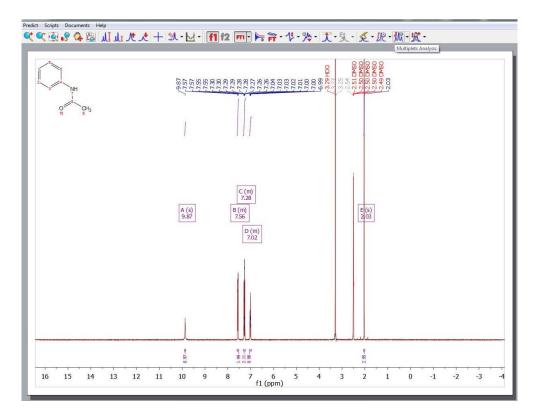

The qNMR functionality is selected from the "Advanced" menu item. The software stores all <u>settings</u> in the registry, so you may not have to change things. But you will need to provide some information the first time you use this. This will be described in more detail, below. For this tutorial, we have clicked on the 'Settings' button of the qNMR panel and then on the 'Load Parameters' button to load the '1\_acetanilide.data' file (which you have downloaded together with the dataset in the previous step):

oncentration	ntegration	Opti	ons R	еро	rt			
Concentration Me	hod							
🔵 Internal Refere	nce							
-rom: -	.10	To:	-0.90	A	ppm			
Reference Pea	c is a Solvent							
Apply Line Fitti	ng to the Ref	erence	Peak		22	2		
Reference Concentration:			100.00	×	M •			
Nuclides of Refere	nce:		1	×				
Concentration	Conversion F							
Conversion Factor:		0.00	08420000	×	M •	📲 🔉 Autoset		
Parameters for F	eference							
Receiver Gain:	64.00		Compens	sate	Receiver Ga	ain		
Number Of Scan	s: 32		Compens	sate	Number of	Scans		
90º Pulse Length	: 12.0000	1	Compensate Tip Angle					
DIGMOD:		No	tes:					
Pulse Program:	zg30	s	um integra	atior	1: MF=15			
Instrument Nam	-				desense en de la co			
Probe Name:								
						🛸 Library		

After having clicked on the OK button, the qNMR panel will be displayed with the information about the multiplets and absolute integrals found for their bounds. Having the correct number of nuclides is important and the software may do this better if the molecular structure is available and plotted.


	Paste Report	Settings Autosele						
	A.815	centration Average	: 20.21 0.243	M	M			
	Multiplet	Autoselected	Shift	Range	Hs	Abs. Integral	Concentration	SNR
1	🔽 C(m)	1	7.28	7.337.22	2	48133.4225	20.2642	316.9591
2	D(tt)	1	7.01	7.076.95	1	23926.4044	20.1460	196.7300
3	📝 E(s)	1	2.03	2.062.00	3	71969.3298	20.1994	2689.9396
4	🔲 A(s)	0	9.87	10.209.54	1	21609.2674	18.1950	84.9604
-	🔲 B(m)	0	7.56	7.64.,7.50	2	47541.2932	20.0149	280.6376

At this stage the qNMR process will be done automatically and the multiplets sorted in the table based on their perceived ranking as candidates for qNMR. The selected multiplets can be changed using the check boxes next to each multiplet, and the effect on the derived concentration will be updated. The concentration averaged calculated for this example is 20.2 mM (the units can be changed by using the applicable combobox)

You will find different button in the qNMR panel above:



Paste Report [Save Report] (Save Report Copy Report of Report qNMR results on the spectrum page, export the report into a txt file or copy the report to the clipboard (depending on the report options that you have selected in the settings)

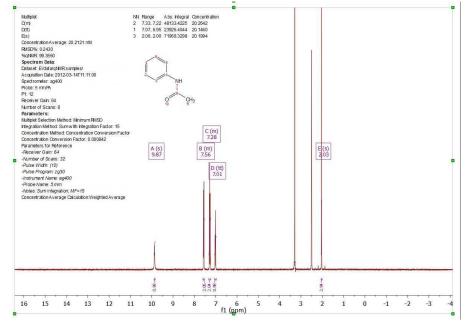

- 2. Show the "Settings" dialogues
- 3. Autoselection Selects best multiplets based on rules (see <u>gNMR Settings</u>)
- 4. Refresh Refresh the calculation. (Not needed if "Autorefresh" is deselected in Settings.)
- 5. Select all/no multiplets. (An alternative to 4)



Ø

The user can check the applicable boxes to manually select/deselect the multiplets that will be used to calculate the concentration information. The "Hs" for a multiplet can be manually changed by clicking on the number.

## 11.1.1 qNMR Settings

Selecting 'Settings' on the qNMR panel, will display the dialog box below, containing different tabs (Concentration, Integration, Options and Report):

oncentration Int	egration	Optio	ns Re	epor	t		
Concentration Meth	bd						
🔵 Internal Referen	ce						
From: -1.	10 🌔	To:	-0.90	×	ppm		
Reference Peak	s a Solvent						
Apply Line Fitting		ence I	Peak	-		-	
Reference Concentra		100.00		М			
Nuclides of Reference	10 C 2		1	×			
Concentration Concentration Concentration				-	665	_	
Conversion Factor: Parameters for Rel		0.000	8420000	×	М	*	🐺 Autoset
Parameters for Ke	erence						
Receiver Gain:	64.00		Compens	ate	Receiver	Gair	i
Number Of Scans:	32		Compens	ate	Number	of Se	ans
90º Pulse Length:	12.0000	1	Compensate Tip Angle				
DIGMOD:		Not	es:				
Pulse Program:	zg30	Sum integration; MF=15					
Instrument Name:	aq400						
Probe Name:							
Probe Name:		1					
						1	Library

Note first the "Save" and "Load" buttons. These will allow you to set up the correct settings for parameters and distribute amongst other users to ensure they do the analysis correctly

### **Concentration**

Fundamentally, there are two ways to determine concentration: using a signal as an "internal reference", or a specified "Concentration Conversion Factor" (CCF). The internal reference may be a real signal area (e.g., residual solvent, TMS) or an artificial signal (e.g. ERETIC or QUANTAS). If a residual solvent is used then the "Reference peak is a solvent" box should be checked, and then only peaks of type "Solvent" in the chemical shift range will be used for area calculation. This can be useful to exclude errors that would result if impurity, analyte or other peaks were used, and this is a nice feature that follows from AutoClassify.

### **Concentration Conversion Factor**

Currently, we only support CCFs that have been determined using data processed within Mnova – there can be significant errors if Bruker 1r files are used. The CCF is determined for a particular experimental setup by processing the spectrum of a compound of known and specified concentration, and adjusting the "Conversion Factor" until the correct concentration is reported.

To calculate the CCF value, just load the spectrum with the multiplet analysis done and click on the 'autoset' button of the 'concentration settings' panel to input the weighed mass and Molecular Wt of the reference, the NN for this multiplet and the applicable multiplet in the spectrum:

Weighted Mass:	1363.23
Mol. Weight:	230.26
Multiplet:	D(dd) 🔻
NN:	1

The CCF will be calculated using:

CCF = (Weight/Mol Wt) \* (NN/AI)

For further information about how to calculate CCFs with Mnova qNMR please take a look at this document.

### Library of CCFs

It is important to account for the fact that a CCF value will have a fundamental, strong dependence on the spectrometer hardware: the particular NMR spectrometer and probe, principally. This must be determined each time empirically, as described above. After that is done, simple mathematical compensations can be made for differences in the spectrum acquisition parameters: receiver gain, number of scans, or 90° pulse length. If necessary, a different value can also be determined and saved for different solvents.

To facilitate this,	, the user ca	an save these	values to a file -	<ul> <li>and distribute them,</li> </ul>	of course.
---------------------	---------------	---------------	--------------------	--	------------

Parameters		GSK_sucrose	unique pa	unique parameters				
Conversion Factor	r:		GSD integration	GSD integration				
Receiver Gain for Reference: Number of Scans:		11.00	Ð	n Hendrick (1990) - Kandonsego (1				
		4						
90° Pulse for Refe	erence:	7.89	•					
Pulse Program for Reference: Instrument Name:		zg		manage	library			
		pt600						
Probe Name:	L	Z-GRD Z44896/011	5					
Name	Conv. Factor	Receiver Gain	N. of Scans	90° Pulse	Pulse Prog			
GSK_sucrose	0.00265	11	4	7.89	zg			
GSK_acetanilide	0.000842	64	32	12	zg30			
		Select the co parameters.						
٠		III			,			

To add a new library condition the user will populate the parameter fields correctly, click the blue "+" button to add to the library, and save the updated data file.

To select a different CFF, highlight the row and click "OK". The software will check that the parameters

match if specified, and this information will be included in all reporting.

## **Integration**

Concentration	Integration	Options	
Integration Me	thod		
🔘 Sum	Multiplication Fa	ctor:	15
Multiplet In	ntegration Metho	d: Peaks with GSD Pe	eak Picking
	for Multiplet 1 quantitation.	<b>hk Picking</b> and <b>Peak</b> Integrals are advised I These settings are a Multiplet Analysis Opti	<sup>f</sup> or accurate vailable in Peak Picking
Options			
and the second second	Fitting Automati	33	

The user can select between these options:

- Sum integration. This is the "traditional" integration method. The "Multiplication factor" should be set to a value of 15-20, and determines the integration limits with consideration of line-width. Sum integration is a poor choice with mediocre or poor S:N spectra, or if the spectrum is quite crowded – multiplets are close to one another. If using this selection the spectrum must be very well phased and baseline corrected.
- 2. <u>GSD integration</u>. As the tip says, this is set from the Peaks/Options, but GSD is the default. This should probably be the default selection for most cases.
- 3. <u>Line fitting checkbox</u>. There may be cases where GSD doesn't do a fantastic job: look for this in the case of singlets. So line fitting may be necessary for QUANTAS/ERETIC internal references, as these signals are singlets. Checking this box has the same effect as pressing the "Line Fitting" button on the results page.

### Options

This is where all other settings are grouped, including the very important multiplet selection criteria.

oncentration Integration Options	
General Options	
Autoselected Multiplets	3 🔹
Concentration Average Calculation:	Weighted Average 💌
Run Automatically	
🔲 Use Labile Protons	
$\fbox{[v]}$ Discard Mismatched Assignments when Av	ailable
🗹 Calculate Area Purity	
Autoselection Method	
Minimum RMSD	
Scoring Rules	
🗇 Hybrid Method	
Rules to Rank Autoselected Multiplets	
Prioritise Aromatic Hs	
Penalise Multiplets with Several Nuclei	
Use Scores from Assignments	
Penalise Undefined Multiplets	
Prioritise Clean Multiplets	
💟 Wide Multiplet	
Score Threshold: 0	.40

### 1. General Options.

- **a.** <u>Autoselected multiplets</u>. The target (max.) number of multiplets that will be used for the final concentration determination. The score threshold, labiles use, etc. will be respected.
- **b.** <u>Concentration average calculation</u>. Difference in how the average is calculated. Simple average will calculate the mean average of the concentrations. Weighted Average will calculate the concentration with the sum of the integrals, divided by the sum of the nuclei and multiplied by the scaling factor.
- c. <u>Run automatically</u>. If deselected the user must click the "Refresh" button to trigger the calculation.
- **d.** <u>Use labile protons</u>. The default is to ignore labile protons (if categorised), but if you check this box then the restriction is lifted. The thinking is that signals from labile protons almost always under-integrate, and should not be included in qNMR calculations. This offers a partial workaround if the user really wants to use labiles. This rule is applied if "Use Labile Protons" is checked; multiplets considered to be or contain labile protons will be penalized by a factor of 0.25. If unchecked, labiles have a score of 0.0 and are therefore omitted from all concentration calculations.</u>
- e. <u>Discard mismatched assignments when available</u>. This test uses nuclide information from AutoAssignment and checks that it matched with NN from the multiplets. If they are not in accord the multiplet will have its score lowered.
- f. <u>Calculate area purity</u>. If checked, this will show with the results summary. It is calculated using the sum of areas for compound and impurities (from GSD), and is something of a rough value:

% Purity = (-A(C) / (A(C) + A(I)) \* 100.0

A(C) is the sum of the GSD areas for peaks labelled as compound A(I) is the sum of the GSD areas for peaks labelled as impurity

### 2. Autoselection Method

These methods will all try to select the number of multiplets in 1a, whilst respecting the score threshold (3g).

- **a.** <u>Minimum RMSD</u>. This option will ignore the multiplet scores and simply chose the multiplets that give the smallest RMSD in the average concentration. It may be used for very pure compound spectra. The maximum number to be used is the user-selectable "Autoselected Multiplets".
- **b.** <u>Scoring rules</u>. This applies the rules selected in section 3, below, and then uses the top multiplets to determine the average concentration (and RMSD). The maximum number to be used is the user-selectable "Autoselected Multiplets".
- **c.** <u>Hybrid method</u>. This method first applies the scoring rules and then chooses amongst the highest scoring multiplets. Using the multiplets whose final score exceeds the score threshold, the multiplets that give the smallest RMSD are identified and used for the final average concentration calculation (and RMSD).

#### 3. Rules to rank autoselected multiplets

- **a.** <u>Prioritise aromatic Hs</u>. Non-aromatic multiplets will have their scores penalised. Especially useful when the aliphatic region is complicated by large residual/impurity peaks or when solvent saturation is used. If the user checks the option, the aromatic Factor will be 1 for an Aromatic multiplet, and a non-Aromatic H is multiplied by 0.5 (Aromatic range=5.5-12ppm).
- **b.** <u>Penalise multiplets with several nuclei</u>. Prioritises multiplets having the fewest NN. This assumes that impurities can lead to a false NN. The score is multiplied by 1/NN: the larger NN, the lower the score.
- **c.** <u>Use scores from assignments</u>. If Verify/AutoAssign was used, the individual multiplet scores will be taken into account. A multiplet with a higher assignment score Q(-1 to 1) will be scored higher. Assignments Factor = 0.75 + Q/4
- **d.** <u>Penalise undefined multiplets</u>. The thought is that a multiplet marked as "m" may be a clear solute multiplet but complicated by impurity peaks. In this case the "m" is penalised. The factor will be 0.6 for 'm' or 's' multiplet types, and 1 for all others.
- e. <u>Prioritise clean multiplets</u>. The presence of impurity peaks will cause a 10X increase in their relevance when determining the score. Use when spectra are very clean.

Clean Multiplets factor=multipletPeaksSum/(multipletPeaksSum+noMultipletPeaksSum)


multipletPeaksSum is the total sum of the areas of all the peaks

noMultpletPeaksSum is the sum of the areas of the peaks not assigned to the multiplet There is a further correction for peaks labeled as impurities: the area for this peak type will be increased x10.

- f. <u>Wide multiplet</u>. Penalises a multiplet having a width >60 Hz. This case can arise when the multiplet picks up impurity peaks. Consider using with dirtier spectra. The score is divided by 2 if the width of the multiplet is greater than 60Hz.
- **g.** <u>Score threshold</u>. Multiplets having a score below this number will not be used in the average concentration determination. A value of 0.3 is typical. (Scores are between 1 and 0.).

### Reports

This is where you can select how to report your results; by pasting the report into the Mnova document, by exporting to an ASCII file or by copying to the clipboard.



You will find also some options to choose which parameters you want to report.

## 11.1.2 Purity qNMR


This new feature is an enhancement of the Purity calculator script by using the qNMR engine to automatically select the best multiplets in a spectrum and use them to calculate *concentration* using a number of industry standard approaches. Analysing sample replicates is facilitated.

The purity qNMR tool has 3 main features:

- Purity: classical compound purity determination against a purity reference
- Counterion: determines a salt ratio when the counterion has proton(s) e.g., acetate salt of an amine
- Solvent: calculates residual solvent residue levels

### Example 1: Purity

The workflow would be the expected. We describe the process for a spectrum of Felodipine with TCNB (tetrachloronitrobenzene) as an internal purity reference. Open your dataset with the molecular structure and apply an automatic multiplet analysis (you can download the dataset and the libraries from this <u>link</u>):

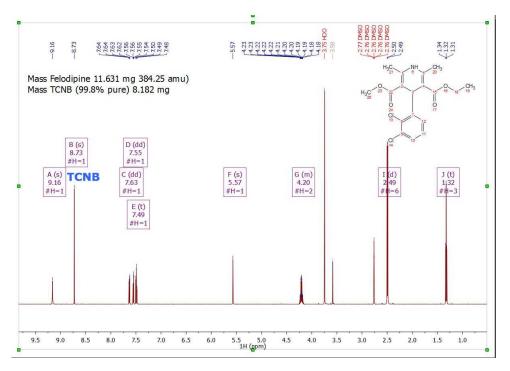

Next, follow the menu 'Advanced/qNMR/Purity' to display this dialog box:

💿 Purity 💿	Counterion 🛛 💮 S	olvent			
Reference Comp	ound Details				
Name:	×	Weigh	it (mg):		
Sample Details					
Mol Weight:			Weight (mg):	-	
Results					
Purity Average:	0.0000		RMSD%:	0.0000	
Multiplet A	utoselected S	hift	Range	Hs	Purity

The next step will be to define the settings, by clicking on the applicable button. For this example, we can load the 'Purity\_settings.data file (by clicking on the load button highlighted in red in the picture below) and the Purity\_library.data (button highlighted in green in the picture below)' of the zip file. Once the library has loaded, we can click on the TCNB row to use the applicable values. You can type the reference compound details by hand (instead of loading the settings).

Reference	Integration	Report	Options				
Reference (	Compound Deta	ils					
Name:	TCNB		Compound:	TCNB	▼ Solv	ent: DMSO 🔻	
Molecular W	eight: 260.89	9	Purity:	99.8			
Туре							
Refer	ence	O	Counterion	C	) Solvent		
Positions							
	From:	8.68	To: 8	.78 💽 ppm	n Nuci	ides: 1 👘	
		3,72	To:	.82 🔆 ppm	n Nucl	Nuclides: 1	
		4.29	To: 4	.39 💠 ppm	n Nucl	ides: 1	
1845	10 2450	257	1 1151115 10		2 🛖 🤅		
Name	Com	ound	Solvent	Mol. Weight	Purity%	Type	
DMP	3,5-dimeth	ylpyrazole	DMSO	96.13	98.6	Reference	
Acetate	CH3CO2		DMSO	59.0	100	Counterion	
TCNB TCNB		DMSO	260.89	99.8	Reference		
ICIND							

Click on the OK button to fill the 'Purity' dialog box with the information about the 'reference compound and sample details' (8.182 mg of TCNB and 11.631 mg of Felodipine). The molecular weight of our compound can be obtained from the molecular structure just by clicking on the 'Mol Weight' button:

💭 Purity	Counterion	Solvent	Ī		
Reference	Compound Details				
Name:	TCNB	▼ Weig	pht (mg):	8,1820	


Finally, click on the 'Recalculate' button to get your purity result (99.7%) and paste the result in Mnova by clicking on the 'Paste Report' button:

	Paste Report	Settings Mol. V	<b>)</b> Veight	Recalculate	Take Snap	 Dishot Load	
	🕲 Purity 🛛 🤇	Counterion	💮 Solver	nt			
	Reference Con	npound Details TCNB	• ] W	'eight (mg):	8,18	20	
	ample Details 10l Weight:	384,25		▼ Weight (mg	): 1	1.6310	
R	esults						
Purity Average: 99.7		99.7	RMSD%:			0.07	
	Multiplet	Autoselected	Shift	Range	Hs	Puri	
1	C(dd)	1	7.63	7.667.61	1	99.7333	
2	V F(s)	1	5.57	5.595.55	1	99.6346	
3	☑ G(m)	1	4.20	4.264.15	2	99.8070	
			an.	-	-		

Note that if your purity standard is not in the drop down list, you will have to add it yourself. From the Settings and Reference tab, enter the information for your reference compound (Molecular weight, purity, ppm range(s), etc.), and the blue "+" button to add it to the library. Once added, don't forget to save this updated library.


It is quite often the case that an analysis is performed with replicates: duplicate, triplicate, etc. samples. That is, 2 or 3 samples of the same compound and reference standard are made, and their spectra recorded. In this case the analysis of the replicates is facilitated allowing the user to apply the same analysis on all samples, and determine an average purity for the replicates.

After performing the analysis on the first sample, the "Take Snapshot" button will temporarily save the selected multiplets, ref. compound, compound MWt - things that stay the same from sample to sample in the replicates. When the 2nd, 3rd, etc. sample is active, press "Load Snapshot" to replicate all the qNMR Purity parameters except the weights of sample and reference. In the last replicated sample you will get the averaged purity value.

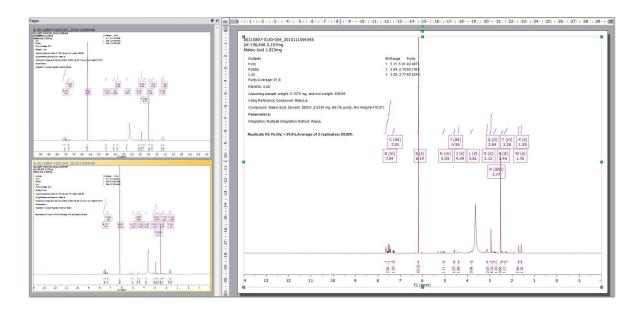

#### **Example 2: Counterion**

The workflow will be basically the same as in the example above, and the library must contain information on your counterion of interest. We load the 1H-NMR spectrum with the molecule, run a multiplet analysis and follow the menu "Advanced/qNMR/Purity' to select (or load) the applicable settings:

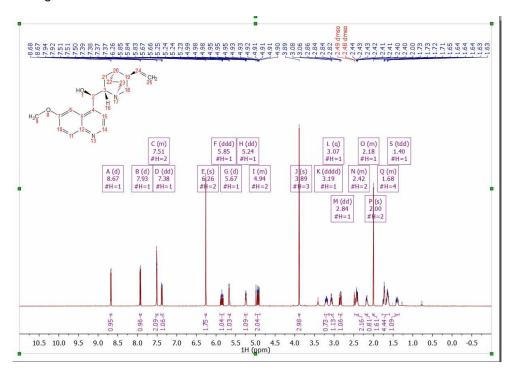

In this example, we want to determine the concentration of the 'acetate' as a counterion (singlet at 2.00 ppm); so we will need to load the Acetate values from the library (or type the applicable reference compound details by hand) making sure that we check the 'Counterion' radio button (this step can be skipped if you want to use the signal at 2 ppm)

Reference	Integration	Report O	otions			
	ompound Details	12	Vert		ov wa	
Name:	Acetate	Com	pound: CH3CC	02 <del>•</del> 5	iolvent: DMSO	•
	eight: 59.0	Puri	ty: 100			
Туре		-				
🔘 Refer	ence	Ount	erion	Solve	nt	
Positions			-			
V	From: 1.95	To:	2.05	ppm	Nuclides: 3	*
0	From: 3.72	To:	3.82	ppm	Nuclides: 1	4
m	From: 4.29	To:	4.39	ppm	Nuclides: 1	4
-			1			
						_
Name	Compound	Solvent	Mol. Weight	Purity%	Туре	
DMP	3,5-dimeth	DMSO	96.13	98.6	Reference	l
Acetate	СНЗСО2	DMSO	59.0	100	Counterion	

Click on OK to display the 'Purity' dialog box and to select the 'Counterion' tab to choose the salt:




Finally, click on the 'Recalculate' button to get the result:

4	🗊 Purity 🛛 💿	Counterion	🔊 Solvent			
	Details Name: A	cetate		•		
	ample Details					
M	iol Weight:	324.4168		Weight (mg):	49.51	00
R	esults					
5	Salt Ratio Average	e: 0.54:1.0		RMSD%:	0	.2464
-	Multiplet	Autoselected	Shift	Range	Hs	Salt Ratio
1	🔽 C(m)	1	7.51	7.537.48	2	0.54:1.0
	<ul><li>✓ C(m)</li><li>✓ J(s)</li></ul>	1	7.51 3.89	7.537.48	2 3	0.54:1.0 0.55:1.0
2	2000 C 1040274	2	1902/201	(1.00 T. 10 (20 T.)	12	
2	J(s)	1	3.89	3.913.87	3	0.55:1.0
1 2 3 4 5	<ul> <li>✓ J(s)</li> <li>✓ N(m)</li> </ul>	1	3.89 2.42	3.913.87 2.482.38	3	0.55:1.0 0.54:1.0

### **Example 3: Solvent**

The workflow will be the same as before. Load the dataset, run a multiplet analysis and follow the menu "Advanced/qNMR/Purity' to select the settings.

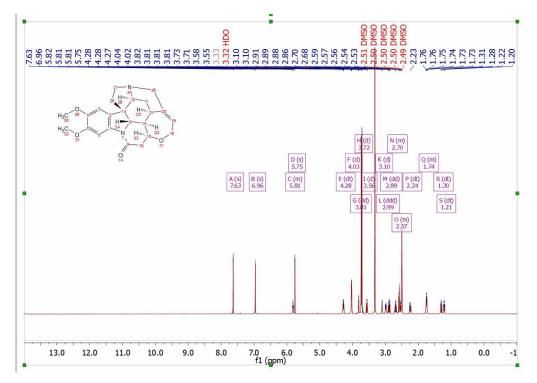

In this example, we will calculate the CH2Cl2 concentration, so select the 'Solvent' tab to choose the solvent. If you are interested in the Solvent Mass% value, you would need to type the applicable sample details:

Derity	Counterio	n 💿 So	lvent			
Details	1		_			
Name:	DCM			▼ Units:	Mole%	•
	C.				-	1

And finally, click on the 'Recalculate' button to get the result:

Pa	aste Report Se	ttings Mol. Wei	ght Reca	Culate Take Sr	napshot	10ad Snapshot	
6	🔊 Purity 🛛 😡	Counterion	🕽 Solvent				
	Details						Ĩ
	Name:	DCM		▼ Unit	s: Mo	le% ▼	J
Sa	ample Details						
м	ol Weight:	394.4635	•	Weight (mg):	38.657	0	-
Re	esults						
Μ	iole%	78.9	1	RMSD%:	0.5880		
	Multiplet	Autoselected	Shift	Range	Hs	Mole	1
1	👿 G(dd)	1	3.81	3.843.77	1	79.6	
2	🔽 M(dd)	1	2.89	2.932.84	1	78.6	-
3	R(dt)	1	1.30	1.331.26	1	78.5	
4	🗐 A(s)	0	7.63	7.677.61	1	43.2	
5	🔲 B(s)	0	6.96	6.996.94	1	72.7	
	[		m		1		

#### Visit also our blog:

http://mestrelab.com/blog/what-is-qnmr/ http://mestrelab.com/blog/qnmr-the-best-pulse-length-for-acquisition/ http://mestrelab.com/blog/determining-concentrations-when-using-nmr-to-model-chemical-reactions/ http://mestrelab.com/blog/determining-concentrations-when-using-nmr-to-model-chemical-reactions/ http://mestrelab.com/blog/automating-qnmr/ http://mestrelab.com/blog/qnmr-purity-recipe-book-i/ http://mestrelab.com/blog/qnmr-purity-recipe-book-ii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-ii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-iii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-iii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-iii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-iii/ http://mestrelab.com/blog/qnmr-purity-recipe-book-iii/

## 11.2 Batch qNMR

You will need to install the Batch qNMR plugin separately, by following the menu 'Edit/Advanced Plugins' and clicking on the 'blue plus' button or just by dragging&dropping the XML file into Mnova.

Having the applicable license, you can run qNMR analysis in batch mode by following the menu 'Advanced/qNMR/Automation/Batch Concentration':

iles	Concentration	Integration	Preprocessing	Autoselection	Options			
Files	Location							
Base Directory:		C:\Users\Usu	C: \Users \Usuario \Desktop \qNMR materials \qNMR datasets \DOCS					
Path	Mask:	*/fid		Examples:				
Molecules Files Location Molecules Directory:		1. PRJ ?????? 2. SMPL-*/10 C: \Users \Usuario \Desktop \qNMR miavenais \quiviec varias		*/10/pdata/1r				
Path	Mask:	*.mol						
Resu	ults		(F	xamples:				
Direc	ctory:	C:/qNMR_Re		1. PRJ ??????/	*.mol /pdata/*.sdf			

From the 'Files' tab, you will be able to select the file locations and also the folder where you want to save your results.

**Path Mask:** From here you will need to type a 'Path Mask' for your datasets describing how to open each of the spectra. All Operating System standard conventions apply (\*, ?, !, etc.). In the example above the 1H datasets are stored in C:\Users\Usuario\Desktop\qNMR materials\DOCS (each dataset in the applicable folder):

You will find several tabs for your 'Concentration', 'Integration', 'Reprocessing' and 'Options' settings (as you have in the <u>gNMR single mode</u>):

Concentration Method						
From:	-1.10	🔹 To:		-0.90	(A.)	ppm
Reference Peak is a S	olvent					
Reference Concentration	;			100.00	A Y	M
Nuclides of Reference:				1	A.	
Concentration Conve	rsion Factor:					
Conversion Factor:		0.000842	0000		*	mM
Parameters for Referen	ce					
📝 Receiver Gain:	64.00	A V	Notes:			
Vumber of Scans:	32	A V	Sum integra	ition; MF=15		-
90º Pulse:	12.00	A Y				
Pulse Program:	zg30					
Instrument Name:	ag400					
Probe Name:	5 mm PABBO BB-1H/	2-GRD Z10861				Library
Load Concentration Data						
				ts Ipocos Ipocos		6

The integration tab will allow you to select the integration algorithm and also some peaks classifications:

Files	Concentration	Integration	Preprocessing	Autoselectio
Integ	gration Method			
<b>0</b> S	Sum			
Multip	plication Factor:	12	9	
0 0	Default Multiplet Int	egration Method		
<b>A</b>	pply Line Fitting			
Peak	Classification			
🔘 I	gnore Molecule			
Ou	Jse Molecule withou	it Assignment		
00	Jse Molecule with A	ssignment		

You can replace the default solvent (with DMSO, for example) and use the 'processing templates':

Files	Concentration	Integration	Preprocessing	Autoselection	Option
Solve	int				
Repla	ace Default With:	1			
Proce	essing				
Proce	essing Template:	Ĩ.			
Func	tion:	Ī			
Scrip	t:				

**Solvent/Replace Default With:** This allows users to handle situations in which the solvent may be wrong in the parameters. It can be the case that a certain batch has been run on a specific solvent but that the user left the default solvent on the spectrometer data entry and therefore the solvent could be wrongly entered. Since the target solvents will affect the performance of the Autoedit function in Mnova qNMR, it is important to be able to correct for this at the script level. Use 'none' if solvent saturation was used, and a blind region excludes it. This prevents GSD from trying to find a non-existent signal and getting confused.

From this menu, you can also apply a processing template or a script or a function the user would like to run prior to each qNMR analysis being performed.

The Autoselection tabbed menu will be similar with the one in the qNMR single mode settings:

Auto	selection Method				
0	1inimum RMSD				
© 5	coring Rules				
© F	lybrid Method				
Rules	to Rank Autoselec	ted Multiplets			
P	rioritise Aromatic H	s			
[] P	enalise Multiplets w	vith Several Nuclei			
	ise Scores from Ass	signments			
[] P	enalise Undefined I	Multiplets			
[]] P	rioritise Clean Multi	plets			
P	enalise Wide Multip	lets			
Score	e Threshold:		0.40		4, '4'
Optic	ins				
Auto	selected Multiplets:		3		*

Finally from the Options tab, we will be able to select some general options:


Files	Concentration	Integration	Preprocessing	Autoselection	Options	
Gene	ral Options					
Conc	entration Average	Calculation:			Weighted Avera	ge 🔹
S	ave to DB					
[[] U	lse Labile Protons					
0	iscard Mismatched	Assignments wh	en Available			
VC	alculate Area Purit	/				
Repo	rting Options					
V R	eport Results in Sp	ectra				
V I	ndude Parameters i	n the Report				

Once the analysis has run the qNMR Viewer can be used. You must navigate to the "results" directory and load the "results.dat" file to get something like this:

	Concentration	RM	IDS	qN	MR%		Spectra	
1 2	20.1604	0. <mark>3</mark> 525		99.3277	r.	AG3682.1	3.fid	
2 2	20.0848	0. <mark>4</mark> 517		99.3154	ŀ	AG3682.1	5.fid	
3 2	20.3183	0.9998		97.2312	2	AG3682.1	11.fid	
4 2	20.1903	0.4424		99.3134		AG3682.14.fid		
5 2	20.4011	0.3092		98.8004	F.	AG3682.1	2.fid	
6 2	20,1073	0.2894		99.3942	2	AG3682.1	6.fid	
7 1	9.9977	0.5416		98.8922	2	AG3682.1	7.fid	
	Multiplet	NN	R	lange	Ab	s. Integral	Concentration	
1	B(m)	2	7.60		47665.	baterres	20.0672	
2	D(m)	1	7.06	5.97	23903.	8798	20.1271	
3	E(s)	3	2.06	2.01	72091	1311	20.2336	

Clicking on each row, will load the dataset in Mnova to allow you to make changes if necessary. The changes made in the Mnova document will be automatically updated in the Viewer.

From the viewer, you can load/save/clear or copy the report to the clipboard (by default). Clicking on the settings button will allow you to change that default (in order to be able to paste the report into Mnova or to save it as HTML):



You can also run Batch qNMR as a **listener**. Mnova can 'listen' to a series of folders or drives and can grab data as is acquired and saved, and run the qNMR analysis automatically, saving the result in the selected folder. The settings for the qNMR listener can be selected under the 'Advanced/qNMR/Automation/Concentration Listener' menu:

	<b>.</b>					
iles	Concentration	Integration	Preprocessing	Autoselection	Options	
Files	Location					
Base	Directory:	C: \Users \Usuario \Desktop \Listener \				
File M	Name:	fid			8	1
Resu	lts					
	tory:	Cult Inerall In	iario\Desktop\Lister	oor\Dogulto		

In that case, we will only need to select the path of the datasets folder, the file name that we want to import (FID) and the path folder to save the results. If the folder contains a .mol file, the applicable molecule will be also loaded.

In that dialog box, we will find the same options for the 'Concentration, Integration, Reprocessing, Autoselection' that we have for the Batch Concentration feature. In addition in the last tab (called Options), we will find an option to select the number of listener folder levels (default value: 2 folders). So by default, the listener will search for the 'File Name' (FID in the example above) in the first two folders of your datasets.


When the listener is working, Mnova will display a dialog box like this:

oncentration Listener	and the second
Listening to C:\Users\Usuario\	Desktop\Listener\

Finally, load the results (in .dat format) with the Concentration Viewer (as it is explained a few lines above).

# 11.3 Purity Calculator script

This new script can be run without a license of the qNMR plugin. You will only need a license of the NMR module. This script is located under the 'Scripts/NMR Tools' menu:

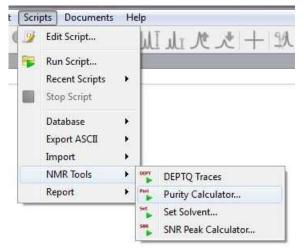


The script method is still heavily used in some Development labs as a final check of compound purity. The spectra used must be of high quality with good shimming, acquired with sufficient time between pulses for full relaxation (typically 20-40 s in DMSO-d6). For processing the spectrum should be well very well phased (manually), and baseline corrected.

The example shown here is typical and doesn't present problems. Practical problems that may arise could be a large broad OH signal (which can sometimes be sharpened by adding a little TFA), or careful baseline correction. Other examples also require that you determine the salt ratio – but we don't deal with that here.


Just load the sample spectrum (which you can download from <u>here</u>) and follow the menu 'Scripts/NMR Tools/Purity Calculator' in order to fill in the sample details and choose the reference compound with the applicable molecular mass of the internal reference and its purity (you can load, modify and add to the reference compound details by loading the csv file that you downloaded in the previous step):

Purity Calculator Options	? ×
Load Previous Parameters	
Load Parameters From File	
Use Parameters From Previous Calculation	
Sample Details	
Sample Mol Weight 410.471	
Weight of Sample (mg) 4.865	
Reference Compound Details	
Load Compound Parameters File	
DMP	•
Reference Compound Purity (%) 98.6	_
Weight of Reference Compound (mg) 1.163	
Use GSD as well as integration	
Calculate salt molar ratio as well	
Re-Calculate	
ОК	Cancel


Clicking on OK, you will be prompted to integrate the signal that will be used as reference compound.

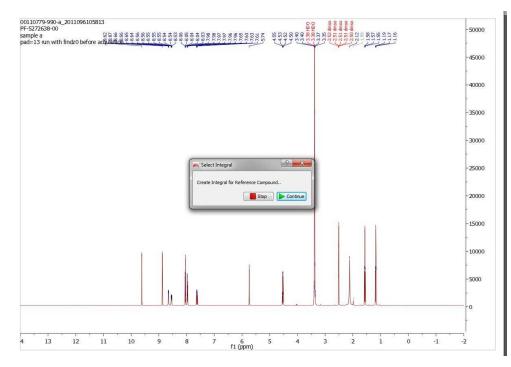

In that case, we will manually integrate the signal at 5.74ppm and click on the 'Continue' button:

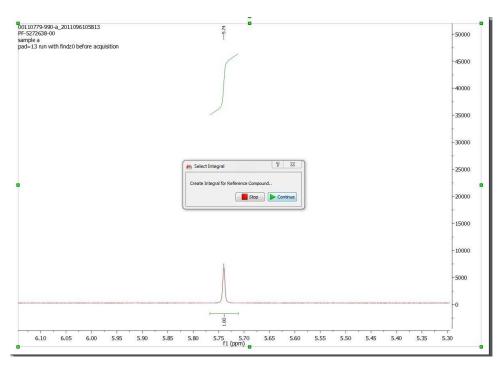


Now, we will integrate 3 multiplets for the analyte (choosing the aromatics close by). Once these have been integrated, click "Continue" again.

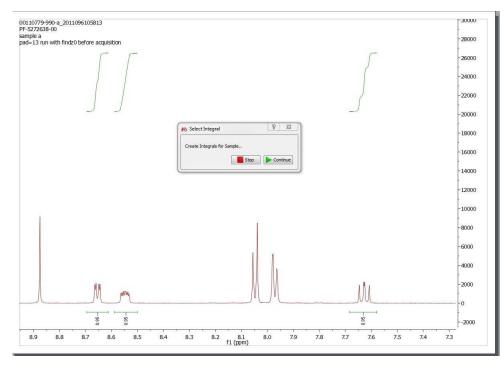

Clicking on the 'Continue button will display the dialog box below:


Purity Calculator Option	15	8
ample Details		
Sample Mol Weight 410.4	171	
Veight of Sample (mg) 4	.865	
leference Compound Deta	ails	
Load Com	pound Parameters File	
DMP		
leference Compound Purit	ty (%) 98.6	
Veight of Reference Comp	oound (mg) 1,163	
Reference Compound I	ntegral	
ntegral 5.49 - 5.95 ppm,	, value = 1	
Nuclide Count	1	
ample Integrals		
📝 Purity = 95.82%		
Integral 7.58 - 7.68 ppr	m, value = 0.95	
Nuclide Count	1	A T
V Purity = 95.84%		
Integral 8.61 - 8.69 pp	m, value = 0.95	
Nuclide Count	1	A V
📝 Purity = 95.34%		
Integral 8.5 - 8.59 ppm	n, value = 0.95	
Nuclide Count	1	×
2	Re-Calculate	
	ave Parameters	
Add report on new page		
nos report on new page		
	ОК	Canci

From that dialog box, if it is necessary, you will be able to adjust masses, see the purity result for each multiplet (they should be similar), see the number of nuclides values and you will be able to change the analyte peaks to be included in the calculation. Once all is OK, click on OK and the report will be added to the spectrum page (if the applicable box was checked) :

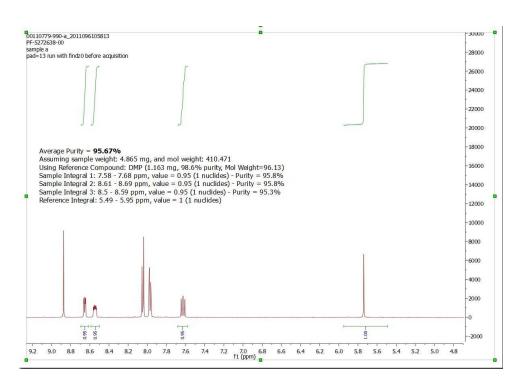

After that, if you plan to work with a similar dataset, you can load the spectrum and re-run the 'Purity Calculator' script, selecting "Use parameters from previous calculation". The only values you would need to change will be the masses.

For further information, please visit our blog: http://mestrelab.com/blog/article/purity-calculation/

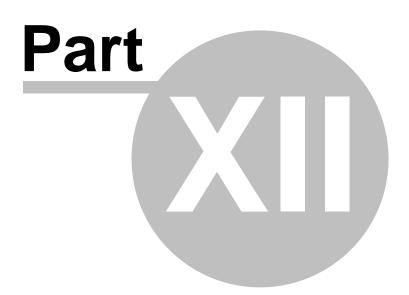

# 12 Scripting with Mnova

### Benefits and uses

The availability of scripting in Mnova provides opportunities and benefits both for skilled NMR and casual, non-expert users:

- Users are less dependent on the application developers for new features since scripting allows them to implement minor features themselves which can be deployed to less expect users.
- NMR administrators can write scripts to customize applications before deploying them to a
  group of users. For example, an NMR manager could create a script to automate some
  particular processing which he can distribute among his users in such a way that they will simply
  have to click one button (e.g. toolbar button) to apply that processing.
- Mnova developers can use scripting to prototype new features that can later be incorporated into the next version of the application. This is ideal when a client requires some processing/analysis feature not available in the application and cannot wait until a new version of Mnova is released.
- Mnova scripting language is based on an ECMAScript-based language making it easier for existing Web developers to customize and extend Mnova.

In essence, nearly everything that can be done with the Mnova graphical interface (UI) can be reproduced with Mnova's scripting module, making it very easy to automate repetitive tasks. For example, you may have to routinely process 1H NMR spectra using the same processing operations. You can create a script which wraps up all these processing functions in such a way that by simply clicking a toolbar button or pressing a keyboard shortcut, all of your 1H NMR spectra will be processed accordingly.

Furthermore, if some particular processing function is not available in Mnova, you can create a script which modifies the spectral data points according to your requirements.

## Introducing Mnova Script – Hello World


A "hello world" program has become the traditional first program that many books use to introduce a programming language. It will act as a cheatsheet for you until you familiarize yourself with the language. The point of this application is to use all the most commonly used elements of Mnova Script language and putting it in a single place so that you can refer to it later. We will start showing the basic elements of an Mnova script and from that point some more advanced methods will progressively be added.

Mnova scripts can be created with any text editor, although Mnova includes a specialized script editor with syntax highlighting and debugging output capabilities. This text editor is available from the Scripts/Edit Script menu command. Issue this command and type in the following text:


<b>⊳</b> • 🖪	🗸 🕨 🔳 🎉 Find:	-
Script		
1 // <gui menuname="HelloWorld" sr<br="">2 function HelloWorld() 3 {</gui>	nortcut="Ctrl+1" tooltip="Hello World" icon="C: /hello,jpg" />	
4 MessageBox.information("H 5 }	tello World");	
Output		

In this example we have defined a function called **helloWorld()** which will simply display a message box with the text 'Hello World'. Note that **MessageBox** is in bold, meaning that Mnova script editor recognizes it as a valid function.

Next, go to the edit control at the top of the script editor and type **helloWorld()**. Do not forget the brackets as they are required by the scripting framework in order to properly interpret the function. Once you have typed it, click on the green arrow at the right side of the edit control. You should get the pop up message box.

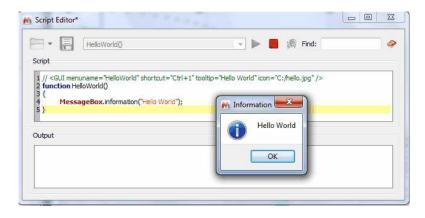

Use the **print** command to write information directly on the **output** control in the script dialog. This is very useful when debugging scripts.

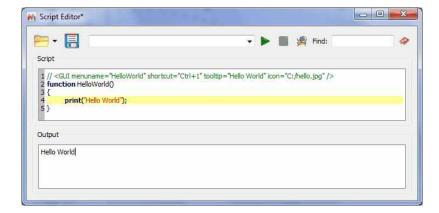



Please note that you will be able to load/save any script by using the applicable buttons The play button will be used to run a script by typing the function on the edit box, whilst the stop button will stop a script in action. Clicking on the 'Help' button or pressing F1 will show you the 'Scripting help' window:


2 Help	×
< 🕨 🕈 💥 🤣   Find:	
GSDPeak	
Index	
A GSD peak	
Enumerations:	
<ul> <li>Flags: Number = {C13Satellite, Hidden, Labile, None, Rotational, Weak}</li> </ul>	
• Types: Number = {Artifact, Compound, Impurity, QReference, Solvent, SReference}	
Properties:	
area: Number [read-only]	
The peak's area	
center: Number [read-only]	
The peak's center position in ppm's	
flags: <u>GSDPeak.Flags</u>	
The peak's flags.	•

As Mnova scripting is an ECMAScript-based language, you can use any of the many functions and statements supported by this standard such as loops, conditions, etc. Remember that JavaScript is ECMAScript based too so if you are familiar with it or with C/C++, writing Mnova scripts should be very easy for you. If you are not familiar with the <u>ECMAScript</u> language, there are several existing tutorials and books that cover this subject, such as <u>JavaScript</u>: The Definitive Guide.

Edit Script	
🍠 • 🔚	
<pre>function helloWorld() {     for (i=0;i&lt;5;i++)         print("Hello World ", i); }</pre>	
Output	
Hello World 0 Hello World 1 Hello World 2 Hello World 3 Hello World 4	× ×

### Where should the scripts be saved?

In principle you could save your scripts anywhere in your computer. However, it's strongly recommended to save them in a custom **scripts** folder, that you can create from the "Edit/Preferences/Scripts/Directories' menu:

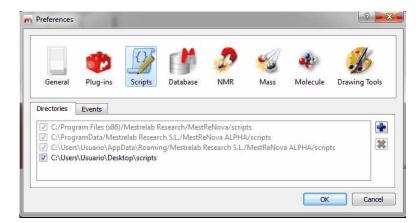


This is very important to allow Mnova to find these scripts when starting in such a way that they can be added to the GUI of Mnova (e.g. Toolbars, Menus, etc).

For example, type the following script:

```
// <GUI menuname="HelloWorld" shortcut="Ctrl+1" tooltip="Hello World"
icon="C:/bin2.jpg" />
function HelloWorld()
{
    MessageBox.information("Hello World");
```

And save it in the scripts directory (program data ...) . Now close Mnova and open it again.




You will appreciate that the script is available in the menu bar. The key to get this working lies in the first line of the script (and of course, in the fact that Mnova can locate the script as it has been saved in the appropriate folder):

```
// <GUI menuname="HelloWorld" shortcut="Ctrl+1" tooltip="Hello
World" icon="C:/bin2.jpg" />
```

This line is used to instruct Mnova about the name to be displayed in the scripts menu along with the keyboard shortcut and the text used as a tooltip. For a full description on the usage of this line, see <u>connecting scripts</u> and <u>Mnova GUI</u> section below.

You can create dialog boxes with controls. The script below shows a simple example.

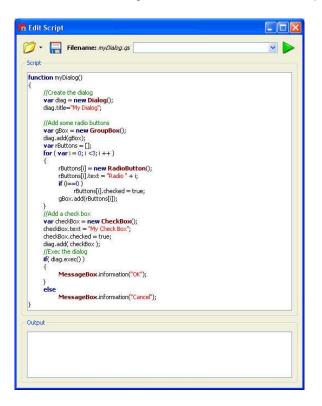

Execution of this script results in the following dialog box:



#### **Scripting Events**

Following the menu "Edit/Preferences/Scripts/Directories', you will find an 'Events' label; which will allow you to add any event (which will run by default in Mnova). You will find an example script about it (eventHandlerExample.qs) in the MestReNova examples script installation folder.

Preference	۲	Database	Mass	 Scripting	Drawing Tools
Shi ms nm nm nm nm nm nm nm nm nm	Events yPress useMove ortcutOverride ChromPeakSchar rAssignmentMida wintegralChange rMultipletClicked rMultipletClicked rMultipletClicked	lighted e d d ted			
					OK Cancel

For example, imagine that you always want to open your 1D datasets with a specific zoom area. You can create an event to do it. To do it, just save this script in your Scripts directories:

```
function spectrumZoom(aJSONString)
     var info = JSON.parse(aJSONString)
     var actDoc = mainWindow.activeDocument
     var spc = new NMRSpectrum(actDoc.getItem(info.itemId));
     if( !spc.isValid() )
          return false;
     spc.horzZoom(1.0, 5.0);
     spc.vertZoom(-100.0,8000.0);
     /*if( spc.dimCount == 1 )
          spc.zoom(3.0, 4.5);
     else
          spc.zoom(1.0, 5.0, 1.0, 5.0);*/
     //spc.zoom();
     spc.update();
     mainWindow.activeWindow().update();
     return true
Application.mainWindow.installEventHandler("nmrSpectrumImported",
"spectrumZoom")
```

Then restart Mnova and select it (spectrum zoom) as an event in the ' Edit/Preferences/Scripts/Events/nmrSpectrumImported' menu. this will open your 1D-NMR spectra with a spectral window from 1 to 5 ppm

	all h	<b>1</b>	2	-	<b>1</b>	()5	<b>S</b> K
General	Plug-ins	Database	NMR	Mass	Molecule	Scripting	Drawing Tools
Directories	Events						
	pectrumImport	ed 🔻					
• *							
Spectr	umZoom						

## **12.1** Connecting scripts with Mnova objects

#### Simple access to an NMR spectrum

The examples we have shown so far are certainly not very useful. The good thing about scripting in Mnova is that it can be used to manipulate objects (e.g. spectra, molecules, pictures, etc) in Mnova and automated repetitive tasks. This section will explain how to access an NMR spectra from within the scripting framework.

Consider the following code snippet:

```
/*globals Application, File, TextStream*/
/*jslint indent: 4, plusplus: true*/
function dumpSpectrum() {
     "use strict";
     //To get the active spectrum
     var d, dumpStream, colCount, rowCount, r, c,
           spec = Application.nmr.activeSpectrum(),
           dumpFile = new File("C:/mnova/dump.txt");
     //The function isValid informs about if the spectrum obtained is correct
     if (spec.isValid()) {
           if (dumpFile.open(File.WriteOnly)) {
                 dumpStream = new TextStream(dumpFile);
                 try {
                       //To dump the spectrum information
                      dumpStream.writeln("Solvent:\t", spec.solvent);
                       //To dump information about each dimension
                      for (d = 1; d \le \text{spec.dimCount}; d++)
                            dumpStream.writeln("Dimension:\t", d);
                            dumpStream.writeln("Frequency:\t", spec.frequency());
dumpStream.writeln("Lowest Frequency:\t", spec.hz());
                            dumpStream.writeln("Nucleus:\t", spec.nucleus(d));
                            dumpStream.writeln("Spectral Size:\t", spec.count(d));
                       }
                       //To dump the values of the spectral points
                       if (spec.dimCount === 1) {
                            rowCount = spec.count();
                            for (r = 0; r < rowCount; r++) {
                                  dumpStream.writeln(spec.real(r), "\t",
spec.imag(r));
                       } else if (spec.dimCount === 2) {
                            colCount = spec.count(1);
                            rowCount = spec.count(2);
                            for (r = 0; r < rowCount; r++) {
```


```
for (c = 0; c < colCount; c++) {
    dumpStream.write(spec.real(r, c));
    if (c < colCount - 1) {
        dumpStream.write("\t");
        }
    }
    dumpStream.writeln();
    }
    }
    finally {
        dumpFile.close();
    }
}</pre>
```

The first thing to note is the **nmr** object. This object gives access to the NMR plug-in framework and as such it allows you to get access to the NMR spectra in Mnova. For example, spec = Application.nmr.activeSpectrum()function makes it possible to select current active spectrum in Mnova. From that point, you can read relevant information of the NMR spectrum such as the number of points, spectral width, etc. For more information about the spectrum properties see the reference.

Let's now move to a more comprehensive example which will illustrate, step by step, how to access all objects within an Mnova page.

#### Having access to multiple objects: the layout script

As an illustrative example, we will build a script which will make it possible to organize different objects contained within a page. This script will be called **layout** for obvious reasons. To start off with, open a spectrum, a molecule and a picture (which could be, for example, your company logo). The following picture shows the initial conditions for this example:

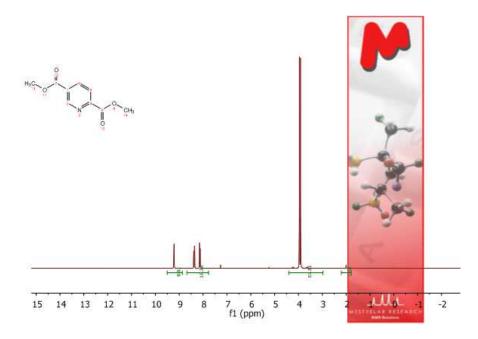

The goal here will be to create a script which will arrange these 3 objects in such a way that the picture will be located at the left side of the page whilst the spectrum and the molecule will be moved next to the picture.

```
//<GUI menuname="Layout" shortcut="Ctrl+1" tooltip="Layout"/>
/*globals Application*/
/*jslint plusplus: true, indent: 4*/
function layout() {
     "use strict";
     var item, i,
         d = Application.mainWindow.activeDocument,
          p = d.curPage(),
          n = p.itemCount();
     for (i = 0; i < n; i++) {</pre>
          item = p.item(i);
          if (["NMR Spectrum", "Molecule", "Image"].indexOf(item.name) !== -1)
                item.translate(p.left - item.left, p.top - item.top); // Move
the item so that its top-left position coincides with page's top-left
          }
          switch (item.name) {
          case "NMR Spectrum":
                item.left = item.left + 50; // Move the spectrum 5 cm right
in order to give space for the logo
                item.right = p.right;
                                         // Resize the spectrum item in order
to take rest of the page
                item.bottom = p.bottom;
                                                // -"-
                break;
          case "Molecule":
                item.translate(50, 30);
                                              // Move the molecule to be
placed below the spectrum title
               break;
     d.update();
```


Every object in Mnova is contained in a page which in turn is contained in a document. So the first thing we should get access to is the document. This is done in this line:

d = Application.mainWindow.activeDocument,

Basically we access to the document window (<u>DocumentWindow</u>) via the **Application** object. Once we have the document, we can easily access to the currently active page through <u>Page</u> object like this:

p = d.curPage()

Now we are ready to navigate through all the objects contained in this page. For every object, the exact type is checked within the switch command and then the objects are repositioned accordingly. This is the result for this example.

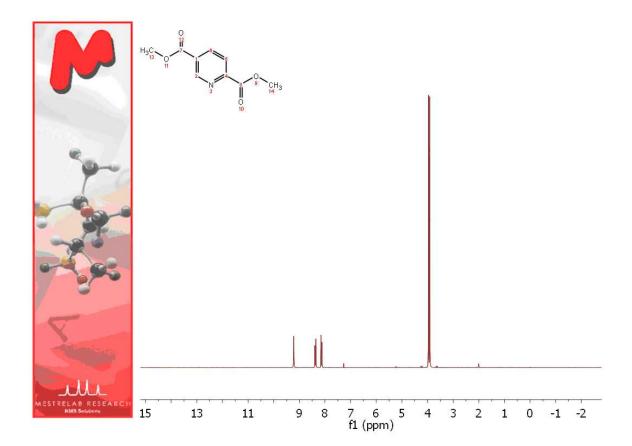

## Tuning up the layout script

We will now modify the layout script in order to achieve the following two objectives:

- 1. Load the image from a file
- 2. Show the spectrum title automatically on the page when the script is executed

First off, we will show how to load an image from the disk. To do that, you have to use the <u>serialization</u> object. For example, assuming that the image is located in c:/mnova/logo.png, you can use this code:

```
serialization.open("c:/mnova/logo.png");
```

Next thing is how to show some parameters (Spectral Width, Solvent, Nucleus) on the page. In order to do that, it will be necessary to create a specialized NMR spectrum object rather than using the default properties available in every item object. See the following code snippet:

The complete new script looks like this:

```
//<GUI menuname="Layout2" shortcut="Ctrl+2" tooltip="Layout"/>
/*globals Application, serialization, NMRSpectrum, draw*/
/*jslint plusplus: true, indent: 4*/
function layout2() {
     "use strict";
     serialization.open("c:/mnova/logo.png");
     var item, i, specItem, textItem,
          d = Application.mainWindow.activeDocument,
          p = d.curPage(),
          n = p.itemCount();
     for (i = 0; i < n; i++) {
          item = p.item(i);
          if (["NMR Spectrum", "Molecule", "Image"].indexOf(item.name) !== -1) {
                item.translate(p.left - item.left, p.top - item.top); // Move the
item so that its top-left position coincides with page's top-left
          }
          switch (item.name) {
          case "NMR Spectrum":
                item.left = item.left + 50;
                                               // Move the spectrum 5 cm right
in order to give space for the logo
                item.right = p.right;
                                         // Resize the spectrum item in order
to take rest of the page
                                                 // -"-
                item.bottom = p.bottom;
                specItem = new NMRSpectrum(item); // Create this object in
order to access spectral parameters
                textItem = draw.text(
                                                      // Generate a text item
with the parameters to report
                      "<b>Frequency (MHz): </b> \{0\}<br/>
                     <b>Spectral Width (Hz): </b> {1}<br/>
                     <b>Solvent: \langle b \rangle \{2\} \langle br/\rangle 
                     <b>Nucleus: </b>
{3}".format(specItem.frequency().toFixed(4),
specItem.scaleWidth().toFixed(2),
                                                      specItem.solvent,
                                                      specItem.nucleus()),
                     true
                );
                // Move the text item to the right-top part of the spectrum
                textItem.translate(specItem.right - textItem.width - 20 -
textItem.left, specItem.top - textItem.top);
                break;
          case "Molecule":
                item.translate(50, 30);
                                           // Move the molecule to be placed
below the spectrum title
               break;
     d.update();
```

Once you have the script saved (please bear in mind that the script file will need to have the same name as the function which you want to call, in this case the name of the script must be 'layout2.qs') in the Mnova scripts folder (and then have restarted the program), you will be able to add it to the toolbar just by following the menu: 'View/Customize User Interface/Customize Toolbars'. This will display the

'Customize Toolbars' dialog box. Then, click on the '+' button to create a new toolbar and type its name (Scripts Toolbar) by clicking on the 'Rename' button.

n Customize Toolbars	? 🛛
Actions	Toolbars 💽 😵 Rename
<separator> Alignment Align Align Tile Bring to Front Bring Up Send Down</separator>	2D NMR Alignment Scripts:Toolbar MMR Process Spectrum View Stacked NMR
Send to Back Align Left Align Right Align Right Align Bottom Align Bottom Center on Page Vertically Center on Page Tile Spectra Hori&zontally Tile Spectra Ve&rtically	Current Toolbar Actions
Tile &Horizontally Tile &Vertically Draw &Select &Line &Rectangle &Ellipse	
Restore All	OK Apply Cancel

Next, navigate to the 'Script' icon (Layout2) in the 'Actions' menu (at the left-hand side of the window) and Click on the 'Right Arrow' button to add the 'Layout2' script to the 'New Toolbar'.

Actions	Toolbars	- E	Rename
Delete Setup Report Special Copy Special NMR Predict 1&H Spectrum Predict 1&H Spectrum Prediction &Options Scripts Layout2 Multi Open Angewandte Angewandte Angewandte Angewandte Angewandte Angewandte SACS Spectrum Coom &Out Scom &Out Scom &Out Spectrum Scom &Out Spectrum Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Scom &Out Spectrum Spectrum Scom &Out Spectrum Scom &Out Spectrum	2D NMR     Alignment     Annotations     Scripts Toolbar     Main     NMR Process     Spectrum View     Stacked NMR     Text      Current Toolbar Actions     Imple Layout2      Imple Layout3      Im		

Finally, click on OK and you will be able to see the 'Layout2' icon in the 'New toolbar'. You will also be able to introduce the script in any existing contextual menu by following a similar procedure in the 'Customize Context menus' dialog box.

## **Custom NMR Processing**

There are two ways to process NMR spectra via scripting:

- 1. By means of Processing Templates
- 2. By using the Processing interface

## 1 Processing templates

Mnova is able to process a 1D or 2D NMR spectrum via scripting by using the processing templates (generated with the Full Processing feature). As you can see in the below example, you can process (with an easy script) any kind of spectrum (1H, 13C, 1D or 2D). You only need to create the processing template for each experiment. In the example below we have created 3 different processing templates, one for the processing of 1H-NMR spectra (1H.mnp), the second for the processing of 13C-NMR spectra (13C.mnp) and the last one for the processing of COSY spectra (COSY.mnp). As you can see in the scripts, the three the templates were saved at c:/mnova/ (of course you can change this path and also the name of the template files).

```
/*globals Application*/
/*jslint indent: 4*/
function procTemplate() {
    "use strict";
```

```
var procFileName,
     spec = Application.nmr.activeSpectrum();
if (!spec.isValid()) {
     return;
if (spec.dimCount === 1) {
     if (spec.nucleus() === "1H") {
          procFileName = "c:/mnova/1H.mnp";
     } else if (spec.nucleus() === "13C") {
          procFileName = "c:/mnova/13C.mnp";
     }
} else if (spec.dimCount === 2) {
     if (spec.nucleus(1) === "1H" && spec.nucleus(2) === "1H") {
          procFileName = "c:/mnova/COSY.mnp";
     }
if (procFileName) {
     Application.nmr.processSpectrum(spec, procFileName);
}
```

## 2 Processing interface

The <u>Processing</u> interface makes it possible to change or apply any processing operation available in Mnova.

For example, let's make a simple script which will set an exponential weighting function:

```
/*globals Application*/
/*jslint indent: 4*/
function myProcess() {
    "use strict";
    var spec = Application.nmr.activeSpectrum(),
        p = spec.proc;
    p.setParameter("Apodization[1].Apply", true);
    p.setParameter("Apodization[1].Exp.Apply", true);
    p.setParameter("Apodization[1].Exp.Value", 0.5);
    spec.process(p);
    Application.mainWindow.activeDocument.update();
}
```

After creating a spectrum object which represents current active spectrum, we create a processing variable (p) which represents the processing operations for that particular spectrum. Once this new object is created, we can read or change its values using getParameter and setParameter functions. For instance, in this example we first set to true the Apodization property (otherwise no apodization will be applied) and then, after setting to true the exponential function, we set the line broadening to 0.5 Hz.

Finally, when we are done, we assign this processing object to the spectrum object (p = spec.proc;) and we call spec.process(); to actually apply all the processing operations.

## 12.2 Connecting scripts with Mnova GUI

As you have seen in the examples above, you can insert any script in the Mnova Scripts menu, contextual menus or toolbars.

The key to get this working lies in the first line of the script (and of course, in the fact that Mnova can locate the script as it has been saved in the appropriate folder):

// <GUI menuname= "MyProcess" shortcut="Ctrl+1" tooltip="Exponential

#### 0.5" icon="C:/bin2.jpg" />

This line is used to instruct Mnova about the name to be displayed in the scripts menu along with the keyboard shortcut and the text used as a tooltip. Please bear in mind that the user is also able to use any created image file as icon. In this case, the name of the script is *MyProcess*, the shortcut is *Ctrl+1*, the tooltip is *Exponential 0.5* and the icon used was saved at *C:/bin2.jpg*.

You will be able to see in the picture below, that we have added the script 'MyProcess' to the 'Scripts' menu with the corresponding shortcut (Ctrl+1) and that we have introduced our own icon in the toolbar (red square in the picture below).



Please bear in mind that the script file will need to have the same name that the function which you want to call, in this case the name of the script must be 'MyProcess.qs', because the name of the function is: myProcess().

### 12.3 Mnova processing scripts

This reference contains a list of objects, functions and properties supported by Mnova script. For a complete ECMAScript Reference, consult this link: <u>http://doc.trolltech.com/4.3/ecmascript.html</u>

Example scripts are present in the examples/scripts installation directory and some of them are described <u>here</u>.

You can see <u>here</u> the Mnova script reference documentation, in the Mnova installation folder ('documents/scripts'), or by clicking on the 'Help' button in the scripts editor (or pressing F1 key).

#### NMRProcessing. Describing Processing parameters (Argument Strings).


You will find <u>here</u> (or in the Mnova installation folder: 'documents/scripts') a list of the argument strings (which have the form *function1.function2...functionN.parameter*) that you will be able to use in your processing scripts. These parameters appear in the graphical interface of the software (in the 'Processing / Full Processing' menu) and are described in depth in the <u>manual</u> of Mnova.

Full Processing       Image: Second state st	the correction
Image: Second	od: Imported -141 -4.39315
Exponential: 0.5 Hz Ref Zero Filling and LP	od: Whittaker Smoother an Filter: Autodetect oth Factor: Autodetect oothing erese erence solute Reference on Reference: : 400 ctor: : 100.000000


You can load a saved processing template by running this easy script:

```
//<GUI menuname="ApplyProcessingTemplate"shortcut="Ctrl+2"tooltip="Apply a saved processing tem
function ApplyProcessingTemplate()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    var processing = new String;
    if (!spec.isValid())
    return;
    processing = "C:\\ProcessingTemplate.mnp";
    nmr.processSpectrum(spec, processing);
    spec.process();
    mainWindow.activeWindow().update();
}</pre>
```


Here you can see additional examples. This is a script to apply an Exponential apodization function of 0.5 Hz:

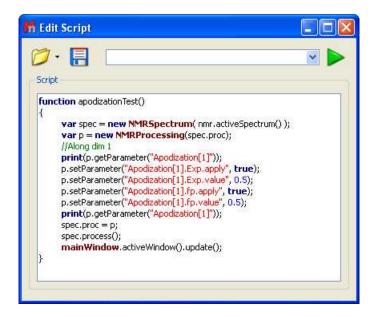


Here you can see an example to Bin your spectra with 0.025 ppm:

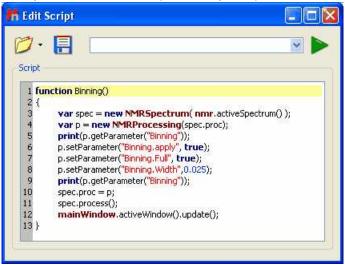

This is an example to apply a phase correction:

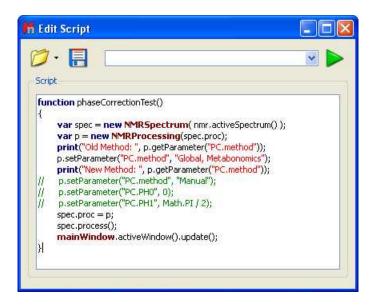


And this script can be used to reference your spectra:

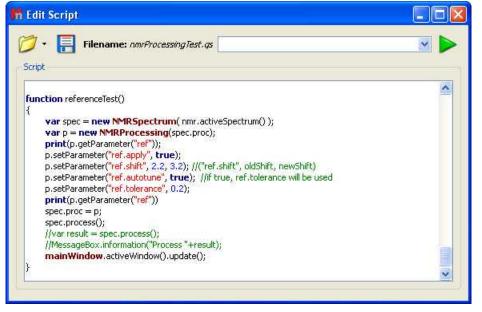

You will find in the example/scripts folder a script called "customImportProcessing.qs", which will allow you to import your NMR spectra without applying any processing. If you add this script to a 'Script directory' you will obtain just the FID of your datasets.

You can also edit the "customImportProcessing.qs" script to always apply a baseline correction when you import a dataset.

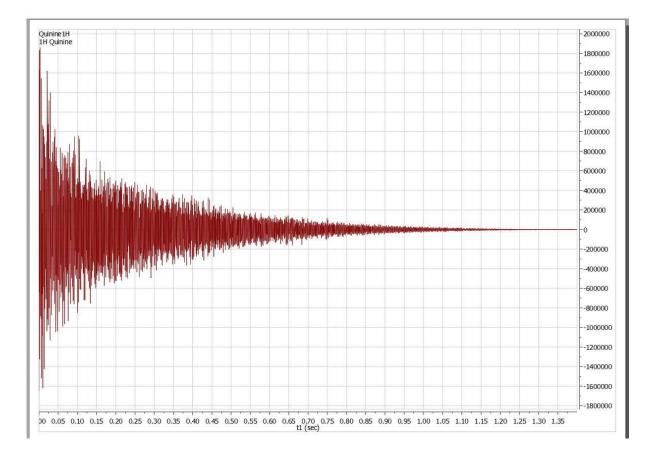

## 12.4 Mnova properties scripts

### NMRSpectrum.getProperty/setProperty Arguments

You will find <u>here</u> (or in the Mnova installation folder: 'documents/scripts') the spectrum properties ( *aParamName*) that you can manage via script, by using the functions <u>'SetProperty</u>' and <u>'GetProperty</u>'. You will find an example script in the examples/scripts installation directory and also in the <u>'Script</u> <u>Samples'</u> chapter. All of these properties can also be selected by using the GUI:

Seometry N	MR. Spectrum		
M	2D Spectrum 1D Spe	ctrum Common	
Spectrum	V Legend		
82	<u>W</u> idth:	4.23 mm	
Scales	Text Width:	12.70 mm	
Peaks	Palette:	Standard	• 8
Peaks	Number of Positive Con	itours:	10
Jax .	Number of Negative Co	intours:	10
Integrals	Scaling:		2.000 🜩
	Ploting method:	Bitmap	•
	Traces		
	I Horizontal:	Projection	•
	Vertical:	Projection	•
	Size		
	Horizontal:		25.00%
	Vertical:		25.00%
			Same size

You will find below an example of a script to change some properties of your spectra. In this case, the colour of the spectrum will be changed to red, the peaks font to Arial and the integral curves will be showed.

```
function properties()
{
    var spec = new NMRSpectrum(nmr.activeSpectrum());
    spec.setProperty("curve.color","red");
    spec.setProperty("peaks.font","Arial");
    spec.setProperty("integrals.curve.show", true);
    spec.update();
    mainWindow.activeWindow().update();
}
```

## 12.5 GUI Actions


You will find <u>here</u> (or in the Mnova installation folder: 'documents/scripts') the GUI actions that you will be easily able to run with an easy script. The script below will apply an "Auto Peak Picking" analysis:

```
function doActionTest()
{
mainWindow.doAction("nmrAutoPeakPicking");
}
```

If you want to run any other action just replace the red action with any action of the the list below. Of

course, you can add to the script as many actions as you want.

Here you can see an example of this tool to apply several actions to all the spectra opened in the same document:

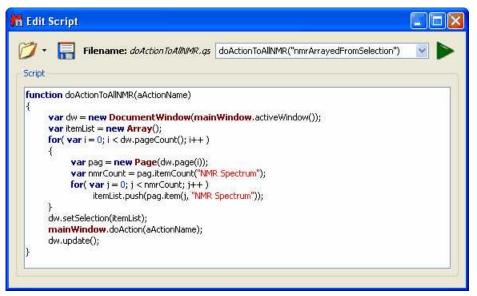

This script will generate a stack plot of all the opened spectra. You can use this script to run whatever doAction you c

## 12.6 Running Scripts from the command line

You can run scripts from the command line, just by typing the paths where the Mnova .exe file and the script are located and -sf "name of the script function": "mestrenovaPathname" "scriptPathname" - sf "scriptFunctionToRun"

For example:

#### 1. mestrenova scriptPath

For example: mestrenova c:\temp\multiOpen.qs will run the function multiOpen() from multiOpen.qs file, i.e. it runs a function with the same file name.

#### 2. mestrenova scriptPath -sf functionName,arg1,arg2,...,argN

This runs functionName(arg1, arg2, ... argN) from the scriptPath file.

#### The below command line is doing the same as the above one: mestrenova -sf functionName,arg1,arg2,...,argN scriptPath

#### Examples:

You can also use: "mestrenovaPath" "scriptPath" -sf "scriptFunctionToRun"

"C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" "C:\Program Files \Mestrelab Research S.L\MestReNova\scripts\myScript.qs" -sf "myFunction" It is also possible to specify arguments:

"C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" "C:\Program Files \Mestrelab Research S.L\MestReNova\scripts\myScript.qs" -sf "myFunction",0.1,10,true,off

In this case, MNova will run myFunction(0.1,10,true,"off") from myScript.qs with the arguments specified. No spaces after commas!

#### 3. mestrenova -sf functionName,arg1,arg2,...argN

In this case it is supposed that the function functionName is taken from one of the script directories, either MNova standard or user defined.

Note: Command line arguments are separated with white-spaces. This is why it is important not to use white-spaces after commas. If script arguments contain white-spaces then use quotes: "C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" -sf openSpecWithMols,"C:\1H\fid".

This doesn't need quotes: "C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" -sf openSpecWithMols,C:\1H\fid

Complex case example: mestrenova specPath1 specPath2 -sf functionName,arg1,arg2 specPath3 specPath4

This will first open the spectra specPath1, specPath2, specPath3, specPath4. Next, apply the script: functionName(arg1, arg2)

There is also a single command line parameter **-w** (w stands for wait). If this parameter is present in the command line and there is no Mnova already running, then Mnova will open, load any files and run any scripts passed in the command line and, finally, it will close.

If this parameter is present but Mnova is already running, then the second Mnova instance will pass the command line information to the first running instance, the first running will load/run files/scripts and finally it will notify to the second instance that it has finished, so the second instance will close.

Some examples:

#### MestReNova.exe -w

Mnova not running: Mnova opens and closes immediately. Mnova running: The second Mnova instance will return immediately.

#### MestReNova.exe myscript.qs -w


Mnova not running: Mnova opens run the myscript function in the myscript.qs file and closes when it finishes.

Mnova running: A second Mnova instance is run and passes the parameters to the already running one. The myscript function from the myscript.qs file is run in the already running Mnova instance and when it finishes, notifies the second one and the second one Mnova instance (the one you have started from the command line) it closes.

## 12.7 Import spectra

There are some specific spectral formats (such as ACD Labs, LC Model ASCII, Philips Achieva or Siemens Syngo) which can only be imported in Mnova by using the scripting engine.

To import these kinds of spectra, just run Mnova, follow the menu Scripts/Import and select the desired format

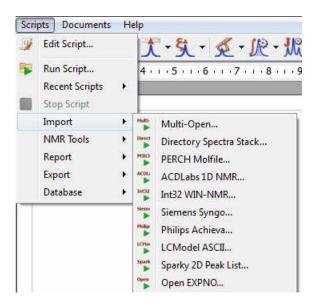

The user can use these scripts as a starting point to import any other spectral format. If you need help about it, just <u>contact us</u>.

**MultiOpen script:** Mnova incorporates a script named 'MultiOpen' (under the 'Scripts/Impor't menu). This tool is very useful if, for example, you always process your spectra in the same way, or when you have to routinely handle a large number of datasets.

'Multiopen script' allows to open simultaneously a collection of several spectra. Make sure that all spectra are located in the same folder. After that, select 'Run Script...' on the 'Script Menu' or click on

the **'Run Script'** icon **w** on the toolbar and then click 'Ok' after finding the corresponding script (in this case, the script is called 'multiOpen'). Then, select the directory where the spectra are located and a window like the one below will open:

Multi-Open	-	
Main Files		
C:\Users\Usuario\Desktop\spectra	•	
*/13C/fid		•
Optional Files C:\Users\Usuario\Desktop\mol	÷	
*/*.mol		•
ОК	Car	ncel

Finally, write the 'Path Mask' name (you can use wildcards, so this could be, for example, \*/10/pdata/1r, or just \*/fid, or \*/ser), and click 'OK'. All selected spectra will open simultaneously.

The user can also use the 'Full Processing' command to automate the processing of both 1D & 2D NMR data sets. (You can find a full description of this tool further on in the <u>Automated Processing</u> chapter.)

You can also extend this script to run batch predictions. Please email us if you need such script.

Mnova includes a powerful script which makes it possible to import all spectra (1D, 2D, mnova

documents, etc) contained in a folder and automatically stack them for forthcoming R-M analysis. This script is under the Scripts menu and it is called '**Directory Spectra Stack**'. It will allow the user to select the directory where the spectra are contained. Then Mnova will open and process all those spectra (FIDs) automatically in bunches of 20 spectra and finally will stack all of them.

Ŷ	Edit Script		0
	Script Directories		
\$	Run Script Recent Scripts	•	
	Verification Export ASCII Export Bruker Time Corrected FID	* *	
	Import	•	ACDLabs 1D NMR
	Report NMR Analysis		

Note: This script has also the option to decimate the spectra while loading (i.e. the program can skip every 10 spectra in the data set) and to apply a processing template (or to load the 1r processed data):

Import Sp	oectra Stack		? ×
Data Folder:	\rxnMon - neat-ac	etylacetone-42 2016-02-04 044	2PM
Order:	By Name		•
File Path Fi	Itering		
File Name	Masks:	fid *.fid *.jdx	
Folder Nan	ne Masks:		•
	Ρ	review Files	
Spectra	l Data Filtering		
Parameter	Nucleus	=	
First Spect Chunk Size		Number of Chunks:         1           Step to Next Chunk:         97	A V
Visualizatio View:	n	Decimation Step: 10	×.
File:	ing Template		
Folder: C	:/Users/Usuario/Ap	pData/Local/Temp	
		ОК	Cancel


The script will firstly apply the spectral data filtering and then the data chunking. The 'Preview Files' button will preview inside the File Path Filtering in order to list all files which will be processed.

- Chunking: the check box will disable/enable the feature, allowing the user to define data intervals. If the 'Number of chunks' checkbox is disabled, it will take all chunks since it found the first spectrum (going up to the end). For example, the settings above could be used to get a stack of just the first 96 spectra. The script will not go on importing the rest of the spectra to end of the directory.

You can change the 'default import' options for your datasets, just by using the 'ImportProcessing' script. You will find an example of that script called "customImportProcessing.qs" in your Mnova installation folder. You can freely edit this script to make your own automatic import processing options or even you can create 'Processing Templates' that will be applied automatically over your spectra after having loaded them in Mnova.

# 12.8 NMR Tools

You will find several scripts under the 'Scripts/NMR Tools' menu:

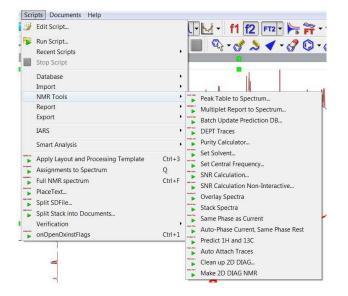

#### Peak Table to Spectrum

This script will allow you to synthesize a NMR spectrum from a peak table:

1	dit Script un <mark>S</mark> cript	f	] f2	×9. • ∮	- 伬 - 坬 - <u>坎</u>	• 🥑 🕨 📲		_
	ecent Scripts top Script	• ru	m					-
	nport IMR Tools	•						? <mark>-</mark> 2
R	eport kport	<ul> <li>Peak</li> <li< td=""><td>Multiplet Report to Spectrum</td><td></td><td>Spectrum Simulatio</td><td>on</td><td></td><td>0</td></li<></ul>	Multiplet Report to Spectrum		Spectrum Simulatio	on		0
1.11	atabase	0071	and the second		Shift (ppm)	Width (Hz)	Intensity	
_		Purk	Purity Calculator		1 1	0.75	1	*
		Set S			2 1.3	1.75	2	
		Over	SINK Peak Calculator		3 1.35	0.75	1	
ð×		stad	Charle Consider		4 1.43	2	3	1
^		Sente	Same Phase as Current				Looperation	k .
		Prest			Spectrum			
			Fiedict In and ISC		Nucleus: [1H	▼ Spectrum	Size 32768	•
					Frequency: 400.00	MHz 💽 Default Lir	ne Width: 0.75 Hz	
		-			From: -2.00 p	pm 🔹 To:	10.00 ppm	۲
	•						ОК	Cancel

#### **Multiplet Report to Spectrum**

To synthesize a spectrum from a multiplet report copied from a paper. See this <u>chapter</u> for further information.

DEPT traces. See this tutorial to process Varian DEPT spectra

Purity Calculator. See this chapter

**Set Central Frequency.** It allows to set the center value of a spectrum by entering a value (in Hz) for f1 (in case of 1D spectra) or f1 and f2 (in case of 2D spectra). The last f1/f2 value used is remembered the following time you open the dialog (the first time the dialog shows the center value of the current spectrum). If several spectra are selected in the page navigator, the entered value is applied to all the selected spectra with equal dimensions.


#### Signal to Noise Ratio Calculation

To calculate the SNR. The script will get the noise level and then calculate the SNR by measuring the height of a peak and dividing this value by the noise level.

After running the script, it's necessary to select a signals-free region to calculate the noise and press 'Continue' (if you have not applied apodization, you could skip this step):

h SNR Peak C	Calculator	
	s-free region to calculate the n to allow Mnova to calculate this	
the whole spec	ctrum	

Next, select the region of the spectrum (or just a single peak) where you want to calculate the Signal to Noise Ratio. Once this is done, the program will populate the 'comment' section in the Peak List table with the SNR values.

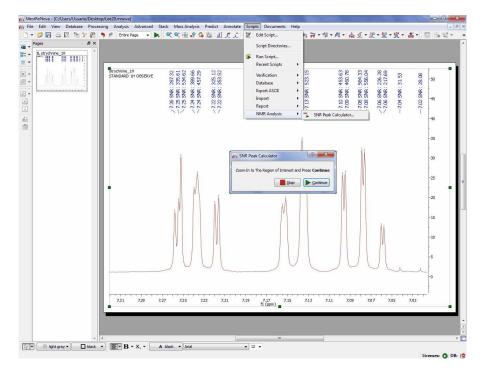

The script to calculate the SNR needs to have two parameters:

- 1) The noise value
- 2) The peak intensity

Then it calculates the SNR using a ratio between those parameters: SNR = Y / noise;

Where Y is the amplitude of the peak and noise is the root-mean-square deviation calculated in a signal free area of the spectrum.

The noise value can be calculated either manually or fully automatically, as follows:

a) Manually. The user needs to select a 'signals-free' region' in the spectrum where the noise will be calculated according to this formula:

$$\sqrt{\sum}(Y_i - Y_m)^2 / (N-1)$$

where:

N = number of points of the signal-free region

 $Y_i$  = value of each digital point in the spectrum (real part)

 $Y_m$  = average of the digital points (real part) in that region

b) Fully automatic (which is different with Bruker); the user does not need to select any region of the spectrum.

With respect to the peak intensity, the script uses the peaks in this way:

1. If the user did a manual peak picking (or Peak by Peak or an automatic PP), the program will use those peaks in the zoomed region.

2. If the user did not applied any PP, the script will apply it for the user over the selected region using the automatic PP options.


# SNR Peak Calculator "Non interactive"

This script will allow the user to select the noise region and the region of interest in order to get the applicable 'signal to noise ratio':

	e Settings					
	8					
Noise Re	gion					
Start X:	13.0000	4	End X:	10.0000	ф р	pn
Signal Re	egion					
Start X:	1.5000	*	End X:	3.0000	🌲 p	pm

## **Overlay/Stack Spectra**

You can 'stack or overlay' the selected spectra **plots** by clicking on the options "Overlay Spectra" and "Stack Spectra" available in Scripts/NMR Tools menu. The result will not be a real stacked/overlaid spectrum, instead of that, you will get the spectral windows stacked or overlaid, allowing you to freely move them up&down, as each spectrum will be an independent item:

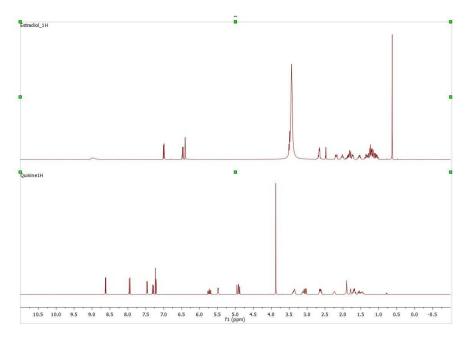


### Scripts to autophase importing autophase stacked spectra when importing.

Following the menu 'Scripts/NMR Tools', you will find a couple of scripts to apply automatic phase correction to a stacked plot:

Scri		
2	Edit Script	たえ 🔶 外・ 🚹 f2 🥅
	Run Script Recent Scripts → Stop Script	
	Database + Export ASCII + Import +	TIIR 14
	NMR Tools	DEPTQ Traces
-	Ref: Sample	Auto-Phase Current, Same Phase Rest
		Same Phase as Current
	Desktop/T1 <del>Ref. Sample</del>	Set Solvent SNR Peak Calculator

- Auto-Phase Current, Same Phase Rest: the active spectrum is automatically phase corrected, and the resulting values of PH0 and PH1 are applied to the other spectra in the stacked.
- Same Phase as Current: PH0 and PH1 values of the active spectrum are applied to the other spectra in the stacked.
- Set Solvent: it can be used to change the 'solvent' in the Parameters table in the case that the solvent is wrong or missing. You can select several pages in the same document and change the solvent to all of them by using this script.

The script 'Predict 1H and and 13C' will generate a plot with both predictions from a given molecular structure (a license of NMRPredict Desktop is needed):

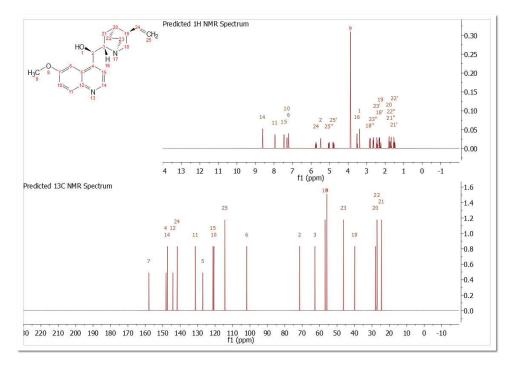


The script **'Auto Attach Traces'** will automatically setup the 1D spectra as external traces of a 2D (all the spectra must be in the same document).

The script **'Make 2D DIAG NMR'** will synthesize a 2D spectrum from a 1D experiment so that the latter will be the diagonal part of the 2D spectrum. It could be useful to obtain 2D pure shift spectra by using Indirect Covariance NMR. <u>See this paper</u> for further information.

# 12.9 Report


We have some scripts to report your <u>multiplets</u>, <u>peaks</u> list, <u>assignments</u>, etc under the 'Scripts/Report' menu:

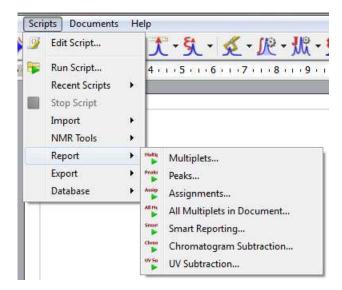

It is possible to export your **assignments** in journal format by following the menu 'Scripts/Report/Assignments'. Then, a dialog will appear, from where you can select to the correlations H-H and C-H to be shown, to copy only to the clipboard or paste to the document and to order by chemical shift.


Options		
📝 Include 13C and X-Nuclei Assignment	ts	
Include Multiplicity		
Include Number of Nuclides		
Order by Chemical Shift		
🔽 Only Copy to Clipboard		
Export To File:		
() Text (TSV) () HTML		
Decimal Places For 1H:	2	4
Decimal Places For13C and X-Nuclei:	1	Å
2D Correlations		
Format:		
<sup>(n)</sup> <sup>(</sup>	tom(δ)	
Drop Lines Without Correlation		
ОК	Cance	-1

Finally, you will get the report of the assignments pasted on the spectral window:

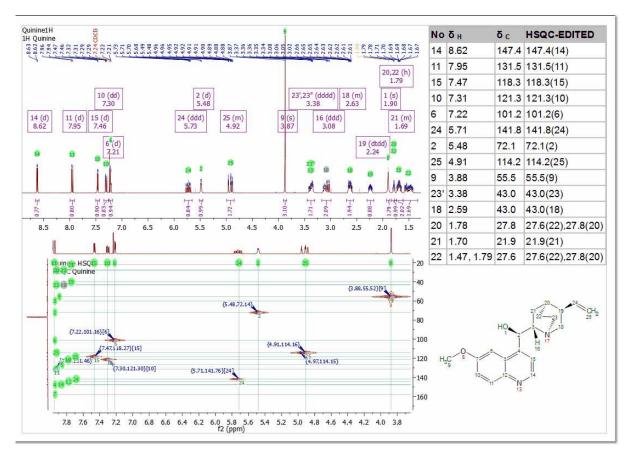

## **All Multiplets in Document**

Follow the menu 'Scripts/Report/All Multiplets in Document' to generate multiplet reports in each spectral page of a document:

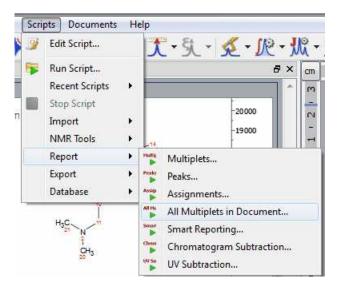

## **Smart Reporting**

This script will allow you to load a layout template, with the option to include the applicable processing template embedded in the layout or to load other processing templates. The script will allow you also to

js1\_jspmsant\_dil DRX\_500 1H 14 6" (qd) 1.72 4 (ddd) 2.04 Smart Reporting ? × 10 (d) 3 (dq) 2.45 (d) 6' (qd) 7" (td) 13 1.83 1.52 Lavout Template ar/smart processing/template.mnova File: 6',7' (ddd) 1.93 Apply Processing Processing Templates 4 7 6' 6" 1H File: ... 13C File Spectral Widths 7.0 6.5 5.5 3.0 2.5 2.0 1.5 1.0 6.0 Spectra From То s1\_jspmsant\_dil DRX\_500 1H 1 H1 0.5 7.5 2 C1 0 200 Update Table Apply Vertical Scaling 14 Vise Settings from Last Run 11 OK Cancel 40 00 190 180 170 160 150 140 130 120 110 90 80 70 60 50 30 20 10 100 f1 (ppm)

select 'Spectral Widths' for each nuclei:

See also <u>'Background and UV subtraction'</u>

# 12.9.1 Scripts Samples

All the scripts are present in the examples/scripts installation directory. Some of them will be described in this chapter. Please bear in mind that it is also possible to run scripts from the command line, just by typing the path where the Mnova .exe file and the script are located and -sf "name of the script function": "mestrenovaPathname" "scriptPathname" -sf "scriptFunctionToRun"

For example:

"C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" "C:\Program Files \Mestrelab Research S.L\MestReNova\scripts\myScript.qs" -sf "myFunction" It is also possible to specify arguments:


"C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" "C:\Program Files \Mestrelab Research S.L\MestReNova\scripts\myScript.qs" -sf "myFunction",0.1,10,true,off

In this case, MNova will run myFunction(0.1,10,true,"off") from myScript.qs with the arguments specified. No spaces after commas!

**SendEmail:** It is possible to send an email containing attachments (it needs Python installed in the same computer).

Send Email	and the second		
From:			Settings
To:			
Subject:			
This is a test			
Attachments:		Rich	Text 🔲 Source
Attachments:	Files	📝 Rich	Text Source
Attachments:	Files	<b>⊘</b> Rich	

When the email is sent a message is shown:



testFilePermissions: this script will allow you to generate 'read-only' documents.

**customImportProcessing:** This script can be used to change the way of Mnova imports your NMR spectra. For example to stop the processing in the FID. Please follow the procedure below to set this script by default:

1: Go to 'Edit/Preference/Scripts' and add a new folder to sample scripts by clicking on the 'blue plus button'

2: Save this script as a .qs file to the folder above.

3: Restart Mnova and load a 1H-NMR dataset. You will get your spectrum without any processing (just the FID).

**Open and Save Document Script:** Let's take a look at an easy script which you can use to open a . mnova file and export it as a PDF file. In this case, we will open a .mnova file named 'Dimethoxy':


function openSaveDocument()

//If the open function gives a 'false', it will mean that Mnova does not recognize the file

```
if (serialization.open ("/dimethoxy.mnova"))
    {
          print("File Opened");
          //Let's see what the document contains
          //To get the active document
          var dW = new DocumentWindow(Application.mainWindow.activeWindow());
          //To get information about the number of the pages of the document
          print(dW.pageCount());
          //To print the number of items and the description of them for each page
          for( var i = 0; i < dW.pageCount(); i++ )</pre>
          {
                 var pag = new Page(dW.page(i));
                 print ( "Page number "+i+" has "+pag.itemCount()+" items" );
                 for( var i = 0; i < pag.itemCount(); i++)
                 {
                       var item = new PageItem(pag.item(j));
                       print( "\t"+item.name ):
                       //If the item is an NMR spectrum, it will print "This is an NMR spectrum", if
not, the function isValid will give a "False"
                       var spectrum = new NMRSpectrum(item);
                       if(spectrum.isValid())
                              print( "This is an NMR Spectrum" );
                 }
          //To save as a PDF file
          serialization.save("/dimethoxy.pdf", "pdf");
    }
}
```

To run this script, just copy it to the 'Edit Script' dialog box and type "openSaveDocument()" in the combobox. Please bear in mind that, you will need to write the corresponding path of the saved Mnova file in the line 4 of the script (in this case the dimethoxy.mnova file was saved in C:\). As you can see in the script, if Mnova does not recognize the spectrum, you will obtain a 'False' message in the output due to the statement: if(serialization.open("/dimethoxy.mnova"))

The line **print**("File Opened"); will give the corresponding message in the output, as you can see in the picture below:

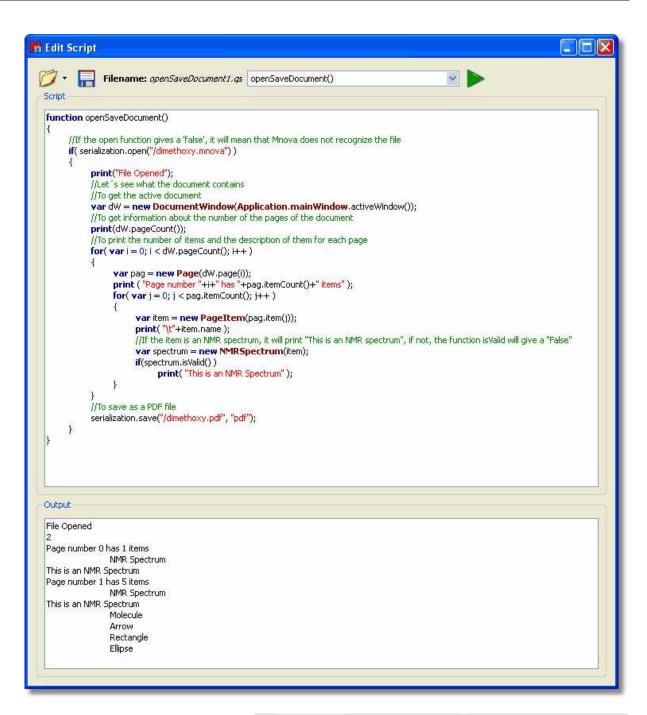

The object 'Application' of the variable **var** dW = new**DocumentWindow(Application.mainWindow**. activeWindow()); gives us the 'Active Window' of the 'Main Window', that is to say, the document which we can see in the screen. The function**print**(dW.pageCount()); is used to know the number of the pages of the document.

The following lines of the script are used to obtain information about the items included on the document. For example the function pageCount is used to know the number of pages of the document. The variable var pag = new Page(dW.page(i)); will analyze page by page to find the information. The line print ("Page number "+i+" has "+pag.itemCount()+" items" ); will print the corresponding phrase in the output, following the number of the page (+i+) and the number of the items included in the page for( var j = 0; j < pag.itemCount(); j++ ). The variable var item = new

**PageItem**(pag.item(j)); will inform about the type of the item, and the function **print**( "\t"+item.name ); will print the name of the item. In this example (as we can see in the output of the picture below), the document has 2 pages; page 0 has 1 item, which is an NMR spectrum and page 1, has 5 items (NMR Spectrum, molecule, arrow, rectangle and ellipse).

The variable **var** spectrum = **new NMRSpectrum**(item); will rebuild the active spectrum, and if the item is an NMR spectrum, it will print "This is an NMR spectrum", if not, the function isValid will give a "False" due to the lines: **if**(spectrum.isValid()) // **print**("This is an NMR Spectrum");.

Finally, the plugin serialization.save("/dimethoxy.pdf", "pdf"); will save the document as a PDF file in the specified location of the hard-disk (in this case, the PDF will be saved in C:\).

#### Open a spectrum with molecules:

It is possible to open spectra with molecules by using the openSpecWithMols.qs example script. You will need to add the directory where you have the script to the 'Scripts directories' (by using the 'Edit/Preferences/Scripting/Scripts Directories' menu). Then restart Mnova and you will be able to run the script from the command line by typing:

#### "MestReNova path" -sf openSpecWithMols, "Spectrum path"

For example:

"C:\Program Files\Mestrelab Research S.L\MestReNova\MestReNova.exe" -sf openSpecWithMols,"C:\1H\fid"

Where, the yellow is the path where you have installed Mnova and the red is the path of the spectrum that you want to open.

// Opens a spectrum at aSpecPath and all the molfiles located in the same directory **function** openSpecWithMols(aSpecPath)

var dirPath = File.absDirPath(aSpecPath);
var dir = Dir(dirPath);
dir.cdUp();
var files = getMaskFiles(dirPath, dir.absPath, "\*.mol", "\*", false);
files.push(dirPath);
serialization.open(files);
}

**Import\_Process\_Save\_Loop Script:** This script can be used to apply a previously existing 'full processing' template (in this case, it is a template saved at C:/temp/proc.mnp) to several spectra (saved at C:/spectra/ and inside sub-folders with the extension ".fid", for example: "C:/spectra/1H.fid") and to save the result in different files formats (.mnova, .pdf and .txt). This script is only valid for these spectra containing a FID file.

```
// This example function demonstrates how to apply some processing to a set of
spectral files and to save the result in the different file formats.
function import_process_save_loop()
     const dirName = "c:/spectra"; // Source directory with spectra to be
processed.
     const resultDirName = dirName; // Destination directory where processed
spectra should be put.
     const procName = "c:/temp/proc.mnp"; // Processing file. It must be created in
the Full Processing dialog of MestReNova.
     const fileMask = "fid"; // This mask specifies files to be processed.
     const dirMask = "*.fid"; // This mask specifies directories to be scanned for
spectra.
     var dir = new Dir(dirName);
     if (!dir.exists)
     ł
          MessageBox.critical("Directory " + dirName + " does not exist.",
MessageBox.Ok);
          return;
     dir.cdUp();
     // The below function getMaskFiles is located in the files.gs script.
     // If you run import_process_save_loop from QSA Workbench then it is necessary
to introduce getMaskFiles to the interpreter by importing files.qs.
     var files = getMaskFiles(dirName, dir.absPath, fileMask, dirMask, true);
     for(var i = 0; i < files.length; i++)</pre>
     {
          var dw = new DocumentWindow(Application.mainWindow.newWindow()); //
Create new document window
          if (serialization.open(files[i]))
          {
               nmr.process(procName);
               const toReplace = new RegExp("[/|:]", "g");
               fileName = resultDirName + "/" + files[i].replace(toReplace, "_");
// Generate a filename for processed spectrum.
               serialization.save(fileName+".mnova", "mnova"); // MestReNova file
format
               serialization.save(fileName+".pdf", "pdf"); // Adobe PDF file
format
               serialization.save(fileName+".txt", "ascii"); // ASCII
               print(fileName); // Prints file name in the debug window
          dw.close(); // Close document window of processed spectrum
     }
```

**Parameters Script:** This script can be used to obtain the desired parameters on your spectrum. You will be able to add or remove any parameter and to change the font by just using HTML code.

```
function spectrumParams()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    var htmlText = "<b>Nucleus</b>: %1 <br/> <b>Frequency: </b> %2 <br/> <b>Pulse
Sequence: </b> %3 <br/> <b>psLabel: </b> %4 <br/> <b>Solvent: </b> %5 <br/><b>Title: </b> %6";
    var nuc = spec.getParam("Nucleus[1]");
    var freq = spec.getParam("Spectrometer Frequency");
    var seqfill = spec.getParam("psLabel");
    var psLabel = spec.getParam("Solvent");
```

In this case, the script will print the parameters Nucleus, Spectrum Frequency, Pulse Sequence, psLabel, Solvent and Title. Please bear in mind that getParam function returns only parameters which exist in the table of parameters (including invisible ones). Please make sure that you have these parameters included on the table of parameters (via customization dialog).

Fid Test Script: you will get information about the real and the imaginary part of the FID by running this script:

```
function fidTest()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    print(spec.fidImag(0));
    if( spec.fidSetImag(0,0) )
        print(spec.fidImag(0));
        print(spec.fidReal(0));
        if(spec.fidSetReal( 0, 0 ) )
            print(spec.fidReal(0));
        spec.process();
    mainWindow.activeWindow().update();
}
```

The command **print**(spec.fidImag(0)) will return the value of the imaginary part of the FID at the *alndex* point (in this case; 0. You can type any number from zero to the number of points of your spectrum), whilst the line **print**(spec.fidReal(0)); will give you the value of the real component. The object *fidsetImag*; sets the imaginary value of the *alndex* point of the spectrum fid.

Integral Test Script: This script can be used to get information about the integrals of the spectrum:

```
function integralTest()
     var spec = new NMRSpectrum( nmr.activeSpectrum() );
     var intList = new Integrals(spec.integrals());
     print(intList);
     print(intList.count);
     print(intList.normValue);
     var myInt = new Integral(intList.at(0));
     print(myInt);
     print(myInt.rangeMax(1));
     print(myInt.rangeMin(1));
     if( spec.dimCount > 1 )
     {
          print(myInt.rangeMax(2));
          print(myInt.rangeMin(2));
     }
     print("Integral Value "+myInt.integralValue());
     print("Normalized value "+myInt.integralValue(intList.normValue));
```

```
var sReg = new SpectrumRegion(7.2, 7.5);
var newInt = new Integral( spec, sReg, false );
print(newInt);
print(newInt.integralValue());
spec.integrals().append(newInt);
spec.process();
```

The first part of the script is used to count the integrals and to report the normalized value applied to the integrals (in the list 'intList'). With the second part of the script, the user is able to select any integral of the list (in this case the integral which appears in the first position, if we wanted to select the second integral, we should have to type **var** myInt = **new Integral**(intList.at(1));). Then the scripts returns the absolute value and the limits of the selected integral. The third part of the script returns the absolute value of the integral.

The last part of the script can be used to add a new integral to the list (in this case an integral with the spectral region from 7.2 to 7.5 ppm). the script reports the absolute value of this integral.

**Multiplet Test Script:** This script is valid to obtain information about the multiplets of the spectrum and also to apply a 'manual multiplet analysis':

```
function multipletTest()
     var spec = new NMRSpectrum( nmr.activeSpectrum() );
     print(spec.multiplets());
     var sMult = new Multiplets(spec.multiplets());
     print(sMult.count);
     print(sMult.at(2));
     var sReg = new SpectrumRegion(7.0, 7.5);
     var mult = new Multiplet( spec, sReg );
     var myMultiplets = new Multiplets();
     myMultiplets.append( mult );
     var mult2 = new Multiplet( spec, new SpectrumRegion(3.80,3.90) );
     myMultiplets.append( mult2 );
     var nM = new Multiplet(new SpectrumRegion(3.65,3.75), "t");
     nM.name="My mulltiplet";
     myMultiplets.append(nM);
     print(myMultiplets);
     spec.setMultiplets(myMultiplets);
     print(spec.multiplets());
     spec.process();
```

The first part of the script creates a list of the multiplets which appear on the spectrum and prints some information about the selected multiplet (in this case, the multiplet number 2, but of course you can select any other multiplet). The second part of the script creates a multiplet in the selected region 'sReg' (in this case the region is 7.0-7.5 ppm. It works as a manual multiplet analysis). Then, it creates a new empty list of multiplets which is added.

The third part of the script consists in a new region (from 3.80 to 3.90 ppm) to apply the multiplet analysis. The following part of the script is used to add a multiplet manually to the multiplet list (the user will be able to remove this part of this script without any problem). In this case, we wanted to add a triplet, which appears in the region from 3.65 and 3.75 ppm, with the name 'My multiplet'.

The end of the script is used to replace the original multiplet list for the list which we have just created.

**Peak Test Script:** A similar script used to obtain information about the chemical shift and the intensity of the peaks of a 1D-NMR spectrum:

```
function peakTest()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    var sR = new SpectrumRegion( 0, 9.5 );
    var ps = new Peaks(spec, sR); //fill the list with the peaks in sR
    print(ps);
    var p = new Peak(1.265, spec);
    print(p);
    ps.append(p);
    spec.setPeaks(ps);//Set the peaks to ps
    print( spec.peaks());
    spec.process();
}
```

After running this script, we will get the peak picking analysis of a 1D-NMR spectrum from 0 to 9.5 ppm (of course, we will be able to change this range). Then, a new peak at 1.265 ppm will be added to the peak list (again, you can add any other peak, if you want), reporting the intensity value of this new peak. Finally, the spectrum will be re-analyzed to obtain the new number of peaks.

A similar script can be used for a 2D-NMR spectrum, but in this case we have to type the corresponding spectrum region in 2D mode:

```
function peakTest()
{
    var spec = new NMRSpectrum( nmr.activeSpectrum() );
    var sR = new SpectrumRegion(4.0, 3.5, 75, 65 );
    var ps = new Peaks(spec, sR); //fill the list with the peaks in sR
    print(ps);
    var p = new Peak(72.73, 3.17, spec);
    print(p);
    ps.append(p);
    spec.setPeaks(ps);//Set the peaks to ps
    print( spec.peaks());
    spec.process();
}
```

**Multiplet Reporter script**: Let's take a look now at a very important part of the 'Multiplet Reporter\_JACS' script:

```
// This function defines JACS-like multiplet report.
// To customize report, edit this class or implement another one.
function JACSMultipletReporter()
{
MultipletReporter.call(this);
this.onlyElementName=false;
// Define font size and font family
this.font = "<font style=\"font-size: 10pt; font-family: Times New Roman\">";
this.nucleusTemplate="%1";
// Report header. %1 will be replaced with nucleusString, %2 with frequency, %
3 with solvent
this.header = "%1 NMR (%2 MHz, %3) δ ";
// Multiplet templates. %1 - delta, %2 - category, %3 - nH
this.reportRange = true; // set to true to get multiplet range instead of
delta.
this.withoutJsTemplate = " %1 (%2, %3H)"; // multiplet template without J's
```

```
this.withJsTemplate = " %1 (%2, %4, %3H)"; // multiplet template with J's
this.rangeTemplate = "%1 – %2";
// J's list template. %1 - list of J's
this.jListTemplate = "<i>J</i> = %1";
this.jPrecision = 1; // J's precision
this.deltaPrecision = 2; // delta precision
this.mSeparator = ", "; // multiplet separator
this.jSeparator = ", "; // J's separator
this.start = this.font;
this.end = ".</font>";
JACSMultipletReporter.prototype = new MultipletReporter();
JACSMultipletReporter.prototype.toString
                                                   function()
                                                                   {
                                           =
                                                                         return
"JACSMultipletReporter()"; }
(...)
```

The user will be able to change the multiplet report template to obtain the desired multiplet report; for example:

this.onlyElementName=false; changing false with true, we will obtain only the element name without the atomic mass (For example: H, C instead of <sup>1</sup>H, <sup>13</sup>C).

The function: **this**.font = "<font style=\"font-size: 10pt; font-family: Times New Roman\">"; will define the font size and the font family of the multiplet report.

The line: **this**.header = "%1 NMR (%2 MHz, %3) δ "; is used to print the header of the report, where %1 will be the nucleus (H or C), %2 the frequency of the spectrometer (in MHz), and %3 the solvent, followed by a delta symbol ( $\delta$ ). For example: "<sup>1</sup>H NMR (500 MHz, CDCl3) ".

The sentence: **this**.reportRange = true is used to obtain the multiplet range instead of the chemical shift.

The functions: **this**.withoutJsTemplate = " %1 (%2, %3H)" and **this**.withJsTemplate = " %1 (%2, %4, %3H)" are used to customize the appearance of the multiplet report by changing the positions of %1, %2, %3H, or %4 (where, %1 means: chemical shift; %2 means: type of multiplet (s, d, t, etc); %3H means: number of hydrogens and %4 means the coupling constant value). As you can see, the first line shows a multiplet without coupling constants, (while the last line shows a multiplet with coupling constants).

So, if you need to obtain something like this (Japanese format):

1H NMR (300 MHz, Solvent)  $\delta$  ppm 6.43-6.22 (1 H, m), 3.17 (1 H, q, J = 7.15 Hz) etc...

You should modify both lines, as you can see below:

this.withoutJsTemplate = %1 (%3H, %2)"; this.withJsTemplate = " %1 (%3H, %2, %4)";

If you prefer to obtain something like this:

1H NMR (300 MHz, Solvent) δ ppm 1.23 (d, *J* = 1.2 Hz, 3 H), etc...

Just replace the original lines with:

this.withoutJsTemplate = %1 (%2, %3H)"; this.withJsTemplate = " %1 (%2, %4, %3H)";

To obtain the coupling constant symbol in normal instead of *'italic'*, just modify the script by removing the italic format (<i>J</i>). If you prefer to obtain it in "**bold**" just type: **this**.jListTemplate = "<b>J</b> = %1";

The following paragraph will be used to customize the appearance of the coupling constants list:

this.jPrecision = 1; // J's precision this.deltaPrecision = 2; // delta precision this.mSeparator = ", "; // multiplet separator this.jSeparator = ", "; // J's separator

The first line is used for the precision of the coupling constants values, the second will be used for the precision of the chemical shift and the remaining two lines will print the separation between the multiplets and the coupling constants values.

If you need to obtain the coupling constants in descending order, replace 'true' with 'false' in the following line:

var jList = new JList(multiplet.jList());
jList.sort(true);

If you want to obtain the multiplet chemical shifts in ascending order, just replace the 'false' with 'true' in the script:

var multiplets = new Multiplets(spectrum.multiplets()); // get multiplets from spectrum jList.sort(true);

To obtain the multiplet range in ascending order, just replace the rangeMin with rangeMax (and vice versa) in the line below of the script:

shiftStr = this.rangeTemplate.argDec(multiplet.rangeMax, 0, 'f', this.deltaPrecision).argDec(multiplet. rangeMin, 0, 'f', this.deltaPrecision);

Title and Solvent: running this script, you will get the title and the solvent on your spectrum

**Zoom:** This script can be used to apply a zoom into a selected range of a spectrum. In order to select the horizontal range, just type the desired values between the brackets on the line spc.horZoom(1.0, 5.0);

If you want to set the vertical zoom, just change the values of the line spc.vertZoom(-100, 7000)

```
function spectrumZoom()
{
    var spc = nmr.activeSpectrum();
    if( !spc.isValid() )
        return;
    spc.horZoom(1.0, 5.0);
    spc.vertZoom(-100, 7000);
    spc.update();
    mainWindow.activeWindow().update();
}
```


**Properties Script:** You will find below a script example to change some properties of your spectra. In this case, the colour of the spectrum will be changed to red, the peaks font to Arial and the integral curves will be showed. You will find all the available properties at the <u>'Mnova Properties'</u> chapter:

```
function properties()
{
    var spec = new NMRSpectrum(nmr.activeSpectrum());
    spec.setProperty("curve.color","red");
    spec.setProperty("peaks.font","Arial");
    spec.setProperty("integrals.curve.show", true);
    spec.update();
    mainWindow.activeWindow().update();
}
```

**Cutting:** This script can be used to apply cuts to the spectra. You will obtain two cuts in your spectrum, between 1.0-3.5 and 7.0-8.0 ppm respectively.

```
function myProcess()
{
  var spec = new NMRSpectrum( nmr.activeSpectrum() );
  var p = new NMRProcessing(spec.proc);
  var regs = new Array(2);
  regs[0] = new SpectrumRegion(1.0, 3.5);
  regs[1] = new SpectrumRegion(7.0, 8.0);
  print(p.getParameter("cuts"));
  p.setParameter("cuts.list", regs);
  spec.proc = p;
  spec.process();
  mainWindow.activeWindow().update();
}
```

**Processing script:** Here you can see a part of the 'mnrProcessingTest" script stores under the examples folder:

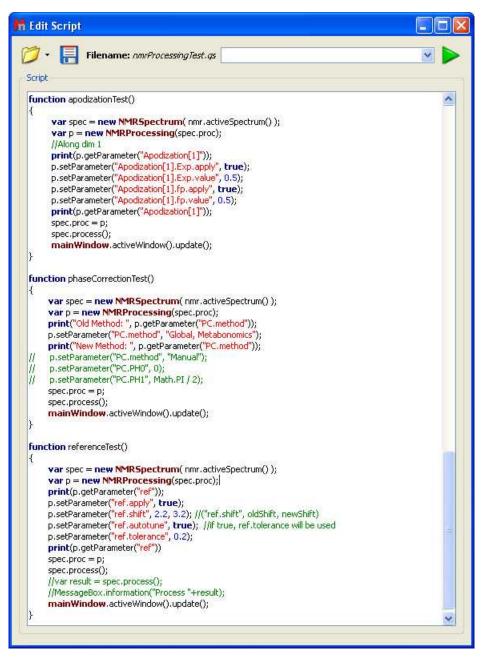

**Magnitude Active Spectrum script**: Let's see another script; in this case this script is used to obtain the 1D-NMR spectra in magnitude. Just open a 1D-NMR spectrum in Mnova, load this script by following the menu 'Script/Edit Script', type "magnitudeActiveSpectrum()" in the edit box and click on the green triangle to run the Script. You will obtain automatically your 1D-NMR spectrum in magnitude.

Please bear in mind that it is also possible to run scripts from the command line, just by typing the path where the Mnova .exe file and the script are located and -sf "name of the script function": "mestrenovaPathname" "scriptPathname" -sf "scriptFunctionToRun"

For example:

"C:\Program	Files\Mestrelab	Research	S.L\MestReNova\MestReNova.exe"	"C:\Program	Files
\Mestrelab	Research	S.L\Me	estReNova\scripts\magnitudeActiveSpe	ectrum.qs"	-sf

"magnitudeActiveSpectrum"

```
Edit Script
                                                                                                            Filename: magnitudeActiveSpectrum1.qs magnitudeActiveSpectrum()
       +
  Script
   function magnitudeActiveSpectrum()
        //The magnitude of the active spectrum is calculated (only for 1D)
        //To get the active spectrum
        var spectrum = nmr.activeSpectrum();
        //To make sure that the spectrum is valid
        if( spectrum.isValid() )
        ł
              //Only interested in 1D-NMR spectra
              if( spectrum.dimCount == 1 )
                    //The functions beginModification and endModification will allow us to save the inicial state of the
   spectrum to be able to apply Undo/Redo
                   nmr.beginModification(spectrum);
                    var ptsCount = spectrum.count();
                   for(var k = 0; k < ptsCount; k++)</pre>
                         //To calculate the module of each point and to asign it
                         re = spectrum.real(k);
                         re *= re;
                         im = spectrum.imag(k);
                         im *= im;
                         spectrum.setReal(k, Math.sqrt(re + im));
                    ĥ
                    nmr.endModification(spectrum);
                    //To get the active window and to refresh it so that the changes in the spectrum become visible
                    Application.mainWindow.activeWindow().update();
              }
        }
  Output
```

**Threshold Script**: This script will allow the user to adjust the threshold of the color scheme in 2D-NMR spectra:

```
// <GUI menuname="threshold2D" shortcut="Ctrl+T" tooltip="threshold2D" />
function threshold2D()
{
    var spectrum = nmr.activeSpectrum();
    if(!spectrum.isValid() )
    return
    var th = spectrum.threshold;
    var dlg = new Dialog();
    dlg.title = "Threshold";
    var edit = new LineEdit();
    edit.label = "Threshold";
    edit.text = th;
    dlg.add(edit);
    if (dlg.exec())
```

```
{
  spectrum.threshold = edit.text;
  }
  spectrum.update();
mainWindow.activeWindow().update();
}
```

Running this script will show the 'Threshold' dialog box. From this window, the user will be able to adjust the threshold of the colour scheme by just typing the desired value and clicking on the 'OK' button.

n Thresh	Iona	
Threshold	30.48750	)114440918
	Ok	Cancel

**ProcessTest Script:** This script can be used to get some data from Mnova, save it as a file, next run some external program in order to make calculations (or whatever you need) and once the external program finishes, Mnova will get the result from another file. In this case the external program is the 'NotePad'.

```
function processTest()
{
    fileName = Dir.temp() + "MNova_Process_Text.txt";
    var f = new File(fileName);
    f.open(File.WriteOnly);
    var s = TextStream(f);
    s.write("Hello Notepad!");
    f.close();
    print(Process.execute("notepad.exe", fileName));


    f.open(File.ReadWrite);
    s.pos = f.size;
    print(s);
    s.write("\r\nHi again!");
    f.close();
    print(Process.startDetached("notepad.exe", fileName));
}
```

# 12.10 Export as ASCII


You can export NMR spectra via 'File/Save As/NMR 1D Custom CSV File' with options to export PPM+Re+Im, Hz+Re, PPM+Re or Hz+Re+Im, either from right to left or from left to right.

Format:	{ppm}{tab}{real}{tab}{imag}	_
i viniat.	{hhu}{ran}{isan}{ran}{is	
Decimal Places:	6 🖉 🕼	Expected column name
Decimal Fiercest		(ppm), (hz), (pts), (real

You can use some scripts from the 'Scripts/Export menu':

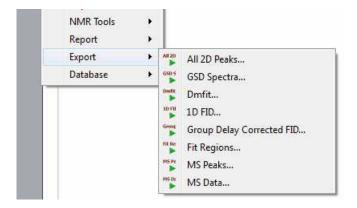

The script called 'All 2D Peaks' will export all the peaks of 2D datasets in the current document. The 'DmFit' will export 1D-NMR spectra to Dmfit ASCII format. The 'FID' script can be used to extract a XY text file for the FID. This script saves original FID independently on what is shown on the screen (FID, or FID', or FT Spectrum). The 'Fit Regions' script will export the fit peaks to a text file. The 'GSD Spectra' script will generate an ASCII file with the GSD peaks.

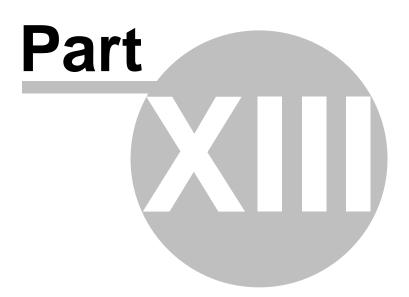

# 13 Tutorials

The goal of the present chapter is to give you a fast introduction to the basic analysis tools which are commonly used to solve structural problems. Not everything is explained in detail; the rest of the manual provides a more comprehensive description of all topics covered here.

# **13.1 Importing Spectrum Parameters**

(Not available in Mnova Lite)

The 'Importing Spectrum Parameters' feature will allow Mnova users to include any variable into the Parameters Table from the raw data file. In addition, the users will be able to create 'Parameters Templates' in order to obtain the same parameters in all of their processed spectra. Before this feature was implemented, only standard spectrum parameters could be included in the corresponding table.

The user will easily be able to add, create, remove or modify any spectrum parameter or even to create templates in order to obtain the same parameters in any processed spectra.

To customize the parameters table just follow the menu: View/Tables/Parameters and click on the 'Customize' icon to display the 'Customize Parameters' dialog box.

lab	les	-	6 🛛
Re	port Copy Setup	Customize	
	Parameter	Value (f2, f1)	~
1	Title	js1pmquin	
2	Origin	inova	
3	Owner		
4	Solvent	"CDCl3"	
5	Pulse Sequence	gHSQC	
6	Acquisition Date		
7	Modification Date	Oct 22 2007	-
8	Temperature	25.0	
9	Number of Scans	8	
10	New1	275 y cdc	
11	Spectrometer Frequency	(399.971, 100.572)	
12	Spectral Width	(4199.916, 25000.000)	
13	Lowest Frequency	(-499.069, -1917.940)	
14	Nucleus	(1H, 13C)	
15	Spectral Size	(1024, 1024)	~
Pa	rameters Peaks Ir	itegrals Multiplets As	ssiç 🔹 🕅

Exp	erimental Dir	nensional	1	
-	Name		Template	^
8	Modification Da	te procpa	ar(date)	
9	Temperature	procpa	procpar(temp) procpar(nt)	
10	Number of Scar	ns procpa		
11	G to G'	procpa	ar(DAC_to_G)	=
12	Echo Delay	procpa	ar(del)	
13	Pulse Width	procpa	ar(gt1)	-1
14 <	New1		unction2(procpar(celem), procpar	~


Clicking on the 'More>>' button will display the 'Current Spectrum Parameters' window, as you can see in the picture below. The user will be able to obtain any parameter from any raw data file (procs, acqus, title, etc...) by selecting the desired file on the 'File/Block' box (red square in the picture below):

🤊 🗸		n Parameters	Current Spectrum Parameters Select a File/Block: procpar
ľ	Name	Template	gstab 3 1 14 14 14 log 1
1	Data File Name		0
2	Title	text()	dgs 2 2 1023 0 0 4 1 6 1 64 4 "1:AXIAL SHIMS:z1:0,z1c:0,z2:0,z2c:0,z3:0,z4
3	Origin	procpar(console)	"2:NON AXIAL SHIMS:x1:0,y1:0,xz:0,yz:0,xy:0,
4	Owner	procpar(username)	"4:AUTOMATION:method,wshim,load,,spin:0,gai "4:SPECIAL:temp;"
5	Solvent		0
6	Pulse Sequence	procpar(seqfil)	cf 7 1 32767 0 1 3 1 1 0 64 1 1
7	Acquisition Date		0 archivedir 2 2 8 0 0 2 1 0 1 64
<		2	1 "/export/home/rgry/vnmrsys/data"
D	elete	Script Restore	0 acqstatus 7 1 32767 0 0 2 1 0 1 64 2 18 13 0 •

In the 'Customize Parameters' dialog box, the user will see an 'Experimental Parameters Template' (pink square in the picture above) which will be common for 1D and 2D (with information about: Title, Origin, Owner, Solvent, Temperature, etc.) and the 'Dimensional Parameters Template' (green square in the picture above) with information about the 'Spectrometer Frequency', "Acquired Size', 'Spectral

Width', etc.). Both sections have blank rows in their last position to allow for addition of further parameters.

You can easily add any existing parameter from the raw data. Start by selecting the location of the parameter in the Experimental or Dimensional Parameters Template by clicking on the relevant cell of the 'Template' column on the table. Once this has been selected, double click on the desired parameter (from the 'Current Spectrum Parameters' box). This will add the chosen parameter to the template.

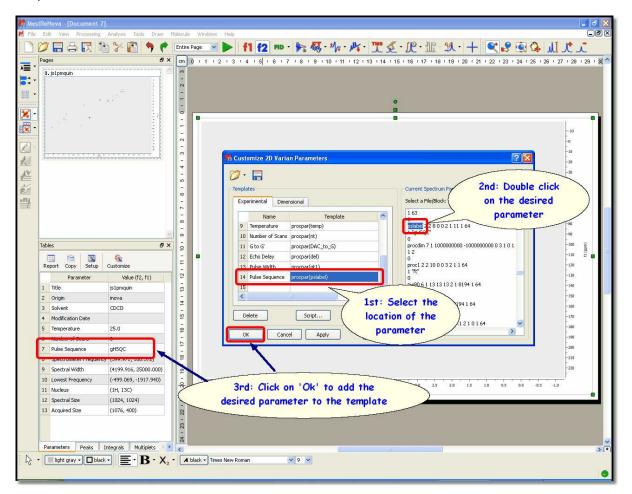

Let's see now how to add the title from the 'parm.txt' file (Bruker):

- 1<sup>st</sup>: Select the location of the parameter in the Experimental Parameter Template.
- 2<sup>nd</sup>: Select 'parm.txt' in the 'Current Spectrum Parameters' combo box.
- 3<sup>rd</sup>: Double click on the desired parameter (NAME, in this case).
- 4<sup>th</sup>: Click on 'OK' to add the parameter to the template.

npla	ates		Current Spec	rum Parameters
Exp	erimental Dime	nsional	Select a File/E	Block: parm.txt 💉
	Name	Template	Prec Current Data	Parameters
t.	Data Eile Name			azgb0044 3rd: Doubl
2	Title	parm.txt(NAME)	-1 PROCNO	1 Click on
3		elect the location	Date_ 2	on Parameters 20061211 14.53 ASX400
5	01			
5	Temperature	acqus(\$TE)	2 PROBHD 4	mm MAS 1H/
1	A STATE OF THE OWNER	acqus(\$TE) acqus(\$PULPROG)	2 PROBHD 4 PULPROG	mm MAS 1H/ 2g 1024 5000

Then, you will obtain the title on the parameters table:

Re	port Copy Sel	up Customize
	Parameter	1
1	Data File Name	H:/Documents and Settings/Usuario/Mis documentos/Manuales/
2	Title	azgb0044
3	Origin	UXNMR, Bruker Analytische Messtechnik GmbH
4	Owner	kmi
5	Solvent	DMSO
6	Temperature	293.00
7	Pulse Sequence	zg
8	Number of Scans	5000
9	Acquisition Date	1165845204
10	FTSIZE	2048.000
11	Date	Friday, September, 14, 2007
<		>

Finally you will be able to add the Parameters Table to the spectrum by just clicking on the 'Report' button (highlighted in red in the picture above).

You can use the first line of a title which contains several lines. To do it, just type this function under the parameter Title template: =(function(aTitle){return aTitle.split("\n")[0];})(title())

This is the way to add the 'easy' parameters to the 'Parameters Table'. However, there are other parameters which need a different procedure to be added from the 'parm.txt' file to the table. For example, some parameters with the same name i.g. for 2D can be written two times (for example the Spectral Frequency for f1 and for f2). Also some parameters have units. The syntax of the *parm.txt* file

parsing allows handling both situations (allowing either to get a number, or a number with the units, or even only the units).

Please bear in mind that the syntax of the 'parm.txt' parsing is:

#### parm.txt(PARAMNAME[;OCCURENCE;FIRST\_WORD;NUMBER\_OF\_WORDS])

Let's see how it works with a real example where we want to include the Spectral Frequency value for f1 and f2. As you can see in the picture below there are two values for the parameter 'SF' in the *parm.txt* file (one for f2 and another for f1):

	ates perimental Dimensio	nal		Current Spectrum Parameters Select a File/Block: parm.txt	
	Name	f2 Template	f1 Templat	F2 - Processing parameters	
2	Spectral Width	acqus(\$SW_h)	propcpar(sw1)	SF 500.1299707 MHz	
3	Lowest Frequency			SSB 0	
4	Nucleus			LB 2.00 Hz	
5	Spectral Size			GB 0 PC 1.40	
6	Acquired Size	acqus(\$TD)	acqu2s(\$TD)	F1 - Processing parameters	
7	=div(acqus(\$TD), 2	=div(acqus(\$TD	=div(acqus(\$TI	5I 1024	
8			~	MC2 TPPI SF 125.7578590 MHz	
<	i w		>	WDW EM	
		2	<u>&gt;</u>	SSB 0 LB 24.00 Hz	

We can not follow the same procedure that we followed a few pages before to insert the title on the parameters table, because now, we have two different parameters (one for f2 and another for f1) with the same name (SF).

For this reason we need to use the syntax of the *parm.txt* parsing, typing in the 'f2 Template' cell: **parm.txt(SF;1;1;1)** where **SF** is the name of the parameter, the first number ('1') indicates the order of appearance (The f2 parameter appears before in the parm.txt file than the f1). The second and the third number indicate the first word and the number of words of the string, respectively. In this case, the parameter has two words: the value (500.1299707) and the unit (MHz), but we are not interested in getting the units, so type (SF;1;1;1). If we were interested in also include the units, we must type: (SF;1;1;2).

In the 'f1 Template' cell; we would type: **parm.txt(SF;2;1;1)**, because the SF parameter for f1 appears in the second position (after the SF value for f2):

	ates erimental Dim	ensional		Current Spectrum Parameters Select a File/Block: parm.txt	
	Name	f2 Template	f1 Template 🔺	F2 - Processing parameters SI 2048	
2	Spectral Width	acqus(\$SW_h)	propcpar(sw1)	SF 500.1299707 MHz	
3	Lowest Frequ			WDW EM SSB 0	
4	Nucleus			LB 2.00 Hz GB 0	
5	Spectral Size			PC 1.40	
6	Acquired Size	acqus(\$TD)	acqu2s(\$TD)	F1 - Processing parameters	
7	=div(acqus(\$	=div(acqus(\$TD)	=div(acgus(\$TD), 2	SI 1024	
8	SF	parm.txt(SF;1;1;1)	) parm.txt(SF;2;1;1)	MC2 TPPI SF 125,7578590 MHz	
•		i j	<u> </u>	WDW EM	
				S5B 0 LB 24.00 Hz	

Similar procedure will be followed, for example, to include the LB parameter for f2 and f1, as you can see in the picture below:

mp	• 🔚 lates perimental Di	mensional		Current Spectrum Parameters Select a File/Block; parm.txt	
	Name	f2 Template	f1 Template	F2 - Processing parameters 5I 2048	1
3	Lowest Frequ			SF 500.1299707 MHz	
4	Nucleus			WDW EM SSB 0	
5	Spectral Size			LB 2.00 Hz	
6	Acquired Size	acqus(\$TD)	acqu2s(\$TD)	PC 1.40	
7	SF	parm.txt(SF;1;1;1)	parm.txt(SF;2;1;1)	F1 - Processing parameters	
8	LB	parm.txt(LB;1;1;1)	parm.txt(LB;2;1;1)	SI 1024	
9			~	MC2 TPPI SF 125,7578590 MHz	
<		ŵ j	2	WDW EM	
-				LB 24.00 Hz	
10	Delete	Script	Restore	GB U	

And here it is the result:


Re	port Copy Setu	A40
	Parameter	Value (f2, f1)
1	Title	lcec671m
2	Origin	UXNMR, Bruker Analytische Messtechnik GmbH
3	Owner	root
4	Pulse Sequence	mm_invigsmltp
5	Acquisition Date	2002-07-24T22:19:15
6	Temperature	300.0
7	Number of Scans	16
8	Spectral Width	(2500.000, 6289.308)
9	Lowest Frequency	(500.455, 6915.965)
10	Nucleus	(1H, 13C)
11	Spectral Size	(512, 512)
12	Acquired Size	(1024, 256)
13	SF	(500.13, 125.76)
14	LB	(2.00, 24.00)

Imagine, that you have a parameter which appears in the middle of another parameters. For example the 'Mixing Time' parameter of a NOESY spectrum (from Bruker); which appears in the acqus file with this format:

You want to display in this case, the D9, so you will need to type **acqus(\$D[9])** in the Parameters template list as it is shown in the picture below:

Report Copy Setup (	Sustomize		
Parameter	Value (f2, f1)		e je e
Origin	Bruker BioSpin GmbH	R Customize 2D Bruker XWIN-NMR Parameters	
5 Owner	nmrsu		
Site		🧭 · 🗐	
Spectrometer	spect	Templates	Current Spectrum Parameters
Author		Experimental Dimensional	Select a File/Block: acqus
Solvent	CDCl3	Differbional	**perdekaz= <>
0 Temperature	295.0	Name Templati 🛆	##\$CPDPRG3= <> ##\$CPDPRG4= <mley></mley>
1 Pulse Sequence	dipsi2etgpsi	17 Acquisition Date =brukerDate(acqus(\$DATE))	##\$CPDPRG5= <mlev></mlev>
2 Number of Scans	2	18 Modification Date acqus(_LASTMODIFIED_)	##\$CPDPRG6= <mlev> ##\$CPDPRG7= <mlev></mlev></mlev>
3 Receiver Gain	9	19 Gto G' "1"	##\$CPDPRG8= <mlev></mlev>
4 Relaxation Delay	0.9644	20 Echo Delay acqus(\$D[20])	##\$CPDPRGB= <> ###CPDPDCT= <>
5 Pulse Width	7.2000	21 aradiene baradon -braken alse widdh(acqus(\$P[30])	##\$D= (063) 3e-06 0.9643645 0 0 0 0 0 0 0 0.0.06 0 0.03 2e-05
6 Acquisition Time	0.2355	22 Mixing Time acqus(\$D[9])	1e-05 1e-0500000000000000000000000000000000000
7 Acquisition Date	2007-11-29T17:57:58		##\$DATE= 1196359078
<ul> <li>Modification Date</li> </ul>	2007-11-20112-03-32		##\$DBL= (07)
9 Mixing Time	0.06		120 120 120 120 120 120 120 120 120 ##\$DBP= (07)
0 Spectrometer Frequency	(500.13, 500.13)	Delete	150 150 150 150 150 150 150 150
1 Spectral Width	(4347.8, 4347.8)	OK Cancel Apply Less <<	##\$DBP07= 0
2 Lowest Frequency	(-85.1, -85.1)		
3 Nucleus	(1H, 1H)		18
24 Acquired Size	(1024, 128)		

The user will also be able to add his/her own parameters by double clicking on the table and typing the corresponding parameter name (between "quotation marks") and value. In the picture below, we have added manually the text "December, 30th, 2007" in the field: 'Original Name' and 'Date' as the 'Visible Name'

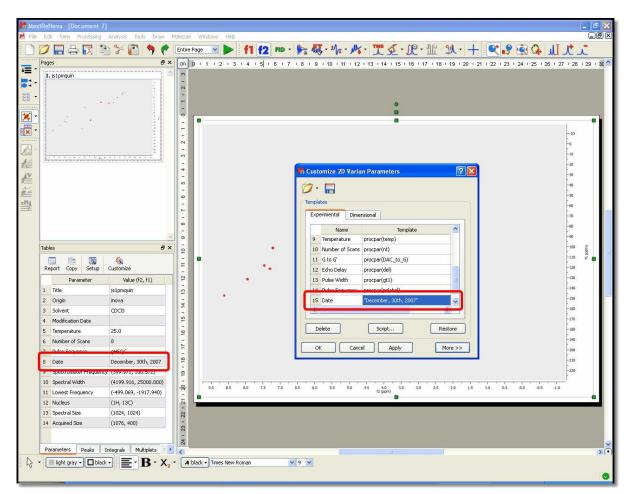

The user will also be able to introduce formulas (available in the script) by typing an *equal* symbol followed by the desired formula (numbers or parameters), for example: =sum(a, b), or =div(acqus(TD), 2). Please note that formulas are case sensitive and should be lower case.

The following example shows the procedure to show the 'Time Delay' in seconds. Firstly, we need to double click on the desired parameter in the 'Current Spectrum Parameters' list to add it to the 'Parameters Template':

100	ates erimental Dime	nsional	Current Spectrum Parameters
-	Name	Template	Double click on the
7	Pulse Sequence	acqus(\$PULPROG)	Parameter to insert it on
8	Number of Scans	acqus(\$NS)	the Parameters Template
9	Acquisition Date	acqus(\$DATE)	-1 The Full unieters reinplute
10	FTSIZE	procs(##\$FTSIZE)	0.50.30.30.30.5
11	Date	"Friday, September, 14, 2907	##\$DBP0/F5=(07) 3 ■ ##\$DBP0/F5=(07)
12	acqus(\$TD), 2	"=div(acqus(\$TD),	3 ##\$DE= 22.5
13	Time Delay	acqu2s(\$DE)	##\$DECBNUC= <off> 3 ##\$DECIM= 1</off>
<	*		##\$DECNUC= <1H>
_			##\$DECSTAT= 7 ##\$DIGMOD= 1

By default the Time Delay is showed in milliseconds, so we need to divide the value by 1000 to obtain it in seconds. So, the user will need to type '=div(acqus(\$DE),1000)' in the 'Parameters Template' to get the division. In this way the user will obtain the 'Time Delay' value in seconds in the Parameters Table, as you can see in the picture below:

	es	₽×	=	n Customize 2D Bri	area watang	- Anni -	1010
	port Copy Setup	Customize	- 12 -	Ø · 🔒			
_	Parameter	<u>^</u>	5	Templates			
	Data File Name	H:/Documents and Setting	4	Experimental Di	mensional		
	Title	DRX-500 ulactocpcl H	<del>ت</del> -	Name		Template	Precisi 🔨
	Origin	UXNMR, Bruker Analytisch	-	7 Pulse Sequenc	e acqus(\$P	ULPROG)	-1
	Owner	root	9			5)	0
	Solvent	D20	Form	la to divide	the	YE)	-1
	122 / //	The state of the s				11000000000	
	Temperature	300.00	Time	Delay by 10	00	JIZE)	3
	Temperature Pulse Sequence	300.00 mm_invigsmltp	Time	Delay by 10	00	eptember, 14, 20	
i i	the second second second		Time	Delay by 10	<	1	
	Pulse Sequence	mm_invigsmltp	Time			eptember, 14, 20	007" 3
	Pulse Sequence	mm_invigsmltp	- 20 - 19	12 acqus(\$TD), 2		eptember, 14, 20 05(540), 2)	007" 3
	Pulse Sequence	mm_invigsmltp 16 1027549155	1 21 - 20 - 19	12 acqus(\$TD), 2 13 Time Delay	=div(acqu	eptember, 14, 20 057340), 2) us(\$DE),1000)	007" 3 3 3 3 2 3
	Pulse Sequence Number Concern Time Delay in seconds	mm_invigsmltp 16 1027549155 024.000	1 22 1 21 1 20 1 19	12 acqus(\$TD), 2 13 Time Delay	=div(acqu	eptember, 14, 20 05(540), 2)	007" 3 3 3
23	Pulse Sequence Number Concern Time Delay in seconds	mm_invigsmltp 16 1027549155 024.000	1 21 - 20 - 19	12 acqus(\$TD), 2 13 Time Delay	=div(acqu	eptember, 14, 20 057340), 2) us(\$DE),1000)	007" 3 3 3 3 2 3

To get the **'Experiment Time'** in a Varian dataset; obtained by adding the 'd1' plus the 'at' and multiplying the result by the 'nt', we could use this function:

=(function(d1, at, nt){return (parseFloat(d1) + parseFloat(at))\*parseFloat(nt);})(procpar(d1),

#### procpar(at), procpar(nt))

Experimental	Dimensional				
	Name	Template	Precision	Meaning	*
18 🔽 Presati	uration Frequency	=varianPresatFreq(procpar(tof), procpar(satfrq), procpar(satmode), procpar(sw), procpar(sfrq), procpar(rfp), procpar(rfl))	5	Presaturation Frequency	
19 🔽 Acquis	sition Time	procpar(at)	4	Acquisition Time	
20 🔽 Acquis	ition Date	=varianDate(procpar(time_complete), log(Acquisition_complete), procpar(_CREATED_))	-1	Acquisition Date	
21 🗹 Modifi	ication Date	procpar(_LASTMODIFIED_)	-1	Modification Date	
22 🔽 Class			0	Class	
23 📝 Experi	ment Time	=(function(d1, at, nt){return (parseFloat(d1) + parseFloat(at))*parseFloat(nt);])(procpar(d1), procpar(at), procpar(nt))	-1		=
24 🔽			-1		-

The parameters will be hidden in the table display if the user removes the corresponding tick mark on the 'Visible' Column. The user can also delete any parameters from the table by highlighting each of them and clicking on the 'Delete' button.

The 'Restore' button is used to recover the default template. The user will be able to save his/her own

template by clicking on the 'Save Template' icon 🛅. To load a template, just click on the 'Open

Template' button **2**. Clicking on 'OK' will save the template in the registry and Mnova will remember it for futures uses. The 'Apply' button is used to view the effect of any changes directly on the parameters table without needing to close the 'Customize Parameters' dialog box.

#### See also:

Scripts

## 13.2 Basics on Arrayed-NMR Data Analysis

In this tutorial we shall cover some basic concepts on the analysis of a very important class of NMR experiments, the so-called Arrayed NMR spectra. The concept is very simple: an arrayed experiment is basically a set of individual spectra acquired sequentially and related to each other through the variation of one or more parameters and finally grouped together to constitute a composite experiment. These experiments are also known as 'pseudo-2D'. For example, in the case of Bruker spectra they have the same file name as 2D spectra, that is ser files (ser = serial spectra). In the case of Varian, the file name is fid (Varian uses the same name for 1D, 2D, 3D, ... and arrayed spectra). However, unlike with actual 2D spectra, arrayed spectra are only transformed along the F2 –horizontal or direct-dimension (assuming 1D arrayed spectra only).


The modus operandi is better explained with an example: let's suppose it is necessary to acquire a pulse field gradient (PFG) experiment. Instead of acquiring independent spectra, it is more convenient to create an array with increasing PFG amplitudes. All resulting spectra are now treated as a single experiment. This grouping greatly facilitates processing as, in general, all subspectra require the same processing operations (apart from some occasional minor adjustments of one or several spectra).

Well known examples of NMR arrayed experiments are, among others:

- Relaxation (T1, T2)
- PFG experiments (DOSY)

• Kinetics and reaction monitoring by NMR

Any good NMR processing software should be able to automatically recognize when an NMR spectrum is an arrayed experiment and will setup all processing operations accordingly. For example, the figure below illustrates the results obtained when a Bruker arrayed folder is dragged and dropped into Mnova:

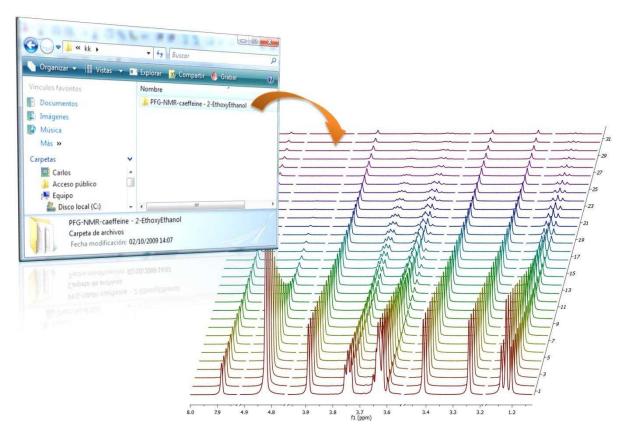


What has happened here are basically 2 things:

- 1. First, Mnova detects that the dropped folder contains an arrayed experiment
- With that knowledge in hand, Mnova proceeds to process all the individual spectra, one after the other and of course, along the only valid dimension (F2). So for every spectrum, Mnova applies appropriate weighting, zero filling, FT, phase correction, etc and stacks all the spectra as shown in the picture above

As a result, all individual spectra grouped within one composite item (i.e. arrayed item) have been processed in the same way. However, it's very common that some subspectra might require independent tuning. For example, many PFG NMR experiments present gradient dependent phase shift so that it becomes necessary to adjust the phase of some individual spectra separately. This is very easy to accomplish with Mnova as you will see below.

# Practical hints

When an arrayed experiment has been detected, all subspectra are grouped together and plotted in the stacked display mode in Mnova (see figure below).

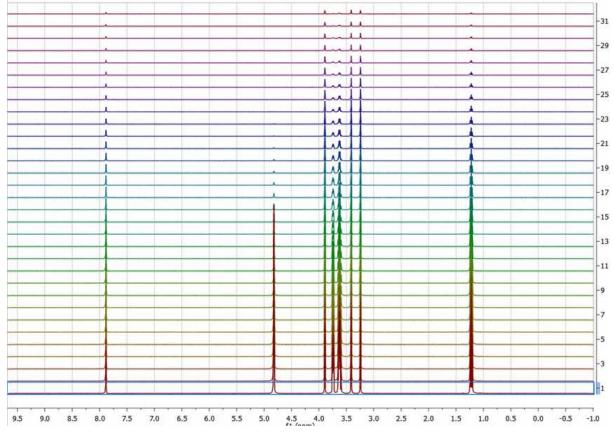


Several points are worth mentioning:

(A). Take a look at the blue box in the figure above: it shows the so-called 'active spectrum'. What does this mean?


The concept of active spectrum is easier to illustrate with the following example: as we said before, in general all the spectra in an arrayed item are processed exactly with the same processing operations. For example, same level of zero filling, same apodization function, same FT type, same phase correction, etc. However, it i's possible that some particular spectra require a slightly different processing, independently from the others. In order to do that, it is necessary to select the applicable spectra. See below the difference between selected and active spectrum:

**Selected spectra:** when the spectra are selected, they are highlighted with a light blue background. Any processing operation will take place only for those selected spectra

Active Spectrum: active spectrum is marked with a blue box and it indicates the spectrum which will be displayed in the *active spectrum* display mode. It's also the reference spectrum used in some processing operations (e.g. alignment)

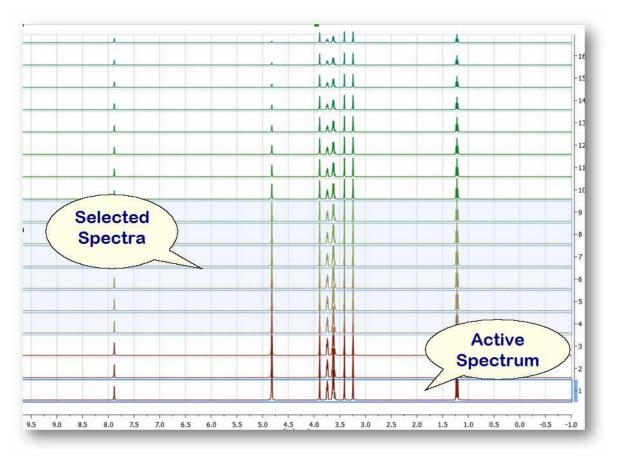


You can also **select** several slides by using the check boxes on the right of the 'Stacked Items Table'. When the spectra are selected, they are highlighted with a light blue background. Any processing operation will take place only for those selected spectra.

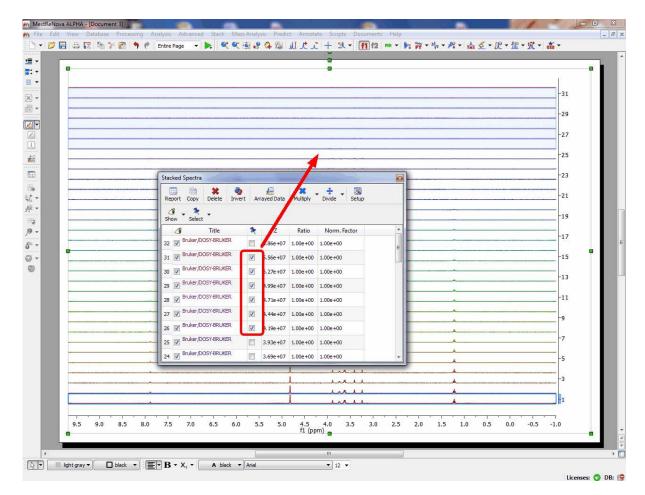


#### Example #1:

If there are no spectra selected and the active spectrum is not either selected (i.e. no spectra have a blue background) then **any processing operations will be applied to ALL spectra (**Active spectrum is not selected)

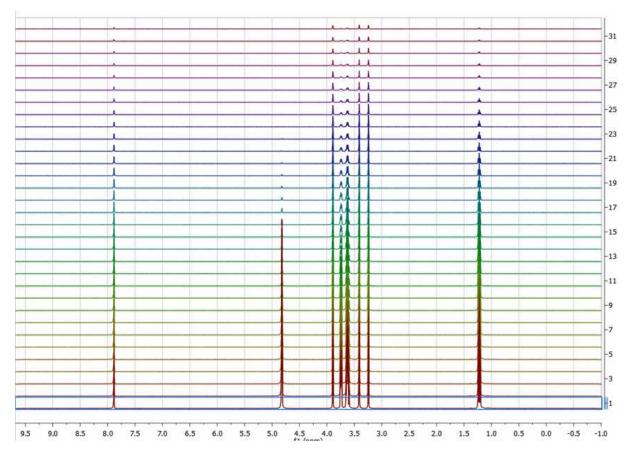


Example #2: If only the active spectrum is selected, *any processing operations will be applied ONLY to the active spectrum.* (Remember, to select a spectrum: left click + Alt)

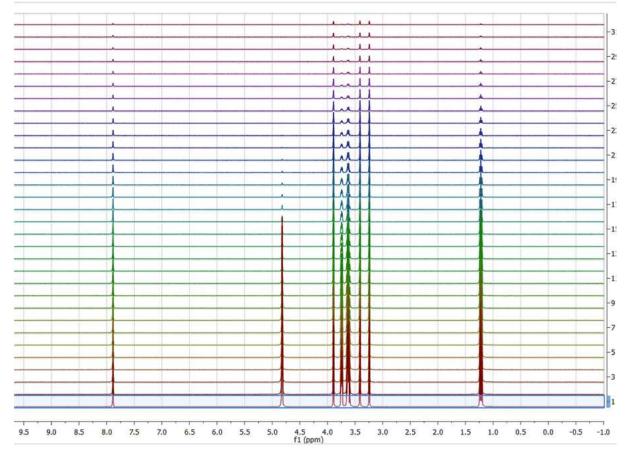

Example #3:


In general, *any processing operation will be applied only to the selected spectra* (and remember that if no spectra are selected, All spectra will be processed):

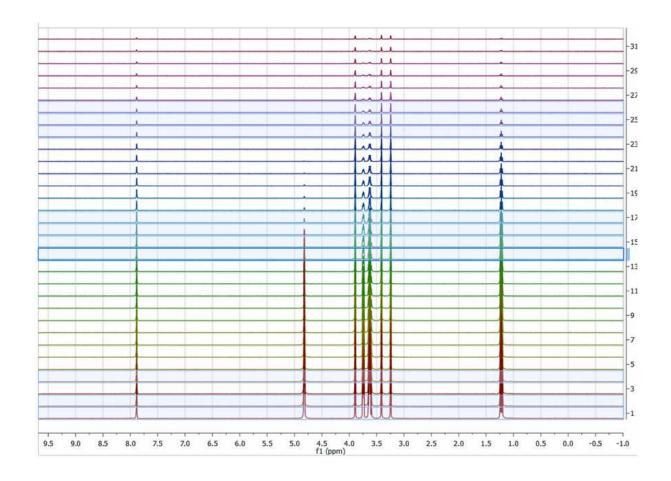

So, how can we change the active spectrum? There are 3 different ways:

- 1. Just click on the spectrum you want to be active.
- 2. Use SHIFT + Mouse Wheel to navigate throughout all the spectra in the stack, one after the other.
- 3. Use SHIFT + Up/Down arrow keys. This is analogous to point 2)


(B). If the number of subspectra (traces) is large (e.g. > 10), working in the stack mode might not be very practical. Quite often, working only with the active spectrum on the screen will be a much better option. This mode can be activated as shown in the image below.

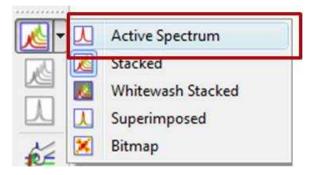


While working on this mode, you will see on the screen just the active spectrum. Should you want to

move to another spectrum without resorting to the stack mode, just use methods 2) and 3) described above (Shift+Mouse Wheel or Shift + Up/Down keys).

(C) Another useful display mode consists of superimposing all subspectra (see figure below). This method is very useful, for example, when you want to check whether some peaks shift their position (for instance, due to differences in pH, temperature, etc., as is common in biofluids spectra).

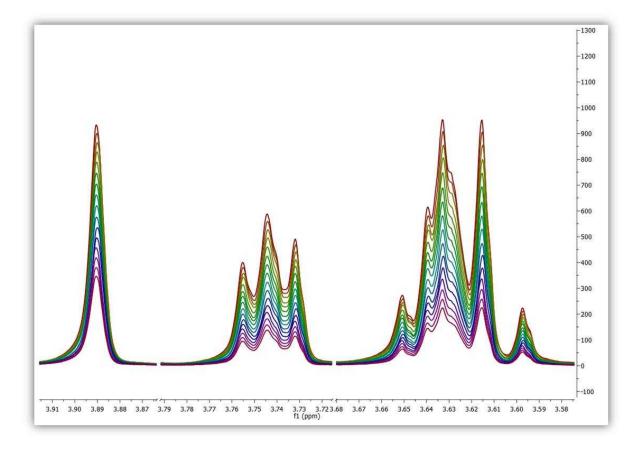

Finally, there is an additional display mode, the so called whitewashed stacked plot. The whitewashing effect means that the spectra at the front of the display hide the spectra behind them from view, as depicted in the figure below.

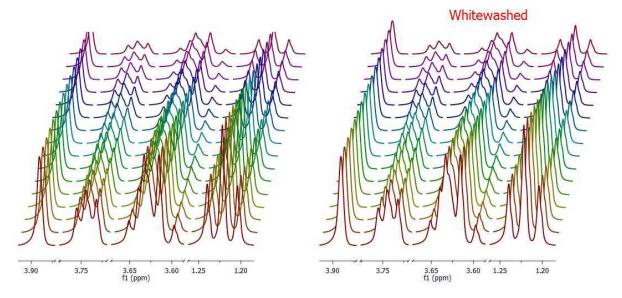

This plotting mode can be useful to create nice reports, but it's important to emphasize that drawing time will be significantly higher than with the other plotting modes, so it is not recommended when processing the spectra in real time (e.g. interactive phase correction).

# Extracting and calculating useful NMR related molecular information


After the basic introductory lines on arrayed NMR experiments, it's now time to get some action and see how to extract relevant information from these experiments and calculate useful NMR related parameters such as diffusion, relaxation times, kinetics constants, etc.

Actually, in this tutorial we will cover the first case, that is, the analysis of PFG experiments to calculate diffusion coefficients.


This is how a PFG (Pulsed Field Gradient) experiment can be analyzed with <u>Mnova</u> with the Data Analysis module (for your information, Mnova includes a DOSY-like processing algorithm based on a Bayesian Algorithm. For further infomration about it, please take a look at this tutorial: <u>http://mestrelab.com/dosy.html</u> and this post: <u>http://nmr-analysis.blogspot.com/2008/09/baydosy-whats-under-hood.html</u>

You can download the full PFG data set used in this tutorial from here.

Once the arrayed spectra has been loaded into Mnova, issue menu command Advanced/Data Analysis. The so-called Data Analysis widget will popup. This will be the central control panel (see figure below) for anything related to the analysis of arrayed experiments.

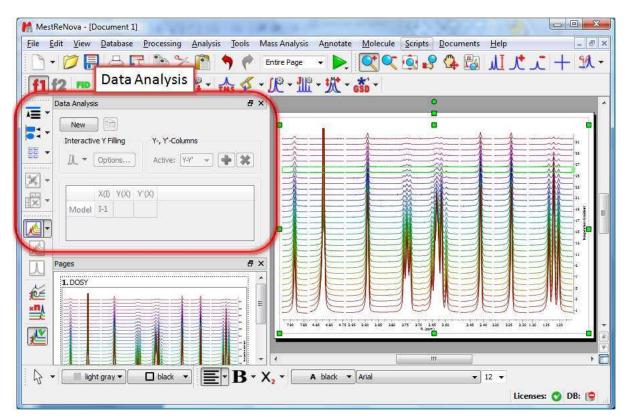

Its operation is very simple. The first thing you have to do is click on the New button. As a result, Mnova will populate the X-Y Table with some initial values (as described below) and create a new item, the so-called Data Analysis Plot. This new item will display the values from the X-Y Table which in general are the values extracted from the arrayed spectra, both experimental (Y) and fitted (Y').

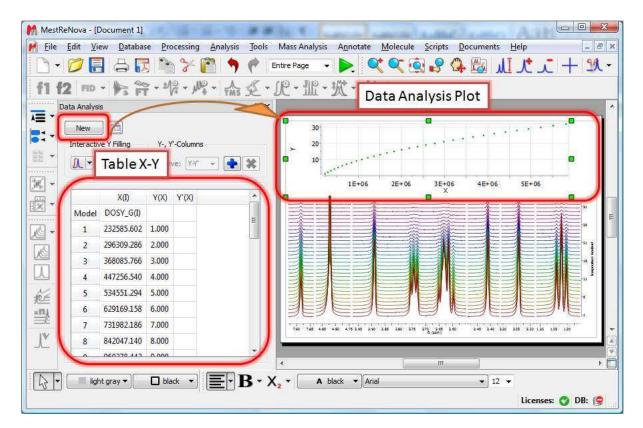

### The X-Y Table

This table is composed by one X column, X(I), one or several Y-columns (Y, Y1, Y2, etc) to hold the experimental values extracted from the arrayed spectra and one or several Y'-columns which hold the fitted values of their Y counterpart columns.

#### X-Column

When the table is initialized, in the case of PFG experiments the X-column is populated with the Z values from the Diffusion table, that is, the gradient strengths scaled by taking into account the constants from the selected Tanner-Stejskal model. In the case of a relaxation experiment, the X column will contain the time delays. Of course, it is possible to change the contents of the X-column by following any of these methods:


• Manual editing of the individual cells

	X(I)	Y(X)	Y'(X)	1
Model	DOSY_G(I)			
1	232585.602	1.000		
2	296309.286	2.000		
3	368085.766	3.000		
4	447256.540	4.000		

• Copy & paste from a text file. For example, you can put the values for the X-column into a text (ASCII) file and then paste its contents into the table. To do that, just right click on the first cell you want the paste action to start from.

	X(I)		Y(X)	Y'(X)	<u>^</u>
Model	DOSY_G	6(T)			
1	232585.6	50.2	1 000		
2	296309.	3	Use Fo	rmula Valu	e
	368085.		Paste		Ctrl+V
3	09572-8575	-010	20201000		1
4	447256.5	540	4.000		

• Enter a formula into the Model cell. Double click on the X(I) model cell (1) and then enter the appropriate equation to populate the X column (2). For example, if you simply enter I, the X column will be filled in with numbers 1, 2,3, etc. If you enter a formula like 10+25\*I, the X column will be filled with numbers 35,60, 85, etc.

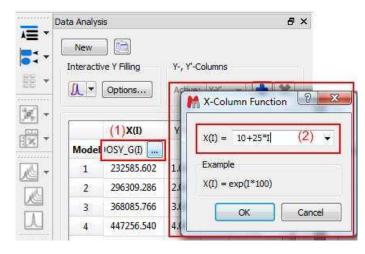


#### Y-Column

In all cases, when the table is initialized, the Y-column is automatically filled in with values 1,2,3, etc. The purpose of this column is to hold the experimental values from the arrayed experiment. For example, in the case of a PFG experiment, it may contain how the intensity (or integral) of a given peak (or set of peaks) evolves as the applied pulse field gradient changes. Likewise, in the case of T1/T2 experiments, this column will show the relaxation profile of a given resonance (or set of resonances). So the question is: how to populate the Y-column with actual information from the spectra?

This is again very easy. There is a graphical way (mouse driven) and a manual one. Let's start with the graphical method:

• **Graphical Selection:** Click on the 'Interactive Y Filling' button (see red-highlighted button in the image below). After doing this, the cursor will change into an integral shaped cursor expecting you to select the region from where you want the integrals to be extracted across all the subspectra in the arrayed item. After the selection is done (see figure below), all the integrals will be placed in the Y column and those values will be displayed in the X-Y plot as green crosses (note: the shape, color, etc of these crosses can be customized from the X-Y plot properties).

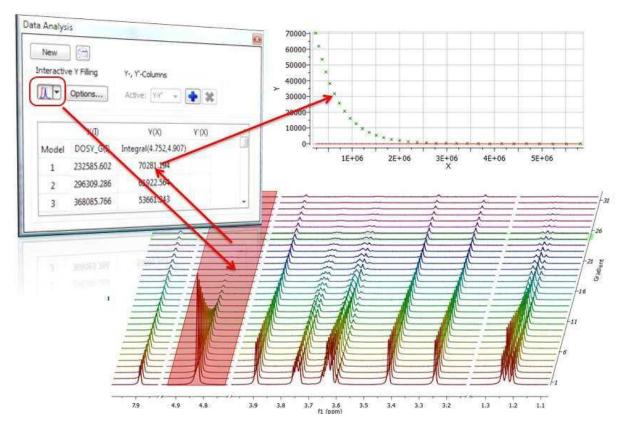

• **Manual selection:** if you take a closer look at the Data Analysis table in the figure above, you can appreciate that once the integral region has been selected, the program shows the following text: Integral(4.752, 4.907). This means that we have selected an integral covering that range. This value can be edited manually so that you can specify the limits by simply editing that cell.

#### Y'-Column

The Y' column is reserved for the fitted values assuming a particular theoretical model (e.g. a exponential decay). In this particular case, as we are dealing with PFG experiments, we will be interested in the calculation of the Diffusion coefficients and thus, our fitting model could be a mono-exponential decay (multi-exponential decays can also be handled with this module, but I will not address this problem in this post). The process is very simple:

First click on the Y'(X) cell and then on the small button with 3 points as indicated in the figure below:

New				
nteractiv	e Y Filling	Y-, Y'-Columns		
	Options	Active: Y-Y' +	+ *	]
	X(I)	Y(X)	Y'(X)	2
Model	DOSY_G(I)	Integral(4.730,4.911		
1	232585.602	70382.682		
2	296309.286	61990.0 <mark>9</mark> 4		
3	368085.766	53716.519		
4	447256.540	45795.940		
5	534551.294	38432.420		
		250.000		13

This will launch a dialog box with powerful fitting capabilities.


	Name	Function	Initialization	Description	Algorithm
Ĺ	Mono-exponential	B*exp(-x*F)		Exponential Decay (e.g DOSY)	monoExponential
2	Three parameter exponential fit	B+F*exp(-x*G)		Exponential Decay with Baseline Offset	monoExponential
3					general
4					
cto	ed Parameters				
1000	Carcolate				

This dialog provides two predefined functions useful for fitting mono-exponential data (such as PFG and Relaxation NMR experiments) using either a 2- or a 3-parameter fit. Furthermore, this dialog offers the possibility to enter user customized functions.


For the time being, suffice to say that if your problem regards mono-exponential functions, just select any of the 2 predefined functions in the dialog box and click on the Calculate button. Mnova will immediately compute the optimal values, returning these optimal values as well as the fitting error and the probability that the acquired series follows the chosen monoexponential model.

	Name	Function	Initialization	Descripti
1	Mono-exponential	B*exp(-x*F)		Exponential Decay (e.
2	Three parameter exponenti	B+F*exp(-x*G)		Exponential Decay wi
	Calculate			
	Calculate			
B=	0.620083, F= 112465, G= 2.0 rror = 2.02261e-09, probnotmon			

Finally, after closing the dialog, it will populate the Y' column and the X-Y will be updated with the fitted curve (Red line in the figure below).

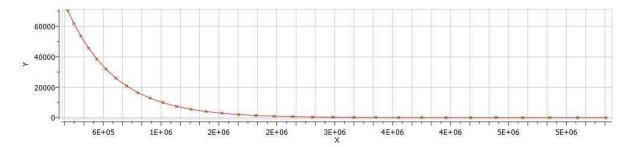

One nice feature of the Data Analysis module is its ability to handle multiple series. For example, it's possible to analyze the decay of several resonances within the same experiment. In order to do that, just click on the (+) button to add a new series and repeat the same process to select the desired resonance range and fit the values. For example, in the figure below I'm showing two curves with different decay rates.

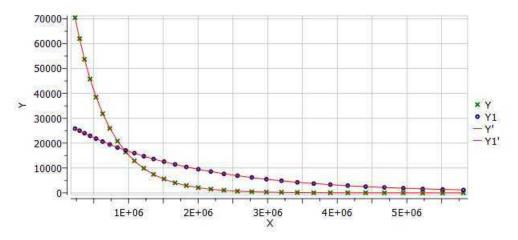


Of the different existing methods for the extraction of peak intensities from arrayed NMR spectra, Mnova provides the following ones:

(1) Peak area integration

This is the default method in Mnova Data Analysis module (see figure below)

Data Analysis	8 ×
New Interactive Y Filling	Y-, Y'-Columns
↓ Pick Integrals	
Pick Peak	

This method consists of a standard numeric integration over the whole peak. Basically, the program is summing up all the points within the selected area of interest) as illustrated in the figure below:

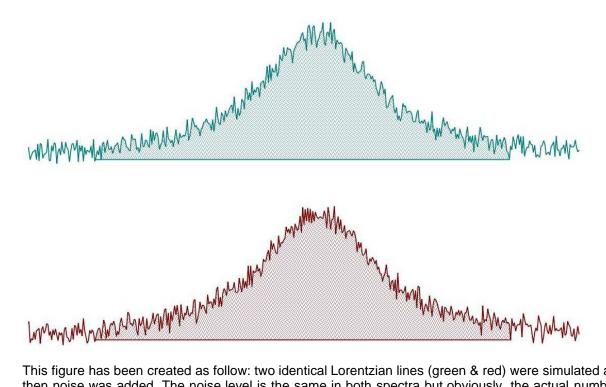

This figure has been created as follow: two identical Lorentzian lines (green & red) were simulated and then noise was added. The noise level is the same in both spectra but obviously, the actual numbers are different (more technically, noise in both spectra was calculated using a different seed in the random number generator).

This peak area method for data extraction is quite robust to noise (provided that the noise level is more or less constant across the different spectra in the arrayed experiment) and more importantly, insensitive to chemical shift fluctuations from trace to trace in the experiment, a situation which is more frequent than generally realized. For these reasons, and for its simplicity of use, this is method of choice for well-resolved peaks. If the peaks of interest exhibit some degree of overlap, this method is not very reliable and some of the next methods will be more convenient

(2) Peak Height Measurement

This is the second method for data extraction (see figure below) and it finds the peak height at a given chemical shift across all the spectra in the arrayed experiment.

Data Analysis	8 ×
New D	
Interactive Y Filling	Y-, Y'-Columns
∬ ▼ Options	Active: Y-Y' 👻
Pick Integrals	
📌 Pick Peak	
Pick Max. Peak	

By default, the program will find the peak intensity at the position indicated by the user (using a vertical cursor) and then it will perform a parabolic interpolation in order to refine the value. In addition, the user can specify an interval in such a way that the program will find the maximum peak within that region. This can be done in 2 different ways:


• i) If you click in the Options button, you can define whether you want to use Parabolic and the interval in which the maximum should be found (in ppm

🖌 Y-Filling Op	otions 💡 🛛 🗙
Peak Intensit	ies
🔽 Parabolio	Interpolation
f1 +/-:	0.00
ОК	Cancel

• (ii) Alternatively, once a peak has been selected, you can change the interval by direct editing of the peak selection model. In the figure below, you can see how the peak selection model is PeakIntensity. The first number (6.001 in the figure) corresponds to the central chemical shift whereas the second number (0.100 in the figure) represents the interval for the peak maximum search.

ta Analysi	S		đ
New	1 🖻		
Interactiv		Y-, Y'-Columns	
Interactiv	errinng		
-	Options	Active: Y-Y' 👻 🌸	×
Land L	S-112		
	ХФ	V(X)	V'(X)
	X(I)	Y(X)	Y'(X)
Model	12-540 R	Y(X) PeakIntensity(6.001,0.100)	Y'(X)
Model	12-540 R	1.5545	

Parabolic interpolation is useful because it minimizes the problems caused by the random noise. For example, let's assume that Parabolic interpolation is not used so that peak heights extraction will be done always at the same fixed chemical shift position (see figure below). When this method is used the values are seen to be quite different in the two cases: here the precision of the measurement will depend strongly on the noise.

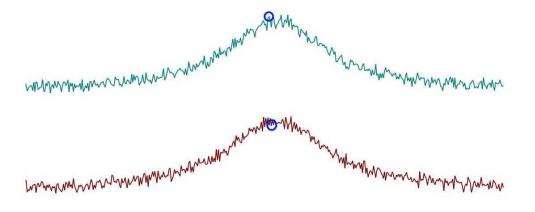

Parabolic interpolation and/or measurement of the intensity as the maximum height within a fixed box around the peak will help to minimize the effects of movements on the chemical shift position of the peaks due to, for example, temperature instability, pH changes, etc.

For convenience, Mnova includes the so-called Pick Max. Peak method which is totally equivalent to the previous one but it allows the graphical selection of the left and right boundaries in which the maximum peak will be searched for.

In a nutshell, peak height measurement can be used in those cases in which peak overlap might represent a problem. However, it should be noted that if for some reasons the line widths of the peaks under analysis change from trace to trace, peak heights will not represent a reliable measurement and peak integrals should be used instead.

In general, we would recommend peak integrals as the most general-purpose method for quantitation of peak intensities in arrayed experiments.


# Binning and NMR Data Analysis

It is well known that many NMR arrayed experiments suffer from unwanted chemical shift variations due to fluctuations in experimental conditions such as sample temperature, pH, ionic strength, etc. This phenomenon is very common in NMR spectra of e.g. biofluids (metabonomics/metabolomics) but

also exists in many other experiments such us Relaxation, Kinetics and PFG NMR spectra (diffusion).


This problem negatively affects the reliability of quantitation using, for instance, peak heights, and for this reason integration is, in general, a more robust procedure as these spectral variations are mitigated by averaging data points over the integral segment. We will try to show you one simple trick which helps to understand, in a pictorial way, why integration is useful to remove the major part of chemical shift scattering.

First, consider the following experiment depicted in the figure below. It shows a triplet and as you can see, some minor peaks shifts are present from spectrum to spectrum:

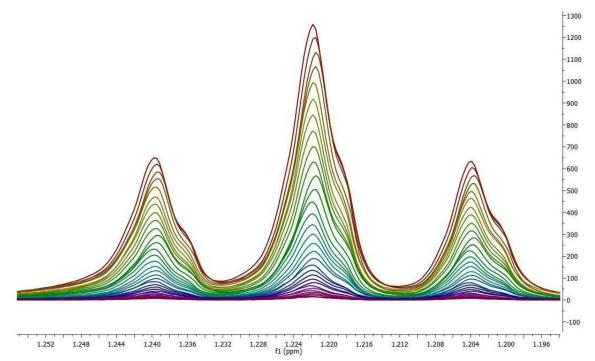

If peak heights are determined at a fixed position, this might introduce appreciable errors in the posteriori quantitative analysis (e.g. exponential fitting). As described before, this could be circumvented in some extent by using parabolic interpolation or peak searching of the maximum in a predefined box.

Nevertheless, integration is a very simple solution as can be appreciated in the figure below. Instead of using the Peak Integrals tool in the Data Analysis module, we will show now a complementary procedure. Basically, what we have applied to all spectra is the well-known <u>binning</u> operation which consists of dividing each spectrum in equally sized (e.g. 0.01 ppm in this case) bins, so that integral (area) of each bin represents a new point in the binned spectrum.

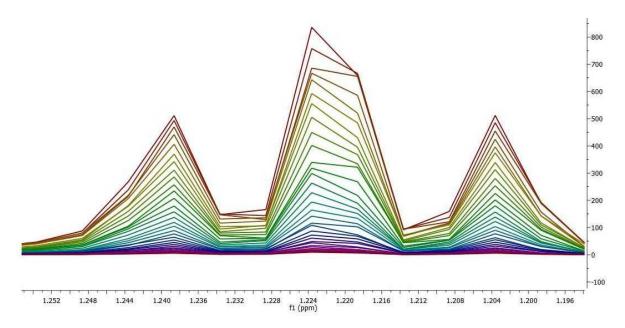


As seen in the figure above, binning clearly removes the effect of chemical shift changes but of course, at the cost of a significant reduction in data resolution.

## 13.3 Superimposed Spectra

It is very easy to **Superimpose Spectra** with Mnova. Just select the desired spectra on the page navigator (by holding down 'CTRL/Cmd key' while clicking on each spectrum) and then issue the command 'Stack/Superimpose spectra'.


- 💋 🖪 👌 I	5 3 7 0	🖣 🥐 🛛 Entire Page	-	🚺 🔏 Stack Spectra			
Pages	8×			Superimpose Spectra			
, 1. Quinine 1H	i E	r		Extract Active Spectrum Extract All Spectra			
		Quinine 1H 1H. Quinine	16 11				
2. Quinine 1H				Show Arrayed Data Table			

Finally, you will obtain the overlaid spectrum (one spectrum on top of the others):

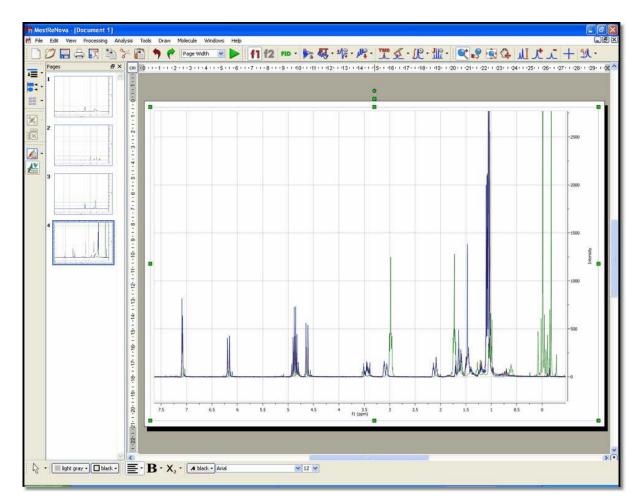

It is possible to apply any analysis feature (peak picking, integration or multiplet analysis) to the superimposed spectra and then take a look at the result over each trace by selecting 'Active Spectrum' in the 'Stacked' scroll down menu. To navigate through the traces, press and hold down **SHIFT** and use the up or down arrow key (or use the mouse scroll wheel)

You will also be able to obtain the superimposed spectrum from a stacked one by selecting **'Superimposed'** on the stacking mode (vertical-left toolbar) or by following the menu 'View/Stacked Mode/Superimposed':

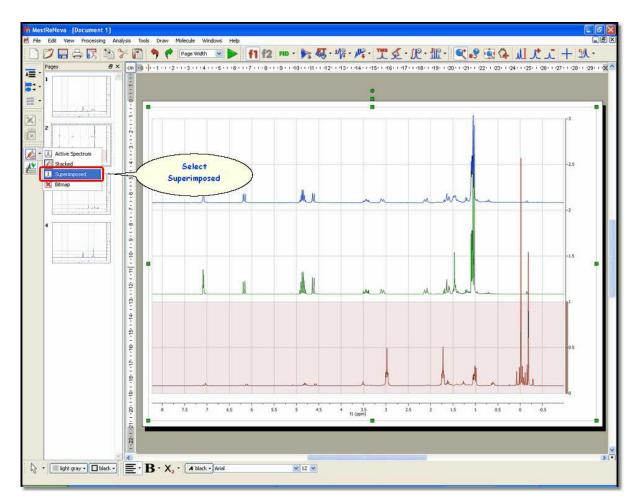


If you have several spectra on the same page (to obtain it, just paste the desired spectra to one page, by using Ctrl/Cmd+C, to copy, and Ctrl/Cmd+V, to paste), you can also superimpose them by following the menu 'Edit/Alignment/Align Left (or by using other alternatives in the vertical-left toolbar) after having selected all of them (by Ctrl/Cmd+A, or Edit/Select All').

## 13.4 How to process Varian DEPT spectra?

This tutorial will show you how to process a Varian DEPT spectrum. As you well know, the DEPT pulse program in Varian generates a stacked plot with four slices, acquired with phase of the last pulse equal to 45, 90, 90, 135 degrees.


When you load this kind of spectra into Mnova, you will obtain something like this (if in the Edit/ Preferences/NMR/Import' you have the VnmrJ DEPT processing unchecked):

#### Tutorials

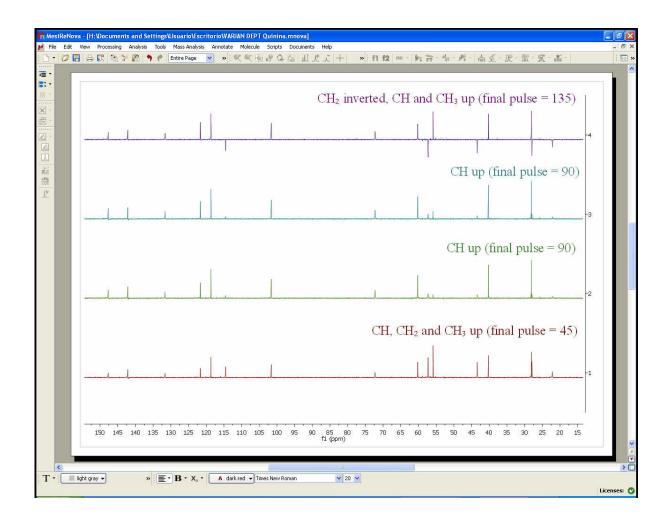


As you can see, you will have in the first slice (red slice with final pulse: 45 degrees) all the protonated signals, in the second and third slices you will get only the CH signals up and in the forth slice (purple slice with final pulse of 135 degrees) a spectrum with the CH and  $CH_3$  up and the  $CH_2$  down

Then, please make sure that the phase of all the slices is right. If not, you will need to apply a phase correction. We recommend you to select 'Active spectrum' in the sixth button of the left-vertical toolbar:



While working on this mode, you will see on the screen just the active spectrum (the spectrum which is highlighted in green in the stacked plot). Should you want to move to another spectrum without resorting to the stack mode just press Shift+Mouse Wheel or Shift + Up/Down keys.


We are going to correct slightly the phase of the first slice (the phase of the other slices will be automatically corrected):

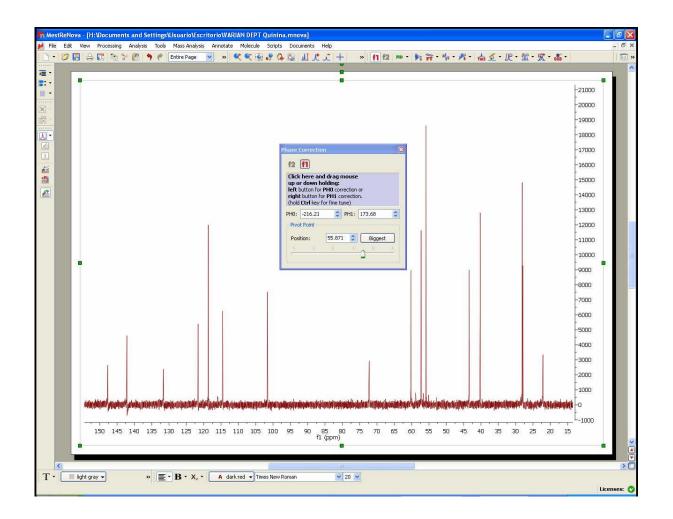




Remember that even if only the active spectrum is visible, unless the "Apply Processing to All spectra in Stack" option is off, all spectra in the stack will also be processed.

Finally, follow the menu 'Scripts/NMR Tools/DEPT Traces':

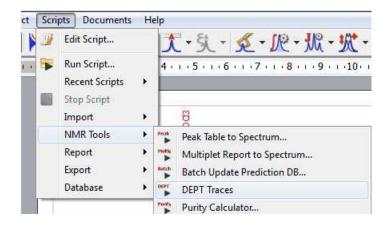

After having applied the script, you will obtain all the protonated carbons in the first slice (red), the CH in the second slice (green), the  $CH_2$  in the third one (blue) and the  $CH_3$  in the forth slice (purple), as you can see in the picture below:

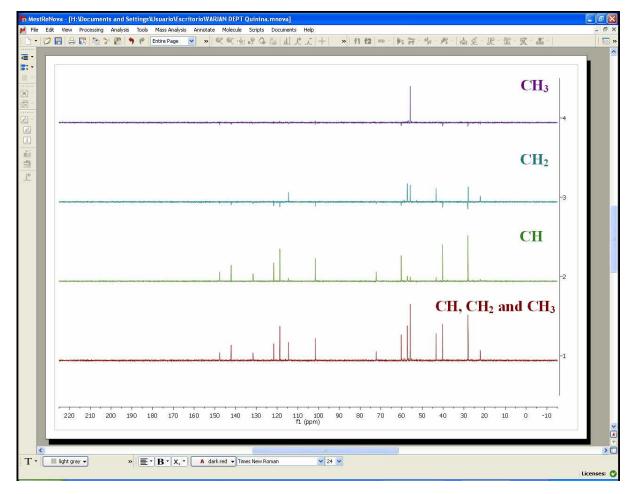


Please bear in mind that the relative intensities of the signals are not exactly the same in all the slices, so it is possible that you get small residues in some of the slices.

You could also use the Arithmetic feature to process your Varian DEPT spectra, by following the menu 'Processing/Arithmetics' and enter the following formula:

ре	ectra	File	name: Varian DEPT formula_new; .mnfr
	Label	Title	Formula
1	A1	dept	3*A1
2	A2	dept	2*A2
3	A3	dept	A3 - 1.5*A4 + A4 + 1.3*A1 - 1.8*A2
4	A4	dept	A4 + 1.3*A1 - 1.8*A2

Please bear in mind that you can save this formula by using the 'Save' button  $\blacksquare$  .

If your dataset shows eight spectra means that it contains two arrayed variables "mult" and "qphase".

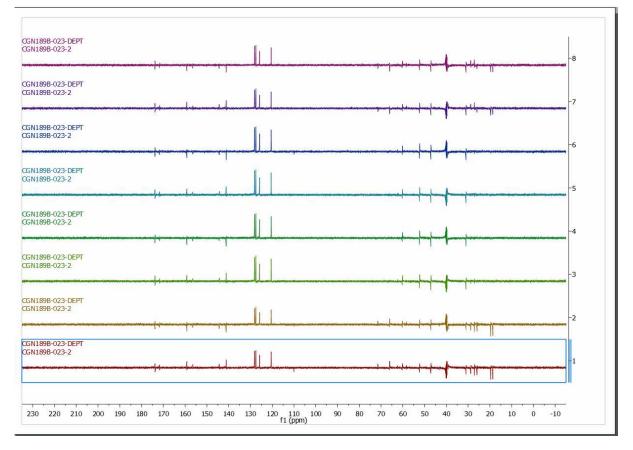

The arrayed variable mult '0.5 1 1 1.5' refers to the type of DEPT spectrum, in this case DEPTQ 45°, DEPTQ 90°, DEPTQ 90° and DEPTQ 135°, respectively

The arrayed variable qphase '1 -1' refers to the sign of the quaternary carbons + and -, respectively.


This is the meaning of the eight spectra:

spectrum1: +CH + CH2 + CH3 + Cq (deptq45 qphase 1) spectrum 2: +CH + CH2 + CH3 -Cq (deptq45 qphase -1) spectrum 3: +CH 0 0 +Cq (deptq90 qphase 1) spectrum 4: +CH 0 0 -Cq (deptq90 qphase -1) spectrum 5: +CH 0 0 +Cq (deptq90 qphase 1) spectrum 6 : +CH 0 0 -Cq (deptq90 qphase -1) spectrum 7 : +CH -CH2 +CH3 + Cq (deptq135 qphase 1) spectrum 8 : +CH -CH2 +CH3 - Cq (deptq135 qphase -1)


By doing aritmetics with the 8 spectra you can obtain the edited spectra. For instance the following combinations:

```
Only Cq: 1 - 2 + 3 - 4 + 5 - 6 + 7 .7
Only protonated carbons: 1 + 2
Only CH = 3 + 4 + 5 + 6
Only CH2 = 1 + 2 - 7 - 8
All carbons = 1
```


You will be able to process those datasets by following the menu 'Scripts/NMR Tools/DEPT traces'.

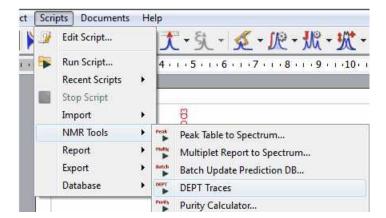

After having run the script, a phase correction may be needed. If you need to apply a different phase correction for each trace, just hold down the Alt key and click on the desired trace (or open the Stacked Items Table) to finally correct the phase:

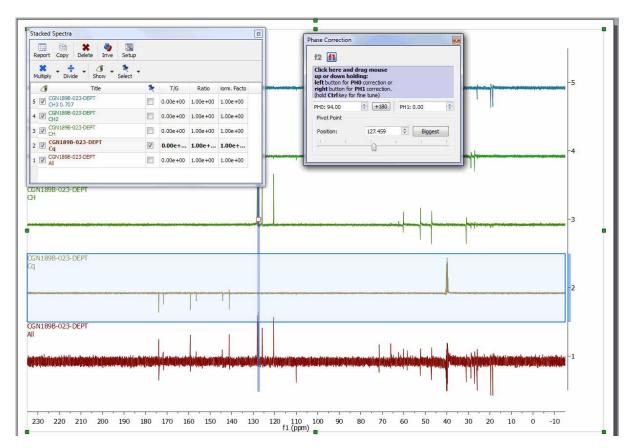

After having corrected the Phase to all the traces, this will be the result (from up to down: CH3, CH2, CH, quaternary and All carbons):

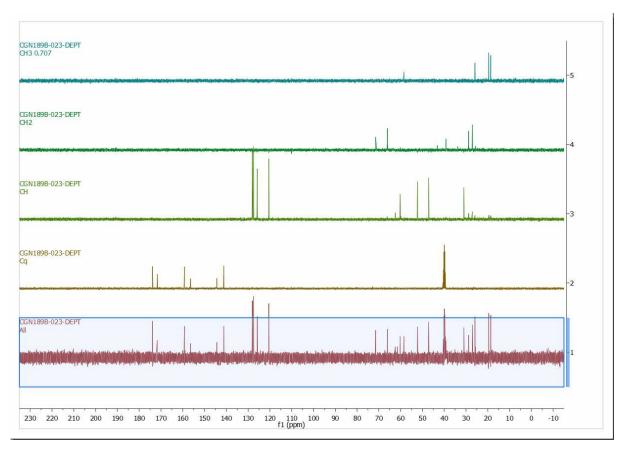

## 13.5 Mnova for metabonomics

Mnova allows you to easily process large datasets with the best quality in order to obtain the most precise results. Once datasets have grown to 20-200 spectra, **manual processing is no longer an option**.

Mnova can automate the processing of **large datasets of biofluids** to extract an ASCII file ready for the statistical measurement.

Mnova includes powerful specific **Phase and Baseline Correction algorithms for** 1D and 2D **biofluid spectra** in order to get the correct quantification

## **Getting Started**

Mnova can be used on large datasets of biofluid spectra in two main ways, depending on the size of the dataset.


**Graphical (<100 spectra)**: this mode allows all processing commands to be executed on a group of spectra simultaneously making possible the interaction with all spectra at the same time.

**Scripting (>100 spectra):** the user will only need to open a single spectrum of the dataset and optimize the processing in order to apply it to the remaining spectra by using the scripting capability implemented in Mnova.


## **Processing Basics**

Let's take a look at the 'graphical method'.

1. When the dataset is small, we can drag the spectra folders to Mnova in order to get all the spectra fully processed (you can also use the multiOpen script). In this case I have dragged 16 spectra folders to the Mnova icon. After about 5 seconds, I got all the spectra fully processed as you can see in the picture below

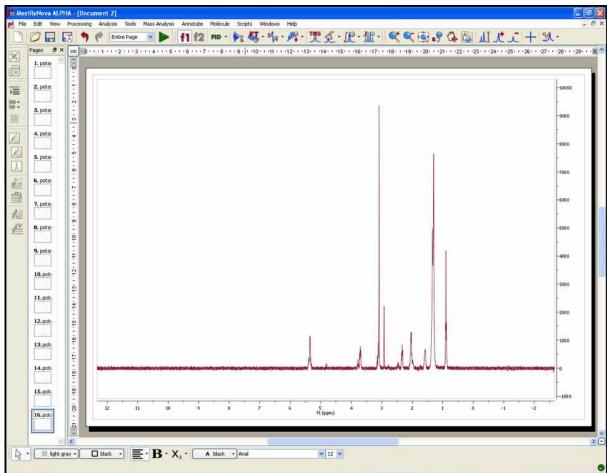


**2.** Select all the spectra in the page navigator in order to create the stacked spectra. We can do it by pressing 'Ctrl/Cmd+A' or by following the menu 'Edit/Select All' and then clicking on the 'Stack Spectra' button (in the left-vertical toolbar) or going to the 'Stack/Stack Spectra' menu.

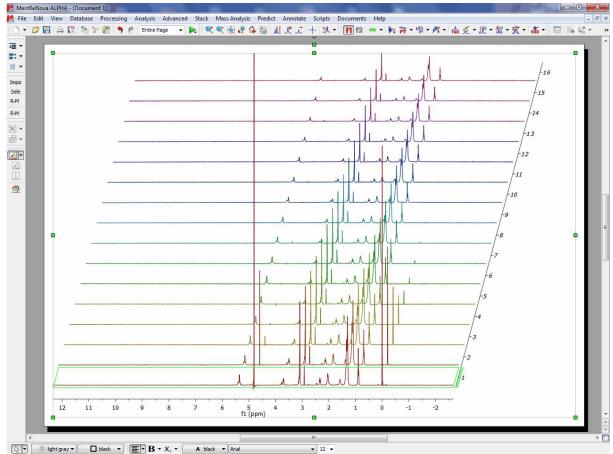

Licenses: 🕥 DB: 🧐


**3.** Select one of them (by selecting 'Active Spectrum' in the Stack scroll down menu of the left-vertical button) and apply the necessary processing and analysis (phase and baseline corrections, binning, signal suppression...). The operations to the first spectrum will be applied simultaneously over the whole dataset.

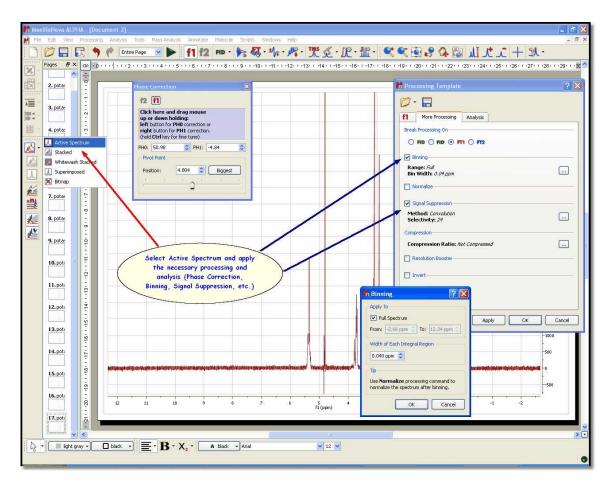

Mnova incorporates several specific features for biofluid samples; such as **Automatic Phase and Baseline corrections algorithms**, **Solvent Suppression** (to remove, for example, the dispersive signal of the water), **Auto-tuning referencing**, **Binning** (or bucketing), **Normalize**, **Global Spectral Deconvolution** (work in progress).

**4.** Once the processing and analysis have been made, we can export to an ASCII file for the PCA or PLS, just by following the menu 'File/Save As/ASCII text file (\*.txt)'.

ave As							?
Guardar en;	C decra	1.fid		 •	÷ 🗈 😋	* 📰 •	
Ò							
Documentos recientes							
B							
Escritorio							
3							
vlis documentos							
<b>S</b>							
Mi PC							
		12	1049620				2000
Mis sitios de red	Nombre:	14	nt 2.mnova			-	Guardar
	Tipo:	ASCII T	ext File (*.txt)				Cancelar

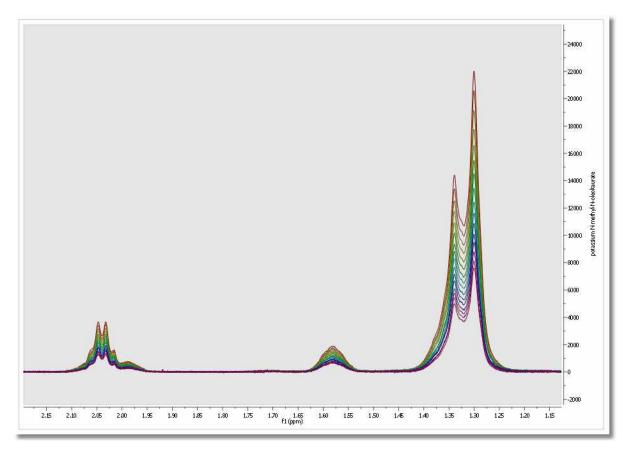

Highlight the stacked spectra and follow the menu 'Stack/Superimpose Spectra' to overlay them (useful for example to check that all spectra are perfectly aligned of referenced):

# **Scripting Method**

Let's take a look at the 'Scripting method'.

Mnova includes **Scripting capabilities** to automate the previous process with the ability to create Processing Templates which can be used with our Script engine to perform batch processing.

**Mnova** includes a powerful and flexible feature which allows the user to easily automate the full processing of both 1D & 2D NMR data sets. This is ideal for the batch processing of spectra of the same type, and can also incorporate analysis operations.

For example, let's say you have acquired 20 proton spectra which you want to process using the same processing operations. The procedure is very simple:

- 1. Load one spectrum and process it as desired.
- 2. Go to Processing/Full Processing. The following dialog appears:




This dialog includes all the processing and analysis features implemented in **Mnova**. You can choose the required options by selecting the check boxes and, if necessary, specify options by clicking the button next to the corresponding command.

3. Once you are happy with the result, **save** the script file to a Mnova Processing file (\*.mnp) by clicking on the save button in the dialog box.


Once you have saved this template, you will be able to run a script to process all the spectra in the same way.

If the number of datasets is too large, Mnova is able to open, process (apodization, FT, Zero Filling, LP, phase and baseline Correction...), analyze (binning, etc.), save to an ASCII file and close the spectrum, in order to open the next one and continue with the processing (to avoid an excessive use of memory). If the number is not large, Mnova can keep all the spectra fully processed on screen.

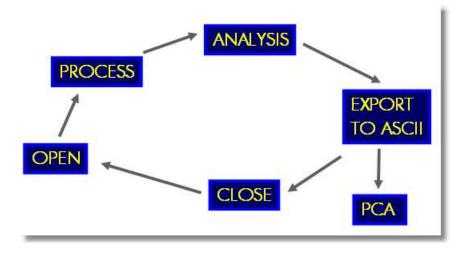

You can use the below script to automate the above process and save all the result into the same ASCII file. You will be able to download it <u>here</u>

Copy this script to the scripts folder of Mnova, restart the software and the script will appear under the ' Scripts' menu.

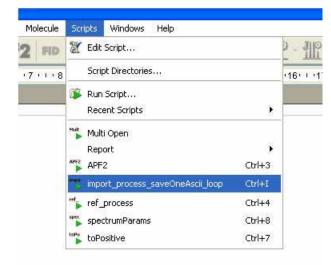

Please bear in mind that you can introduce this script into the toolbar by using the 'Toolbar Customization' feature (View/Customize User Interface/Customize Toolbars').

To read more about Mnova scripting, please click here

```
//<GUI menuname="import_process_saveOneAscii_loop"shortcut="Ctrl+I"tooltip="Auto Process and</pre>
Save as ASCII"/>
                                                                 * * * * * * * * * * * * * * * * * * *
Copyright (C) 2008 Mestrelab Research S.L. All rights reserved.
This file is part of the MNova scripting toolkit. Authorized users of MNova Software may use
this file freely, but this file is provided AS IS with NO WARRANTY OF ANY KIND, INCLUDING THE
WARRANTY OF DESIGN, MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.
// This example function demonstrates how to apply some processing to a set of spectral files
and to save the result in a single ASCII file.
function import_process_saveOneAscii_loop()
      const procName = "c:/procTemplates/proc.mnp"; // Processing file. It must be created in
the Processing Template dialog of MestReNova.
      const fileMask = "fid"; // This mask specifies files to be processed.
const dirMask = "*"; // This mask specifies directories to be scanned for spectra.
      // Select a directory with spectral data
      const specDirKey = "import_process_saveOneAscii_loop/SpectraDir";
      var dirName = FileDialog.getExistingDirectory(settings.value(specDirKey, Dir.home()),
"Select Spectra Directory");
      if (!dirName)
            return
      var dir = new Dir(dirName);
      dir.cdUp();
      // Select a file to save the output
      const outDirKey = "import_process_saveOneAscii_loop/OutputDir";
      var saveDir = settings.value(outDirKey, Dir.home()); // Get last used directory name
      var fileName = FileDialog.getSaveFileName("ASCII Files (*.txt)", "Select Output File",
saveDir);
      if (!fileName)
            return;
      // Open the selected file and create a text stream mapped to it
      var fout = new File(fileName);
      settings.setValue(outDirKey, fout.absDirPath); // Save the directory name to be used
```

```
another time the script is called
     var sout = new TextStream(fout);
      sout.precision = 10;
      // Temporary file name
      const lastOutName = Dir.temp() + "/import_process_saveOneAscii_loop.lastOut.tmp";
      if (File.exists(lastOutName))
            File.remove(lastOutName);
      // The below function getMaskFiles is located in the files.qs script.
      var files = getMaskFiles(dirName, dir.absPath, fileMask, dirMask, true);
      for(var fi = 0, length = files.length; fi < length; fi++)</pre>
            var dw = new DocumentWindow(Application.mainWindow.newWindow()); // Create new
document window
            if (serialization.open(files[fi]))
            {
                  nmr.process(procName); // Apply processing template
                  var spec = new NMRSpectrum(nmr.activeSpectrum());
                  fout.open(File.WriteOnly);
                  var flastOut = new File(lastOutName);
                  var slastOut = new TextStream(flastOut);
                  if (!fi)
                        // Put fist column of the file in ppm. The scale is taken from the
                  ł
first spectrum.
                        flastOut.open(File.WriteOnly);
                        slastOut.precision = 10;
                        var ppm = spec.hz()/spec.frequency();
                        var dPpm = spec.scaleWidth()/spec.count()/spec.frequency();
                        for(var si = spec.count()-1; si >= 0; si--)
                        ł
                              slastOut.write(ppm, "\n");
                              ppm += dPpm;
                        flastOut.close();
                  flastOut.open(File.ReadOnly);
                  for(var si = spec.count()-1; si >= 0; si--)
                        sout.write(slastOut.readLine(), "\t\t", spec.real(si), "\n");
                  fout.close();
                  flastOut.close();
                  flastOut.remove();
                  if (fi < length-1)
                        File.copy(fileName, lastOutName);
            dw.close(); // Close document window of processed spectrum
```

### 13.6 Show Traces in 2D-NMR

The user can show the traces of the 2D-NMR spectrum, just by clicking on the **'Show Traces'** icon (or by using the contextual menu by right clicking over the spectral window). On the same icon, you will find a scroll bar menu to setup the vertical and herizontal traces of a bidimensional spectrum.

you will find a scroll bar menu to setup the vertical and horizontal traces of a bidimensional spectrum. The user can increase or decrease the intensity of the traces simply by scrolling the mouse wheel, after hovering the mouse over the desired trace (or by using Ctrl/Cmd+Shift+Up/Down for the horizontal trace and Ctrl/Cmd+Shift+Left/Right for the vertical trace).


To move the trace, just hover the mouse over the top-right areas of the slices (the arrow cursor will change to a vertical panning cursor) and then click & drag your mouse in the desired direction. You will obtain the same result by holding the 'Ctrl' (Cmd in Mac) key while scrolling the mouse wheel over the trace.


Mnova automatically detects the 1D spectra and use them as external traces of a 2D plot if the applicable option is checked under the 'Edit/Preferences/NMR/Import' menu.(All the spectra must be opened in the same document).

If the 'Auto Attach Traces' option is not checked, you can drag and drop any currently opened 1D-NMR spectrum to a 2D NMR dataset in order to get them as traces. Here you can see how the page number 1, containing a 1H dataset is dropped to the HSQC to get the horizontal trace:



The same can be done with the page 2 (containing a 13C spectrum) to get the vertical trace:

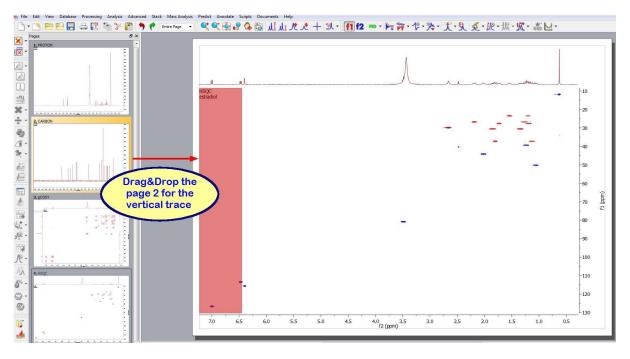

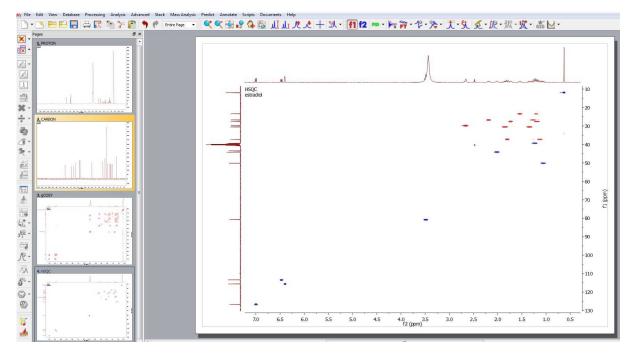


Here you can see the result:

There is also a script under the menu 'Scripts/NMR Tools/Auto Attach Traces' which will automatically setup the 1D spectra as external traces of a 2D.

You can also choose any currently opened 1D-NMR spectrum as a trace by clicking on 'Setup' on the '**Show Traces'** scroll bar menu (or by using the traces contextual menu by right clicking over one of the traces).

	Show Horizontal Trac	e:
	🚰 Setup	
and a literation	Mul Fit Horizontal Trace b	o Height
Show Traces     Show Vertical Trace	> Cut	Ctrl+X Ctrl+C
Show Horizontal Trace	Copy	Ctrl+C Ctrl+V
Fit Traces to Height     Fit Horizontal Trace to Height     Fit Horizontal Trace to Height     Fit Vertical Trace to Height	🗱 Delete 📄 Select All	Del Ctrl+A
+ Select Traces Graphically	Alignment	٠
+ Select Traces Graphically	Properties	

and next selecting the desired 1D-NMR spectrum for the horizontal and then for the vertical trace.

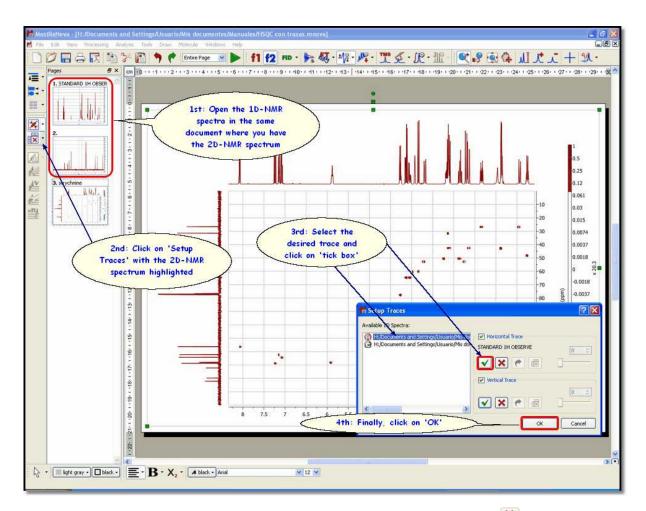


The user will be able to remove the external trace by clicking on the 'Delete' icon 🗱

You can show the **'Internal Projections'** in 2D spectra as either a calculation of the sum of all traces across a given dimension (Sum) or by computing the maximum of every trace (Maximum), just by clicking on the 'Projections icon' 💽. Click again on this icon 💷 to show the **'Internal Traces'**.

n Setup Traces	2 🛛
Available 1D Spectra: Hr/Documents and Settings/Usuario/Mis c H:/Documents and Settings/Usuario/Mis c	Horizontal Trace  Internal Projection (Sum)  421  421  421  421  421  421  421  42
s	Internal Trace #0 of 1024 (13.982 ppm)         0 \$           ✓         ★         ●           OK         Cancel


The user can also select the traces directly from the 2D-NMR spectrum by using the **'Select Traces Graphically'** tool in the 'Show Traces' scroll bar menu.

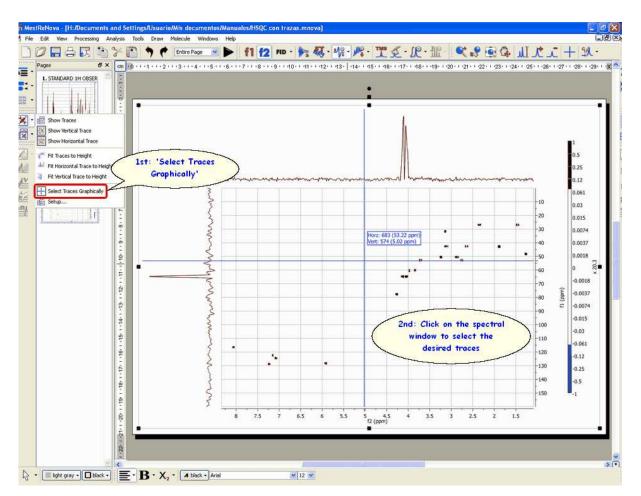

The user will be able to 'Fit Traces to Height' (the vertical, the horizontal or both), just by following the menu 'View/2D Traces' or by using the 'Show Traces' scroll bar menu on the left vertical toolbar:



The user can also extract a current trace (or projection) as a new spectrum by clicking on the button in the 'Setup traces' dialog box. In the figure below, you can see how to extract the vertical trace (# 517).

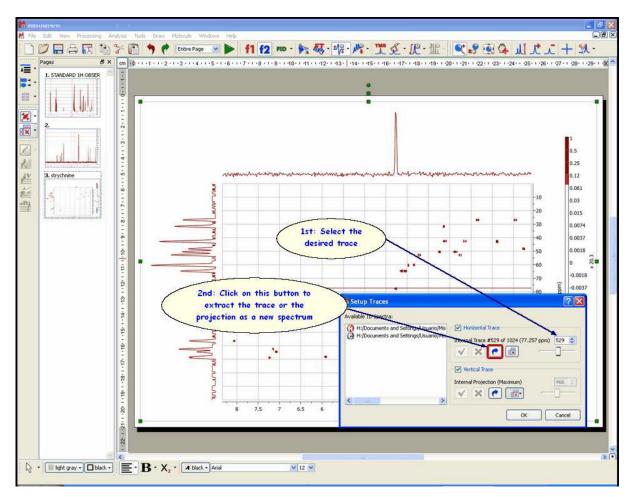


The user will be able to add or remove the 1D traces frame from the 'Grid Properties' dialog box (displayed by double clicking on the 2D-NMR spectral window):

- 📳		
metry NMR Spectrum General Grid 1D	Show Horizontal	Show Over
2D Traces	Color: Line Width:	light gray →

You can select the size of the traces (or to show them by default) by selecting the applicable option on the 'Properties' dialog box:

General Grid JD	Legend Width: Text Width:	4.23 mm	(4) (4) (4) (4) (4) (4) (4) (4) (4) (4)
2D Traces Stacked Scales Horizontal Vertical Peaks Meaks Meaks Assignments	Palette: Number of Positive Cont Number of Negative Con Scaling: Ploting method:		) 😿 10 🜩 10 🜩 2.000 🜩


You can move the traces across the 2D spectrum to freely to compare peaks, as floating traces:

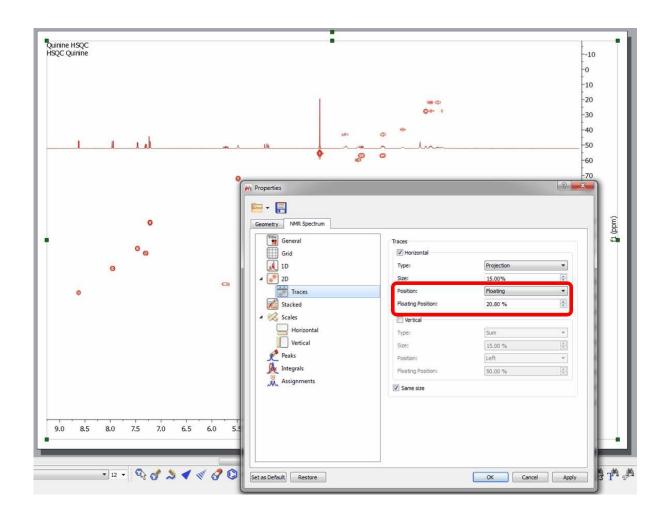

#### Automatic reference of 2D-NMR spectra with the 1D external trace.

You can reference the 2D-NMR spectra directly with the 1D external trace. Currently this feature only works which those bidimensional experiments which internal traces are equivalent with the external ones. For example: COSY, NOESY, etc...


Let's see how this feature work with a unreferenced COSY spectrum:

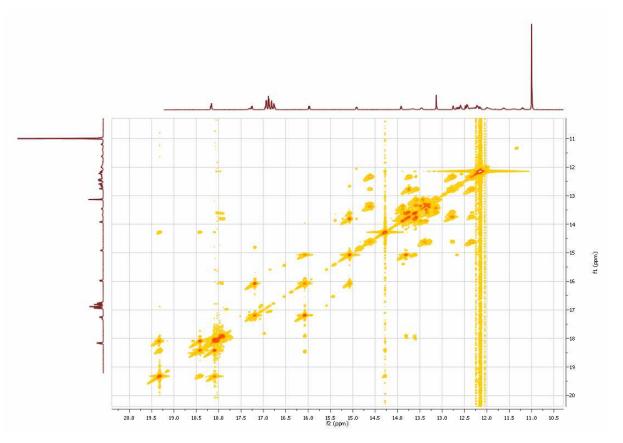

As you can see, this spectrum is not referenced. To apply an automatic referencing, just right click over one of the traces and select 'Setup' to display the 'Setup Traces' dialog box. Once there, select the desired external trace an click on the **AutomaticRreference** button (highlighted in red in the picture below):

👫 Setup Traces	? 🔀
Available 1D Spectra:	
💮 C:/Documents and Settings/carlos/Mis c	I Horizontal Trace
	Vertical Trace
	OK Cancel


Automatically, you will obtain your COSY spectrum referenced, as you can see in the screenshot below:

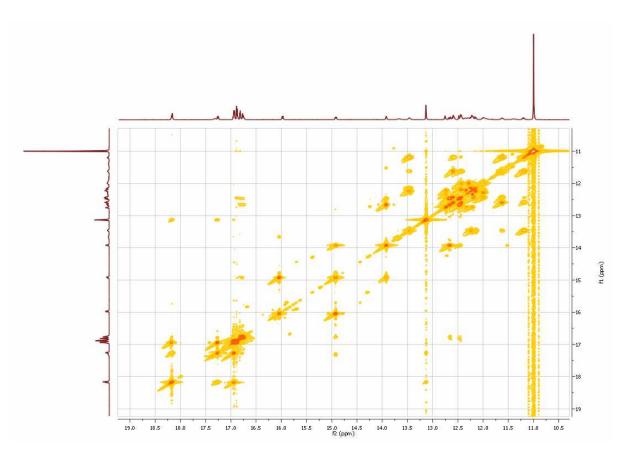


## 13.7 Manual Phase Correction in 2D-NMR

In this tutorial, we will explain how to phase the spectrum in real time, directly on the 2D spectrum.

We will show how to correct the phase of a gNHSQC experiment (see figure below).

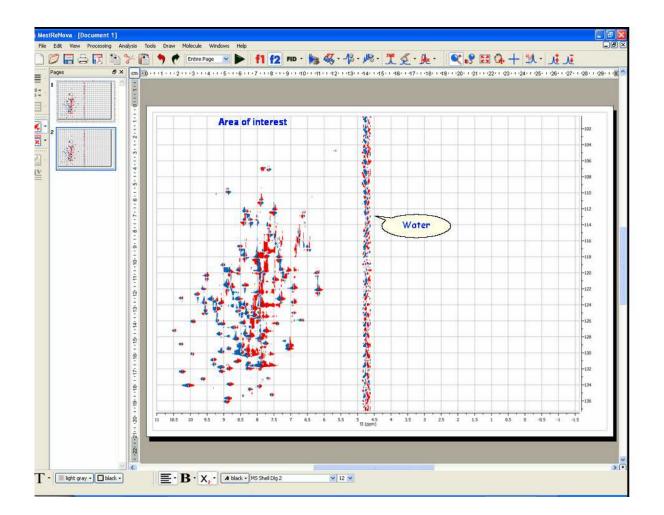

Once you have opened the spectrum; 'zoom in' the area of interest (in this case, we only need to worry about the left half of the spectrum):

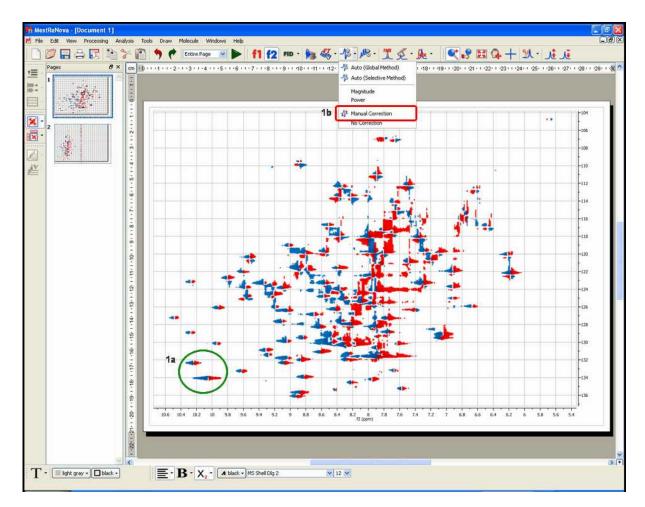


**1.** Then, take a look at the signal, or the group of signals (**1a**), which appear in a corner of the spectrum (for example, the signals highlighted with a green circle in the capture above); select 'manual correction' (**1b**) from the drop down menu on the 'Phase Correction' toolbar button and adjust the zero order (PH0) phase parameter along f2 (by dragging the mouse up or down over the blue rectangle in the 'Phase Correction dialog box' whilst holding the left mouse button (**1c**).

f2	f1			1c	
ip o eft igh	c here and or down he button for t button fo	olding: PHO cor r PH1 co	rection prrectic	or	
noia	Ctrl key f	or time u	uie)		
	-	or nne d	PH1:	20.27	\$
HO: Pivo	1	7.880		20.27 Bigges	•




Please note that the Phase Correction dialog is **modeless**, so you will be able to use any other tool (i.e. zooming) whilst you are applying the correction.

The goal (1d) will be to make all the **signals of the area of interest** (highlighted with the green circle in the picture above) positive (note that in this example, positive signals are red whereas negative are blue). Remember that we are adjusting the phase along f2, so do not worry if the phase of the peaks along the indirect (vertical) dimension (f1) is not correct.

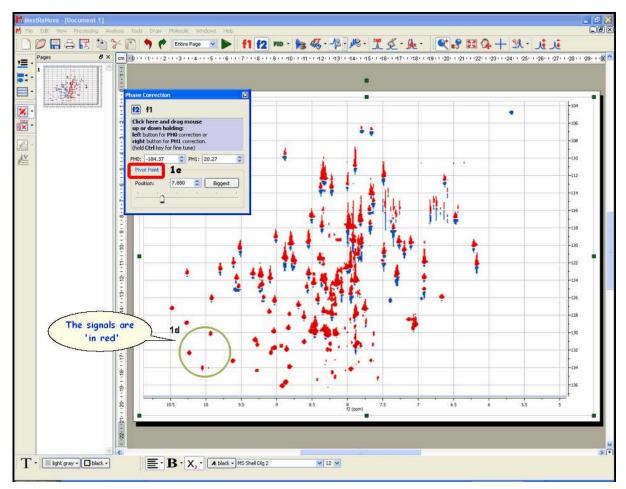

Next, if some peaks on the right side of the area of the spectrum shown on screen require phase correction (remember, still along f2), you can place the pivot point (**1e**) over the signal we have selected as reference (in the green circle) and carry out the first order phase correction PH1 (by dragging the mouse up or down over the blue rectangle in the 'Phase Correction dialog box' whilst holding the right mouse button). In this particular case, the spectrum does not require first order correction.

**2.** Finally, if necessary (as in this case), you can proceed in the same manner to correct the phase along **f1.** Just click on the f1 button on the dialog box and then proceed as explained along f2, by starting with a zero order phase correction and following with a first order phase correction (remember: along **f1**):

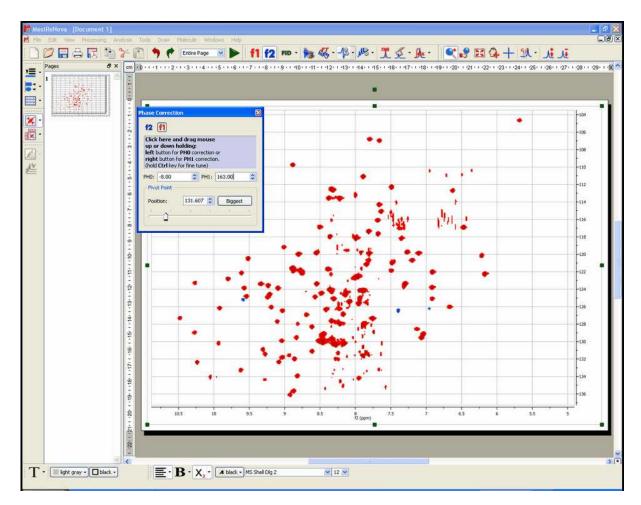

Bear in mind that this procedure is exactly the same as with 1D-NMR spectra, but it is necessary to correct the phase along 2 dimensions.

Note that, in our specific example, the resulting spectrum has 3 negative signals, but this is something that a phase correction is not able to correct.

### 13.8 Pasting Spectra into Reports

When the user copies a spectrum, he is copying a graphic. A graphic is any kind of image displayed by a computer. There are two kinds of graphics: vector graphics and raster graphics. A vector graphic (metafile) is a graphic drawn as lines, polygons and text while a raster graphic is drawn as an array of colored dots (bitmap).

A *metafile* is a list of commands that can be played back to draw a graphic. Typically, a metafile is made up of commands to draw objects such as lines, polygons and text and commands to control the style of these objects. So, internally, a metafile is an array of variable-length structures called metafile records. The first records in the metafile specify general information such as the resolution of the device on which the picture was created, the dimensions of the picture, and so on. The remaining records, which constitute the bulk of any metafile, correspond to the graphics device interface (GDI) functions required to draw the picture. These records are stored in the metafile after a special metafile device context is created. This metafile device context is then used for all drawing operations required to create the picture. When the system processes a GDI function associated with a metafile, it converts the function into the appropriate data and stores this data in a record appended to the

metafile.

NOTE: Some people equate metafiles with vector graphics. In most cases this is correct but, strictly speaking, a metafile can contain any mix of vector and raster graphics. For example, a metafile could contain just one command to display a bitmap. This is the approach used in Mnova, which by default pastes the spectrum as a metafile which contains a bitmap in order to reduce the file size (without too great a loss in resolution). Mnova also allows the user to use (only in Windows) the graphical format known as **Enhanced Windows Metafiles** in order to keep the maximum graphical resolution possible (at the expense of an increase in the file size). This will usually be the preferred way to copy NMR spectra.

Enhanced metafiles provide true device independence. You can think of the picture stored in an enhanced metafile as a "snapshot" of the video display taken at a particular moment. This "snapshot" maintains its dimensions no matter where it appears—on a printer, a plotter, the desktop, or in the client area of any application.

You can use enhanced metafiles to store a picture created by using the GDI functions (including new path and transformation functions). Because the enhanced metafile format is standardized, pictures which are stored in this format can be copied from one application to another; and, because the pictures are truly device independent, they are guaranteed to maintain their shape and proportions on any output device. In addition, the user is able to work with the copied spectrum in the document just by double clicking on it (Mnova will automatically open due to the Object Linking and Embedding technique; OLE).

A *bitmap* is another name for a raster graphic. In Windows, these are typically saved in a BMP file. However, other common bitmap formats include PC Paintbrush (PCX), Tagged-Image File Format (TIFF), Graphics Interchange Format (GIF) and JPEG.


In general, vector graphics take longer to display but can be scaled to any size with no degradation, whilst raster graphics are faster to display but image quality suffers when they are scaled up or down.

#### See also this post:


http://mestrelab.com/blog/making-publication-quality-images/

# How to paste a spectrum in a Report?

Mnova provides the ability to copy&paste spectra into other applications (e.g. MS Office apps) via the clipboard. Just be sure that you have highlighted the desired objects (Edit/Select All, if you want to select all the objects) and then follow the menu 'Edit/Copy' or alternatively use the shortcut 'Ctrl+C' (or 'Cmd+C' in Mac). You can also select the page on the page navigator and do Ctrl/Cmd+C (or right click->Copy) to copy to the clipboard all the content of the page.

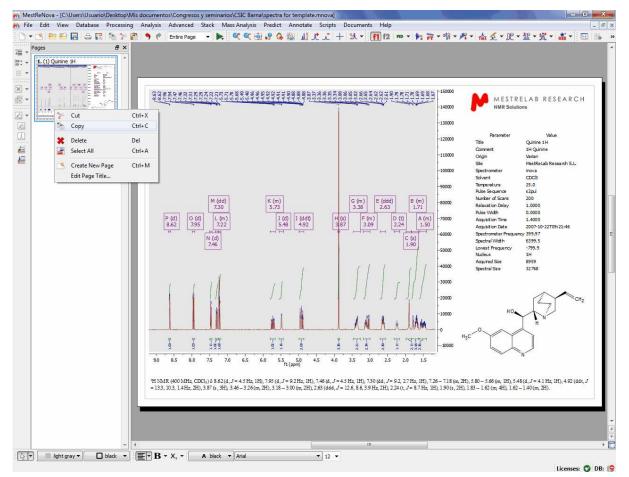

Next, open the document (PowerPoint in this case) where you want to paste the spectrum and follow the menu Edit/Paste or alternatively use the shortcut, Ctrl+V (or Cmd+V in Mac).

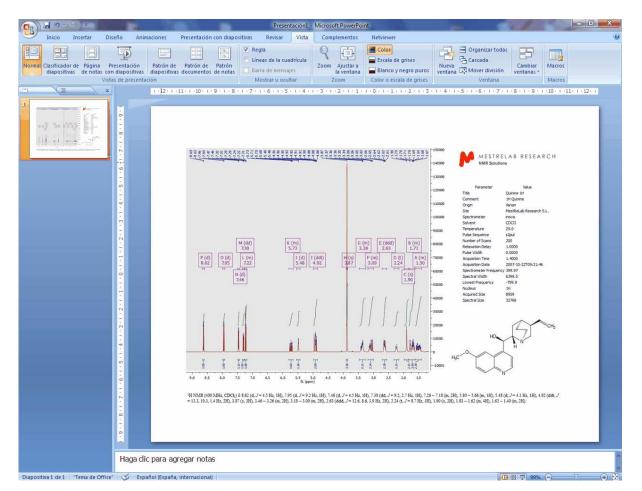

Mnova will copy to the clipboard, by default, the object as a metafile. This object will have OLE properties in Windows, so the user will be able to work with the copied spectrum in the document just by double clicking on it (Mnova will automatically open due to the Object Linking and Embedding technique; OLE). Please bear in mind that the size of this 'image' will be bigger than a regular image, because you are storing the FID to allow Mnova to reprocess the NMR spectrum in the future if it is needed.

However, the user can change this default by following the menu 'Paste/Paste Special' (or Ctrl/Cmd+Alt+V) before pasting (in the corresponding document; PowerPoint in this case). It will open the 'Paste Special' dialog box where the user will be able to select between Mnova Document (by default), Enhanced Windows Metafile, Bitmap, etc.

Paste Speci	al	2 🔀
Source: Unkn	The user is able to select	ОК
• Paste	the type of graphic that is going to be pasted	Cancel
C Paste (nix	Picture (Program Picture Picture (Enhanced Metafile)	E Display as icon
Result	Pastes the contents of the Clipboard into your presentation as an enhanced metafile picture.	

The user can also copy the spectra just as an image (very useful for large datasets) by following the

menu 'Edit/Copy Special/Copy as an image'. This will reduce the file size of the document but the image will not contain OLE properties.

Edit	View Database	Processing	Analysis	Advanced Stack
4	Undo	Ctrl+Z	19 1	Entire Page 🔹
۴	Redo	Ctrl+Y	8 >	¢
de la	Cut	Ctrl+X		
	Сору	Ctrl+C		
	Copy Special		ዿ Сору	/ as Image
	Paste	Ctrl+V		19

From the '**Drawing Tools Preferences**', you will be able to select the exporting 'Resolution' and 'Quality' of the graphics and also the resolution of the image copying:

		1	2	-	4	ELS.
General	Plug-ins	DB	NMR	Mass	Molecule	Drawing Tools
	r log ma	00		111133	molecule	Drawing 1001.
Image Expo	rting					
Resolution:	Display Resoluti	ion				
	50 %	A.				

The user can also save the spectrum by following the menu 'File/Save as' and then 'paste it' in the corresponding document by selecting 'Insert/Picture'. Mnova allows the user to save the data in Mnova (\*.Mnova) or MestRe-C (\*.mrc) formats as well as in ASCII text (\*.txt), adobe PDF or several kinds of image files, such as bitmap (bmp), enhanced metafile (emf), JPEG, PNG, SVG, TIFF, XBM, XPM, etc...

ave As					?
Guardar en:	80		] ← 🗈	r 📰 -	
Documentos recientes	🛅 pdata				
Escritorio					
Mi PC	10				
Mis sitios de red	Nombre:	Select the name		•	Guardar
	Tipo:	MestReNova Document (*.mnova)		<b>_</b>	Cancelar
		MestReNova Document (*.mnova) ASCII Text File (*.tx) Adobe PDF Files (*.bmp) BMP Image Files (*.bmp) Enhanced MetaFile (*.emf) JPEG Image Files (*.jpg) MestReC (*.mc)			

'ASCII Text File' (\*.txt): It is essentially raw text just like the words you are reading now. Each byte in the file contains one character which conforms to the standard ASCII code. This kind of text file becomes a common denominator between applications which do not import each other's formats. If both applications can import and export ASCII files, you can transfer your files between them. Almost all word processors import and export ASCII files as well as many database and spreadsheet programs.

'Adobe Text File' (\*.pdf): Portable Document Format (PDF), is an open file format used for representing two-dimensional documents in a device independent and resolution independent fixed-layout document format. Each PDF file encapsulates a complete description of a 2D document which includes the text, fonts, images, and 2D vector graphics which compose the document.

'JPEG Image File' (\*.jpg): JPEG stands for Joint Photographic Experts Group; it is a lossy compression algorithm which has been conceived to reduce the file size of natural, photograph-like true-colour images as much as possible without affecting the quality of the image as perceived by the human sensory engine.

'PNG Image File' (\*.png): PNG (Portable Network Graphics) is another bitmapped image format which employs lossless data compression.

XPM Image Files (\*.xpm): XPM stores image data in the form of ASCII text formatted as a Standard C character string array. This type of format allows XPM files to be edited easily with any text editor, to have comments inserted at any point within the file, to be included as data in C and C++ programs, and to be easily transmitted via electronic mail.

### **13.9** How to predict a spectrum with NMRPredict Desktop?

Carrying out of predictions in Mnova with the NMRPredict Desktop plugin is very easy.

1. Just, import a molecular structure. Currently, molecular structures can be imported as a **.mol** file by simply using the Open command exactly in the same way as this would be applied to a spectrum. Bear in mind, that you are actually able to copy&paste **.cdx** structures from **ChemDraw** and **.mol** from **IsisDraw** but not drag&drop them. Support to 'drag & drop' operations are currently limited to


#### ChemSketch.




#### ATTENTION

Bear in mind that, in terms of stereochemistry, drawing a structure as a chair or as a boat means nothing to the .mol file and the computer. In those cases the user must draw all the corresponding bonds to show the stereochemistry of the molecule, i.e., you must explicitly draw up and down bonds using wedges.

2. Right click on the molecule structure and select 'Predict 1H Spectrum' or 'Predict 13C Spectrum'.

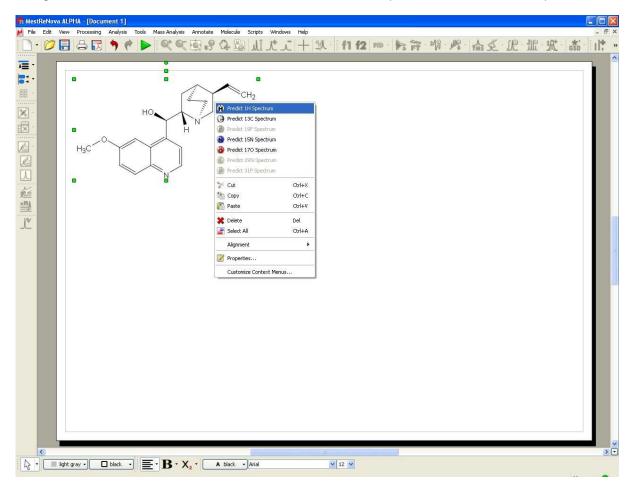


3. After that, you will obtain the desired predicted spectrum which can be analyzed as a real one (e.g. it can be integrated, peak picking, etc).

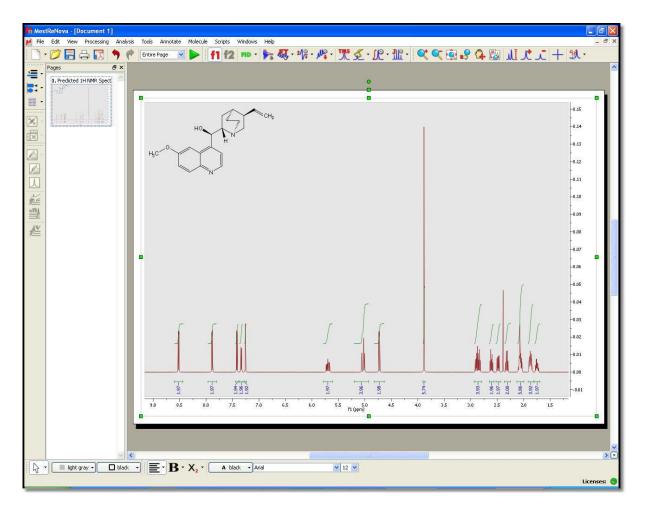


You can also modify the chemical shift and the coupling constant values from the table of the predicted spectrum. Just, highlighted the spectrum, follow the menu 'View/Table/1HPrediction' and then double click on the value that you want to edit. The changes made on the table will take effect automatically in the simulated spectrum.

Please bear in mind that the peak labels and the multiplet boxes will show the corresponding atom numbers of the molecule.

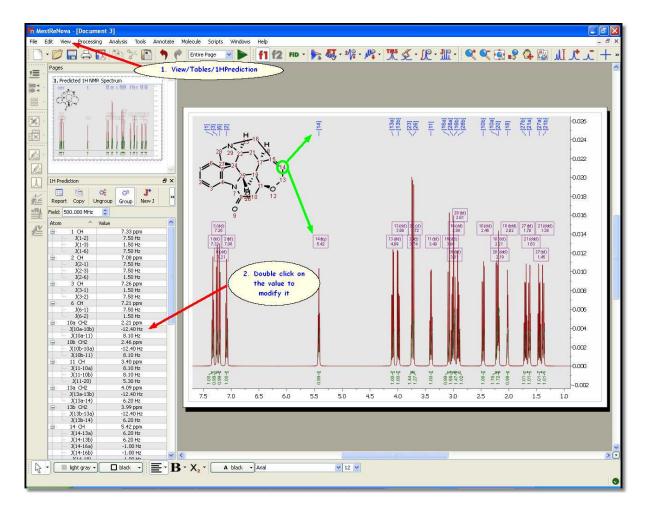


Finally, if you want to know the "predicted assignment", just hover the mouse over the desired atom, (so that it becomes highlighted in a red box) and the corresponding signal in the spectrum will automatically highlight in blue (increasing slightly its intensity); or vice versa (hovering the mouse over the peak will highlight the corresponding atom on the molecular structure).

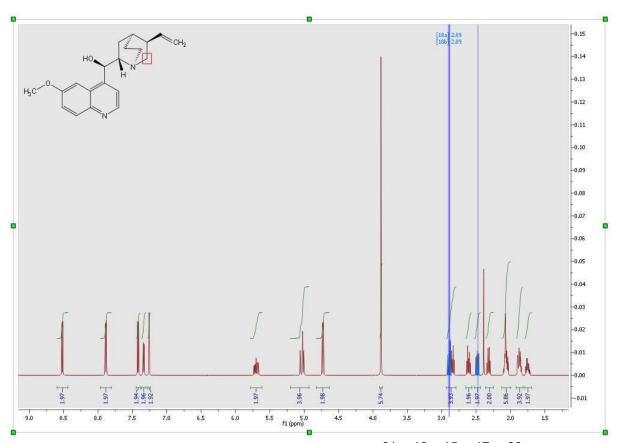

A similar procedure will be followed to run X-Nuclei predictions:  ${}^{31}P$ ,  ${}^{19}F$ ,  ${}^{15}N$ ,  ${}^{17}O$ ,  ${}^{29}Si$ . In this case, just follow the menu 'Predict' and select the desired option:

Pre	dict Scripts Documents Help		
A Q	1H Spectrum 13C Spectrum HSQC Spectrum	M	小九九山
	X-Nuclei Prediction	B	11B Spectrum
22	Prediction Options		15N Spectrum
	Update 1H Prediction DB Update 13C Prediction DB X-Nuclei Prediction DB	0 12 5	170 Spectrum 19F Spectrum 29Si Spectrum
-	Rrowse Prediction DR	P	31P Spectrum

Of course you will be able to change the appearance of your simulated spectra as you prefer. Here is a sample:

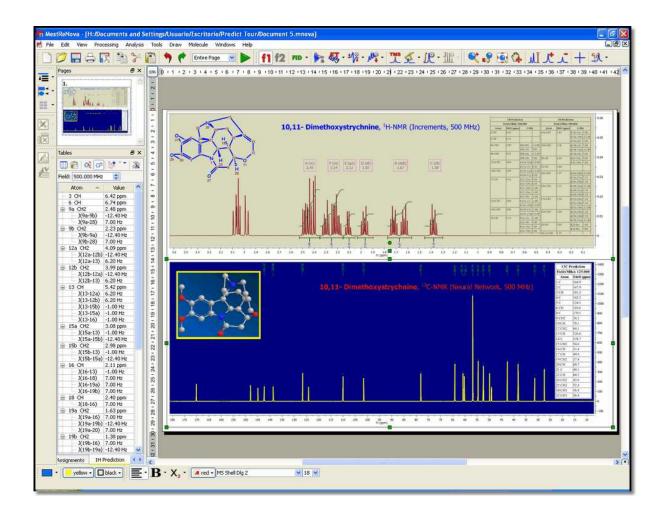




# 14 Mass Plugin


Mnova incorporates a new plugin to process LC/GC chromatograms and mass spectra. The concept behind the multiplatform, multipage Graphical User Interface of Mnova is to allow the average chemist easy access to high quality processing and analysis of analytical data on the desktop computer and OS of choice. The new Mnova MS plugin gives the chemist the ability to work with LC/GC/MS data in combination with NMR data, within a single document.

The **Mnova GUI gives you much more**. Benefit from day one of many other Mnova capabilities, such as scripting, reporting templates, graphical annotations, multiple exporting formats, including PDF, OLE integration with MS Office and many, many more.

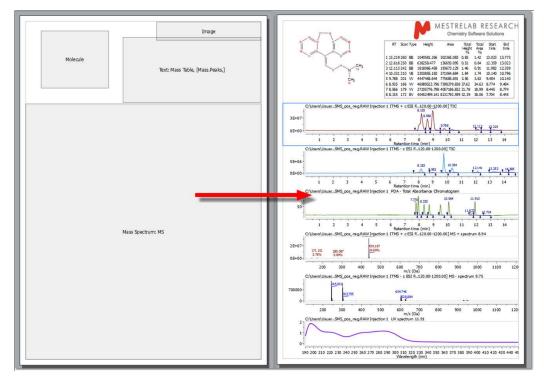


In the picture below you can see an example of a layout template used for the MS plugin:


Mnova is an extremely versatile reporting tool, which will allow users to report even NMR and LC/GC/MS data together in the same document (or page):

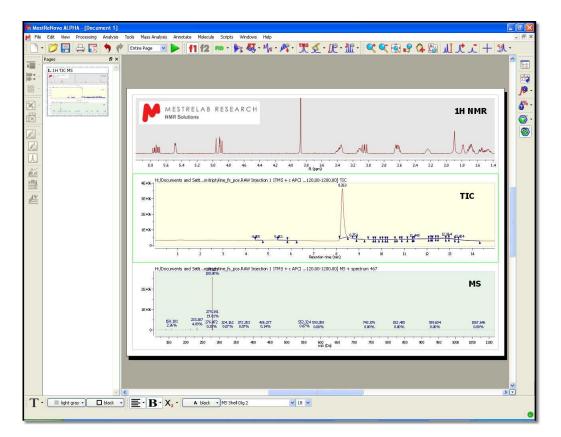

Here you can see another example with a MS and a 1H-NMR spectrum, containing a molecule structure and multiplet report:

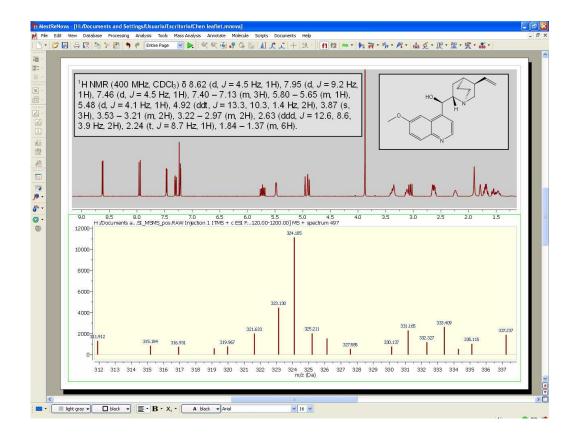


Following the Mnova concept, seamlessly interact with and handle data from different vendors. HP Agilent (ChemStation, Ion trap, MassHunter), Thermo Scientific–Xcalibur, Waters MassLynx, Bruker (Compass, XMass), JEOL MSQ1000, SCIEX Analyst, Shimadzu, NetCDF ANDI-MS, Varian Saturn, mzData and mzXML. It provides a graphical user interface (GUI) for interaction with and display of dataset contents and tools and algorithms for basic processing of chromatograms and mass spectra.

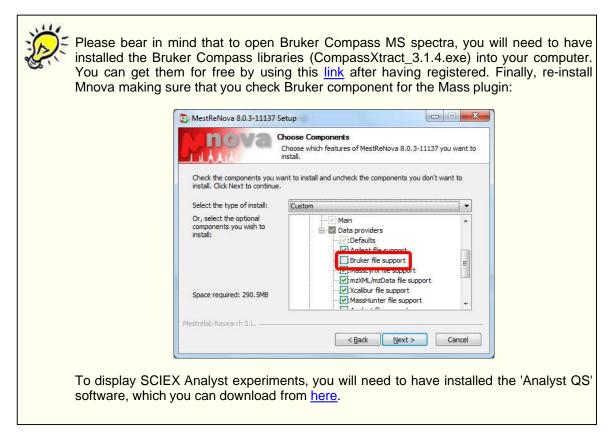

Please bear in mind that Mnova MS under Mac and Linux only supports:

- Agilent ChemStation
- Bruker XMass
- FSU Midas
- mzData and mzXML
- Waters MassLynx (Mac only)

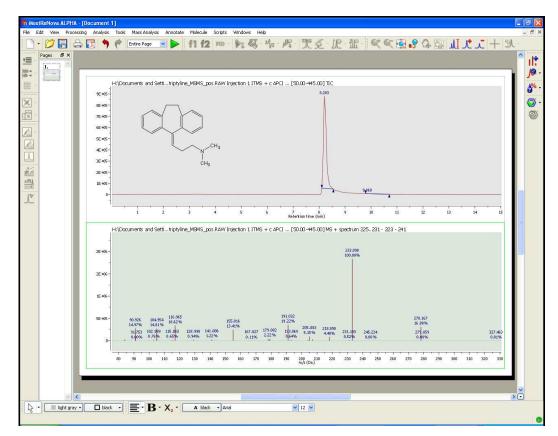

The target user for the first version of the MS plug-in is one whose goals are the elucidation and confirmation of small molecule structures.

The Mnova framework will allow the user to combine the results of multiple analyses into a consolidated report of results.

You will find below a glossary of the main terms relating to the MS plugin:

- Adduct: Ion formed by the interaction of an ion with one or more atoms or molecules to form an ion containing all the constituent atoms of the precursor ion as well as the additional atoms from the associated atoms or molecules.
- Accurate Mass: Experimentally determined mass of an ion that is used to determine an elemental formula. Typically, a mass accuracy of 5 ppm or better, at relatively low m/z values, is necessary to compute a correct elemental formula. See the section on elemental composition later in this document.
- **Base Peak**: The most intense peak of the mass spectrum which is assigned a relative abundance value of 100 percent. The lesser peaks are reported as a fraction of the base peak abundance.
- Chemical ionization (CI): Formation of an ion in the gas phase by the reaction of a neutral species with an ion. The process may involve transfer of an electron, a proton or other charged species between the reactants. Note: When a positive ion results from chemical ionization the term may be used without qualification. When a negative ion results the term negative ion chemical ionization should be used.
- Electron lonization (EI): Ionization of an atom or molecule by electrons that are typically accelerated to energies between 10 and 150 eV in order to remove one or more electrons from the molecule. The term electron impact is deprecated.
- Electrospray Ionization (ESI): A process in which ionized species in the gas phase are produced


from a solution via highly charged fine droplets, by means of spraying the solution from a narrow-bore needle tip at atmospheric pressure in the presence of a high electric field (1,000 to 10,000 V potential).

- Fast Atom Bombardment (FAB): A method in which ions are produced in a mass spectrometer from non-volatile or thermally fragile organic molecules by bombarding the compound in the condensed phase with energy-rich neutral particles.
- Isotope Cluster: Set of mass peaks related to ions with the same chemical formula but containing different isotopes; e.g. the 16 and 17 Da peaks in a CH4 sample arising from 12CH4+ and 13CH4+ ions.
- Mass Spectrometry/Mass Spectrometry (MS/MS): The acquisition and study of the spectra of the electrically charged products or precursors of m/z selected ion or ions, or of precursor ions of a selected neutral mass loss. MS/MS can be accomplished using beam instruments incorporating more than one analyzer (tandem mass spectrometry in space) or in trap instruments (tandem mass spectrometry in time).
- Mass Spectrum: A plot of the relative abundances of ions as a function of their m/z (mass to charge ratio) values, representing data produced by a mass spectrometer.
- Mass Resolution: In a mass spectrum, the smallest mass difference (m) between two equal magnitude mass peaks such that the valley between them is a specified fraction of the peak height. Typically, a 10% valley is specified, or 50%, which is known as full width at half-maximum height (FWHM).
- Mass Resolving Power: In a mass spectrum, the observed mass divided by the difference between two masses that can be separated: m/ m.
- Mass Chromatogram: A chromatogram obtained from the plot of the intensity of a single m/z value or of a range of m/z values for each mass spectra in a dataset versus time.
- Molecular Isotope Cluster Chromatogram (MICC): The MICC is the sum of the mass chromatograms of each m/z value of an isotope cluster.
- Total Ion Chromatogram (TIC): The chromatogram obtained from the plot of the sum of intensities for each mass spectrum in a dataset versus time.


### 14.1 First Steps with the Mass Plugin

It is very easy to obtain your first results with the Mass plugin of Mnova:


1. Drag&drop the raw folder to Mnova in order to display the TIC (at the top of the window) and the MS spectrum of the highest signal (this default can be changed in the '<u>Preferences'</u>)

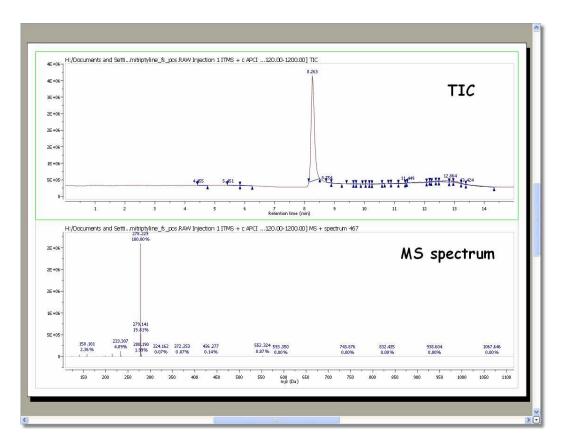


2. You can expand any scale (in either the TIC or MS) by using the 'zoom in' feature, which can be accessed by just pressing the 'Z' key or by using the corresponding icon of the toolbar  $\$ .

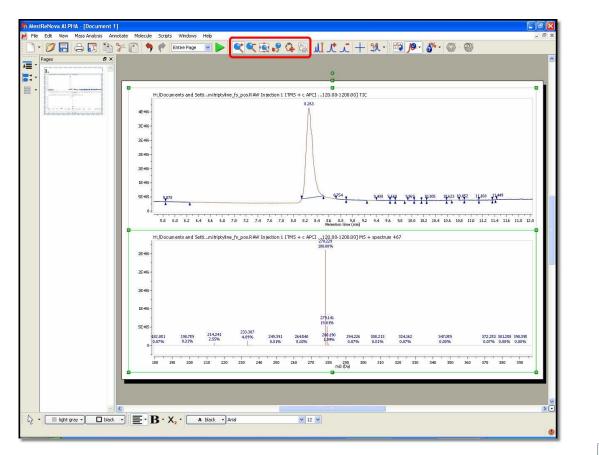


3. You can select any other mass spectrum for a particular time point with the crosshair feature is just by clicking on the corresponding signal of the TIC. For example in this case, we have selected the spectrum number 467 at a 'Retention time' of 8.26 min:

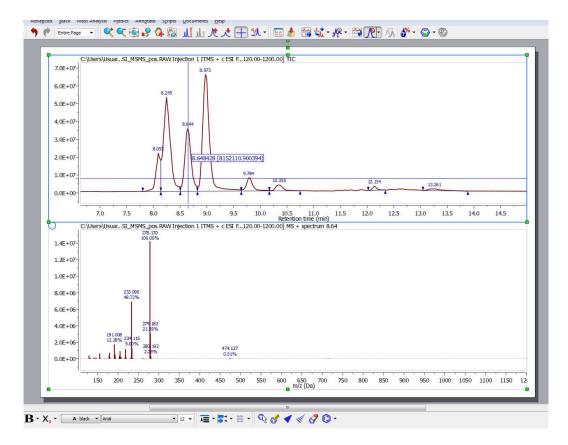


4. If you need to average the mass spectra over a certain time range (CoAdd), just select the crosshair, hold down the left mouse button and drag over the appropriate time span in the TIC. A label at the top of the MS will inform you about the spectrum ranges (red rectangle in the picture below):

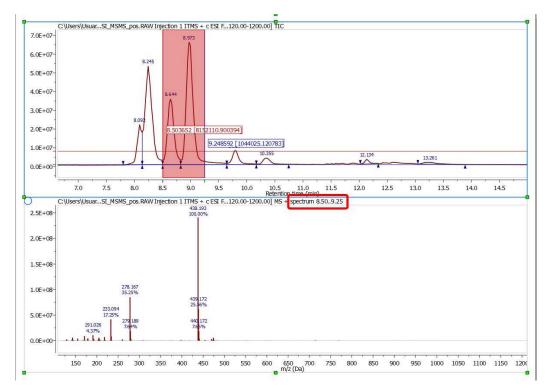

If you want to 'CoAdd' the whole peak, just follow the menu 'Mass Analysis/Spectrum Selection Mode/Peak' and finally select the desired peak in the TIC.

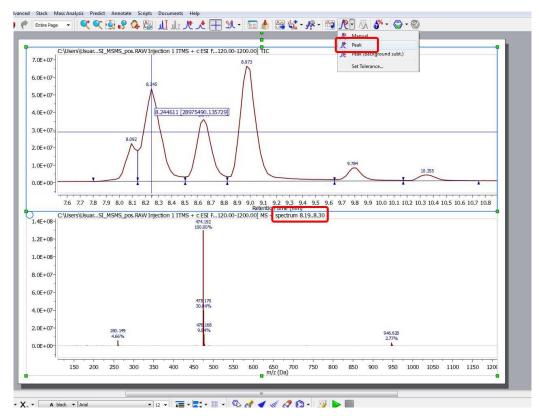


To generate a 'CoAdd' of the whole peak without the tail-peaks just select the mode 'Peak

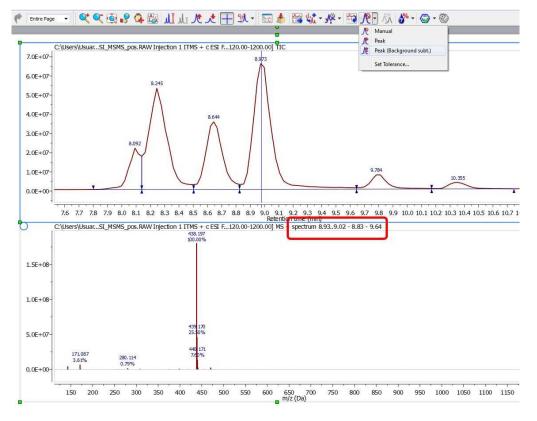

(Background Subt.)' under the 'Mass Analysis/Spectrum Selection Mode' menu.

5. It is possible to add another MS spectrum to the page, just by clicking on the 'Append' button . Next, select the desired time span in the TIC in order to obtain the corresponding MS spectrum. In this case we have added the MS spectrum 738 which appears at 12.90 min.

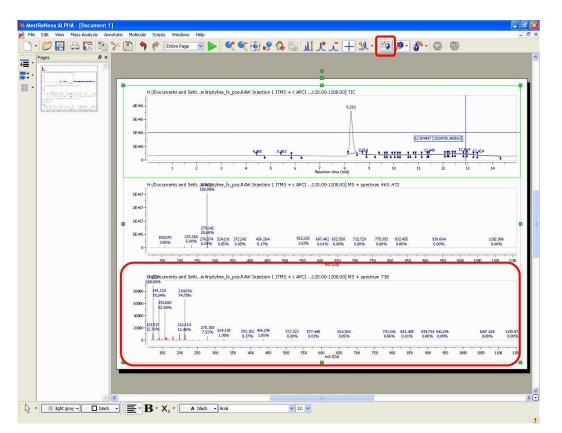


6. The 'Molecule Match' is very useful to see if a mass spectrum and a chromatogram match with one of the molecular structures of the document. With the TIC and the mass spectrum displayed on the screen and some .mol or .sdf files opened in the .mnova document, click on the 'Calculate Molecule Match' button of the toolbar . The 'Molecule Match' table will be displayed to see the results. This table will contain information about the 'Retention Time', Scan (number of spectrum), Match Score...

Rep	and the second second	© Calc	<ul> <li>View</li> </ul>	Sett	Setup						
1	Molecule	0	Formul	a	Molecular Weight	atc 📥	Match Score	Similarity	MS Purity	RT	Scar
1 12		C2	OH23N		277	~	0.999	0.999	0.868	8.26	467
2 0	>	CI	9H21N		263	V	0.544	0.544	0.000	8.26	467
3	÷	⊂1	8H19NO		265	×	0.000	0,000	0.000		
4	8	C2	0H24N2	02	324	×	0.000	0.000	0.000		
5 3	5	C2	1H22N2	02	334	36	0.000	0.000	0.000		

Clicking on any molecule will display the MICC (Molecular Isotope Cluster Chromatogram), overlaid with the TIC.

In this case, the best result is for the compound number 1 (C20H23N). You can see in the picture below the MICC (in green) over the TIC (in red):

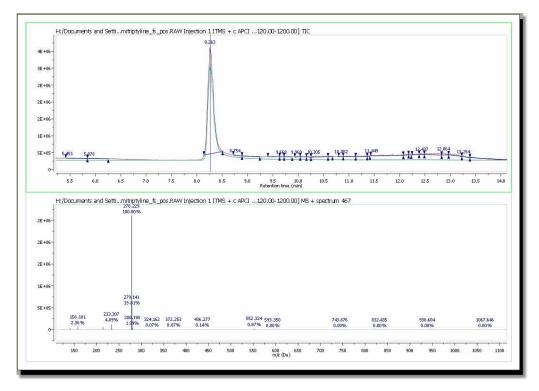

In addition, Mnova shows you in the chromatogram the retention time of the match (with a blue vertical line) and displays the corresponding MS spectrum (the number 467 in this case) overlaid with the theoretical one (in green at a M/Z around 278, in this case).

7. If you are using high resolution MS, it is possible to do an 'Elemental Composition' analysis of any peak of the Mass spectrum. First of all, follow the menu 'Mass Analysis/Elemental Composition/Constraints' or select the corresponding option in the scroll down menu of the 'Elemental Composition' icon of the toolbar:



This will open the 'Elemental Composition Constraints' dialog box:

er	nent Const	raints:		Double Bond Equiva	alence:		
			-	Minimum:	-0.50	\$	ОК
			+ *	Maximum:	20.00	٢	Save
	Element	Minimum	Maximum	Tolerance:			Restore
1	с	0	100		0.41703		Cancel
2	н	0	200	Units:	ppm	~	-
3	N	0	10	Value:	5.00	~	
4	0	0	10	Maximum Resul	Countr		
5	s	0	5		-		
				Maximum:	1	1	
				Other Constraints:			
				Electron Mode:	All	~	
				Charge State:	1	-	
				Adduct:	н		
				Fitness Threshold:	0.00	2	

Click on this icon 💽 to add more 'Element Constraints'. Once you have finished with the constraints,

click on the 'Elemental Composition' icon and select with the crosshair the desired peak of the Mass spectrum. A table with the results will be displayed (it is also possible to find this table under the 'View/Tables' menu). All the results obtained will satisfy the composition, DBE, and tolerance constraints, and will be ranked in decreasing order of fitness. Please bear in mind that a fitness value of 1 will be the perfect match.

8. Follow the menu 'View/Tables/Parameters' to display and report the 'Parameters table' :

Re	eport Copy Setup	Garage Customize	
	Parameter	Value	
1	Data Path	C:\DATA\2005\02-February\Ref- Mix-050220_ESI_MSMS02.RAW	
2	Acquired Date	2005-02-21T15:55:37	
3	Sample Name	Ref Mix (with dyn exd)	H
4	Comment	Xterra_MS_C18 2.5u 1x50mm	
5	Operator	Administrator	
6	Submitter	ROLLFR9	
7	Sample Position	99	
	l m		

Finally, the user will be able to save  $\blacksquare$ , print  $\boxdot$  or export to PDF  $\blacksquare$ , the document by clicking on the corresponding icon in the toolbar.

## 14.2 Working with the MS plugin

Mnova MS allows the user to navigate the TIC and display simultaneously any number of MS traces of interest, corresponding to specific points or to ranges in the TIC. All Mnova graphical functionalities (zooming, panning, create expansions, fit to height, increase/decrease intensities, etc) are available on all active spectra on screen. Spectra can be visualized in different modes: Standard, Peak spectrum,

Background Subtracted Spectrum. Molecular structures (MOL files, SD files and copy/paste from ChemDraw, IsisDraw and ChemSketch) are also supported.

The Mass plugin of Mnova supports the following formats:

- HP Agilent (ChemStation, Ion trap, MassHunter)
- Thermo Scientific Xcalibur
- Waters MassLynx
- Bruker (Compass, XMass)\*
- JEOL MSQ1000
- SCIEX Analyst<sup>\*\*</sup>
- Shimadzu<sup>\*\*\*</sup>
- Data Explorer\*\*\*\*
- Varian Saturn
- mzXML/mzData (\*.mzXML, \*.mzData, \*.xml)


\* Please bear in mind that to open Bruker Compass MS spectra, you will need to have installed the Bruker Compass libraries (CompassXtract\_3.0.1\_01.exe) into your computer. You can get them for free by using this link after having registered

\*\* To display SCIEX Analyst experiments, you will need to have installed the 'Analyst QS' software, which you can download from here.

\*\*\*Mnova MS supports Shimadzu files, but it is necessary to have the Shimadzu software installed on the same computer for this to work.

\*\*\*\*It is necessary to have the Data Explorer software installed on the same computer for this to work.

In order to load any sample in Mnova just Drag&drop the corresponding file to Mnova to display the TIC (at the top of the window) and the MS spectrum of the highest signal (this default can be changed in the '<u>Preferences</u>'). You can also use the '*File/Open*' menu, the keyboard shortcut <**Ctrl+O**> (Cmd+O in Mac) or click on the '**Open'** icon on the toolbar.

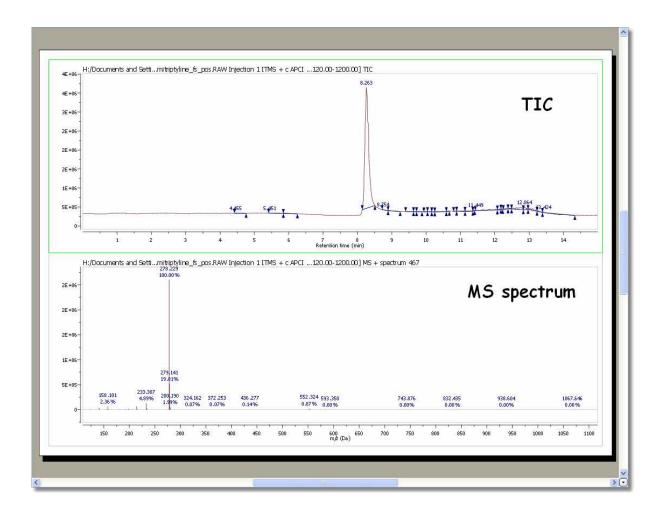

Double clicking on the spectral window will display the properties dialog box. From here you can modify the Grid, Axes, Line, Peaks and Title properties of the TIC and MS spectrum by selecting the corresponding tab in the dialog box. For further information about the Properties, please click <u>here</u>.

You can expand any scale (in either the TIC or MS) by using the 'zoom in' feature, which can be accessed by just pressing the 'Z' key or by using the corresponding icon of the toolbar . Please note that the intensity of the expanded region will be automatically fitted. However if you are not happy with

it, you can change it by just clicking on the 'Increase or Decrease Intensity' icons: Metal. Or by using the '+' or '-' keys.


You can select multiple chromatograms of the same dataset to zoom in/out simultaneously. The chromatograms can be selected as in a stack of NMR spectra:

- To select a single spectrum, left click on the spectrum while keeping pressed the Alt key

- To deselect a spectrum: left click + Ctrl/Cmd + Alt

- In order to select multiple spectra, follow the same operation as above while keeping pressed Alt and/or Shift keys.

You can select any other mass spectrum for a particular time point with the crosshair feature is just by clicking on the corresponding signal of the TIC. For example in this case, we have selected the spectrum number 467 at a 'Retention time' of 8.26 min:

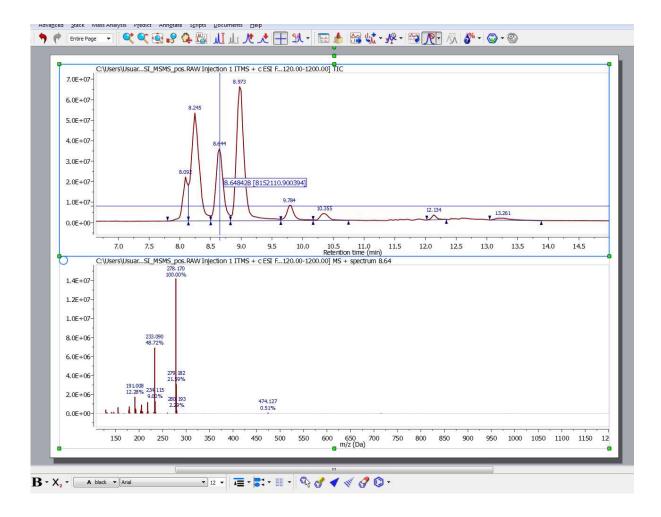


## 14.2.1 MS Browser

This panel can be showed by clicking on the corresponding icon (or by following the menu 'View/ Panels/MS Browser' or 'Mass Analysis/Show MS Browser'). It is very useful and we recommend to dock it to the page navigator. From this panel you can easily open additional chromatograms or spectra at the same item:

RATAROCL	LOR_S9_GSH_NADPH.RAW	
vser		
t) 🕕 🚺		
ataset		
Injection Func		
4 1	FTMS + p ESI Full ms [200.0	0-800.00]
	FTMS + p ESI d Full ms2 [115.00	-475.00]
▲ Trace	es PDA - Total Absorbance	
1	PDA - Maximum Absorbance	
4 L	☑ Chromatogram UV A (254, 9)	
L.	Chromatogram UV B (290, 9)	
	UV C (0, 0)	
<i>a</i> [	DAD V PDA - Chromatogram 25	4 nm


This dialog box will contain information about the 'Data Source'. If the current spectrum contains the original spectrum file, the 'Data Source' will show a green tick mark. If not, it will show a red cross (and the spectrum will have a red frame); which indicates that you will not be able to load any other part of the chromatogram and you will only be allowed to work with the spectrum that you have on the screen.

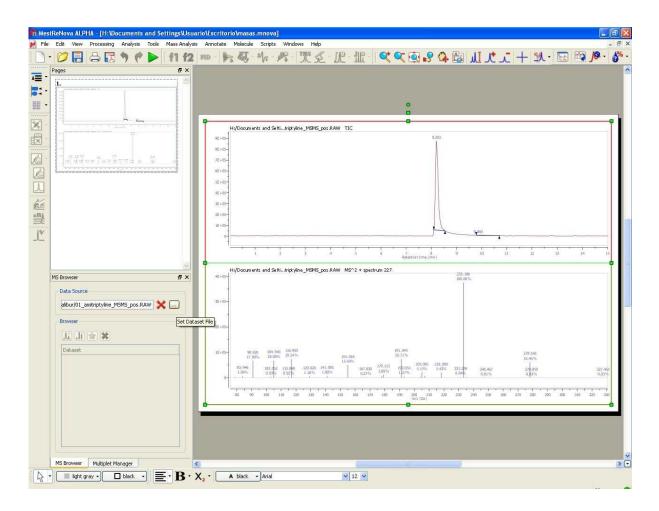

## Attention: Please bear in mind that when you save a Mnova document with a TIC and a Mass spectrum, by default the raw file is not stored in the document (to avoid the generation of huge files), so you will need to keep the original raw file on your computer if you plan to continue working with the experiment in the future. If you want to store the raw file on the Mnova document, click on the 'Fetch Full Dataset' button of the MS Browser. Please make sure that if you change the path of the raw file (after having saved a Mnova document); you will need to load it by clicking on the 'Set Dataset File' button (of the MS Browser table) if you want to work with the experiment. Be careful in this situation, because Mnova will not be able to identify if you load an erroneous raw file (instead of the correct one).

You can hide any chromatogram or MS spectrum by checking the corresponding check box in the 'MS Browser' or by selecting 'Hide Plot' in the context menu of the spectrum (which can be accessed by right clicking on the spectral window).

If you want to delete the plot from the Browser, just select it and click on the red cross button **B**. The same result will be obtained by selecting 'Delete Plot' in the context menu. You can also hide and extract to any page the selected plot.

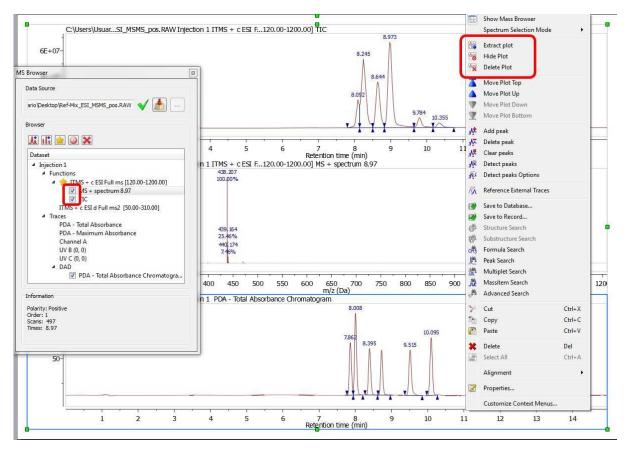

Double clicking on any function from the MS brower, will display the applicable dialog box, which will allow you to open the TIC, Base Peak or the Mass spectrum. The same result will be obtained by highlighting the applicable function and clicking on the 'New Chromatogram' icon  $\overline{M}$ :

🖁 New chromatogram	? 🛛
Chromatogram Type Total Ion Current Base Peak Mass	OK Cancel

- **TIC** (Total Ion Current): The sum of all the separate ion currents carried by the different ions contributing to a complete mass spectrum or in a specified m/z range of a mass spectrum (this is sometimes called the reconstructed ion current).
- **Base Peak**: The peak in a mass spectrum corresponding to the separated ion beam which has the greatest intensity which is assigned a relative intensity value of 100. The lesser peaks are reported as a percentage of it.

• Mass: clicking on this option will display the below dialog box which will allow you to select the range of the chromatogram between two values of m/z. You will obtain the TIC corresponding to the selected m/z range.

New chror	natogram	? 🛛
Chromatogra	m Type	ОК
O Total Ion		Cancel
<ul> <li>Base Pea</li> <li>Mass</li> </ul>	k	
Range		
From m/z:	120.23 📚	
To m/z:	120.23	


You will obtain the same result by selecting 'Manually' on the scroll down menu of the 'Open Mass chromatogram' button of the toolbar:

📻 📸	- 🔍 🚌 - 松 🗗	<u>8</u> * - ⊘ - ⊚
	Graphically	1
pos.RAW Inje	Manually	200.00] TIC

You can display any trace (i.e PDA or UV chromatograms) by double clicking on it or by selecting it on the MS Browser and then clicking on the 'Open new Chromatogram' icon **W**.

Browser	
Data Source	
prio/Thermo Scientific	: - Xcalibur/01_amitriptyline_MSMS_pos.RAW 🛛 🗸 📖
Browser	
Datet	
	c APCI corona d w Full ms2 [50.00-445.00] TIC M5^2 + spectrum 227
⊡- Tracec PDA Tra	15 + c APCI corona sid=15.00 Full ms [120.00-1200.00]
PDA Ira Channe	(ez


If your dataset contains UV traces (DAD) and it is in Masshunter, Bruker Compass, Shimadzu v5, Xcalibur or MassLynx format; you can extract them or select a range in the wavelength; by selecting the applicable option after having clicked on the 'Open new Chromatogram' icon

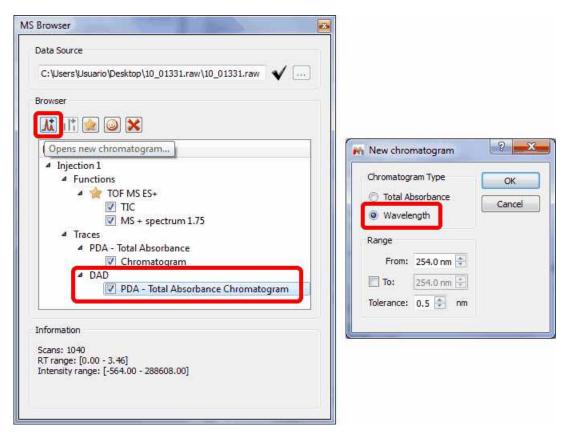

From the PDA-Total Absorbance Chromatogram, you will be able to extract the complete **UV spectrum.** 

To select a UV spectra: the dataset must have the full UV spectra set (and not just a single or a set of UV chromatograms, ie, MS browser panel must show a sub-item called DAD under the Traces item).

Using the crosshair mode and **clicking** on a UV chromatogram while **holding Alt** pressed, will display the UV spectrum for the clicked retention time.

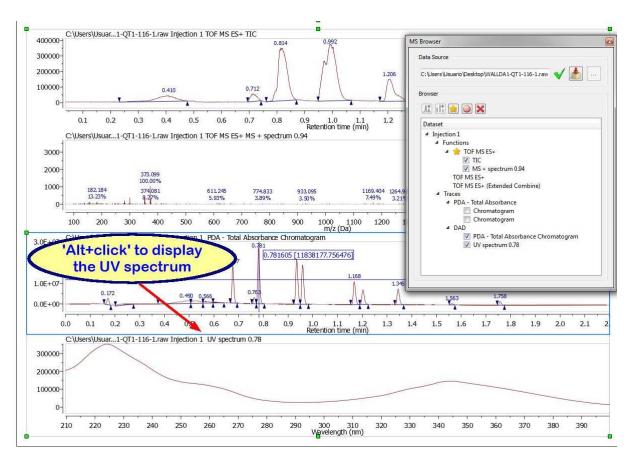


You can also Co-add UV chromatograms by clicking and dragging the crosshair to select a range on DAD chromatograms as you can do with the TICs. Please bear in mind that Mnova MS only supports UV spectra from Masshunter, Bruker Compass, Shimadzu v5, Xcalibur or MassLynx formats.

Highlighting any function in the MS Browser and clicking on the 'New Spectrum' icon  $\amalg$  will display the corresponding dialog box which will allow you to open the desired spectrum by just typing the number on the edit box:




The below picture will show you a TIC (red), a Mass spectrum (number 467), the Base Peak (green) and the chromatogram between m/z=150.23-320.23 (pink):

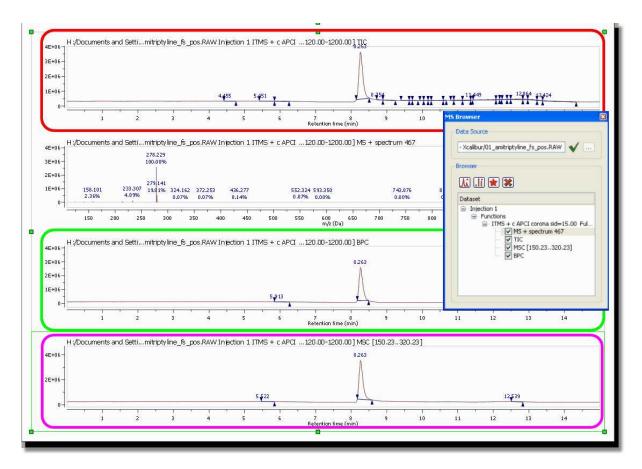

In the example below, you can see two TICs of two different functions:



Selecting a function on the MS Browser window and clicking on this button . will set the selected function as active. This option will allow you to work with the traces chromatogram of different functions. It will be very useful for example if you have a PDA-Total Absorbance Chromatogram and you want to display the MS of one of the functions only:

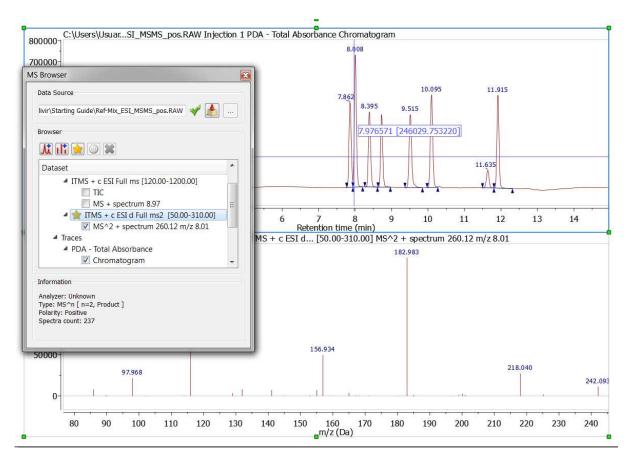


If you have two or more spectra opened in the document, you can use the feature to 'Select the spectrum plot as selection target' in order to change that plot when you decide to display any other MS (after having clicked on a chromatogram under the crosshair mode). You will obtain the same result by clicking on the blue radio button of the MS spectrum:

N	4S Browser & X		
1	Data Source	C:\Users\UsuarSI_MSMS_pos.RAW Injection 1 PDA - Total Absorbance Chromatogram	
•		8E+057 86/08/2018 80/08	
	Aedivir\Starting Guide\Ref-Mix_ESI_MSMS_pos.RAW 💜 🃩	8.018980 [451571.114678]	
		6E+05- 10.095 11.915	
	Browser	1,002 8.395 9,515	
		4E+05-	
	Dataset Set selected spectrum plot as selection target	2E+05-	
	Injection 1		
	<ul> <li>Functions</li> </ul>		
	ITMS + c ESI Full ms [120.00-1200.00]	1 2 3 4 5 6 7 8 9 10 11 12 13 14	_
	TIC	Retention time (min)	
	MS + spectrum 8.97	O C:\Users\UsuarSI_MSMS_pos.RAW Injection 1 ITMS + c ESI F120.00-1200.00] MS + spectrum 8.97	
	4 👷 ITMS + c ESI d Full ms2 [50.00-310.00]		
	MS^2 + spectrum 260.12 m/z 8.01	4.0E+07-	
	Traces     PDA - Total Absorbance	3.0E+07-	
	Chromatogram		
	PDA - Maximum Absorbance	2.0E+07- 439.164	
	Channel A	1.0E+07- 171.091 280.120 470.148	
	UV B (0, 0)	1.0±+07- 3.57% 0.84% 1.43%	
	UV C (0, 0)	0.0E+00-	
	DAD	· · · · · · · · · · · · · · · · · · ·	
		150 200 250 300 350 400 450 500 550 600 650 700 750 800 850 900 950 1000 1050 1100 115 m/z (Da)	0 120
		C:\Users\UsuarSI_MSMS_pos.RAW Injection 1 ITMS + c ESI d [50.00-310.00] MS^2 + spectrum 260.12 m/z 8.01	
		182.983	
		150000-	
		115.939	
		100000-	
		156.934	
		50000- 97.968 218.040	
		97,968	242.093
	Information	0	
1	Polarity: Positive		1
1	Order: 2 Scans: 31	80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 m/z (Da)	240
	Times: 8.01	e e <sup>niy</sup> z (ba)	•

Please bear in mind that different mass spectrometer acquisition data systems do different things with the names of traces. When we import traces, we do our best to retrieve sensible names, but they are not always present (or appear as 'Channel A' for example). We hope that the chemist who acquired the data will usually know what "Channel A" actually is.

ata Source)	
C:\Users\U	suario \Desktop \Ref-Mix_ESI_MSMS_pos.RAW 🛛 😽 🗔
rowser	
<b></b>	
Dataset	
<ul> <li>Injecti</li> </ul>	on 1
⊿ Fu	nctions
4	👷 ITMS + c ESI Full ms [120.00-1200.00]
	MS + spectrum 8.25
	TIC TIC
	MS + spectrum 8.97
	🔽 🥥 MS + spectrum 9.78
	ITMS + c ESI d Full ms2 [50.00-310.00]
▲ Tra	
	PDA - Total Absorbance
	PDA - Maximum Absorbance
	Channel A
	UV B (0, 0)
	UV C (0, 0) DAD
1	PDA - Total Absorbance Chromatogram
	V UV spectrum 8.00
	V UV spectrum 8.02
	V Spectrum 10.08
<b>6</b>	
nformation	
Polarity: Pos	itive
Order: 1 Scans: 528	
Times: 9.78	

You can select several chromatograms or spectra in the same page, for example to 'zoom in' or extract them to a new page at the same time. To do it, just hold down the 'Ctrl+Alt' ('Cmd+Alt' in Mac)key and click. To release the selection, press 'Ctrl+Alt' (Cmd+Alt in Mac) and click on the undesired item:

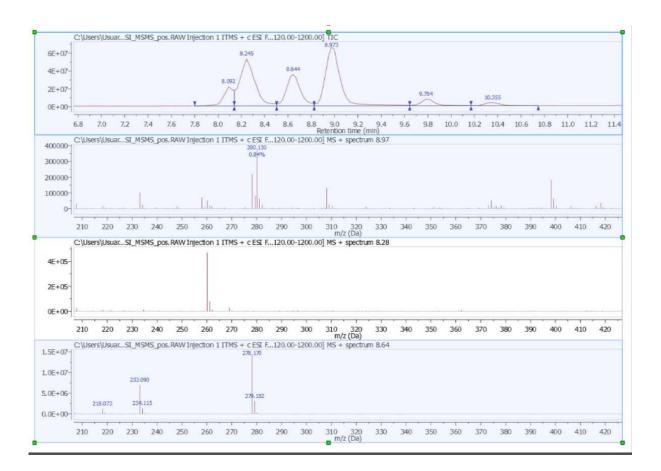

### 14.2.2 Mass Analysis

Mnova MS allows the user to carry out fully automatic analysis of LC/GC/MS data. Easily obtain:

- Automatic TIC integration values and MS trace m/z values
- Automatically compute potential Elemental Compositions for a given mass ion peak
- Automatically match proposed molecular structures to a TIC spectrum


The Mass Analysis menu contains these useful features:

- Peak Detection
- Spectrum Selection Mode
- Elemental Composition
- Molecular Match
- New Mass chromatogram
- Align Traces retention time
- Spectrum Prediction

Let's take look at them one by one.

#### 14.2.2.1 Peak Detection (Integration)

It is possible to integrate the desired peaks of your TIC chromatogram with Mnova MS by following the menu 'Mass Analysis/Peak Detection' or by using the corresponding icon of the toolbar:

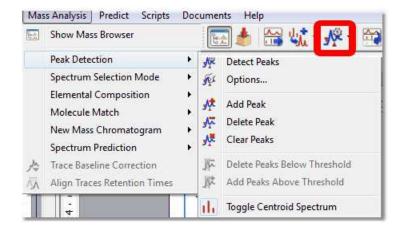

You will find several features under the 'Peaks Detection' menu:

Detect Peaks: applies an automatic peaks detection to your TIC.

**Detect Peaks Options:** from here you can customize the threshold of the minimum area of the peaks for the automatic detection and also to define the regions to Peak Pick and keep those as default:

Settings		Ok
Minimum Aro	a Threshold: 0.50%	<u>U</u> N
		<u>C</u> ancel
Excluding R		<< More
Units:	Time (min)	
Up to:	0.00 min	
After:	1000.00 min	
Apply to		
Ourrent		
🔿 All		Save


The regions which are ignored from peak picking will be highlighted in grey to indicate that they are not included in the peak picking.

Clicking on the 'More' button will allow to select other advanced options; such as sensitivity, smoothing or shoulders sensitivity:

ttings				Qk
	a Threshold:	0.50%	×	<u>C</u> ance
Advanced				Less >
Sensitivity:		55.00	×	
Smoothing		Auto	*	
Shoulder S	ensitivity:	0.10		
Wide Peaks	s:			
Excluding R	egions			
Units:	Time (min)		•	
Up to:	0.00 min	(A) (V)		
After:	1000.00 m	in 🛓		
ply to				
F 1/				

Add/Delete and Clear Peaks: these features are used to manually add or delete peaks to your TIC or to delete all the peaks.


Please bear in mind that it is possible to change the integral region of any peak just by clicking and dragging on the wedges:

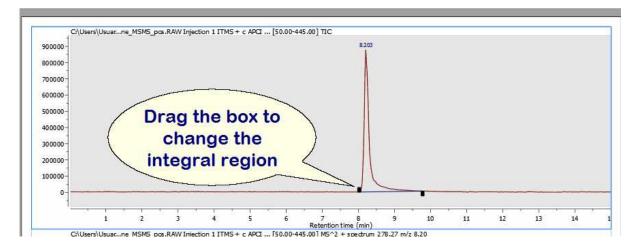


You can freely move the wedges by moving the integrals handler while shift is pressed.

#### Add/Delete Peaks (Threshold)

You can graphically add peaks above a threshold and delete peaks below a threshold:

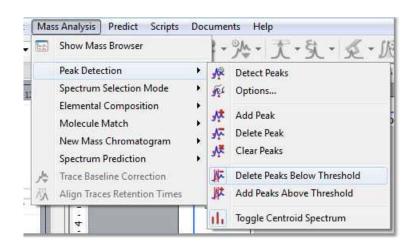


**Toggle Centroid Spectrum:** This is a toggle to switch between profile and centroid mode of the MS spectrum.

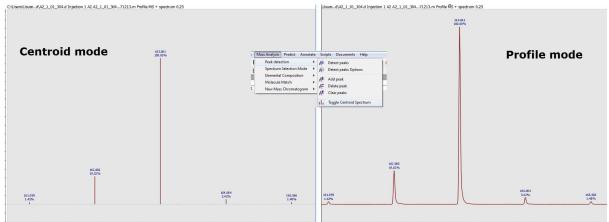

165.8 161.0 161.2 161.4 161.6 161.8 162.0 162.2 162.4 162.6 162.8 163.0 163.2 163.4 163.6 163.8 164.0 164.2 164.4 164.5 164.2 165.4 165.0 165.2 161.4 161.6 161.8 162.0 162.2 162.4 162.6 163.0 163.2 161.4 164.6 164.8 165.0 165.2


You can export mass peaks as ASCII by following the menu 'File/Save As' and selecting the option "Script: Mass Peak Table (\*.csv \*.txt)". You will get a list of m/z and Relative Abundance. You can follow the menu 'Scripts/Export/MS Peaks (or MS Data for the chromatograms).

The user can manually adjust the peak detection settings, allowing to specify the desired resolution to build the centroid spectrum:

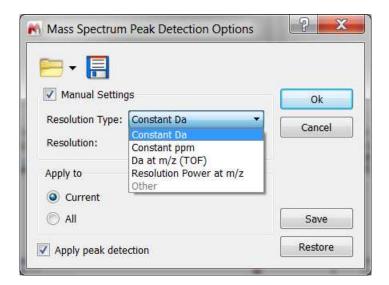


#### 14.2.2.2 Spectrum Selection Mode

This feature will allow you to add additional Ms spectra to your document and also to generate 'CoAdds' and subtractions.

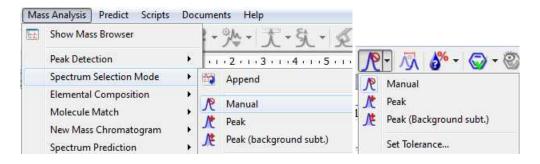

**Append**: This feature will allow you to add additional MS spectra to the main window just by selecting 'Append' in the corresponding menu and clicking with the crosshair on the corresponding signal of the TIC. If the 'Append' option is not selected, the current MS spectrum will change after having clicked on the corresponding signal of the TIC.


In this case we have added the MS spectrum 738 which appears at 12.90 min.

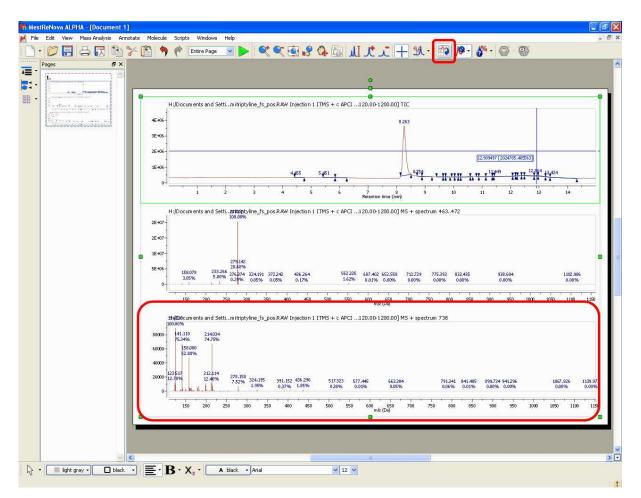


You can combine the 'Append' option with the 3 different modes of the crosshair (Manual, Peak and Peak (Background Subt)):

Manual Manual This is the default mode of the crosshair. In this mode, you can select any other mass


spectrum for a particular time point with the crosshair feature is just by clicking on the corresponding signal of the TIC. For example in this case, we have selected the spectrum at a 'Retention time' of 8.64 min:

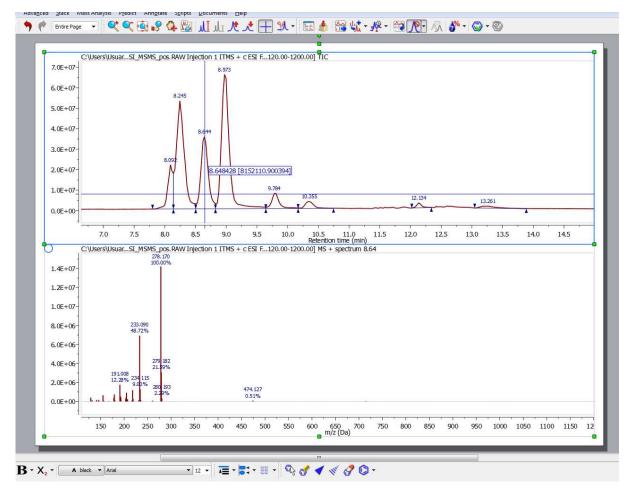


If you need to average the mass spectra over a certain time range (CoAdd), just hold down the left mouse button (after having selected the crosshair) and drag over the appropriate time span in the TIC. A label at the top of the MS will inform you about the spectrum ranges (red rectangle in the picture below):

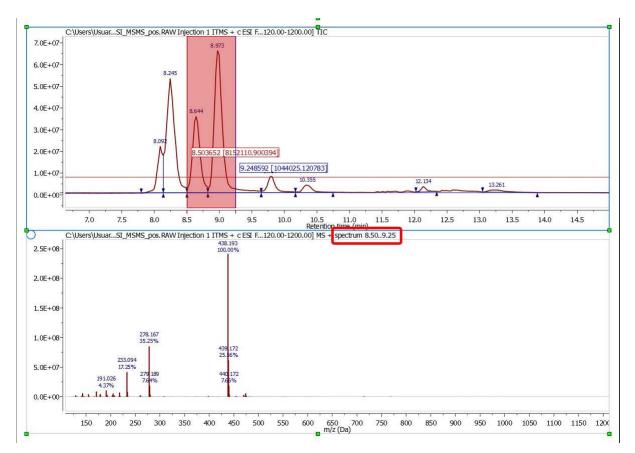

After having done the 'CoAdd' you can do a 'subtraction' by just selecting the 'Crosshair' feature, pressing the 'SHIFT' key and holding down the left mouse button and dragging over the desired time span in the TIC.

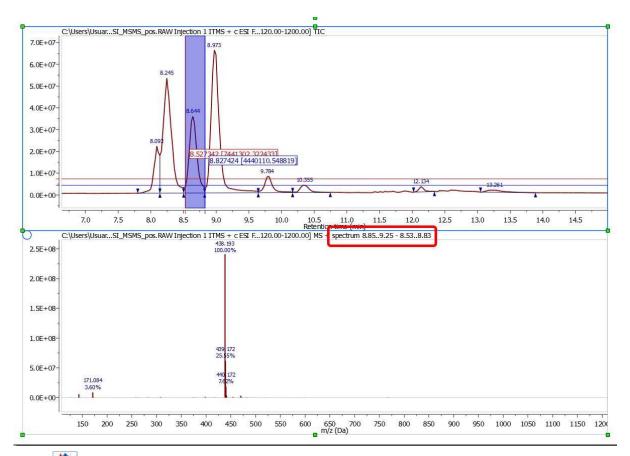


**Peak:** Me Selecting this mode and clicking with the crosshair on the corresponding signal of the TIC, will generate a 'CoAdd' of the midle part of the peak. The spectra from the middle half are used because they're the highest intensity and s/n. Spectra at the peak edges are then the opposite, lower s/n and more likely to contain background. Often when a peak elutes, background is actually suppressed, especially with higher concentration components. This approach is a common technique.

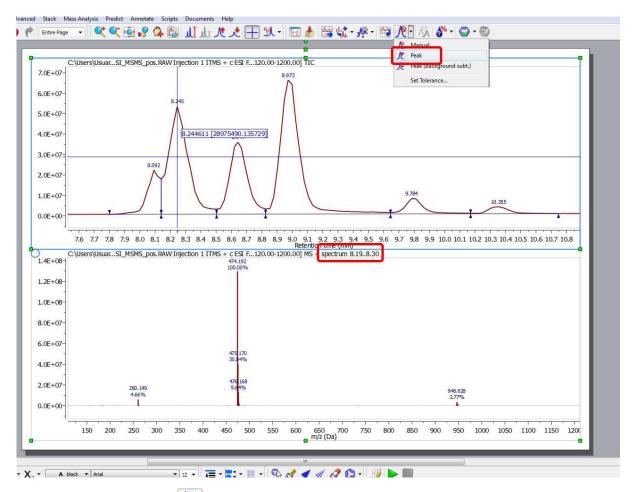


# Peak (Background subt.):

To generate a 'CoAdd' of the whole peak without the tail-peaks just select the mode 'Peak (Background Subt.)' under the 'Mass Analysis/Spectrum Selection Mode' menu and click with the crosshair on the desired signal of the TIC:

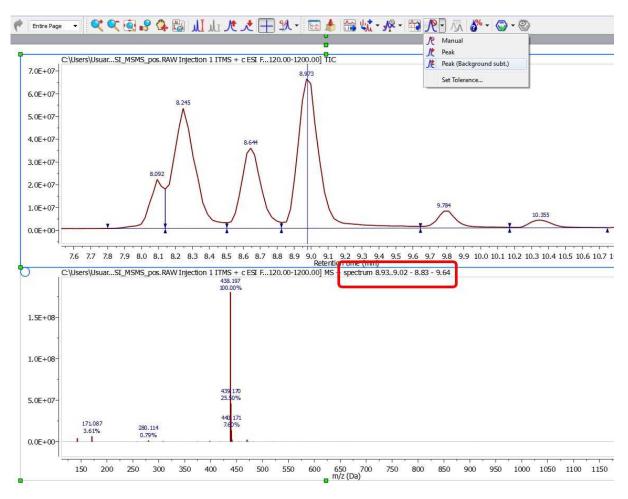

When you are in the spectrum selection mode (with the append mode disabled), you can choose graphically (by checking the blue circle <sup>(2)</sup>) which of the plots must be replaced when you select a spectrum in a chromatogram. The selection target can be also done from the MS Browser, just by selecting the applicable MS and clicking on the 'selection' button <sup>(2)</sup>.

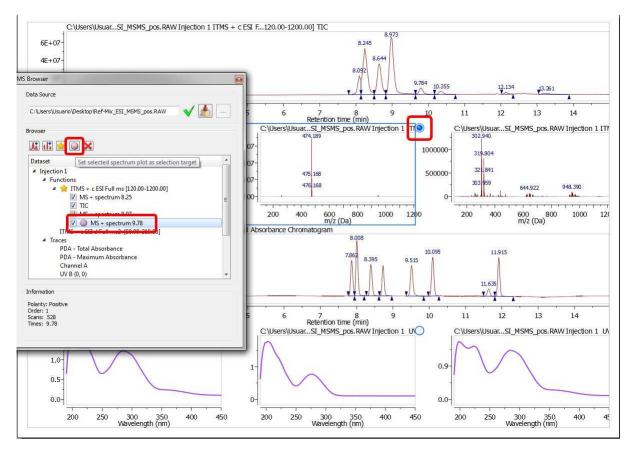

Set Tolerance: From this dialog box, you can select the tolerance (in Da or ppm) of the spectrum selection mode.

Tolerance:		ОК
0.100 Da 🌩	Units: () Da	Cancel
	O Ppm	

Merged tolerance is a m/z tolerance used any time mass spectra are summed or subtracted. The tolerance is applied to m/z values. Thus a merge tolerance of 0.1 Da means that if two spectra being summed contain, respectively, m/z 100.100 and m/z 100.150, the two mass peaks with be logically summed, since they're within 0.1 Da. The resultant intensity is the simple sum; the resultant m/z value will be the intensity-weighted average of 100.100 and 100.150.

#### 14.2.2.3 Elemental Composition


Elemental composition analysis is one of the most informative techniques in mass spectrometry. With appropriate mass spectral data, elemental composition can quite often determine the unambiguous elemental composition of a molecular ion.

This technique, however, only produces sensible results from high accuracy mass spectra. For ions less than or equal to m/z 200, a measured accurate mass within 5 ppm is often required to determine elemental composition. At higher m/z values, measured accurate mass values of significantly less than

5 ppm may be required.

The algorithm that is used exhaustively computes all possible combinations of elemental formulae subject to the constraints provided by the user (see below). In some cases, millions of possible formulae are evaluated, but because of the speed of the algorithm, this happens very quickly.

This feature will be very useful to calculate the elemental composition of one or more mass peaks of a spectrum, if the m/z values are of high accuracy, typically 5 ppm mass accuracy or better.

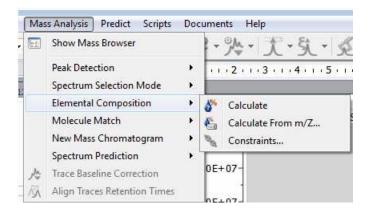

First of all, you should establish the constraints of the calculation, just by clicking on the applicable option of the menu, which will display the dialog box below:

ler	ment Constraints:			Double Bond Equiva		<u>о</u> к	
			*	Maximum:	-0.50		<u>S</u> ave
	Element	Minimum	Maximum	Tolerance:			Restore
1	с	0	100	Units:	ppm	•	Cancel
2	Н	0	200	Value:	5.00	\$	
3	N	0	10	Maximum Resul	t Count:		
4	0	0	10	Maximum:	1		
5	S	0	5		1		
				Other Constraints:			
				Electron Mode:	Both	•	
				Charge State:	1		
				Adduct:	н		
				Fitness Threshold:	0.00		

Click on this icon 💽 to add more 'Element Constraints':

Element			TÍ		c	0k												
Element Symbol:	N	•			Ca	ncel												_
Minimum Count:	н																	H
Paramoni Courte.	Li	Be											В	С	N	0	F	Ne
Maximum Count:	Na	Mg											AI	Si	Р	S	CI	Ar
	K	Ca	Sc	Ti	٧	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr
	Rb	Sr	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	I	Xe
	Cs	Ba			Ta	Propagation	Re				and states and							Rr
	Fr	Ra		Df	Dh	Sq	Bh		and the second second			and the second second						

You can also select the 'Double Bond Equivalence', 'Tolerance', 'Maximum Result Count', 'Electron Mode', 'Charge State', 'Adduct' and Fitness Threshold'.

#### Double Bond Equivalence (DBE): Rings + double bonds

**Tolerance:** Tolerance for matching computed composition to the target m/z. If spectral mass accuracy is expressed in ppm, then the tolerance for matching should also be in ppm. The typical values in Da should be 0.01 or less, or in ppm 5 or less. Tolerances much larger than this, generally give too many hits to be useful.

m/z: symbol used to denote the quantity, in units of Daltons (Da), formed by dividing the mass of an ion in unified atomic mass units by its charge number (regardless of sign).

Maximum Result Count: The maximum number of results to return.

**Electron Mode**: Electron mode can be even, odd, or both. Typically, El (electron impact) produces positively charged, odd electron ions, whereas ESI (electrospray ionization) produces even-electron ions with either a positive or negative charge.

El: lonization of an atom or molecule by electrons that are typically accelerated to energies between 10 and 150 eV in order to remove one or more electrons from the molecule. The term electron impact is deprecated.

ESI: A process in which ionized species in the gas phase are produced from a solution via highly charged fine droplets, by means of spraying the solution from a narrow-bore needle tip at atmospheric pressure in the presence of a high electric field (1,000 to 10,000 V potential).


**Charge State:** is a signed value. The magnitude (1, 2, 3, ...) is a function of the experimental ionization technique, while the sign (+/-) is determined by the mode in which the experimental spectrum was produced and detected. For electron impact (EI) spectra, charge state is usually +1, while for ESI charge state is usually +1 or -1 for most organic compounds. Peptides may have higher charge states.

**Adduct:** Adducts are typically found in soft ionization techniques such as ESI. Proton (H) is most common for organic compounds, while H and/or Na (or other Group 1A alkali metal cation) may be found in protein, peptide or polymer spectra. NOTE: If an adduct is specified, the mass (\* charge state) is subtracted from the target mass before compositions are computed. The composition calculation assumes a neutral (uncharged, non-adducted) mass.

**Fitness Threshold:** Results that match the other criteria but have fitness lower than this threshold will be discarded. Fitness ranges from 0.0 (no match to experimental spectrum) and 1.0 (perfect match).


Once you have finished with the constraints, click on the 'Elemental Composition' icon elect with the crosshair the desired peak of the Mass spectrum. A table with the results will be displayed (it is also possible to find this table under the 'View/Tables' menu). All the results obtained

will satisfy the composition, DBE, and tolerance constraints, and will be ranked in decreasing order of fitness. Please bear in mind that a fitness value of 1 will be the perfect match.

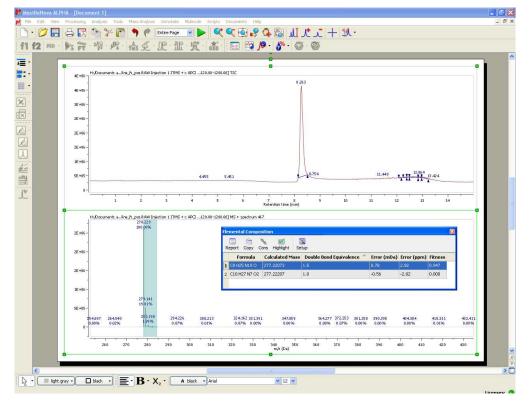

Click on the applicable button of the Elemental Composition table to remove the highlighted area .

You can also calculate the elemental composition table from a given m/z value:

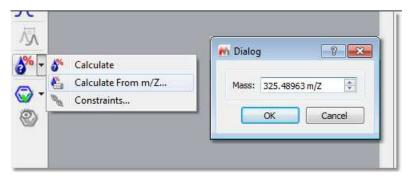

Please bear in mind that mass spectrometers measure monoisotopic m/z values which is different with the Molecular weight value (calculated using the average mass of each element weighted for its natural isotopic abundance). For example, for C20H23N, the chemical mw is 277.402, and monoisotopic mw is 277.182. Here you can see a list of the exact mass of some elements:

Element	Symbol	Exact Mass
Hydrogen	H 2H (D)	1.00783 2.0141
Carbon	12C	12

	13C	13.0034
Nitrogen	14N	14.0031
	15N	15.0001
Oxygen	16O	15.9949
	170	16.9991
	18O	17.9992
Fluorine	F	18.9984
Silicon	28Si	27.9769
	29Si	28.9765
	30Si	29.9738
Phosphor	Р	30.9738
us		
Sulphur	32S	31.9721
-	33S	32.9715
	34S	33.9679
Chlorine	35CI	34.9689
	37CI	36.9659
Bromine	79Br	78.9183
	81Br	80.9163
lodine	l I	126.9045

#### 14.2.2.4 Molecular Match


Molecule match analysis determines the possible presence of a given structure or structures within a mass spectral data set. The molecular ion cluster of each structure is computed and compared to each spectrum in the data set. If one or more spectra contain the computed isotope cluster within reasonable matching constraints, the most intense spectrum within the most closely matched chromatographic peak is returned as a positive result. Structures not matched are assigned a "not found" result. The constraints dialog allows the user to select one or more adducts, specify ion polarity, and other parameters.

The algorithm makes use of fast isotope cluster calculations and a sophisticated spectral matching technique.


Molecule match analysis is very general purpose. Applications include small molecule confirmation and metabolite identification.

Limitations are few but include the requirement that the acquired spectra of the compounds being analyzed exhibit at least partial molecular ion clusters.

The 'Molecule Match' is very useful to see if a mass spectrum and a GC chromatogram match with one of the molecular structures of the document.



Just load your spectrum (TIC and MS) and paste the molecular structures into any page of the same document (or load whole spectral libraries by opening an sdf file). Next click on the 'Calculate Molecule Match' button of the toolbar 💇 (or follow the menu 'Mass Analysis/Molecule Match/Calculate').

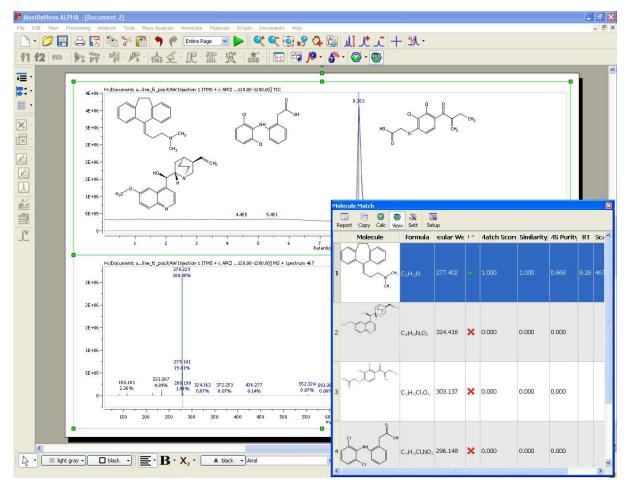

The 'Molecule Match' table with the results will be displayed (this table can also be found under the 'View/Tables' menu). This table will contain information about the 'Retention Time' (RT), Scan (number of spectrum), Match Score, Similarity, MS Purity, etc..

**Similarity** is the comparison of the computed isotope cluster spectrum of a given molecule's molecular formula, plus optional adduct - that is, the mass spectral peaks of the molecular ion - with the mass peaks of the acquired spectrum in that mass region. The similarity value can be from 0 to 1, and you will note that a threshold of 0.8 is used. For instance, a pesticide named Pydrin, with a molecular formula of C25H22NO3CI, plus an adduct of H, has an isotope cluster of 420.137 - 100%, 421. 140 - 28%, 422.135 - 36%, 423.137 - 10%, 424.140 1.5%. This is compared with the mass peaks of the acquired spectrum in the mass range of about 420 to 425.

Match Score is the product of Similarity and MICC value (see below).

MICC is molecular isotope-cluster chromatogram. Which is the sum of mass chromatograms of all the significant peaks in the isotope cluster. Using the example above, m/z 420.137 + 421.140, and so on.

This is almost the same as the mass chromatogram, across several Daltons, in the case listed above, from m/z 420 425. The reason it is not the same is that for accurately measured mass spectral data, a

small tolerance on the order of a few ppm might be used for matching.


For any given molecule, the MICC chromatogram is normalized to 1.0, and this value is what is used for Match score above.

**MS Purity** is the proportion of the total intensity of the mass peaks matched in the Similarity measurement relative to the total intensity of the whole spectrum. MS Purity is then, the fraction of the found molecular ion intensity versus the total intensity of the spectrum. This assumes that most of the intensity of the whole spectrum will be due to the molecular ion cluster, which is true for soft ionization mass spectra, which is true for most forms of ionization in use today. Which is not to be confused with MS/MS experiments, which have impart additional energy to produce fragmentation. So, using the MS purity as a metric generally provides a useful value that is a larger value with "pure" spectra, that is spectra without a lot of background (or overridden by the intensity of the molecular ion) or without a coelutant.

Purity is the ratio of the matched peak area (in the TIC) of the signals of matched compounds.

Clicking on any "matched molecule" will display the MICC (Molecular Isotope Cluster Chromatogram), overlaid with the TIC. The MICC shows the summed response of the isotope cluster for each MS spectrum over the entire data set. The MICC is the sum of the mass chromatograms of each m/z value of an isotope cluster.


In this example, the best result was for the compound number 1 (C20H23N). You can see in the picture below the MICC (in green) over the TIC (in red):

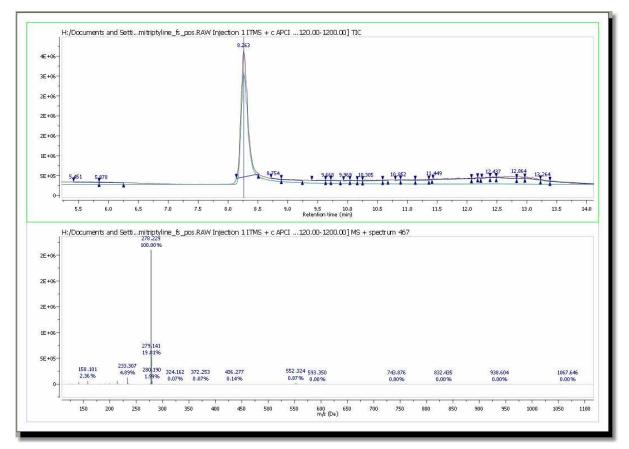


In addition, Mnova shows you in the chromatogram the retention time of the match (with a blue vertical line) and displays the corresponding MS spectrum (the number 467 in this case) overlaid with the

theoretical one (in green at a M/Z around 278, in this case). It is possible to show/hide the MICC and the theoretic MS just by clicking on the 'View Molecular Match' icon .

Here you can see another example, where the compound 8 (amitriptyline) is present in the mixture:

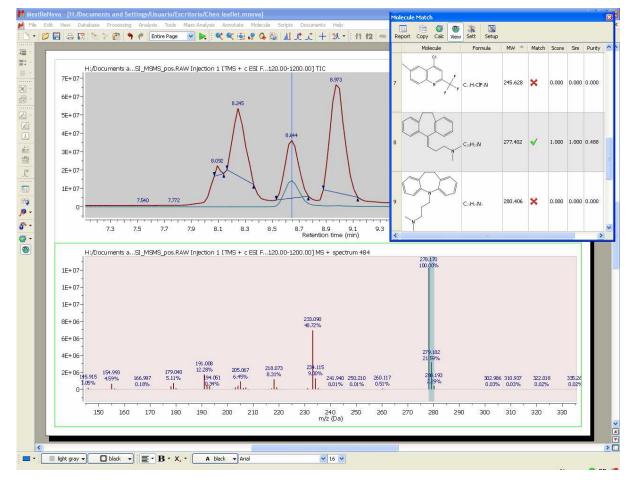

It is also possible to run a Molecular Match with a MS/MS spectrum and see the result directly in the MS/MS. Here you can see an example:

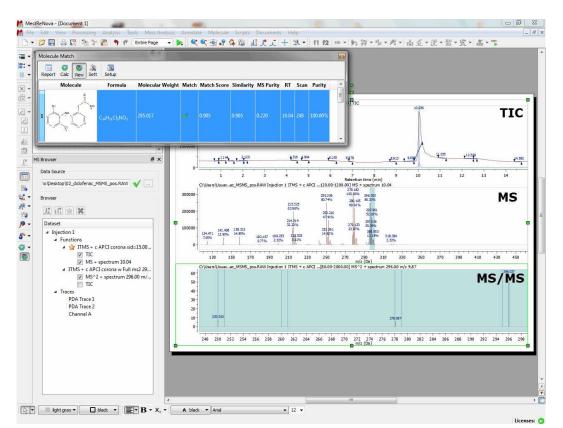

The user can also run the 'Molecular Match' feature just by entering a molecular formula after having clicked on the 'Calculate From Molecular Formula' in the applicable scroll down menu:

		m	Molecular Formul	a	? ×
		Mo	lecular Formula:	C6H15N	•
			Formula	Weight	
0	10	1	C₅H <mark>15</mark> N	101.120	*
	Calculate From Molecules Calculate From Molecular Formula Settings			ОК	Cancel

Select 'Settings' on the 'Mass Analysis/Molecule Match' to display the 'Molecule Match Settings' dialog box:

Tolerance					Thr	esholds					
Units:		Da		-	Score Threshold: Matches per Molecule:			0.25		<u>O</u> K	
For MS:		0.30						3		<u>S</u> ave	
For MS/MS:		1.00			Matched Molecules per Spectrum:		1		Restore		
Positive Polariza Adducts/Losses					3	jative Polar ducts/Losse					Cancel
Adduct	Loss					Adduct	Loss				
1 H+	1				1		H+				
2 Na+			=		2	CI-			=		
3 K+					3	Na+	2H+				
4 CH3OHH+	Ę				4	K+	2H+				
5 NH4+					5		H2OH+				
 Max Charge:		1				- x Charge:		1	•		

**Tolerance:** To set the m/z tolerance for matching predicted spectra to experimental; by default, MS spectra are matched to either 5 ppm or 0.5 Da, and MS/MS to 10 ppm or 1.0 Da, depending on whether the spectra are derived from high or low resolution instruments.

**Thresholds:** Set match score threshold for acceptable result; in most cases the default value of 0.5 is more than enough, however for weak / noisy spectra, the threshold may be lowered.

**Matches per molecule:** To set the maximum number of results per molecule; by default, a molecule is allowed to match only once, in which case the best result is returned. However, if no MS/MS spectra are available and the sample is known to contain isomers, then increasing this limit will allow the molecule to match every isomer peak.

**Matches per spectrum:** Set maximum number of molecules allowed to match a spectrum; by default, each spectrum (or set of related spectra) is allowed to match only one molecule. However, if isomers are present in the molecule list, then allowing all matches may be desired.

Adducts: Set adduct/loss pairs using proper atomic or chemical formulas with charge notation.

Charges: Set maximum charge states to consider. By default, +/- 1 are the maxima.


**Dimers:** Set to enable consideration of dimers when matching; by default, dimer matching is disabled. A dimer (in this case) is a non-covalently bound molecule pair (e.g. bound by van der Waals, hydrogen bond, or electrostatic forces, not a covalent inter-atomic bond). If you have a molecule M, then in ESI+ it normally gives an [M+H]+ ion. If it forms a dimer in the ESI source, then the ion observed is [2M+H]+, and the m/z value we look for is twice the mass of M plus the mass of H.

#### 14.2.2.5 New Mass chromatogram


It is very useful to extract a MS spectrum by following the menu 'Mass Analysis/New Mass Chromatogram' or by clicking on the corresponding icon of the toolbar:

	Mass Analysis Annotate Mole	cule	e Scripts Documents Help
add a	Peak detection Spectrum Selection Mode Elemental Composition Molecule Match	* * *	<mark>↓ + % •</mark> <mark>% •</mark> /*• 6 •
ï	New Mass Chromatogram	Þ	Graphically Manually


It is possible to extract the MS chromatogram **graphically** or **manually**. To extract the MS graphically, just select the option and click on the MS (or click and drag if you want to select a range):

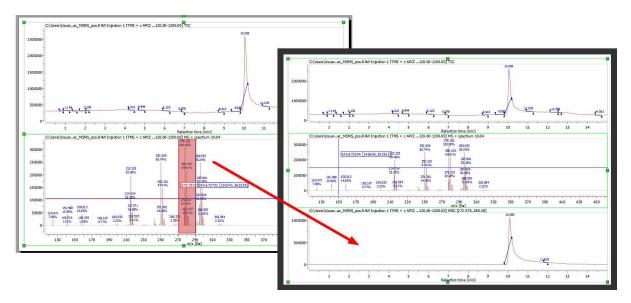

You can also select the range of the new chromatogram manually:



This also can be done from the MS Browser ('New chromatogram/Mass'):



### 14.2.2.6 MS Spectrum Prediction


Follow the menu 'Mass Analysis/Spectrum Prediction/Settings' to choose the desired adducts and losses used for the predictions:

10	0.00 🚖 pp	m 🔻				
dd	lucts:					
	Adduct	Loss	Charge	Mass	m/z	
1	H+		+1	+1.0073	+1.0073	
2	Na <sup>+</sup>		+1	+22.9892	+22.9892	
3	K⁺		+1	+38.9632	+38.9632	
4	CH₃OHH+		+1	+33.0335	+33.0335	
5	NH4 <sup>+</sup>		+1	+18.0338	+18.0338	
6		H⁺	-1	-1.0073	-1.0073	
7	CI-		-1	+34.9694	+34.9694	
8		2 (	-2	-38.0357	-19.0178	
9	Br		-1	+78.9189	+78.9189	

You can add new adducts by clicking on the 'blue plus' button. For example, to add an electron, just type 'H' for the adduct and 'H+' for the loss (the net result will be an electron):

Adduct: Formula: H	Resolution: 100.00 ppm v Adducts:							
Formula: H+		Adduct	Loss	Charge	Mass	m/z	]	
	1	H+		+1	+1.0073	+1.0073		
Formula Syntax: n(formula z)	2	Na <sup>+</sup>		+1	+22.9892	+22.9892		
parenthesis and a single ion is assumed.		K+		+1	+38.9632	+38.9632		
<ul> <li>formula: A chemical formula like C21H22N2O2. You can type roups enclosed in parenthesis like (NH4)2SO4 or you can specify</li> </ul>	4	CH₃OHH⁺		+1	+33.0335	+33.0335		
rmula: A chemical formula like C21H22N2O2. You can type ps enclosed in parenthesis like (NH4)2SO4 or you can specify pes by preceding the atom symbol with the mass number like I4. Be careful to enclose the isotope between parenthesis or to	5	NH4 <sup>+</sup>		+1	+18.0338	+18.0338		
dd and an extra space if it appears in the middle of the formula ke Na(37Cl) or Na 37Cl	6		H+	-1	-1.0073	-1.0073		
<ul> <li>- z: An optional charge like +1 or -2. If only the sign is present ten one charge is assumed.</li> </ul>	7	CI-	-1	+34.9694 +34.9694	+34.9694			
Examples: 3(H+)	8		2 ( H <sub>2</sub> OH+ )	-2	-38.0357	-19.0178		
Na+	9	Br		-1	+78.9189	+78.9189		
CI- (H2O)3(H)2 +2 CH3OHH +	10	0 H	H+	-1	+0.0005	+0.0005		

Select 'Predict' to simulate the mass spectra with the desired losses and adducts:



This will display a new window to enter the desired molecular formula or to select between the recent used or from the compounds available in the <u>'table of compounds'</u>:


Mo	lecular Formula:			-
1	Recent			
	C20H24N2	02		
	C19H22N3	03F1		*
	C152H136N	11608Zn		
4	Compounds			
	C20H24N2	2.73		
	C13H12Cl2	S .		
	C16H21NO	-		
	C14H11Cl2			
	C20H21CIC			
	C22H26F3N C20H23N	1305		
	C20H23N	AC .		
	C13H20N20			
	C27H46O	~~		
-	<u>s w</u>			1
	Formula	Weight		
1	C14H11CI2NO2	295.017		
	$C_{22}H_{26}F_3N_3OS$	437.175		
2		473.166		
	$C_{28}H_{27}NO_4S$			
	C <sub>28</sub> H <sub>27</sub> NO <sub>4</sub> S			

After having clicked on the blue plus button to add the desired formula and clicked OK, you will get the MS prediction table with all the applicable adducts:

6E+07-								8.973	
	Ma	ss Prediction					×		
4E+07-		port Copy	Highlight Export	Delete Clea	r Setup			8.644	
2E+07-		Formula	Adduct / Loss	Charge State	m/z	Status	*	8.092	
22107	1	C <sub>22</sub> H <sub>22</sub> NO <sub>4</sub> S	H* /	+1	474.17391	4			9.784
0E+00-	2	C28H27NO4S	Na* / —	+1	496.15585	*	E		
	3	C28H27NO4S	К*/—	+1	512.12979	*			· · · · · ·
_	4	C29H27NO4S	CH₃OHH+/-	+1	506.20012	*		7 8 9 Retention time (min)	10 1
.0E+07-	5	C28H27NO4S	NH+* / —	+1	491.20045	*		0.00] MS + spectrum 8.28 100.00%	
-	6	C28H27NO4S	—/H⁺	-1	472, 15826	*		T	
.0E+07-	7	C28H27NO4S	cl-/	-1	508.13493	*			
-	8	C28H27NO4S	—/2(H₂OH*)	-2	217.56465	*			
.0E+07-	9	C28H27NO4S	Br <sup>-</sup> / —	-1	552.08442	*		475.174 31.08%	
	10	C22H26F3N3OS	H*/—	+1	438.18269	*	-	476.161 9.59%	
0E+00-		-							

The simulated mass spectrum can be obtained even if there is no experimental spectrum present:

- if there is an experimental spectrum, the simulated spectra will be superimposed on the experimental spectrum by selecting each of them in the Mass Prediction table. Each of the predicted mass spectra can be exported to a new page by clicking on Export button from the table.

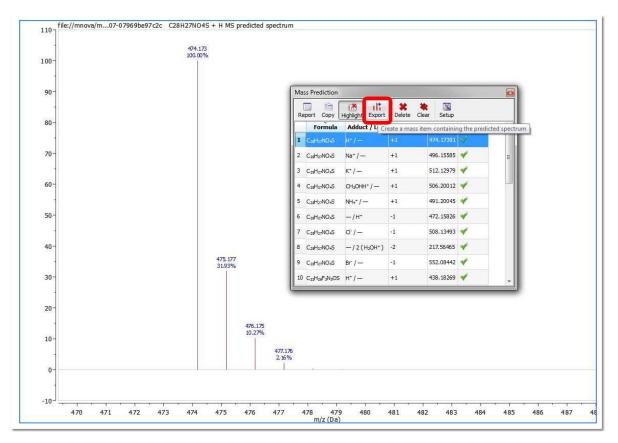


- if there is no experimental spectrum, the simulated spectra can be displayed just by exporting each of them using the Export button.

See also this video


### 14.2.2.7 Trace Baseline Correction

It is possible to correct the baseline of DAD traces just by following the menu 'Mass Analysis/Trace Baseline Correction:

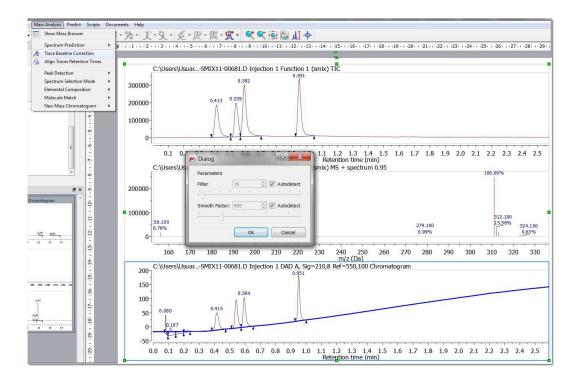

#### 14.2.2.8 Align traces retention times

For some technical reasons, the TIC peaks can be delayed compared to the UV peaks. This feature will re-calibrate the chromatograms so that the peaks match across them. You will only need to click on a peak in the selected chromatogram and enter the new value to change the X scale (time).

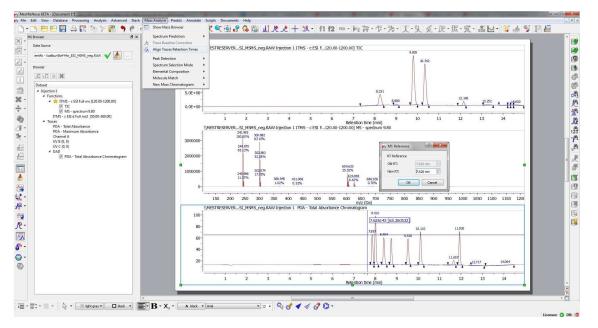

#### 14.2.2.9 Traces autoalignment

This feature will be useful to align UV/DAD and MS traces by using a correction value.

All the mass items have automatic trace alignment parameters that can be set by following the menu

'Mass Analysis/Traces Auto Alignment':

Paramet	ers	ОК
Apply	aces	Cancel
Offset:	0.102 min	1

Those parameters can be predefined from the 'Edit/Preferences/Mass/Import' menu:

Geni	eral Plug-in	Import Verify	ss Molecule S	Scripting Drawing	
		Parameters Apply a 2.000 min offset to all traces Apply a 1.000 min offset to all traces			


The trace alignment parameters are automatically applied to any new trace or DAD chromatogram and the default value for those parameters is determined by the selected preferences. When importing a dataset, if any of the rules match, then the parameters present in the matched rule are copied to the new item.

For the rules, you can specify to which provider (or any provider) the rule applies, and a set of parameter rules based on pattern matching:

Providers			Rules
Any Provider JEOL-FastFlight Bruker-Compass JEOL-MSQ1000 Agilent-IonTrap Shimadzu-LCMS Waters-MassLynx Thermo-XCalibur AB-DataExplorer Agilent-Chemstati NetCDF	on	× III	<ul> <li>All these rules match</li> <li>Any of these rules match</li> <li>         Image: Construct a state of the second secon</li></ul>
AB-Analyst Agilent-MassHunt MS-Text Parameters Apply To	er	-	
V Traces V DAD	2.000 min	4	

### 14.2.2.10 Peak Purity

This feature will calculate the chromatogram peak (or region) purity associated to the most abundant mass peaks which are displayed under the selected peak:

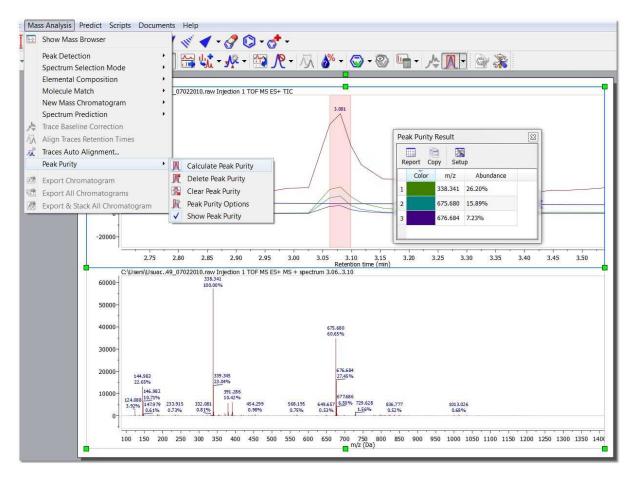


By default the number of curves are 3 and the tolerance is 0.5 Da, but it can be customized via 'Peak Purity Options'.

Extracted Chromatograms Count:	3	Å	<u>0</u> k
Tolerance:	A V	<u>C</u> ancel	
to to			
Apply to		1	<u>S</u> ave


'Delete' and 'Clear' buttons allow to delete peak purity regions in the current chromatogram or in all, respectively.

### 14.2.2.11 Chromatography

You can export TICs and chromatograms from the MS plugin with the Chromatography tool by selecting the MS spectra (in the 'Page Navigator') and following the menu 'Mass Analysis' to select the appropriate option.

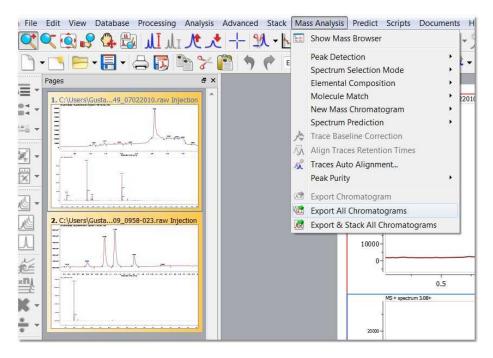

You can export only one chromatogram ('export one Chromatogram') or all the chromatograms in a MS spectrum ('export all Chromatograms'). You can also stack all the chromatograms by selecting 'Export&Stack All chromatograms' option:

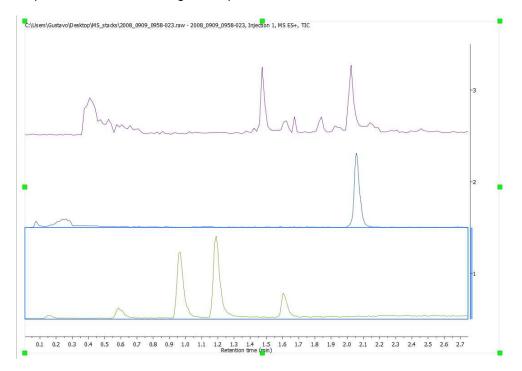


You can also stack chromatograms by selecting them in the 'Page Navigator' and following the menu 'Stack/Stack items'.

#### 14.2.2.12 Background and UV subtraction

This script will subtract a blank background run from the run of interest, for example to ensure a good baseline for quantitation purposes, or to accurately measure differences between two or more runs.

Just follow the menu 'Scripts/Report/Chromatogram Subtraction' and select the folders containing the datasets (foreground and background) and the applicable path masks. Once the script has run, it will generate a report with information about the impurities found:

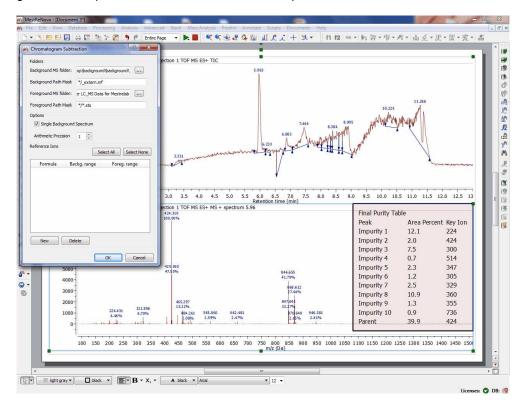

First thing the scripts does is subtraction of the Analysis chromatogram (foreground) minus the blank (background), this will give us the real chromatogram we are interested in, which will only show peaks which are not in the background chromatogram.

To do this subtraction, it is necessary to align the spectra, and this will be done by introducing known peaks at the beginning and end of the run (they will use compounds with certain known very short and very long retention times, which they will introduce in the sample). Finally in the resulted chromatogram, the scripts does a peak picking and integration, which will allow to identify impurity peaks (assumption is that this should be a pure compound, therefore the big peak is the compound, the others are impurities). The script continues until all impurities are check, and repeat process for every analysis chromatogram and its respective blanks. The script generates a Mnova document with the result in the Users folder and an output which is a set of tables as follows:

- Table with parent compound and impurities for analysis 1, with retention times and relative areas, as well as with the key ions which identify the impurity or parent compound
- Same table for subsequent analysis (2, 3, 4, etc.)
- Summary purity table, with averages from all analysis for each one of the peaks

Similarly to chromatogram subtraction, there is another script for UV subtraction (under the 'Scripts/ Report/UV Subtraction' menu). So you will subtract a background UV chromatogram from a foreground one:

Folders	
Background MS folder:	C:/Users/Usuario
Background Path Mask	1
Foreground MS folder:	C:/Users/Usuario
Foreground Path Mask	
Results	
Directory:	C:/Users/Usuario
Options	
Single Background S	pectrum
Peak Subtraction Se	lection Mode
Arithmetic Precision	4

### 14.2.3 MS Tables

You will find all the information about the peaks of your chromatograms and mass spectra by following the menu 'View/Tables/Mass Peaks' (or by right clicking on any toolbar and selecting 'Mass Peaks'):

You can see below an example of a 'Peaks Table' of a chromatogram; which includes information about the '*Retention Time*', the number of the 'Scan', 'Type' (to describe peak ends. Possible values: 'Unknown', BB (Baseline to baseline), 'BV' (Baseline to valley); 'VB' (Valley to baseline); 'VV' (Valley to valley) and 'Shoulder'), 'Height', 'Area' 'Start and End Time':

1.25	eport Co	py S	etup							
	RT 🐣	Scan	Туре	Height	Area	Total Height %	Total Area %	Start time	End time	^
1	14.600	709	VB	311755.386	3865292.127	0.72	1.81	14.529	14.956	
2	14.443	700	٧V	277872.176	2871082.085	0.64	1.34	14.355	14.529	
3	14.286	691	٧V	268608.253	1778055.206	0,62	0.83	14.237	14.355	
4	14.202	687	٧V	255163.880	932628.873	0.59	0.44	14.140	14.220	
5	13.935	675	VV.	171321.197	1148264.482	0.40	0.54	13.898	14.007	
6	13.844	670	٧V	155463.812	879709.497	0.36	0.41	13.808	13.898	
7	13,577	659	٧٧	169826.278	1403073.413	0.39	0.66	13.541	13.753	
8	13.252	641	٧٧	470147.815	6421264.905	1.09	3.00	13.066	13.523	
9	12.876	627	VV	107815,178	939931.616	0.25	0.44	12.791	13.066	×

A table like the below one will be obtained in the case of a 'Mass' spectrum:

Repo	rt Copy	Setup		
1	m/z 🐣	Intensity	Rel. Abundance	^
120	242.199	359.924	0.18	
121	243.006	3021.458	1.51	9
122	244.086	431.711	0.22	
123	245.008	3019.712	1.51	
124	246.266	15926.770	7.95	
125	247.020	200259.203	100.00	
126	248.067	33786.750	16.87	
127	249.021	71883.750	35,90	
128	250.013	13517.686	6.75	
129	251.013	2806.494	1.40	
130	252.098	1653.903	0.83	
131	252.991	561.074	0.28	

Following the menu 'View/Tables/Parameters' will display the Parameters table:


Report Copy Setu	Customize	
Parameter	Value	
1 Data Path	C:\DATA\2005\02-February\Ref- Mix-050220_ESI_MSMS02.RAW	
2 Acquired Date	2005-02-21T15:55:37	
3 Sample Name	Ref Mix (with dyn excl)	
4 Comment	Xterra_MS_C18 2.5u 1x50mm	
5 Operator	Administrator	
6 Submitter	ROLLFR9	
7 Sample Position	99	
* [ III	- <u>N - 2</u>	P.

You can customize the content of the 'Parameters' table by clicking on the applicable button (as you can do with the  $\underline{\sf NMR \ parameters}$ )

ēm	olates				Current Parameters
	Name	Template	Meaning	*	Select a File/Block: METADATA.TXT 🔻
1	📝 Data Path	METADATA.TXT(AcqPath)	Data Path		AcqDate: 2005-02-21T15:55:37
2	👿 Acquired Date	METADATA.TXT(AcqDate)	Acquired Date		AcqPath : C:\DATA\2005\02-February\Ref-Mix-050220_ESI_MSMS02.RAW SampleName : Ref Mix (with dyn excl)
3	Sample Name	METADATA.TXT(SampleName)	Sample Name		SampleID : Vial : 99
4	📃 Sample ID	METADATA.TXT(SampleID)	Sample ID		Instrument :
5	🔲 Task Code		Task Code		Operator : Administrator Comment : Xterra_MS_C18 2,5u 1x50mm
6	📃 Job Code		Job Code	111	Client : Company :
7	📃 Title		Title		Laboratory : ROLLFR9 Phone :
8	Description	METADATA.TXT(Comment)	Description		Study :
9	🔽 Comment	METADATA.TXT(Comment)	Comment		
10	🔲 User		User		
11	V Operator	METADATA.TXT(Operator)	Operator		
12	Submitter	METADATA.TXT(Laboratory)	Submitter		
13	🕅 Instrument	METADATA.TXT(Instrument)	Instrument		
14	👿 Sample Position	METADATA.TXT(Vial)	Sample Position		
15	Laboratory	METADATA.TXT(Laboratory)	Laboratory	-	

### 14.2.4 Context menu


You can access to the context menu just by right clicking on the spectral window:

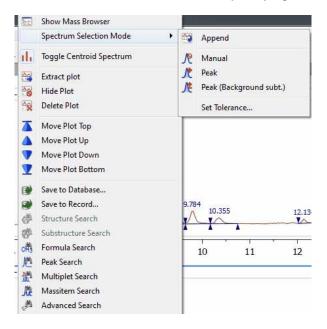

From here you can show the Mass Browser, select the spectrum selection mode, extract the active(s) plot to a new page and hide or delete the plots. You can select several chromatograms or spectra in the same page, for example to extract all of them to a new page. To do it, just hold down the 'Ctrl+Alt' ('Cmd+Alt' in Mac) key and click on the desired plots, next right click and select 'Extract plot'.



It is also possible to freely move up and down the plots just by right clicking on them and selecting the desired option (Move Plot Top, Up, Down or Bottom):

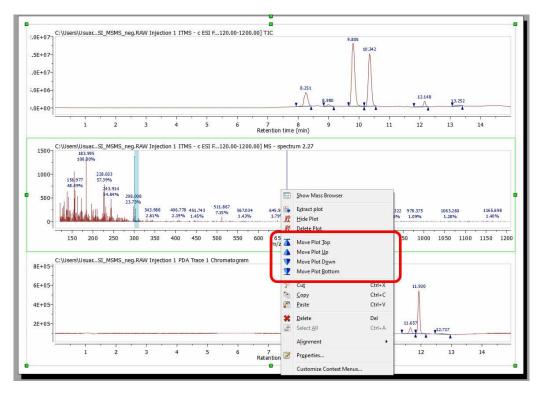

### 14.2.5 Properties and layouts

Mnova allows you to customize nearly all the attributes of the spectrum. You can select the properties of the spectrum by following the menu 'Edit/Properties' or by double clicking the left mouse button or pressing the right mouse button on the spectrum display and selecting '*Properties*' from the *pop-up* menu.

Double clicking on the spectral window will display the properties dialog box. From here you can modify the Line, Title, Peaks, Highlight, Axes and Basic properties of the TIC and MS spectrum by selecting the corresponding tab in the dialog box.

	- 8						
Line Title Highlight Peaks Axes Basic	etadata	Geom	etry Plots	Layout	Mass Sp	ectrum	
	ots: TIC		•				
				1	The second second	C ann ann 1	
Line		Title	Highlight	Peaks	Axes	Basic	
	Line	1999220					
Color: marcon		1000					
			maroon 🔻	·			

The majority of these properties are similar to <u>NMR spectral properties</u>. The most important difference will be in the 'Plots Layout' and 'Peaks' tab.

### Plot Layouts

You can see below the dialog box for the 'plots layout' properties:

<b>-</b>			
Geometry		Plots Layout Mass Spectrum	
Plot Grou	ps		Preview
Layout:	E	Vertical	<u> </u>
Groups:		Description	
	1	Default	
(In the			
et as Defau		Restore	OK Cancel Apply

Clicking on the 'Add new group' button  $\textcircled{1}{2}$ , will allow you to add another plot group. If you click on the new created group (called 'Any plot'), you will be able to select some settings (highlighted in red in the picture below):

eometry Plots Lay	out Mass Spectrum	
Plot Groups	4F	Preview
Layout: 🔚 Vertical		
Groups:	Description	
2 Any plo		2
Add new group		
		11
		Group Settings:
		Layout:
		Constraints:
		Data Type:
		Mass DAD Trace
		Plot Type:
		☑ Chromatogram ☑ MS Spectrum ☑ UV Spectrum

You can select the layout of the group (vertical, horizontal or grids) and several constraints about the Data Type (Mass, DAD or Traces) and Plot Type (Chromatogram, MS or UV spectrum). You can check the boxes for the applicable constraints or combine several options.


In the example below, it is shown how to create plot with 4 new groups. One group (number 5) for any Mass chromatogram plot (with any polarity or order), other group for any Mass spectrum plot with a horizontal layout (number 4), other group for any DAD chromatogram plot (number 3 with vertical layout) and another for any DAD spectrum plot (number 2; UV spectra with horizontal layout). The default group will be used in the case of any other object not present in the other groups.

Geometry		Plots Layout Mass Spectrum	
Plot Grou	ps		Preview
Layout:	E	Vertical 🗸	
Groups:	Ē	Description	
	5	Any mass chromatogram plot	
	4	Any mass spectrum plot	
	3	Any DAD chromatogram plot	3
	2	Any DAD spectrum plot	
	1	Default	2
			Group Settings: Layout: Vertical  Constraints:  Data Type: Mass DAD Trace Plot Type: Chromatogram MS Spectrum UV Spectrum Polarity Order Any

You can download the 'Property' file used above from <u>here</u>. Next load it, by clicking on the 'Load' button of the 'Properties' dialog box and open a MS dataset. Use the <u>MS Browser</u> to display the DAD chromatogram and the <u>crosshair</u> to select the applicable MS or UV at a given retention time in the


chromatogram. To get the additional spectra, you will need to click on the 'Append' button it toolbar.

Here you can see the result with the TIC on top followed by several MS spectra, the Total Absorbance Chromatogram (as a DAD) and several UV spectra:

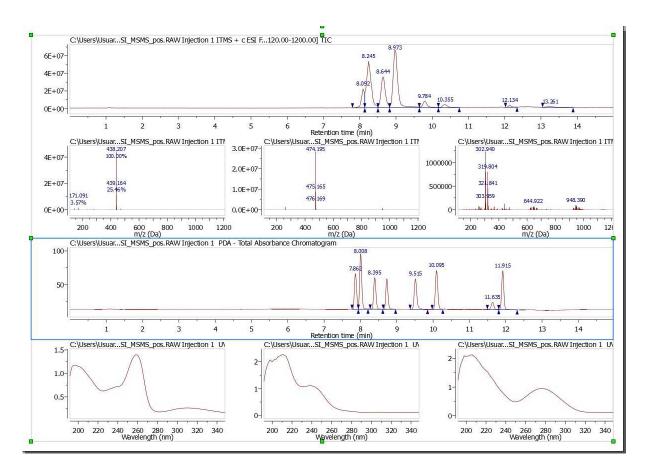

You can load/save and select the plot layout as default by using the applicable options in the 'Properties' dialog box.

You can generate <u>layout templates</u> from your MS documents. Here you can see an example:

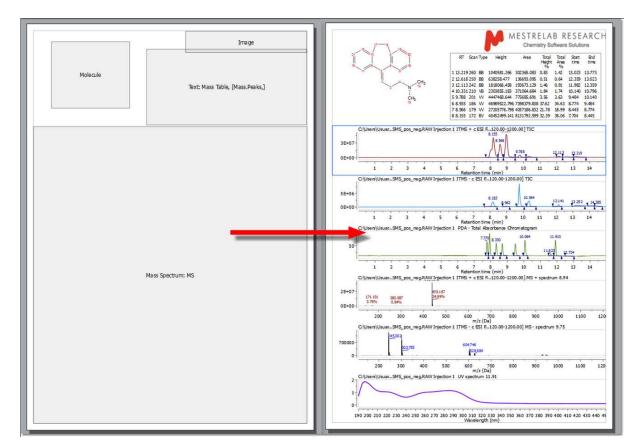

Of course, the layout templates will include the desired 'Properties' embedded, including the selected 'plots layout'. You can see the Properties embedded in a layout template, just by double clicking on each item. Double clicking on the MS box of the layout template will show you the properties of the layout for each plot (spectra and chromatograms):

Geometry	Plots Setup	Plots Layout	Mass	Spectrum
Lin Chr Chr	omatogram 1 • romatogram 1 omatogram 2 omatogram 3	Highlight	Axes	Basic
Mass Spectrum 4 Mass Spectrum 5 UV Spectrum 6 Color:		<b>marc</b>	22.0	
Widt		4.50		


### **Peaks Properties**

You can see in the picture below the 'Peaks properties' of the TIC. From here, you can 'show the wedges' and the 'baseline' (and select the threshold) or add a second line in the peak label, with information about the Intensity, the Height from the baseline, the Area, or the Purity (which will show the integral of each peak as the percentage of all integrated peaks). Please bear in mind that the Area

can not be used as a quantitative value.

adata Geometry Plo	ots Layout Mass Spe	ectrum
s: TIC 🔹	]	
Line Title Peaks	Highlight Axes	Basic
V Peaks		
<u>C</u> olor:	navy	•
MS Shell Dlg 2	Font	
Orientation:	Horizontal	
Decimals:	3	4
Decorations Visibility		
Vedges	Vertical Bounda	ries
🔽 Baseline	💟 Exclusion Regio	ns
Show Second Line La	bel	
Intensity		
🔘 Height		
Area		
Purity		
Decimals:	2	*

Here you can see an example of a TIC with the Purity values in the second line:

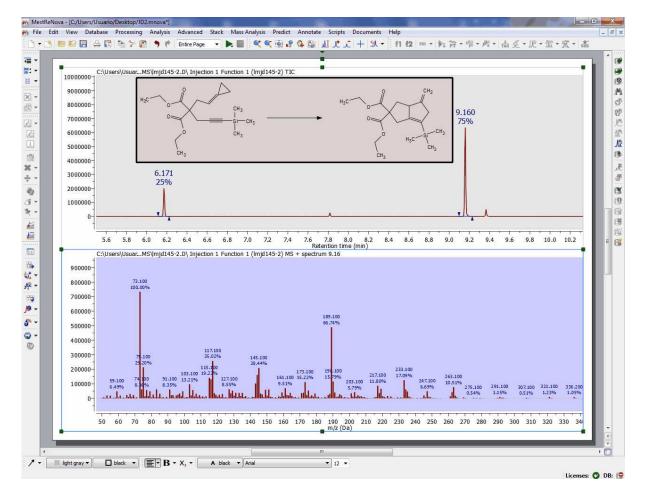

You can see below the 'Peaks Properties' dialog box of the MS spectrum. In this window, you can change the Color, Font and Number of Decimals of the Peak label and you can also show/hide the 'Second Line Label (which can contain information about the 'Intensity' or the 'Relative Abundance').

tadata Geometry Plots: MS + spectrum 1,12 💌	ots Layout M	lass Spectrun	n
Line Title Peaks	Highlight A	xes Basi	c
Color:		navy	
MS Shell Dlg 2		Font	
Orientation:	Horizontal	1	2
Decimals:	3		
Threshold:	0.50% of	Мах	A THE O
Show Second Line La	ibel		
Intensity			
Relative Abundance	2		
Decimals:	2	0	A V

From 'Properties/Peaks' dialog, it will also be possible to change the orientation of the peak labels (horizontal/vertical).


Selecting Title in the tabbed menu, will display the below window:

etadata Ge	ometry F	Plots Layout	Mass S	oectrum
ots: MS + spec	trum 1,12	•]		
revel lesses		-		
Line Title	Peaks	Highlight	Axes	Basic
Title				
<u>C</u> olor:				1
MS Shell	Dlg 2		Font.	
Decimals:	3			E
		,32,m} {funcl		lesc}

Clicking on this icon 🗔 will allow you to customize the format of the title; for example to display the 'RT' or 'Scan ranges' or to select the number of characters (Max Length; 32 by default) or the position (n: none, l: left, r: right, m: middle):

ext			QK
{file,32,m} {injN,32,m} {funcN,32,n	n} {desc}		Cancel
dd Macro			
<b>_</b>			
<b>1</b>	_		
wailable Macros:	Parameters:	autore de la companya	
Description	Name	Value	
File	1 Max Length		
Function Index			
Function Name	2 Position		
Function Polarity			
Injection Index			
Injection Name			
Order			
Precursors			
RT ranges			
Scan ranges			


Here you can see an example of a TIC and MS after having changed some properties:

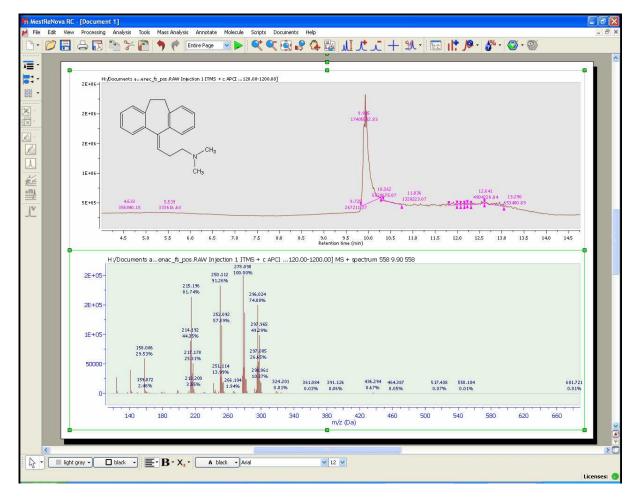

Line	Title	Highlight	Peaks	Peak Purity	Axes 🖣	
H	orizontal	Common	Vertical	lan l		
	Primary Ti Secondary		Auto -			

Selecting the Axes tab will allow you to change the Units individually for each plot:

If you want to change the units for all the Mass spectra, youy would need to use the context menu (by right clicking on the vertical axis):

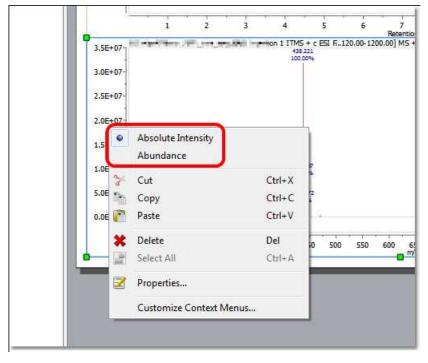

**Label:** When the default box is checked, it means that the label will be set by Mnova to the default value for that kind of plot (so the label line editor remains disabled). If it's unchecked, then the label will be set to whatever the user sets in the line editor.

The default values are: <u>Horizontal axis:</u> Mass spectrum: m/z (Da) UV spectrum: Wavelength (nm) Chromatogram: Retention time (min)

#### Vertical axis:

Mass spectrum: Intensity

UV spectrum: Absorbance

Chromatogram: If the current data provider, provides an axis label, that will be used. If not, either Absorbance or Intensity regarding if it is a UV chromatogram or any other kind of chromatogram respectively.

You can read more about general Mnova properties here.

### 14.2.6 Preferences

Follow the menu Edit/Preferences/Mass to change your MS preferences:

1	-	-		ale
General	Plug-ins	Database	NMR	Mas
General Saving Op	Setup Ver	ify		
Item <u>C</u>	<u>2</u> nly			
Ttem 8 Your choic		ly to newly impo	rted items.	
Scales Beh	0V 22			
V Fit to F	Height After Zo		Scale	

The user will be allowed to select the saving options (item only or item+dataset).

You will find also an option to fit to height after zoom (selected by default). When this option is checked, a fit to height is applied after making a horizontal zoom in a mass spectrum or a chromatogram. In case of the other zoom modes (vertical or in both dimensions), a fit to height is never applied.

When the option 'Synchronized chromatogram's Time Scale' is selected, you can zoom, pan and cut to all showing chromatograms.

It is possible to choose which chromatogram and spectra are displayed when loading an MS dataset via Edit/Preferences/Mass/Setup. This mass setup will be stored when saving the preferences:

eferences	3	-			8
General	Plug-ins Database	NMR Mass	Molecule	Scripting D	rawing Tools
eneral	Setup Verify				
	hich data to show when loadi MSC 200.0000 m/z	ng a new mass item			•
	m Dialog		3	×	*
	Plot Type: Mass Chron Injection Ist Trace Chron DA Chroma Trace Chron DA Spectru	natogram trum itogram matogram			
	Mass Function	Mass function of 1st	🗢 order		
	Mass Chromatogram: Type: TIC	•			
				Load.	Cano



# 15 Mnova Database


This plugin is not included in Mnova Suite. If you want to try it, please email us to support@mestrelab.com

This new plugin of Mnova was born as a new concept to the shared storage for molecules, Mnova objects (texts, drawings, images, etc...), NMR and MS analysis data.

Please bear in mind that you will also need a server to store your databases. You will find <u>here</u> the instructions to set up that server. See also <u>this video</u> for further information.

## 15.1 Create a Database


If you do not have any previously database, you will need to create one. To do it, just follow the menu 'Database/Create Database':



For further information about it, please go to this chapter.

# 15.2 Connecting to the Server

Firstly, you will need to connect with the database server by following the menu 'Database/Connect' (or by clicking on the applicable icon of the toolbar <sup>[1]</sup>) and entering the corresponding password:

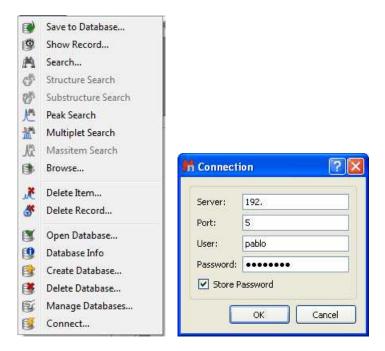


If you do not have any Database created, you will need to create one. In that case, please go to the applicable <u>chapter</u>.

# 15.3 Saving items to Database

You will find the quinine datasets in the installation folder of Mnova (under the examples/datasets folder)

It will be really easy to add objects (spectra, molecules, etc...) to a database; just open your Mnova document (containing for example a 1H-NMR spectrum, a molecule and some objects) and follow the menu 'Database/Save to Database' (or click on the applicable icon of the toolbar, highlighted in red in the picture below)

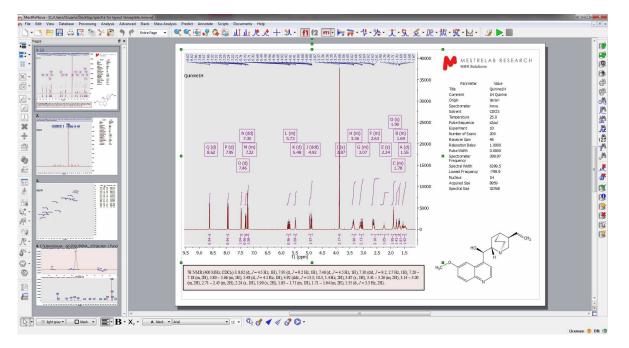

You can also 'Save to Database' by right clicking on the spectrum to display the spectrum context menu.

After having selected 'Save to Database', you will get a new dialog box where you will see how the spectrum and the molecule are selected by default to be added to the database. If you want to add also the other objects, you will need to check the corresponding boxes or click on the 'All' button. (Please bear in mind that it will not be possible to save more than one molecule for each spectrum):


I		r. P			
lect		Page	Туре	Preview	Description
None	1	1	Molecule	-136 m	
All	2	1	NMR Spectrum	11-11	Quinine1H
	3	2	NMR Spectrum		Quinine 13C
	4	3	NMR Spectrum	and a	Quinine HSQC
	5	4	Mass Spectrum	و حد	MS + spectrum.
	6	1	Text	200000000000000000000000000000000000000	1H NMR (400
	7	1	Image	M 11/111.43 -1111.41 -1	Image
	8	1	Text	- fi	
	9	2	Text	2000 State Common Science	13C NMR (101
	10	2	Text	T	
	11	3	Text	1	

Once you have done the selection just click on OK to save to the database. During this procedure, Mnova will check the database to find similar spectra or molecules.


If your dataset is new in the database, you will only get a 'Save Complete' message and your dataset will be added to the database:



If it finds a match during the saving procedure, it will ask you to add the new items to the compound (to avoid duplications). for example imagine that you want to add the 13C NMR spectrum of the 'compound 1' (quinine in this case) to your database.

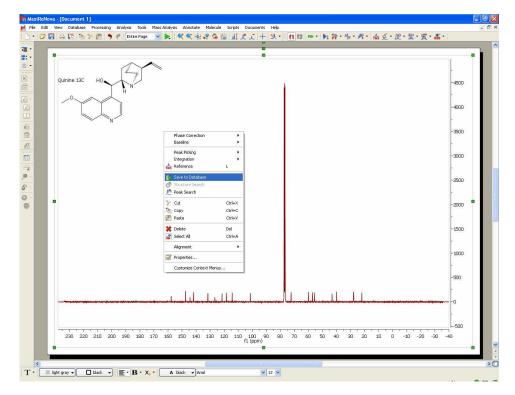

In that case, Mnova will find a compound with the same molecule structure, so you will only need to check the OK button (highlighted in red in the picture below) to add the new spectrum to the compound 1 of the database:

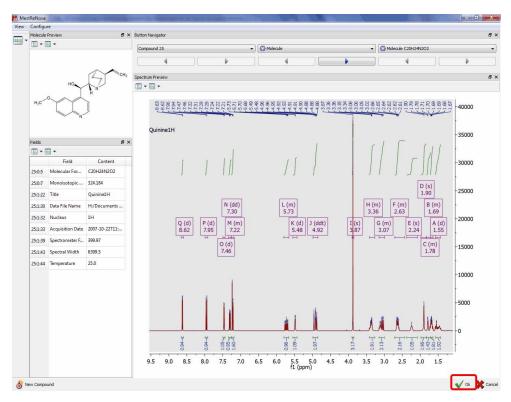

After having clicked on the OK button, a new dialog box will be displayed to ask you whether to add or


replace (when existing	items have been found	I matching those being saved):	

Add Replac		ce Ignore		Skip	Abort
Add All Repla		e All 🛛 🗌 Ignore All			Hide Details.
			Current	Replace With	
Atoms		23.0		23	
Bonds		26.0		26	
MoleculeId		{8aebeaa5-9f5e		{8aebeaa5-9f5e	
CHEMICAL S	TRUCTURE	88.5254 -64.7 1 2 1 0 0		1210000	
Molecular Fo	rmula	C18H24O2		C18H24O2	
Average Mass		272.382		272.3819599999	
Monoisotopic Mass		272.178		272.17762999999	
Uuid		{7fe8fb4b-d763		{7fe8fb4b-d763	
Туре		Mole	cule	Molecule	
Text				-	
Preview			.cuff	CTIT	
User		Pablo		Pablo	
Host		MESTREPABLO		MESTREPABLO	
Document		C:\Users\Usuari		C:\Users\Usuari	
Created		vie 16. abr 08:19		vie 16. abr 08:22	
Modified		vie 10	5. abr 08:19	vie 16. abr 08:22	
MNova Versio		6354		6354	

If for some reasons, you do not want to add the 13C spectrum to the compound 1, just click on the 'New Compound' button (left-bottom side of the screen).

You can add 2D NMR or MS datasets to the database. In the case of 2D datasets, if the file size is too big, we recommend to use the <u>'Compression'</u> feature (under the Processing menu) before uploading the experiments to the database.

If your document contains more than one compound and several molecules are selected for saving, a warning message will be displayed:



When the user chooses to continue, several records (one for each selected molecule) are created in db and each of the records will contain all of the selected spectra.

# **15.4 Displaying database contents**

In this chapter you will find information about how to display the content of your Database.

## 15.4.1 Operations

Once you have created the database, you will be able to search for any record just by using the 'Show Record' or the 'Browser'.



# **Show Record**

This feature will allow you to find compounds by using their ID. The first record added to the database will have the ID number 1; the second record will have the ID number 2 and so on:

Show Record	rd 😵 📂
Record ID	
5	•
ОК	Cancel


### **Browser**

The Browser will allow you to show a range of records:

Record	s	
From:	þ	A V
To:	187	×


### 15.4.2 Searching in the Database

You can use the applicable commands to search 'structures', 'substructures', 'formulas', 'peaks', 'multiplets', 'Massitems', 'numbers', 'texts', etc':



## **Structure Search**

You can search for any molecular structure in the database by right clicking on the molecular structure (or highlight the molecule and follow the menu 'Database/Structure Search') and selecting 'Structure Search' (which will display the Query Editor). Click on OK to run the search.



From here, you will be able to run also Substructure searches just by checking the applicable box.

Clicking on the 'Convert to advance query' button is will allow you to convert it to an advanced search so that you can add new queries and combine them.

You can also see the mol file as plain text, by selecting the applicable option in the 'Select Display Mode' scroll down menu:

Molecule Q													. M
1967	fault	-											27
- 10 C	olecule	P											
Te:	đ	0999	V20	000	)								
7.1354	0.2303	0.0000 C	192	100	0	100	0	100	0	12	87	12	0
7.1334	7.0598	0.0000 C	100	0	0	0	0	0	0	0	35.	0.75	0
8,5597	6.2363	0.0000 C	100	0	0	0	0	0	0	0	0	1.5	0
7.8445	7.4747	0.0000 C	0	0	0	0	0	0	0	0	0	1.25	0
6.4223	7.4747	0.0000 C	0	0	0	0	0	0	0	0	0	0	0
9.2729	5.8235	A 0000.0	0	0	0	0	0	0	0	0	0	0	
7.8445	8.3043	0.0000 C	0	0	0	0	0	0	0	0	0	0	0
8.5557	7.0598	0.0000 C	0	0	0	0	0	0	0	0	0	0	0
6.4223	8.3043	0.0000 C	0	0	0	0	0	0	0	0	0	0	0
5.7111	7.0598	0.0000 C	0	0	0	0	0	0	0	0	0	0	0
9.9861	6.2363	0.0000 C	1.50	0	0	0	0	0	0	0	0	0	0
9,2729		0.0000 C	1.1	0	0	0	0	0	0	0	0	1.75	0
7.5482		0.0000 C	100	0	0	0	0	0	0	0	8 F.	~	0
Q 5557	g 7101	0.0000.0	0	0	0	0	0	0	0	0	0	0	0
Substr	ucture												

This button will allow you to select which molecule you want to search in the case that you have several molecules in the same document.

After having clicked on OK, Mnova will search for the molecule in the database.

• If the molecule is not in the database you will obtain this message:




• If the molecule structure is stored in your database, Mnova will show you the information which appears in the database about this compound. For example, imagine that you load the molecule structure of the quinine and you select 'Structure Search'. In that case, you will obtain a window like this one (with a Match Score of 1000 which is the maximum value):


Molecular Structure Query	Select search results Hits: 1/3 Records: 1/3				None	All
1/2-20	Database	Record	Item Type	Item Number	Field	Score
	1 NMR_MS_October_2010	3	Molecule	0	CHEMICAL STRUCTURE (4)	1000
H <sub>5</sub> C <sup>-1</sup>						
10 11 12 N 14						

Note: Clicking on the Copy to database button, will allow you to copy the result to another database. Clicking on the 'Rerun Query' button will allow you to refine your search.

Click on OK to get a similar window like the one below:

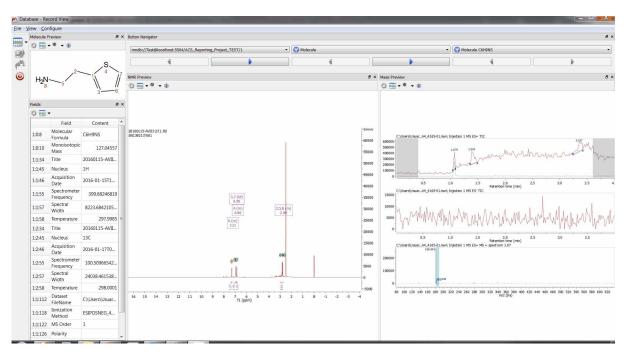

Please bear in mind that you can also see the any other spectrum (such as a 13C NMR) if we have previously added to the database, just by clicking on the 'blue arrow' (highlighted in red in the picture above):

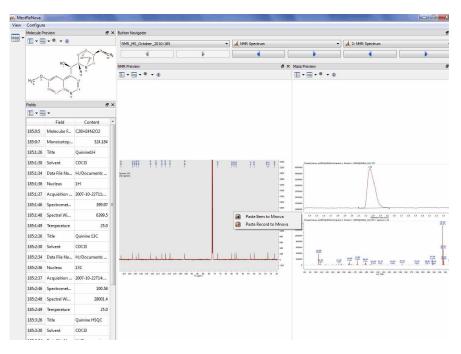


You can also copy the spectra or the molecules to a Mnova document just by double clicking on it (or right clicking and selecting 'Paste Record or Item to Mnova').


You can also use generic atoms like R (any chain, except H, D and T), Z (any chain; including H, D and T), A (any atom, except H, D, T), X (any halogen), Ht (any heteroatom) in the molecular structures. For example, to search for alcohols or amines, draw the corresponding group (and anything else you want the results to contain), add Zs (Z-NH<sub>2</sub>, Z-OH), and do a structure search.

Here you can see an example to find compounds containing C=C double bonds:

If you want for example to find compounds with at least four C=C double bonds, you can draw this:

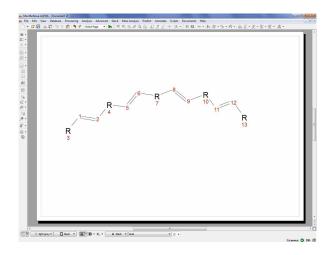

If you wan to search for ketones, you can draw this molecular structure:

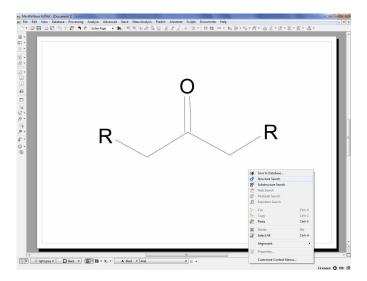

## **Substructure Search**

The SubStructure Search feature is used to locate products by chemical structure. Simply copy a structure fragment, right click on it and select 'Substructure Search':

Image: Server to Database         Structure Search         Multiplet Search         Image: Conject Conject         Search         Dela         Alignment         Image: Control Menus	🎢 🅈 🥐 Entire Page 🔹 📐	(大山 盛みな通び	+	以 <b>、 f1 f2</b> n	n •       1 =    1 = 1	8×興×南≰×伬×	监 • 戎 •   志 •   団   勁 屿
2 Properties		N	· · · · · · · · · · · · · · · · · · ·	Structure Search Substructure Search Multiplet Search Cut Copy Paste Delete	Ctrl+C Ctrl+V Del		
Customize Context Menus					,		
				Customize Context N	Ienus		

In that case we have obtained three hits (for the records 5, 10 and 25):

None		Compound	Item Type	ltem Number	Field	Score
All	1	5	Molecule	0	CHEMICAL STRUCTUR	1000
	2		Molecule		CHEMICAL STRUCTUR	1000
fits: 3/3 Compounds: 3/3	3	25	Molecule	0	CHEMICAL STRUCTUR	1000

You can also use generic atoms like R (any chain, except H, D and T) ,Z (any chain; including H, D and T) ,A (any atom, except H, D, T) ,X (any halogen) ,Ht (any heteroatom) in the molecular structures. For example, to search for alcohols or amines, draw the corresponding group (and anything else you want the results to contain), add Zs (Z-NH<sub>2</sub>, Z-OH), and do a substructure search.

## **Formula Search**

This feature will allow you to search for any specific molecular formula of your database. To do that, just type the molecular formula in the 'edit box' and click on OK. You can restrict (it is not mandatory) the search by using the 'ItemType' and 'Field' options:

Query Editor	8
Search for Molecular For	mula:
C20H24N2O2	•
Restrict	
Itemtype:	Ŧ
Field:	· •
ОК	Cancel

The format for a **molecular formula search** is quite flexible. It can be explained with some examples:


- If you type: C1,4 H3,8 N1,1; the program will search for molecular structures with 1 to 4 carbons, 3 to 8 H and exactly one N; other elements are allowed but not necessary. Note that spaces can be omitted.
- Elements can be in lower case, as long as there are not 2 without space, so "c1,4h3,8n1,1" would be OK, whereas "c4,7no" is not, since "no" will be interpreted as "No".
- Ranges can be omitted, so "C" is the same as "C1,1", "C3" is the same as "C3,3", "C,4" is the same as "C1,4" and "C2," is the same as "C2,8"
- The meta symbol "HT" can be used for hetero atoms, "X" for halogens, and "!" (exclamation mark) at the end of the formula to only allow specified elements. Thus, "C1,4 Ht3" searches for 1 to 4 carbons and exactly 3 hetero atoms, whereas "C3,5 H6,10!" would search for hydrocarbons with 3 to 5 C and 6 to 10 H.

### **Peak Search**

If you have a spectrum loaded in Mnova (this is not mandatory) and you select 'Database/Peak Search' (or right click/Peak Search'), the application will look for these peaks in the database. If you have expanded any area of the spectrum, it will only look for the peaks of the expanded area (and not for the whole spectrum). Please bear in mind that if you have forgotten to apply the Peak Picking to the expanded area, Mnova will do it (by using the automatic Peak Picking).

Quinine1H		-7.99 		~7.49 ~7.48	L734 L733 R732 R731 R731 R724	-13000
						-12000 -11000 -10000 -9000
	Reference	L	r		T.	-
	Save to Databa	:h				-8000
	Substructure S     Peak Search	earch				
-	Multiplet Searc	:h				-6000
	⊁ Cut	Ctrl+X			1	1
	Сору	Ctrl+C		1.		-5000
	Paste	Ctrl+V				-4000
	Delete	Del Ctrl+A				
						-3000
	Alignment	•				-2000
	Properties					2000
	Customize Cor	ntext Menus	]			-1000
J.		M		<u>M</u>		
						-0
						1000
8.7 8.6 8.5 8.4 8.3	8.2 8.1	8.0 7.9	7.8 7.7	7.6 7.5	7.4 7.3 7.2	
		f1 (ppm)				

After having selected the Peak Search feature, the Query Editor dialog box will be displayed:

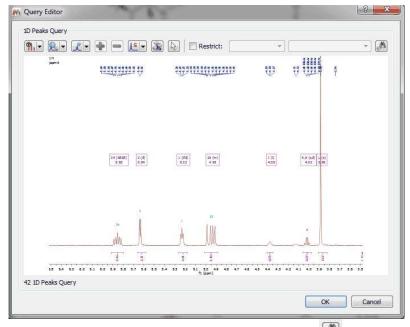

Clicking on the 'Convert to advance query' button is will allow you to convert it to an advanced search so that you can add new queries and combine them.

In the dialog box above, you will find a toolbar with different buttons: 🐘 🖭 🗶 🖝 📼 💵 🗟

- Select Display Mode: it will allow you to show the peaks table or the spectrum preview
- Peaks: to show 'All Peaks' or only 'Visible Peaks' of the expanded region
- Select Peaks by Compound: to search only for some specific compound peaks
- Add/Remove: To add or remove peaks from the table

#### • Purity/Mixture/Reverse:

١	
E	Purity
LE	Mixture
<u>ال</u>	Reverse

The peak and multiplet search dialogs have a tool button for changing the search mode. The default mode is "Reverse", which penalize peaks which are in the query but not in the db spectrum. The default mode can be set in the user preferences.

The scoring by using 'reverse search' assumes that the sample is one compound and is based on how well a stored spectrum fits the total query. Peaks or multiplets that are in the query, but not in the stored spectrum, count against the score. This works well for spectra composed primarily of a single compound, but can lead to problems and excess "bad" hits when searching against a mixed sample. Another way that would be useful for binary, tertiary, etc. type mixtures would be a "content" score in which any potential hit is scored based on how well it's peaks compare back to the queried spectrum. To get a "1000" for a "content" score all peaks in the stored spectrum must be present in the queried spectrum, but there is no penalty for extra peaks in the query spectrum. It is almost a reverse grading of the spectra

For example: If you have a ~50:50 mixture of compound A and compound B and run a query, you get what would be approximately a "500" scores for both compounds using the traditional scoring method. If you were to additionally display the scoring method proposed above, each stored spectrum would get "1000" scores for a "content" grade. This way of scoring would better indicate the presence of particular compounds in the analyzed sample. This would also additionally help to completely rule out compounds that get low grades in the traditional scoring method, but show up in the scoring due to coincidental overlap of multiplets/peaks.

Purity Search: unclean spectra in the db (with many spurious peaks) will get low search scores.

Mixture means that peaks in the query spectrum but not the library spectrum will be ignored. This is for cases where the query spectrum might be a mixture containing additional compounds.

#### • Parameters: to set the 1D Peak Search Tolerances


1D Peak Sea	rch Tolerances
Position:	
1H:	þ. 10 ppm ≑
Other:	1.00 ppm 🌲
Width:	1.00 🌻
Intensity:	1.00 🔹
ОК	Cancel

• Select from document: to select the spectrum if you are in a document with several datasets.

After having clicked on the OK button, the peak search will be run. In the example below, we have obtained a match for the compound number 25, with a score of 1000 (maximum value):

None		Compound	Item Type	Item Number	Field	Score
All	1	25	Spectrum	1	Peaks1D (18)	1000
lits: 1/1 Compounds: 1/1						


The Peak Search feature (combined or not with the Verification plugin) can be very useful to identify impurities in the datasets.

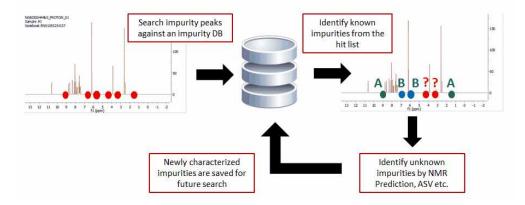

Please note, that you can also use the 'Peak Search' feature without any spectrum loaded. In that case, you will need to type in the table, the information of the peaks that you want to find in your database:

							-
	f1 from	f1 to	Width from	Width to	Intensity from	Intensity to	
1							

Alternatively, you can also use the 'Peak Search' feature from a molecular structure with assignments:

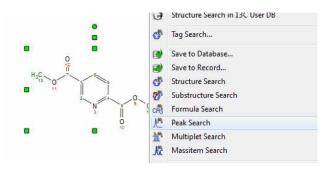


If your spectrum has more than one compound, you can run peak searches of only one of the compounds:


9 <u>R</u> - (			🔝 🛛 🕅 Restric	:	-	7	9
tH a jams s	All Primary Sc Secondary Any Solver EtOAc Quinine	Solvent			W		
2	(d) 38	(ad) (a)	G (t.ds) 5.44	22'(m) 319 300	15'(dd) 2.54	121(227)(840) 2.42	
		uli	<u>"M</u>	Ah		NN NN	
			5		\$	· · · · · ·	
•3 •4 57 1D Peaks Quer			18 3.3 3.4 3 (1.(ppn)	1 11 11 11	2.5 2.8 2	7 23 23 2A 23	

## **Multiplet Search**

To search for multiplets, you will only need to open a spectrum with the desired multiplet analysis and finally select 'Multiplet Search' (after having right clicked on the spectral window):

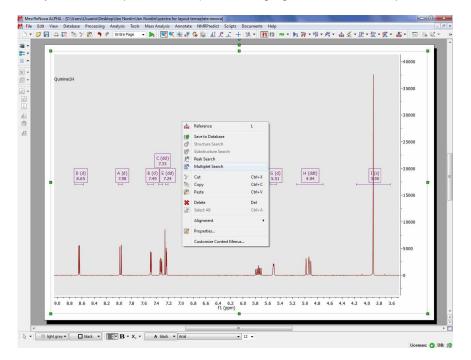


After that, the query editor will be displayed, to how you which multiplets will be searched. This dialog box is similar with the 'Peaks Query Editor' (explained above)

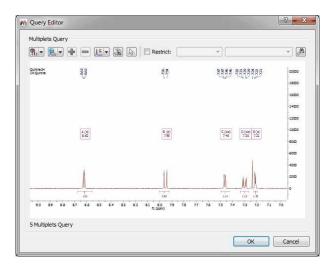


### Mass Item Search

If you have a MS dataset loaded in Mnova and you select 'Database/Massitem Search' (or right click/MassitemSearch' or by clicking on the icon of the toolbar), the application will look for these MS peaks in the database.

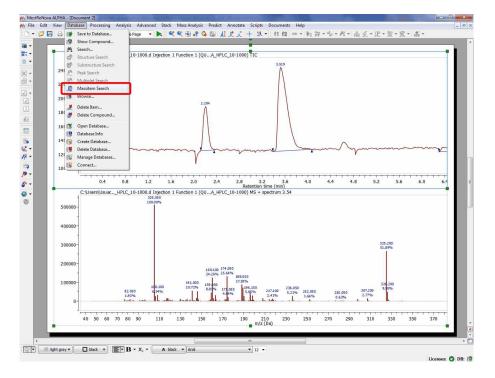

After having selected the 'Mass Item Search' feature; the query editor will be displayed:

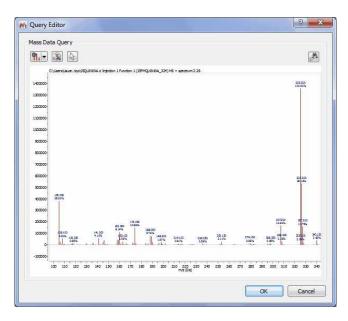

From here, you will be able to change the view (preview or plain text), or to select the tolerance of the Mass Item Searches.

Finally, click on the OK button and wait for the result:

stken	ova				
	figure				
	cule Preview	6 ×		MR Preview	ð×
	• 🔳 •			<b>□ • ⊞ •</b>	
		2 20 19 224 CH2			40000
		HO N IS			35900
	0	H 17 16			30000
	H <sub>3</sub> C *	5 16 		1	25000
	102	11 12 N 14		Middle         Supp         <	20000
Butt	on Navigator	6 ×	1	N(d) 246	15000
Ce	impound 1 🔹	Molecule			10000
	4 ] [ • • ] [				
Field	\$	6 ×	1		\$2.00
	- 📰 -			ALLAAAAAAAAAAAAAAAAAAAAAAAAAA	
	Field	Content			
1:0:	5 Molecular Formula	C20H24N2O2		9.8 6.5 6.0 7.5 7.0 6.5 6.8 5.5 <u>5.0</u> 4.5 4.0 3.5 3.0 2.5 2.0 1.5	
1:0:	7 Monoisotopic Mass	324.184	Mass I	ass Preview	ð×
1:1:	25 Title	QuininelH		□ • Ⅲ •	
1:1:	29 Solvent	CDCI3		Cl/seer(Inser, _1PLC,10.1003.d legetor 1 Function 1 (QLLA, 1PLC, 10.0000) TIC 2.2m	
1:1:	33 Data File Name	C:/Users/Usuario/Desktop/Quinine1H/fid		20000-	
1:1:	35 Nucleus	1H		200000-	
1:1:	36 Acquisition Date	2007-10-22T10:21:46		180000-	
1:1:	45 Spectrometer Frequency	399.97		second A	
1:1:	47 Spectral Width	6399.5		120000	E.
1:1:	48 Temperature	25.0		0.4 0.8 1.2 1.6 2.0 2.4 2.8 52 3.6 4.0 4.4 4.8 5.2 5.6 4.0 Reset Time Junit	
1:2:	25 Title	Quinine 13C		C(Liter)(Incore, LHPL), 10:1000 d Septime 1 Function 1 (QLLA, HRUC, 10:1900) MS + spectrum 1.14 30.000 30.000	
1:2:	29 Solvent	CDCI3			
1:2:	33 Data File Name	C:/Users/Usuario/Desktop/Quinine 13C/fid		30000 Store	
1:2:	35 Nucleus	13C		20000 In 10 19 19	
1:2:	36 Acquisition Date	2007-10-22T13:02:47		5435 20% (mast) (1000) 10000 1000 10000 10000 1000 1000 1000 10000 10000 10000 10000 10000 10000 100000	
1:2:	45 Spectrometer Frequency	100.58		e the second state of the	
1.2			1	+6 56 66 76 66 74 110 139 150 170 210 220 239 290 270 290 310 339 350 3	179

NOTE: The Database definition within the MassItem, will include information about: RT, Scan, Type, Height, Area, Total Height %, Total Area %, Start Time, End Time, for each chromatographic peak corresponding to that particular MassItem in each Chromatographic run. The database definition accommodates up to 8 traces (TIC, Total UV (or DAD or PDA), ELSD, CNLD + 4 UV traces as specific wavelengths).

# **Retention Time Search**

The 'Retention Time Search' will allow the user to enter a range of retention times and choose to work within the 'RT', 'Start time' or 'End time' fields of the DB, within the Itemtype MassItem.

Query Editor		
Retention Time Q	luery	
Search for:		
RT:	8.48	A. V
+/-:	0.10	A V
Chromatogram:	Any	+
Time:	Any	
rime.	TIC	
	UVT	
ОК	CNLD	
	UV	

### **Numeric and Text Search**

You can search for numbers or for any text in the database just by selecting one of these options:


Numeric Query	Text Query
Search for numbers:	Search for text:
0	*
Restrict	Restrict
Itemtype:	Itemtype:
Field:	Field:
OK Cancel	OK Cancel

Please bear in mind that the numeric search can contain ranges like "10 < 20" or "10.2 <= 20.5".

To search for all the items of your database, type "-" (without the quotation marks) in the search dialog.

## **Advanced Searches**

This option will allow you to combine several queries (in the same document) for the same search. In the example below, you can see how we are combining the peaks of 1D and 2D NMR datasets with the Mass spectrum.

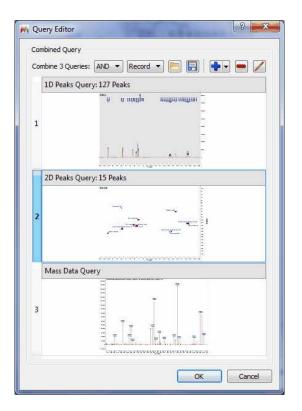

You can look for any of the 3 queries (by selecting '*OR*' in the applicable scroll down menu) or for all the queries (by selecting '*AND*'). You can also load/save combined queries in XML format, or to add/remove/edit the queries by using the applicable buttons of the dialog box.

The settings specifies how the search results from the subqueries are combined into the single result of the advanced query.

Let A be the results returned by subquery a, and B the results returned by subquery b. Let R be the final search scores of the advanced query. Then, With Combinator = "AND", score(R) = min(score(A), score(B)) With Combinator = "OR", score(R) = max(score(A), score(B))

With combination = records, A and B must be matches within the same record for the subquery results to be combined.

With combination = items, A and B must be matches resulting from the same item (in the same record) for A and B to appear in the final result.

So, with your advanced query where for example subquery a="1D Peaks>2" and subquery b="1D Peaks<3", when you select combinator "Records", you will get matches for records which may contain one msitem with 1D Peaks 5 (5>2, match for a) and another msitem with 1D Peaks 1. (match for b). When you select combinator "Items", these matches are excluded as A and B need to occur in the same item for the match to appear in the final result, so you will only get items where both conditions hold true for the same item, which is in effect msitems with both 1D Peaks>2 and 1D Peaks<3.

Combinator "Records" is useful if you want to combine conditions from different items, for example: search for records where "Methyl" appears in the molecule name and which have an NMR spectrum with 1D Peaks between 1 and 3.


# 15.5 View Results

Once you have searched your items in the database, you will get this view by default with the results:


ecule	Preview	5>	MMR Preview d	X	Scores				
2 111	• ® • ®		0 m + 0 + 0		ŵ	0			
			200401544CD222.06 54L352.3701 6000		Î.	Record	Item Type	Item Numbe	HEMICA I RUCTUE
		,S	3000		1	mndb	Molec		
		2 4 7	3001		7		Molec		21.50
Ho	N-		400		13		Molec		dia
4	8 5	\\ //	400		18	mndbr	Molec	00	1
		3-6	3,7 (0) 6.00		24	mndbr	Molec	00	20
ids		8 >	1 (1) (1) (1) (1) (1) (1) (1) (1)		29	mndbr	Molec	00	50
1	•		232		35	mndb	Molec	00	09-0
	Field	Content	2008		41	mndbr	Molec	00	
0.8	Molecular	C6H9NS			47	mndbr	Molec	00	e5
	Formula Monoisotopic		900		53	mndbr	Molec	00	20,
0:10	Mass	127.04357			59	mndb	Molec	0 0	1.20
:34	Title	20160115-AVIII-27.1.fid			65	mndbr	Molec	00	103
1:45		1H	аанаааа т <sub>аро</sub> учууну чуунучучу		71	mndbr	Molec	0	124
1:46	Acquisition Date	2016-01-15T16:30:00	Mass Preview d	×	76	mndbr	Molec	0 🖸	1.572
1:55	Spectrometer	399.68246819	C/UserSUsser, Ad., 5159-01, evol. 1465 ED: TC		79	mndb	Molec	0 🖸	
	Frequency		10000 MM		83	mndbr	Molec	🖸 0	
1:57	Spectral Width	8223.6842105263	1 Now Marken Marken		89		Molec		
L:58	Temperature	297.9985	22000- 12000-		95	mndbr	Molec	0 🖸	-80
234	Title	20160115-AVIII-27.2.fid	0 0.5 1.8 1.5 Research received 2.5 3.0 3.5 4			1 mndbr			1024
545	Nucleus	13C	Clumifumer. A4_4505-01.nev( treater 1 He 16-170 1999)			7 mndbr			de.
46	Acquisition	2016-01-17003-17:00	1000			3 mndbr		-	1010
rγ		87	200 March 1990 Martin All and Anna Anna Anna Anna Anna Anna Anna			9 mndbr			
			1 A.A. C. C. A. MACH. C. MAAAAA MAAAAAAAA MAAAAAAAAAAAAAAAAA			5 mndb			10-02
			0.5 1.8 1.5 assessor tree (ma) 2.5 3.8 3.5			1 mndb			0.01-
			C/UberfUbace.A4, 6059 D Level. Tigetten 1 MS ES= MS + spedner L07 190 m)			7 mndbr			0-0-
			20000			3 mndbr			-14S
			10000			9 mndbr			.2.9
			6			4 mndbr			-\$6,
			80 100 120 146 146 146 146 240 200 200 240 246 146 100 120 340 240 440 460 490 500 500 500 500 460 450		16	0 mndbr	Molec	O O	det.O

As you can see, you will get the molecular structure, a table with several fields, the query window, spectral views and the item list to change the compound or the spectrum of the preview (just by clicking on the applicable item of the list).


You can add new widgets to the 'Search Results View' by following the menu 'Configure/Add Widget'.

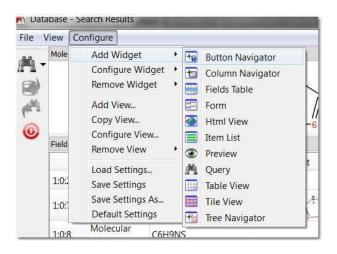


You can select the desired fields to be displayed by clicking on the 'configure button' en by following the menu 'Configure/Configure Widget/Fields' and checking the desired fields from the list:

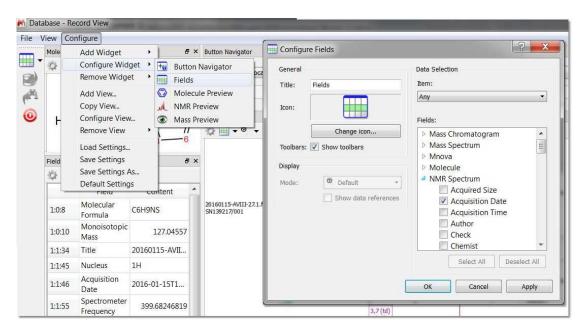


This is the template called 'Search Result', but there are several templates by default which you will find by following the 'View' menu (or by clicking on the 'binoculars' scroll down menu):



Here you can see for example the 'Record view', with information about molecular structure, a table with several fields, a spectral view and a button navigator to change the compound or the spectrum of the preview.

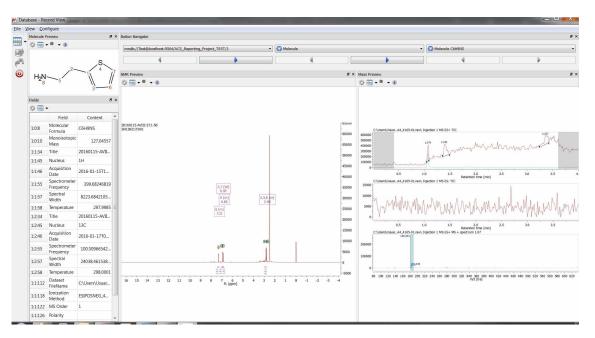


Here you can see the Table view, with information about the compound ID, molecular Formula, Molecular Preview, Title, Solvent, Nucleus, Frequency and Spectrum Preview.

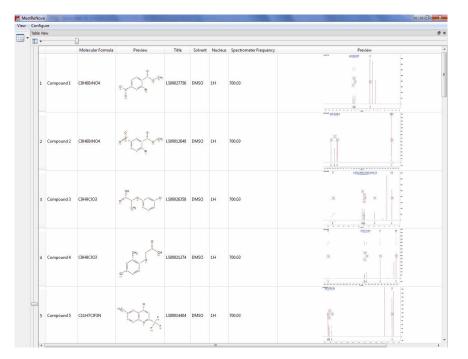

Of course you can add additional information to the table view just by following the menu 'Configure/ Configure Widget/Table View' and checking the applicable fields from the list:

Add Wid	lget 🕨		Configure Ta	ble View	? <mark>- X</mark>
Configur	e Widget 🔸	Table View Spec			
Remove	Widget 🔸 🗍	Mass Data Polarity	General		Data Selection
Add View	N	Į	Title: Tab	le View	Item:
Copy Vie	:w				
Configur Remove			Icon:		Fields:
Load Set Save Set	tings		Toolbars: 📃 :	Change icon Show toolbars	Mass Chromatogram     Mass Spectrum     Mnova
	tings As	1	Display		▷ Molecule
Default S	Settings	I MARINE I	Mode:	🕲 Default	MMR Spectrum
mndb://Test				Show data reference	Acquired Size
nndb://Test	1	il	Row height:		Acquisition Date
nndb://Test			Column width:		Author
mndb://Test	1	<u>.</u>	Column wider.	100	Check
nndb://Test					Chemist 👻
mndb://Test	1	Į.			Select All Deselect All
nndb:// <mark>T</mark> est					OK Cancel Apply
nndb://Test	1	Į			
mndb://Test					13C
mndb://Test	1		8	200 C6H4	4N2OS 152.004434 1H


You will find below the HTML view:

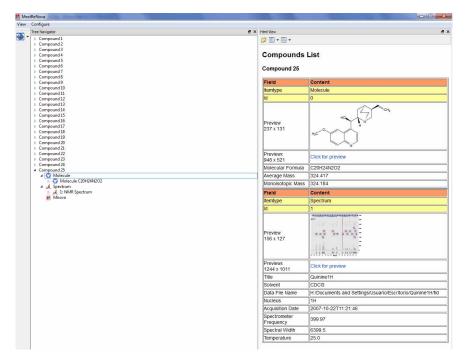


If you have used the Verification plugin to build your database, then you will find useful the 'Well Plate View' which will contain information about the Verification results (by using the typical color code for the plates; green for a good verification result, yellow for a doubt and the red for a bad result in the verification).

Clicking on any of the plates, will show the corresponding molecule, spectrum and table of fields.


Double clicking on the plate will copy all the information to Mnova as a new document. Right clicking on the well plate (or on several) will allow you to 'Paste the item(s) or the compound(s) to Mnova' or to 'Update the 1H or 13C Prediction <u>Database</u>':

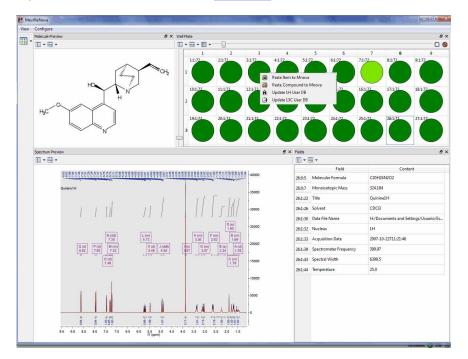

Of course the user will be able to freely customize any of the templates or even create their own ones. All the objects are linkable and the user will be able to change its position by just clicking&dragging. In the example below, we are changing the location of the 'Fields' table:

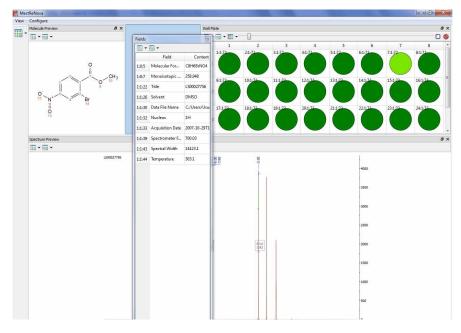

In the example below, we are showing a template with 1H and MS datasets.

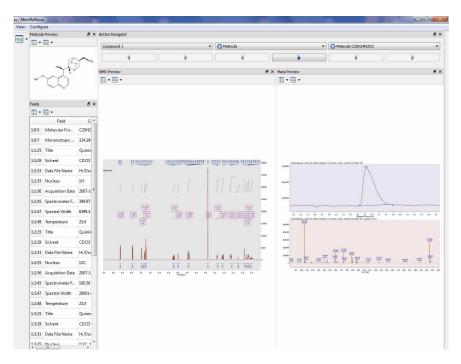

To create it, we have used the default 'Record View' template and added the MS preview by following the menu 'Configure/Add Widgets/Preview'. Once the new 'Preview' has been created, we have selected 'Mass Spectrum/Preview' after having clicked on 'Configure' button.

In addition the user will be able to customize the 'Views' by adding/changing information of the 'Previews' or 'Tables' boxes.


Even, the user will be able to create his own new templates (or customize the existing ones) by following the menu 'Configure':

Configure		
Add Widget Configure Widget Remove Widget	) )	Button Navigator Column Navigator Fields Table
Add View Copy View Configure View Remove View	•	Form Html View Item List Preview
Load Settings Save Settings Save Settings As		Query Table View Tile View Tree Navigator
Field		Well Plate

From here, the user will be able to add configure and remove widgets (such as 'button, column or tree' navigators, Fields Tables, Previews, etc...). From this menu, you can Add/Copy/Configure or remove views or to load/save the settings of different templates.


If you want to show the original spectrum or molecule that you used for the search, you will need to add the 'Query' widget and you will be able to compare the query spectrum with the hits from the database.

Here you can see another example combining NMR, MS and well plates:

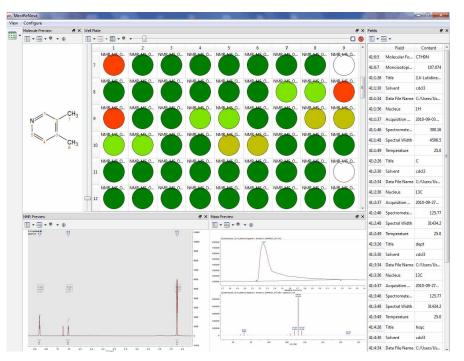

# 15.6 Deleting items/Records

The user will be able to delete items or records by using these options of the menu:



Clicking on the 'Delete Item' option, will display a new window with some edit boxes to fill with the information (Compound, Type and number) about the item that the user wants to delete. In the example below, it is shown how to delete the Spectrum 1 of the compound 2:

Delete Item	
Record:	2
Item Type:	MR Spectrum 👻
Item Number:	1

To permanently delete a record:

	rd		ord	te Reco	Delet
Record: 127	27	_	27	ord: 1	Reco

# **15.7 User Preferences**

It is possible to select set up the preferences for the DB plugin, just by following the menu 'Edit/ Preferences' and selecting DB:

	Pluq-ins	DB	NMR	Drawing Tools	U	
tabase <u>C</u> onnection Connection		Sgarch	MMR Search	MS Search		
Connection Response 7 Log Directo	limeout:		60s 🜩 60s 🜩			

From here, you can select the number of seconds to wait for a connection or response with the server or the path to store the packet log file.

Selecting the Storage label, will allow you to select the resolution of the 'Previews' and to load layout templates (which will be applied when you copy items or compounds from the DB to Mnova). Unchecking the 'Show Data Dialogs' will disable the pop-up windows (to introduce additional information) which appear when you are uploading MS datasets to the database.

			2	b		
General	Plug-ins	DB	NMR	Drawing To	ools	
atabase						
	Storage	Search	MR Search	MS Search	1	
Saving						
Max. Prev	iew Size:	1024				•
Save (	Object Data					
	Data Dialogs					
Layout Ter	mplates					
Items:	C:/demo.mn	ova				
Records:	C:/My docum	ients				

From the Search label, the user will be able to select the maximum number of hits or compounds returned by a search or the 'Preselection Threshold' (the minimum number of search hits for preselection dialog to be shown).

You can select the minimum score for Peaks, multiplets or free search hits to be included in the results. If for example you are searching for 3 peaks and Mnova DB finds spectra with 2 of the 3 peaks, then the score will be 666. From here, it will be possible to set different databases to be searched in:

tabas	ie				
Conn	ection	Storage	Retrieval Sgarch	<u>NMR Search</u> <u>M</u> S Sear	rch
Sea	arch			Search Results Quality	
Ma	x. Hits:	10	1000 🌲	Peak Search:	600 🚔
Ma	x. Records:		100 🌲	Multiplet Search:	600 🌲
Preselection Threshold:		hreshold:	1	Massitem Search:	800 🤤
				Free Search:	900 🤤
Dat	abases				
	Always she	ow the databa	ase selection dialog		
V	Search the	current data	base		
Sei		lowing databa	ses:		
	Enabled	Password		Connection	•
1	V	V	mndb://Test@loca	Ihost:5504/RSDCDatabase	e 🖉
2	V	1	mndh <sup>.</sup> //Test@192	.168.2.13:5555/Wiley-hnmi	rOC2014

From the NMR Search label, you can set the Peak and multiplet search tolerances and select the desired databases to search.

tabase							
Connection	Storage	Searc	h <u>N</u> MR S	earch MS	Search	1	
Position: 1H: Other: Width: Intensity:	0.10 ppm 1.00 ppm 1.00 1.00		Position: 1H: Other: Width: Intensity:	0.20 ppm 5.00 ppm 1.00 1.00		Position: 1H: Other: Width: Integral:	0.10 ppm ↓ 1.00 ppm ↓ 1.00 ↓ 1.00 ↓

From the MS Search, you can select the Scoring type (purity, mixtures or reverse) and tolerance.

	<b>e</b> h			<u>a</u> k	8
General	Plug-ins	DB	NMR	Drawing Tools	
atabase					
Connection	Storage	Search	MR Search	MS Search	
Tolerance:				0.50	•

The purity setting will take into account all mass peaks in both the unknown spectrum and library spectra.

Mixture means mass peaks occurring in the unknown spectrum but not the library spectrum are ignored. This is for cases where the unknown spectrum might be a mixture containing additional compounds.

Reverse is the opposite of mixture - mass peaks in the library spectrum that don't occur in the unknown spectrum don't lower the score. This is like saying my unknown spectrum is better than the library spectrum.

Tolerance - m/z tolerance in Da or ppm. Most commonly, MS acquisition is done with "nominal mass accuracy", where the m/z values are only accurate to 0.1 to (say) 0.3 Da. In this case, a tolerance in

Da of 0.5 is sensible. High accuracy acquisition can produce mass spectra with m/z accuracy to 10 ppm or better. In that case, the user might select a mass tolerance of 20 ppm.

## 15.8 Managing Databases

You can manage the Databases from the menu:

	Save to Database	
ø	Show Record	
A	Search	
S.	Structure Search	
C.	Substructure Search	
严	Peak Search	
諙	Multiplet Search	
JC.	Massitem Search	
•	Browse	
x	Delete Item	
3	Delete Record	
ľ	Open Database	
1	Database Info	
8	Create Database	
1	Delete Database	
Ø	Manage Databases	
6	Connect	

You can create a new database just by following the menu 'Database/Create Database' to display the dialog box below:

Create Database		2
Database		
Name: <u>New_Database</u>	Server: localhost:5504	
Description:		Advanced

Click on the 'Advanced' button to customize the options of your Database:

#### **Mnova Database**

lame	New Databa						Server: localhost:5504						
		ise					Server. localitosc.5504					=	
Jescri	ption:											Į	A Basic
	Save				Load		Сору	Default	t			Clear	
tems													
ID	Name		Туре	Fields	Comme	ent							Add
1	Molecule		COMP	28	Molecules (mar	ndatory).							Edit
2	NMR Spectrum		NMR	57	1D and 2D NM	R spectra.						H	Delete
3	Mass Chromatog	ram	MS	25	Mass chromato	grams.							
4	Mass Spectrum		MS	102	Mass spectra.								
5	Mnova		GENERIC	14	Mnova items.							-	
ields													
ID	Item		Name		Туре	Size	Content	Comment	Editable	Required	Unique		Add
2.29	NMR Spectrum	Peak	s1D		PEAKLIST1A	65535	=getNMRPeaks(item,1)		false	false	false		Edit
2.30	NMR Spectrum	Peak	s2D		PEAKLIST2A	65535	=getNMRPeaks(item,2)		false	false	false	H	Delete
2.31	NMR Spectrum	Mult	tiplets1D		MULTIPLET	65535	=getNMRMultiplets(item,1)		false	false	false	(	Delete
2.32	NMR Spectrum	Integ	grals1D		INTEGRAL1A	65535	=getIntegrals(item,1)		false	false	false		
2.33	NMR Spectrum	Integ	grals2D		INTEGRAL2A	65535	=getIntegrals(item,2)		false	false	false		
2.34	NMR Spectrum	Title	в		TEXT	10000	=NMRSpectrum(item).title		false	false	false		
2.35	NMR Spectrum	Spee	ctrum Com	ment	TEXT	10000	=NMRSpectrum(item).comment		false	false	false		
2.36	NMR Spectrum	Expe	eriment Typ	be	TEXT	500	=NMRSpectrum(item).experimentType		false	false	false		
2.37	NMR Spectrum	Orig	inal Forma	t	TEXT	500	=NMRSpectrum(item).originalFormat		false	false	false		
2.38	NMR Spectrum	Solv	ent		TEXT	500	=NMRSpectrum(item).solvent		false	false	false		
2.39	NMR Spectrum	Peak	sPurity		NUMERIC	0	=NMRSpectrum(item).calcPeaksPurity()		false	false	false		
2.40	NMR Spectrum	Orig	in		TEXT	500	=NMRSpectrum(item).getParam("Orig		false	false	false	-	

From here, you can define several fields for each object just by using small scripts (after having clicked on the 'Add...' button of the Field menu). For example in the example above, you can see how we have defined 40 fields for the object 'Spectrum', such as 'Peaks1D', 'Peaks2d', 'Multiplets1D, 'Title', etc. You can also get the information of the Database (showed in the picture above) just by following the menu 'Database/Database Info'.

You can set a flag as 'Editable', 'Required' or 'Unique' for each item:

<u>Editable</u>: a field set as Editable will be editable after being stored in the DB. <u>Required</u>: a field set as Required will need to have a value when saved to a DB. Unique: a field set as Unique will be used to check for duplicated records when saving.

You can add new items, edit the existing ones or delete them by using the applicable buttons.

For example, if you want to add a new field, you will need to click on the 'Add' button to add a new field. For example, let's add a 'text' field called 'CAS NUMBER' in a molecule:

Vame	New_Data	abase			Server:	localhost: 5504
Descri	ption:					A Basic
	Save		Load		Copy	. Default Clear
tems	015269/01		2000 200 000			
ID	Name	Type	Fields	Com	ment	Add
1	Molecule	COMP	29	Molecules (r	mandatory).	Edit
2	NMR Spectrum	NMR	55	1D and 2D N	IMR spectra.	E Delete
3	Mass Spectrum	MS	30	Mass spectra	5.	
4	Mnova	GENERIC	14	MNova item	15.	
5	Page Note	GENERIC	15	MNova page	e notes.	
ields			1. T	(	M Add Fiel	
ID	Item	N	lame	T	Field	Add
1.15	Molecule	LinkID		TEXT	ID:	1.143 Edit
1.15	Molecule	Туре		TEXT	Item:	Molecule
1.17	Molecule	Description		TEXT	Name:	
1.17	Molecule	Preview	n	BINA	Type:	TEXT
1.10	Molecule	User		TEXT	Size:	100
1.19	Molecule	Host		TEXT	Content:	
1.20	Molecule	Document		TEXT	Comment	
1.21	Molecule	Document		TEXT		Add Cancel
1.22	Molecule		u)	INTEG	ER 0	
1.23	Molecule	Page		TEXT	IER U	
1.24	Molecule	PageID Created		DATE		-CREATED-
					<i>.</i>	
1.26	Molecule	Modified		DATE		-MODIFIED-
1.27		Mnova Ver	-	TEXT	100	=Application.version
1.142	2 Molecule	CAS NUM	BER	TEXT	100	

Here you can see an example to add a couple of parameters as new fields into the 'Mass Chromatogram' item; by typing **=***MassItem(item).parameters['Sample Name']* under the 'Content' field':

lame:	New_Database						Server: localhost:5504				
escri	ption:										A Basic
	Save	)		L	oad		Сору	Default	]	Clear	
ems				-							
ID	Name	Туре	Fields	Co	omment					-	Add
1	Molecule	COMP	28	Molecules	(mandatory	).				Ξ	Edit
2	NMR Spectrum	NMR	57	1D and 2D	NMR spect	ra.					Delete
3	Mass Chromatogram	MS	27	Mass chro	matograms.						
4	Mass Spectrum	MS	102	Mass spec	tra.					~	
ields											
ID	Item		Nam	e	Туре	Size	Content	Comment	Editable	Requi 🔦	Add
3.1	Mass Chromatogram	Host			TEXT	100			false	false	Edit
B.1	Mass Chromatogram	Docur	nent		TEXT	1000			false	false	Delete
3.1	Mass Chromatogram	Docur	nentID	tID TEXT		100 0			false	false false	
3.1	Mass Chromatogram	Page		INTEGER				false			
3.1	Mass Chromatogram	PageII	C	-	TEXT	100			false	false	
3.1	Mass Chromatogram	Create	d	1	DATETIME	0	-CREATED-		false	false	
3.1	Mass Chromatogram	Modif	ied	1	DATETIME	0	-MODIFIED-		false	false	
3.1	Mass Chromatogram	Mnova	a Versior	n -	TEXT	100			false	false	
3.2	Mass Chromatogram	Vial			TEXT	100	=MassItem(item).parameters['Vial']		true	false	
3.2	Mass Chromatogram	Sampl	e Name	-	TEXT	100	=MassItem(item).parameters['Sample Name']		true	false	
•						Ш		4			

Once you have selected the desired items, click on the 'Create&Open button.

If you want to delete any existing database, just follow the menu 'Database/Delete Database' and select the undesired database in the window displayed:

Databases	? ×
Delete Databas	
[mn_testcase1	•
ОК	Cancel

#### 15.8.1 Create custom fields

It is possible create custom text fields by using a layout template. Let's see an example which you can download from <u>here</u>

First of all, you will need to create a new Database with the new text fields. You can do it by following the menu 'Database/Create Database/Advanced/Load' and select the XML which is on the file that you downloaded above (or you can add the new text fields that you want). This will add two new text files ('Project Name' and 'Analysis Comments') to the Database. Click on the 'Create&open' button to generate the new Database:

	ase						1		
Name Descr	iption:	mhei	dsExample				Server: localhost:5504		A Basic
	Save				Load		Copy Default		Clear
Items									
ID	Name		Туре	Fields	Comm	ent			Add
1	Molecule		COMP	22	Molecules (ma	ndatory).			Edit
2	NMR Spect	rum	NMR	46	1D and 2D NM	R spectra.			Delete
3	Mass Spect	rum	MS	28	Mass spectra.				
4	Mnova		GENERIC	12	MNova items.				
Fields									-
ID	ltem		Nam	e	Туре	Size	Content	Comm *	Add
1.9	Molecule	Uui	uid		TEXT	100	=item.uuid		Edit
1.10	Molecule	Link	dD		TEXT	100	=item.linkId		Delete
1.11	Molecule	Тур	e		TEXT	100	=item.name		
1.12	Molecule	Text			TEXT	65535	=getText(item)		
1.13	Molecule	Pre	view		BINARY	16777215	-PREVIEW-		
1.14	Molecule	Not	ies		TEXT	65535	-NOTES-		
1.15	Molecule	Use	r		TEXT	100	-USER-		
1.16	Molecule	Hos	st		TEXT	100	-HOST-		
1.17	Molecule	Doc	ument		TEXT	1000	-DOCUMENT-		
1.18	Molecule	Cre	ated		DATETIME	0	-CREATED-	1	
1.19	Molecule	Mo	dified		DATETIME	0	-MODIFIED-		
1.20	Molecule	Mn	ova Versior	'n	TEXT	100	=Application.version		
1.10	7 Molecule	Pro	ject Name		TEXT	1000	=getNamedTextField("Field", "[ProjectNam		
			alysis Com	mantr	TEXT	100	=getNamedTextField("Field", "[Comments]")		

Then, you will need to create a <u>layout template</u> (in the example the template is called "LayoutOrig.mnova".

Here you can see a layout template with 5 pages (molecule, 1H-NMR, 13C-NMR, 2D-NMR and MS):

M Mest		estieds/Castenie/intex.ayee(Urg moon)	- 0 ×
mne		hain Administa Santa Manshadhain Pentital Arenthale Sanjas Documents Halp 学習のや Conservas ・ 父父国家住国社社犬之十次・打12 110、1162、12、13、13、13、13、13、13、13、13、13、13、13、13、13、	[= [0'] X
1.1.1			
图•	non 6 X	MESTRELA RESEARCH	
	2		68 68 68
÷ · Ø			●●四日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日日
●● 道理 田舎 田城泉	2		10 A
		Kakoule	
₩			1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
· · · ·	S. Parate		
B			
×		K	
P.	III light gray • Dlack •	🖥 🖪 * X, * 🔺 A MAA * ANA * 12 * 🖅 * 📰 * 💱 * 🖤 🔇 🟈 🏈 🔗 *	Licenser O DE 10

Then, run the script called "addNamedFields.qs". This will add two named text fields [ProjectName] and [Comments] to the layout:


	MESTRELAB RESEARCH
( Fill in project name )	
( Fill in analysis comments )	
	Molecule

Then save the results as "LayoutWithFields.mnova" by following the menu 'File/Save As'. Those text fields will have its own Properties, even you could add new text properties to the page items and edit them by selecting the 'Metadata' tab:

		Pro	pe	rties	l	? ×
			•			
Project:	add Project name	Met	ad	lata Geometry	Shape	
			ł	*		
Subproject:	add subproject name		ıl	Property	Value	
Mol Code:		1	L	type	Field	
MOI COUE.		2	2	subtype	[Code]	
•	• •	3	3			
Comments:	add analysis comments					
				ОК	Cancel	Apply
		<u>(</u>		_		_

Finally apply the layout template over your datasets, fill the text fields manually and save the documents to the Database (by following the menu 'Database/Save').

To display the new custom fields after a search, go to the DBBrowser and add the new fields to views as desired and save the configuration by following the menu "Configure/Save Settings As":

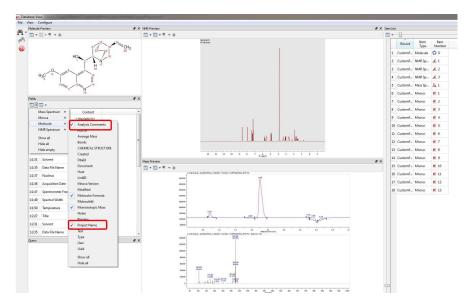

You can create **mandatory fields** in order to save them to the Database, You will find an example script called "dbMandatoryFieldsExample1.qs" into the examples installation folder of Mnova. Save this script into one of your 'Scripts directories' (Edit/Preferences/Scripting), restart Mnova and then create a new database with two added custom fields "Project" and "NotebookRef" in the Molecule item type:

Datab								
Name	New_	Database			Server	i localhost:5504	_	
Descri	ption:							A Basic
	Save		Loa	d	Copy	Default	Cle	ar
[tems								
ID	Name	Туре	Field	s Comme	ent		1	Add
1	Molecule	COMP	29	Molecules (ma	ndatory).			Edit
2	NMR Spect	rum NMR	55	1D and 2D NM	R spectra.			Delete
3	Mass Spect	rum MS	30	Mass spectra.			-	
Fields								
ID	Item	Nai	me	Туре	Size	Content	- C	Add,
1.23	Molecule	Page		INTEGER	0			Edit
1.24	Molecule	PageID		TEXT	100			Delete
1.25	Molecule	Created		DATETIME	0	-CREATED-		
1.26	Molecule	Modified		DATETIME	0	-MODIFIED-		
1 77	Molecule	Mnova Versio	20	TEXT	100	= Application.version		
1.142	2 Molecule	Project		TEXT	100			
1.143	8 Molecule	NotebookRe	f	TEXT	100		-	
4			ш		1		•	

Next, save any dataset to the new database and a dialog asking for the content of the mandatory fields will be shown with each save operation:

Data Fields	2 ×
Mandatory Fields	
Project	
Notebook Ref.	
OK	Cancel

# 15.9 Mnova DB scripts

The user will find in the Scripts menu some useful scripts for the Database plugin:

Scri	pts Documents Help		
y.	Edit Script	-	爬• 俞爻•伲•龃•娀• 谲
-	Run Script		
	Recent Scripts	• -	
	Report	•	
	Verification		
CONTENT	comment Ct	rl+T	
	Database	Corry	Copy Database
	Export ASCII	Espo	Export Documents
	Import	1 Inpe	Import Documents
	NMR Tools	Impe	Import Files (By Location)
PHS	APMS0	lings	Import Files (Pairwise)
	MS_LEO	Tres	Import Pages
-	Apply Layout and Processing Template Ct	rl+I Impe	Import SDFile
ato .	Autoload Files	Play	Play MNSR File
-		Sear	Search MS in Chromatogram

The **Copy Database** script will allow you to export databases to any destination:

ource		Destination		
Connection Host: Port: User: Password: Save Pass	localhost 5504	Connection Connection Same as S Host: Port: User: Password: Save Pass	localhost 5504	
Database Database: Records From: To:	0	🔿 Default	abase:	

The **Export Documents** scripts will be very useful to export all the selected compounds of the Dabatase as Mnova documents into the desired directory:

Select Compounds		
From:	1	* *
To:	141	*
Export to:		
Base Directory: C:	/Users/Usuario	

The **Import Documents** script will allow you to save to the Database Mnova documents from a selected directory. This script looks for Mnova documents on disk, everything in the same document goes into the same database record:

Select Directory	
📃 Escritorio	
Bibliotecas	E
👂 🧾 Usuario	
🖻 🌉 Pablo	
🖻 🗣 Red	
🔰 Assign	
🔒 Base Datos	

The **Import Files (by Location)** will save to the database the desired type of files from a selected directory:

Main Files				
Base Directo	tory: C:/Users/Usuario			
Path Mask:	.*\.mol\$			
V Optional	Files	Examples:		
Path Mask:	.*fid\$	PRJ ????\/(fid 1r)\$		

For the 'Path Mask'; you can use wildcards, so this could be, for example, .\*\.mol\$; or just .\*fid\$ and click 'OK'. The \$ symbol means in '.\*fid\$' that it will search for the FIDs that are stored at the end of the folders structure (valid for those cases where all the spectra of a given molecule are grouped in the same folder).

This script looks for main files matching the given path mask in the specified folder. Then, for each

main file found, it looks for optional files according to the second path mask \*relative to each main file location\*. Depending on your situation, main files could be molfiles and optional files spectra, or vice versa. E.g. You have many spectra (main files), and for some of them you have a molfile (optional files). Or, you have molfiles (main files), and for each molfile you have zero, one, or several spectra (optional files).

E.g:

\Data\ABC123\ABC123.mol \Data\ABC123\NMR\XBlah.fid \Data\ABC124\Molecule.mol \Data\ABC124\NMR\124.fid \Data\ABC125\Whatever.mol \Data\ABC125\NMR\Any.fid

The **Import Files (pairwise)** will import pairs of molecules and spectra (first spectrum with the first molecule in the applicable folder; second spectrum with second molecule and so on...) and will save them into the Database. Please bear in mind that you must have the same number of molecules and spectra.


Main Files	
Base Directory:	C:/Users/Usuario/Desktop/Mis documentos/Espectros de RMN/Lee/spec
Path Mask: */2	io/fid
Optional File	s
Base Directory:	C:/Users/Usuario/Desktop/Mis documentos/Espectros de RMN/Lee/mol
Path Mask: *.n	lo

You can use wildcards for the 'Path Mask', so this could be, for example, \*/10/pdata/1r, or just \*/fid, or \*/ser. Finally click 'OK' and all the selected spectra and molecules will be saved in the database.

It works exactly as the Multi-Open script: You give it two path masks and it will look for files of each type according to the corresponding path mask. Files are associated to each other by the order in which they are found. So there needs to be a 1-to-1 correspondence between spectra and molecule files. The order in which they are found is determined by the file names. You would use is this script if you have two folders (one for molecules and another for spectra) and the files can be associated witch each other via the file name.

E.g: \Data\Molecules\ABC123.mol \Data\Molecules\ABC124.mol \Data\Molecules\ABC125.mol \Data\Spectra\NMR\ABC123.fid \Data\Spectra\NMR\ABC124.fid \Data\Spectra\NMR\ABC125.fid

The **Import Pages** script will save all the pages in the current document to the current Mnova Database:

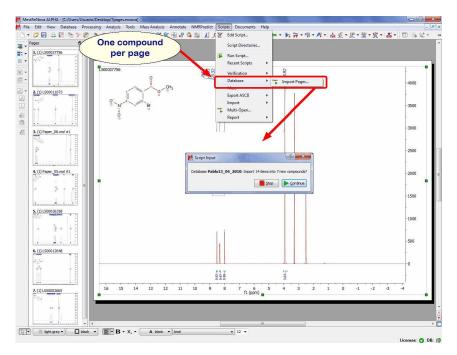

This script goes through the currently open Mnova document, creates a new record for each page, everything on the same page goes into the same database record.

The 'ImportSD File' script will allow you to import to your Database the molecules contained in a SDF file.

Mnsr files can be played to the MnDB server either via the Mnova client (Scripts/Database/Play Mnsr File), or via the MnDB test client.

The **'Export CSV'** script will "dump" all the metadata information from a selected database into a text file format.

The "**SDFile to definition**" script takes an SDFile and outputs a database definition .xml file. The Database definition .xml file can then be used to create new databases into which the SDFile which can be imported by using Scripts/Database/Import SDFile, preserving 'all tags' and data. So, if you want to import all the tags of your SDF file into a Database, you will need to use this script.

The Search MS in Chromatogram script, will search for all the mass spectra under each TIC peak. You will only need to load your GC/MS dataset and after having run the script, a dialog box will be displayed asking for the options for matching MS peaks:

MS Search Se	ettings		
Scoring:	Purity		
Tolerance:	0.50	Dalton	•
Minima <mark>l</mark> Hit S	core:	800	×
Global Settin	gs		
Selection Mo	de: Manual		¥
Max top hits	per peak:	5	<u>A</u>   <del>T</del>
Results Setti	ings		
Report folde	er: C:/User	s/Usuario	

You will need to select the maximum number of top hits to report for each peak (default: top 5).

Clicking on OK, the script will get the mass spec under each TIC peak (depending on the current setting of the Selection Mode: Manual, Peak, or Peak with Background Subtraction), do peak picking, and search the peaks against the selected DB.

#### **Export Assignments to Prediction Database**

This script will be useful for example to export a third party prediction DB into the Mnova Prediction Database. For example, let's import a SDF file containing all the assignments (you can see those assignments by loading the SDF file and following the menu 'View/Table Assignments'. The molecules and the assignments contained in the SDF file can be stored in a Database by following the steps below:

- 1. Create a DB definition from SDFile with "SDFile to Definition" script (under the 'Scripts/Database' menu).
- 2. Create the database with the desired definition by following the menu 'Database/Create/Advanced/Load' and selecting the xml file created in the step 1
- 3. Import the SDFile to the DB with "Import SDFile" script (under the Scripts/Database menu)
- 4. Finally the assignments can be exported to a Prediction DB using the script "Export Assignments to Prediction DB":

Scripts Document	s H		🖌 附 Export Assignments To Prediction D	B 2
Run Script Recent Scripts Stop Script Import NMR Tools Report Export		<u> </u>	Source Connection Host: localhost Port: 5504 User: Pablo Passonod:	Destination Database Existing: N  Saving Options Werfy Score Range Confy Score Values in the Range
Database	•	Import Decementaria Import Pages Import Files (by location) Import Spfile Export Documents Export Documents Copy Database Search Ms in Chromatogram	Save Password      Database      Database      Records      From:      To:      0	From:         0.00         ©           Connect.         To:         0.00         ©           v         Predictor DF/s to Update         ©           v         14         Ø         157           0         150         0         0           0         150         0         0           0         0         0         0         0           0         150         0         0         0           0         0         0         0         0         0           0         3154         0         0         0         0           0         319         0         0         0         0         0
		Play MNSR File		OK Cancel

You can also load the SDF file into Mnova containing several molecules with assignments and update

Scripts Documents Help 大・気・ゑ・虎・衆・衆・♥●回四山や 🔰 📝 Edit Script... 🖐 Run Script... · · 9 · · · 10 · · · 11 · · · 12 · · · 13 · · · 14 · · · 15 · · · 16 · · · 17 · · · 18 · · · 19 · · · 20 · · · 21 · · · 22 · · · 23 · · · 24 · Recent Scripts 🔹 Stop Script Import • NMR Tools Peak Table to Spectrum...
 Multiplet Report to Spectrum... n Send Molecules to Prediction DB Report Batch Update Prediction DB... DEPT Traces Purity Calculator... Export Nucleus: 1H • Database DB: N • Solvent: Chloroform 👻 Set Solvent... SNR Peak Calculator... OK Cancel 
 Overlay Spectra

 Stack
 Stack Spectra
 🚏 Same Phase as Current Auto-Phase Current, Same Phase Rest Predict 1H and 13C

the prediction Database by following the menu 'Scripts/NMR Tools/Batch Update Prediction DB':

# Thank you!

Thank you for reading this manual, and for purchasing this release version of Mnova. We will be very keen to read your feedback on the application, to hear about any bugs you may find and to also listen to any additional ideas or suggestions you may have.

Please remember that you can send all those, and any queries about the software, or requests for help, to:

support@mestrelab.com

Keep checking our web site (www.mestrelab.com) for additional information on our range of software packages, and for news on our company.